

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
 Data File : P0076308.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2021 18:59
 Operator : DD\AJ
 Sample : M1712-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EXTERNAL-PAD-1

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:35:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:43:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.936	1483950	1084982	26.122	26.005
2) SA Decachlor...	10.928	9.201	1161777	1141582	30.205	29.731
Target Compounds						
26) L6 AR-1254-1	7.158	6.050	24128	34762	11.773	15.210 #
27) L6 AR-1254-2	7.390	6.208	57033	23607	18.353	11.919 #
28) L6 AR-1254-3	7.771	6.627	53679	58983	16.872	19.582
29) L6 AR-1254-4	8.069	6.867	43969	31190	20.986	17.675
30) L6 AR-1254-5	8.499	7.293	178573	94993	77.753	36.284m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
Data File : P0076308.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2021 18:59
Operator : DD\AJ
Sample : M1712-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
EXTERNAL-PAD-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:43:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

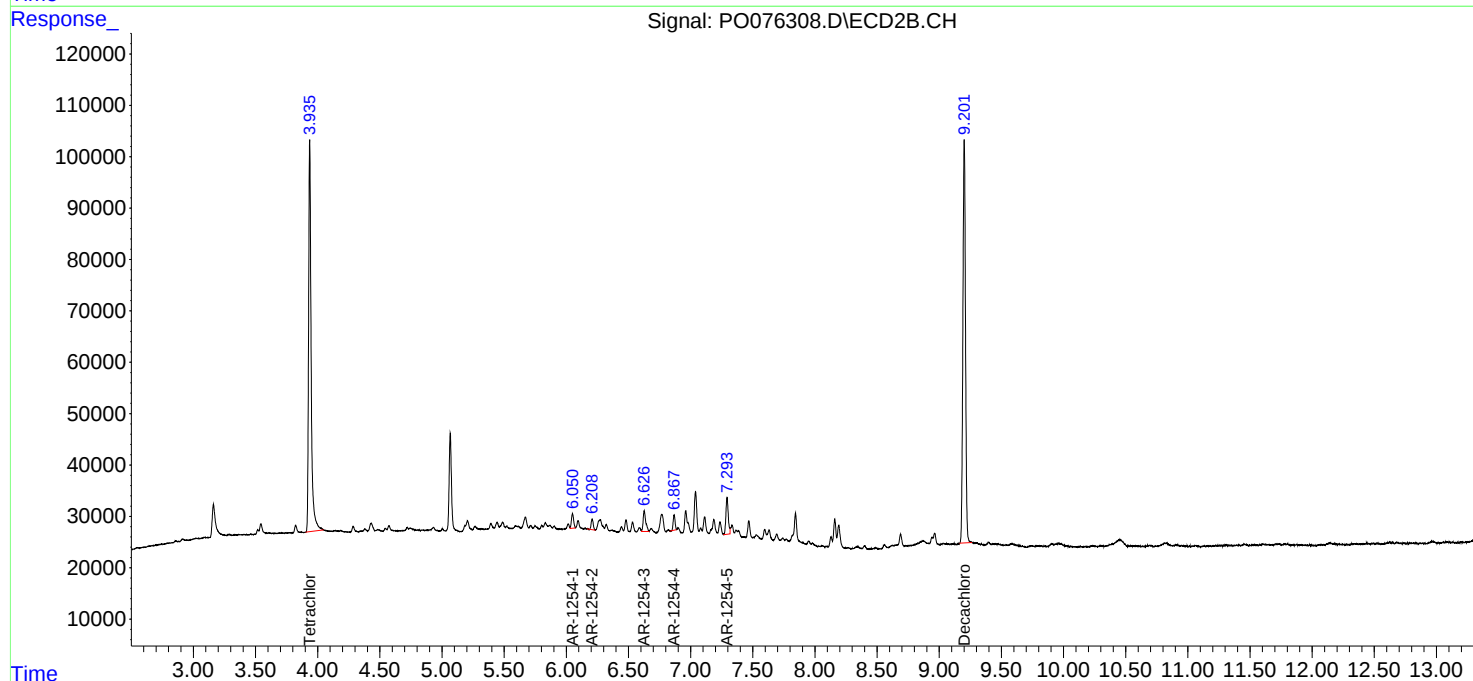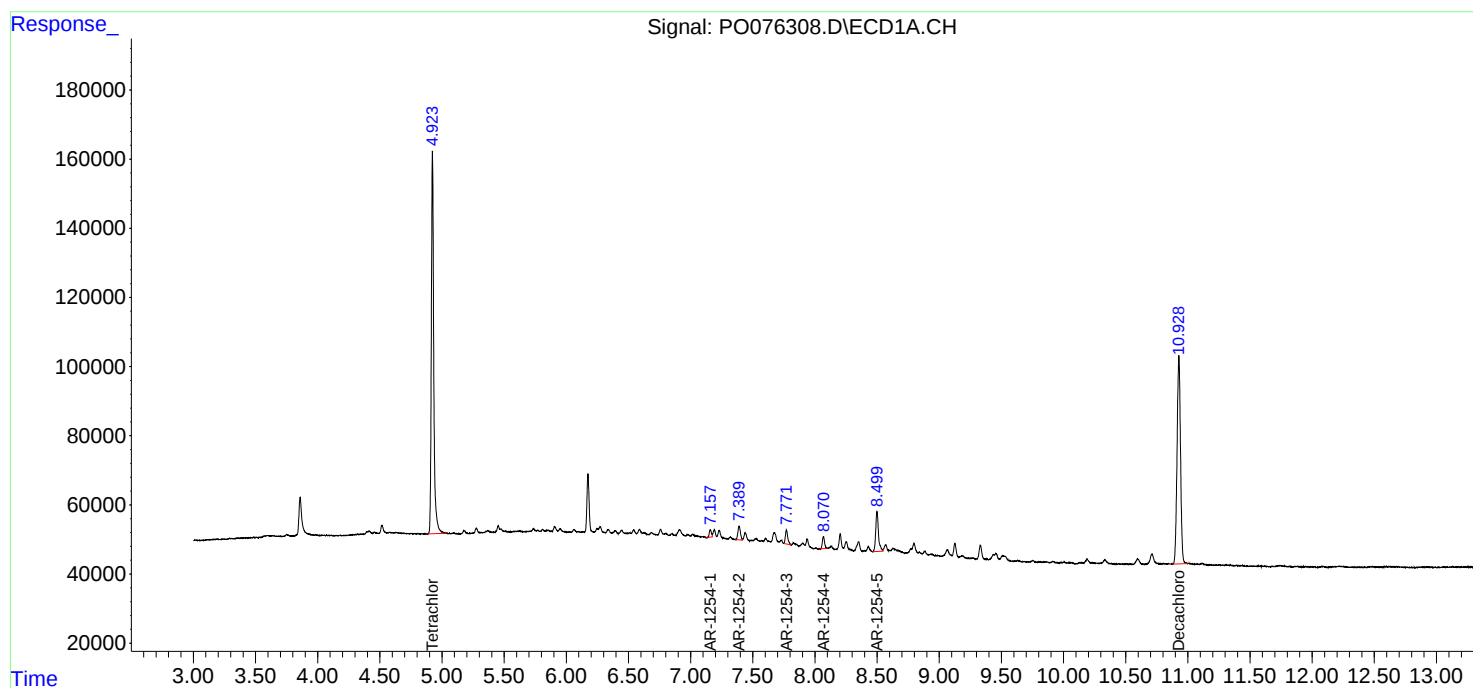

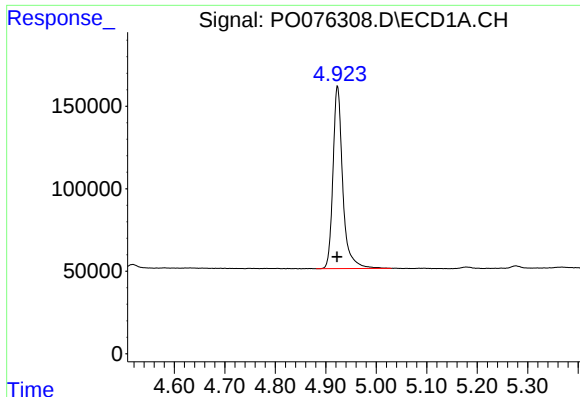


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.001 min
Response: 1483950
Conc: 26.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:38 PM

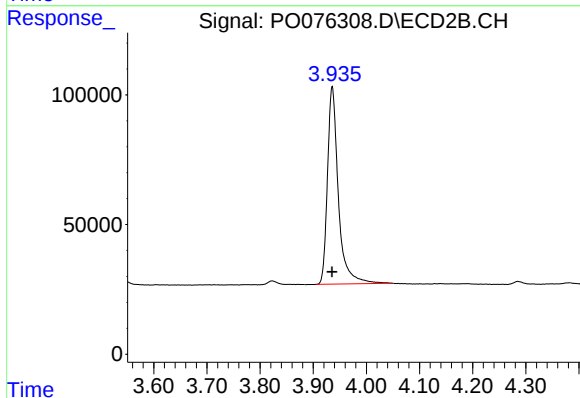


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 1084982
Conc: 26.01 ng/ml

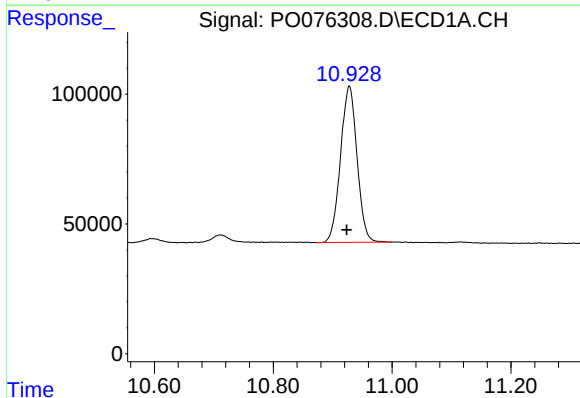


#2 Decachlorobiphenyl

R.T.: 10.928 min
Delta R.T.: 0.004 min
Response: 1161777
Conc: 30.20 ng/ml

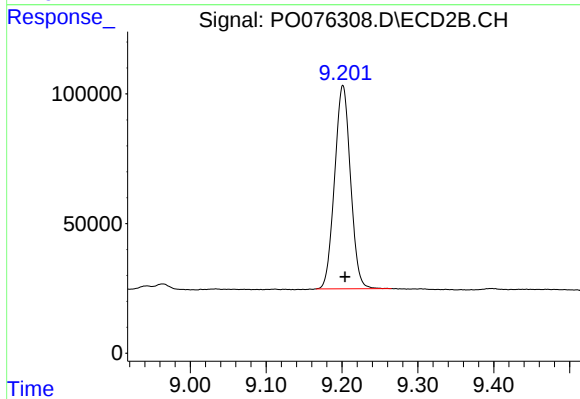

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.003 min
Response: 1141582
Conc: 29.73 ng/ml

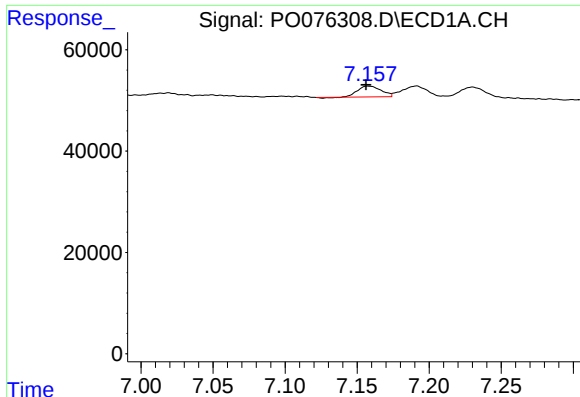


#26 AR-1254-1

R.T.: 7.158 min
Delta R.T.: 0.002 min
Response: 24128
Conc: 11.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:38 PM

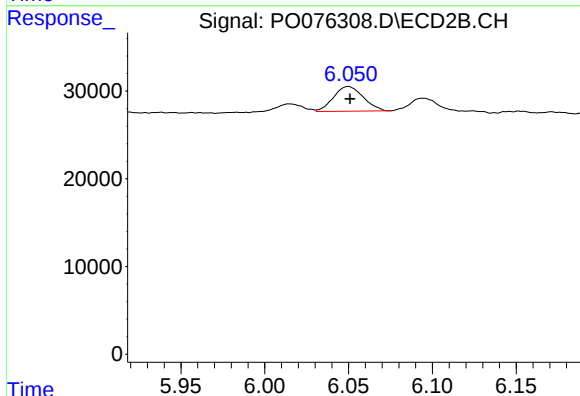


#26 AR-1254-1

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 34762
Conc: 15.21 ng/ml

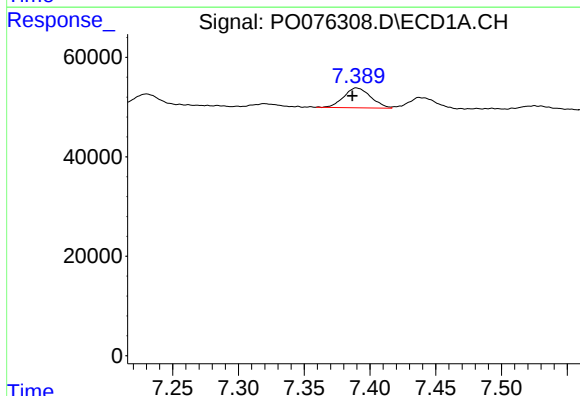


#27 AR-1254-2

R.T.: 7.390 min
Delta R.T.: 0.003 min
Response: 57033
Conc: 18.35 ng/ml

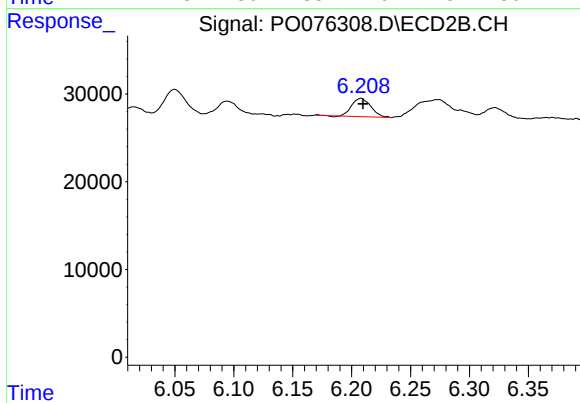

#27 AR-1254-2

R.T.: 6.208 min
Delta R.T.: -0.002 min
Response: 23607
Conc: 11.92 ng/ml

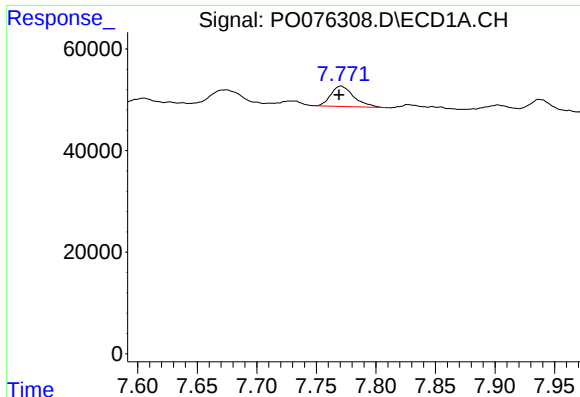


#28 AR-1254-3

R.T.: 7.771 min
Delta R.T.: 0.002 min
Response: 53679
Conc: 16.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:38 PM

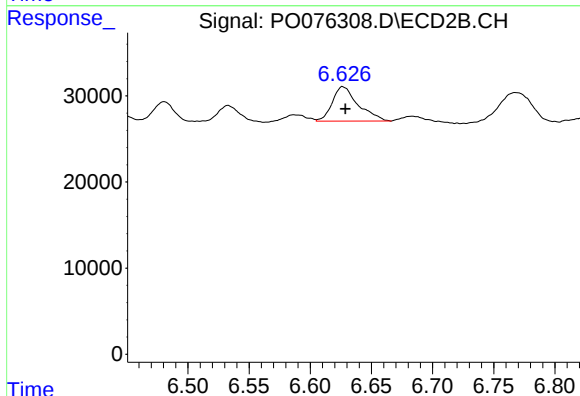


#28 AR-1254-3

R.T.: 6.627 min
Delta R.T.: -0.002 min
Response: 58983
Conc: 19.58 ng/ml

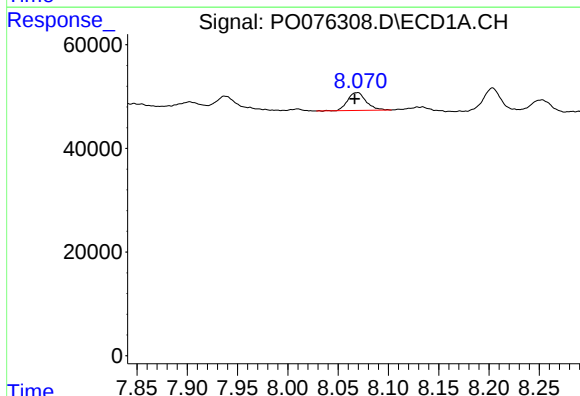


#29 AR-1254-4

R.T.: 8.069 min
Delta R.T.: 0.002 min
Response: 43969
Conc: 20.99 ng/ml

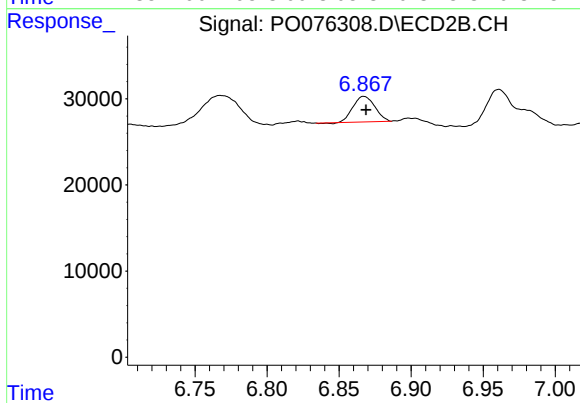

#29 AR-1254-4

R.T.: 6.867 min
Delta R.T.: -0.001 min
Response: 31190
Conc: 17.67 ng/ml

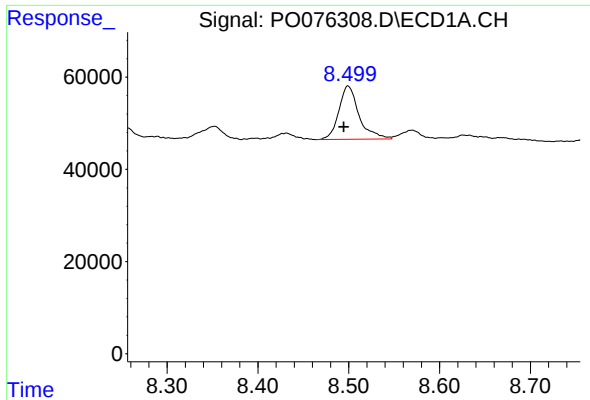


#30 AR-1254-5

R.T.: 8.499 min
Delta R.T.: 0.005 min
Response: 178573
Conc: 77.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-1

Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:38 PM

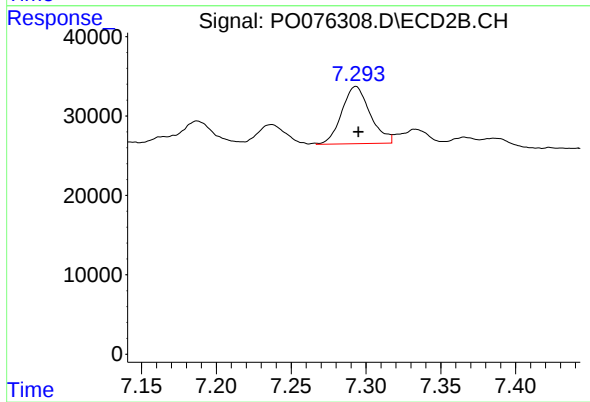

#30 AR-1254-5

R.T.: 7.293 min
Delta R.T.: -0.002 min
Response: 94993
Conc: 36.28 ng/ml m