

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031821\
 Data File : P0076309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2021 19:17
 Operator : DD\AJ
 Sample : M1712-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 EXTERNAL-PAD-2

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:35:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:43:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.934	1337302	972350	23.540	23.306
2) SA Decachlor...	10.924	9.200	1041772	1017123	27.085	26.489
Target Compounds						
26) L6 AR-1254-1	7.155	6.046	54945	74665	26.810	32.669
27) L6 AR-1254-2	7.388	6.206	106989	52085	34.429	26.298
28) L6 AR-1254-3	7.770	6.625	130347	151052	40.971	50.149
29) L6 AR-1254-4	8.066	6.865	94162	107834	44.943	61.107 #
30) L6 AR-1254-5	8.497	7.291	321775	182995	140.105	69.897 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031821\
Data File : PO076309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2021 19:17
Operator : DD\AJ
Sample : M1712-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-2


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:43:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

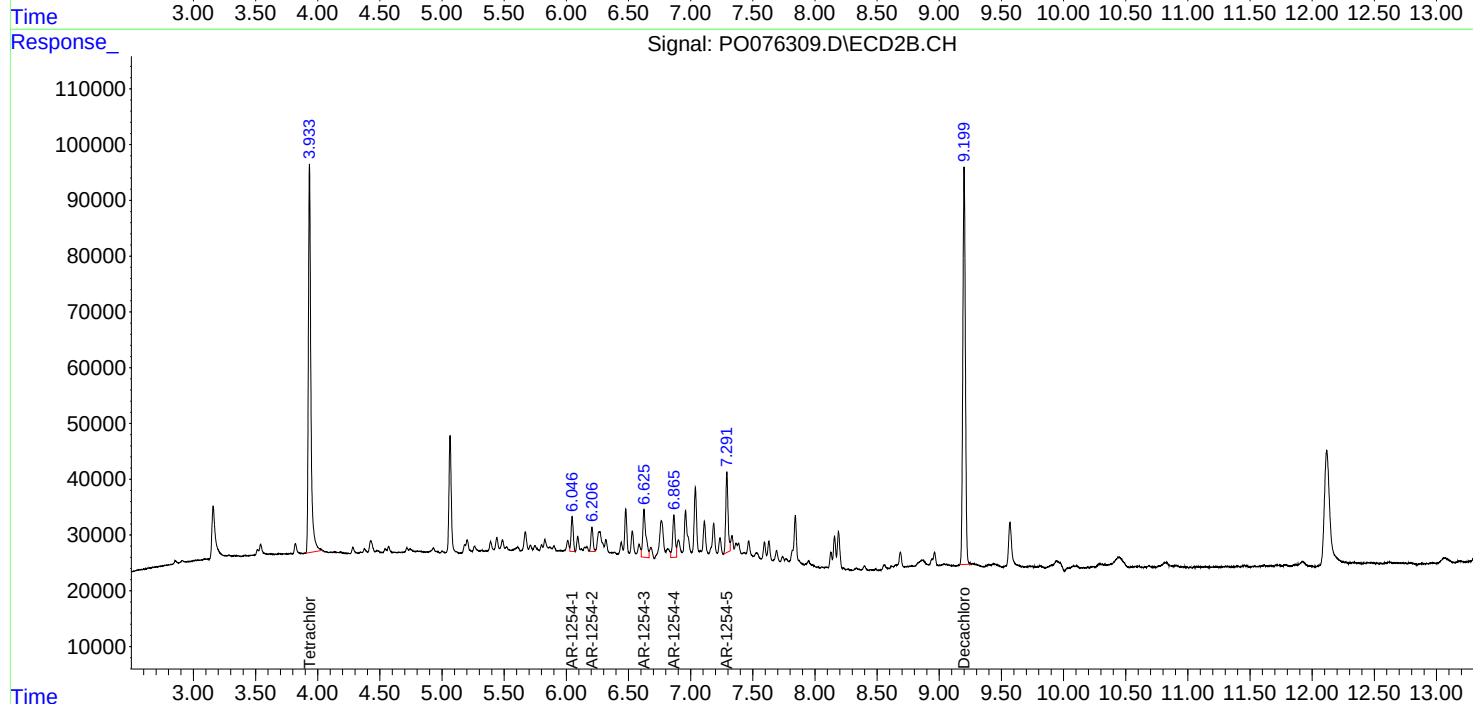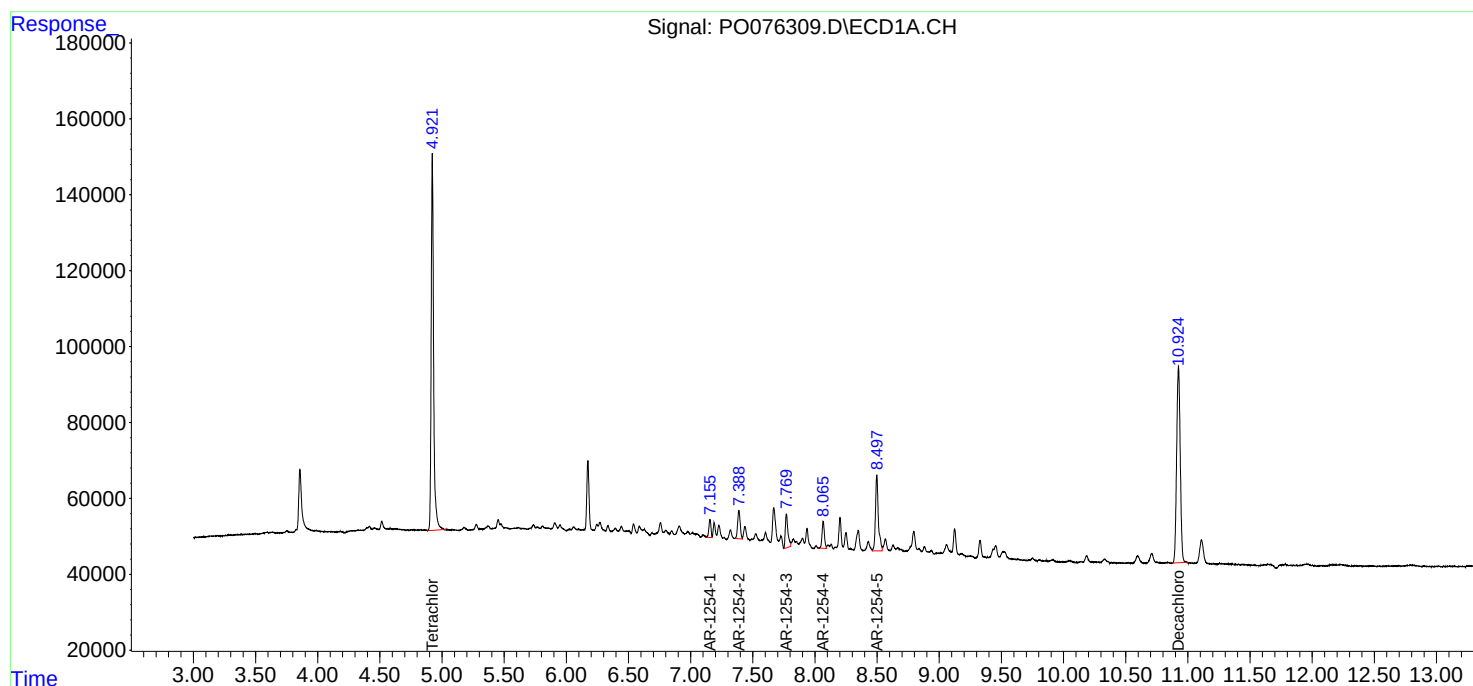

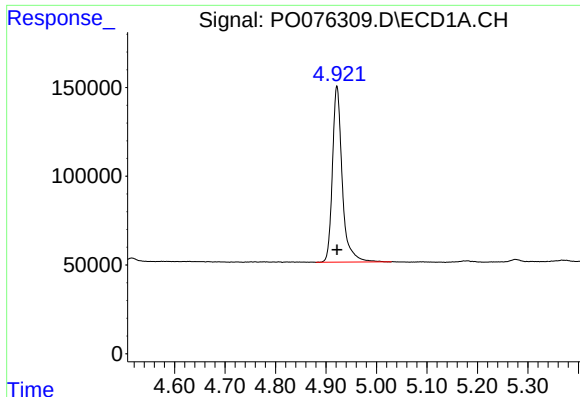


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 1337302
Conc: 23.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-2


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:40 PM

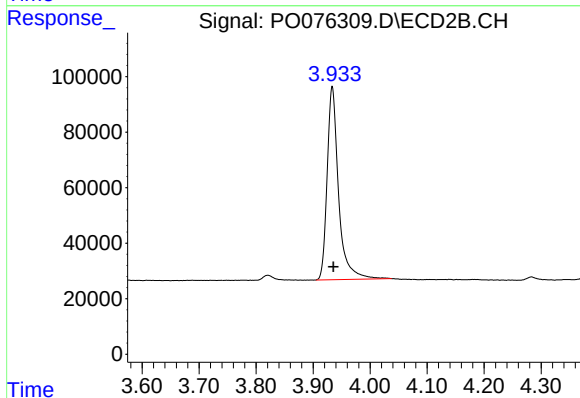


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 972350
Conc: 23.31 ng/ml

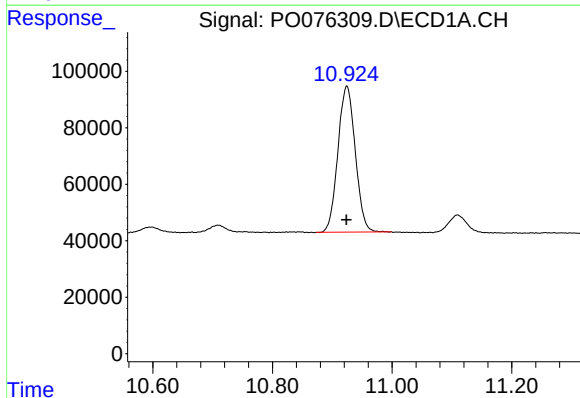


#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: 0.000 min
Response: 1041772
Conc: 27.08 ng/ml

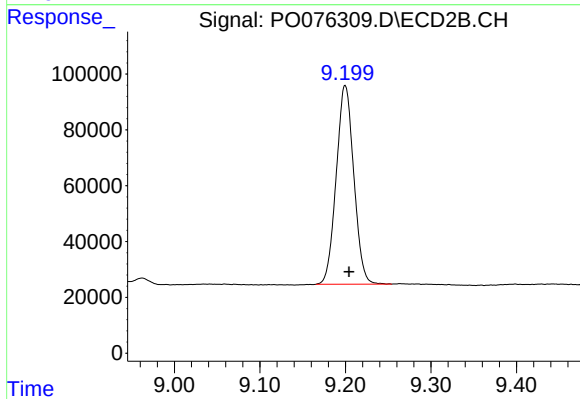

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.004 min
Response: 1017123
Conc: 26.49 ng/ml

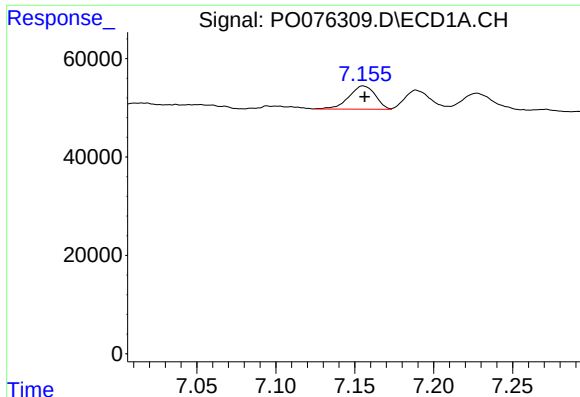


#26 AR-1254-1

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 54945
Conc: 26.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-2


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:40 PM

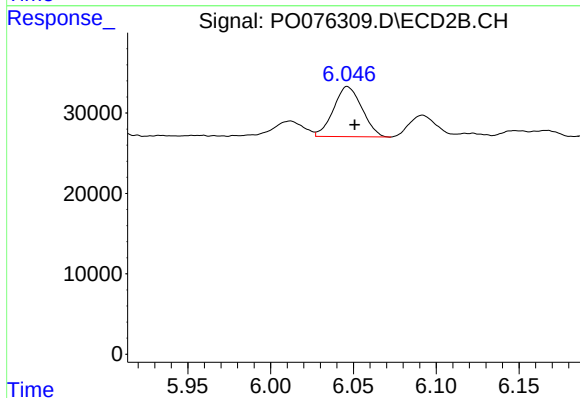


#26 AR-1254-1

R.T.: 6.046 min
Delta R.T.: -0.004 min
Response: 74665
Conc: 32.67 ng/ml

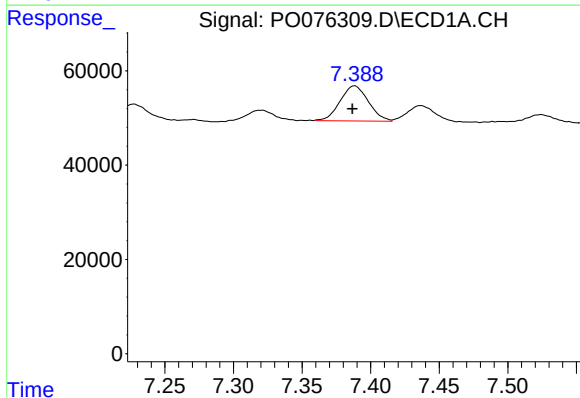


#27 AR-1254-2

R.T.: 7.388 min
Delta R.T.: 0.002 min
Response: 106989
Conc: 34.43 ng/ml

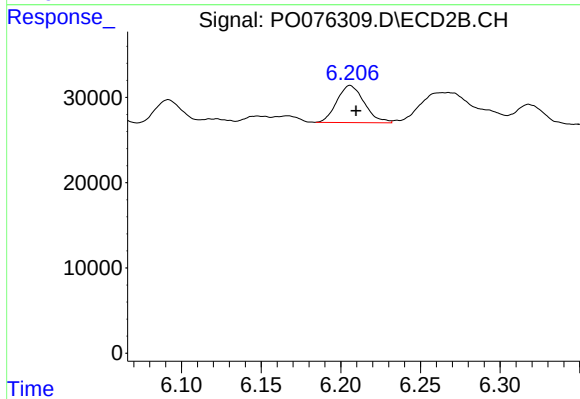

#27 AR-1254-2

R.T.: 6.206 min
Delta R.T.: -0.004 min
Response: 52085
Conc: 26.30 ng/ml

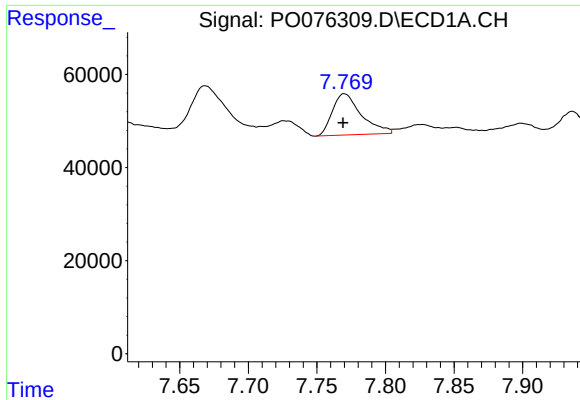


#28 AR-1254-3

R.T.: 7.770 min
Delta R.T.: 0.001 min
Response: 130347
Conc: 40.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-2


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:40 PM

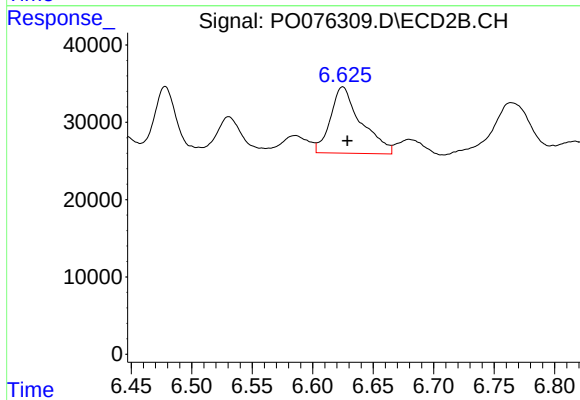


#28 AR-1254-3

R.T.: 6.625 min
Delta R.T.: -0.004 min
Response: 151052
Conc: 50.15 ng/ml

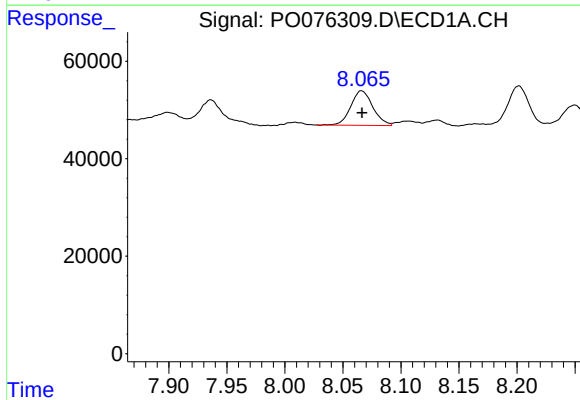


#29 AR-1254-4

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 94162
Conc: 44.94 ng/ml

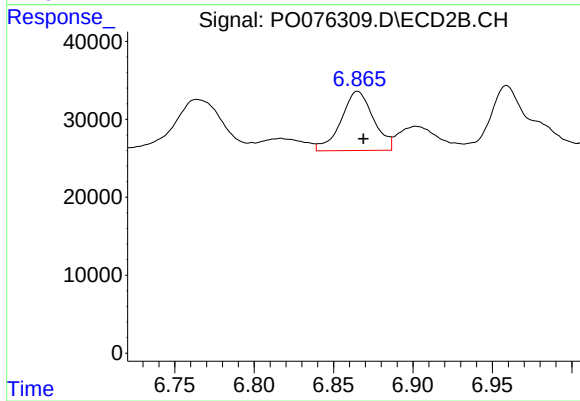

#29 AR-1254-4

R.T.: 6.865 min
Delta R.T.: -0.004 min
Response: 107834
Conc: 61.11 ng/ml

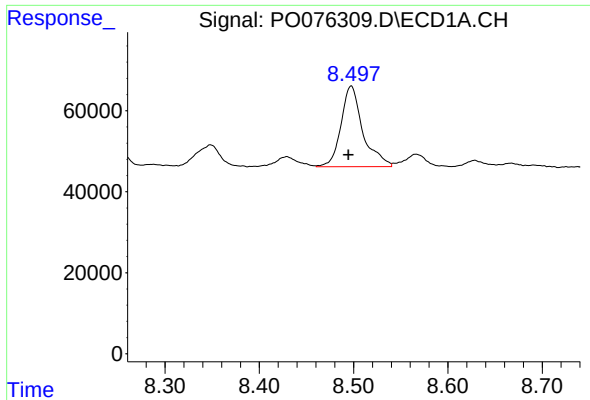


#30 AR-1254-5

R.T.: 8.497 min
Delta R.T.: 0.003 min
Response: 321775
Conc: 140.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERNAL-PAD-2

Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:40 PM

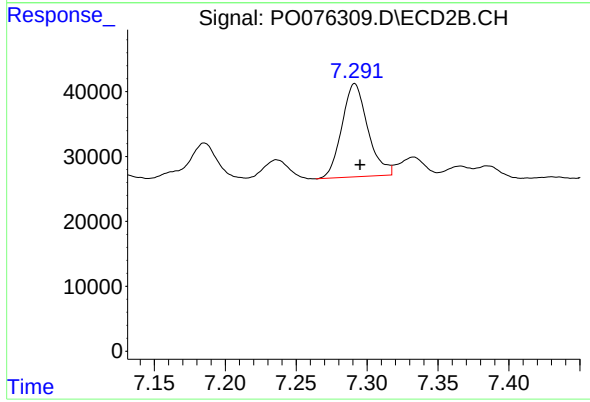

#30 AR-1254-5

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 182995
Conc: 69.90 ng/ml