

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
 Data File : P0076335.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 3:51
 Operator : DD\AJ
 Sample : M1702-01 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CT-1

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:35:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:46:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.934	154587	119607	2.721	2.867
2) SA Decachlor...	10.923	9.199	122441	116903	3.183	3.045
Target Compounds						
21) L5 AR-1248-1	6.247	5.180	15703	14949	16.656m	21.766m#
22) L5 AR-1248-2	6.539	5.441	18052	15962	11.983m	12.337m
23) L5 AR-1248-3	6.756	5.486	25979	17203	14.979m	13.459m
24) L5 AR-1248-4	7.185	5.668	20215	18664	11.490m	12.693m
25) L5 AR-1248-5	7.224	6.091	15224	15877	8.608m	10.266m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031821\
Data File : PO076335.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 3:51
Operator : DD\AJ
Sample : M1702-01 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CT-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:46:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

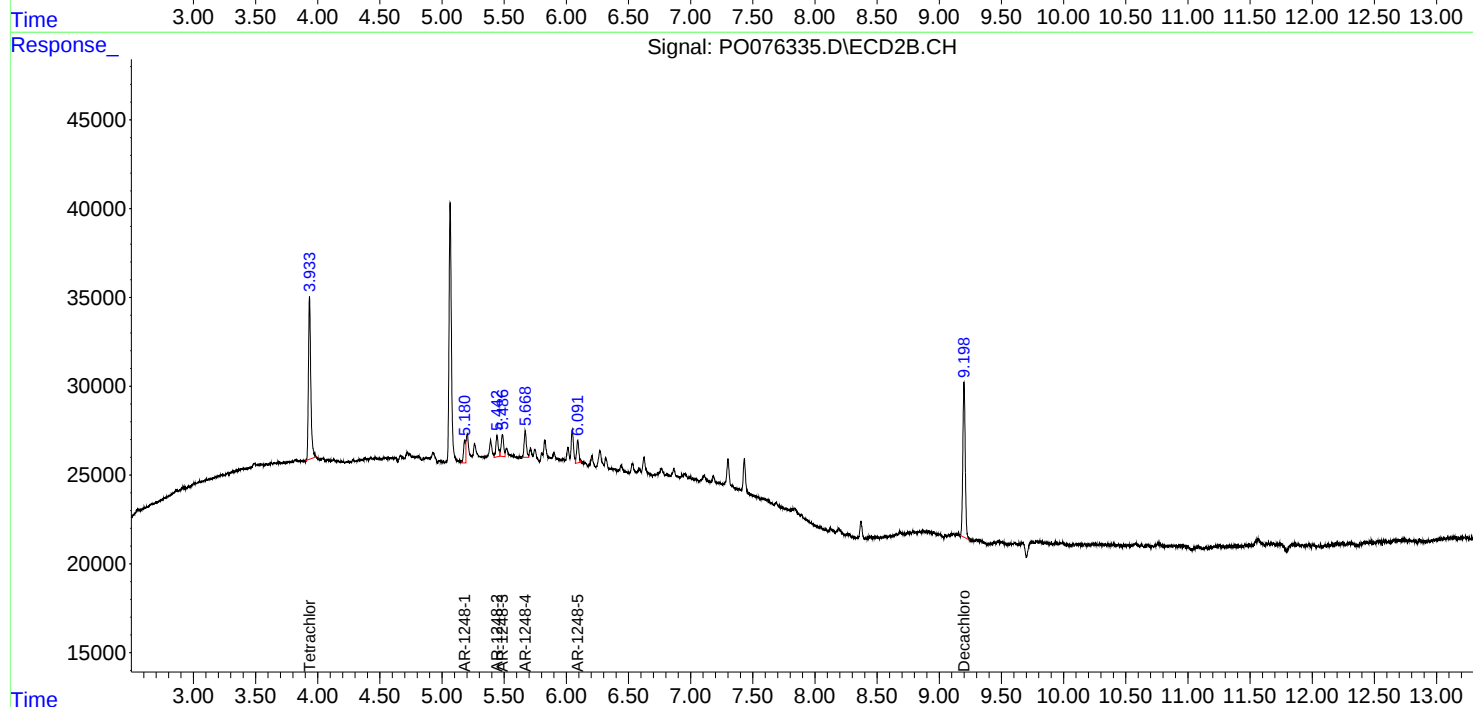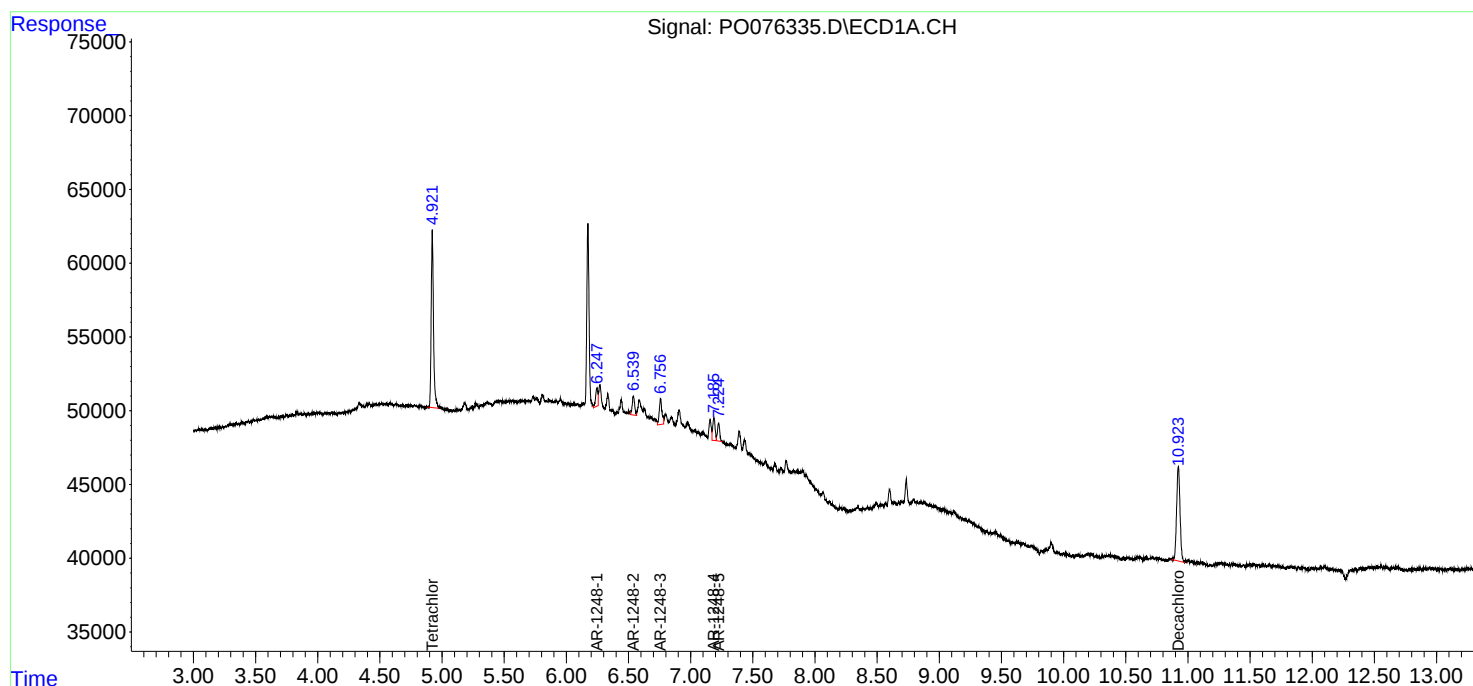

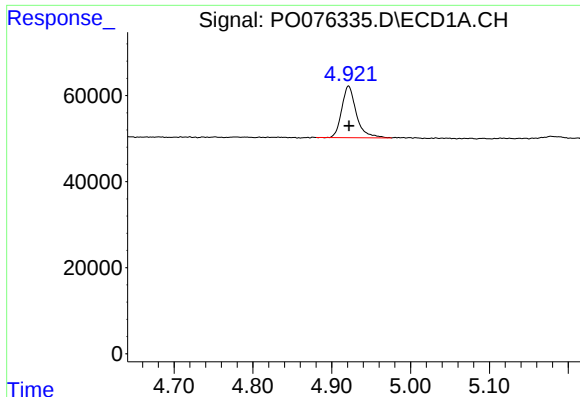


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 154587
Conc: 2.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
CT-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:55 PM

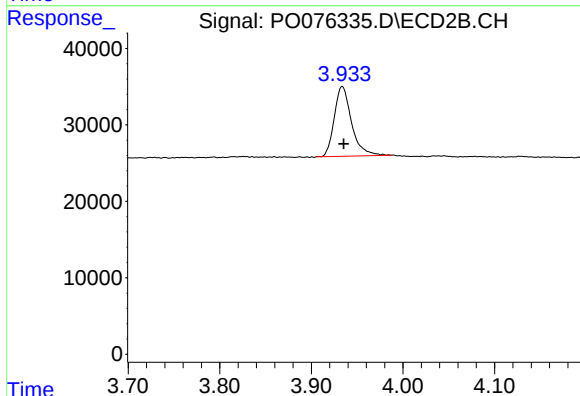


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 119607
Conc: 2.87 ng/ml

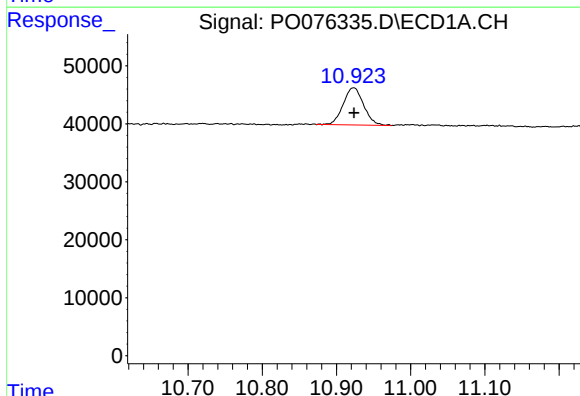


#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.000 min
Response: 122441
Conc: 3.18 ng/ml

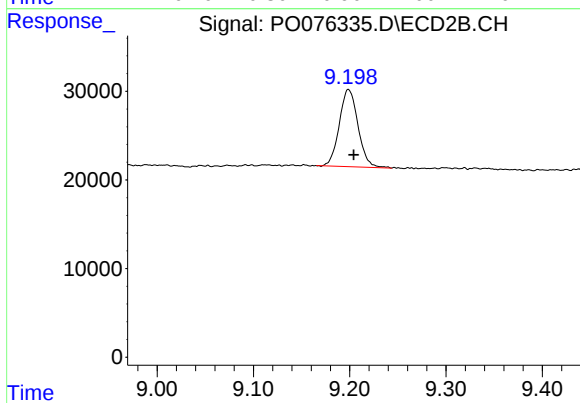

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.005 min
Response: 116903
Conc: 3.04 ng/ml

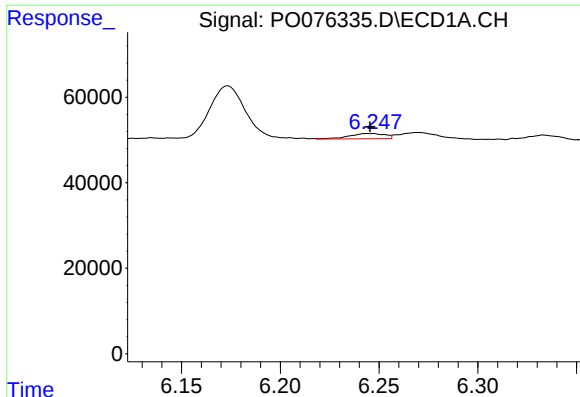


#21 AR-1248-1

R.T.: 6.247 min
Delta R.T.: 0.001 min
Response: 15703
Conc: 16.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:55 PM

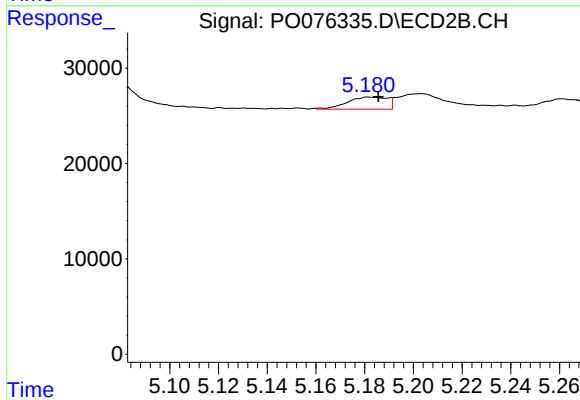


#21 AR-1248-1

R.T.: 5.180 min
Delta R.T.: -0.005 min
Response: 14949
Conc: 21.77 ng/ml m

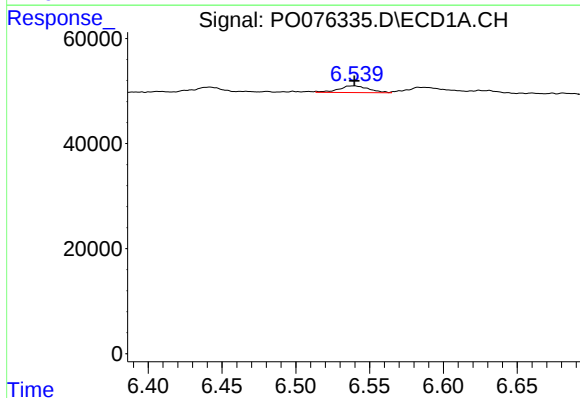


#22 AR-1248-2

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 18052
Conc: 11.98 ng/ml m

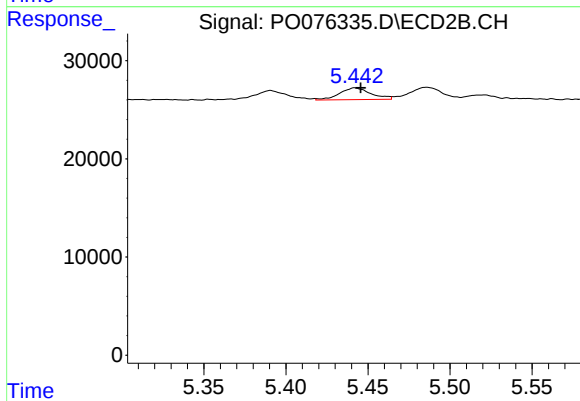

#22 AR-1248-2

R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 15962
Conc: 12.34 ng/ml m

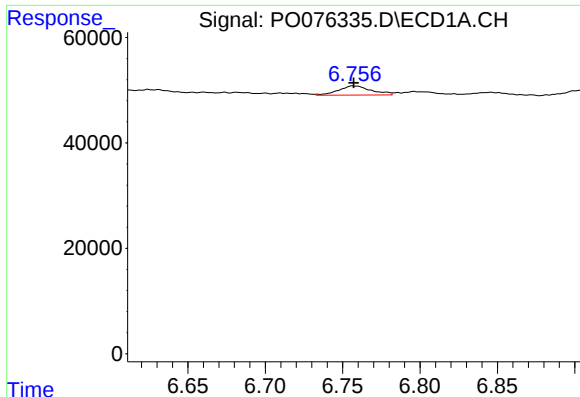


#23 AR-1248-3

R.T.: 6.756 min
Delta R.T.: -0.001 min
Response: 25979
Conc: 14.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-1


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:55 PM

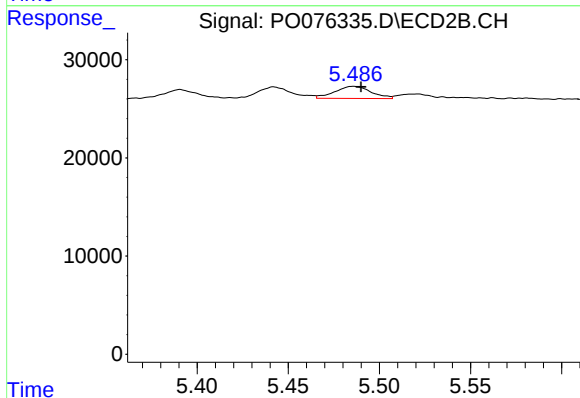


#23 AR-1248-3

R.T.: 5.486 min
Delta R.T.: -0.004 min
Response: 17203
Conc: 13.46 ng/ml m

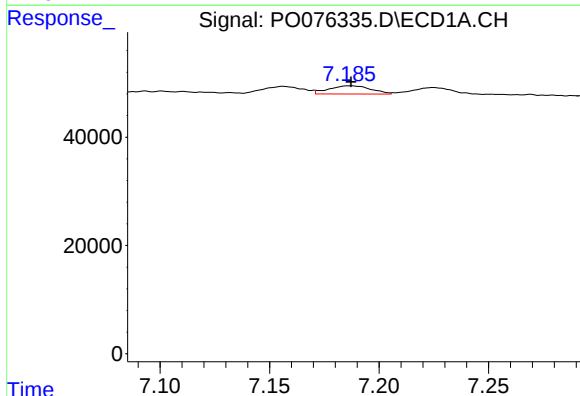


#24 AR-1248-4

R.T.: 7.185 min
Delta R.T.: -0.002 min
Response: 20215
Conc: 11.49 ng/ml m

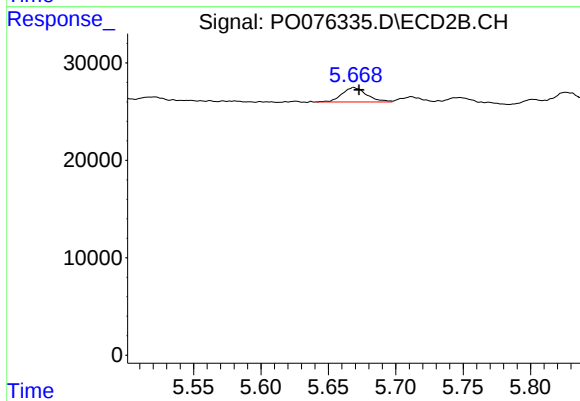

#24 AR-1248-4

R.T.: 5.668 min
Delta R.T.: -0.004 min
Response: 18664
Conc: 12.69 ng/ml m

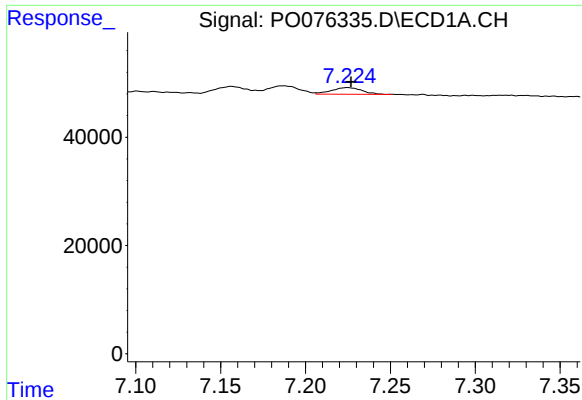


#25 AR-1248-5

R.T.: 7.224 min
Delta R.T.: -0.003 min
Response: 15224
Conc: 8.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-1

Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:55 PM

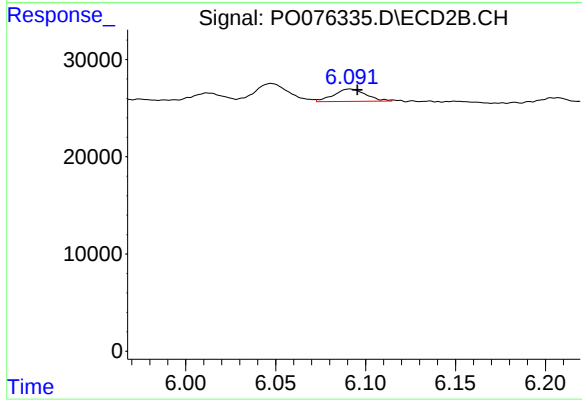

#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: -0.005 min
Response: 15877
Conc: 10.27 ng/ml m