

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
 Data File : P0076339.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 5:00
 Operator : DD\AJ
 Sample : M1702-05 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CT-5

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:36:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:47:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.934	135122	106125	2.379	2.544
2) SA Decachlor...	10.923	9.199	114313	106461	2.972	2.773
Target Compounds						
21) L5 AR-1248-1	6.249	5.183	16865	15512	17.888m	22.586m#
22) L5 AR-1248-2	6.540	5.441	15146	16484	10.054m	12.740m#
23) L5 AR-1248-3	6.757	5.486	17851	21662	10.292m	16.947m#
24) L5 AR-1248-4	7.186	5.668	21759	19150	12.368m	13.023m
25) L5 AR-1248-5	7.227	6.092	16028	16704	9.063m	10.801m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
Data File : P0076339.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 5:00
Operator : DD\AJ
Sample : M1702-05 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CT-5


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:47:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

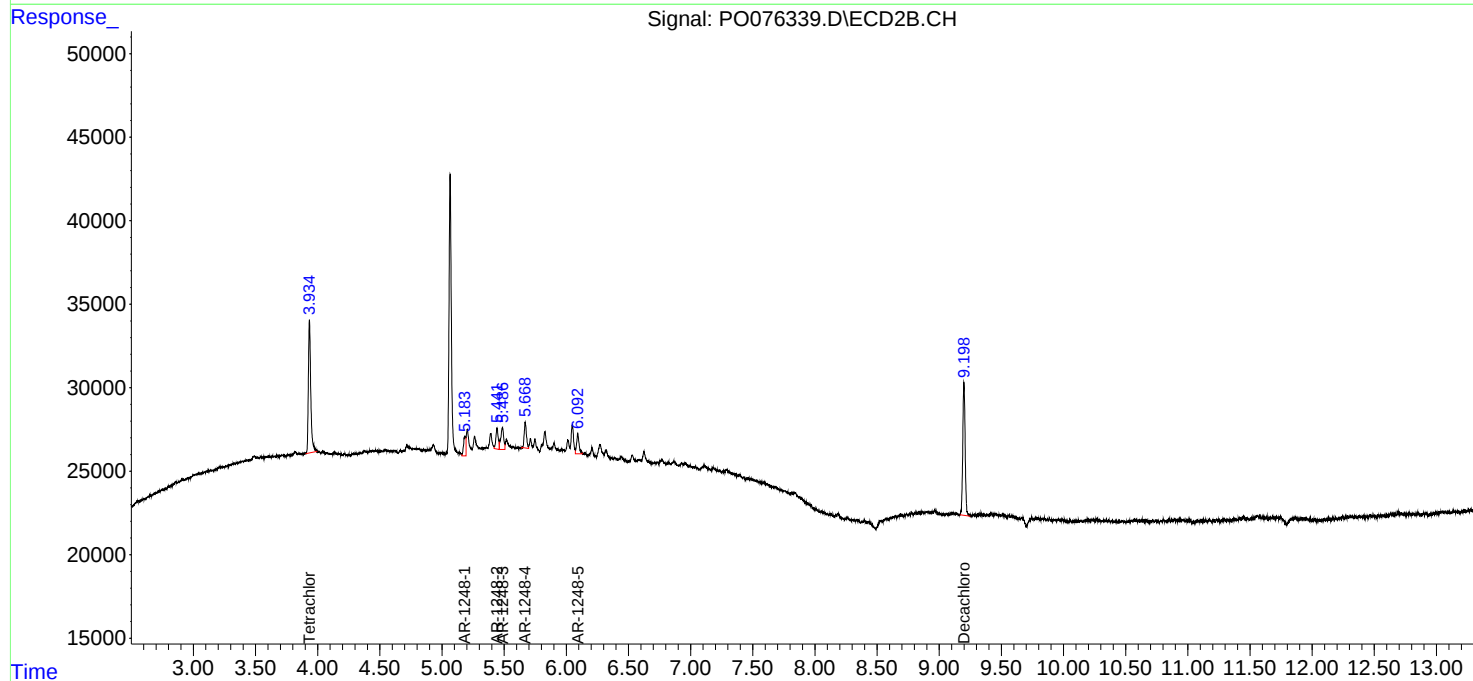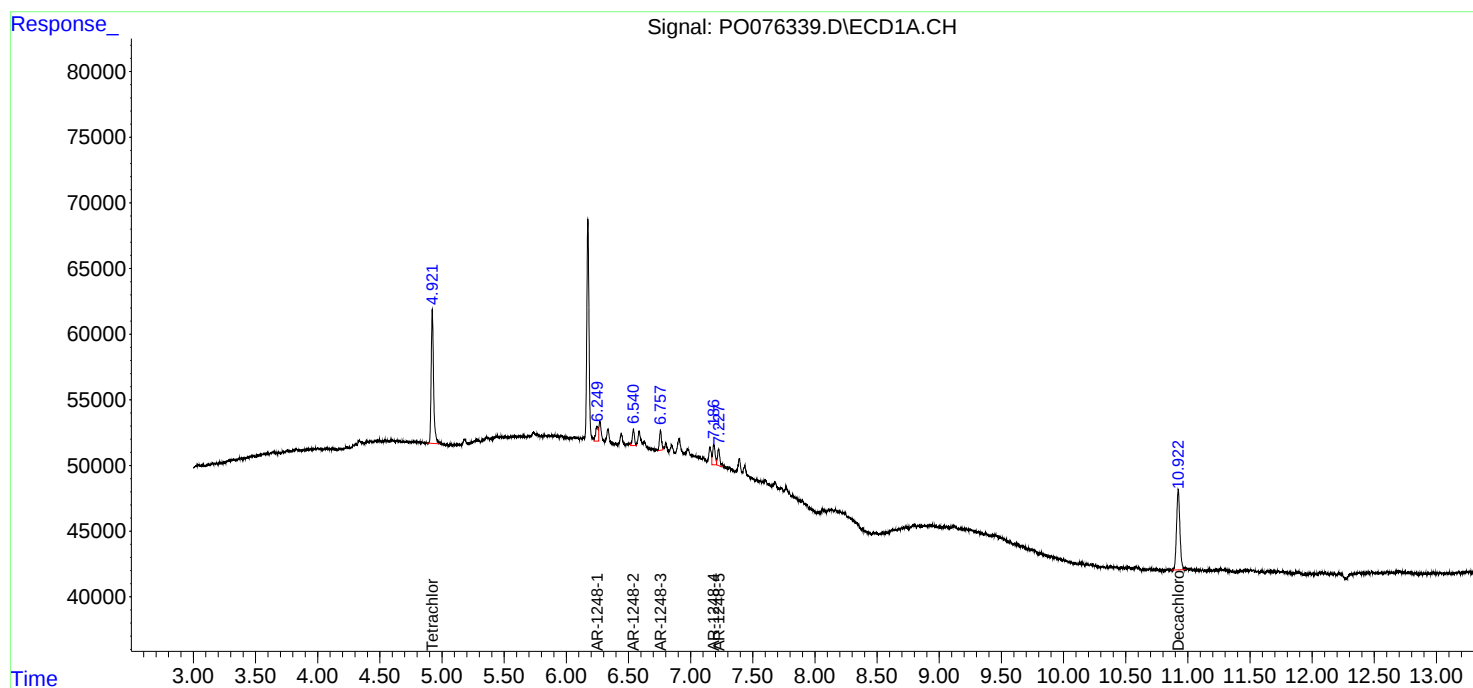

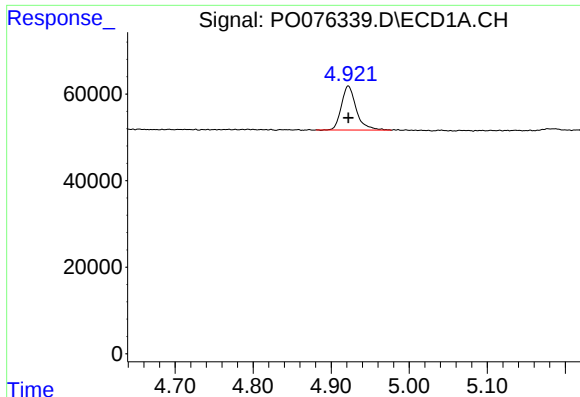


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 135122
Conc: 2.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
CT-5


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:01 PM

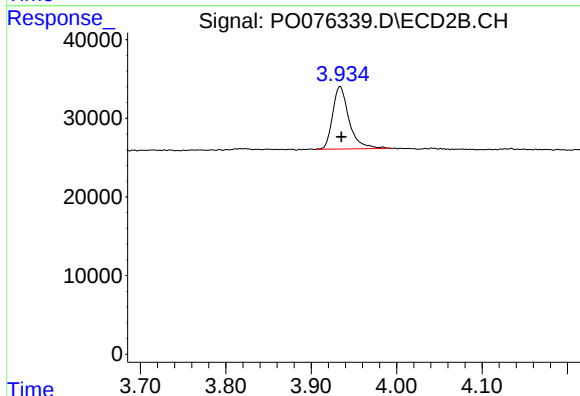


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 106125
Conc: 2.54 ng/ml

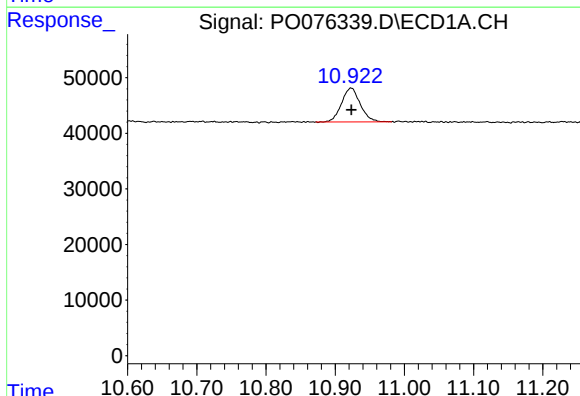


#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.000 min
Response: 114313
Conc: 2.97 ng/ml

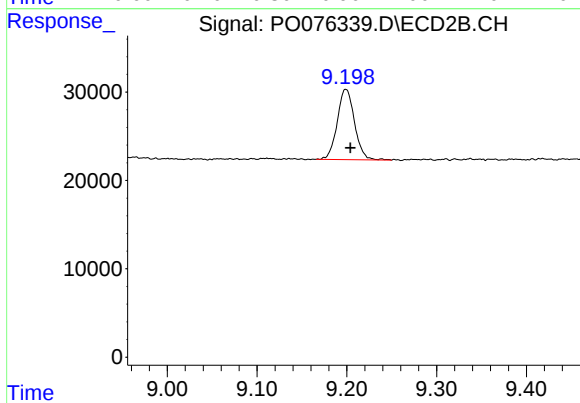

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.005 min
Response: 106461
Conc: 2.77 ng/ml

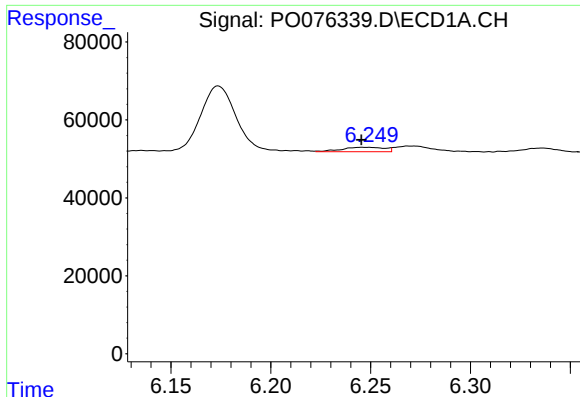


#21 AR-1248-1

R.T.: 6.249 min
Delta R.T.: 0.004 min
Response: 16865
Conc: 17.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-5


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:01 PM

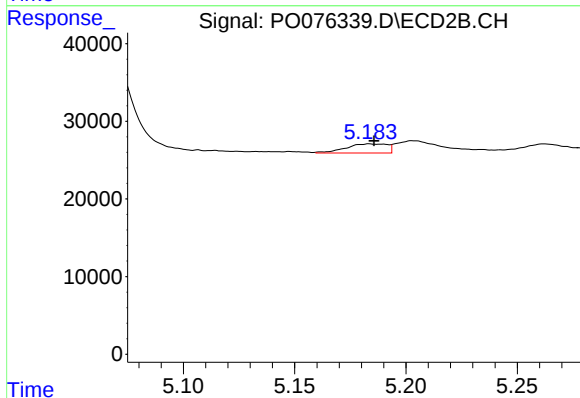


#21 AR-1248-1

R.T.: 5.183 min
Delta R.T.: -0.003 min
Response: 15512
Conc: 22.59 ng/ml m

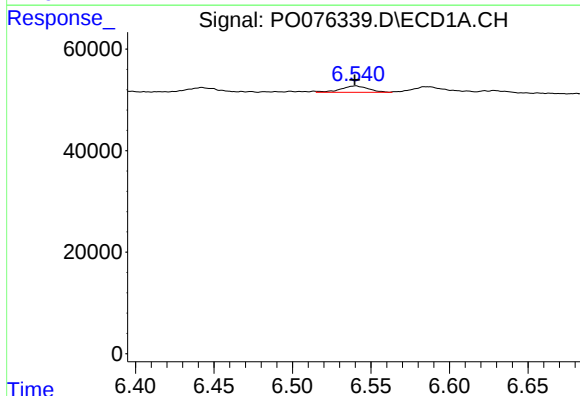


#22 AR-1248-2

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 15146
Conc: 10.05 ng/ml m

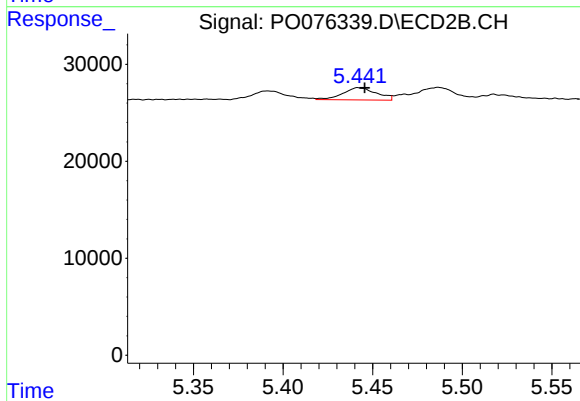

#22 AR-1248-2

R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 16484
Conc: 12.74 ng/ml m

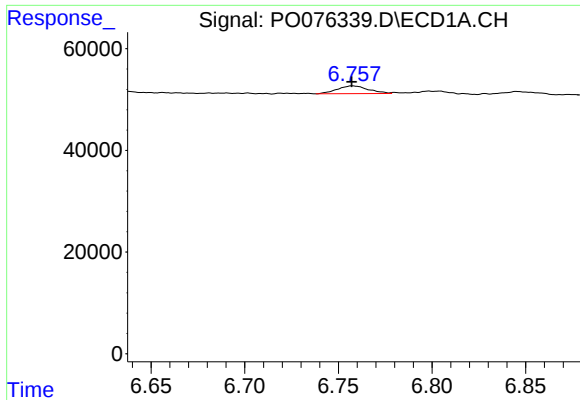


#23 AR-1248-3

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 17851
Conc: 10.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-5


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:01 PM

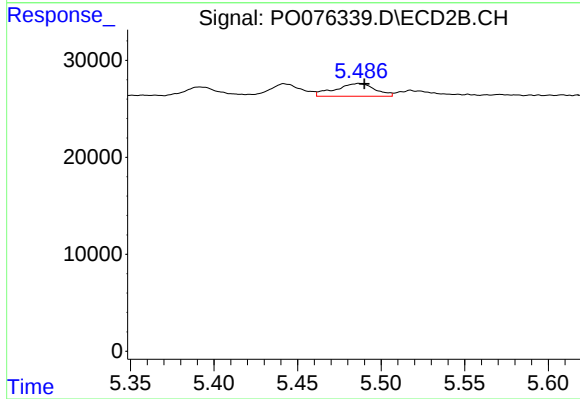


#23 AR-1248-3

R.T.: 5.486 min
Delta R.T.: -0.004 min
Response: 21662
Conc: 16.95 ng/ml m

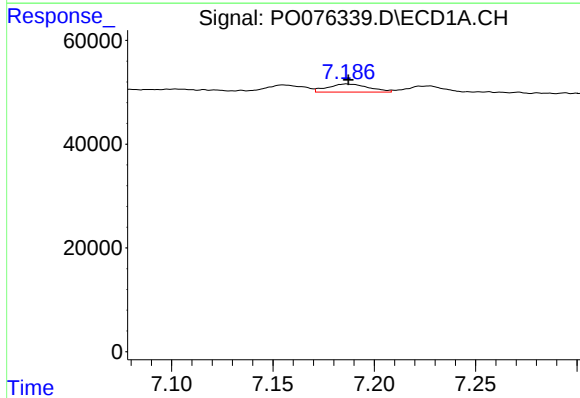


#24 AR-1248-4

R.T.: 7.186 min
Delta R.T.: -0.001 min
Response: 21759
Conc: 12.37 ng/ml m

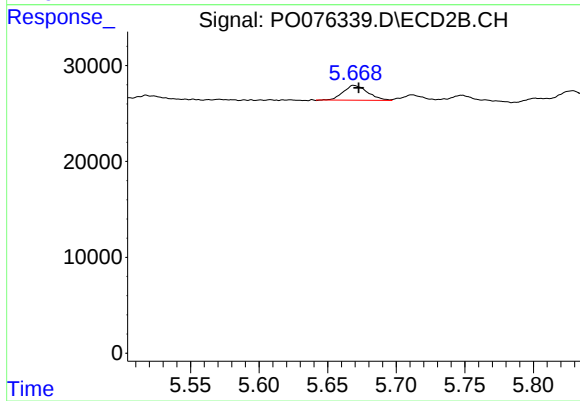

#24 AR-1248-4

R.T.: 5.668 min
Delta R.T.: -0.004 min
Response: 19150
Conc: 13.02 ng/ml m

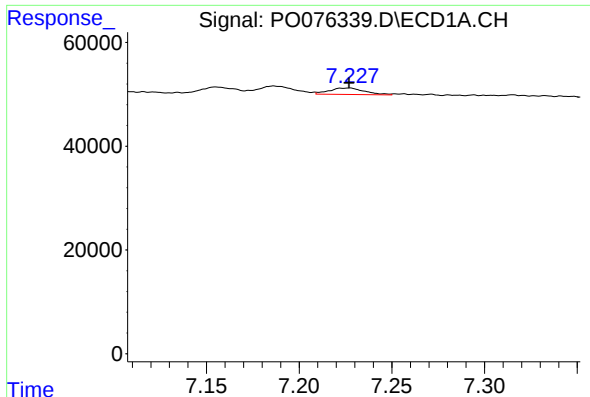


#25 AR-1248-5

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 16028
Conc: 9.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CT-5

Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:01 PM

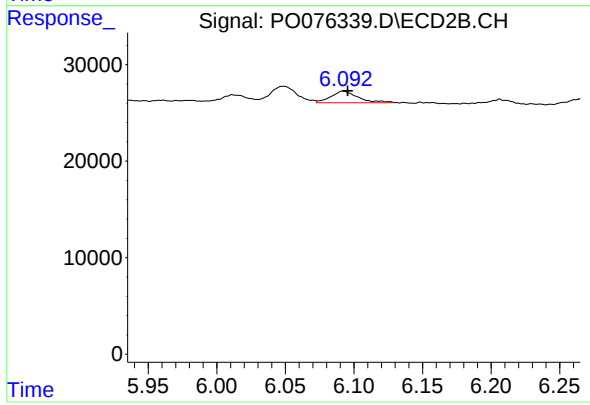

#25 AR-1248-5

R.T.: 6.092 min
Delta R.T.: -0.003 min
Response: 16704
Conc: 10.80 ng/ml m