

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
 Data File : P0076345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 7:17
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:36:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 07:50:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.934	3127655	2233927	55.055	53.544
2) SA Decachlor...	10.923	9.199	2292549	2075586	59.603	54.055
Target Compounds						
26) L6 AR-1254-1	7.156	6.047	1053212	1222133	513.912m	534.731
27) L6 AR-1254-2	7.386	6.207	1681655	1108295	541.151m	559.590
28) L6 AR-1254-3	7.769	6.625	1789508	1682053	562.486m	558.444
29) L6 AR-1254-4	8.066	6.865	1217017	943955	580.875m	534.914
30) L6 AR-1254-5	8.494	7.292	1333492	1491744	580.619	569.787

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031821\
Data File : PO076345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 7:17
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 07:50:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

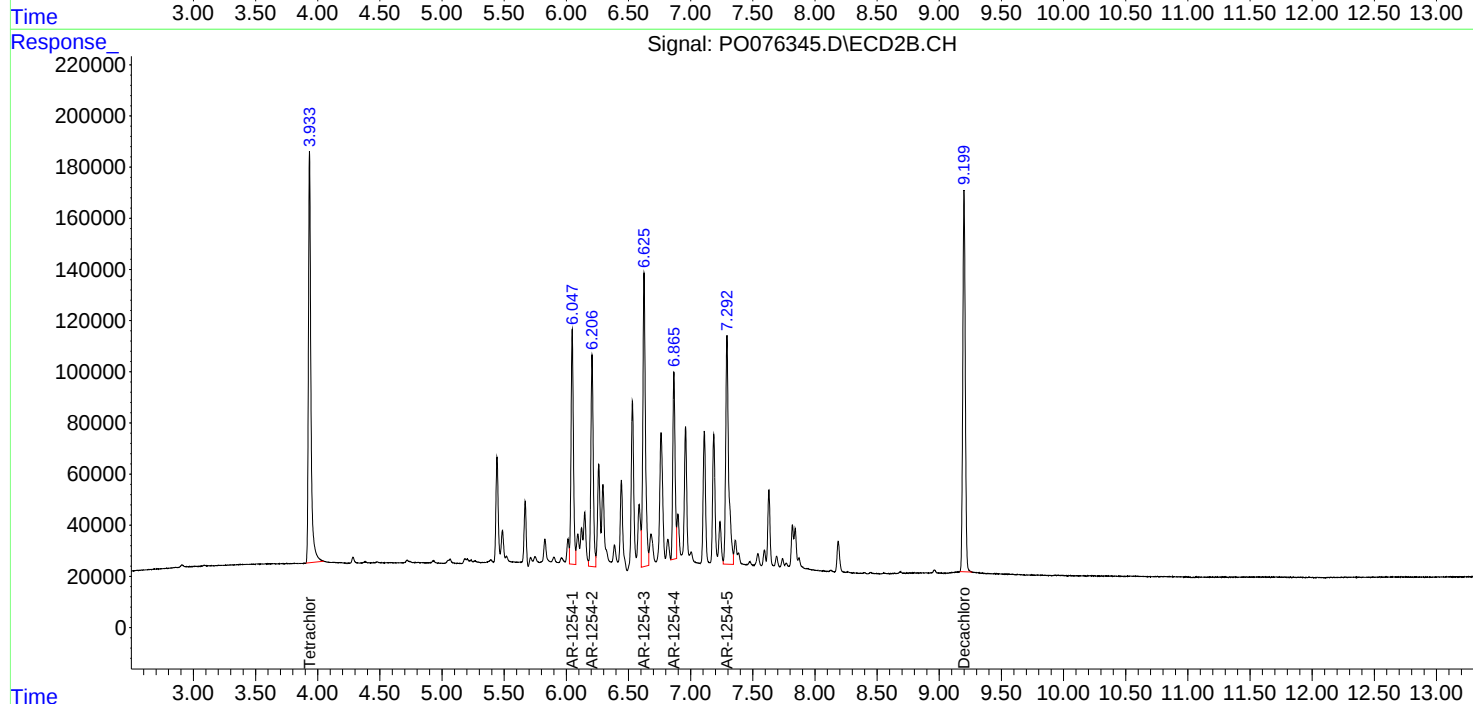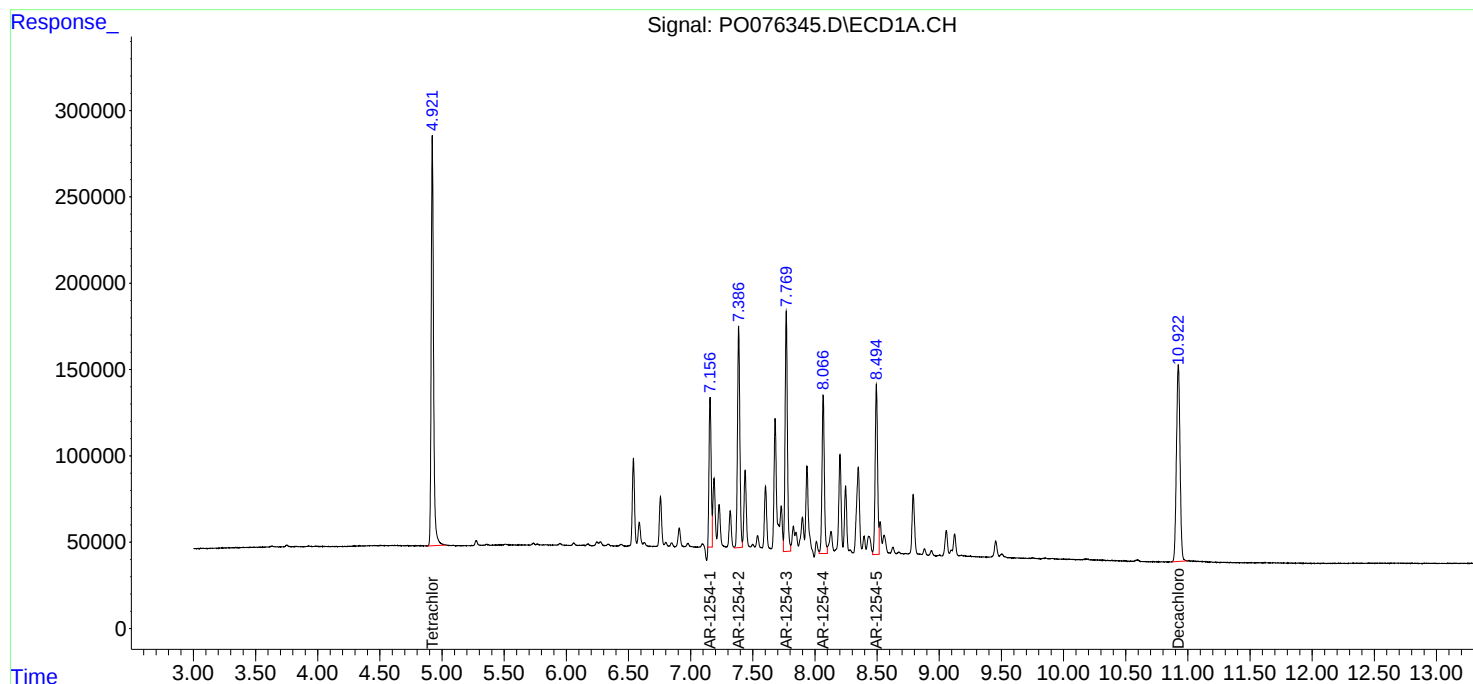

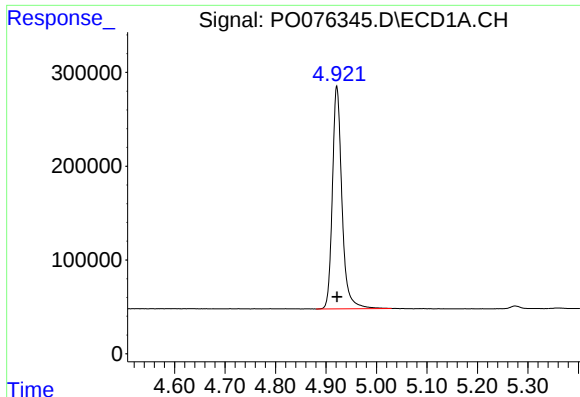


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 3127655
Conc: 55.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:05 PM

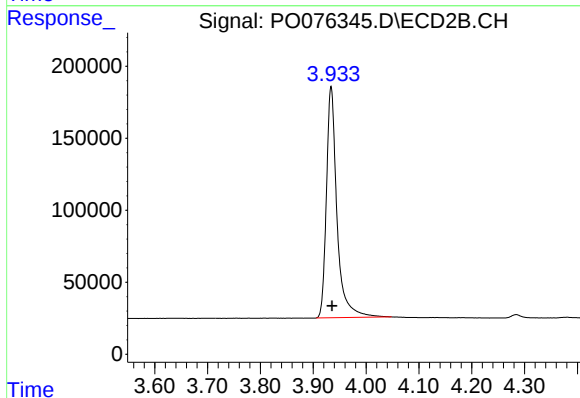


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 2233927
Conc: 53.54 ng/ml

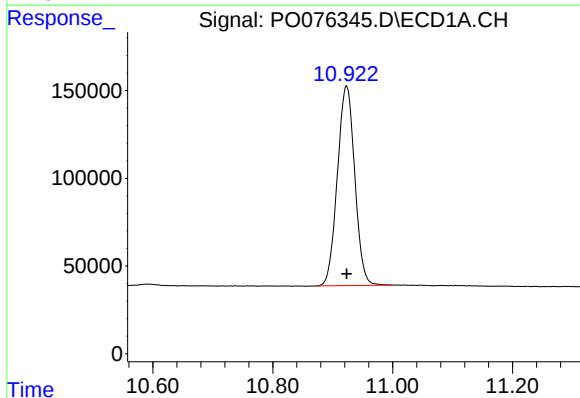


#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.000 min
Response: 2292549
Conc: 59.60 ng/ml

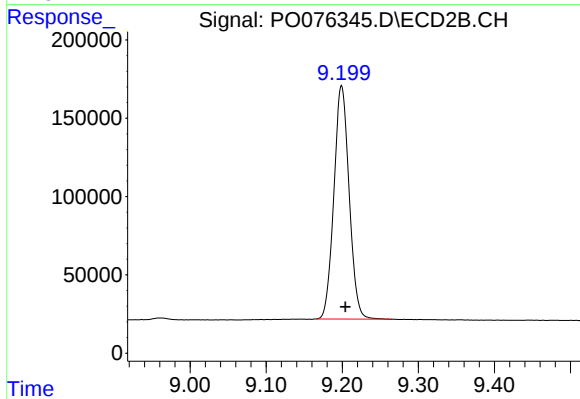

#2 Decachlorobiphenyl

R.T.: 9.199 min
Delta R.T.: -0.005 min
Response: 2075586
Conc: 54.06 ng/ml

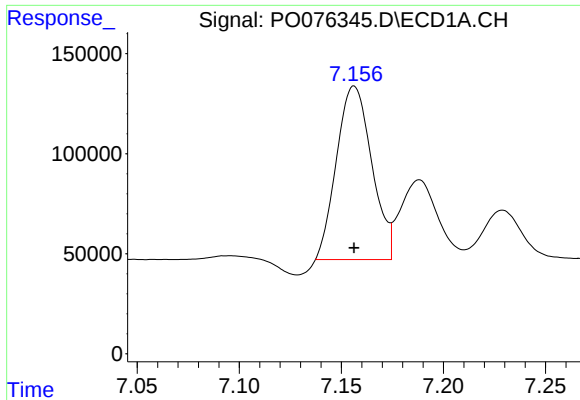


#26 AR-1254-1

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 1053212
Conc: 513.91 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:05 PM

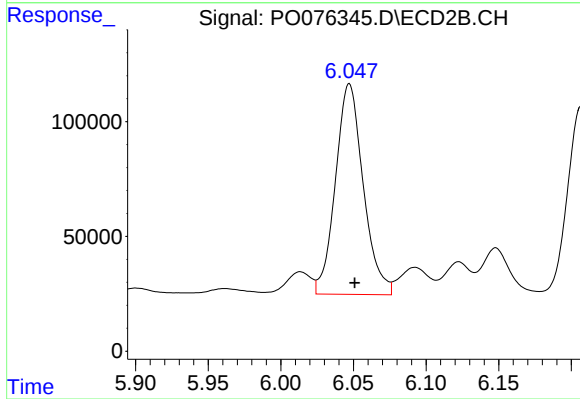


#26 AR-1254-1

R.T.: 6.047 min
Delta R.T.: -0.004 min
Response: 1222133
Conc: 534.73 ng/ml

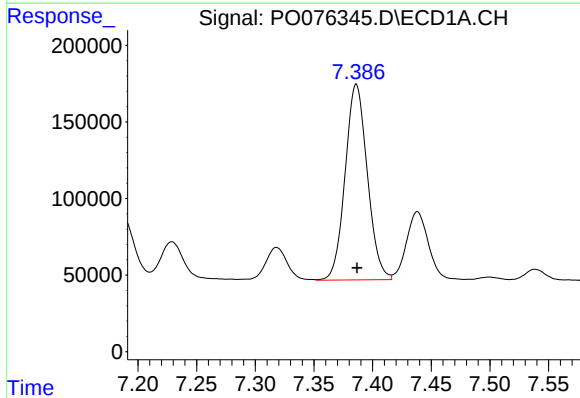


#27 AR-1254-2

R.T.: 7.386 min
Delta R.T.: 0.000 min
Response: 1681655
Conc: 541.15 ng/ml m

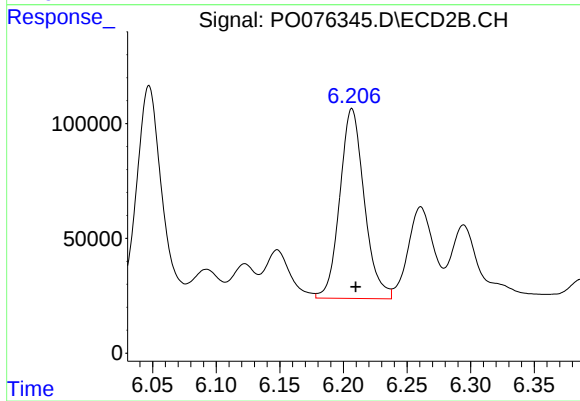

#27 AR-1254-2

R.T.: 6.207 min
Delta R.T.: -0.003 min
Response: 1108295
Conc: 559.59 ng/ml

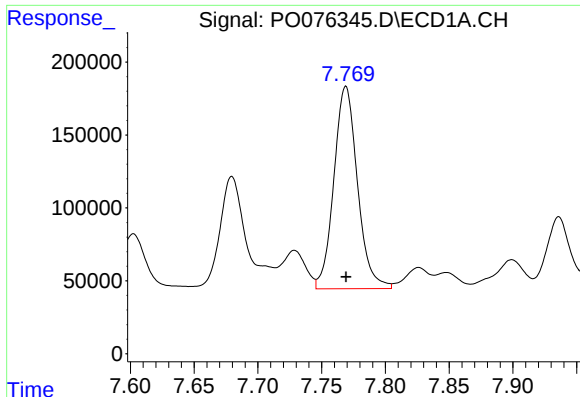


#28 AR-1254-3

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 1789508
Conc: 562.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:05 PM

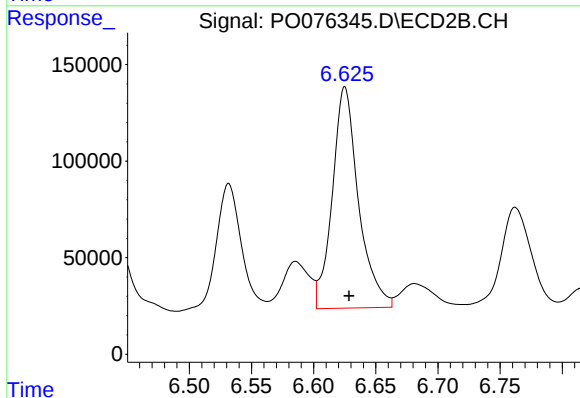


#28 AR-1254-3

R.T.: 6.625 min
Delta R.T.: -0.003 min
Response: 1682053
Conc: 558.44 ng/ml

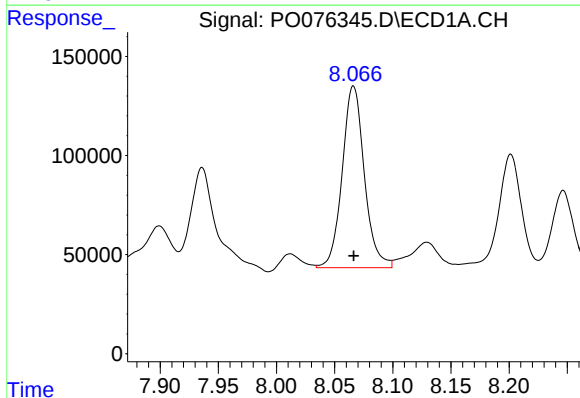


#29 AR-1254-4

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 1217017
Conc: 580.88 ng/ml m

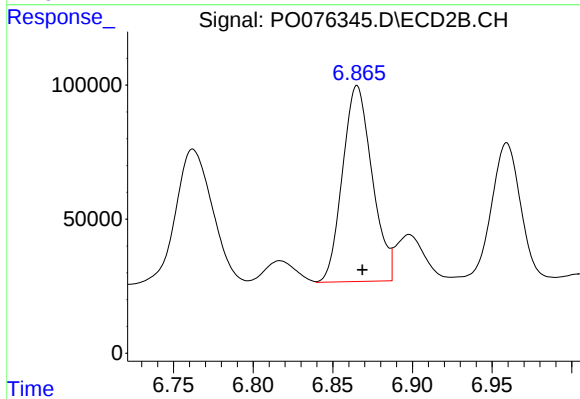

#29 AR-1254-4

R.T.: 6.865 min
Delta R.T.: -0.003 min
Response: 943955
Conc: 534.91 ng/ml

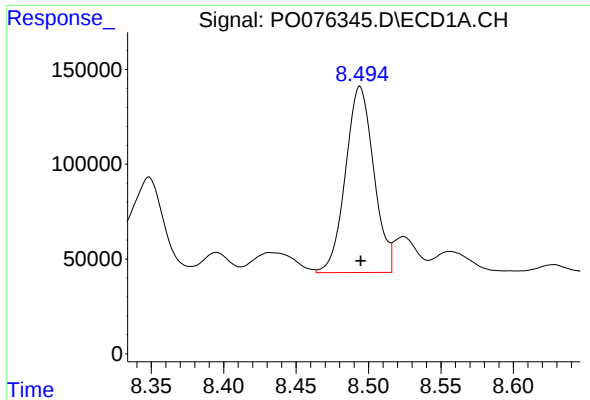


#30 AR-1254-5

R.T.: 8.494 min
Delta R.T.: 0.000 min
Response: 1333492
Conc: 580.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
3/19/2021 2:36:05 PM

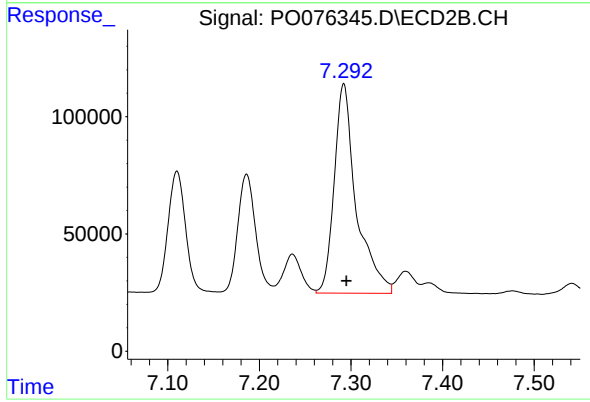

#30 AR-1254-5

R.T.: 7.292 min
Delta R.T.: -0.003 min
Response: 1491744
Conc: 569.79 ng/ml