

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031822\
 Data File : P0085515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2022 22:51
 Operator : YP\AJ
 Sample : N1958-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 C-7-6-7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/21/2022
 Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:22:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.590	3128185	758917	15.298m	17.714
2) SA Decachlor...	10.392	8.607	1755576	566494	14.605	14.755
Target Compounds						
26) L6 AR-1254-1	6.545	5.481	206937	71359	31.225	27.151
27) L6 AR-1254-2	6.770	5.629	479739	83084	47.937	35.607 #
28) L6 AR-1254-3	7.140	6.032	305570	130316	29.691m	35.481
29) L6 AR-1254-4	7.428	6.262	246039	63768	35.069	28.788
30) L6 AR-1254-5	7.852	6.681	350435	241242	45.799	74.165 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031822\
Data File : P0085515.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2022 22:51
Operator : YP\AJ
Sample : N1958-07
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C-7-6-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2022
Supervised By :mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:22:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

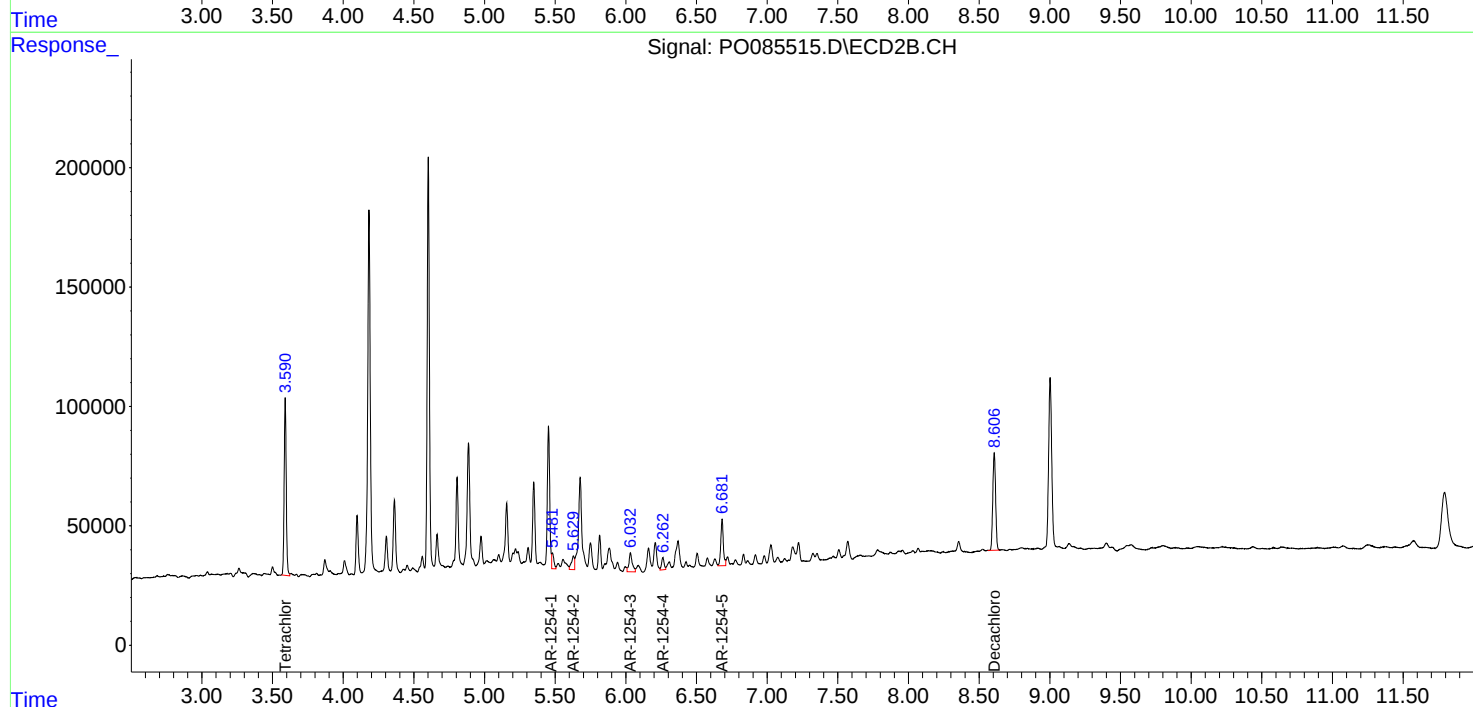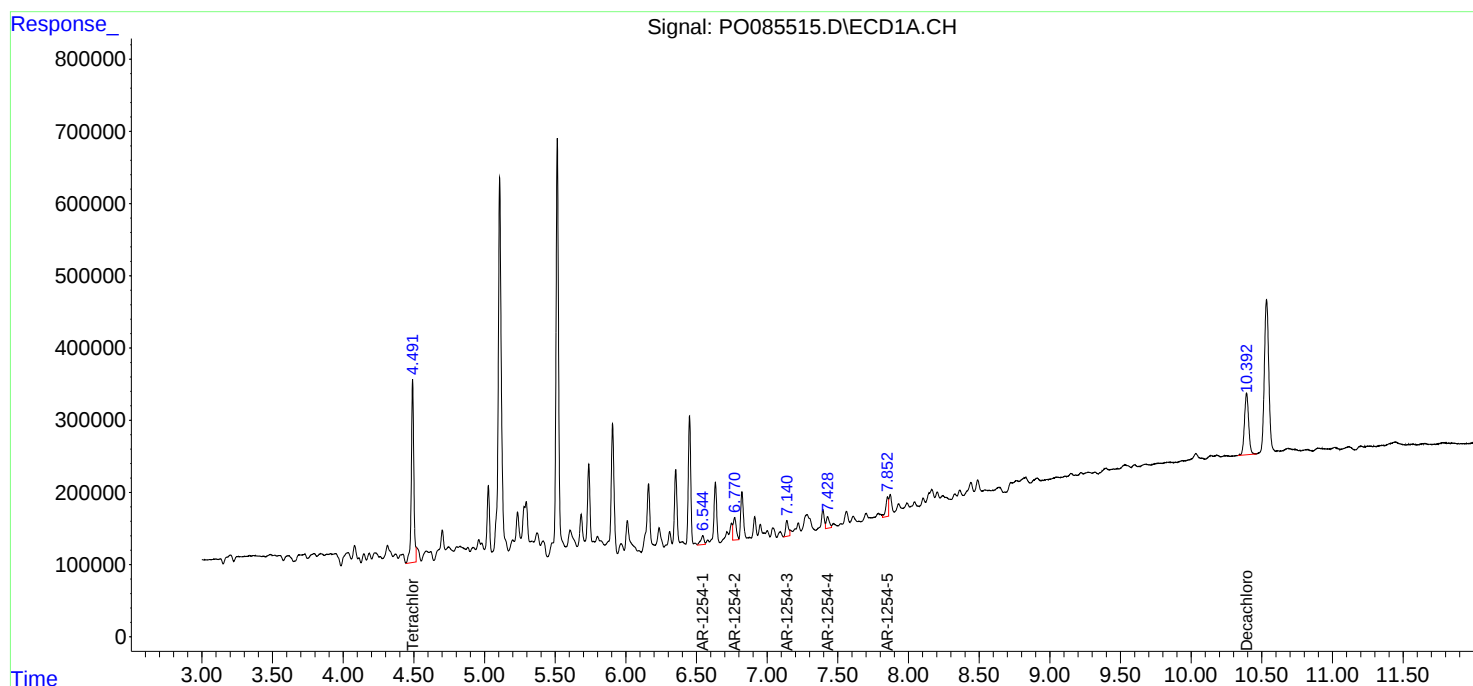

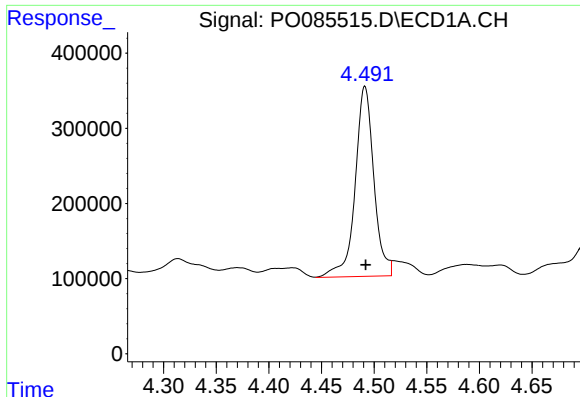


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.001 min
Response: 3128185
Conc: 15.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-7-6-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2022
Supervised By :mohammad ahmed 03/23/2022

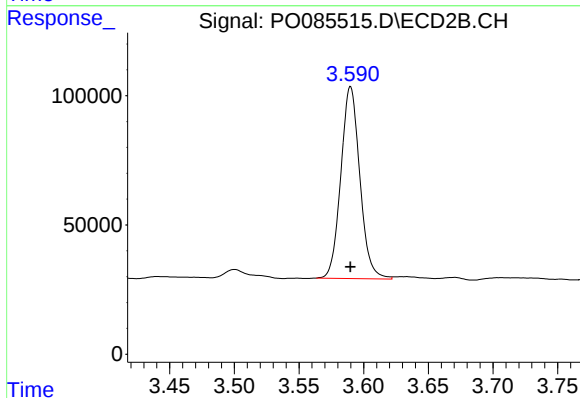


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: 0.000 min
Response: 758917
Conc: 17.71 ng/ml

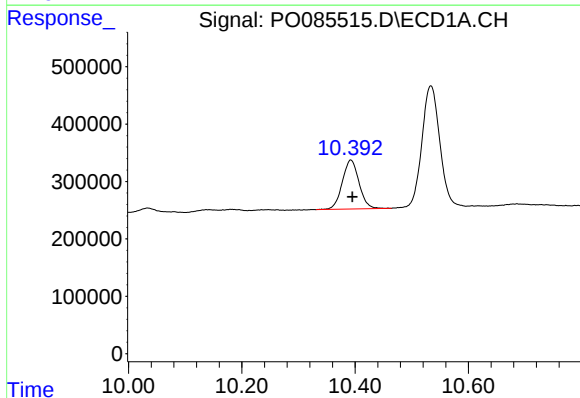


#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.003 min
Response: 1755576
Conc: 14.60 ng/ml

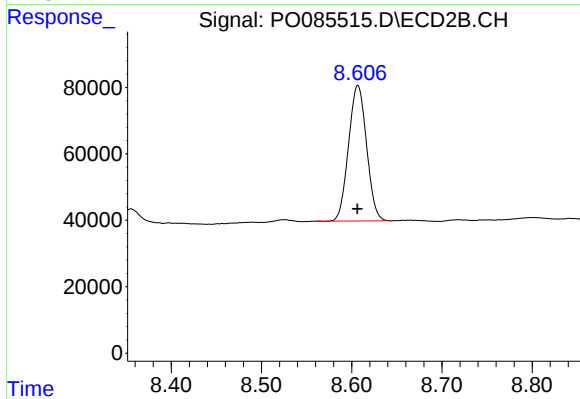

#2 Decachlorobiphenyl

R.T.: 8.607 min
Delta R.T.: 0.000 min
Response: 566494
Conc: 14.76 ng/ml

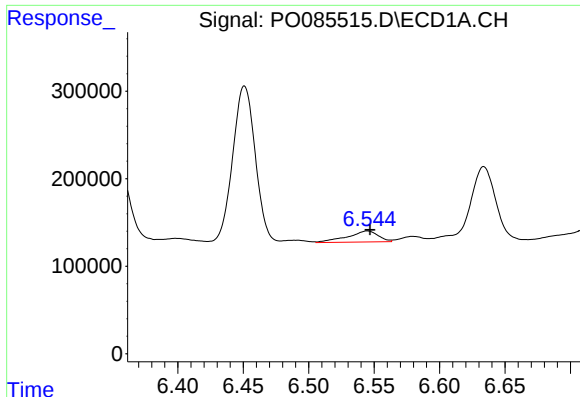


#26 AR-1254-1

R.T.: 6.545 min
Delta R.T.: -0.002 min
Response: 206937
Conc: 31.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-7-6-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2022
Supervised By :mohammad ahmed 03/23/2022

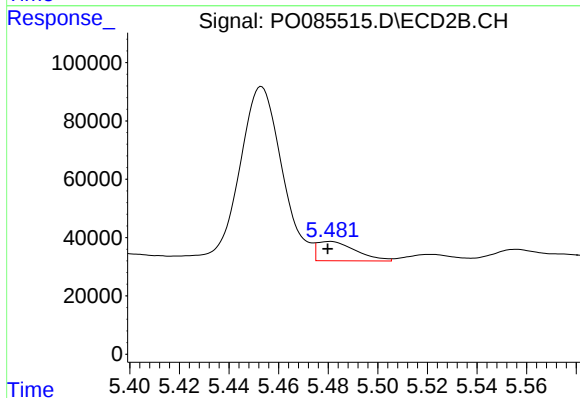


#26 AR-1254-1

R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 71359
Conc: 27.15 ng/ml

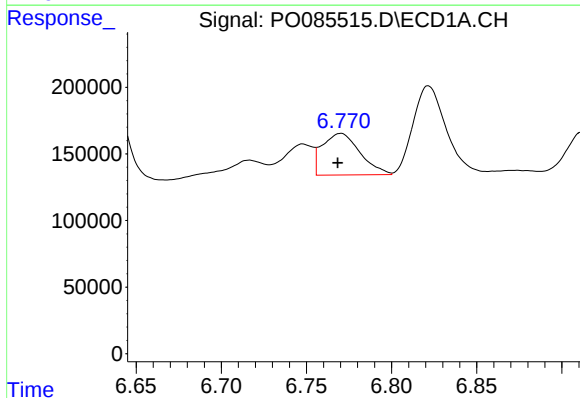


#27 AR-1254-2

R.T.: 6.770 min
Delta R.T.: 0.002 min
Response: 479739
Conc: 47.94 ng/ml

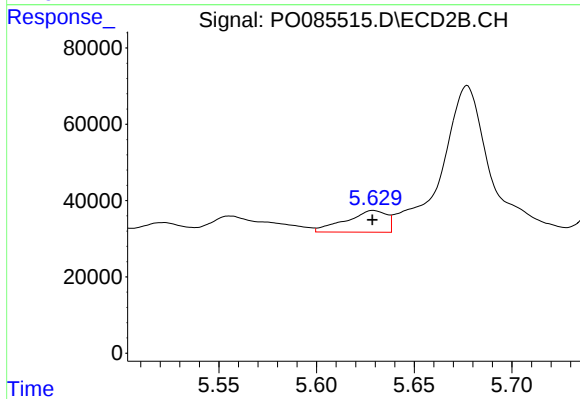

#27 AR-1254-2

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 83084
Conc: 35.61 ng/ml

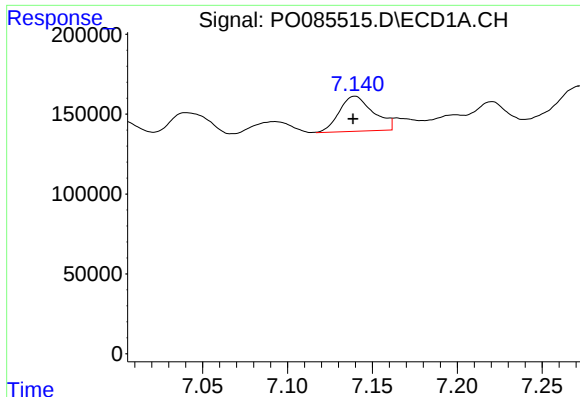


#28 AR-1254-3

R.T.: 7.140 min
Delta R.T.: 0.001 min
Response: 305570
Conc: 29.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-7-6-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2022
Supervised By :mohammad ahmed 03/23/2022

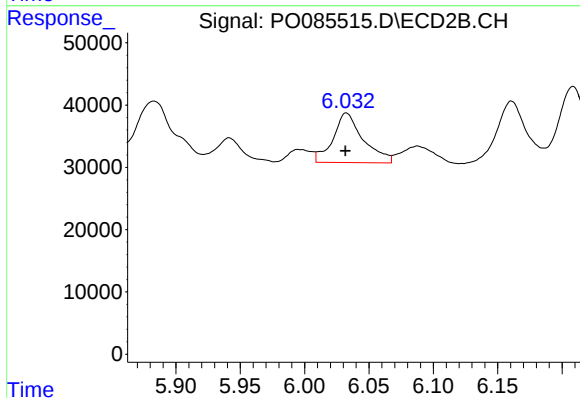


#28 AR-1254-3

R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 130316
Conc: 35.48 ng/ml

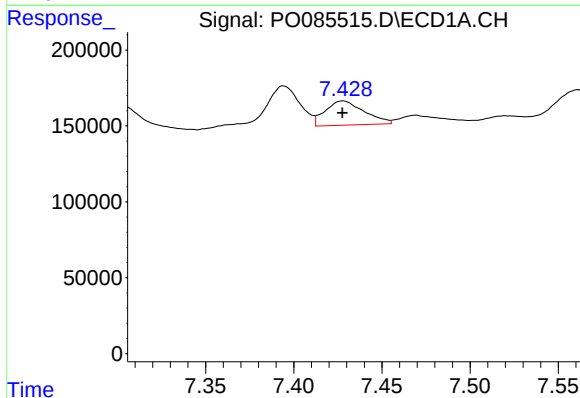


#29 AR-1254-4

R.T.: 7.428 min
Delta R.T.: 0.000 min
Response: 246039
Conc: 35.07 ng/ml

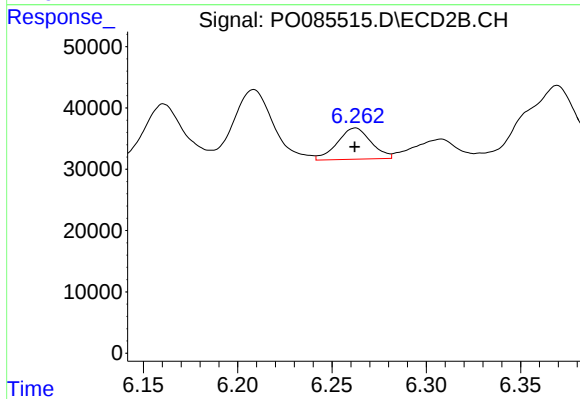

#29 AR-1254-4

R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 63768
Conc: 28.79 ng/ml

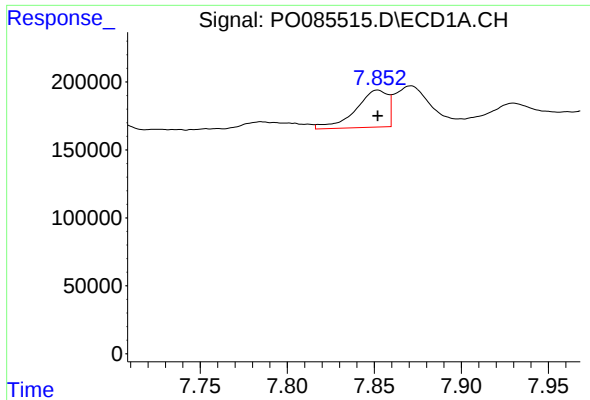


#30 AR-1254-5

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 350435
Conc: 45.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-7-6-7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2022
Supervised By :mohammad ahmed 03/23/2022

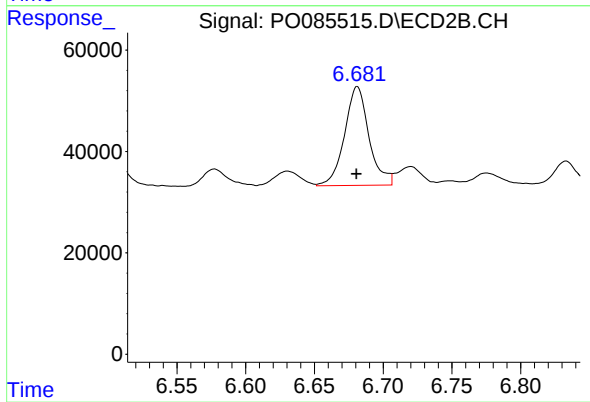

#30 AR-1254-5

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 241242
Conc: 74.16 ng/ml