

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076374.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 17:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 22:38:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.920	3.932	1122162	835325	19.753	20.022
2) SA Decachlor...	10.917	9.194	953408	848559	24.787	22.099
Target Compounds						
29) L6 AR-1254-4	8.065	0.000	76770	0	36.642	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076374.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 17:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 22:38:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

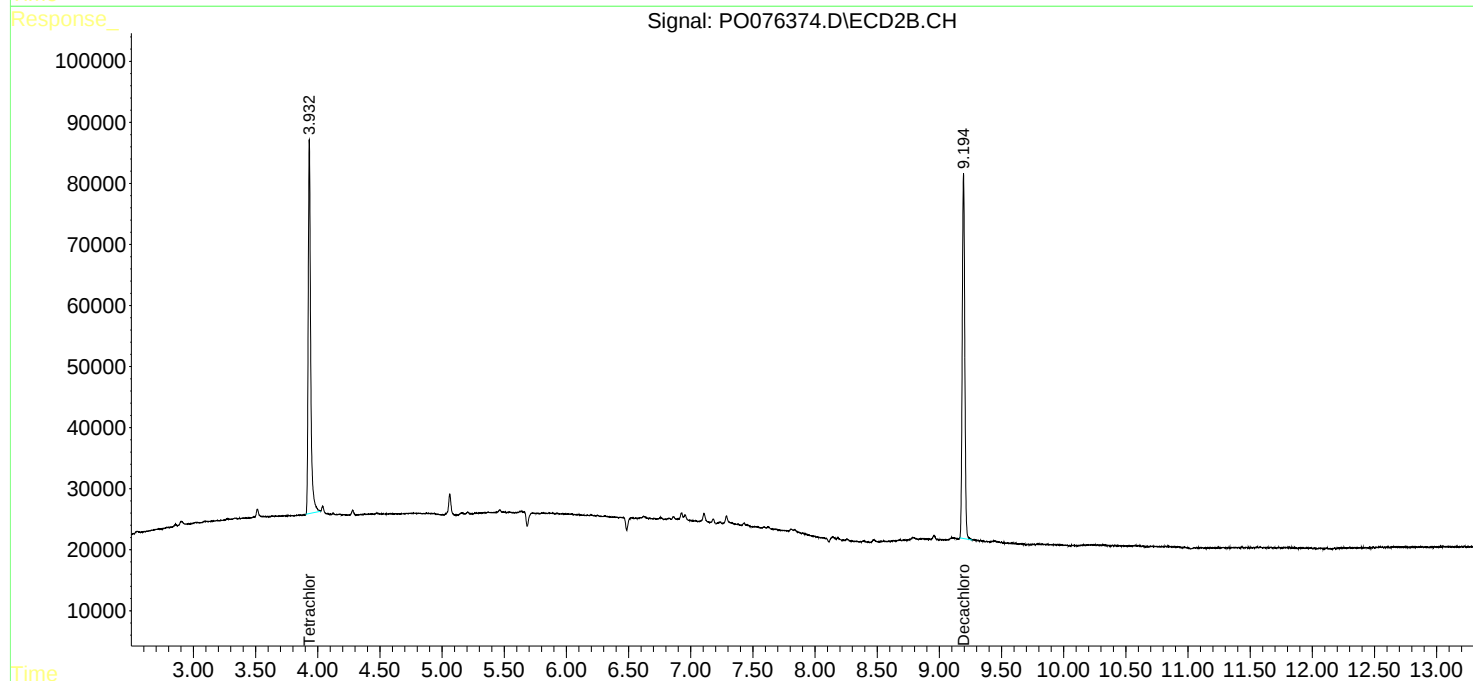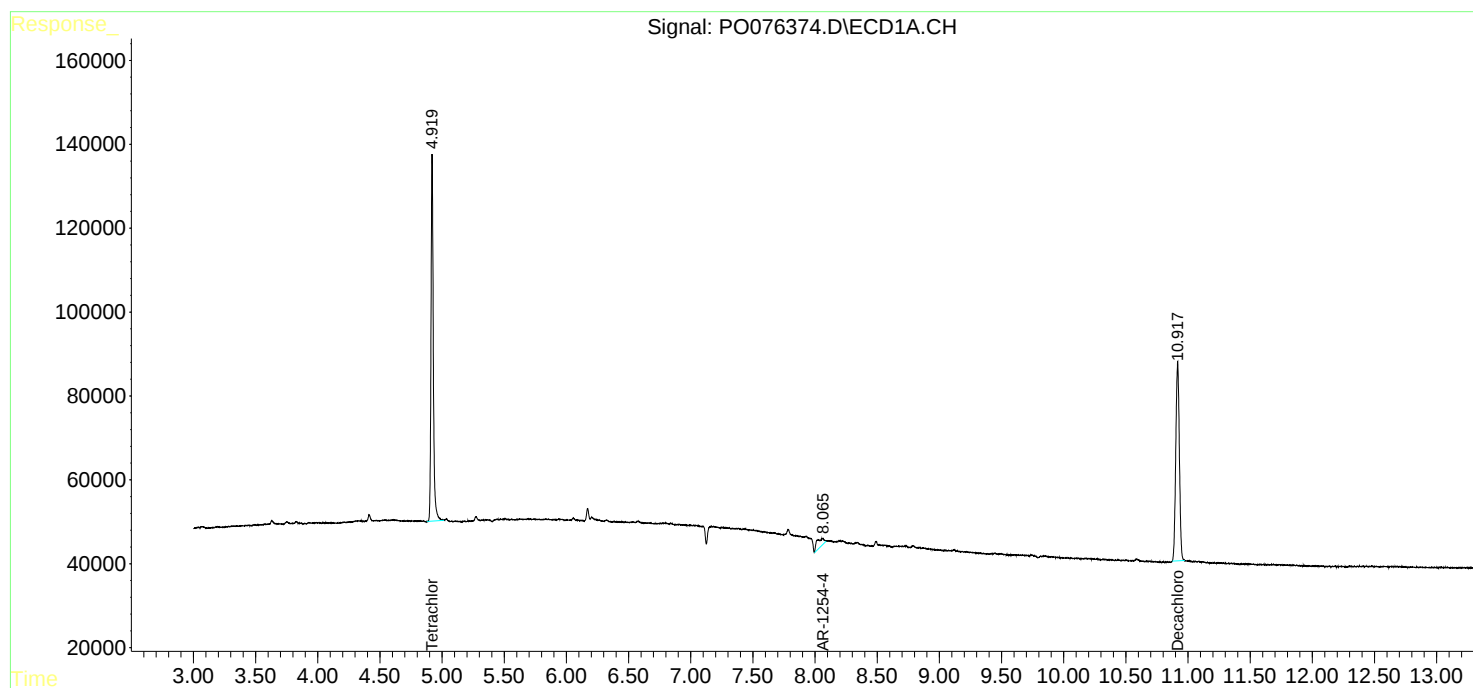


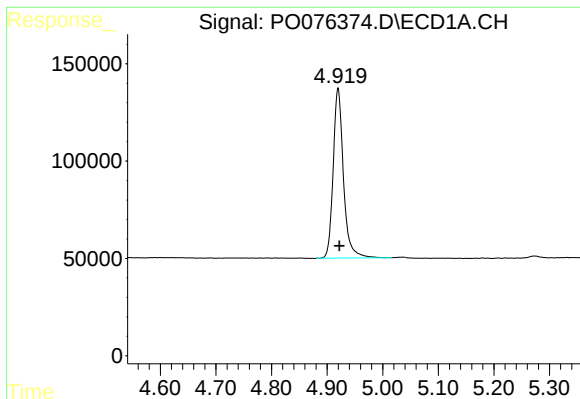

#1 Tetrachloro-m-xylene


R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 1122162
Conc: 19.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

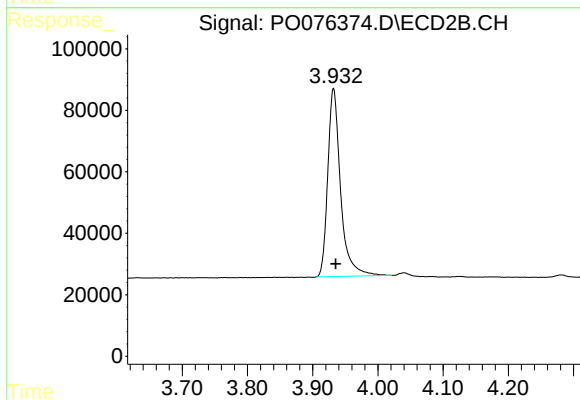


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 835325
Conc: 20.02 ng/ml

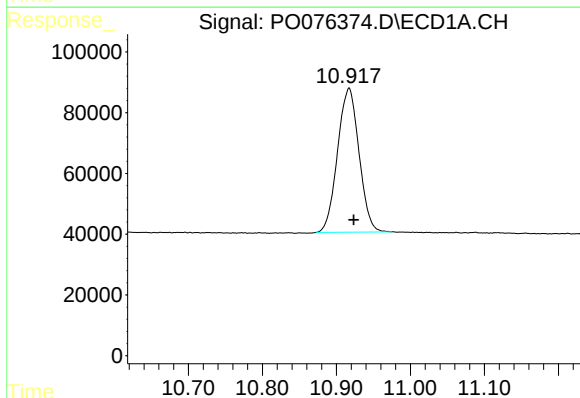


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: -0.006 min
Response: 953408
Conc: 24.79 ng/ml

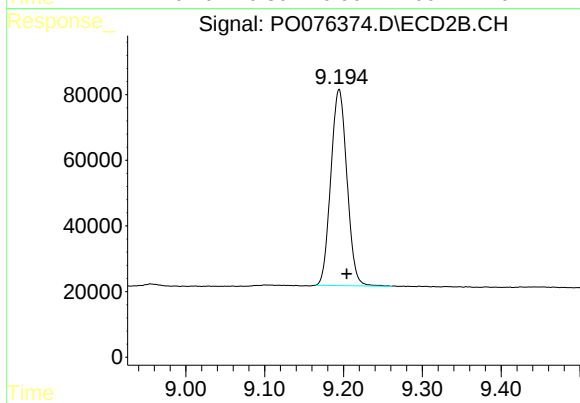

#2 Decachlorobiphenyl


R.T.: 9.194 min
Delta R.T.: -0.010 min
Response: 848559
Conc: 22.10 ng/ml

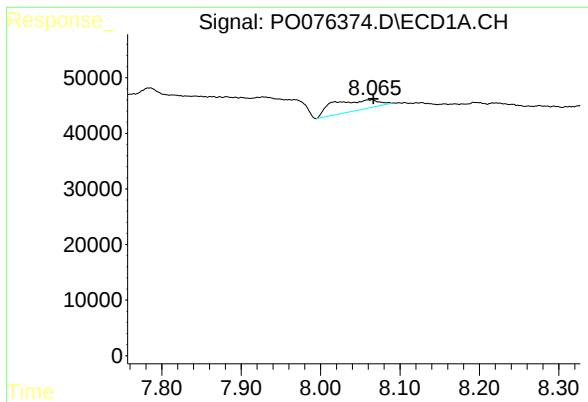

#29 AR-1254-4

R.T.: 8.065 min
Delta R.T.: -0.001 min
Response: 76770
Conc: 36.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

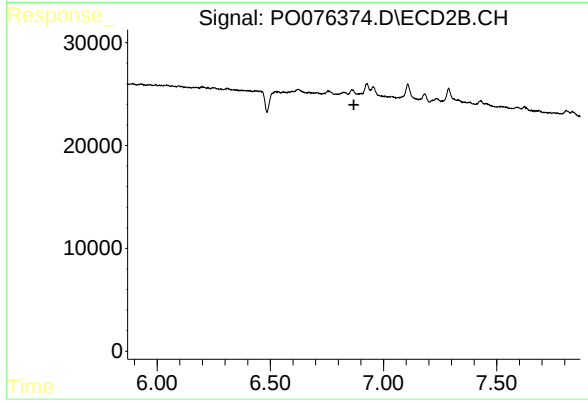

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.869 min
Response: 0
Conc: N.D.