

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076356.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 11:35
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 22:30:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.933	2782246	1999025	48.975	47.914
2) SA Decachlor...	10.916	9.196	2051210	1870310	53.329	48.709
Target Compounds						
26) L6 AR-1254-1	7.154	6.045	913873	1114347	445.922m	487.570
27) L6 AR-1254-2	7.383	6.205	1544684	1026840	497.074	518.462
28) L6 AR-1254-3	7.765	6.623	1613549	1549829	507.178m	514.545
29) L6 AR-1254-4	8.063	6.864	1095751	870048	522.996m	493.032
30) L6 AR-1254-5	8.491	7.290	1221016	1346704	531.645	514.388

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031921\
Data File : PO076356.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 11:35
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 22:30:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

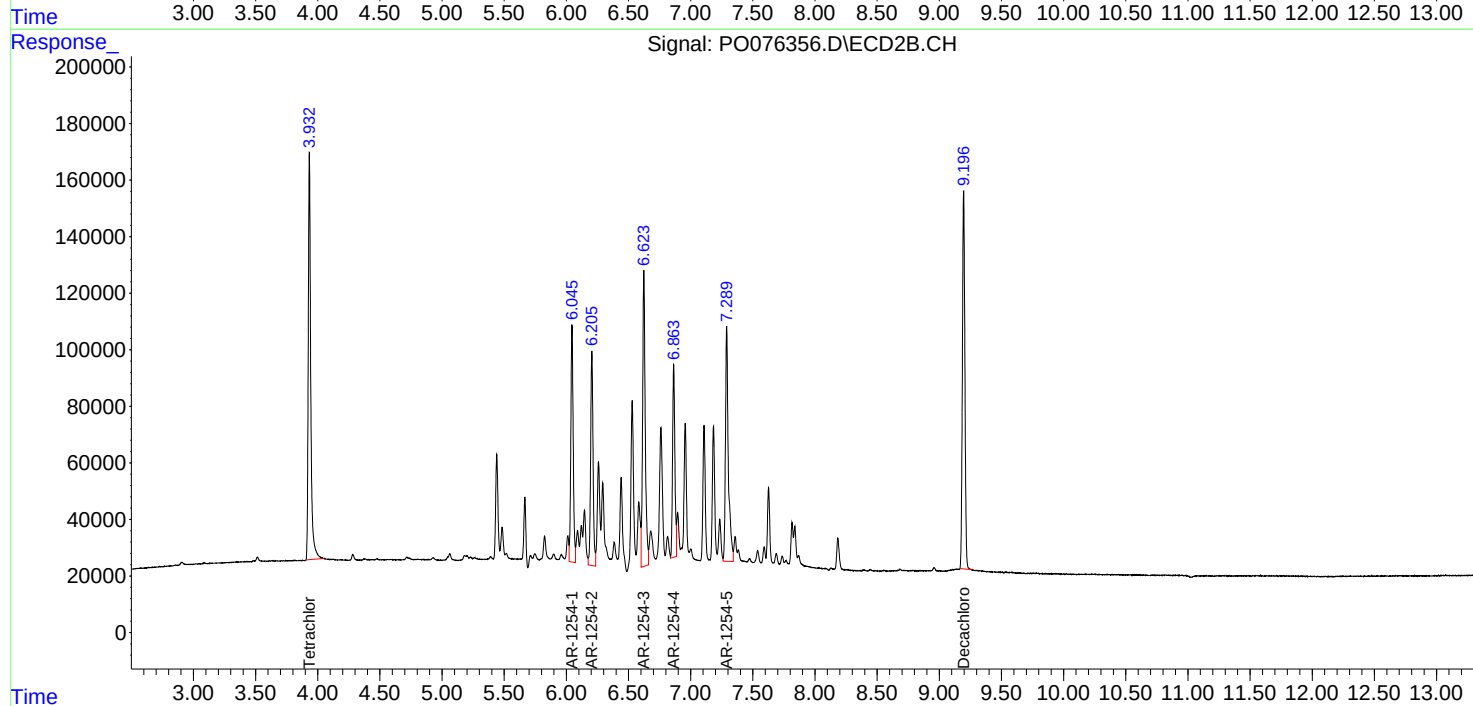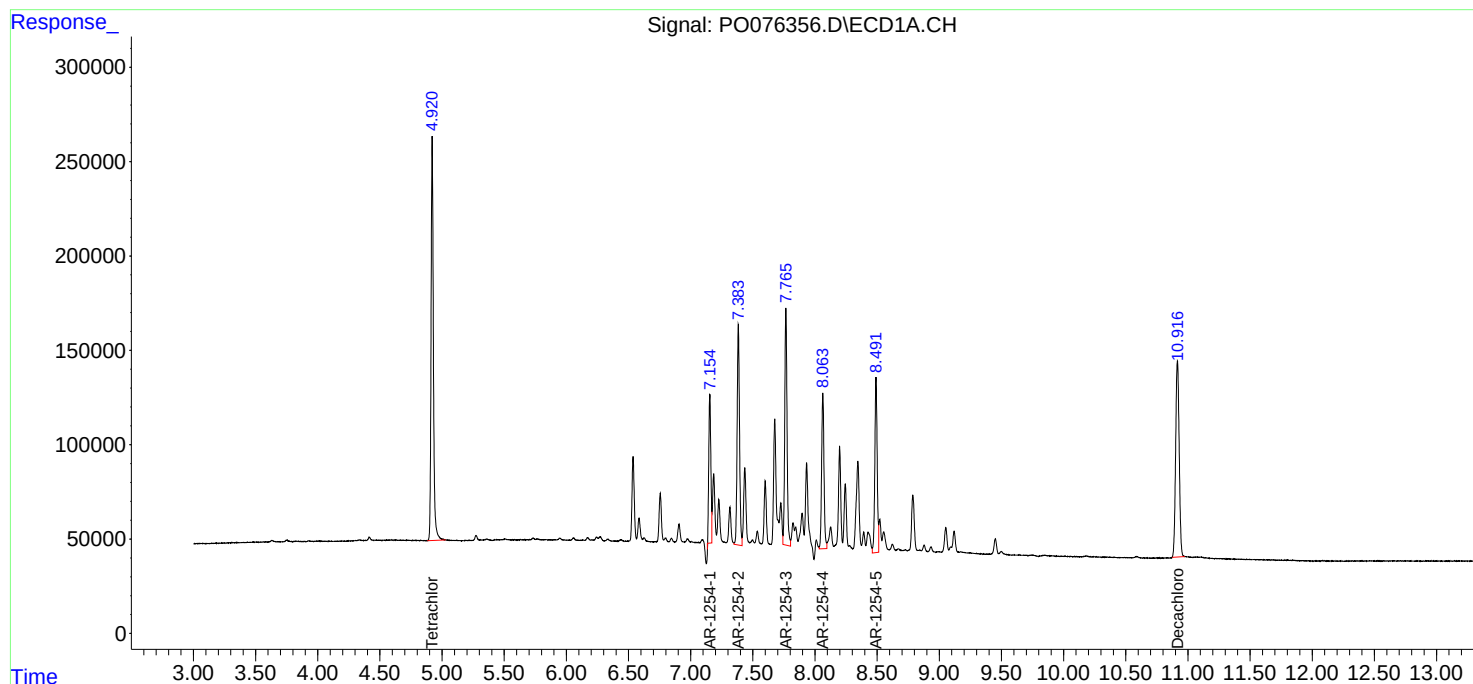

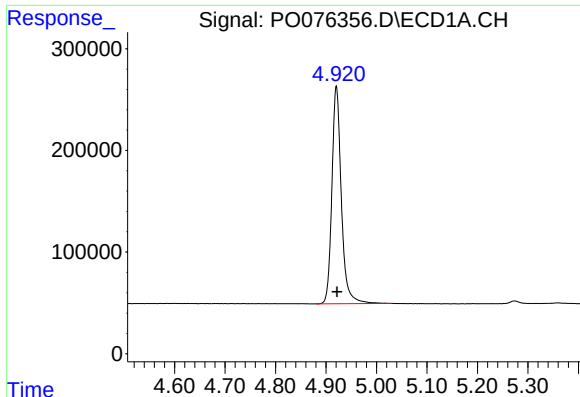


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 2782246
Conc: 48.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:09 PM

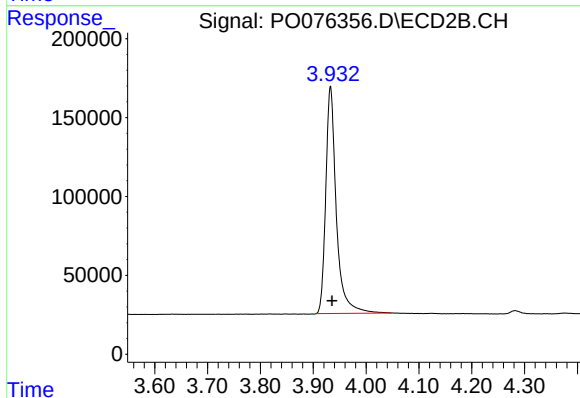


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 1999025
Conc: 47.91 ng/ml

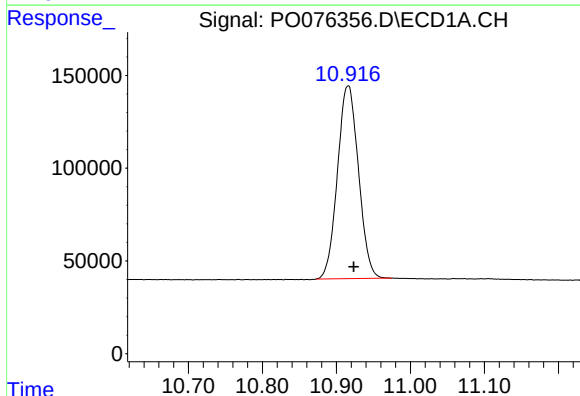


#2 Decachlorobiphenyl

R.T.: 10.916 min
Delta R.T.: -0.008 min
Response: 2051210
Conc: 53.33 ng/ml

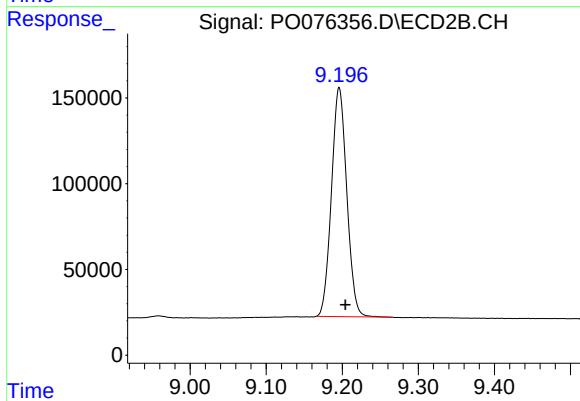

#2 Decachlorobiphenyl

R.T.: 9.196 min
Delta R.T.: -0.008 min
Response: 1870310
Conc: 48.71 ng/ml

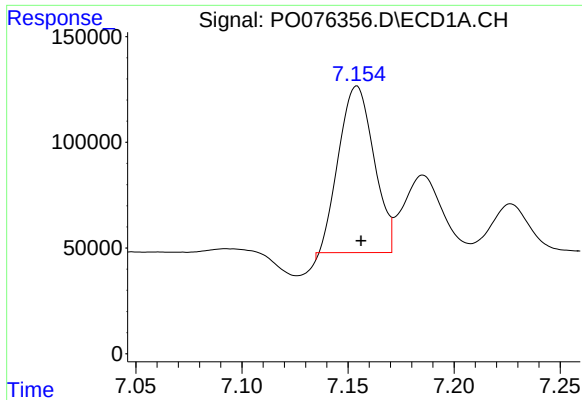


#26 AR-1254-1

R.T.: 7.154 min
Delta R.T.: -0.002 min
Response: 913873
Conc: 445.92 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:09 PM

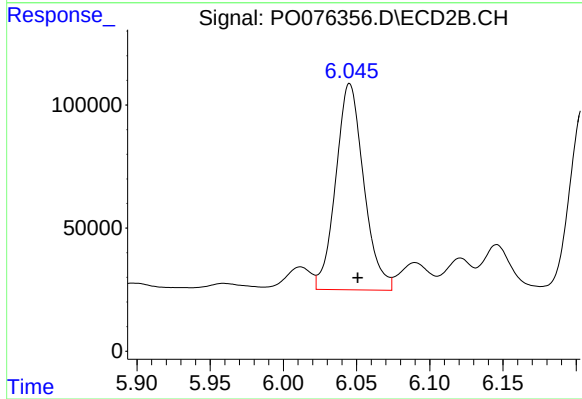


#26 AR-1254-1

R.T.: 6.045 min
Delta R.T.: -0.006 min
Response: 1114347
Conc: 487.57 ng/ml

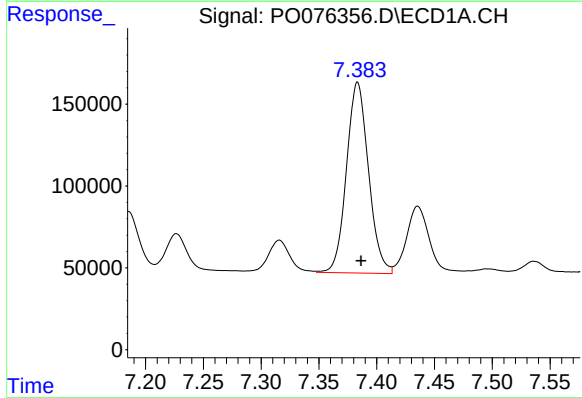


#27 AR-1254-2

R.T.: 7.383 min
Delta R.T.: -0.003 min
Response: 1544684
Conc: 497.07 ng/ml

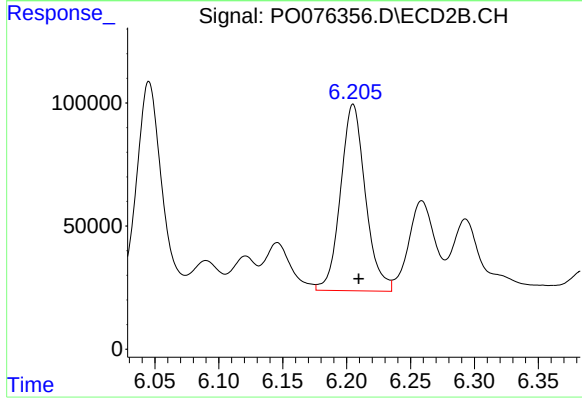

#27 AR-1254-2

R.T.: 6.205 min
Delta R.T.: -0.005 min
Response: 1026840
Conc: 518.46 ng/ml

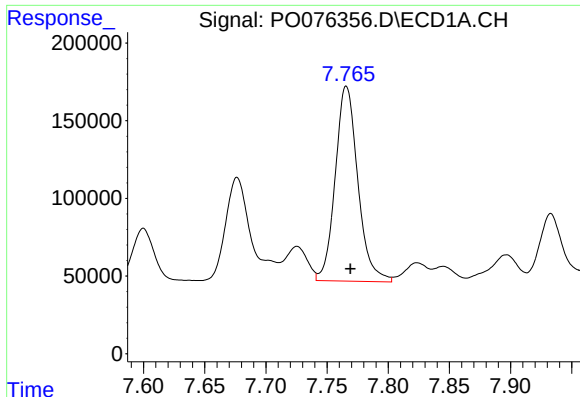


#28 AR-1254-3

R.T.: 7.765 min
Delta R.T.: -0.004 min
Response: 1613549
Conc: 507.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:09 PM

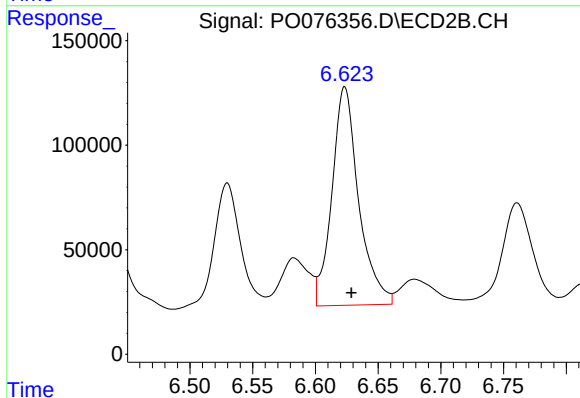


#28 AR-1254-3

R.T.: 6.623 min
Delta R.T.: -0.005 min
Response: 1549829
Conc: 514.55 ng/ml

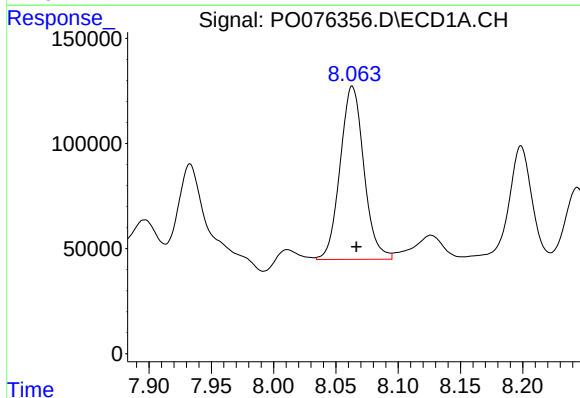


#29 AR-1254-4

R.T.: 8.063 min
Delta R.T.: -0.004 min
Response: 1095751
Conc: 523.00 ng/ml m

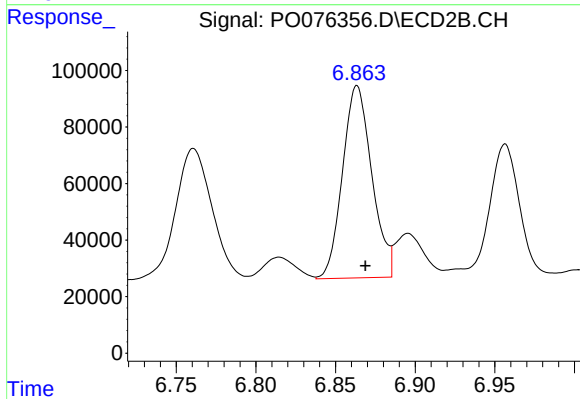

#29 AR-1254-4

R.T.: 6.864 min
Delta R.T.: -0.005 min
Response: 870048
Conc: 493.03 ng/ml

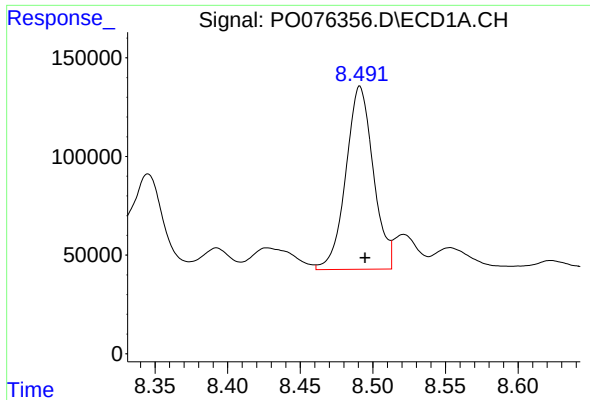


#30 AR-1254-5

R.T.: 8.491 min
Delta R.T.: -0.003 min
Response: 1221016
Conc: 531.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:09 PM

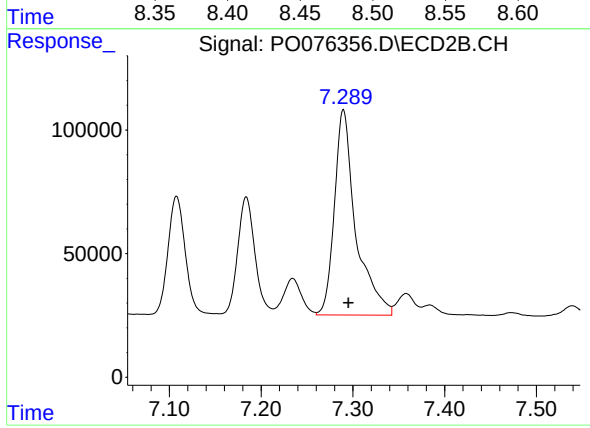

#30 AR-1254-5

R.T.: 7.290 min
Delta R.T.: -0.005 min
Response: 1346704
Conc: 514.39 ng/ml