

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076370.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 15:53
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 22:36:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.920	3.933	2474320	1788810	43.555	42.875
2)	SA Decachlor...	10.917	9.196	1944242	1688383	50.548	43.971
Target Compounds							
21)	L5 AR-1248-1	6.243	5.180	451158	340805	478.541	496.232
22)	L5 AR-1248-2	6.537	5.440	658512	553788	437.145	428.013
23)	L5 AR-1248-3	6.754	5.484	764584	557799	440.831	436.393
24)	L5 AR-1248-4	7.185	5.667	810466	623099	460.666m	423.744
25)	L5 AR-1248-5	7.224	6.090	753825	653716	426.218m	422.689

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076370.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 15:53
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 22:36:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

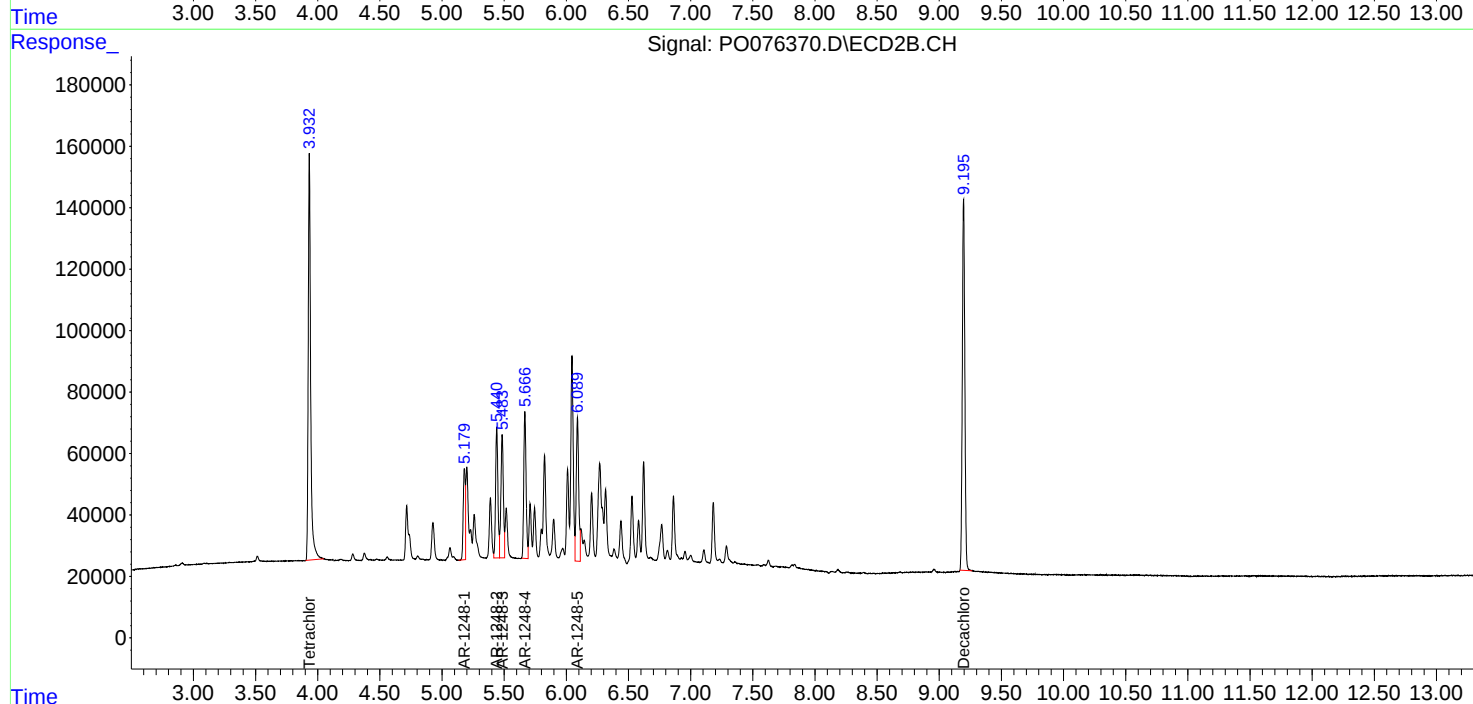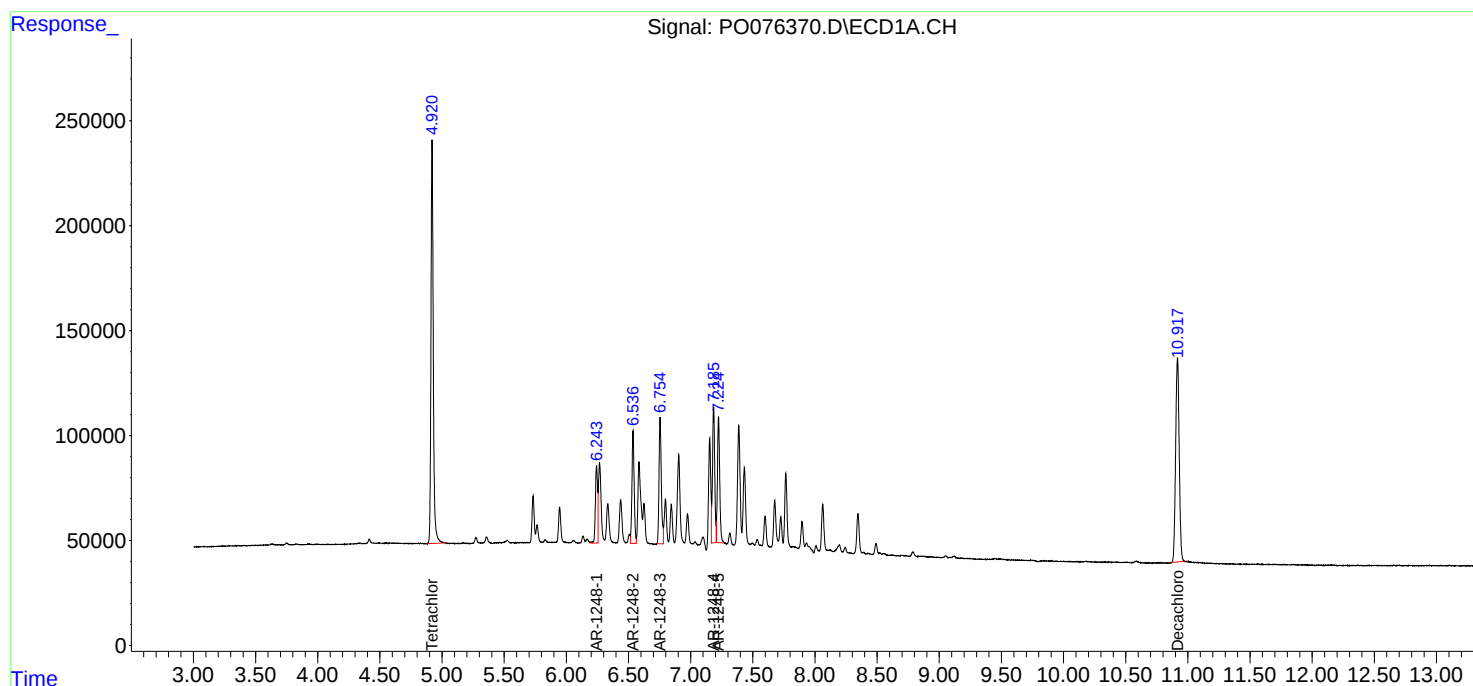

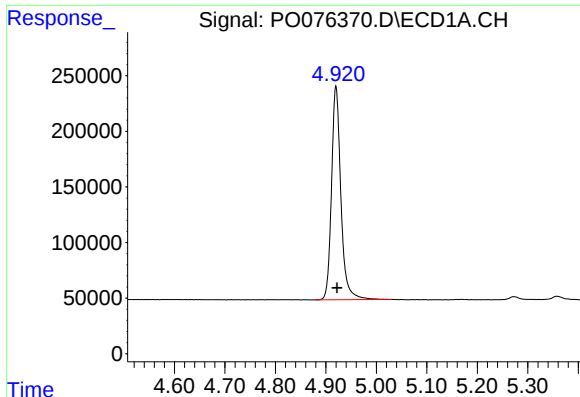


#1 Tetrachloro-m-xylene

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 2474320
Conc: 43.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:17 PM

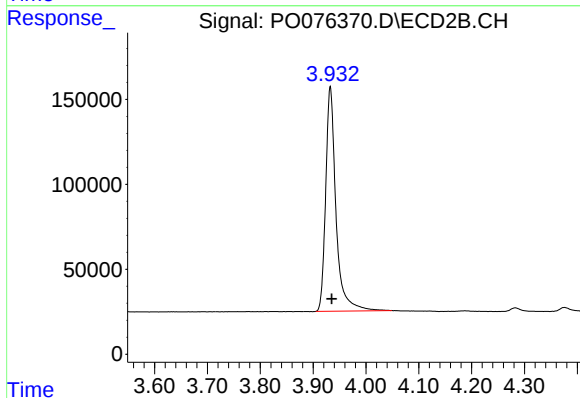


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 1788810
Conc: 42.88 ng/ml

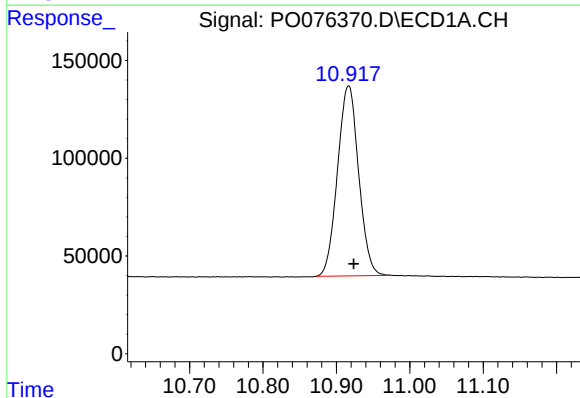


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: -0.007 min
Response: 1944242
Conc: 50.55 ng/ml

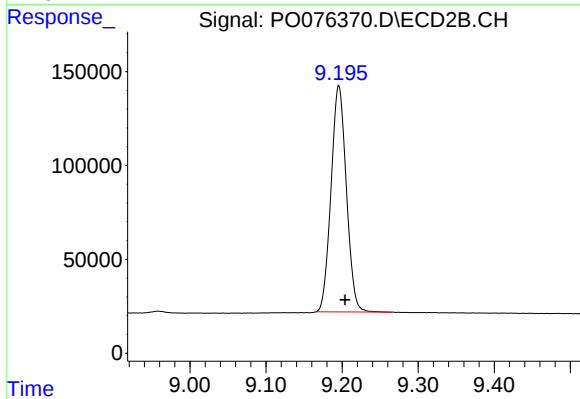

#2 Decachlorobiphenyl

R.T.: 9.196 min
Delta R.T.: -0.008 min
Response: 1688383
Conc: 43.97 ng/ml

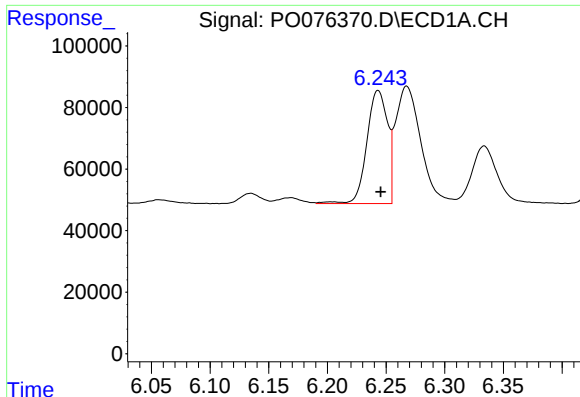


#21 AR-1248-1

R.T.: 6.243 min
Delta R.T.: -0.002 min
Response: 451158
Conc: 478.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:17 PM

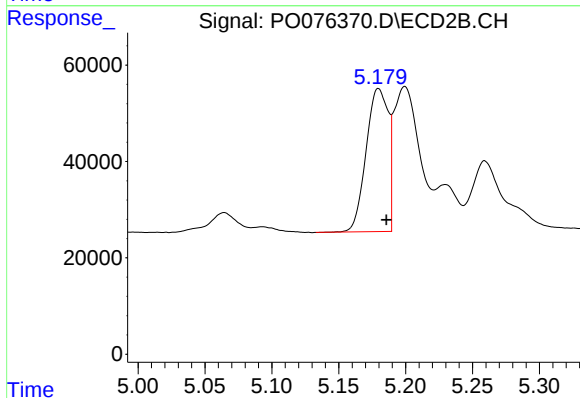


#21 AR-1248-1

R.T.: 5.180 min
Delta R.T.: -0.006 min
Response: 340805
Conc: 496.23 ng/ml

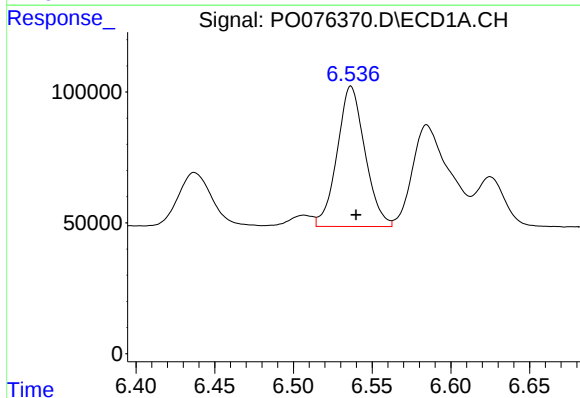


#22 AR-1248-2

R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 658512
Conc: 437.15 ng/ml

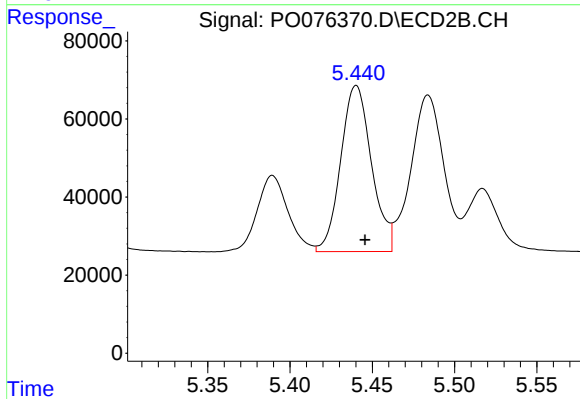

#22 AR-1248-2

R.T.: 5.440 min
Delta R.T.: -0.005 min
Response: 553788
Conc: 428.01 ng/ml

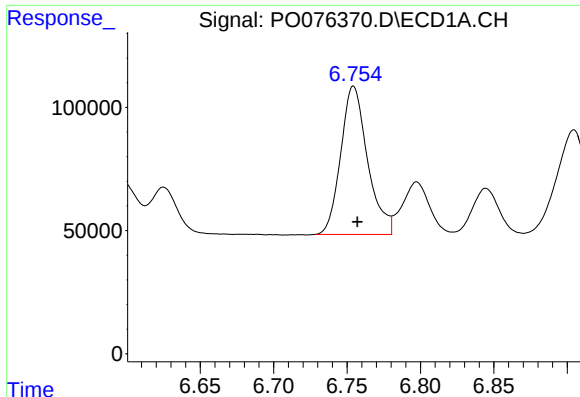


#23 AR-1248-3

R.T.: 6.754 min
Delta R.T.: -0.003 min
Response: 764584
Conc: 440.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:17 PM

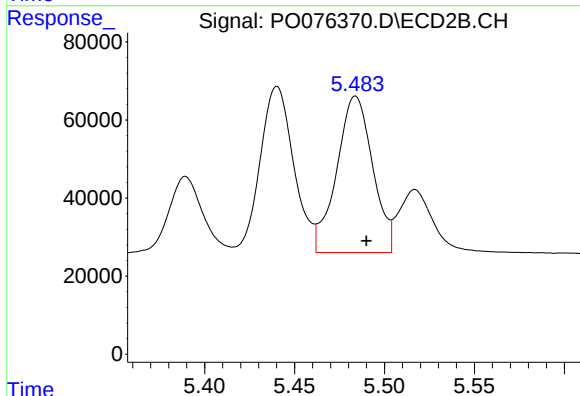


#23 AR-1248-3

R.T.: 5.484 min
Delta R.T.: -0.006 min
Response: 557799
Conc: 436.39 ng/ml

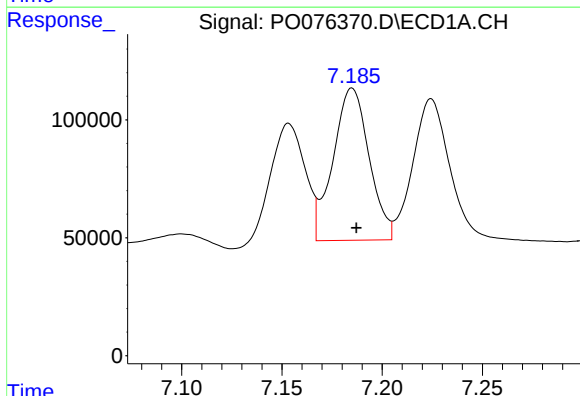


#24 AR-1248-4

R.T.: 7.185 min
Delta R.T.: -0.003 min
Response: 810466
Conc: 460.67 ng/ml m

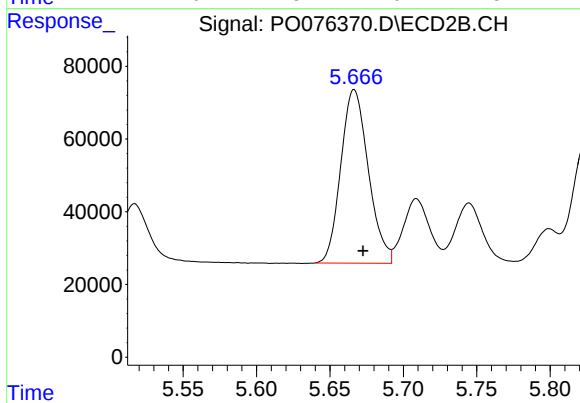

#24 AR-1248-4

R.T.: 5.667 min
Delta R.T.: -0.006 min
Response: 623099
Conc: 423.74 ng/ml

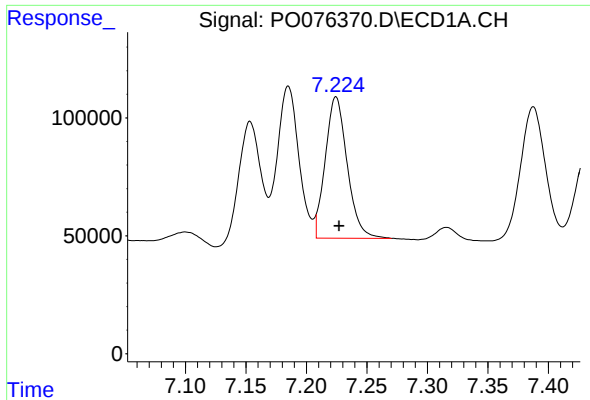


#25 AR-1248-5

R.T.: 7.224 min
Delta R.T.: -0.003 min
Response: 753825
Conc: 426.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:17 PM

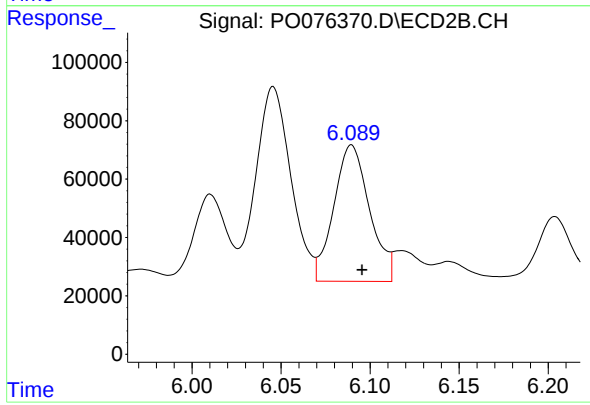

#25 AR-1248-5

R.T.: 6.090 min
Delta R.T.: -0.006 min
Response: 653716
Conc: 422.69 ng/ml