

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0031921\  
 Data File : P0076384.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 19 Mar 2021 19:53  
 Operator : DD\AJ  
 Sample : M1725-01  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 72-11948-124018

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 22:41:07 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031521.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 16 07:18:57 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|--------|--------|--------|
| -----                       |        |       |         |        |        |        |
| System Monitoring Compounds |        |       |         |        |        |        |
| 1) SA Tetrachlo...          | 4.919  | 3.932 | 1265463 | 935631 | 22.276 | 22.426 |
| 2) SA Decachlor...          | 10.913 | 9.193 | 887294  | 777524 | 23.068 | 20.249 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0031921\  
Data File : P0076384.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 19 Mar 2021 19:53  
Operator : DD\AJ  
Sample : M1725-01  
Misc :  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
72-11948-124018

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 19 22:41:07 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031521.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Mar 16 07:18:57 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

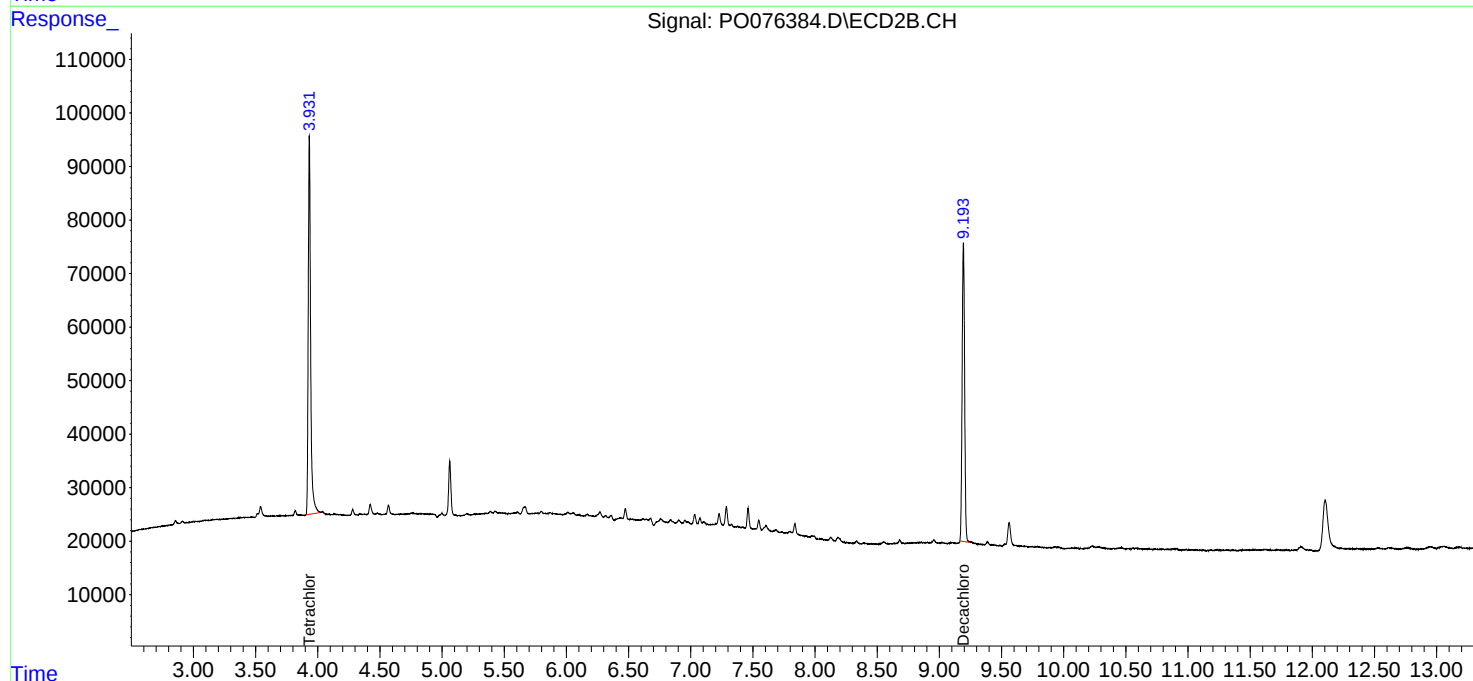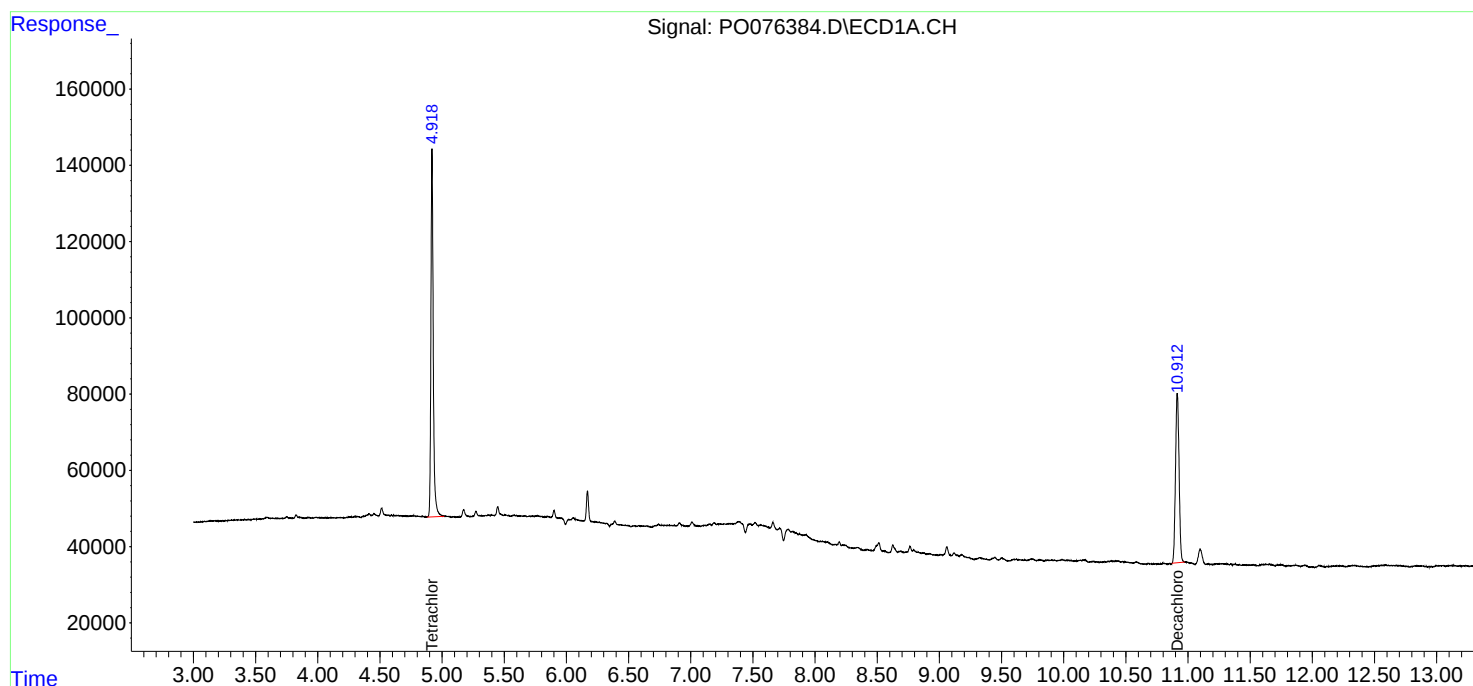


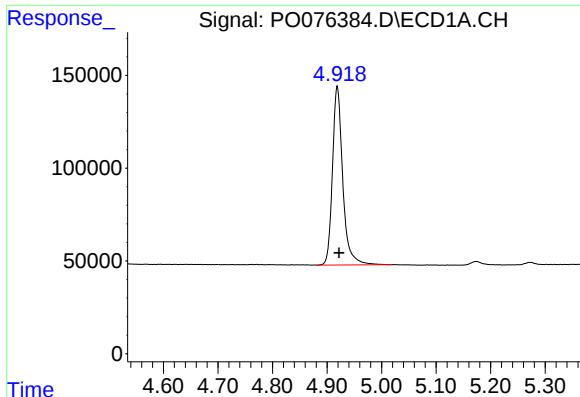

#1 Tetrachloro-m-xylene


R.T.: 4.919 min  
Delta R.T.: -0.003 min  
Response: 1265463  
Conc: 22.28 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
72-11948-124018

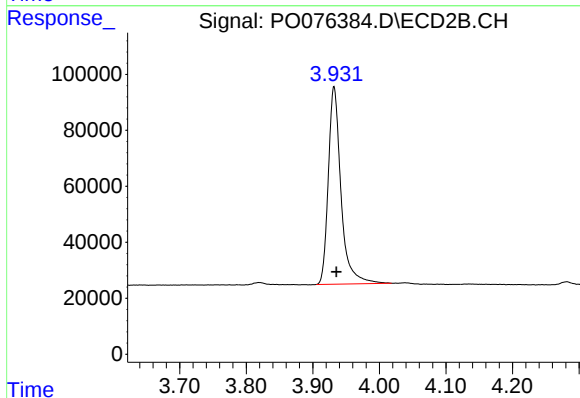


#1 Tetrachloro-m-xylene

R.T.: 3.932 min  
Delta R.T.: -0.003 min  
Response: 935631  
Conc: 22.43 ng/ml

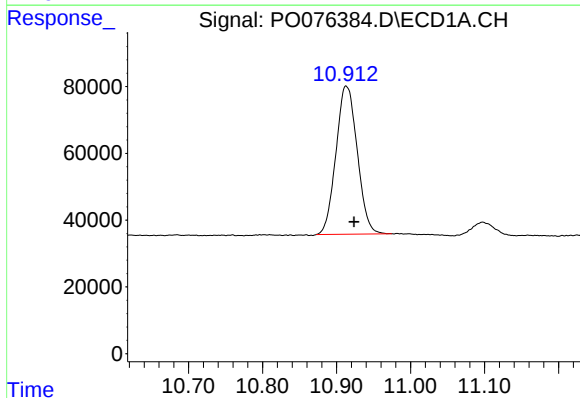

#2 Decachlorobiphenyl

R.T.: 10.913 min  
Delta R.T.: -0.011 min  
Response: 887294  
Conc: 23.07 ng/ml

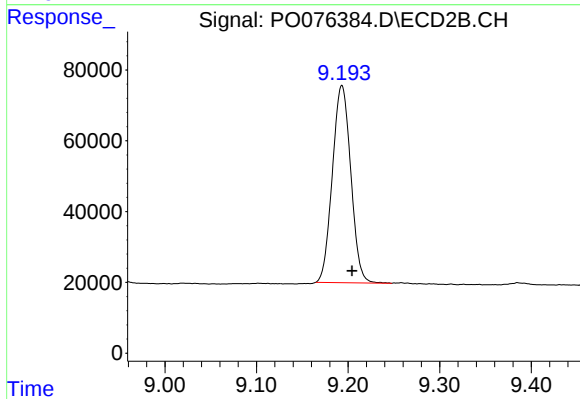

#2 Decachlorobiphenyl

R.T.: 9.193 min  
Delta R.T.: -0.011 min  
Response: 777524  
Conc: 20.25 ng/ml