

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076386.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 20:44
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 22:41:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.934	2524872	1837959	44.445	44.053
2) SA Decachlor...	10.915	9.195	1812984	1579108	47.135	41.125
Target Compounds						
16) L4 AR-1242-1	6.243	5.181	621297	450454	491.971	507.721
17) L4 AR-1242-2	6.267	5.200	926894	806141	467.673	465.752
18) L4 AR-1242-3	6.333	5.390	593959	399300	468.733	495.724
19) L4 AR-1242-4	6.440	5.484	463208	396217	478.372	456.453
20) L4 AR-1242-5	7.225	6.046	453022	503619	450.912m	499.725

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031921\
Data File : PO076386.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 20:44
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 22:41:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

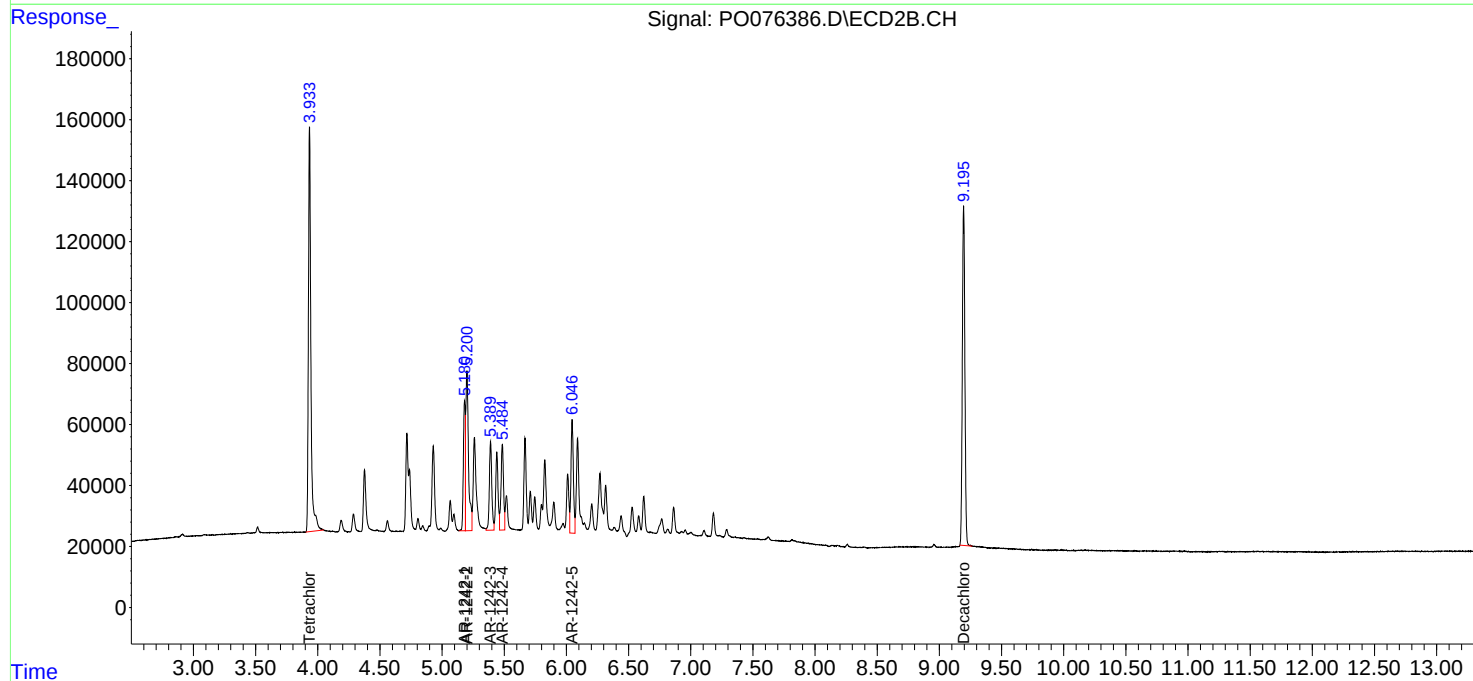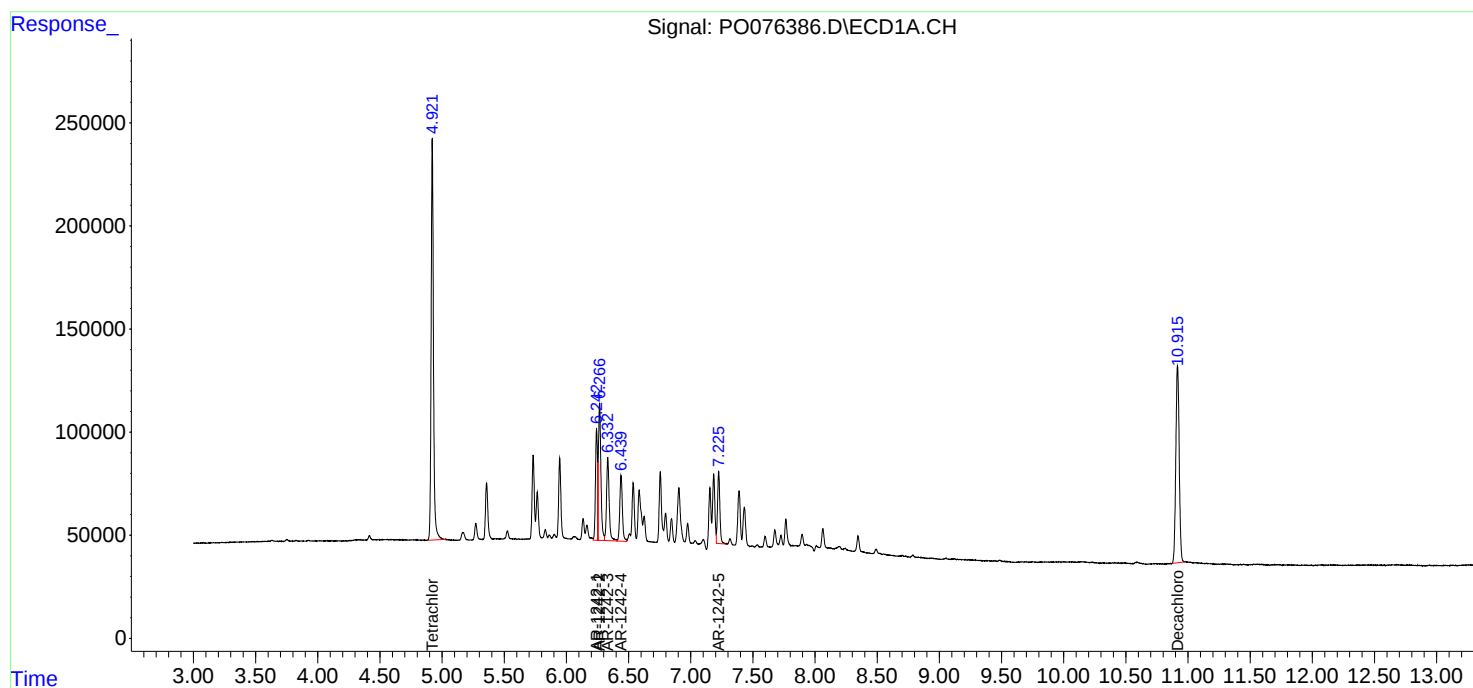

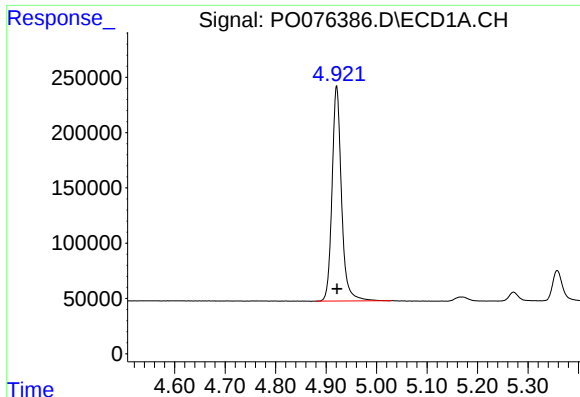


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 2524872
Conc: 44.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:24 PM

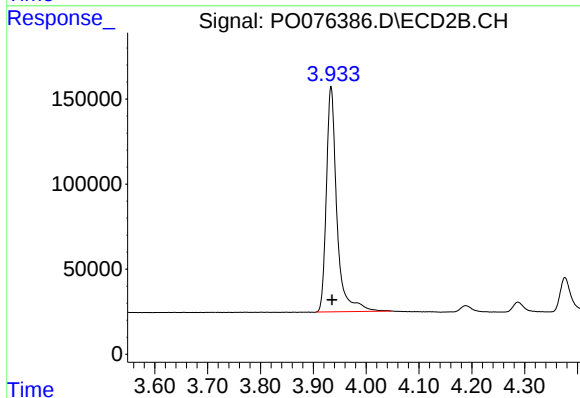


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 1837959
Conc: 44.05 ng/ml

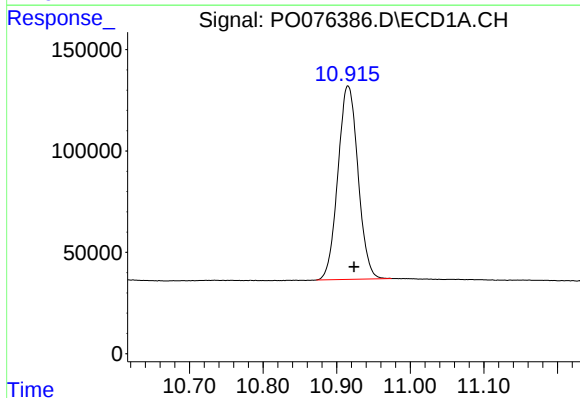


#2 Decachlorobiphenyl

R.T.: 10.915 min
Delta R.T.: -0.008 min
Response: 1812984
Conc: 47.14 ng/ml

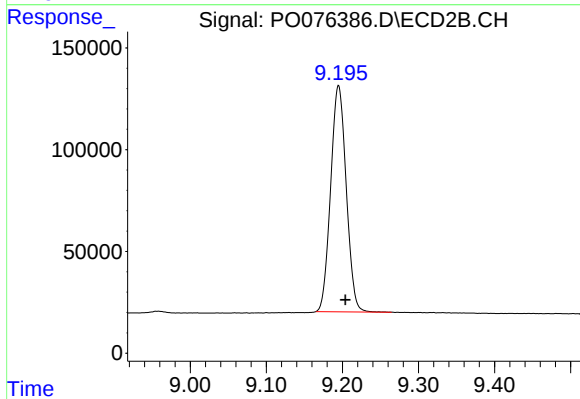

#2 Decachlorobiphenyl

R.T.: 9.195 min
Delta R.T.: -0.009 min
Response: 1579108
Conc: 41.13 ng/ml

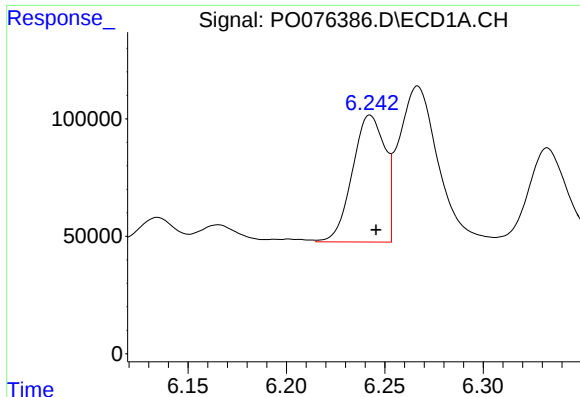


#16 AR-1242-1

R.T.: 6.243 min
Delta R.T.: -0.003 min
Response: 621297
Conc: 491.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:24 PM

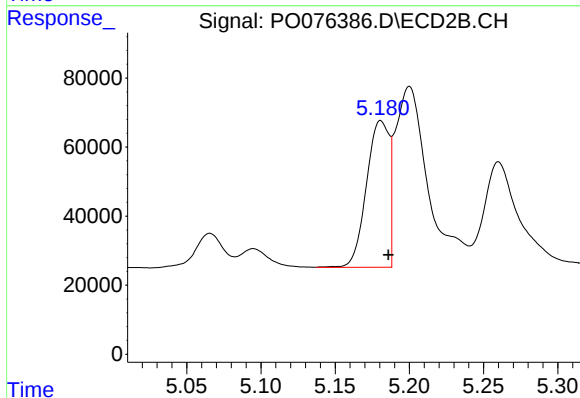


#16 AR-1242-1

R.T.: 5.181 min
Delta R.T.: -0.005 min
Response: 450454
Conc: 507.72 ng/ml

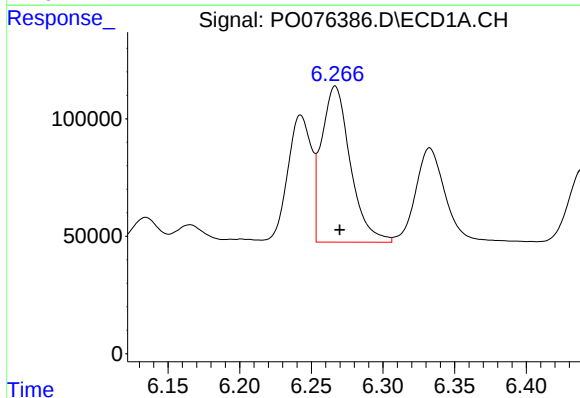


#17 AR-1242-2

R.T.: 6.267 min
Delta R.T.: -0.003 min
Response: 926894
Conc: 467.67 ng/ml

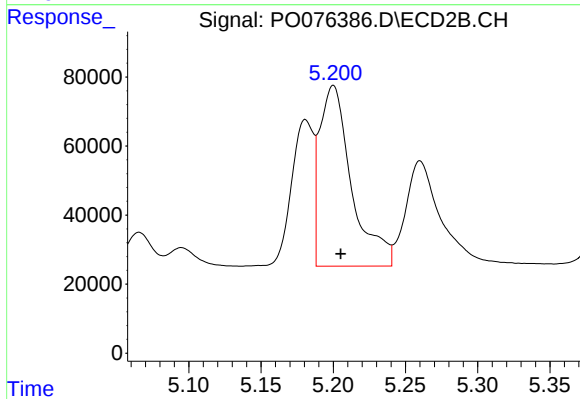

#17 AR-1242-2

R.T.: 5.200 min
Delta R.T.: -0.005 min
Response: 806141
Conc: 465.75 ng/ml

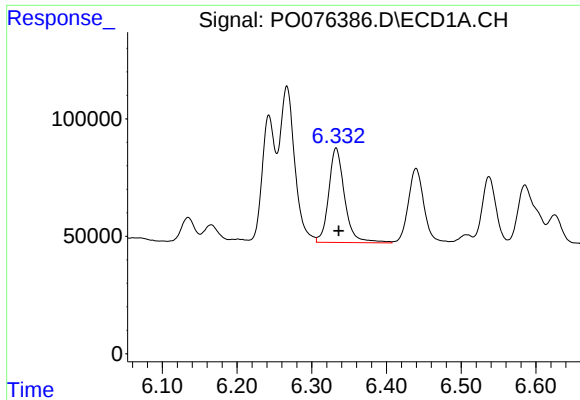


#18 AR-1242-3

R.T.: 6.333 min
Delta R.T.: -0.003 min
Response: 593959
Conc: 468.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:24 PM

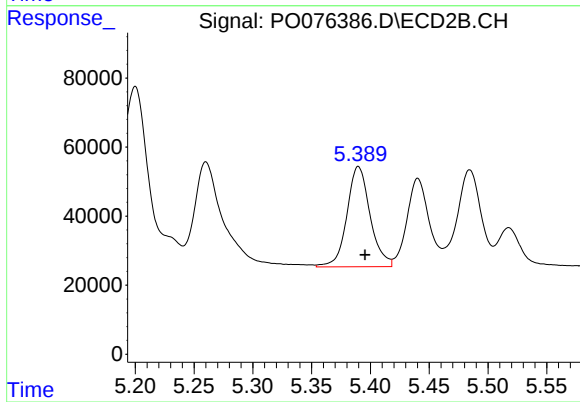


#18 AR-1242-3

R.T.: 5.390 min
Delta R.T.: -0.006 min
Response: 399300
Conc: 495.72 ng/ml

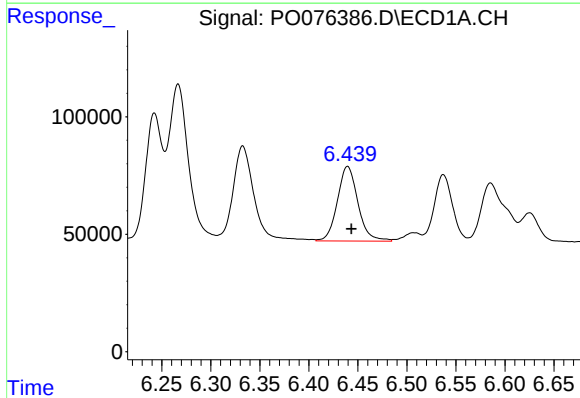


#19 AR-1242-4

R.T.: 6.440 min
Delta R.T.: -0.004 min
Response: 463208
Conc: 478.37 ng/ml

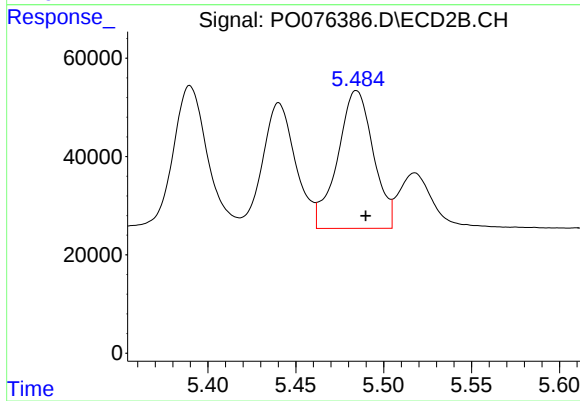

#19 AR-1242-4

R.T.: 5.484 min
Delta R.T.: -0.005 min
Response: 396217
Conc: 456.45 ng/ml

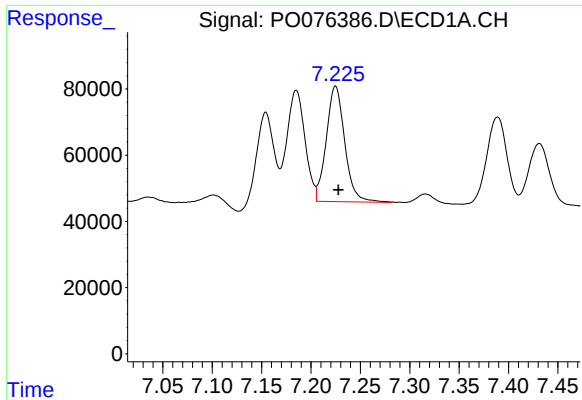


#20 AR-1242-5

R.T.: 7.225 min
Delta R.T.: -0.003 min
Response: 453022
Conc: 450.91 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:24 PM

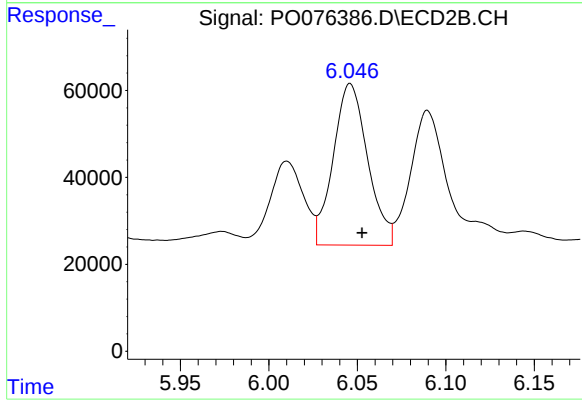

#20 AR-1242-5

R.T.: 6.046 min
Delta R.T.: -0.007 min
Response: 503619
Conc: 499.73 ng/ml