

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 23:35
 Operator : DD\AJ
 Sample : M1745-02 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 00:35:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.918	3.931	155715	115831	2.741	2.776
2) SA Decachlor...	10.914	9.190	102770	116755	2.672	3.041m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 23:35
Operator : DD\AJ
Sample : M1745-02 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 00:35:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

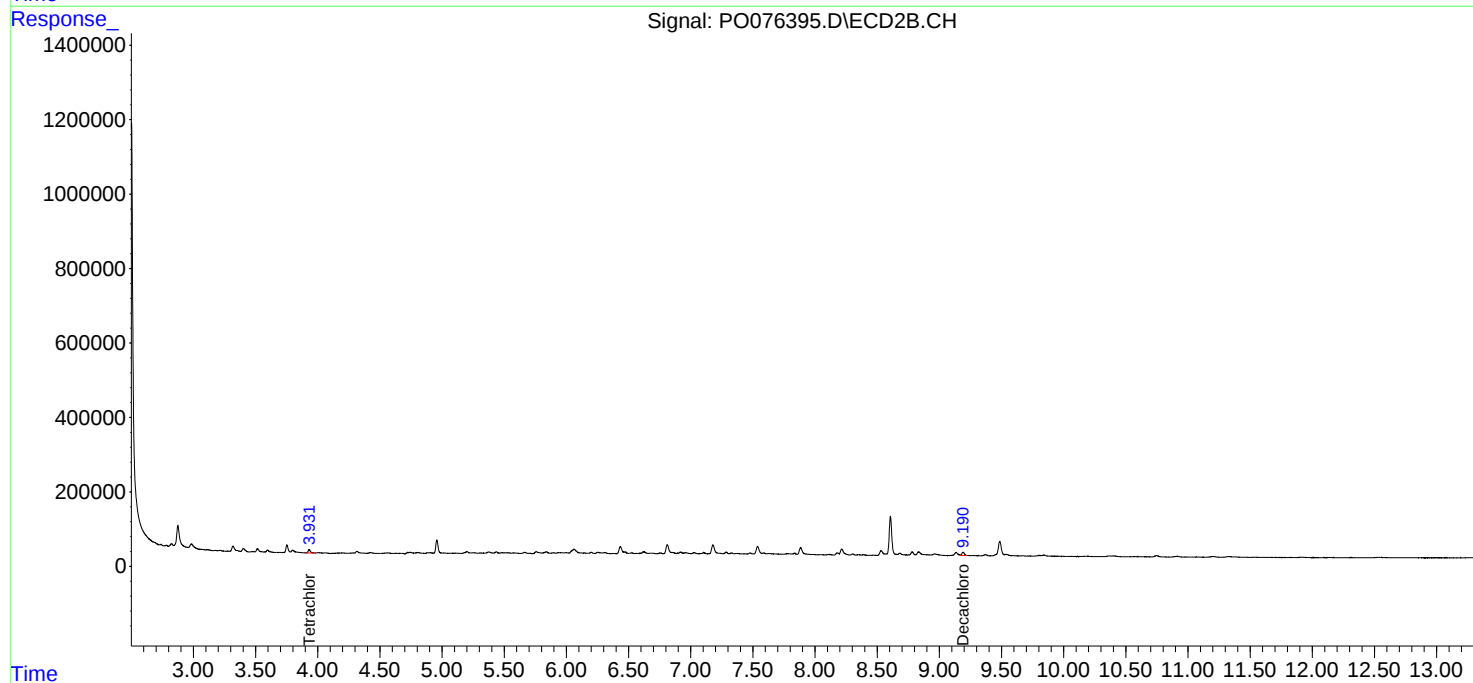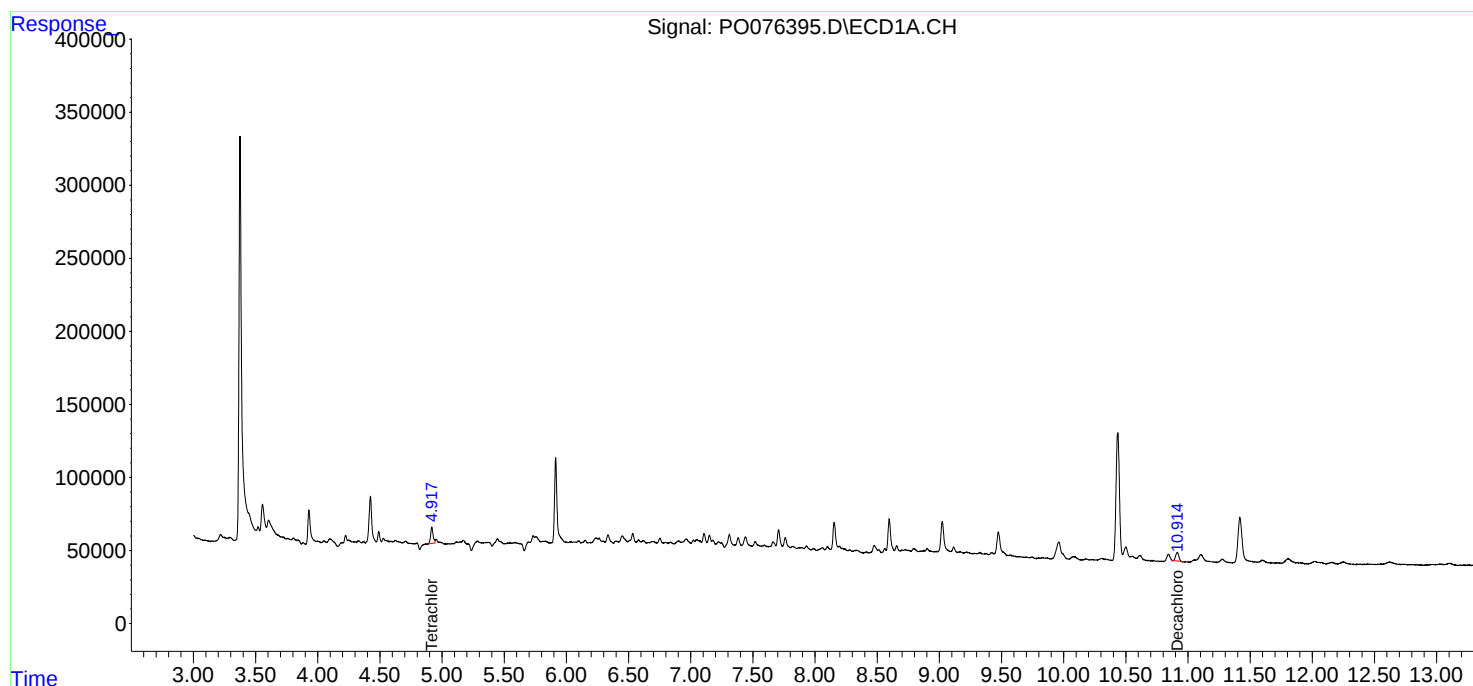

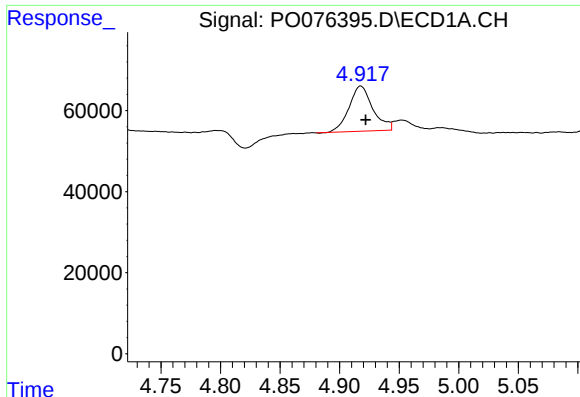


#1 Tetrachloro-m-xylene

R.T.: 4.918 min
Delta R.T.: -0.004 min
Response: 155715
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:34 PM

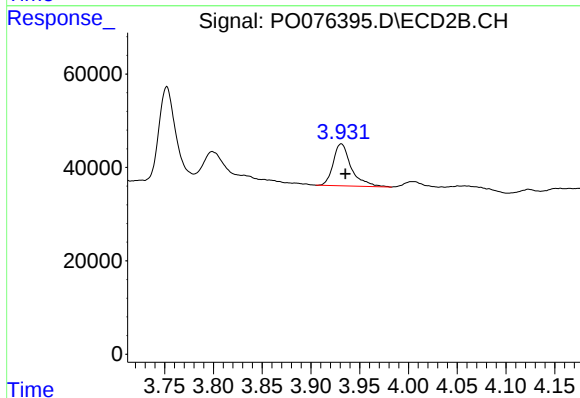


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 115831
Conc: 2.78 ng/ml

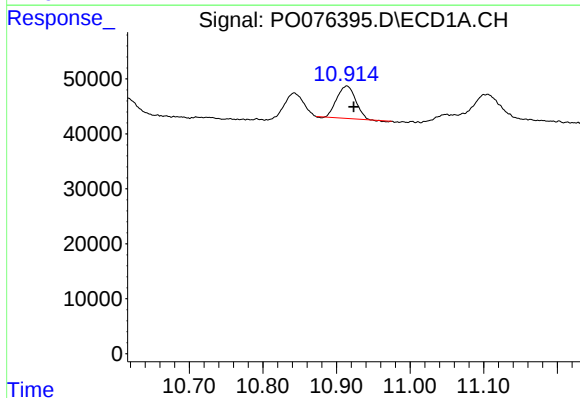

#2 Decachlorobiphenyl

R.T.: 10.914 min
Delta R.T.: -0.010 min
Response: 102770
Conc: 2.67 ng/ml

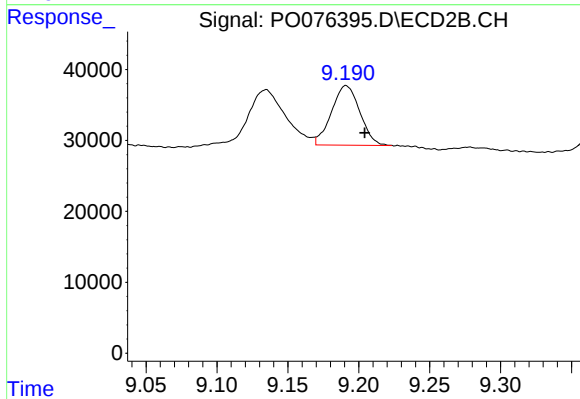

#2 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.014 min
Response: 116755
Conc: 3.04 ng/ml m