

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031921\
 Data File : P0076396.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2021 23:52
 Operator : DD\AJ
 Sample : M1745-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 00:35:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.919	3.931	195339	115162	3.438	2.760
2) SA Decachlor...	10.907f	9.190	289009	135107	7.514	3.519 #
Target Compounds						
26) L6 AR-1254-1	7.151	6.043	372412	357890	181.717	156.591
27) L6 AR-1254-2	7.382	6.203	369470	202108	118.894	102.046
28) L6 AR-1254-3	7.764	6.621	249980	197543	78.575	65.585
29) L6 AR-1254-4	8.060	6.861	94734	74686	45.216	42.323
30) L6 AR-1254-5	8.489	7.286	57794	186920	25.164m	71.396 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076396.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2021 23:52
Operator : DD\AJ
Sample : M1745-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 00:35:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

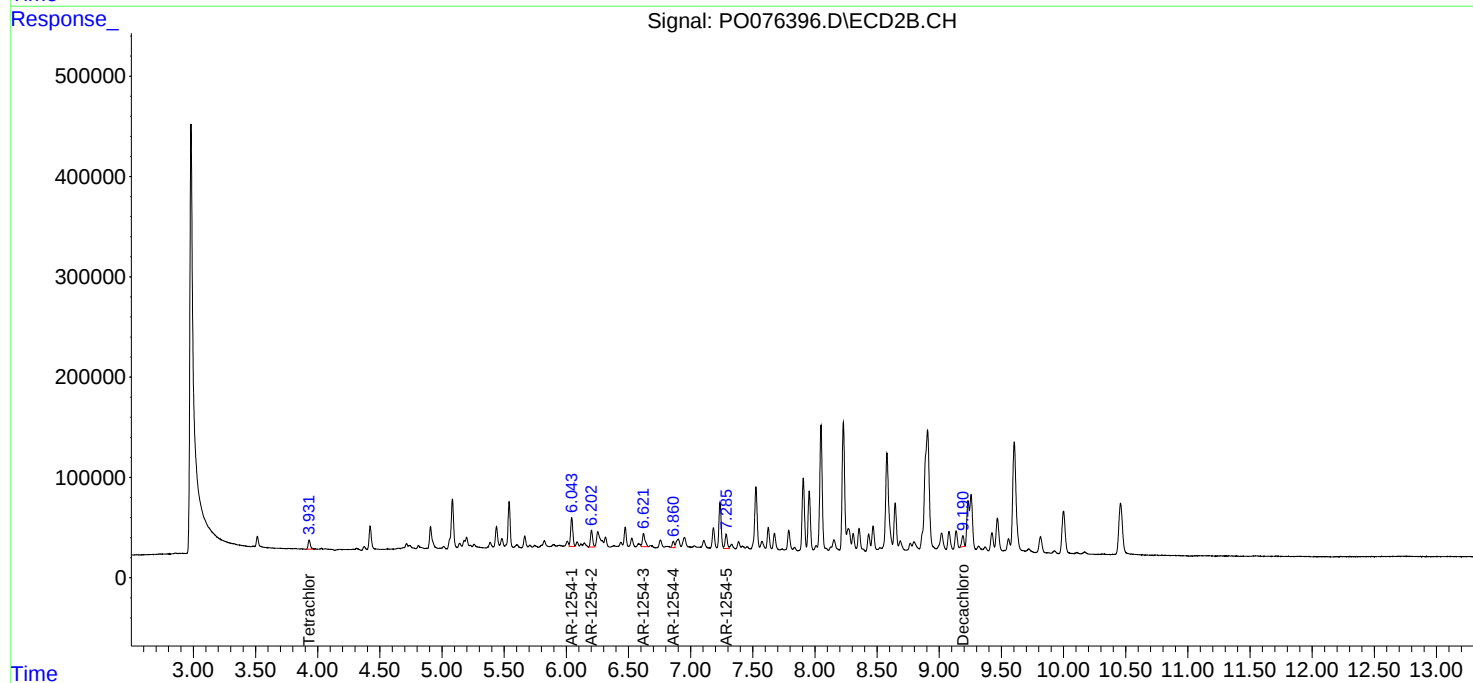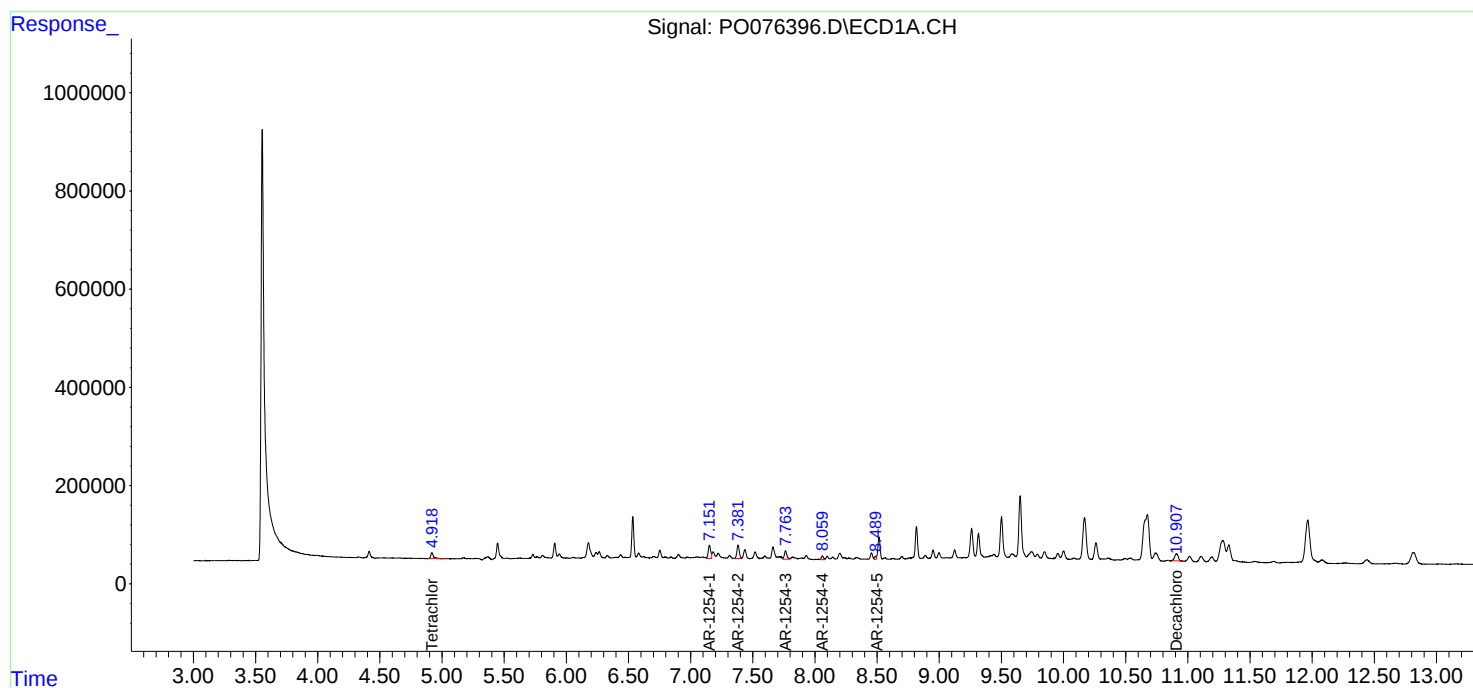

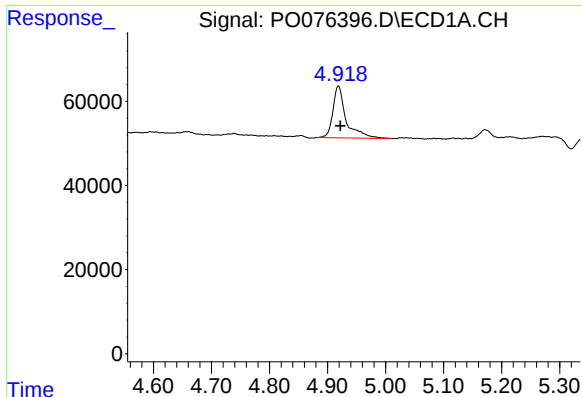


#1 Tetrachloro-m-xylene

R.T.: 4.919 min
Delta R.T.: -0.003 min
Response: 195339
Conc: 3.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:36 PM

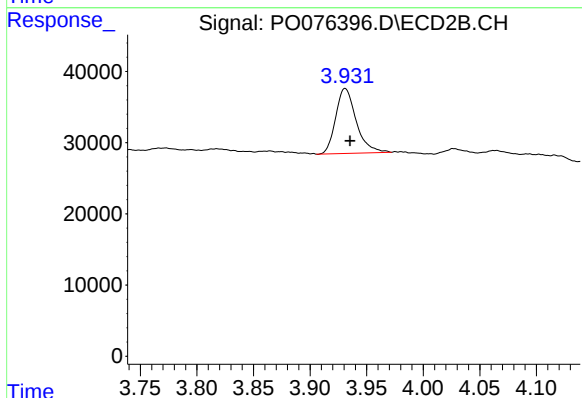


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 115162
Conc: 2.76 ng/ml

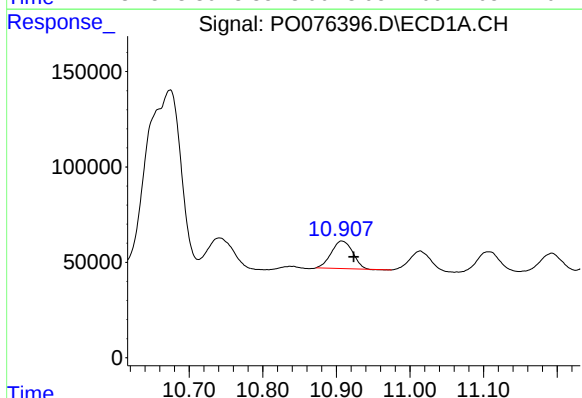


#2 Decachlorobiphenyl

R.T.: 10.907 min
Delta R.T.: -0.016 min
Response: 289009
Conc: 7.51 ng/ml

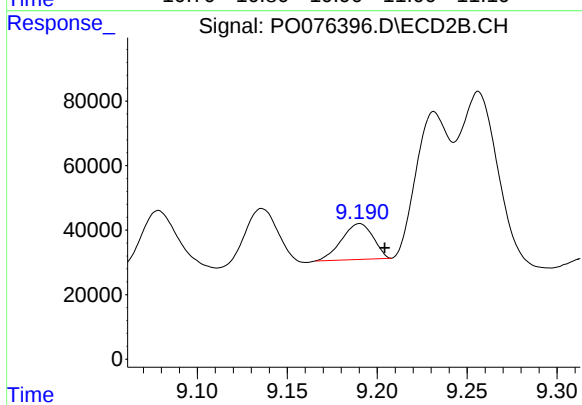

#2 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.014 min
Response: 135107
Conc: 3.52 ng/ml

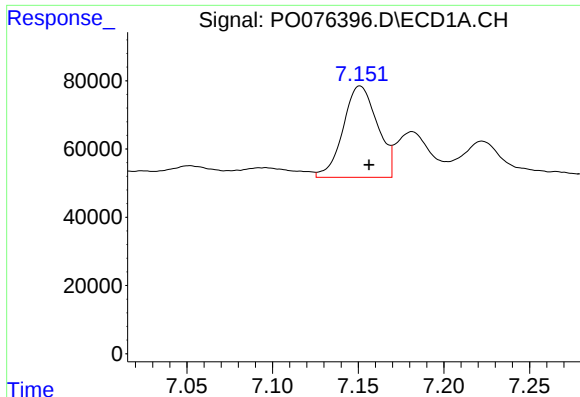


#26 AR-1254-1

R.T.: 7.151 min
Delta R.T.: -0.005 min
Response: 372412
Conc: 181.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:36 PM

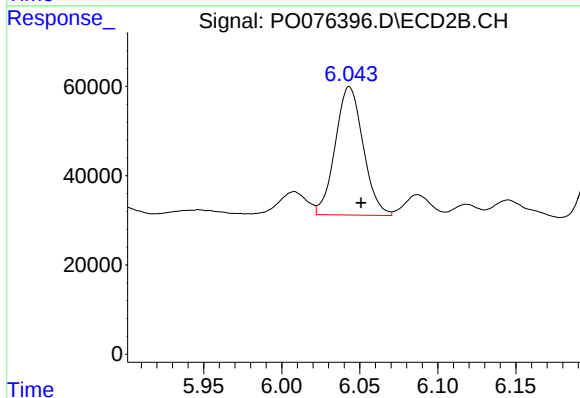


#26 AR-1254-1

R.T.: 6.043 min
Delta R.T.: -0.008 min
Response: 357890
Conc: 156.59 ng/ml

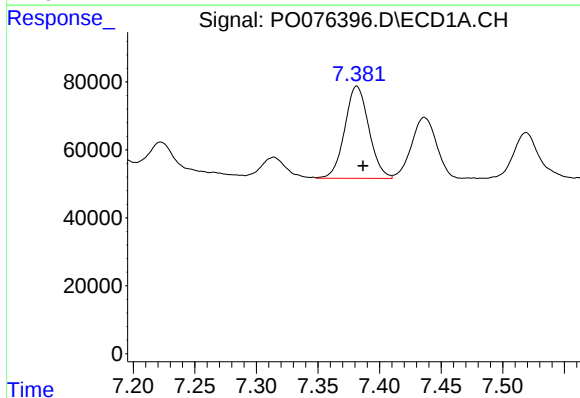


#27 AR-1254-2

R.T.: 7.382 min
Delta R.T.: -0.005 min
Response: 369470
Conc: 118.89 ng/ml

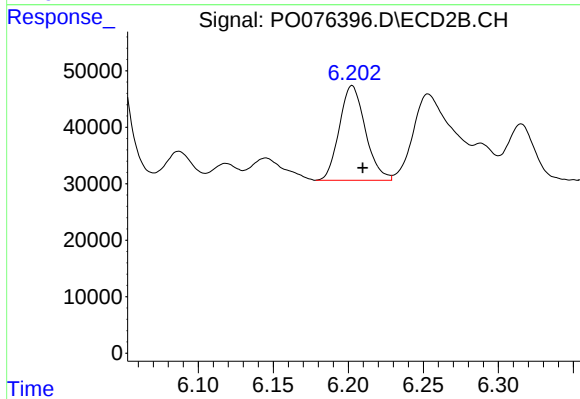

#27 AR-1254-2

R.T.: 6.203 min
Delta R.T.: -0.007 min
Response: 202108
Conc: 102.05 ng/ml

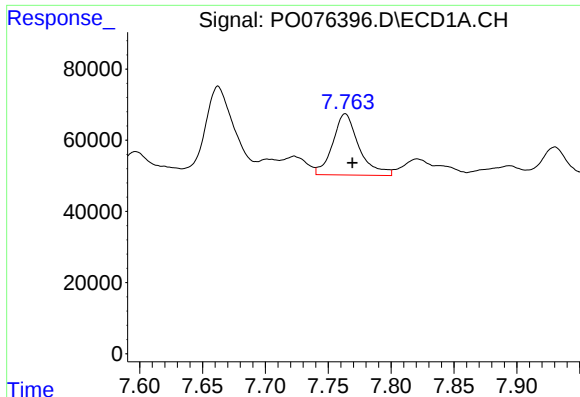


#28 AR-1254-3

R.T.: 7.764 min
Delta R.T.: -0.006 min
Response: 249980
Conc: 78.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:36 PM

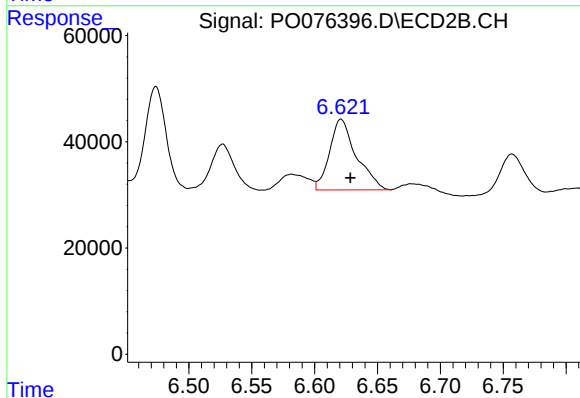


#28 AR-1254-3

R.T.: 6.621 min
Delta R.T.: -0.008 min
Response: 197543
Conc: 65.58 ng/ml

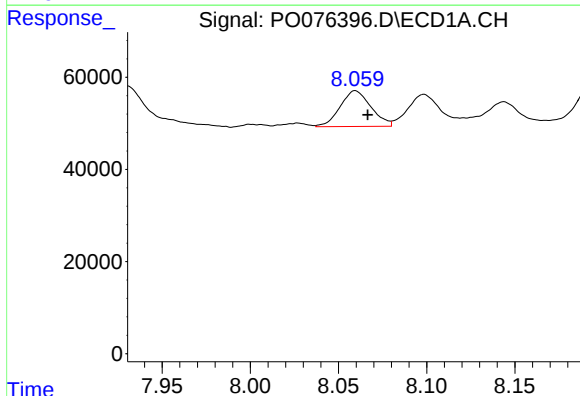


#29 AR-1254-4

R.T.: 8.060 min
Delta R.T.: -0.007 min
Response: 94734
Conc: 45.22 ng/ml

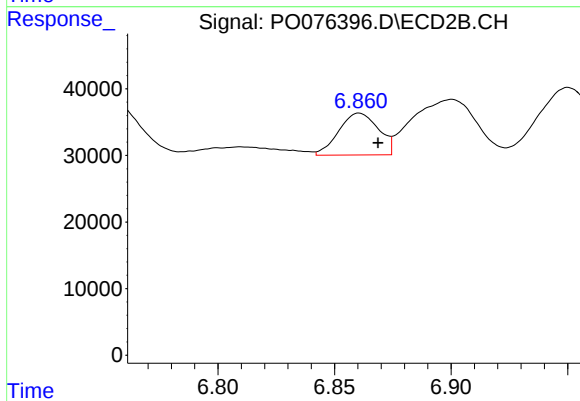

#29 AR-1254-4

R.T.: 6.861 min
Delta R.T.: -0.008 min
Response: 74686
Conc: 42.32 ng/ml

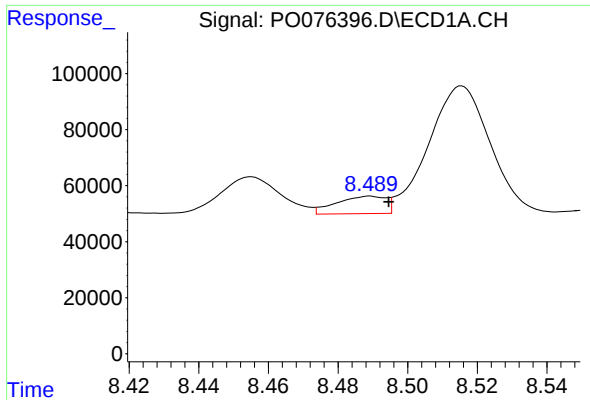


#30 AR-1254-5

R.T.: 8.489 min
Delta R.T.: -0.006 min
Response: 57794
Conc: 25.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:36 PM

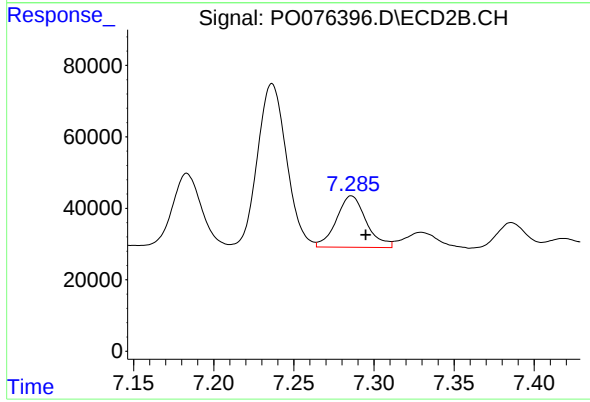

#30 AR-1254-5

R.T.: 7.286 min
Delta R.T.: -0.009 min
Response: 186920
Conc: 71.40 ng/ml