

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2021 00:27
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 00:52:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.919	3.931	2524457	1816970	44.437	43.550
2)	SA Decachlor...	10.912	9.191	1856432	1619428	48.265	42.175m
Target Compounds							
16)	L4 AR-1242-1	6.241	5.178	622977	445435	493.301	502.064
17)	L4 AR-1242-2	6.264	5.198	924373	787806	466.401	455.159
18)	L4 AR-1242-3	6.330	5.387	573973	371643	452.961	461.389
19)	L4 AR-1242-4	6.439	5.482	449272	383567	463.980	441.880
20)	L4 AR-1242-5	7.221	6.044	465138	498830	462.972m	494.974

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2021 00:27
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 00:52:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

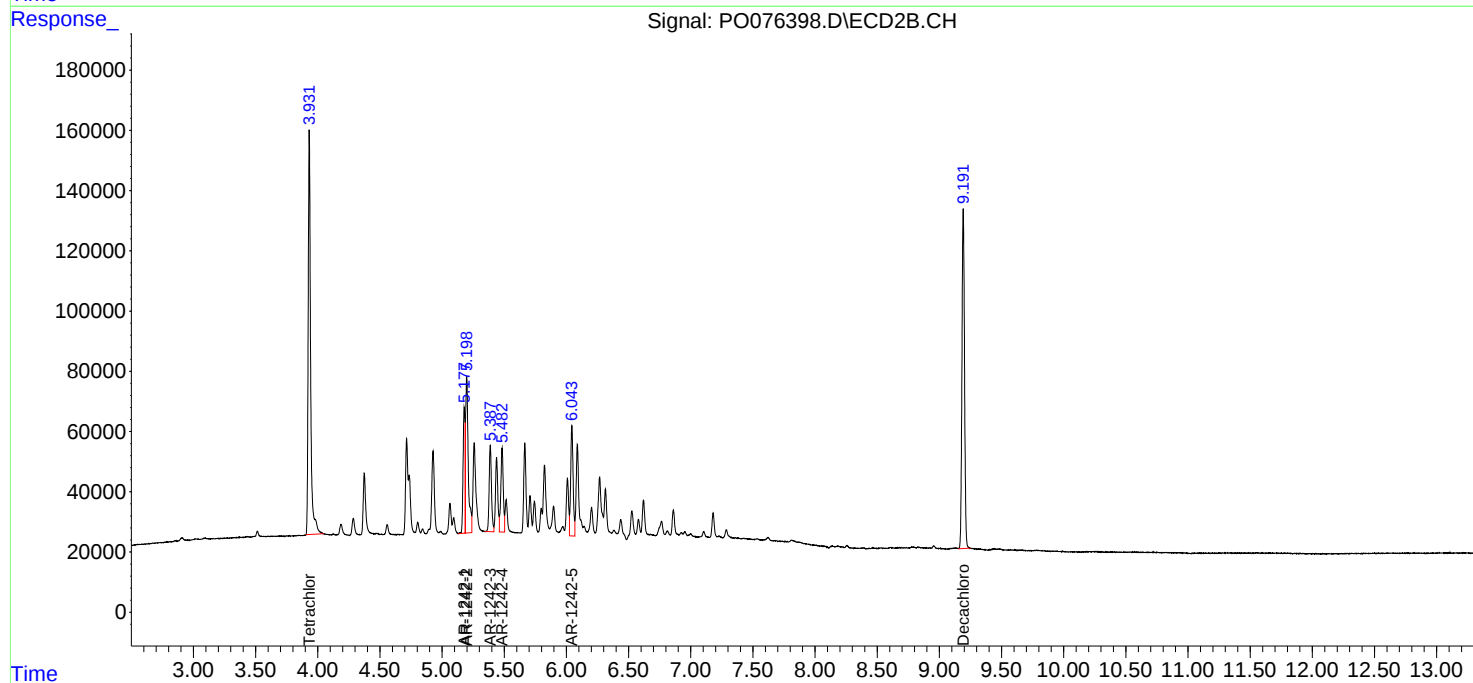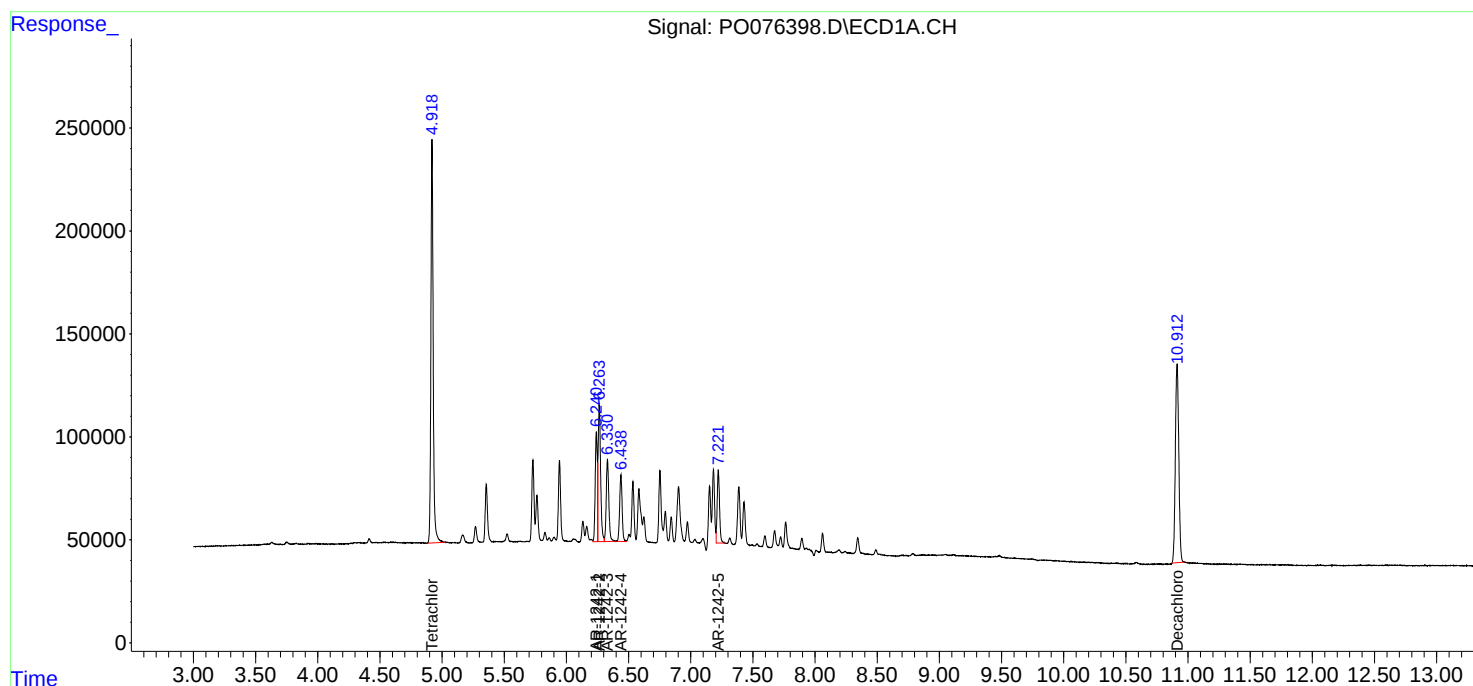

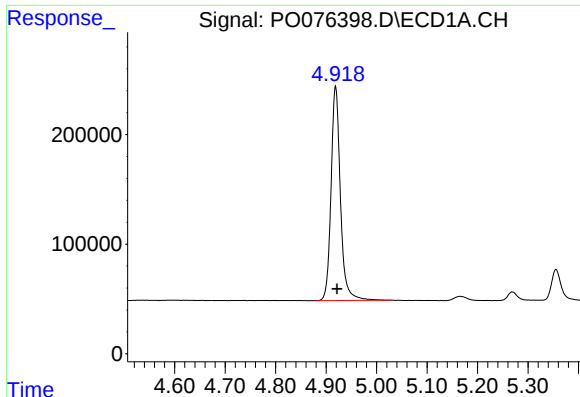


#1 Tetrachloro-m-xylene

R.T.: 4.919 min
Delta R.T.: -0.003 min
Response: 2524457
Conc: 44.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:39 PM

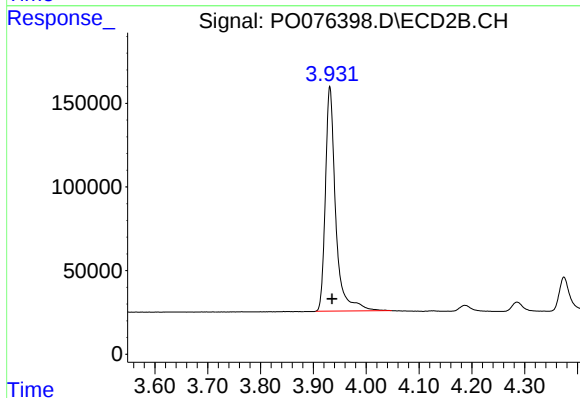


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 1816970
Conc: 43.55 ng/ml

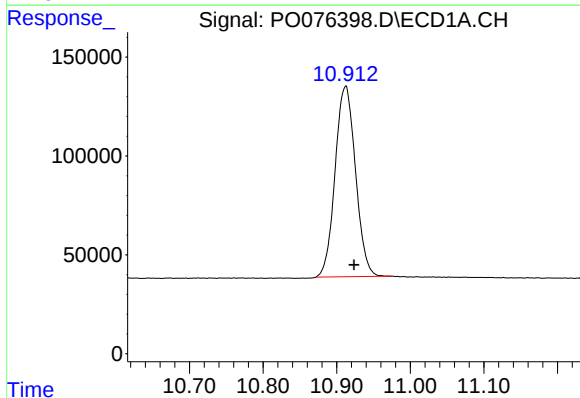


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.011 min
Response: 1856432
Conc: 48.26 ng/ml

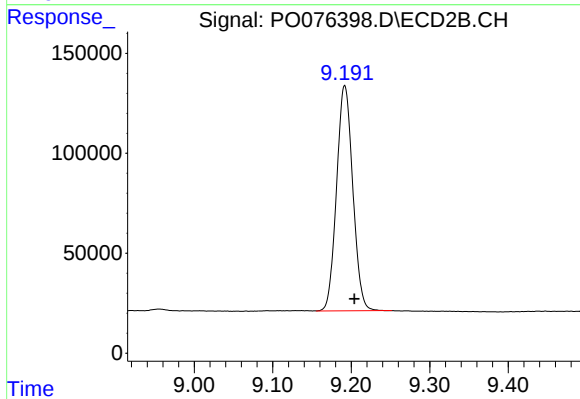

#2 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: -0.013 min
Response: 1619428
Conc: 42.18 ng/ml m

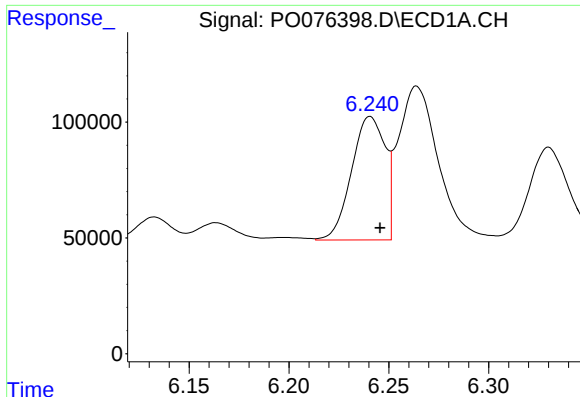


#16 AR-1242-1

R.T.: 6.241 min
Delta R.T.: -0.005 min
Response: 622977
Conc: 493.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:39 PM

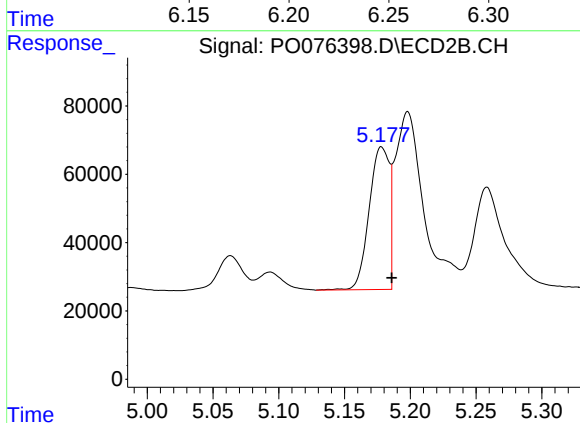


#16 AR-1242-1

R.T.: 5.178 min
Delta R.T.: -0.008 min
Response: 445435
Conc: 502.06 ng/ml

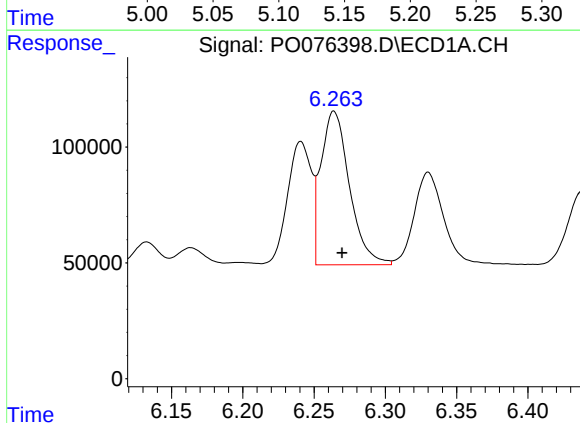


#17 AR-1242-2

R.T.: 6.264 min
Delta R.T.: -0.006 min
Response: 924373
Conc: 466.40 ng/ml

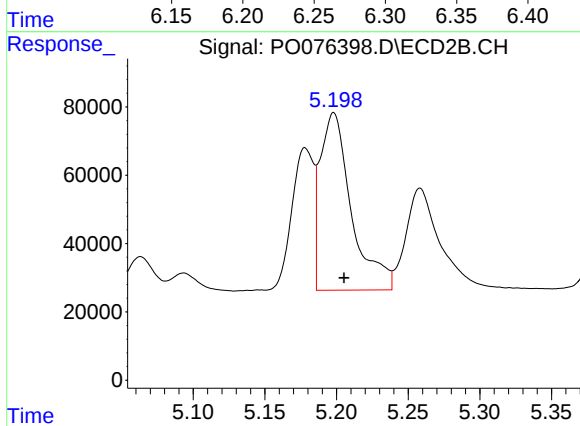

#17 AR-1242-2

R.T.: 5.198 min
Delta R.T.: -0.007 min
Response: 787806
Conc: 455.16 ng/ml

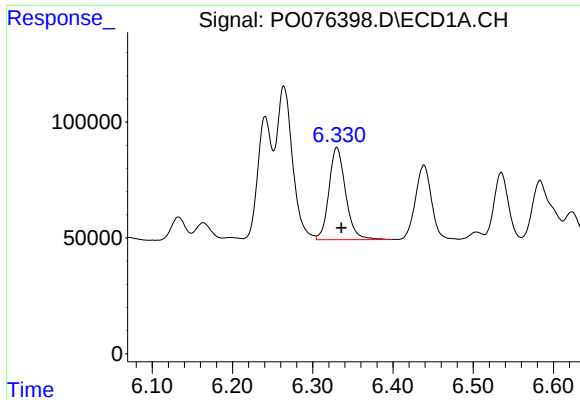


#18 AR-1242-3

R.T.: 6.330 min
Delta R.T.: -0.006 min
Response: 573973
Conc: 452.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:39 PM

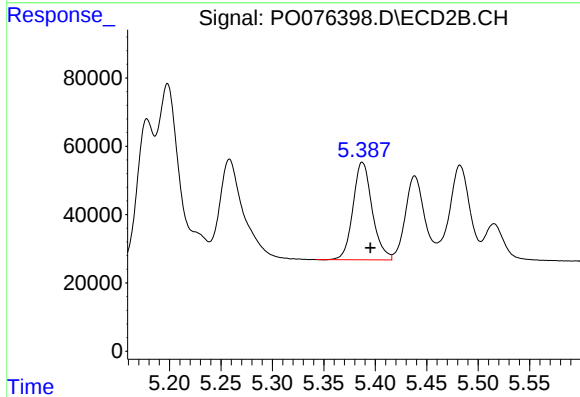


#18 AR-1242-3

R.T.: 5.387 min
Delta R.T.: -0.008 min
Response: 371643
Conc: 461.39 ng/ml

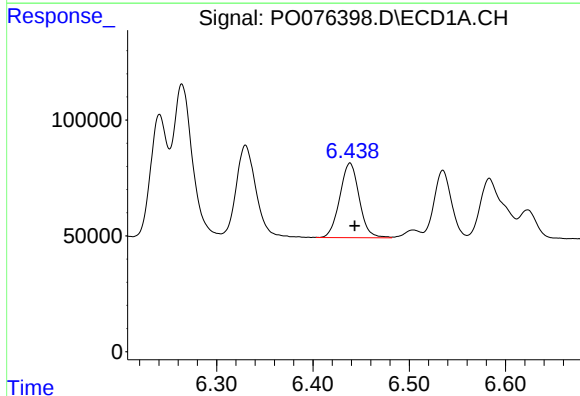


#19 AR-1242-4

R.T.: 6.439 min
Delta R.T.: -0.005 min
Response: 449272
Conc: 463.98 ng/ml

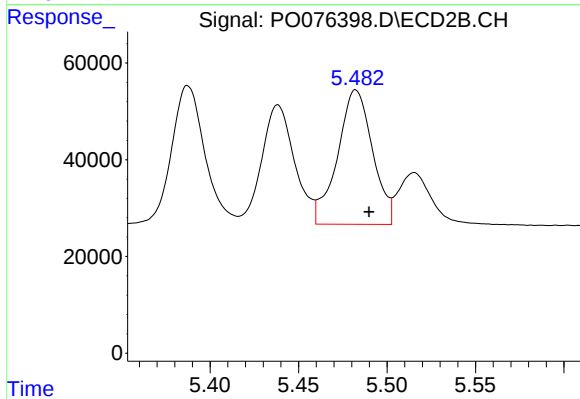

#19 AR-1242-4

R.T.: 5.482 min
Delta R.T.: -0.007 min
Response: 383567
Conc: 441.88 ng/ml

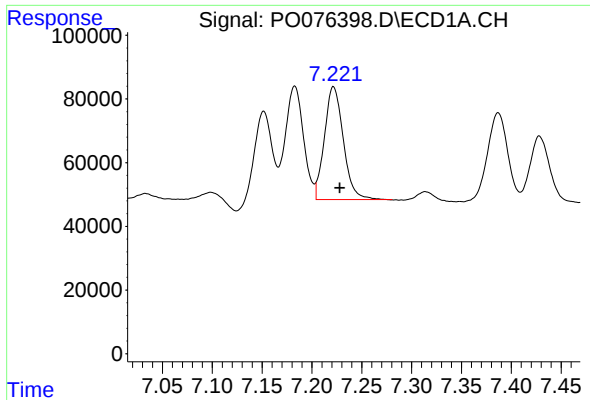


#20 AR-1242-5

R.T.: 7.221 min
Delta R.T.: -0.007 min
Response: 465138
Conc: 462.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:39 PM

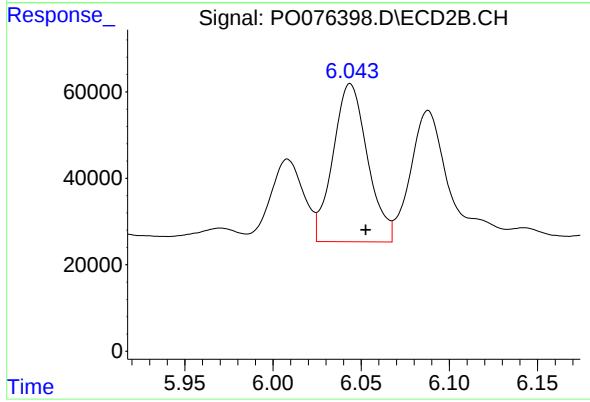

#20 AR-1242-5

R.T.: 6.044 min
Delta R.T.: -0.009 min
Response: 498830
Conc: 494.97 ng/ml