

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
 Data File : P0076399.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2021 00:44
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/22/2021 2:42:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:02:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.921	3.934	2519664	1818353	44.353	43.583
2)	SA Decachlor...	10.915	9.194	1874148	1633448	48.725	42.540
Target Compounds							
21)	L5 AR-1248-1	6.243	5.181	470397	354352	498.948	515.957
22)	L5 AR-1248-2	6.537	5.441	675402	562294	448.357	434.587
23)	L5 AR-1248-3	6.755	5.485	791316	562463	456.244	440.042
24)	L5 AR-1248-4	7.184	5.667	829909	624951	471.718m	425.003
25)	L5 AR-1248-5	7.224	6.090	798405	679400	451.424m	439.296

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031921\
Data File : P0076399.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2021 00:44
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:02:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

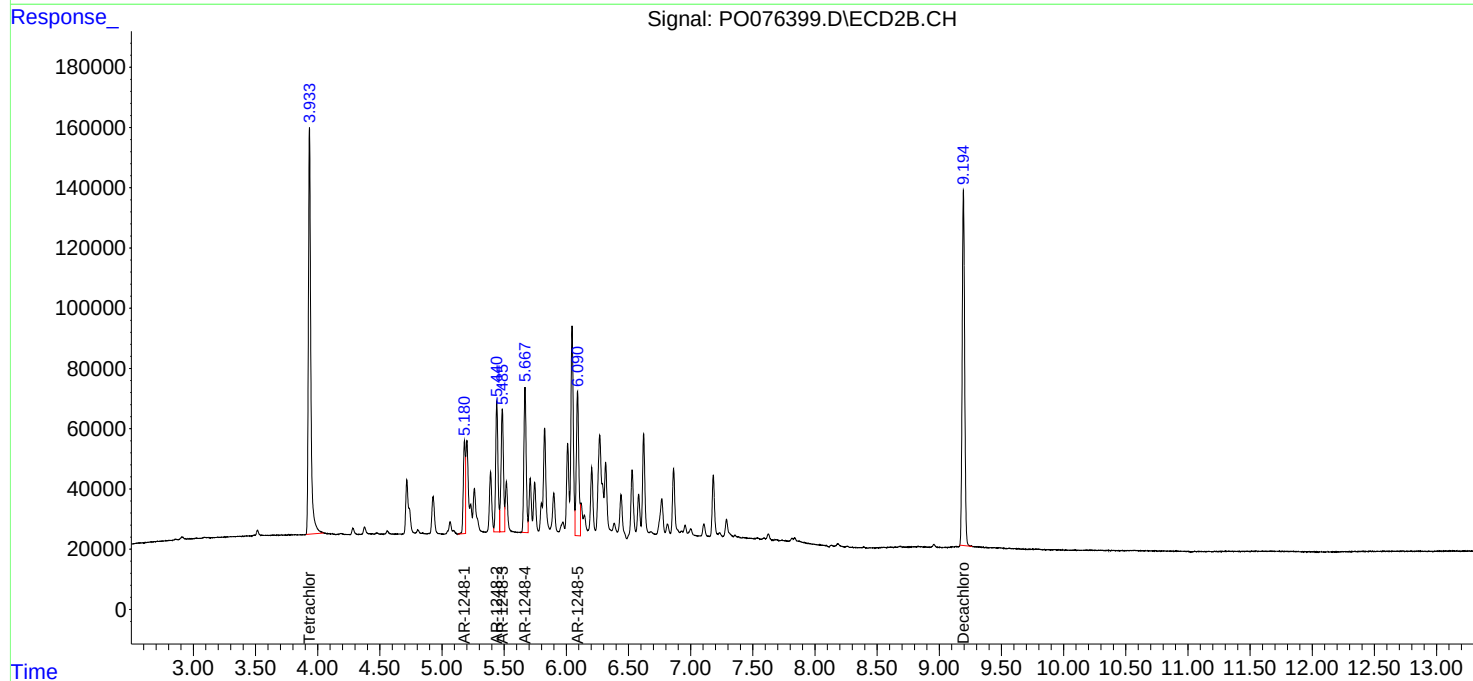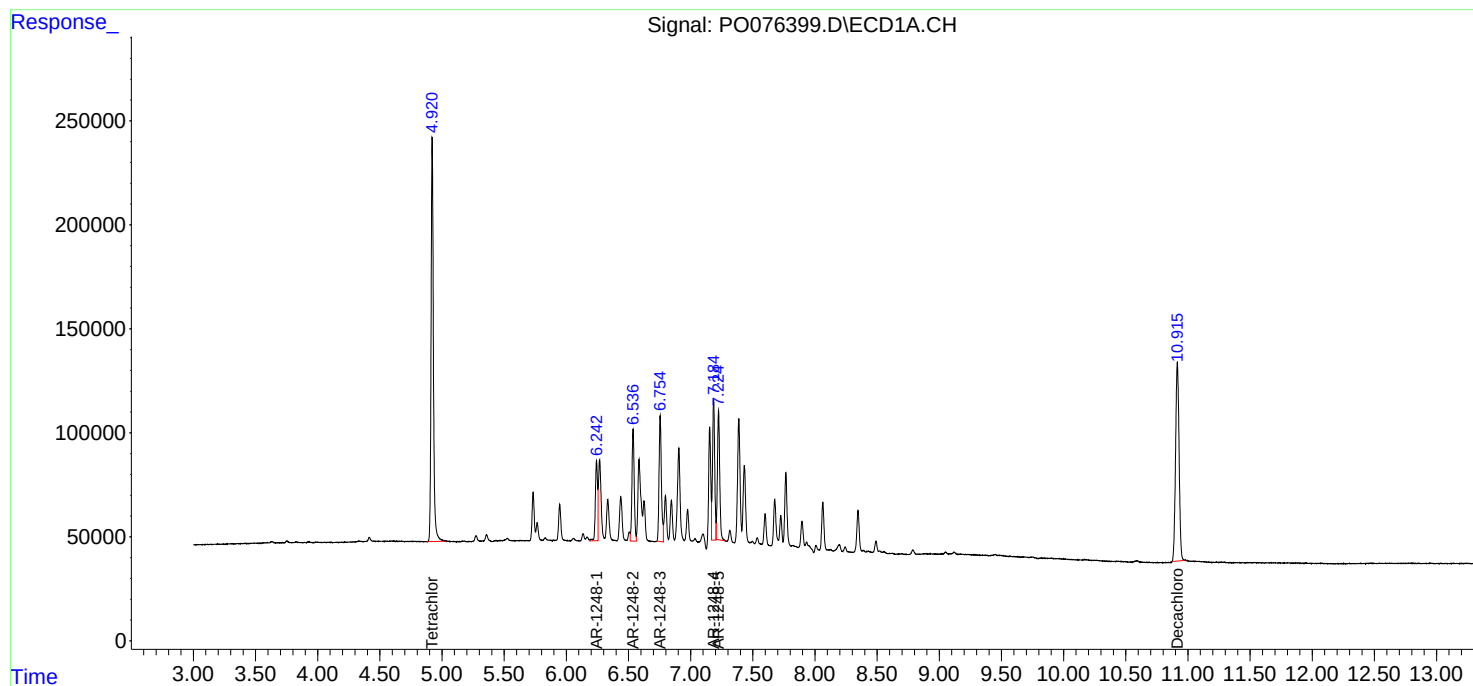

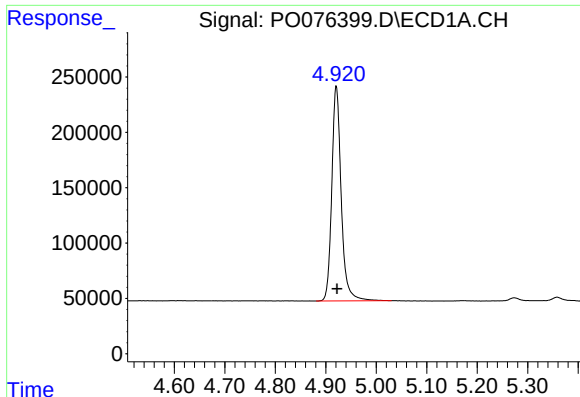


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 2519664
Conc: 44.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:55 PM

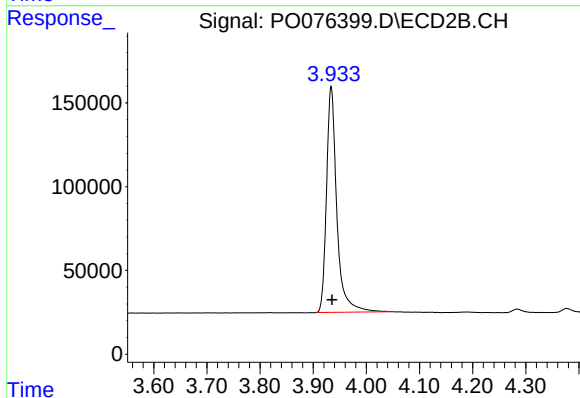


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 1818353
Conc: 43.58 ng/ml

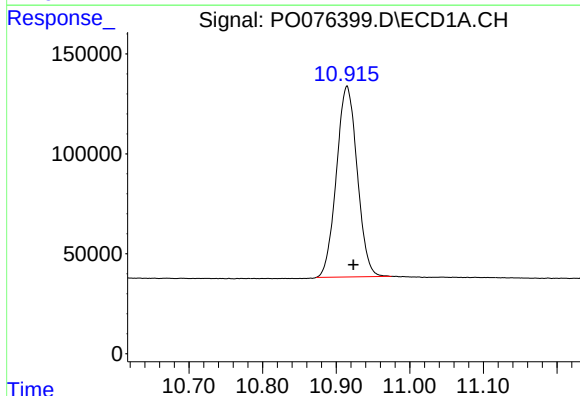


#2 Decachlorobiphenyl

R.T.: 10.915 min
Delta R.T.: -0.009 min
Response: 1874148
Conc: 48.73 ng/ml

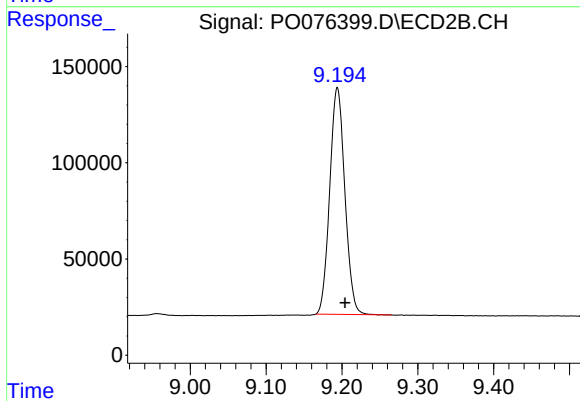

#2 Decachlorobiphenyl

R.T.: 9.194 min
Delta R.T.: -0.010 min
Response: 1633448
Conc: 42.54 ng/ml

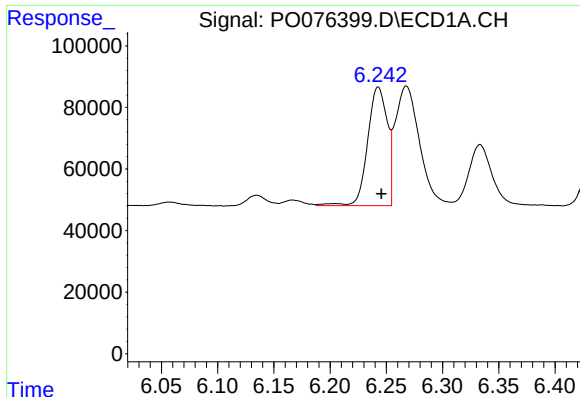


#21 AR-1248-1

R.T.: 6.243 min
Delta R.T.: -0.003 min
Response: 470397
Conc: 498.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:55 PM

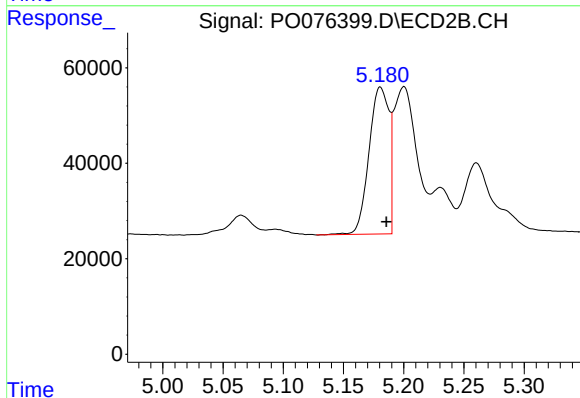


#21 AR-1248-1

R.T.: 5.181 min
Delta R.T.: -0.005 min
Response: 354352
Conc: 515.96 ng/ml

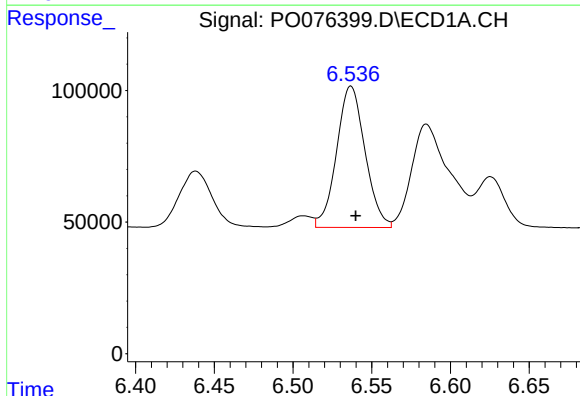


#22 AR-1248-2

R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 675402
Conc: 448.36 ng/ml

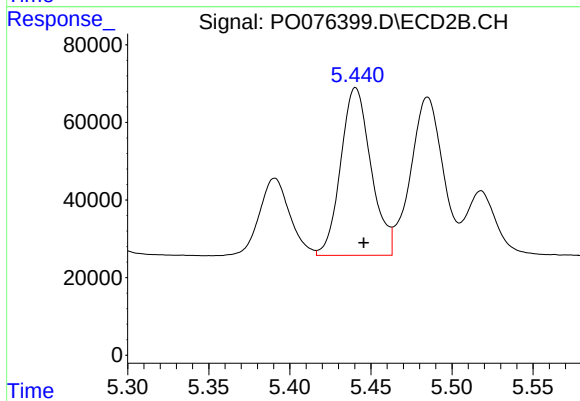

#22 AR-1248-2

R.T.: 5.441 min
Delta R.T.: -0.005 min
Response: 562294
Conc: 434.59 ng/ml

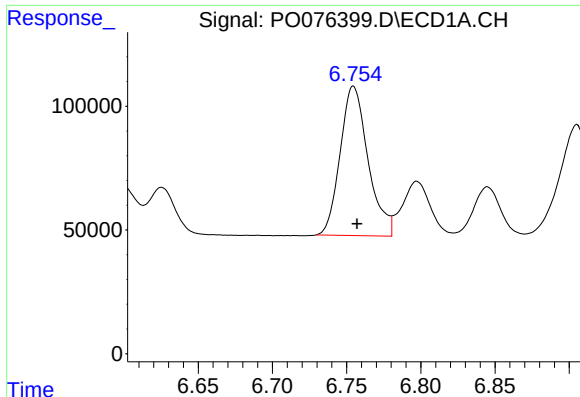


#23 AR-1248-3

R.T.: 6.755 min
Delta R.T.: -0.003 min
Response: 791316
Conc: 456.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:55 PM

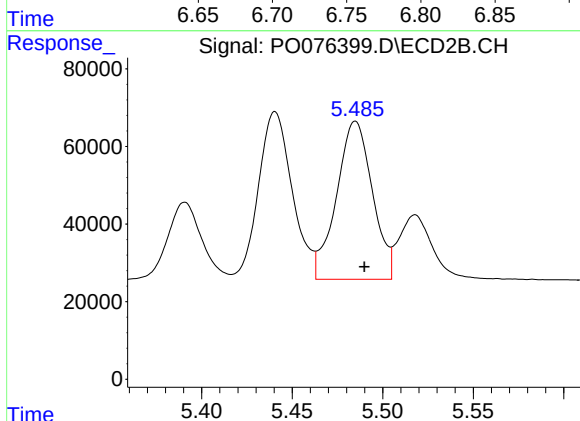


#23 AR-1248-3

R.T.: 5.485 min
Delta R.T.: -0.005 min
Response: 562463
Conc: 440.04 ng/ml

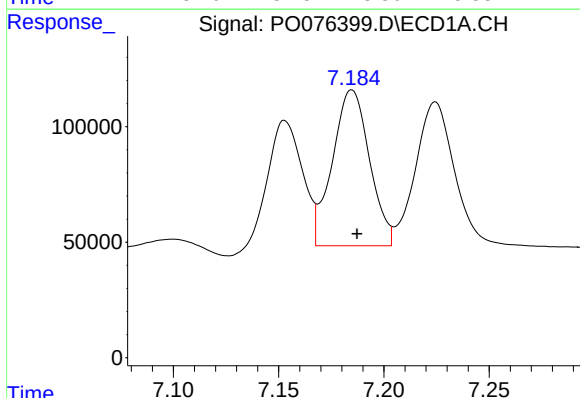


#24 AR-1248-4

R.T.: 7.184 min
Delta R.T.: -0.003 min
Response: 829909
Conc: 471.72 ng/ml m

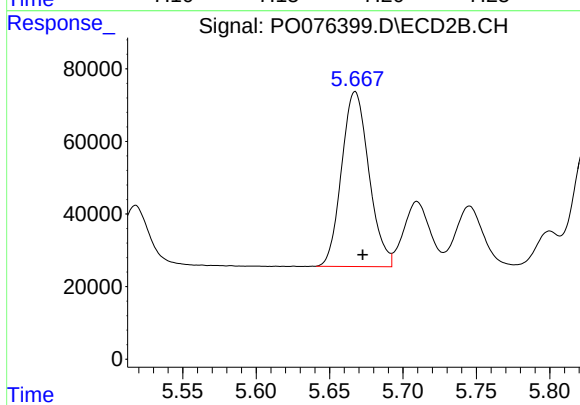

#24 AR-1248-4

R.T.: 5.667 min
Delta R.T.: -0.005 min
Response: 624951
Conc: 425.00 ng/ml

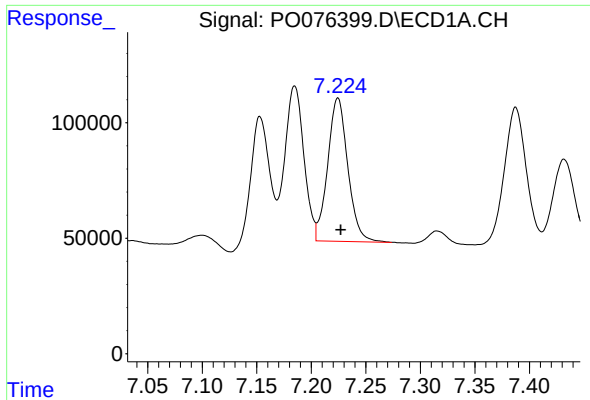


#25 AR-1248-5

R.T.: 7.224 min
Delta R.T.: -0.003 min
Response: 798405
Conc: 451.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/22/2021 2:42:55 PM

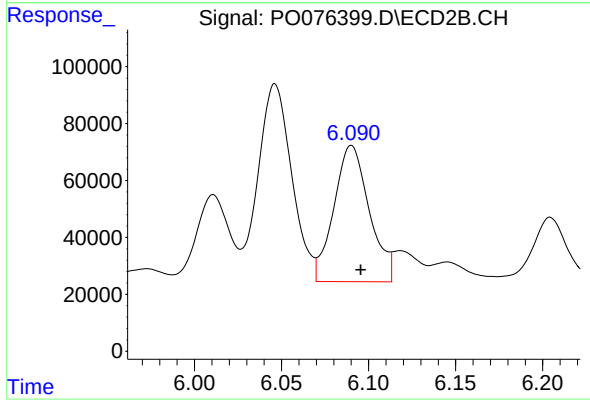

#25 AR-1248-5

R.T.: 6.090 min
Delta R.T.: -0.005 min
Response: 679400
Conc: 439.30 ng/ml