

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031923\
 Data File : P0093324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2023 13:02
 Operator : YP/AJ
 Sample : 01975-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHAMBER-C-72-WEST

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/20/2023
 Supervised By :Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 20:36:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.631	27610661	6069475	8.817	5.381 #
2) SA Decachlor...	10.256	8.659	14751625	7496956	6.816	7.657
Target Compounds						
31) L7 AR-1260-1	7.196	6.202	555.3E6	161.7E6	4286.576m	2659.031 #
32) L7 AR-1260-2	7.481	6.413	297.3E6	407.1E6	2014.108	5630.383m#
33) L7 AR-1260-3	7.843	6.547	190.3E6	94011596	1692.199	1405.915
34) L7 AR-1260-4	8.070	7.021	164.2E6	73991764	1280.699	1344.534
35) L7 AR-1260-5	8.397	7.264	455.9E6	217.6E6	2040.445	1848.510

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031923\
Data File : PO093324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2023 13:02
Operator : YP/AJ
Sample : 01975-04
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 20:36:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

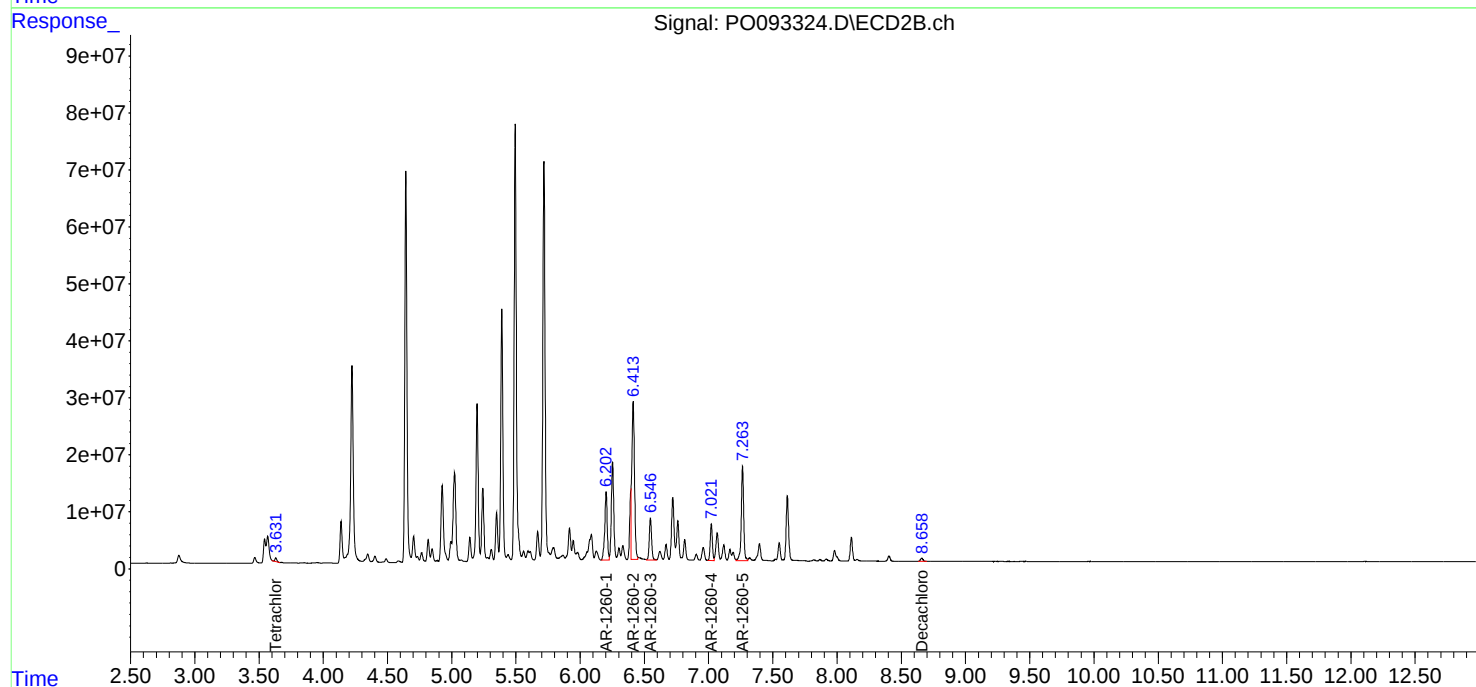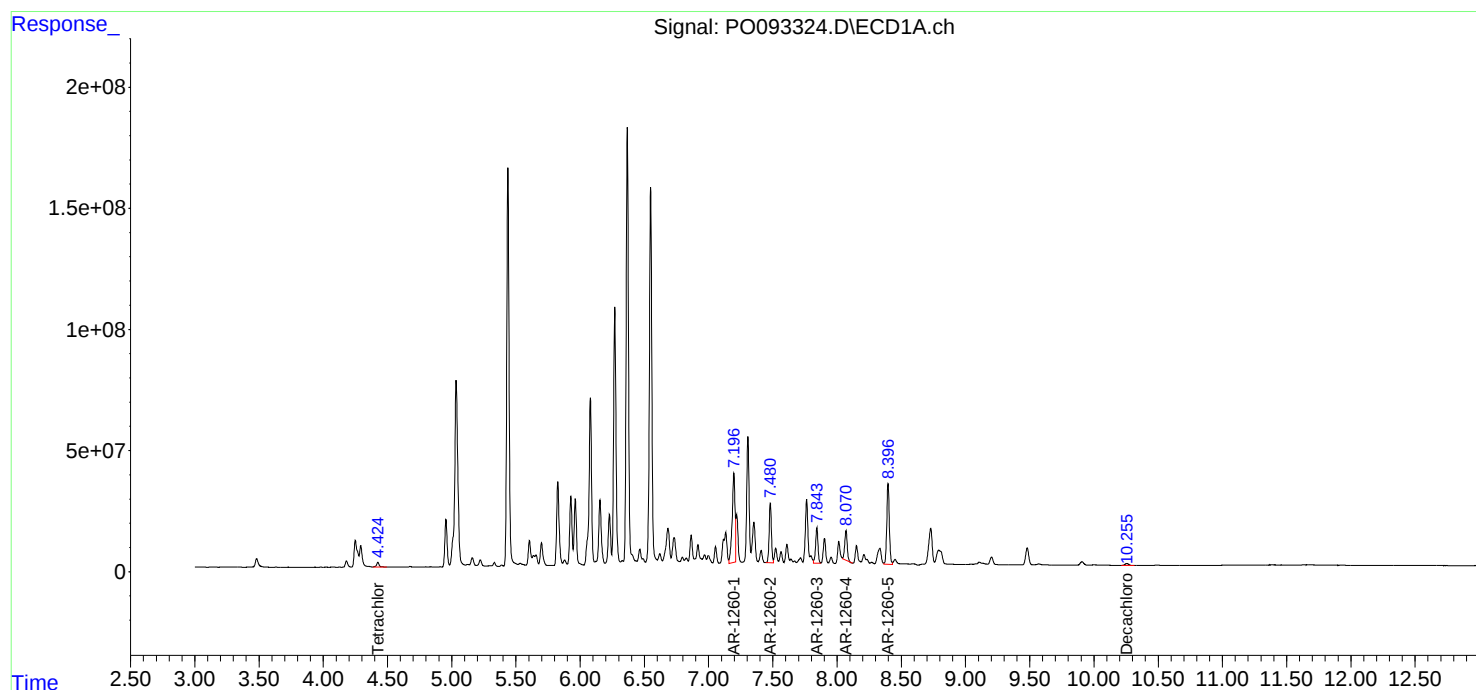

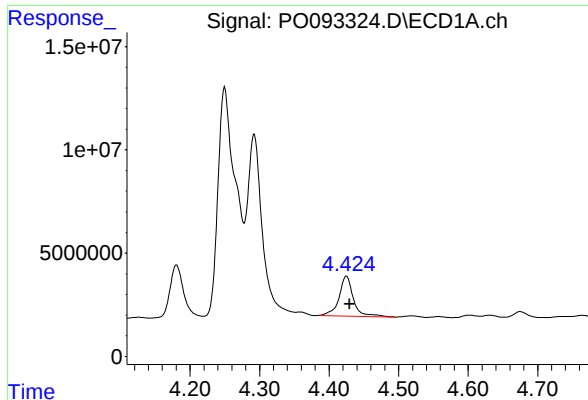


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 27610661
Conc: 8.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

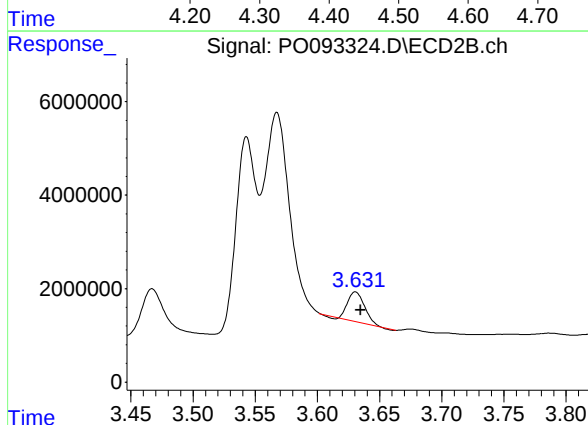


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 6069475
Conc: 5.38 ng/ml

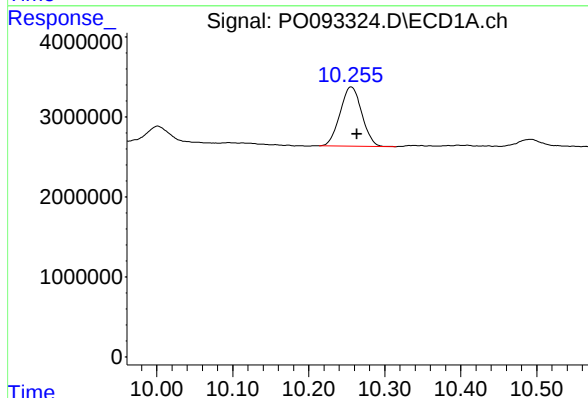


#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: -0.007 min
Response: 14751625
Conc: 6.82 ng/ml

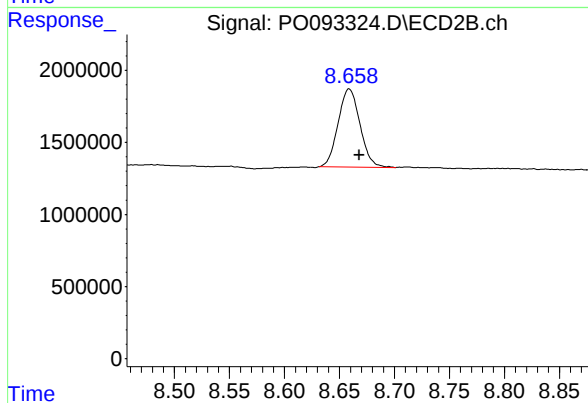

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.009 min
Response: 7496956
Conc: 7.66 ng/ml

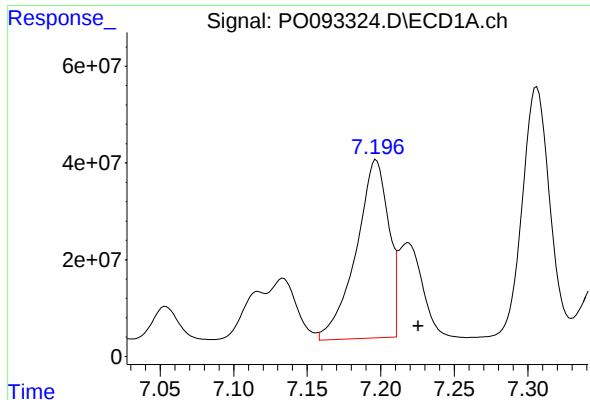


#31 AR-1260-1

R.T.: 7.196 min
Delta R.T.: -0.029 min
Response: 555337189
Conc: 4286.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

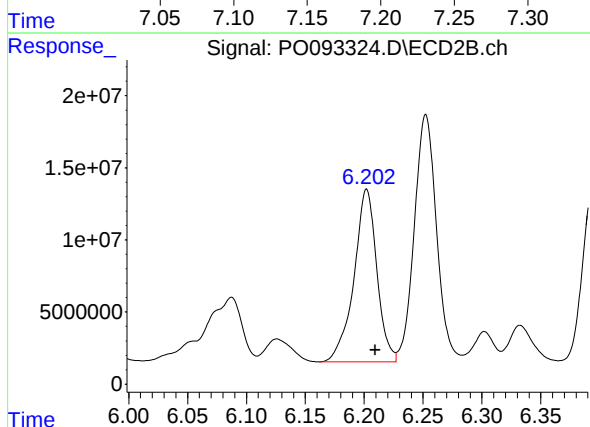


#31 AR-1260-1

R.T.: 6.202 min
Delta R.T.: -0.007 min
Response: 161665083
Conc: 2659.03 ng/ml

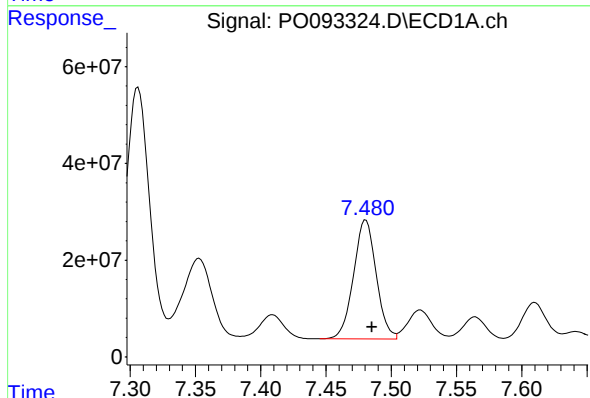


#32 AR-1260-2

R.T.: 7.481 min
Delta R.T.: -0.005 min
Response: 297332686
Conc: 2014.11 ng/ml

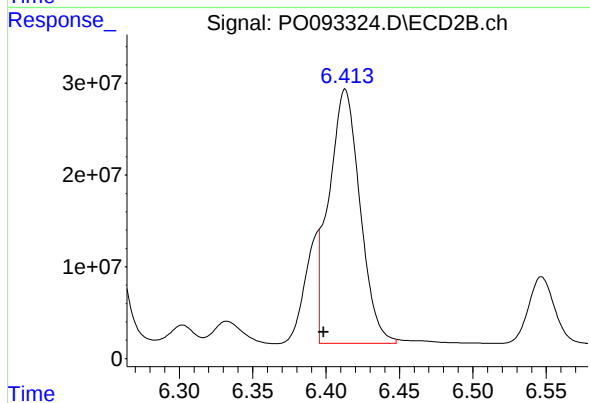

#32 AR-1260-2

R.T.: 6.413 min
Delta R.T.: 0.014 min
Response: 407058211
Conc: 5630.38 ng/ml m

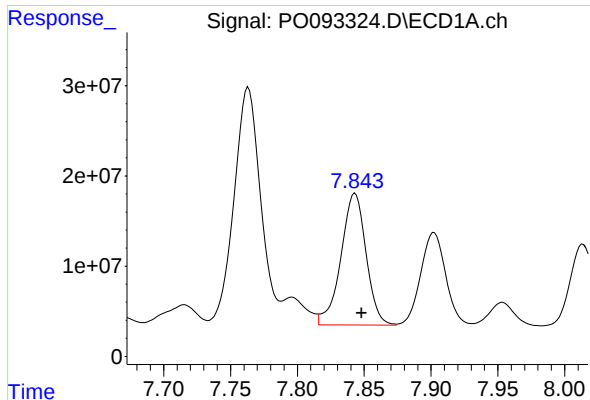


#33 AR-1260-3

R.T.: 7.843 min
Delta R.T.: -0.005 min
Response: 190339897
Conc: 1692.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

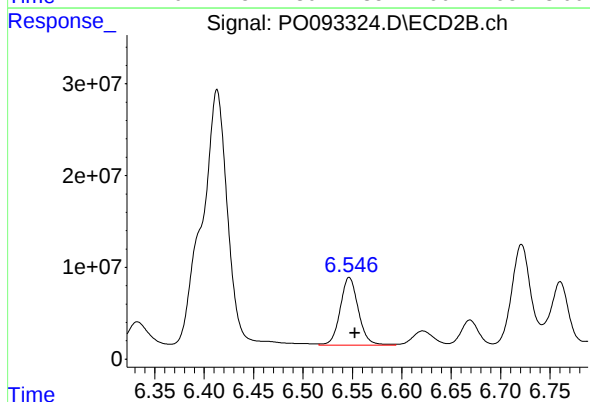


#33 AR-1260-3

R.T.: 6.547 min
Delta R.T.: -0.006 min
Response: 94011596
Conc: 1405.91 ng/ml

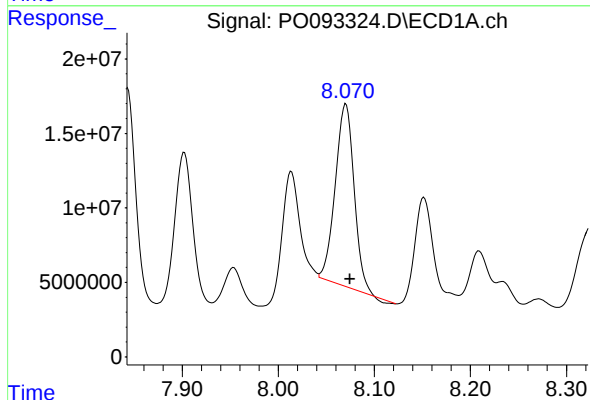


#34 AR-1260-4

R.T.: 8.070 min
Delta R.T.: -0.005 min
Response: 164234190
Conc: 1280.70 ng/ml

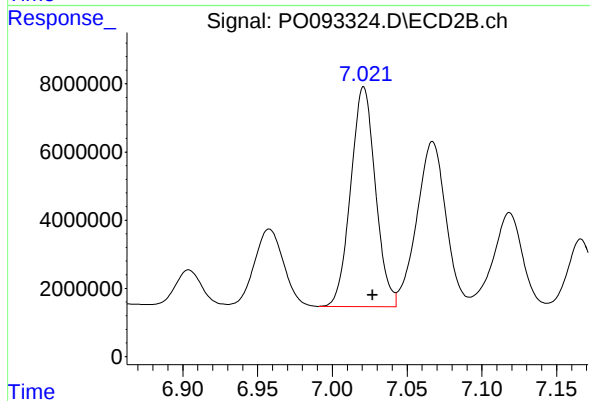

#34 AR-1260-4

R.T.: 7.021 min
Delta R.T.: -0.006 min
Response: 73991764
Conc: 1344.53 ng/ml

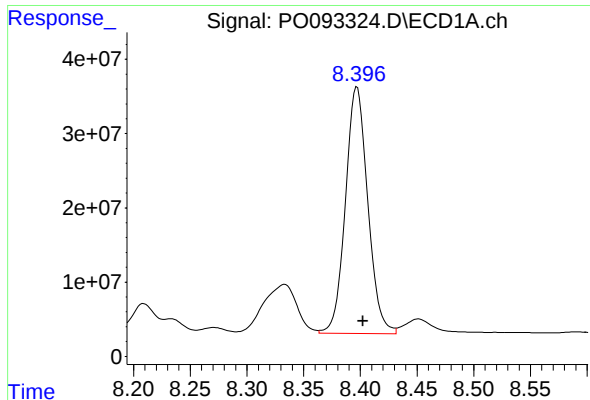


#35 AR-1260-5

R.T.: 8.397 min
Delta R.T.: -0.005 min
Response: 455907239
Conc: 2040.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WEST

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

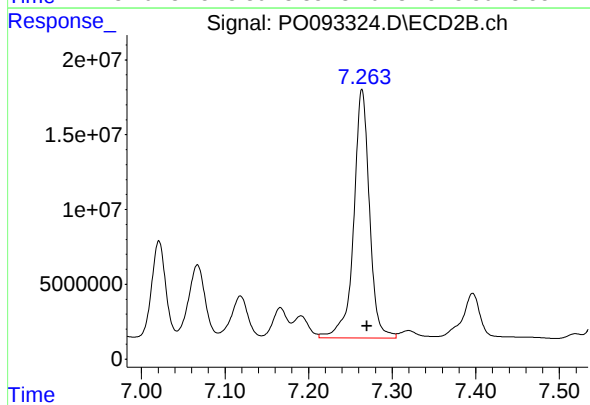

#35 AR-1260-5

R.T.: 7.264 min
Delta R.T.: -0.006 min
Response: 217626316
Conc: 1848.51 ng/ml