

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031923\
 Data File : P0093325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2023 13:20
 Operator : YP/AJ
 Sample : 01998-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BRAOD-CHANNEL-SUBSTATION-TP1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/20/2023
 Supervised By :Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 20:36:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.427	3.632	72465821	25700594	23.141	22.787
2) SA Decachlor...	10.256	8.661	56227421	23501998	25.980	24.003

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031923\
Data File : PO093325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2023 13:20
Operator : YP/AJ
Sample : 01998-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BRAOD-CHANNEL-SUBSTATION-TP1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 20:36:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

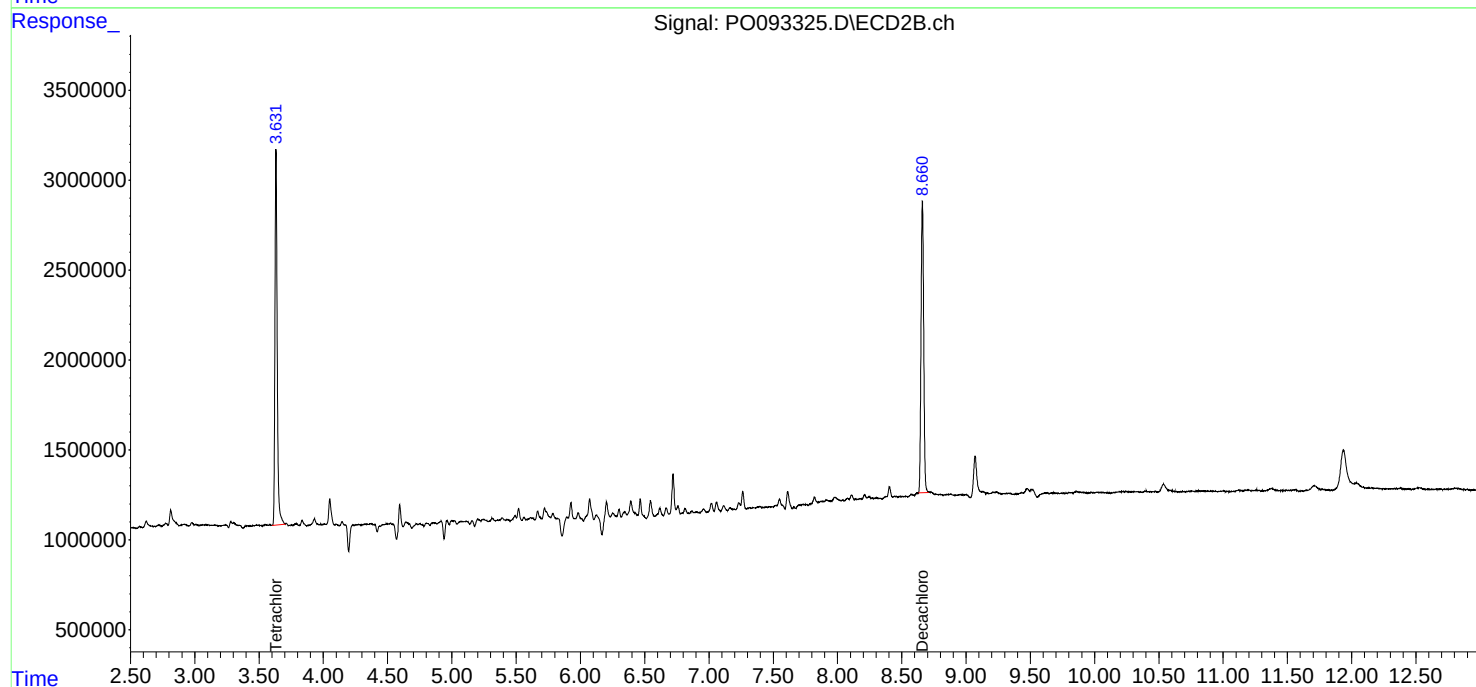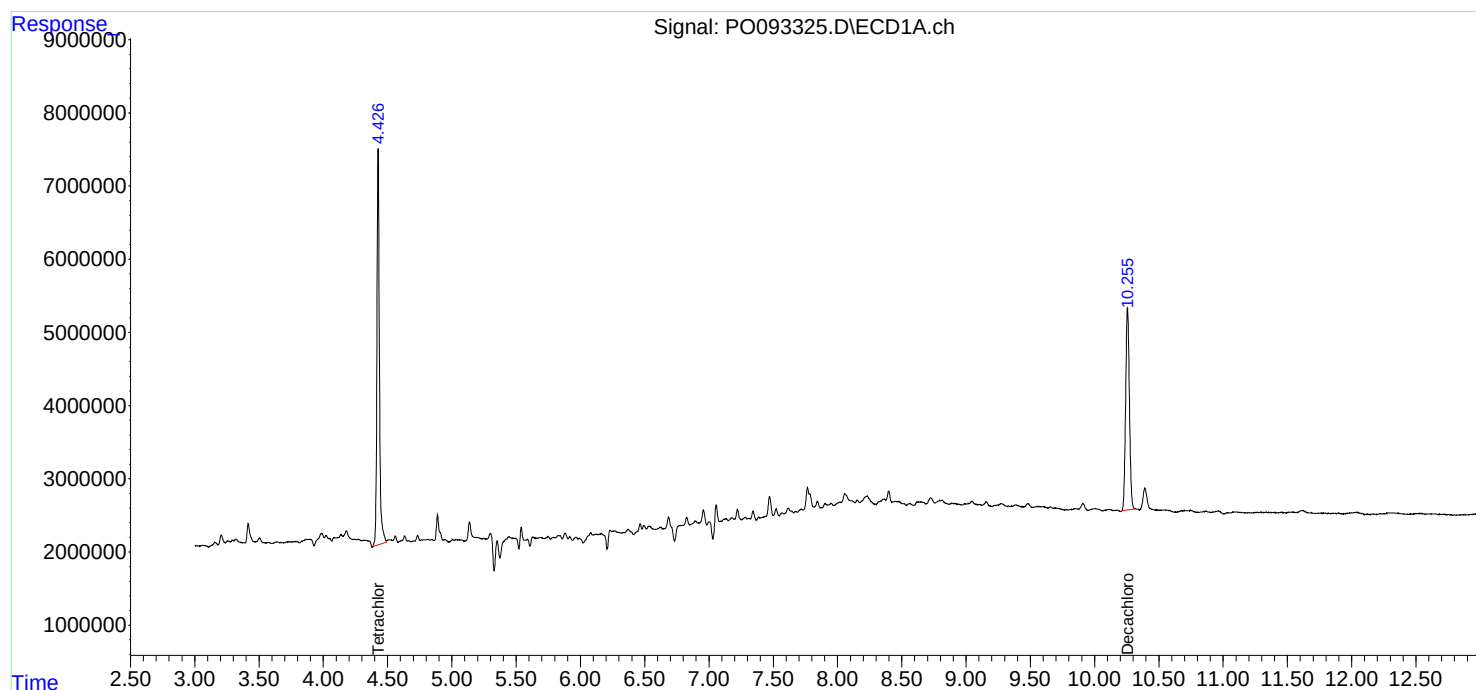

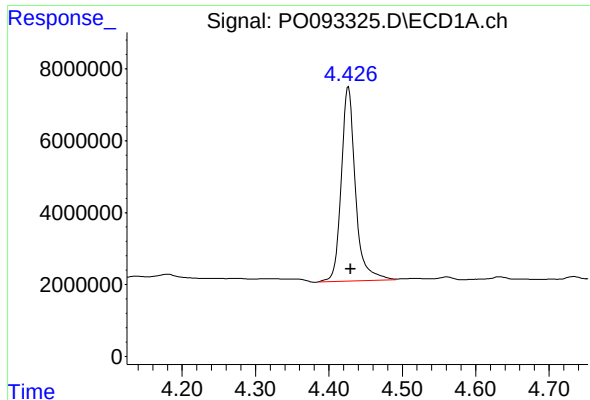

#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: -0.003 min
Response: 72465821
Conc: 23.14 ng/ml

Instrument :

ECD_O


ClientSampleId :

BRAOD-CHANNEL-SUBSTATION-TP1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 03/20/2023
Supervised By :Ankita Jodhani 03/20/2023

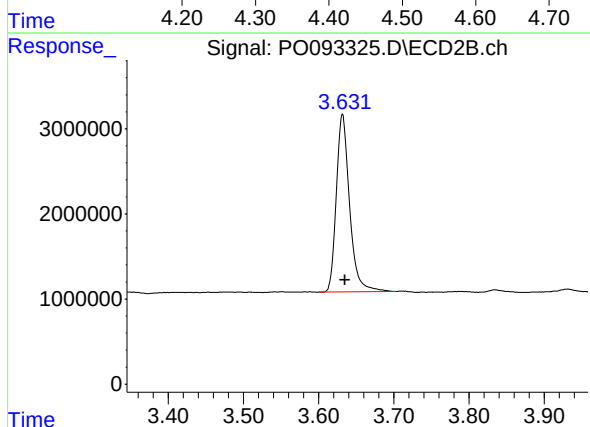


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.003 min
Response: 25700594
Conc: 22.79 ng/ml

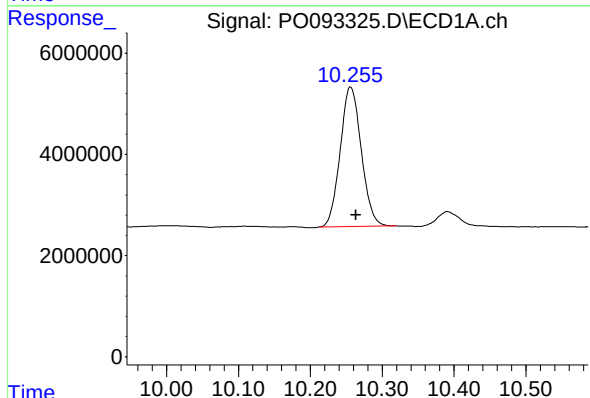

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: -0.007 min
Response: 56227421
Conc: 25.98 ng/ml

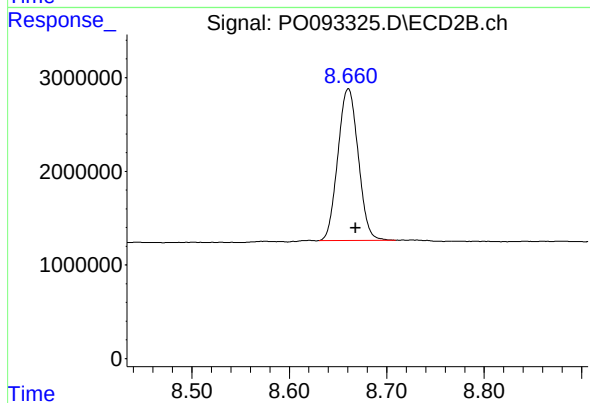

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: -0.007 min
Response: 23501998
Conc: 24.00 ng/ml