

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031924\
 Data File : P0102591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 15:37
 Operator : YP/AJ
 Sample : P1616-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 146-BAY-AVENUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:22:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.266	3.382	71456849	47301696	16.207	16.439
2) SA Decachlor...	9.809	8.248	29259165	19707801	10.538	10.863

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031924\
Data File : PO102591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 15:37
Operator : YP/AJ
Sample : P1616-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
146-BAY-AVENUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:22:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

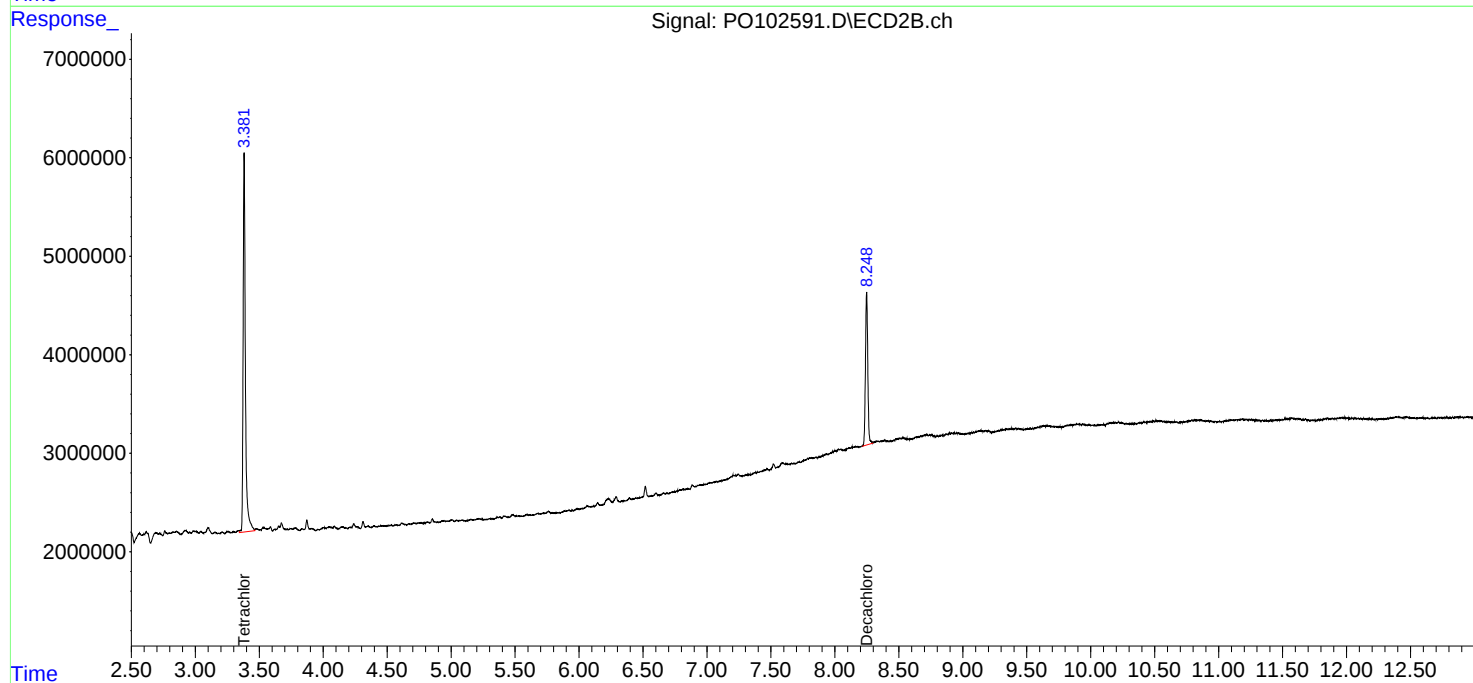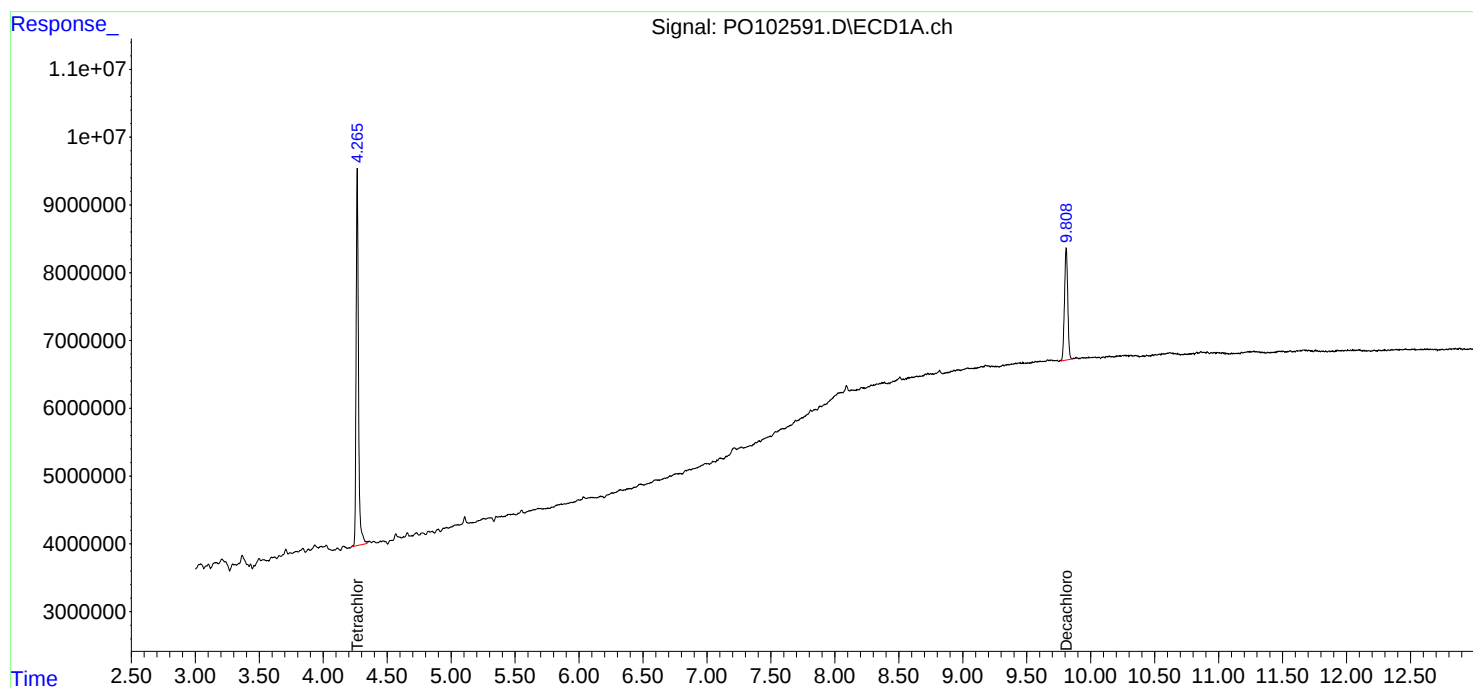


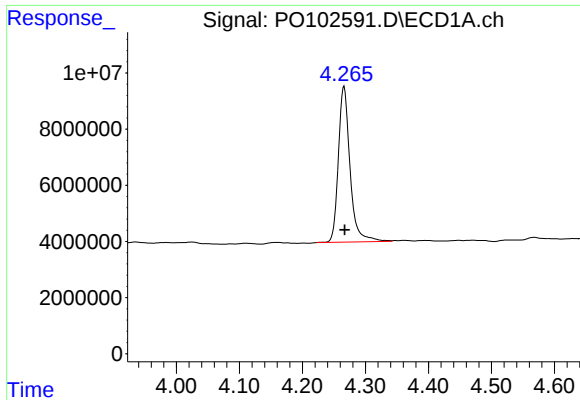

#1 Tetrachloro-m-xylene


R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 71456849
Conc: 16.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
146-BAY-AVENUE

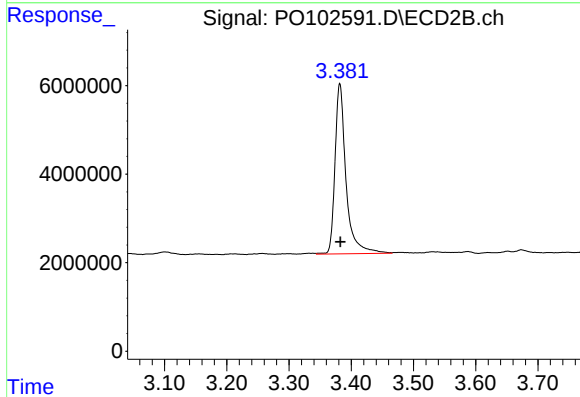


#1 Tetrachloro-m-xylene

R.T.: 3.382 min
Delta R.T.: 0.000 min
Response: 47301696
Conc: 16.44 ng/ml

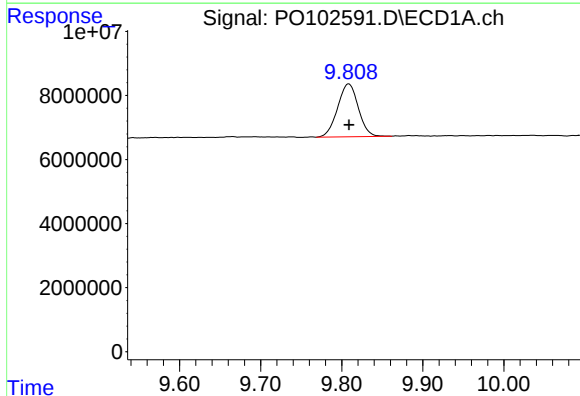

#2 Decachlorobiphenyl

R.T.: 9.809 min
Delta R.T.: 0.000 min
Response: 29259165
Conc: 10.54 ng/ml

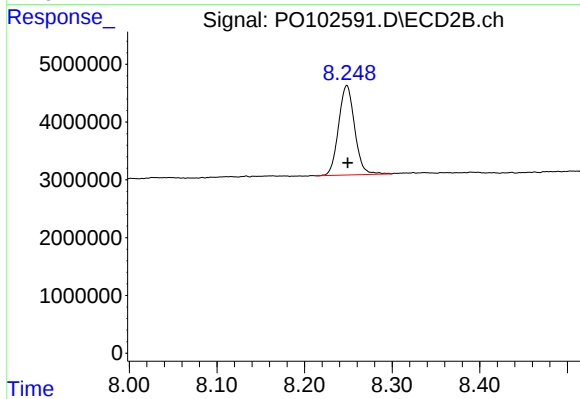

#2 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: -0.001 min
Response: 19707801
Conc: 10.86 ng/ml