

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032023\
 Data File : P0093352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2023 11:07
 Operator : YP/AJ
 Sample : 01975-04DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CHAMBER-C-72-WESTDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/21/2023
 Supervised By :Ankita Jodhani 03/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:44:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.629	6587620	2495037	2.104	2.212m
2) SA Decachlor...	10.252	8.656	2657076	1523208	1.228	1.556 #
Target Compounds						
31) L7 AR-1260-1	7.216	6.200	48437535	36888164	373.883	606.728 #
32) L7 AR-1260-2	7.477	6.410	63721623	82524931	431.645	1141.475m#
33) L7 AR-1260-3	7.840	6.544	41127626	22698505	365.641	339.449
34) L7 AR-1260-4	8.066	7.018	43521583	17305878	339.381m	314.472
35) L7 AR-1260-5	8.394	7.261	89933777	46017969	402.505	390.875

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032023\
Data File : P0093352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2023 11:07
Operator : YP/AJ
Sample : 01975-04DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WESTDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2023
Supervised By :Ankita Jodhani 03/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:44:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

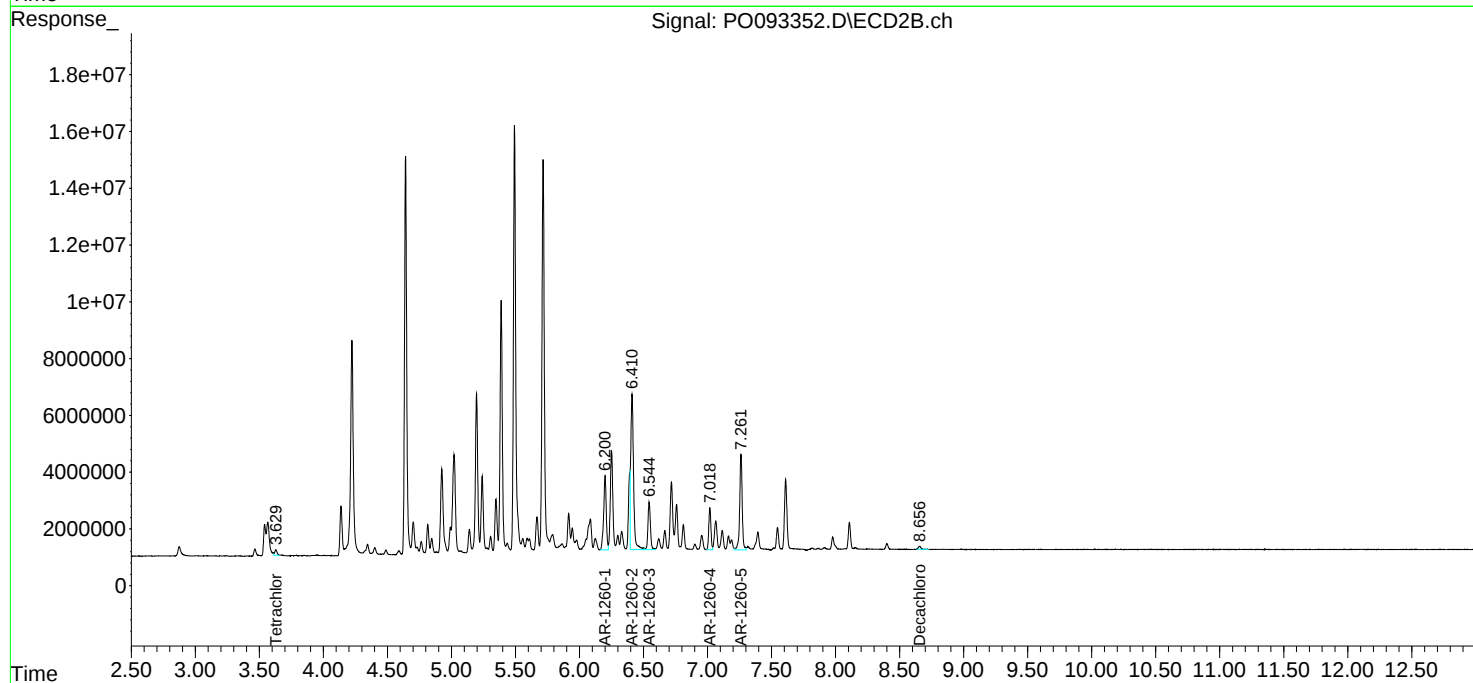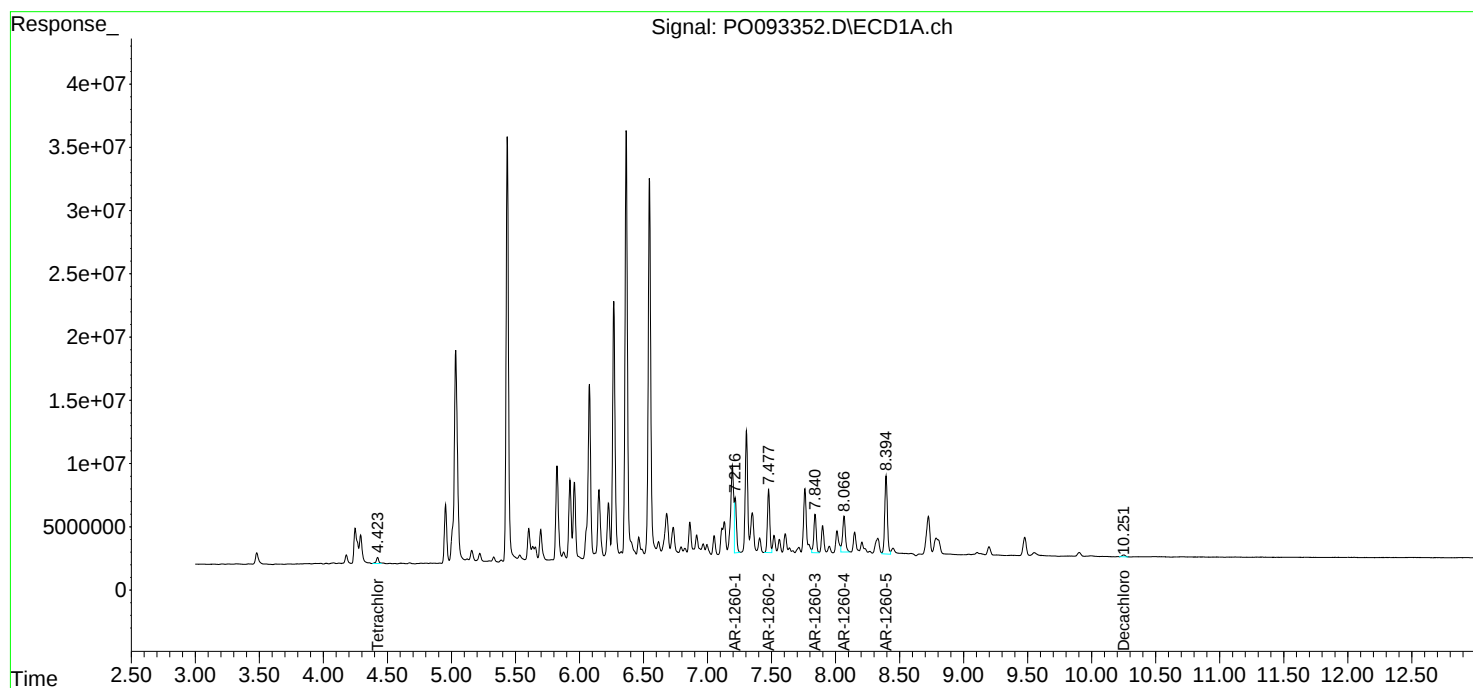

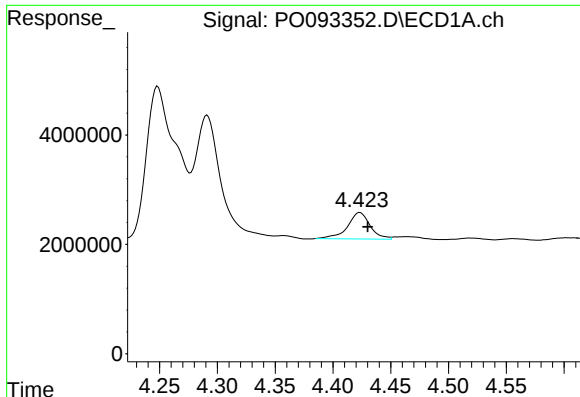


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.007 min
Response: 6587620
Conc: 2.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WESTDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2023
Supervised By :Ankita Jodhani 03/21/2023

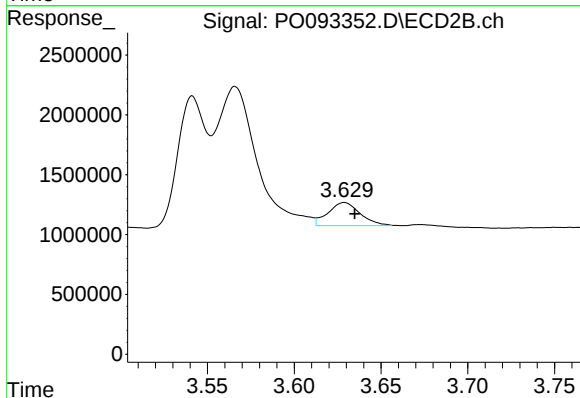


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.006 min
Response: 2495037
Conc: 2.21 ng/ml m

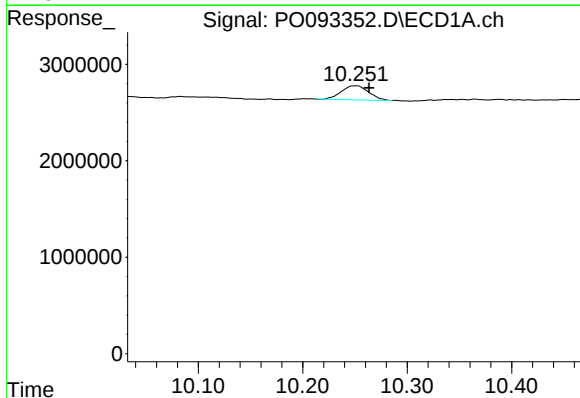


#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: -0.012 min
Response: 2657076
Conc: 1.23 ng/ml

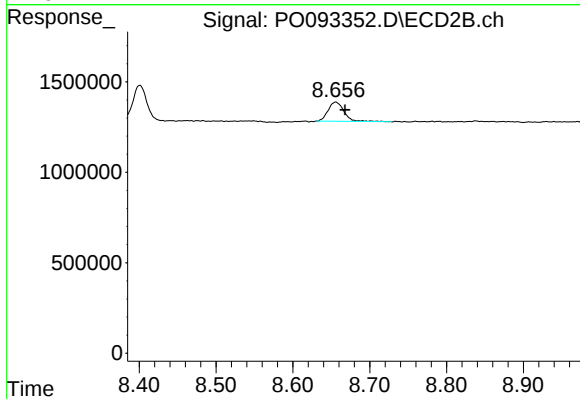

#2 Decachlorobiphenyl

R.T.: 8.656 min
Delta R.T.: -0.012 min
Response: 1523208
Conc: 1.56 ng/ml

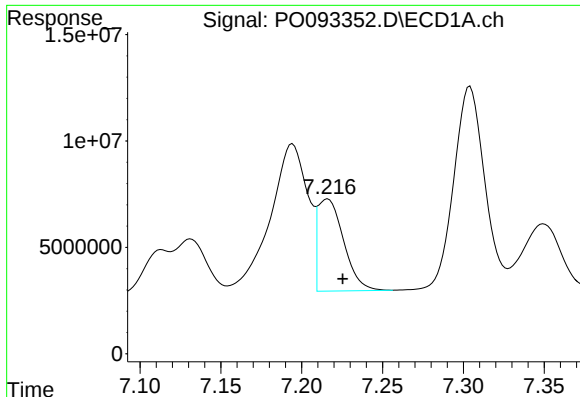


#31 AR-1260-1

R.T.: 7.216 min
Delta R.T.: -0.009 min
Response: 48437535
Conc: 373.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WESTDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2023
Supervised By :Ankita Jodhani 03/21/2023

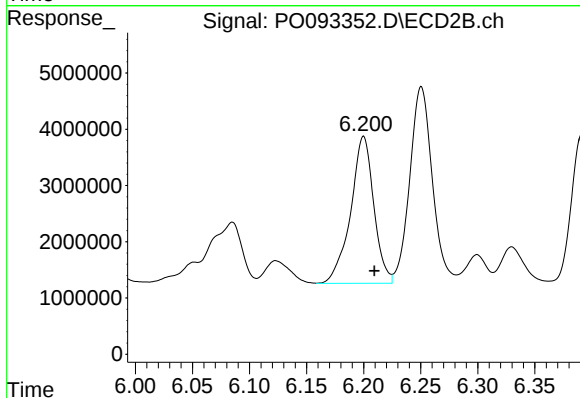


#31 AR-1260-1

R.T.: 6.200 min
Delta R.T.: -0.010 min
Response: 36888164
Conc: 606.73 ng/ml

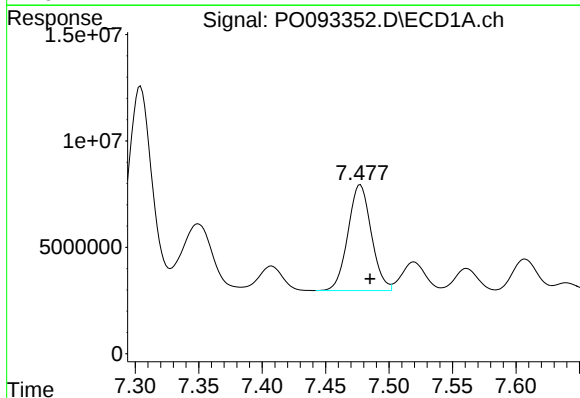


#32 AR-1260-2

R.T.: 7.477 min
Delta R.T.: -0.008 min
Response: 63721623
Conc: 431.65 ng/ml

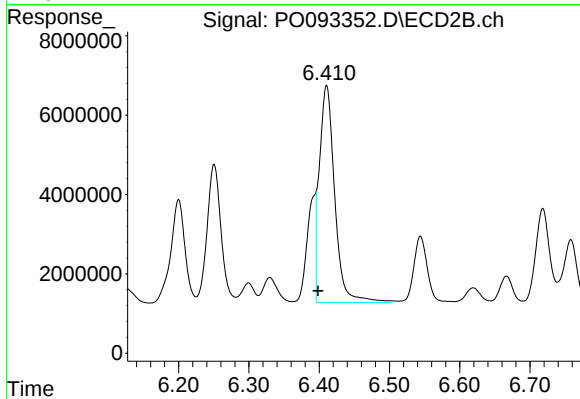

#32 AR-1260-2

R.T.: 6.410 min
Delta R.T.: 0.012 min
Response: 82524931
Conc: 1141.48 ng/ml m

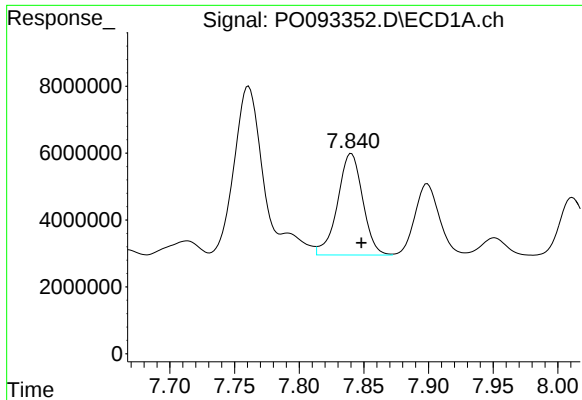


#33 AR-1260-3

R.T.: 7.840 min
Delta R.T.: -0.008 min
Response: 41127626
Conc: 365.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WESTDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2023
Supervised By :Ankita Jodhani 03/21/2023

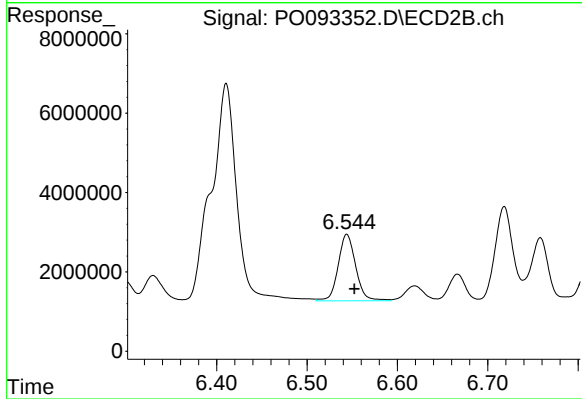


#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: -0.008 min
Response: 22698505
Conc: 339.45 ng/ml

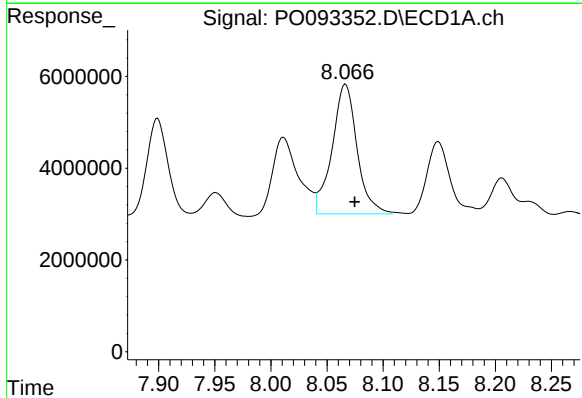


#34 AR-1260-4

R.T.: 8.066 min
Delta R.T.: -0.009 min
Response: 43521583
Conc: 339.38 ng/ml m

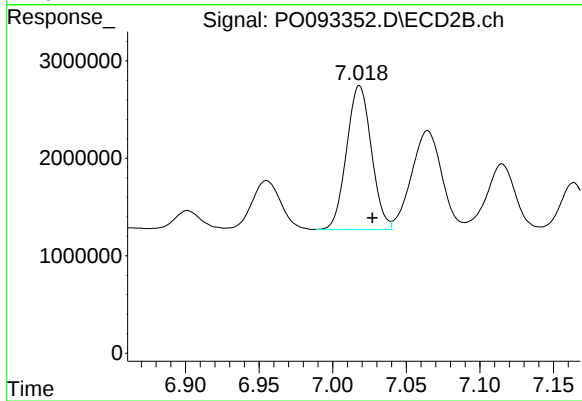

#34 AR-1260-4

R.T.: 7.018 min
Delta R.T.: -0.009 min
Response: 17305878
Conc: 314.47 ng/ml

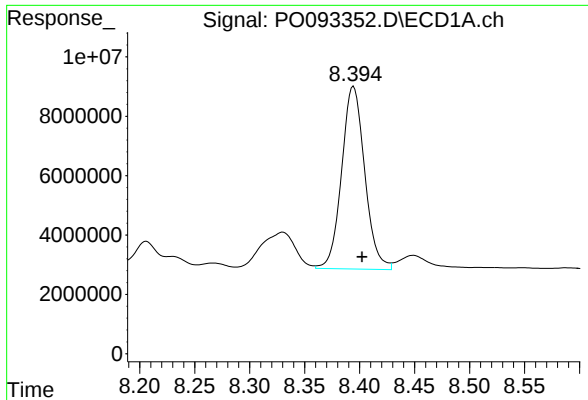


#35 AR-1260-5

R.T.: 8.394 min
Delta R.T.: -0.008 min
Response: 89933777
Conc: 402.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-WESTDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2023
Supervised By :Ankita Jodhani 03/21/2023

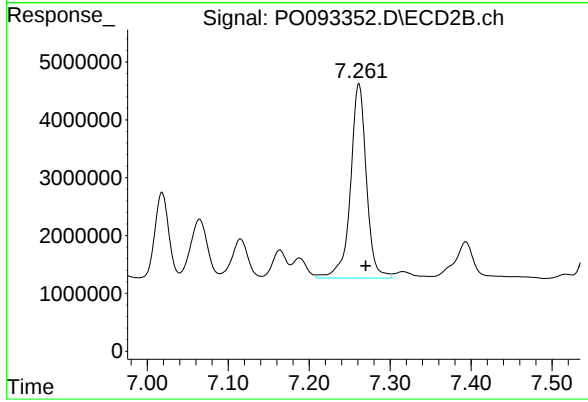

#35 AR-1260-5

R.T.: 7.261 min
Delta R.T.: -0.009 min
Response: 46017969
Conc: 390.87 ng/ml