

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032123\
 Data File : P0093406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 03:49
 Operator : YP/AJ
 Sample : 02014-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1711

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/22/2023
 Supervised By :Ankita Jodhani 03/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 05:38:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.424	3.631	32986273	14863834	10.534m	13.179 #
2) SA Decachlor...	10.250	8.656	14134069	5829232	6.531	5.953m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032123\
Data File : PO093406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 03:49
Operator : YP/AJ
Sample : 02014-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1711


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2023
Supervised By :Ankita Jodhani 03/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 05:38:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

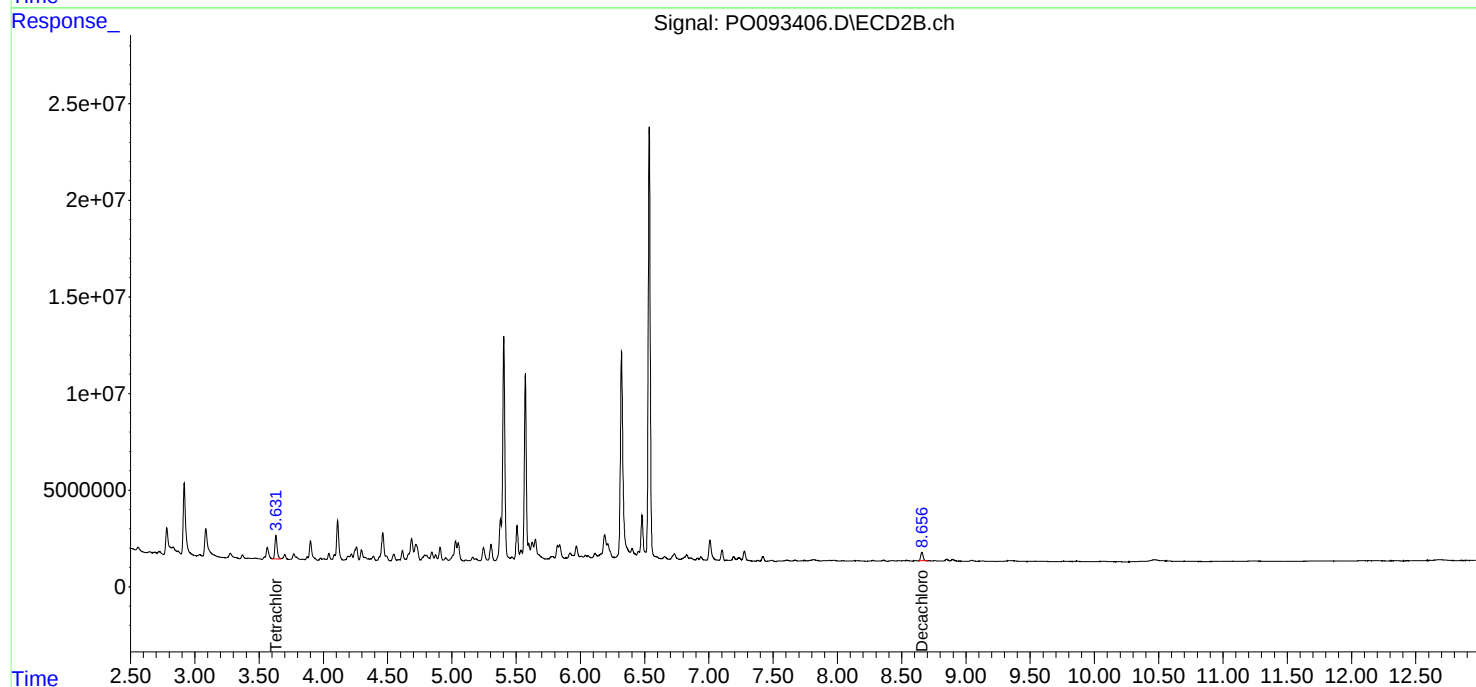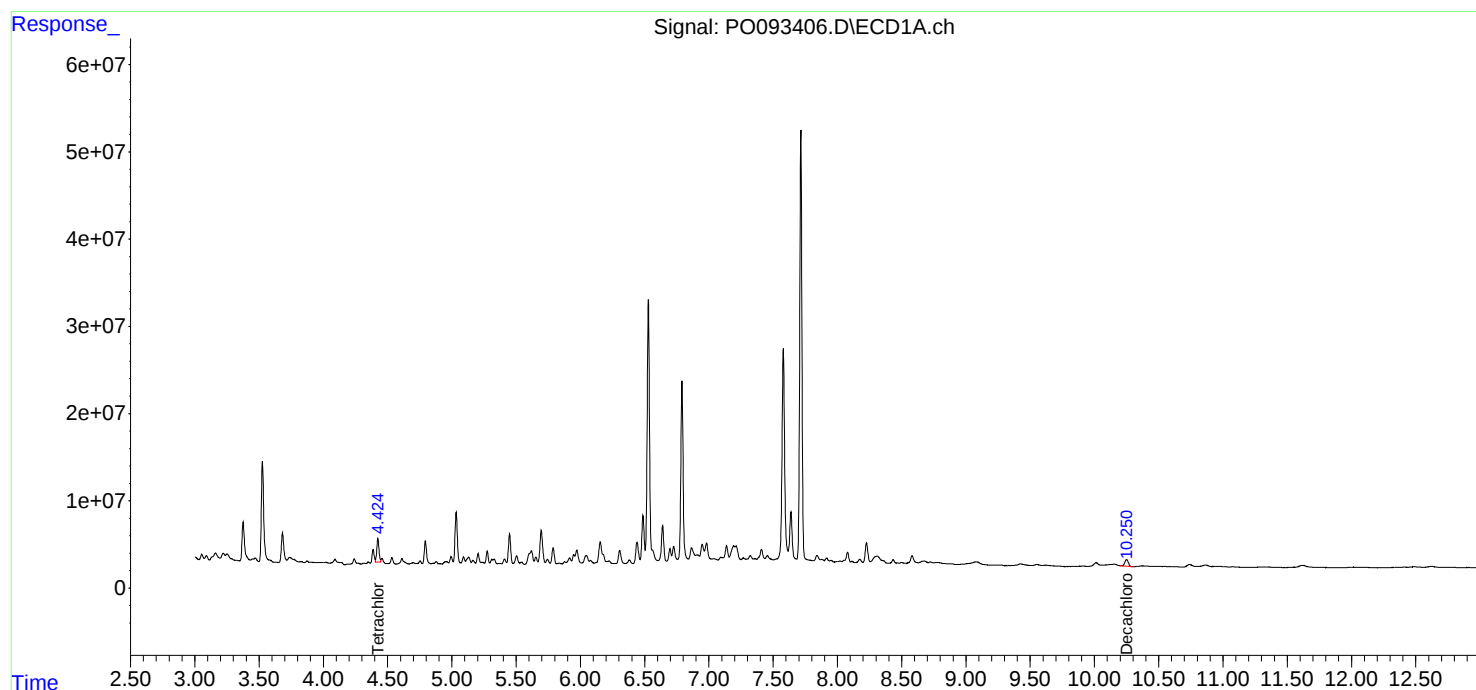

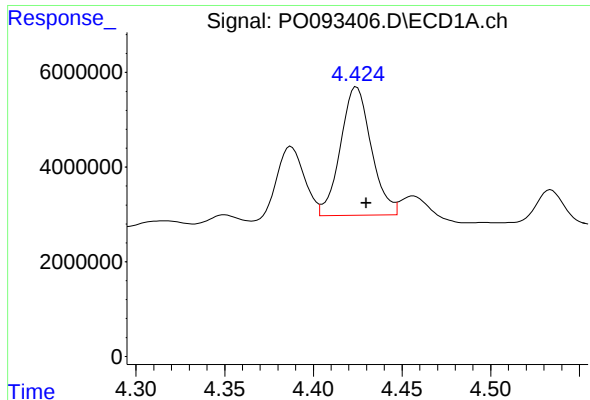


#1 Tetrachloro-m-xylene

R.T.: 4.424 min
Delta R.T.: -0.006 min
Response: 32986273
Conc: 10.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
1711


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2023
Supervised By :Ankita Jodhani 03/22/2023

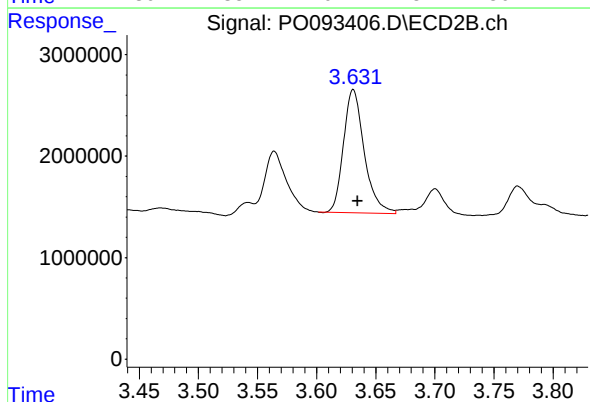


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 14863834
Conc: 13.18 ng/ml

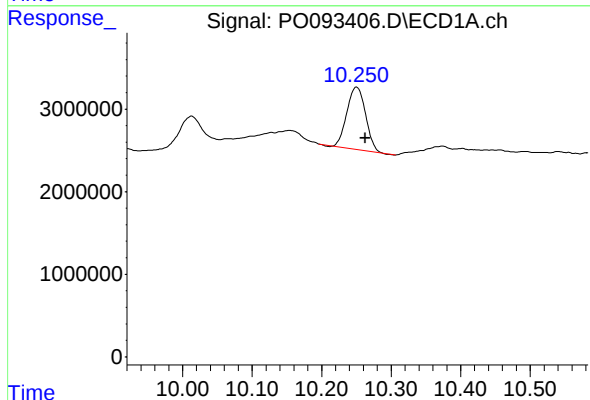

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: -0.013 min
Response: 14134069
Conc: 6.53 ng/ml

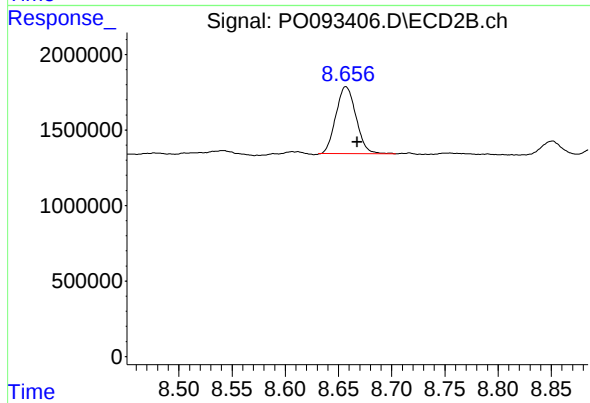

#2 Decachlorobiphenyl

R.T.: 8.656 min
Delta R.T.: -0.012 min
Response: 5829232
Conc: 5.95 ng/ml m