

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032124\
 Data File : P0102669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2024 11:43
 Operator : YP/AJ
 Sample : P1798-15DL 200X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-15DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/22/2024
 Supervised By :Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:35:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
16)	L4	AR-1242-1	5.405	4.428	87401687 49189463	970.116m 842.774m
17)	L4	AR-1242-2	5.427	4.446	104.0E6 70256795	787.764m 861.635m
18)	L4	AR-1242-3	5.488	4.617	65923708 31756200	777.494m 704.929
19)	L4	AR-1242-4	5.585	4.699	48767514 23089539	726.932m 445.482 #
20)	L4	AR-1242-5	6.310	5.210	15330511 14574417	244.853 260.291

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032124\
Data File : P0102669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2024 11:43
Operator : YP/AJ
Sample : P1798-15DL 200X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-15DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:35:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

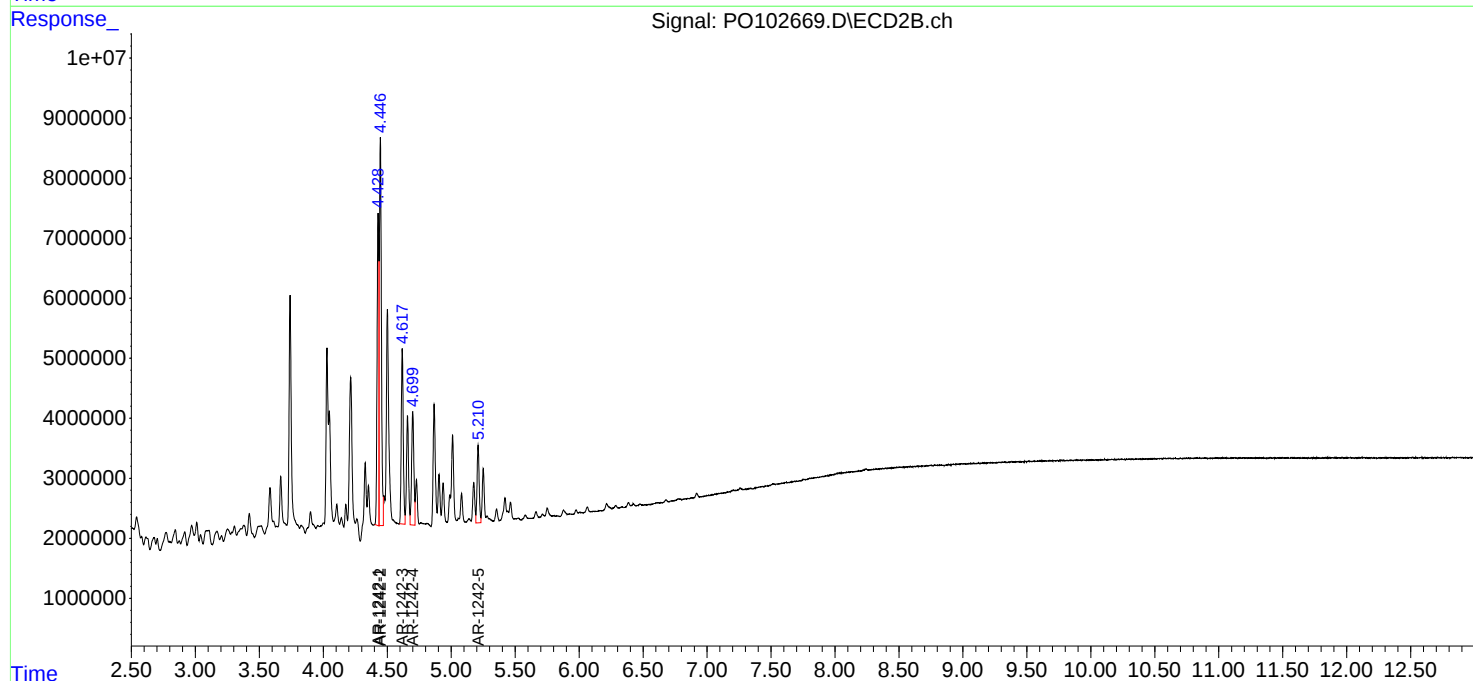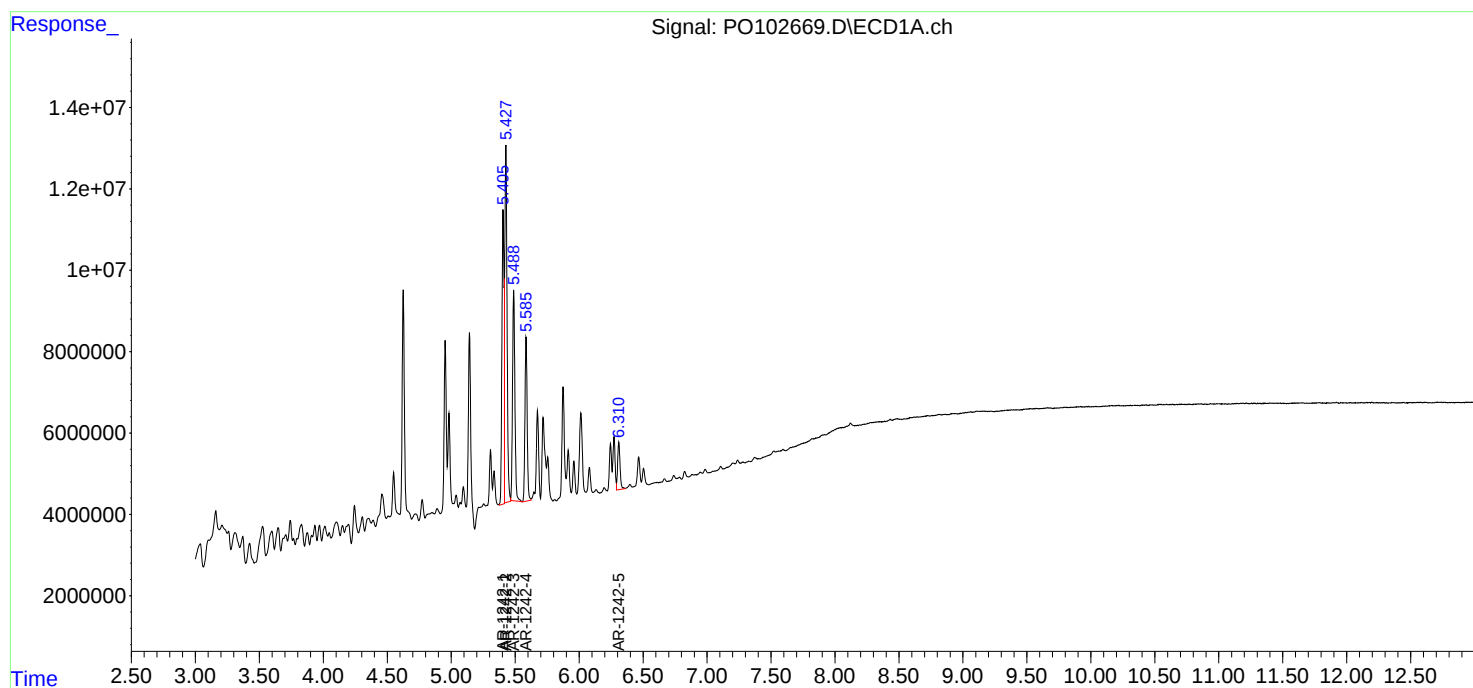

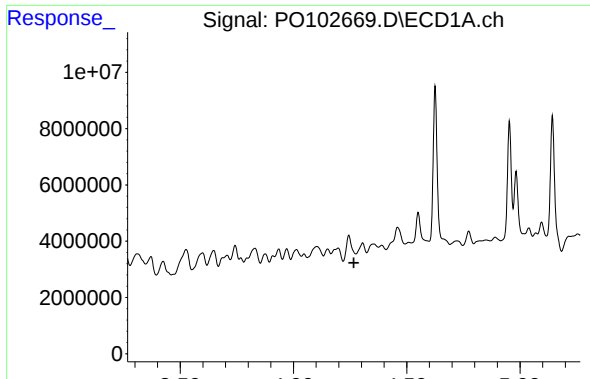


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
S-15DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

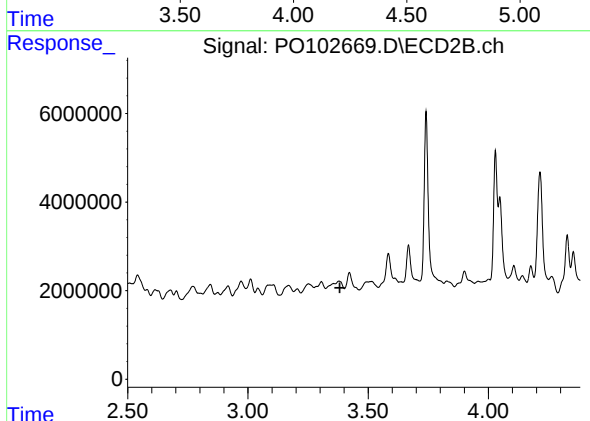


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.382 min
Response: 0
Conc: N.D.

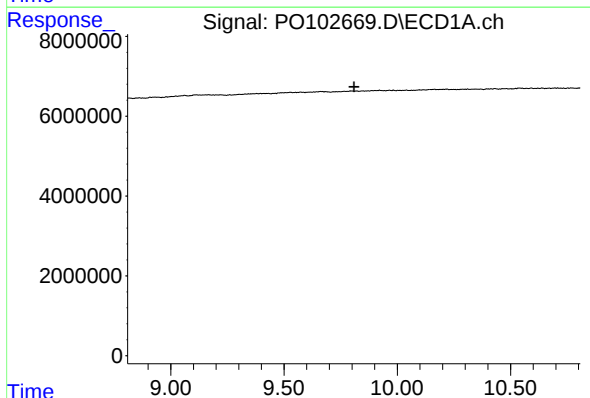


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.809 min
Response: 0
Conc: N.D.

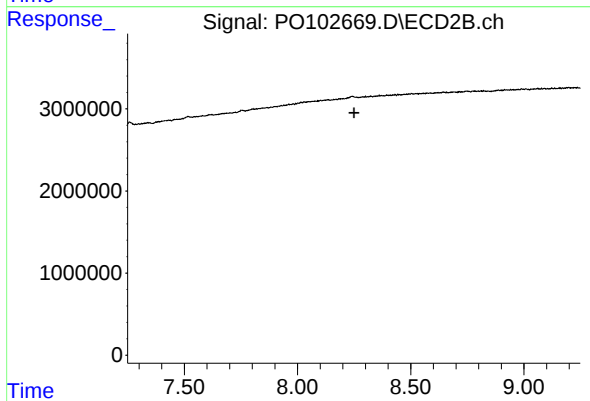

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.249 min
Response: 0
Conc: N.D.

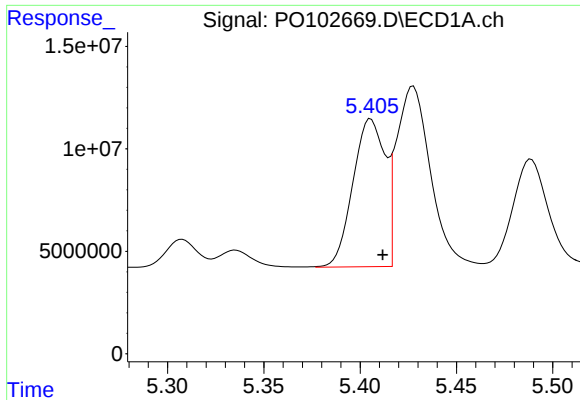


#16 AR-1242-1

R.T.: 5.405 min
Delta R.T.: -0.007 min
Response: 87401687
Conc: 970.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-15DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

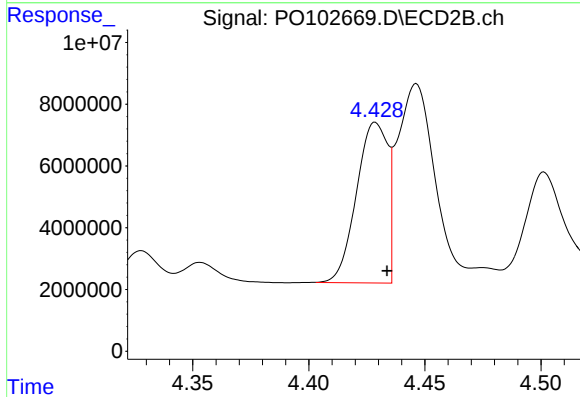


#16 AR-1242-1

R.T.: 4.428 min
Delta R.T.: -0.006 min
Response: 49189463
Conc: 842.77 ng/ml m

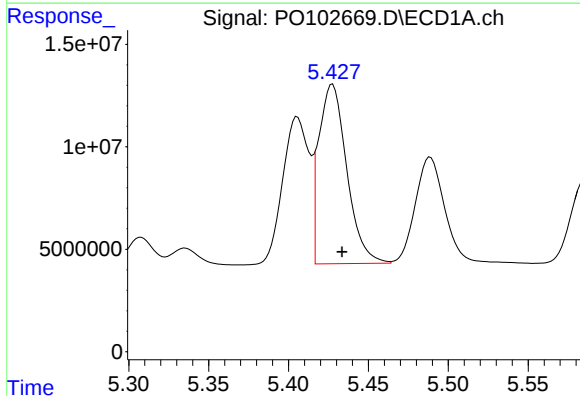


#17 AR-1242-2

R.T.: 5.427 min
Delta R.T.: -0.007 min
Response: 103978835
Conc: 787.76 ng/ml m

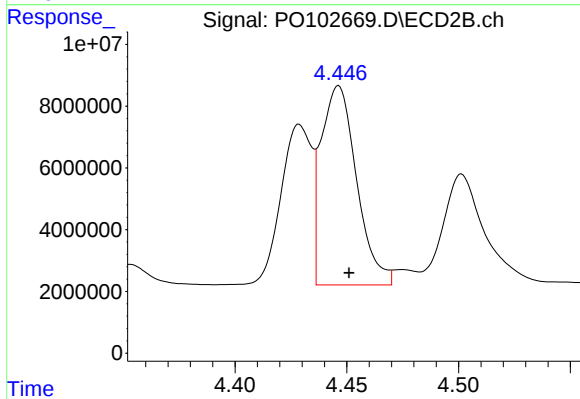

#17 AR-1242-2

R.T.: 4.446 min
Delta R.T.: -0.005 min
Response: 70256795
Conc: 861.64 ng/ml m

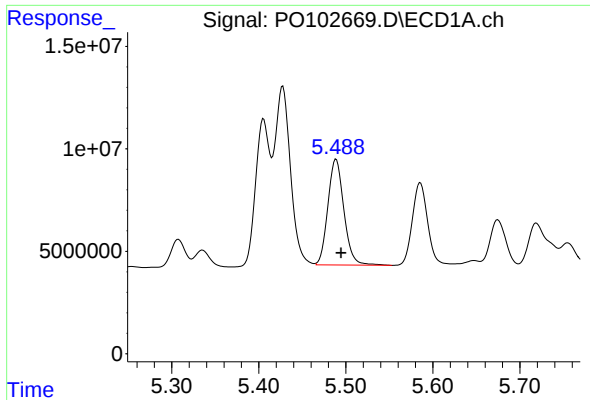


#18 AR-1242-3

R.T.: 5.488 min
Delta R.T.: -0.007 min
Response: 65923708
Conc: 777.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-15DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

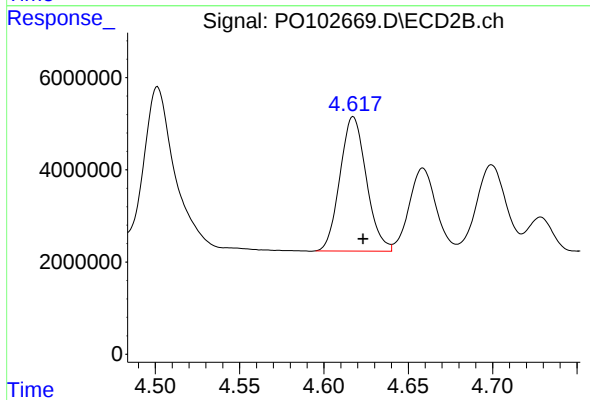


#18 AR-1242-3

R.T.: 4.617 min
Delta R.T.: -0.006 min
Response: 31756200
Conc: 704.93 ng/ml

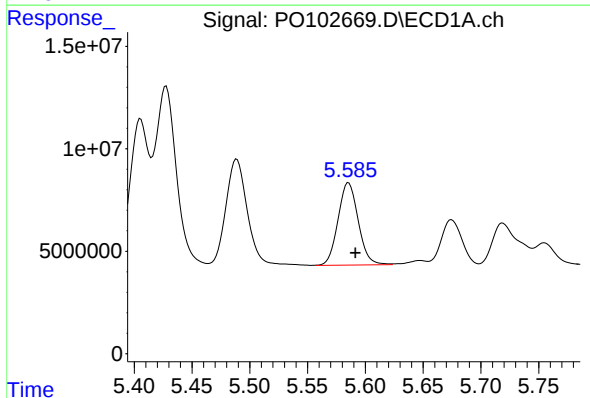


#19 AR-1242-4

R.T.: 5.585 min
Delta R.T.: -0.007 min
Response: 48767514
Conc: 726.93 ng/ml m

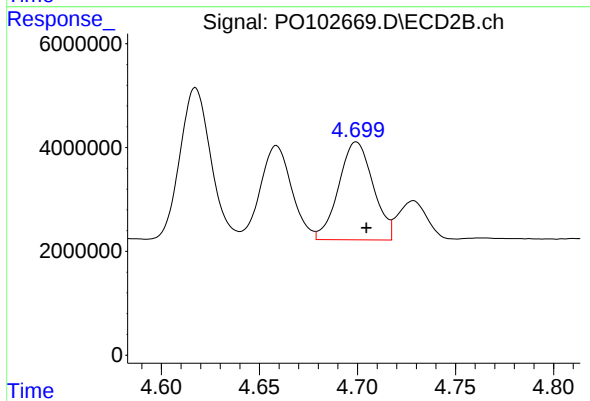

#19 AR-1242-4

R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 23089539
Conc: 445.48 ng/ml

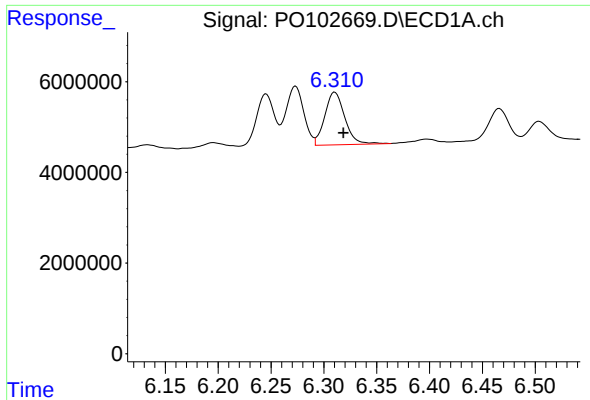


#20 AR-1242-5

R.T.: 6.310 min
Delta R.T.: -0.008 min
Response: 15330511
Conc: 244.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-15DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

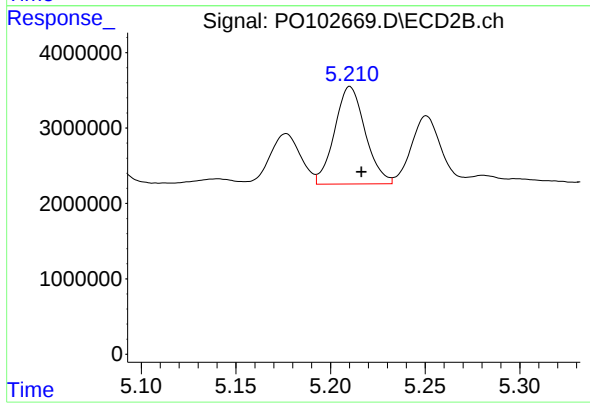

#20 AR-1242-5

R.T.: 5.210 min
Delta R.T.: -0.006 min
Response: 14574417
Conc: 260.29 ng/ml