

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076418.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 14:04
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 18:10:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.916	3.929	1217331	844346	21.428	20.238
2)	SA Decachlor...	10.911	9.191	891125	853715	23.168	22.234
Target Compounds							
9)	L2 AR-1221-2	5.268	0.000	21875	0	53.408	N.D. #
10)	L2 AR-1221-3	5.355	4.373	36777	23228	27.398	22.033
11)	L3 AR-1232-1	5.355	4.373	36777	23228	34.090	27.177



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
Data File : P0076418.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 14:04
Operator : DD\AJ
Sample : M1458-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 18:10:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

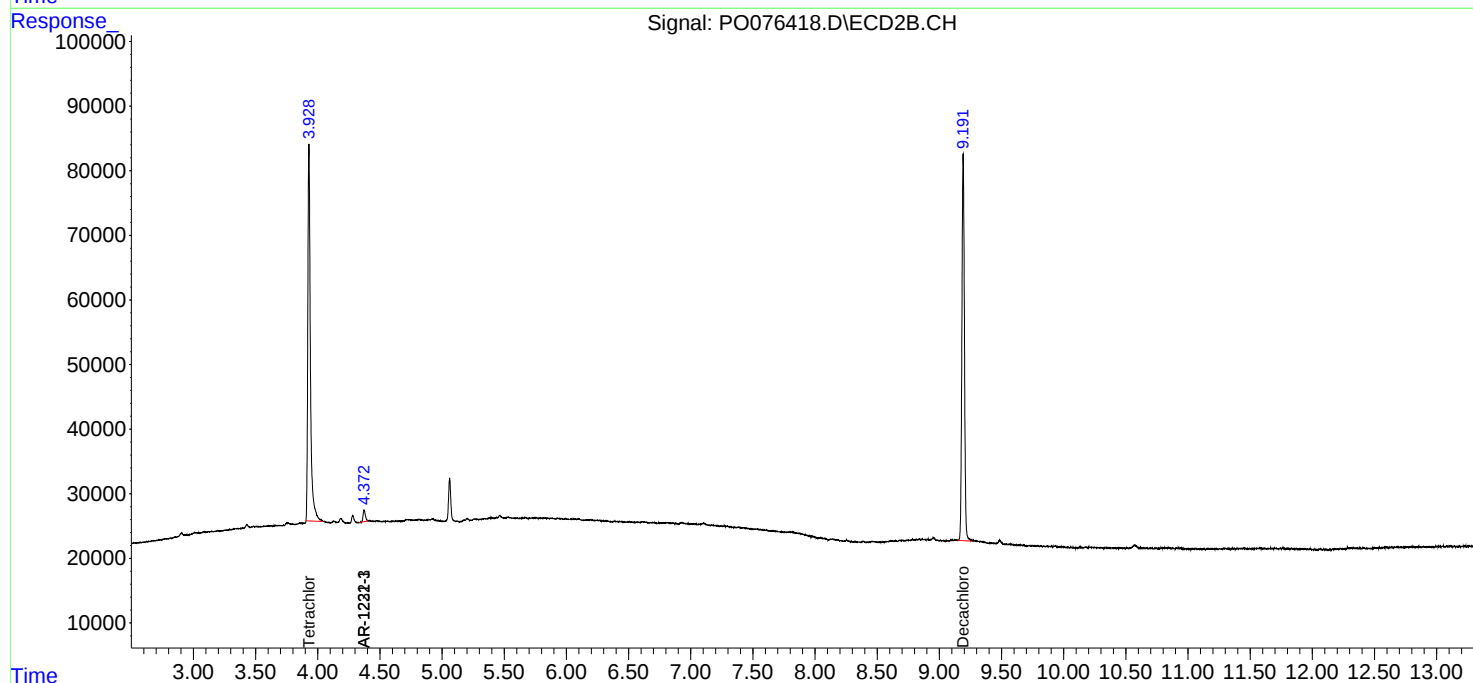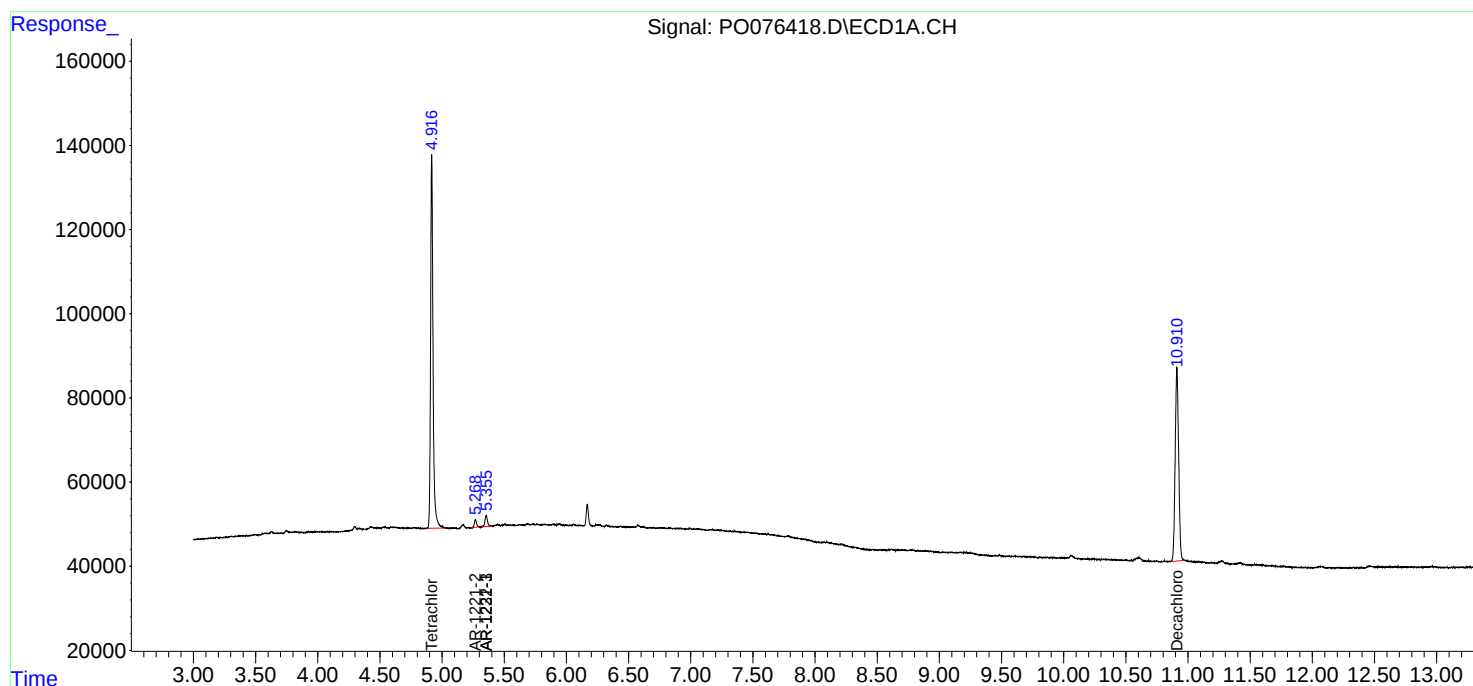


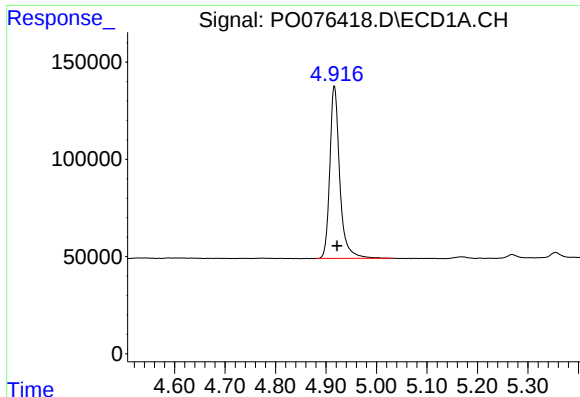

#1 Tetrachloro-m-xylene


R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 1217331
Conc: 21.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

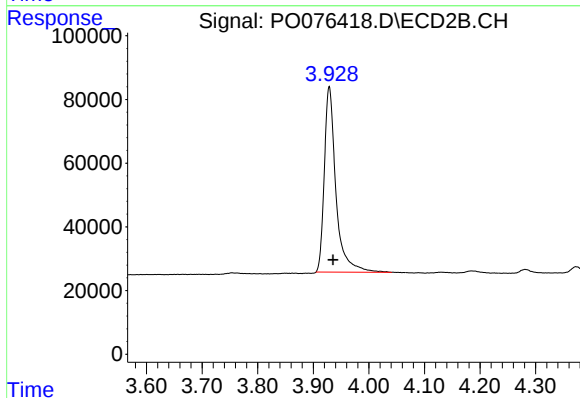


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.007 min
Response: 844346
Conc: 20.24 ng/ml

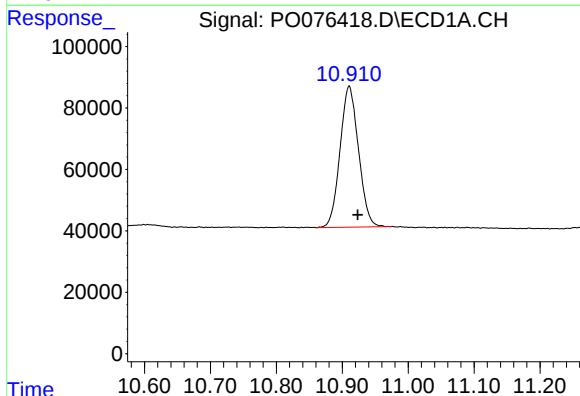


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.013 min
Response: 891125
Conc: 23.17 ng/ml

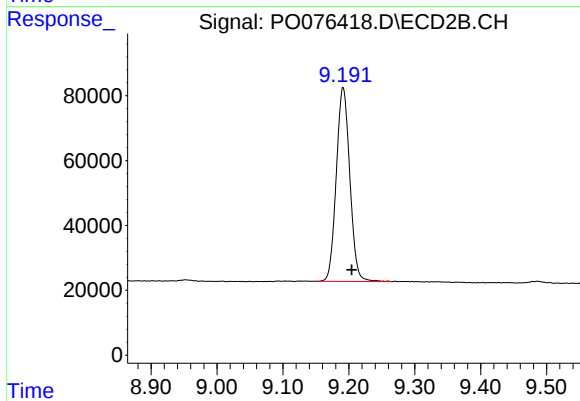

#2 Decachlorobiphenyl


R.T.: 9.191 min
Delta R.T.: -0.013 min
Response: 853715
Conc: 22.23 ng/ml

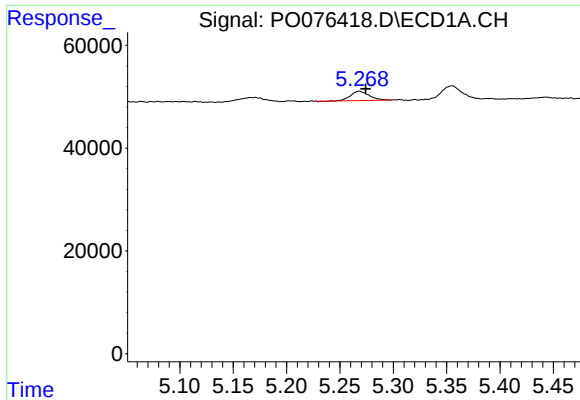

#9 AR-1221-2


R.T.: 5.268 min
Delta R.T.: -0.006 min
Response: 21875
Conc: 53.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

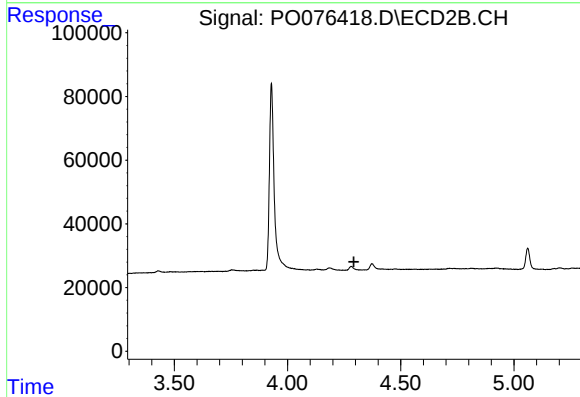


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.293 min
Response: 0
Conc: N.D.

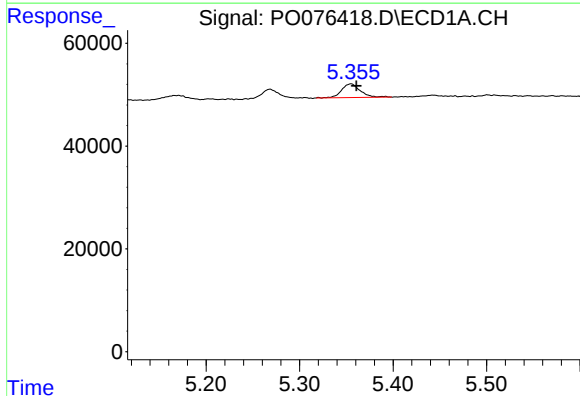


#10 AR-1221-3

R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 36777
Conc: 27.40 ng/ml

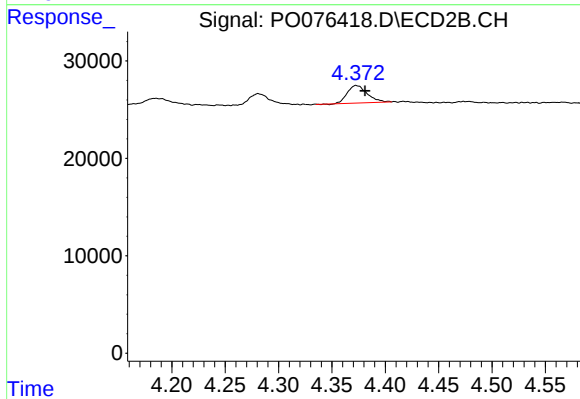

#10 AR-1221-3


R.T.: 4.373 min
Delta R.T.: -0.008 min
Response: 23228
Conc: 22.03 ng/ml

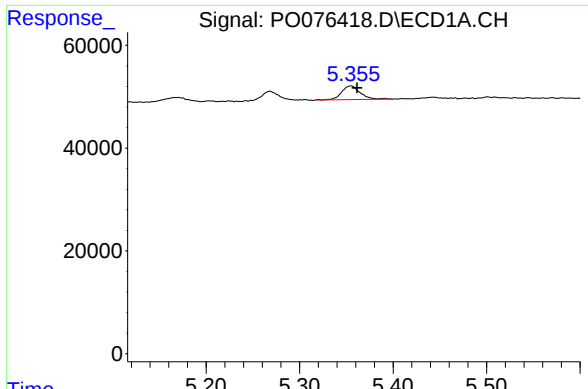

#11 AR-1232-1

R.T.: 5.355 min
Delta R.T.: -0.007 min
Response: 36777
Conc: 34.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

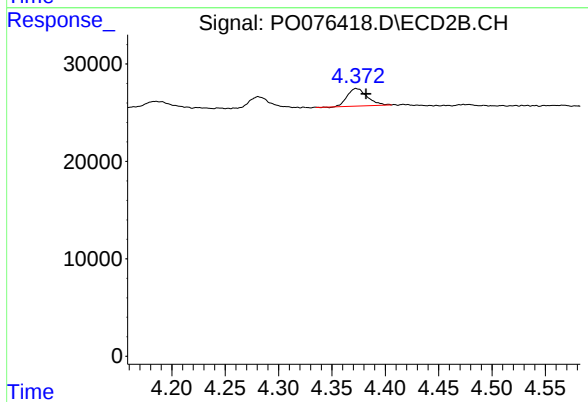

#11 AR-1232-1

R.T.: 4.373 min
Delta R.T.: -0.009 min
Response: 23228
Conc: 27.18 ng/ml