

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 14:21
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 18:11:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.917	3.929	1229548	853751	21.643	20.463
2)	SA Decachlor...	10.912	9.192	894939	860402	23.267	22.408
Target Compounds							
10)	L2 AR-1221-3	5.355	0.000	29326	0	21.847	N.D. #
11)	L3 AR-1232-1	5.355	0.000	29326	0	27.183	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
Data File : P0076419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 14:21
Operator : DD\AJ
Sample : M1458-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 18:11:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

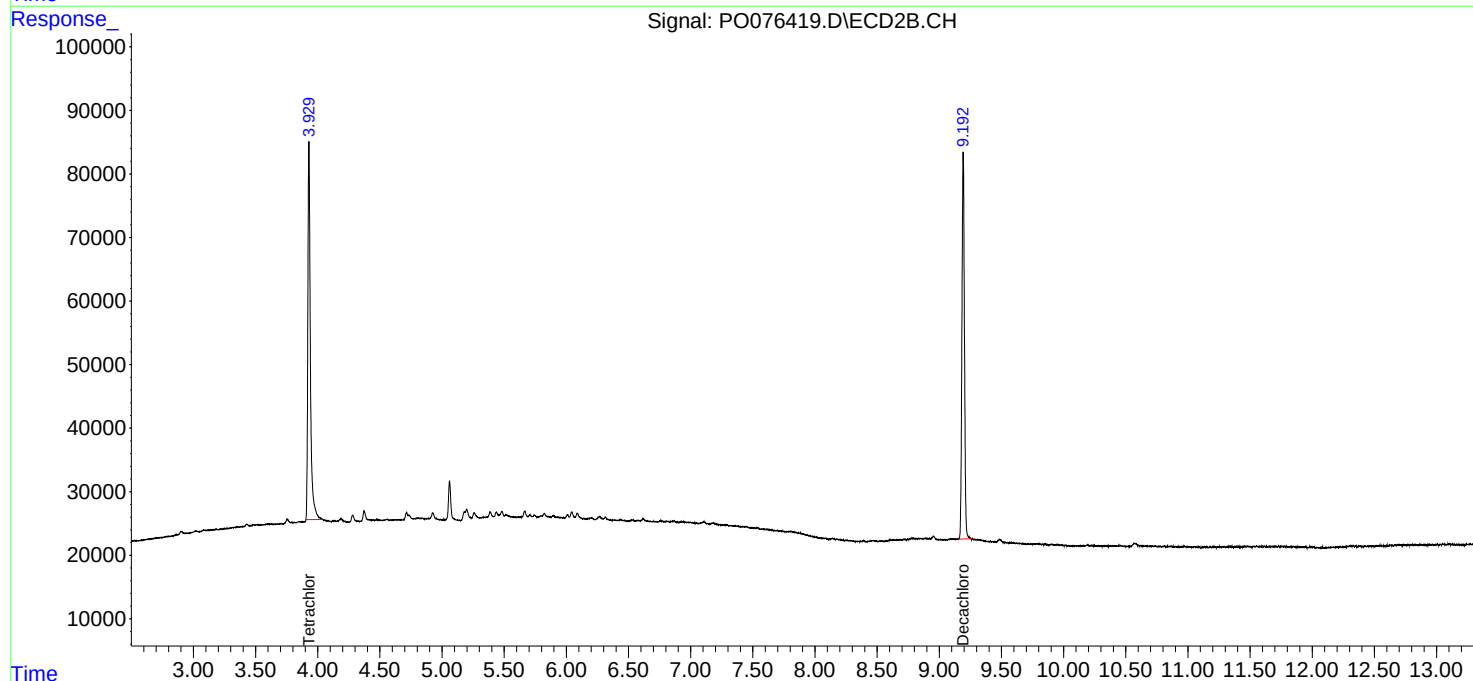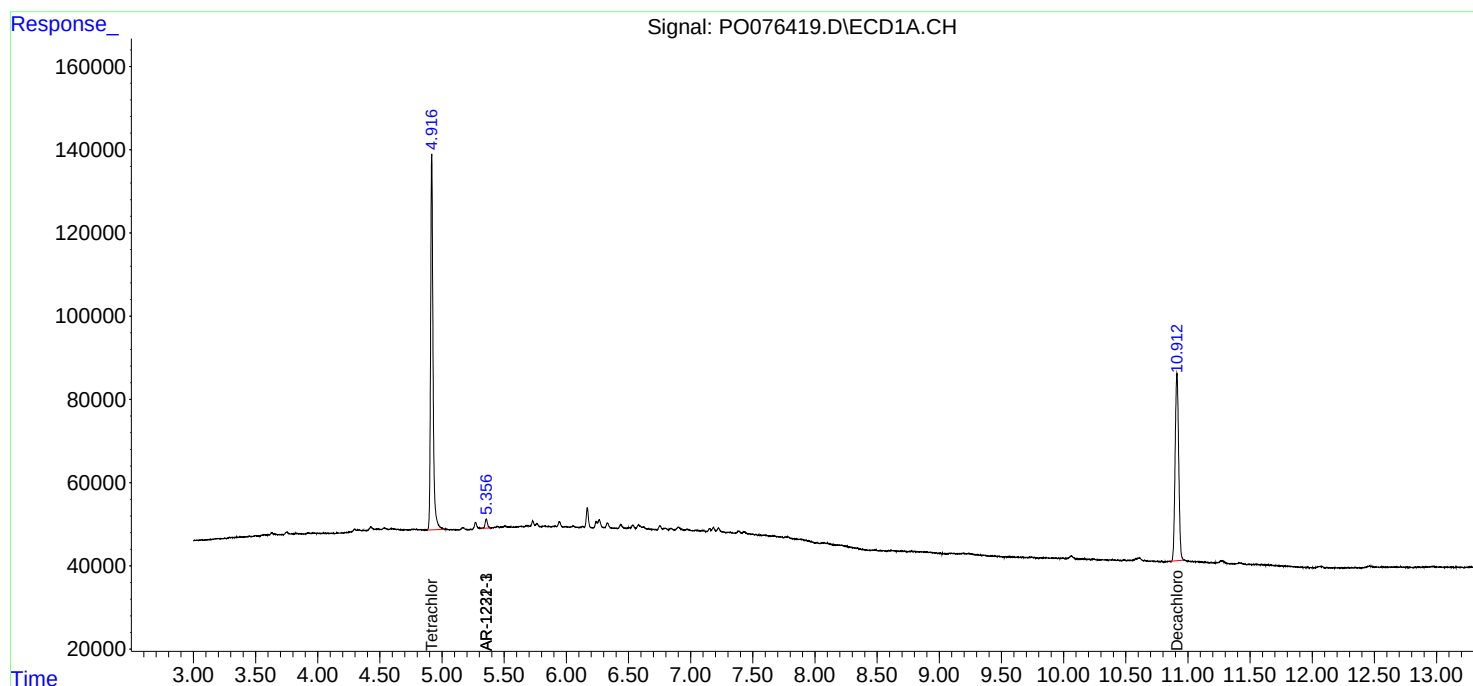


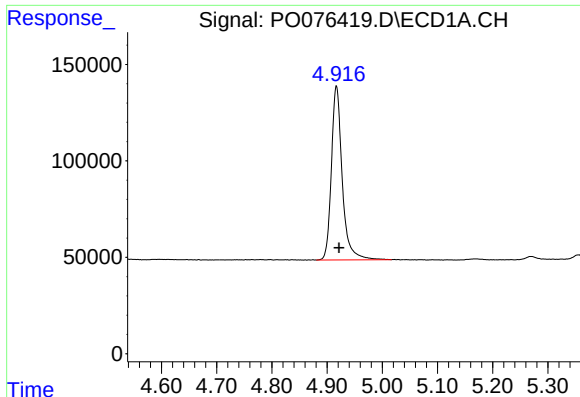

#1 Tetrachloro-m-xylene


R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 1229548
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

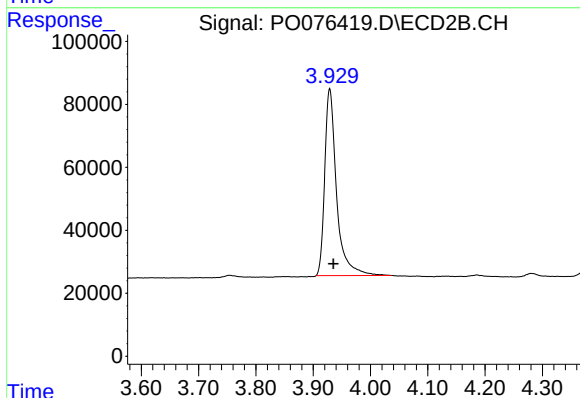


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.006 min
Response: 853751
Conc: 20.46 ng/ml

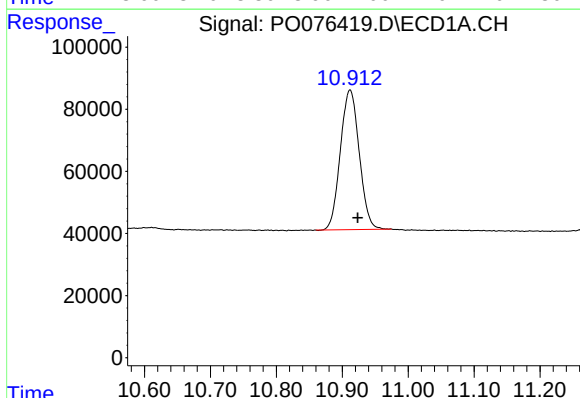


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.012 min
Response: 894939
Conc: 23.27 ng/ml

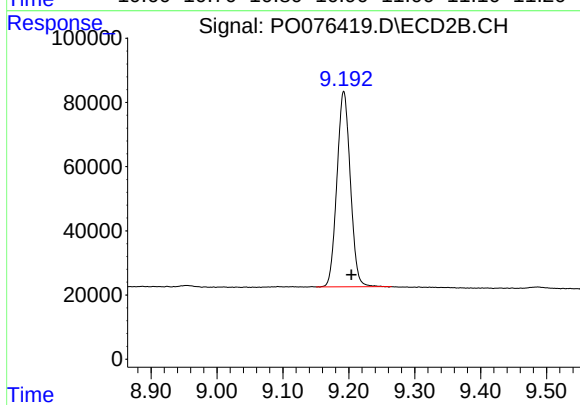

#2 Decachlorobiphenyl


R.T.: 9.192 min
Delta R.T.: -0.012 min
Response: 860402
Conc: 22.41 ng/ml

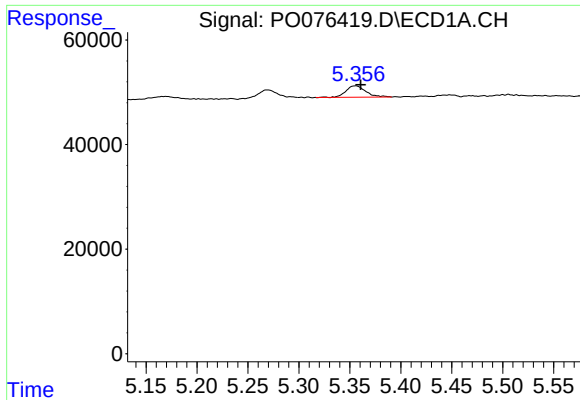

#10 AR-1221-3


R.T.: 5.355 min
Delta R.T.: -0.005 min
Response: 29326
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

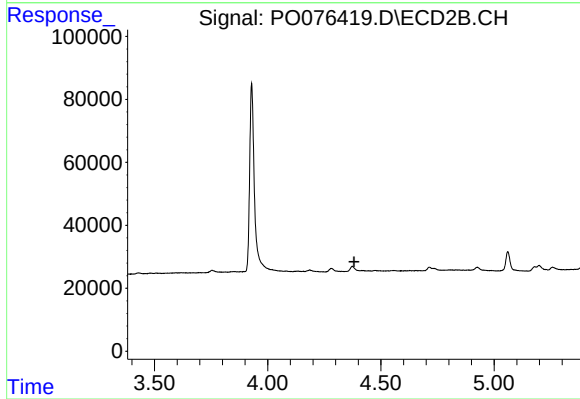


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.381 min
Response: 0
Conc: N.D.

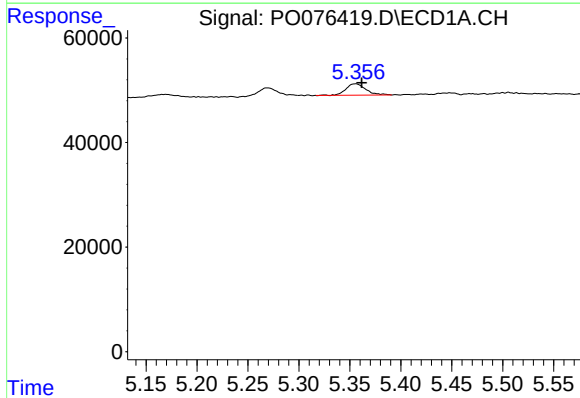

#11 AR-1232-1

R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 29326
Conc: 27.18 ng/ml

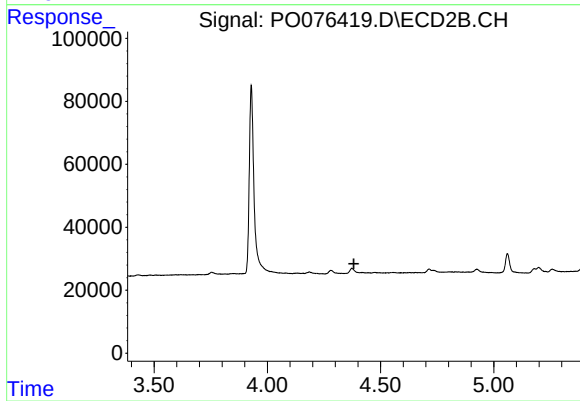

#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.382 min
Response: 0
Conc: N.D.