

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 15:46
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 18:13:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.915	3.928	1295239	871579	22.800	20.890
2)	SA Decachlor...	10.909	9.189	976879	933144	25.397	24.302
Target Compounds							
33)	L7 AR-1260-3	8.559	0.000	26611	0	13.423	N.D. #
34)	L7 AR-1260-4	8.807	7.584	38995	42209	17.261	21.904 #
36)	L8 AR-1262-1	8.559	0.000	26611	0	8.994	N.D. #
38)	L8 AR-1262-3	9.422	8.119	151044	158959	45.704	73.990 #
39)	L8 AR-1262-4	9.518	8.184	150584	142099	58.578	37.570 #
40)	L8 AR-1262-5	10.173	8.679	45560	47824	27.697	27.626
41)	L9 AR-1268-1	9.422	8.119	151044	158959	25.930	27.066
42)	L9 AR-1268-2	9.518	8.184	150584	142099	28.386	26.679
43)	L9 AR-1268-3	9.740	8.389	118755	128839	25.616	27.165
44)	L9 AR-1268-4	10.173	8.679	45560	47824	26.142	25.735
45)	L9 AR-1268-5	10.580	8.953	365197	370704	26.526	27.777



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032221\
Data File : P0076424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 15:46
Operator : DD\AJ
Sample : M1458-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 18:13:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

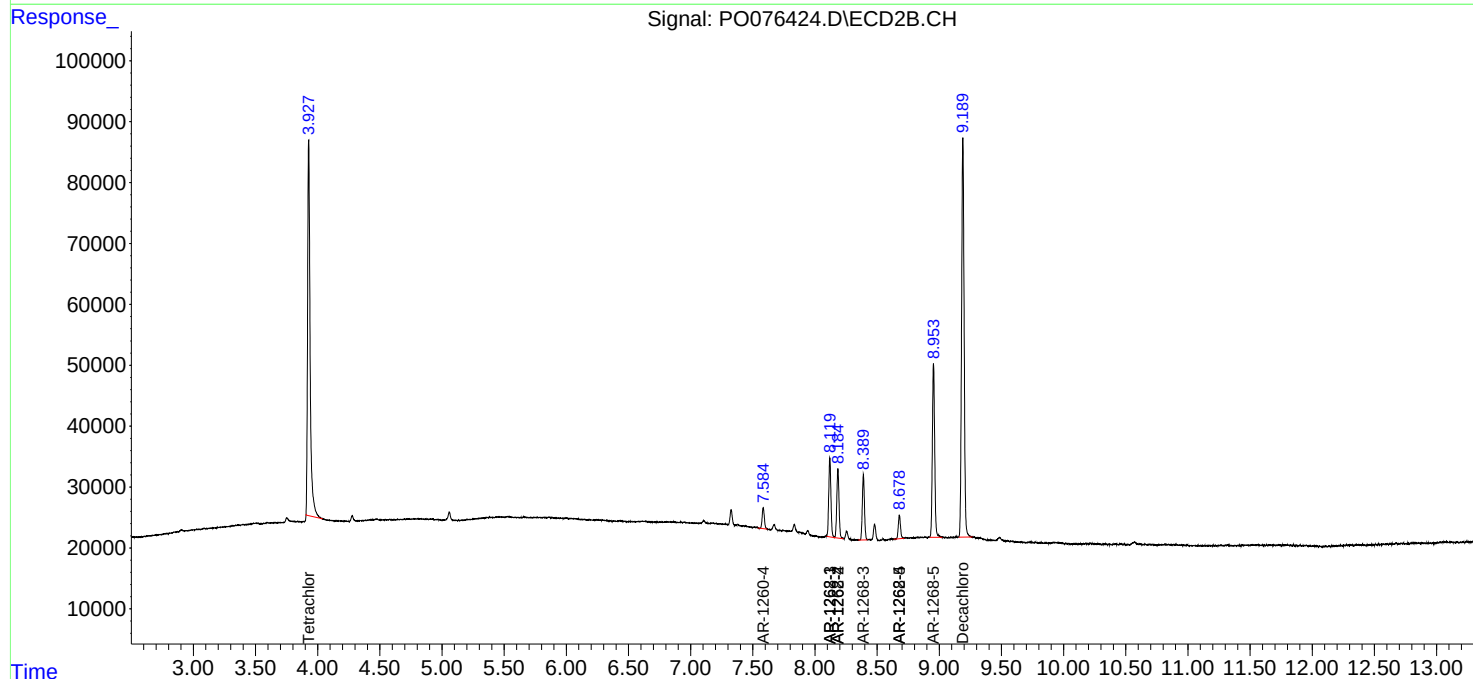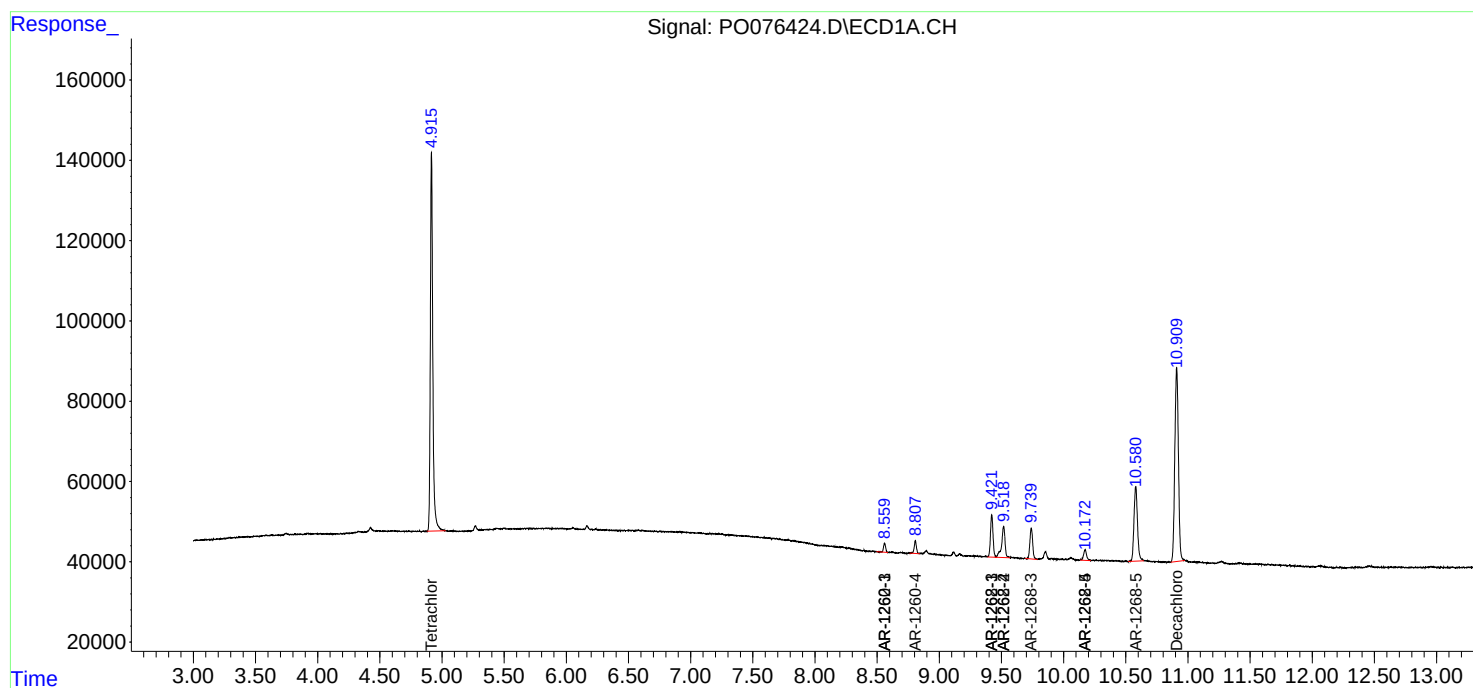


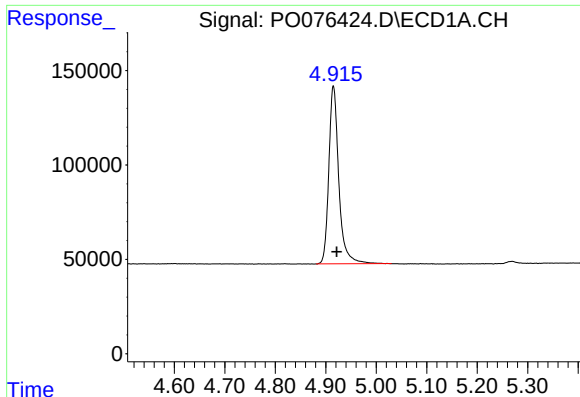

#1 Tetrachloro-m-xylene


R.T.: 4.915 min
Delta R.T.: -0.007 min
Response: 1295239
Conc: 22.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

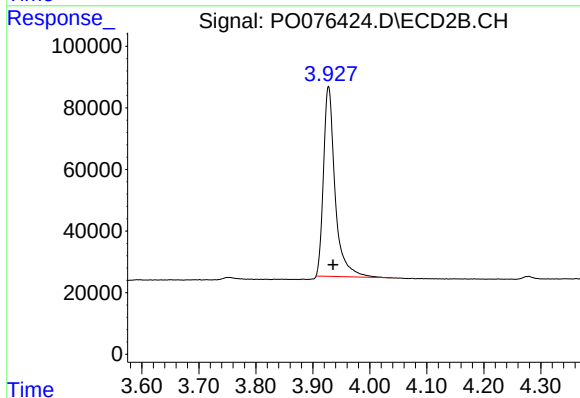


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.008 min
Response: 871579
Conc: 20.89 ng/ml

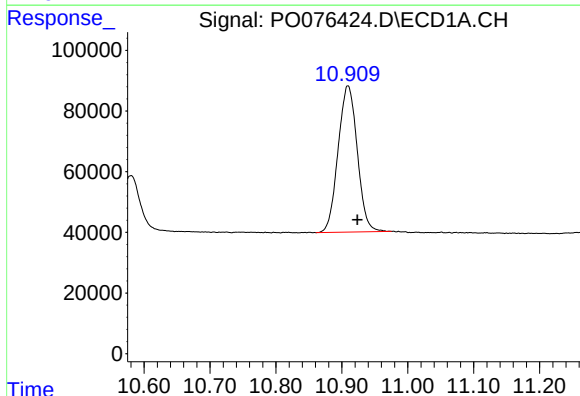


#2 Decachlorobiphenyl

R.T.: 10.909 min
Delta R.T.: -0.014 min
Response: 976879
Conc: 25.40 ng/ml

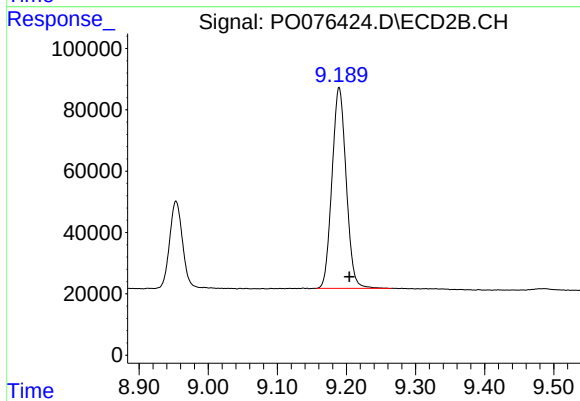

#2 Decachlorobiphenyl


R.T.: 9.189 min
Delta R.T.: -0.015 min
Response: 933144
Conc: 24.30 ng/ml

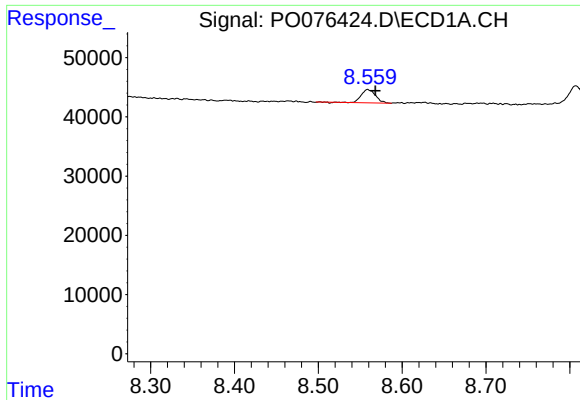

#33 AR-1260-3


R.T.: 8.559 min
Delta R.T.: -0.009 min
Response: 26611
Conc: 13.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

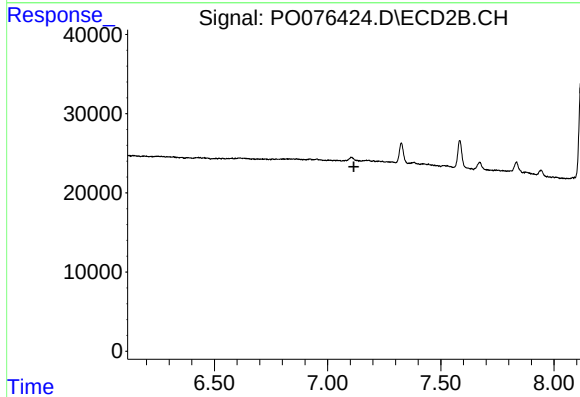


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.116 min
Response: 0
Conc: N.D.

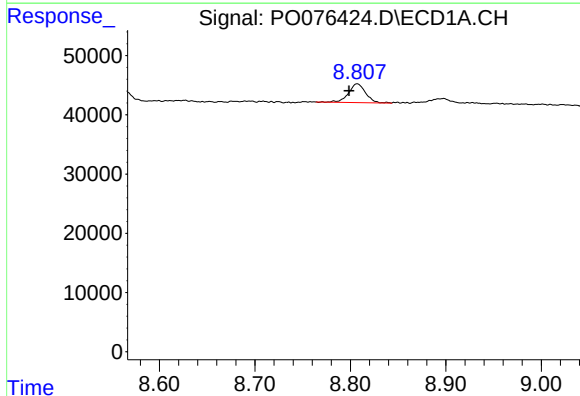


#34 AR-1260-4

R.T.: 8.807 min
Delta R.T.: 0.009 min
Response: 38995
Conc: 17.26 ng/ml

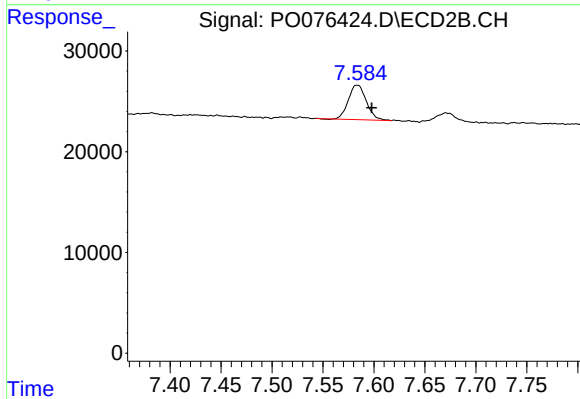

#34 AR-1260-4


R.T.: 7.584 min
Delta R.T.: -0.014 min
Response: 42209
Conc: 21.90 ng/ml

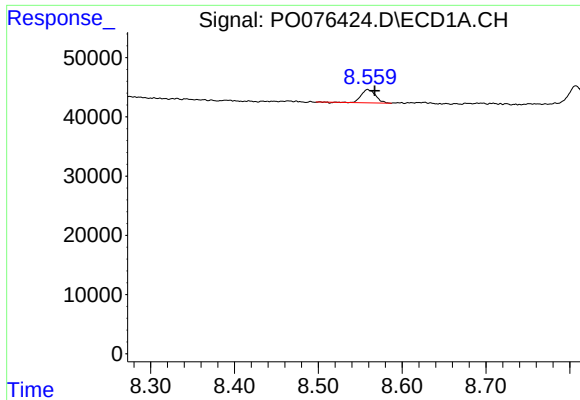

#36 AR-1262-1


R.T.: 8.559 min
Delta R.T.: -0.009 min
Response: 26611
Conc: 8.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

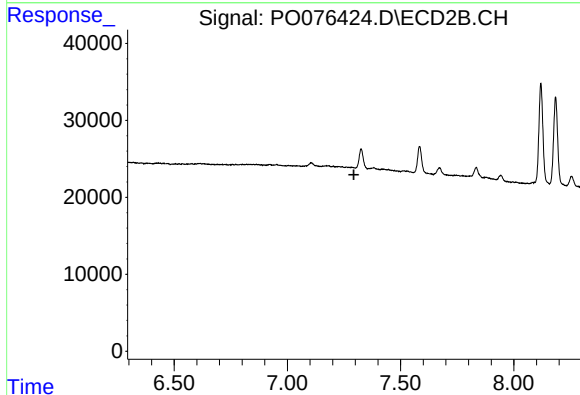


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.294 min
Response: 0
Conc: N.D.

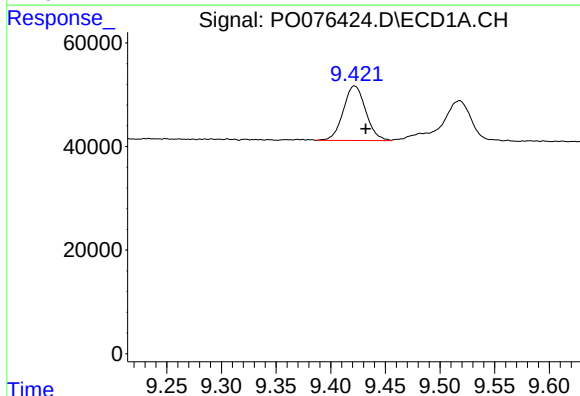


#38 AR-1262-3

R.T.: 9.422 min
Delta R.T.: -0.010 min
Response: 151044
Conc: 45.70 ng/ml

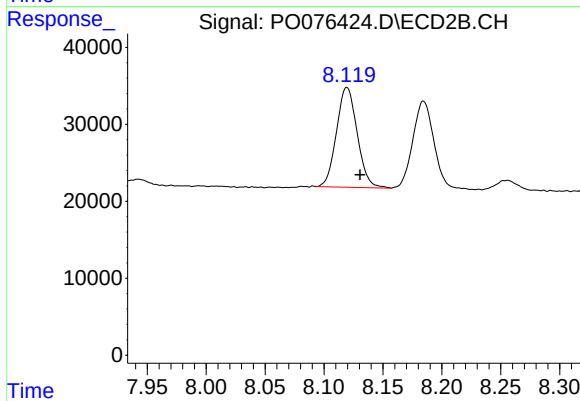

#38 AR-1262-3


R.T.: 8.119 min
Delta R.T.: -0.011 min
Response: 158959
Conc: 73.99 ng/ml

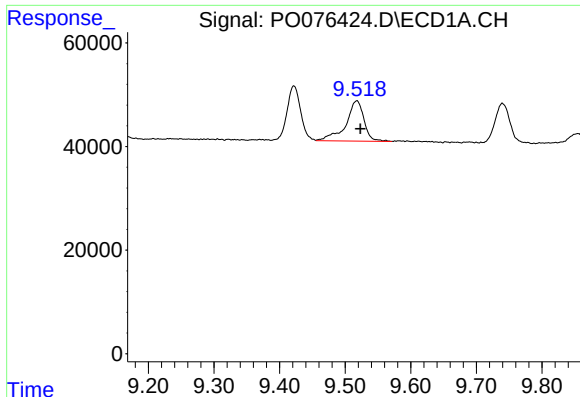

#39 AR-1262-4


R.T.: 9.518 min
Delta R.T.: -0.005 min
Response: 150584
Conc: 58.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

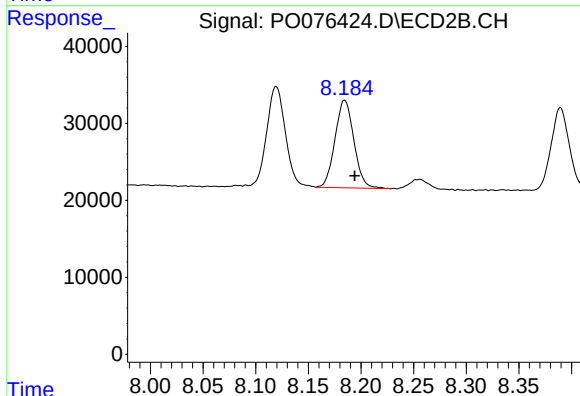


#39 AR-1262-4

R.T.: 8.184 min
Delta R.T.: -0.010 min
Response: 142099
Conc: 37.57 ng/ml

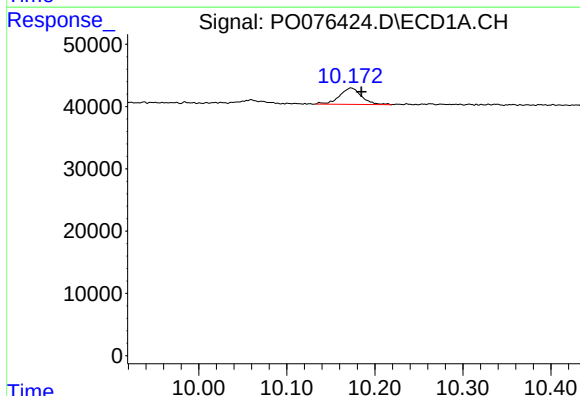


#40 AR-1262-5

R.T.: 10.173 min
Delta R.T.: -0.011 min
Response: 45560
Conc: 27.70 ng/ml

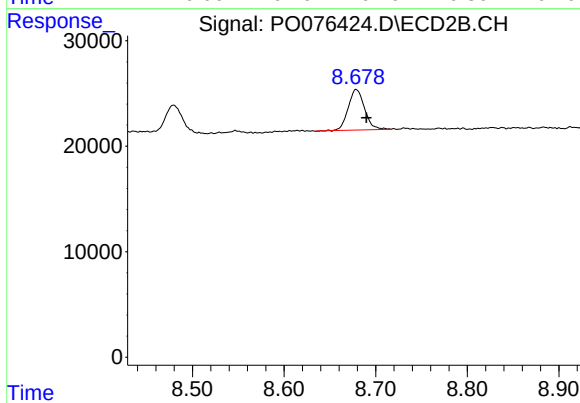

#40 AR-1262-5


R.T.: 8.679 min
Delta R.T.: -0.011 min
Response: 47824
Conc: 27.63 ng/ml

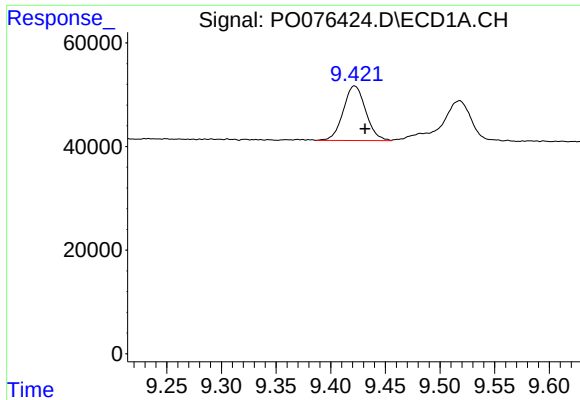

#41 AR-1268-1


R.T.: 9.422 min
Delta R.T.: -0.009 min
Response: 151044
Conc: 25.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

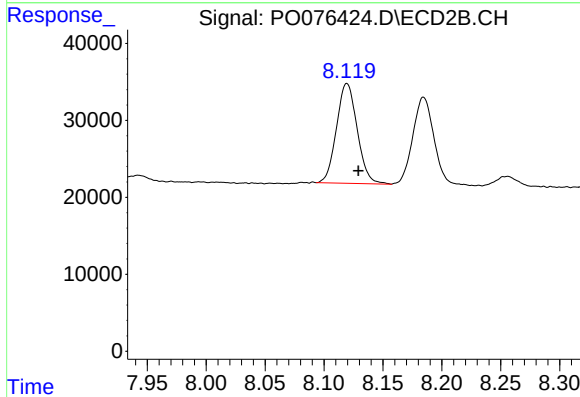


#41 AR-1268-1

R.T.: 8.119 min
Delta R.T.: -0.010 min
Response: 158959
Conc: 27.07 ng/ml

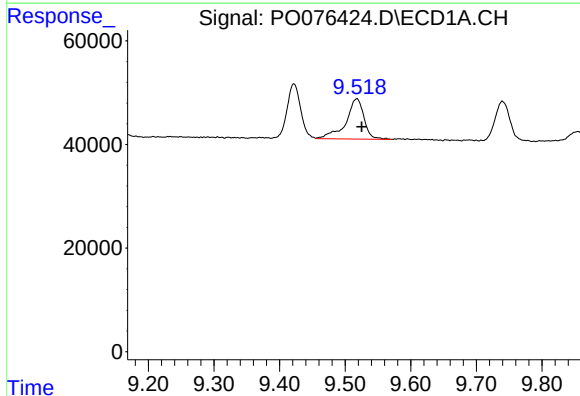


#42 AR-1268-2

R.T.: 9.518 min
Delta R.T.: -0.008 min
Response: 150584
Conc: 28.39 ng/ml

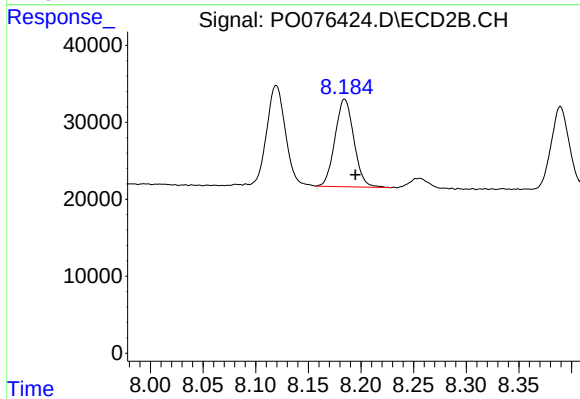

#42 AR-1268-2


R.T.: 8.184 min
Delta R.T.: -0.010 min
Response: 142099
Conc: 26.68 ng/ml

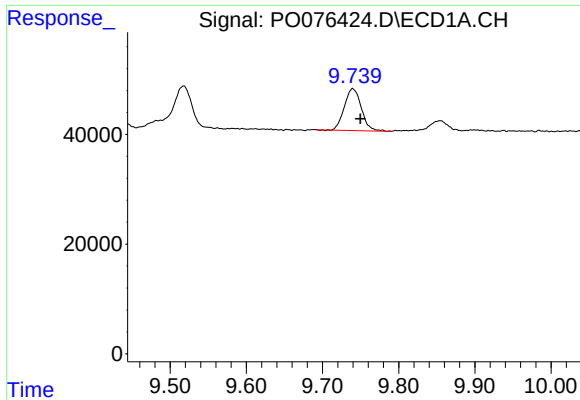

#43 AR-1268-3


R.T.: 9.740 min
Delta R.T.: -0.010 min
Response: 118755
Conc: 25.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

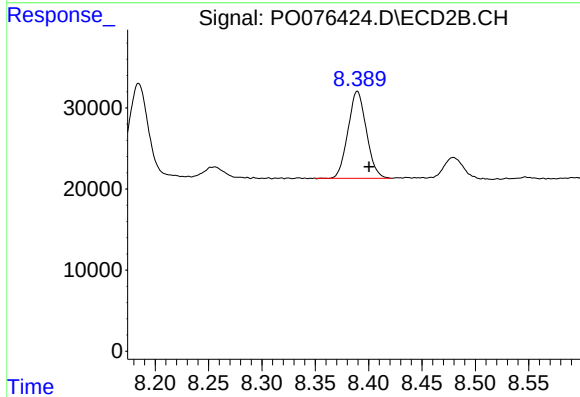


#43 AR-1268-3

R.T.: 8.389 min
Delta R.T.: -0.011 min
Response: 128839
Conc: 27.16 ng/ml

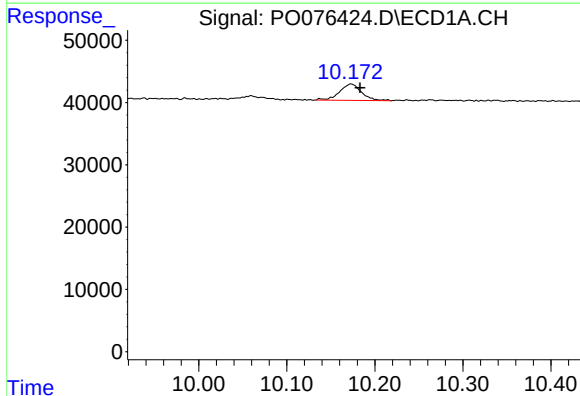


#44 AR-1268-4

R.T.: 10.173 min
Delta R.T.: -0.010 min
Response: 45560
Conc: 26.14 ng/ml

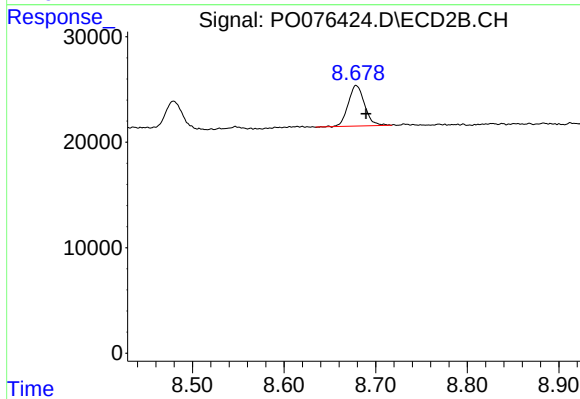

#44 AR-1268-4


R.T.: 8.679 min
Delta R.T.: -0.011 min
Response: 47824
Conc: 25.73 ng/ml

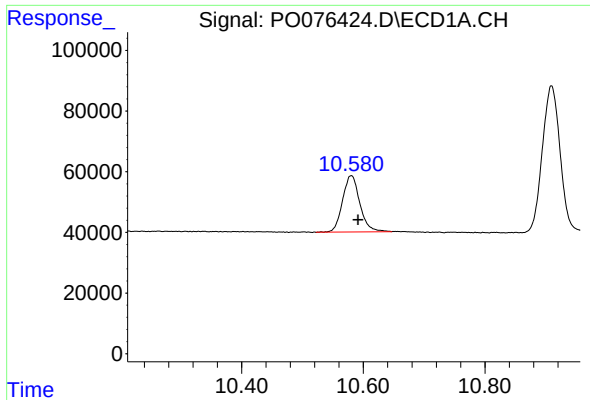

#45 AR-1268-5

R.T.: 10.580 min
Delta R.T.: -0.011 min
Response: 365197
Conc: 26.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2021

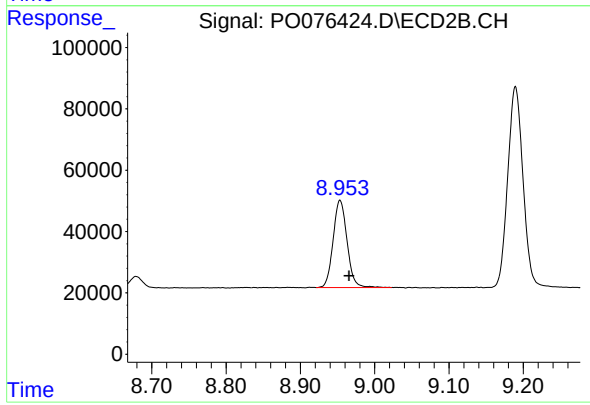

#45 AR-1268-5

R.T.: 8.953 min
Delta R.T.: -0.012 min
Response: 370704
Conc: 27.78 ng/ml