

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032221\
 Data File : PS014315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2021 19:45
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:35:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 22 09:06:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
2)	SA Decachlor...	10.583	0.000	649313	0	0.128	N.D.	#
Target Compounds								
6)	L1 AR-1016-4	6.031	0.000	24006464	0	178.273	N.D.	#
7)	L1 AR-1016-5	6.337	0.000	8857278	0	66.011	N.D.	#
14)	L3 AR-1232-4	6.031f	0.000	24006464	0	444.739	N.D.	#
15)	L3 AR-1232-5	6.148f	0.000	7542181	0	183.842	N.D.	#
19)	L4 AR-1242-4	6.031	0.000	24006464	0	236.597	N.D.	#
20)	L4 AR-1242-5	6.809f	0.000	6123119	0	57.207	N.D.	#
22)	L5 AR-1248-2	6.148f	0.000	7542181	0	48.912	N.D.	#
23)	L5 AR-1248-3	6.337	0.000	8857278	0	50.774	N.D.	#
25)	L5 AR-1248-5	6.809f	0.000	6123119	0	31.934	N.D.	#
27)	L6 AR-1254-2	0.000	6.048	0	533.4E6	N.D.	12396.807	#
28)	L6 AR-1254-3	7.281f	0.000	6492822	0	19.580	N.D.	#
29)	L6 AR-1254-4	7.613f	0.000	18067035	0	73.175	N.D.	#
30)	L6 AR-1254-5	7.993f	0.000	1045576	0	3.919	N.D.	#
33)	L7 AR-1260-3	0.000	6.920	0	66006041	N.D.	827.731	#
34)	L7 AR-1260-4	0.000	7.365f	0	173.7E6	N.D.	2073.629	#
38)	L8 AR-1262-3	9.020f	0.000	6680189	0	17.232	N.D.	#
39)	L8 AR-1262-4	0.000	7.973	0	407.6E6	N.D.	1610.512	#
41)	L9 AR-1268-1	9.020f	0.000	6680189	0	9.763	N.D.	#
42)	L9 AR-1268-2	9.118f	7.973	5562.4E6	407.6E6	8972.800	1004.872	#
43)	L9 AR-1268-3	9.306f	0.000	4133.6E6	0	7873.871	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032221\
Data File : PS014315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2021 19:45
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:35:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 22 09:06:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

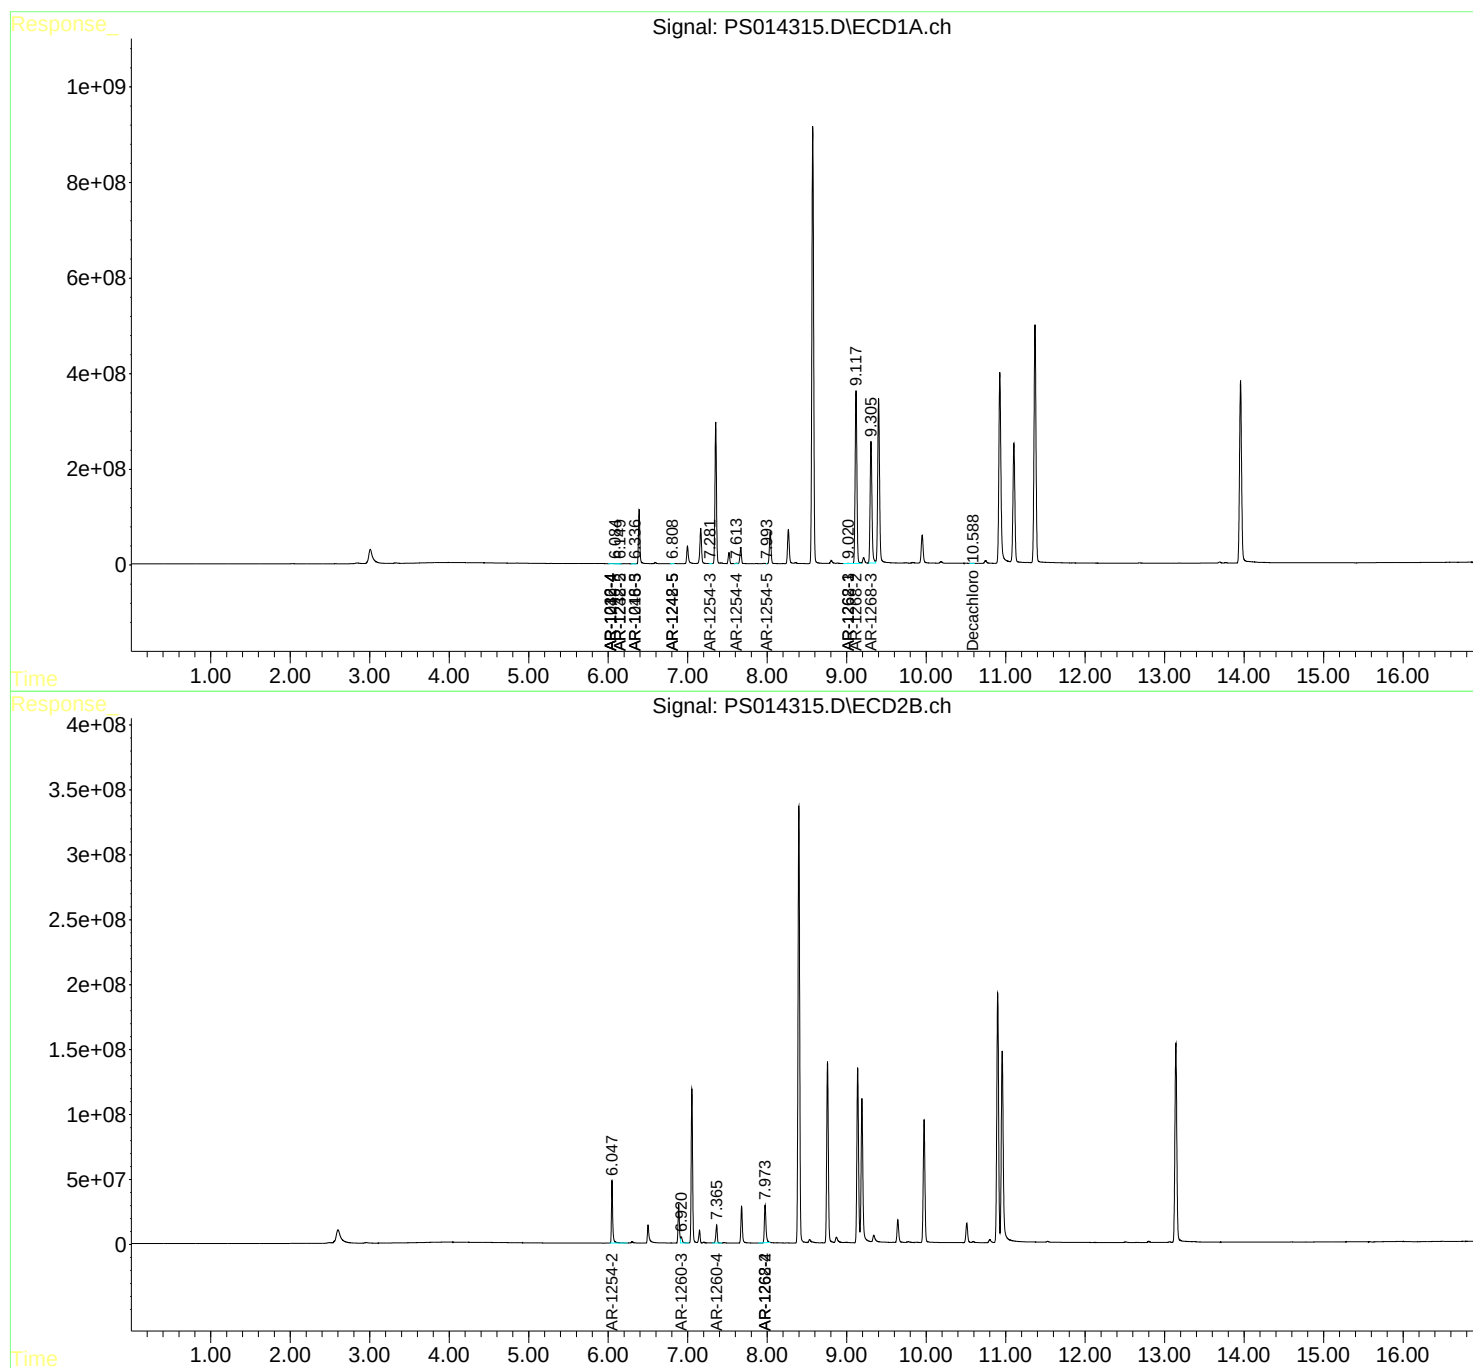


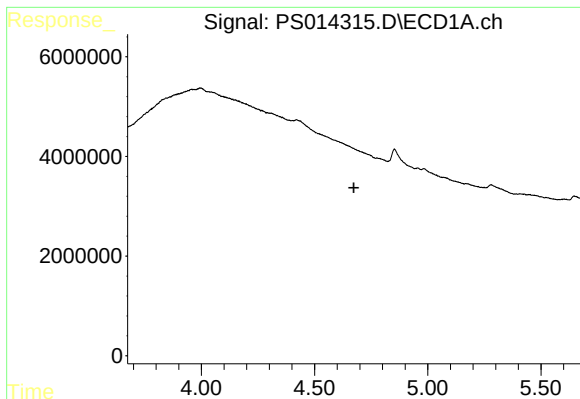

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

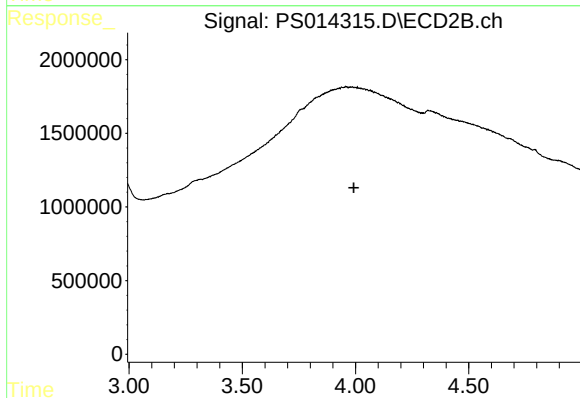


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.993 min
Response: 0
Conc: N.D.

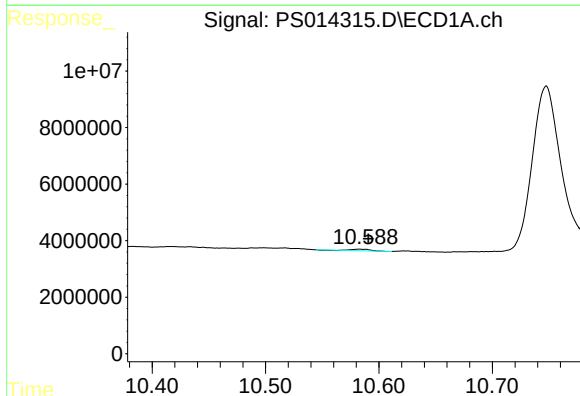


#2 Decachlorobiphenyl

R.T.: 10.583 min
Delta R.T.: -0.008 min
Response: 649313
Conc: 0.13 ng/ml

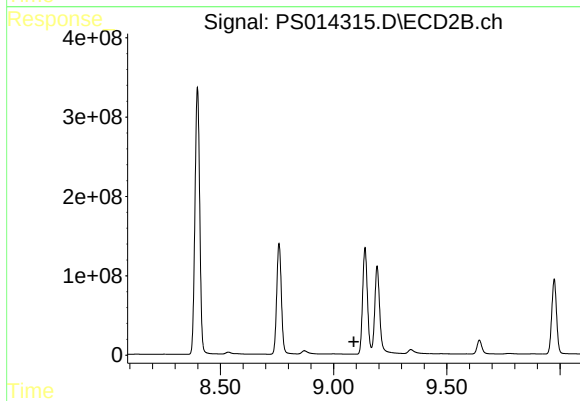

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 9.089 min
Response: 0
Conc: N.D.

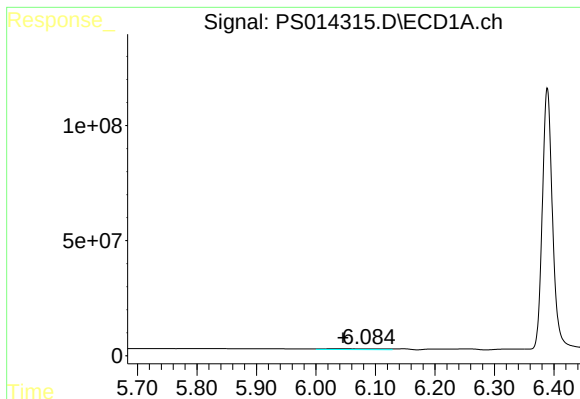

#6 AR-1016-4


R.T.: 6.031 min
Delta R.T.: -0.015 min
Response: 24006464
Conc: 178.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

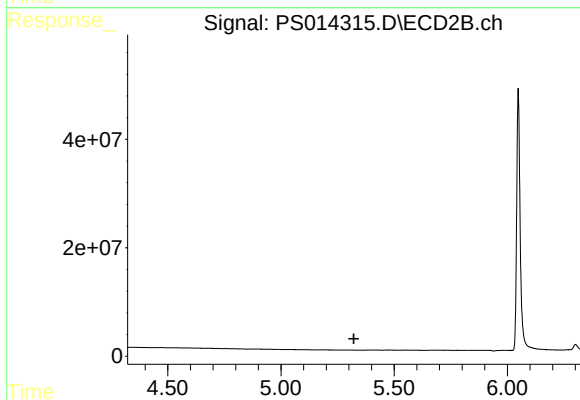


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.322 min
Response: 0
Conc: N.D.

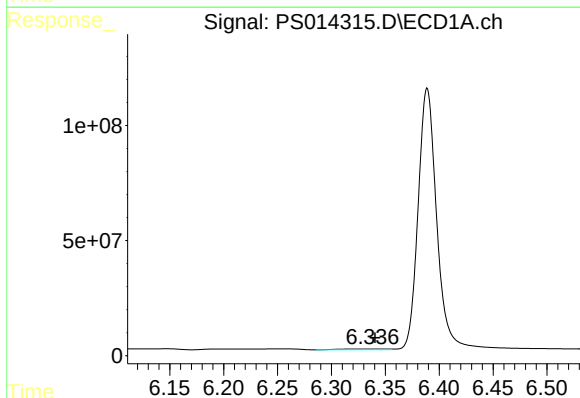


#7 AR-1016-5

R.T.: 6.337 min
Delta R.T.: -0.004 min
Response: 8857278
Conc: 66.01 ng/ml

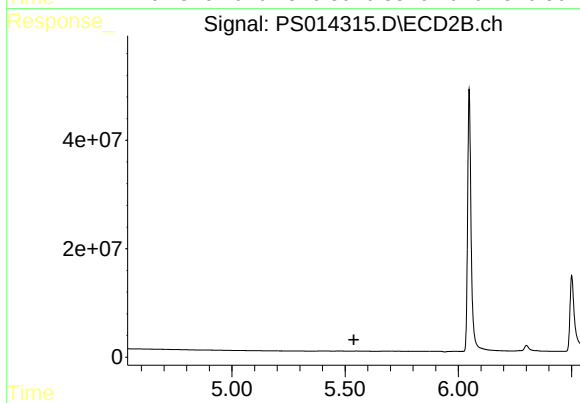

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.539 min
Response: 0
Conc: N.D.

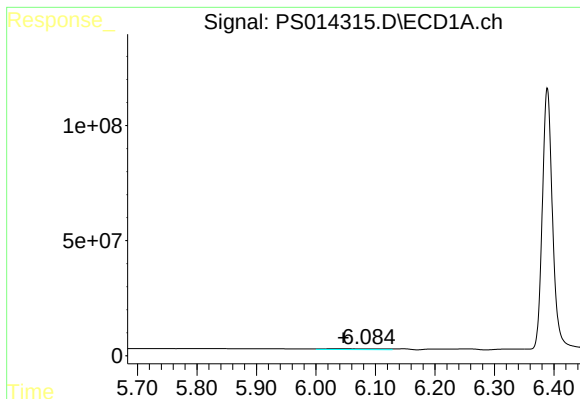

#14 AR-1232-4


R.T.: 6.031 min
Delta R.T.: -0.015 min
Response: 24006464
Conc: 444.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

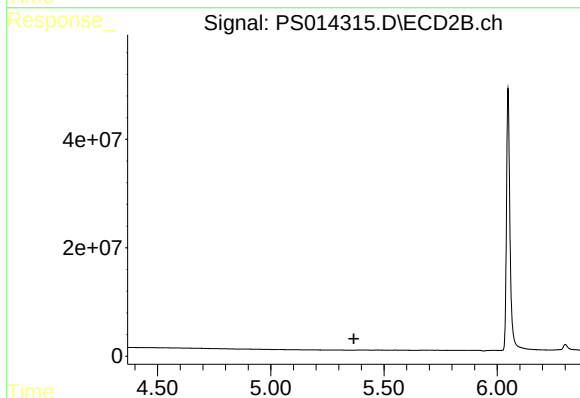


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.367 min
Response: 0
Conc: N.D.

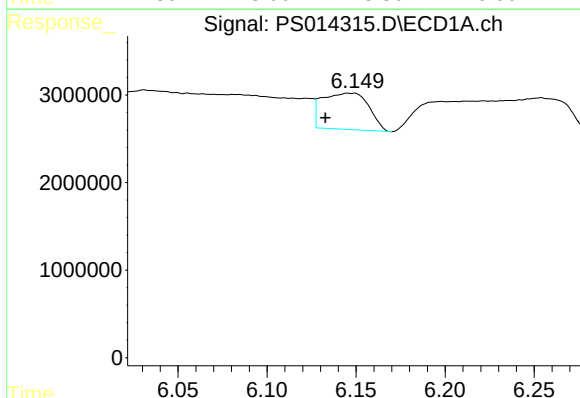


#15 AR-1232-5

R.T.: 6.148 min
Delta R.T.: 0.015 min
Response: 7542181
Conc: 183.84 ng/ml

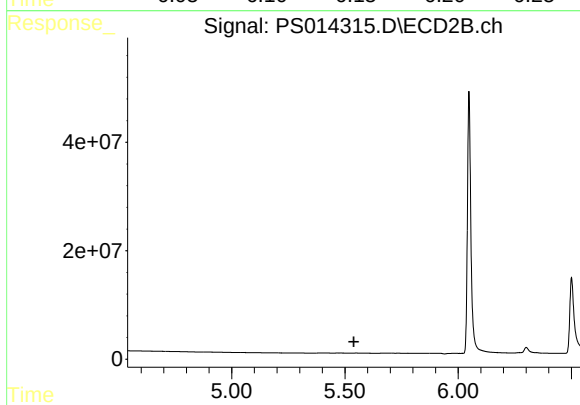

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.540 min
Response: 0
Conc: N.D.

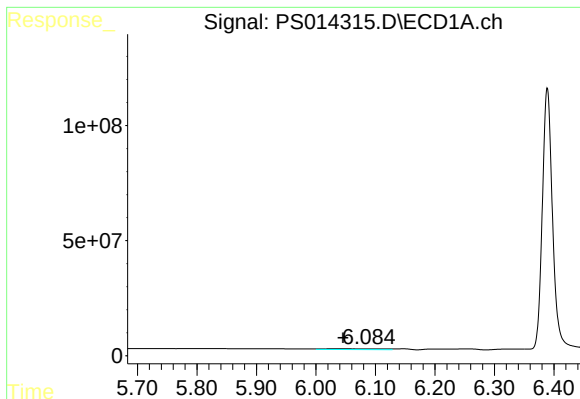

#19 AR-1242-4


R.T.: 6.031 min
Delta R.T.: -0.015 min
Response: 24006464
Conc: 236.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

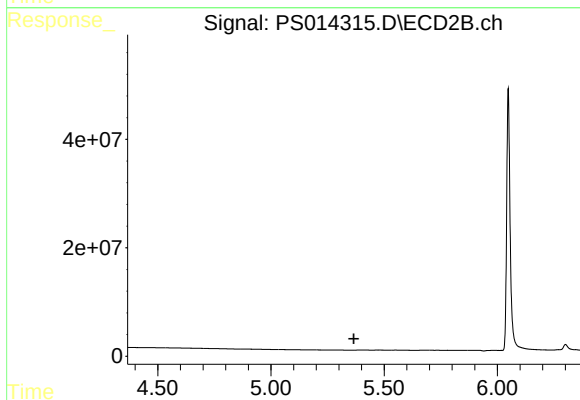


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

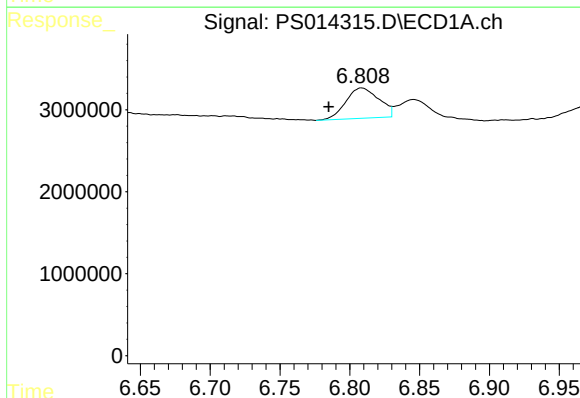


#20 AR-1242-5

R.T.: 6.809 min
Delta R.T.: 0.024 min
Response: 6123119
Conc: 57.21 ng/ml

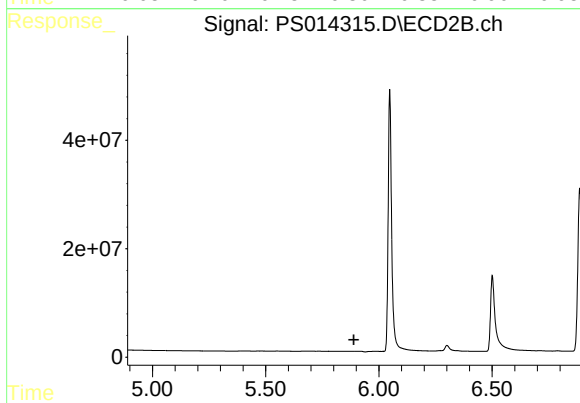

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.890 min
Response: 0
Conc: N.D.

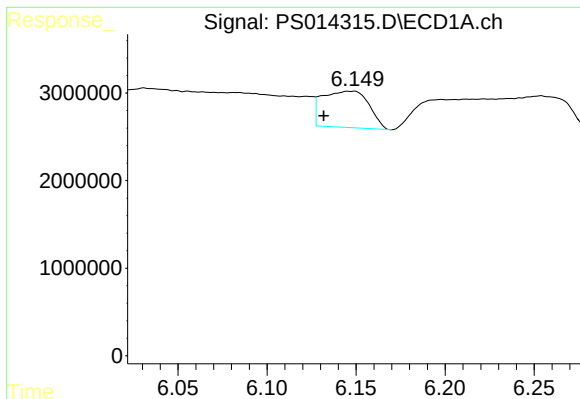

#22 AR-1248-2


R.T.: 6.148 min
Delta R.T.: 0.016 min
Response: 7542181
Conc: 48.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

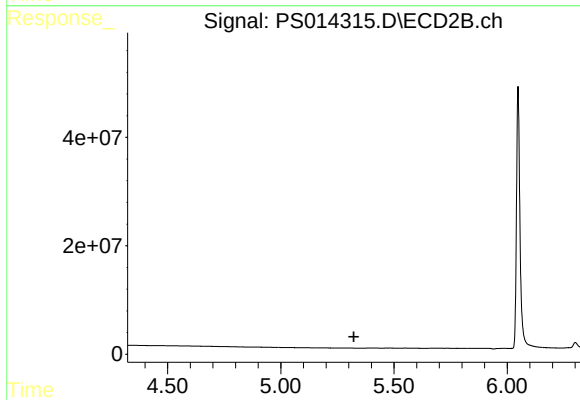


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.323 min
Response: 0
Conc: N.D.

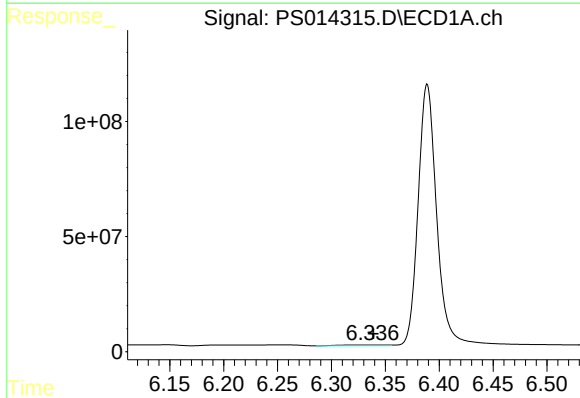


#23 AR-1248-3

R.T.: 6.337 min
Delta R.T.: -0.002 min
Response: 8857278
Conc: 50.77 ng/ml

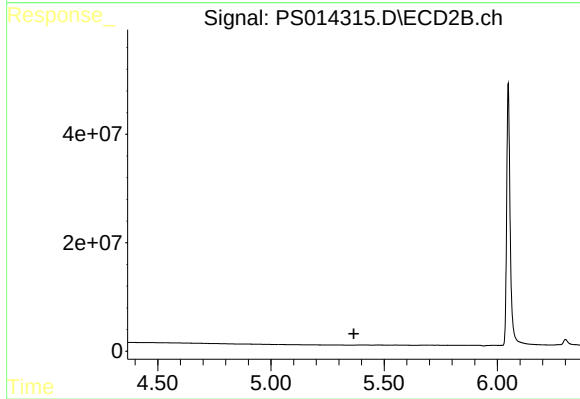

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

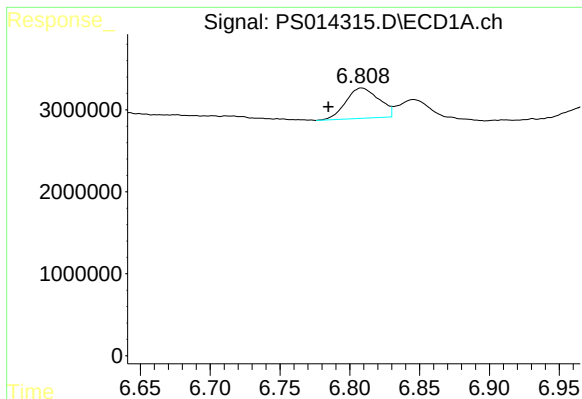

#25 AR-1248-5


R.T.: 6.809 min
Delta R.T.: 0.024 min
Response: 6123119
Conc: 31.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

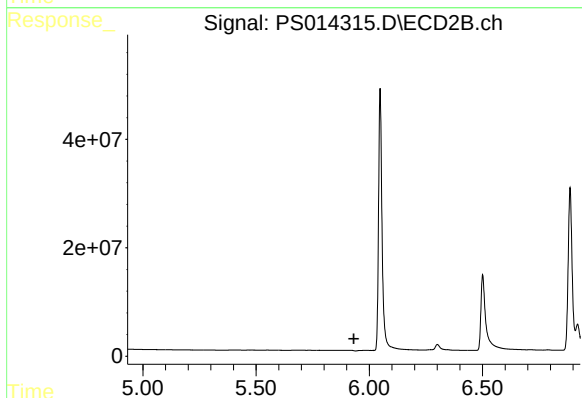


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.932 min
Response: 0
Conc: N.D.

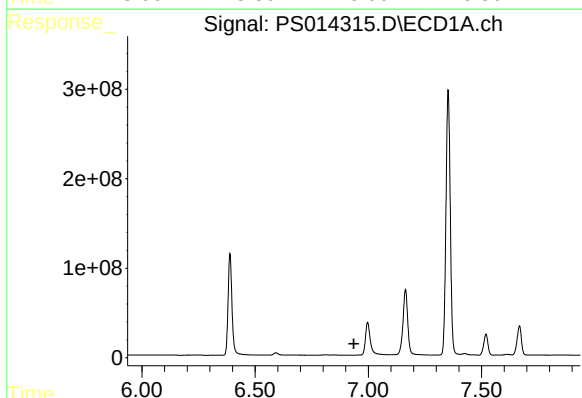


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

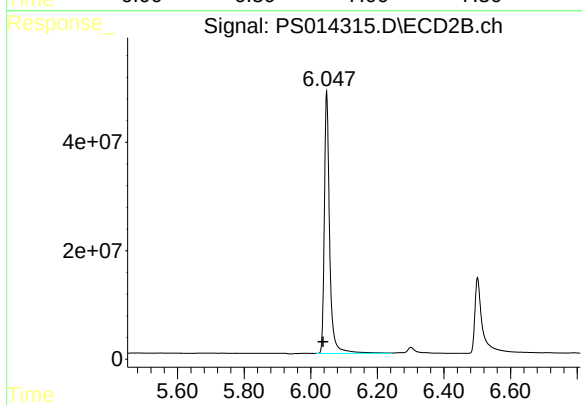

#27 AR-1254-2


R.T.: 6.048 min
Delta R.T.: 0.011 min
Response: 533401661
Conc: 12396.81 ng/ml

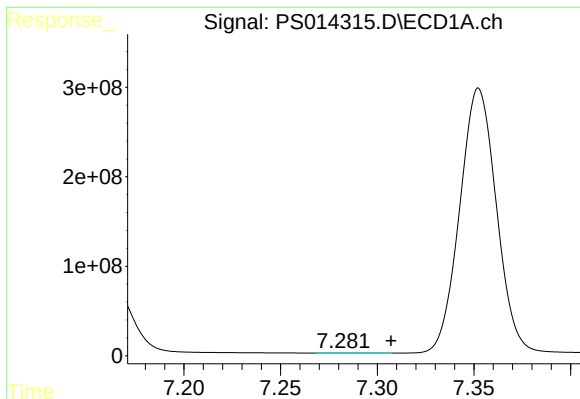

#28 AR-1254-3


R.T.: 7.281 min
Delta R.T.: -0.026 min
Response: 6492822
Conc: 19.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

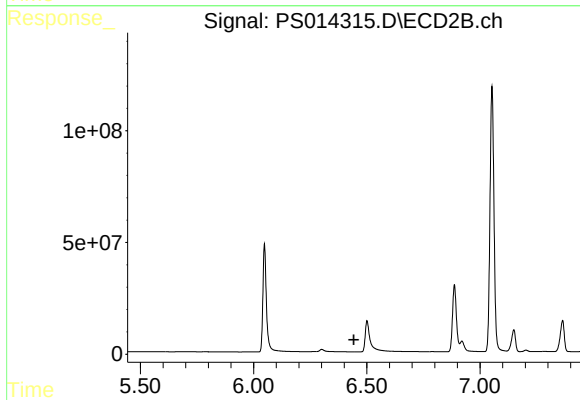


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

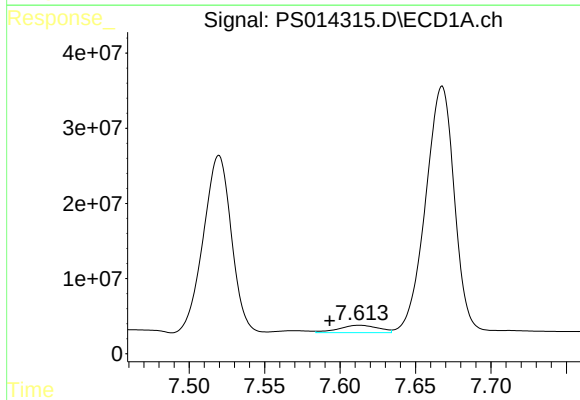


#29 AR-1254-4

R.T.: 7.613 min
Delta R.T.: 0.020 min
Response: 18067035
Conc: 73.18 ng/ml

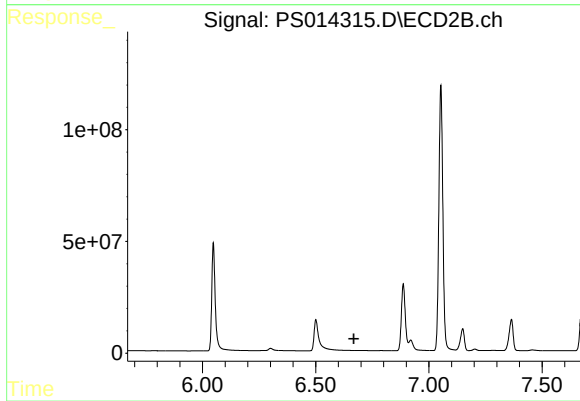

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.669 min
Response: 0
Conc: N.D.

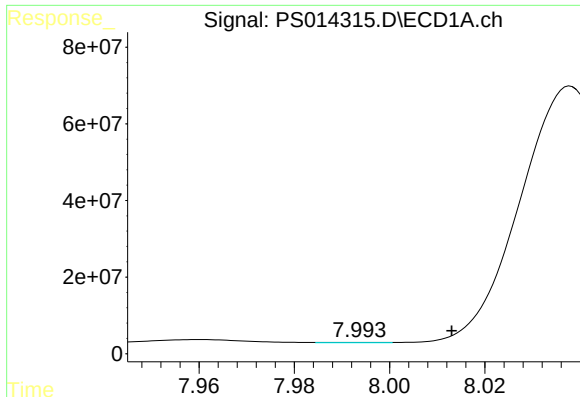

#30 AR-1254-5


R.T.: 7.993 min
Delta R.T.: -0.020 min
Response: 1045576
Conc: 3.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

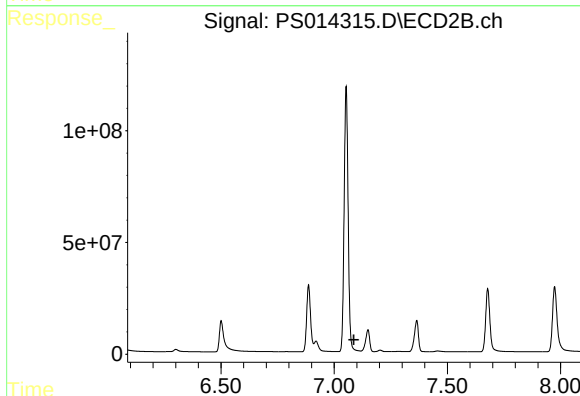


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

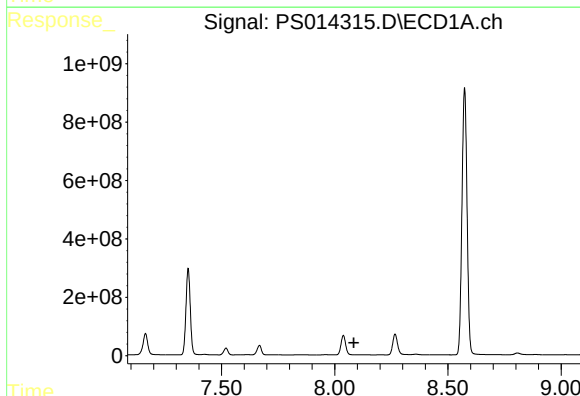


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.084 min
Response: 0
Conc: N.D.

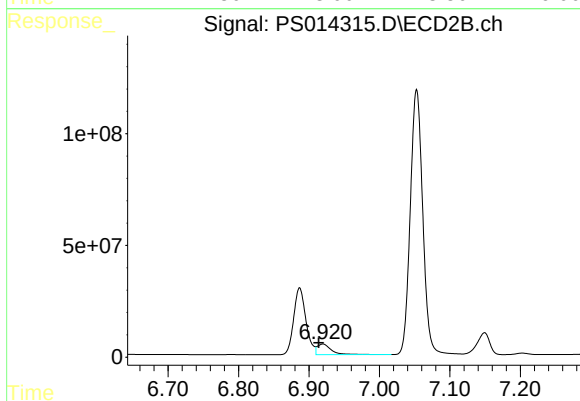

#33 AR-1260-3


R.T.: 6.920 min
Delta R.T.: 0.006 min
Response: 66006041
Conc: 827.73 ng/ml

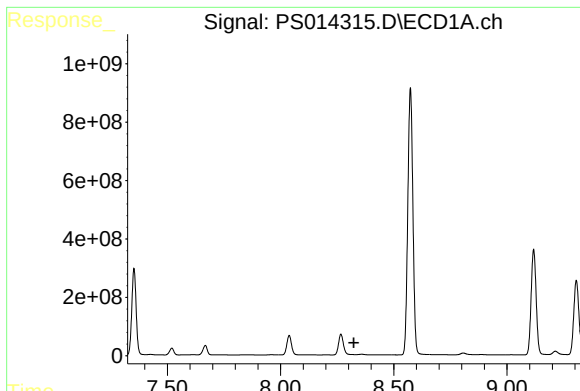

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

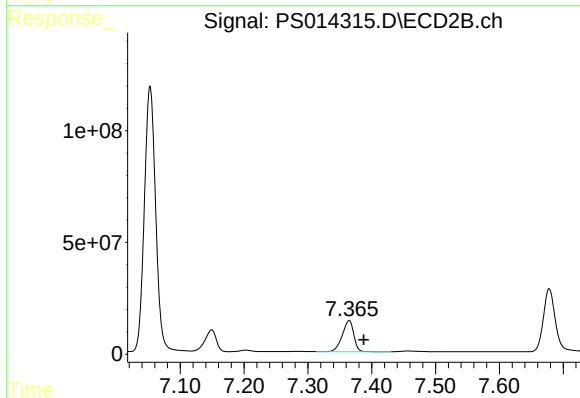


#34 AR-1260-4

R.T.: 7.365 min
Delta R.T.: -0.023 min
Response: 173698442
Conc: 2073.63 ng/ml

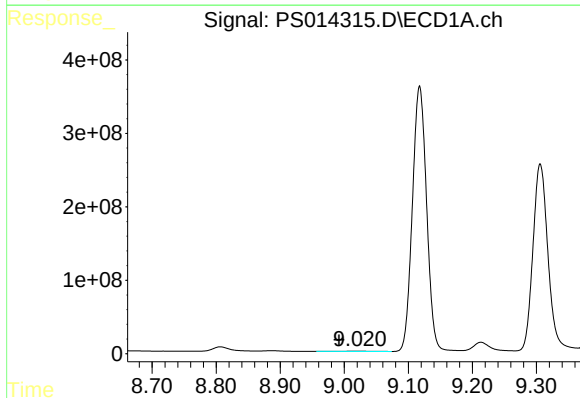


#38 AR-1262-3

R.T.: 9.020 min
Delta R.T.: 0.027 min
Response: 6680189
Conc: 17.23 ng/ml

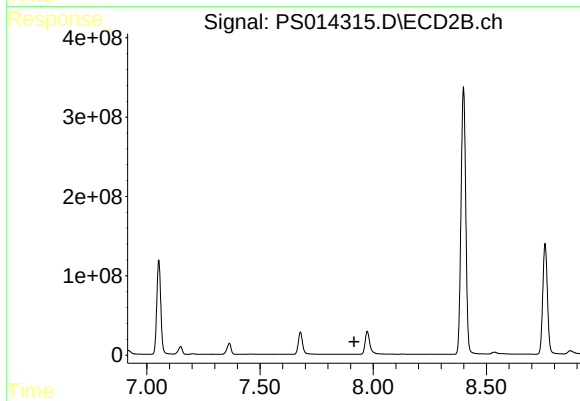

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.915 min
Response: 0
Conc: N.D.

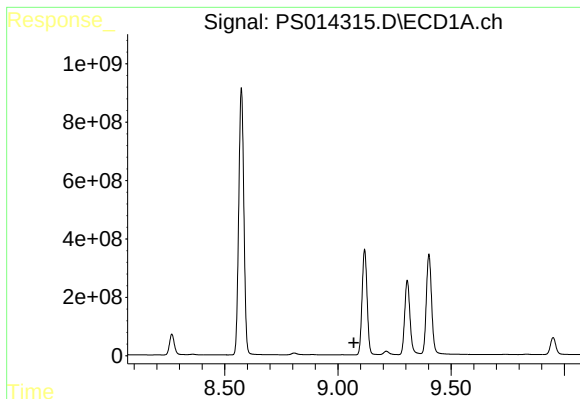

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

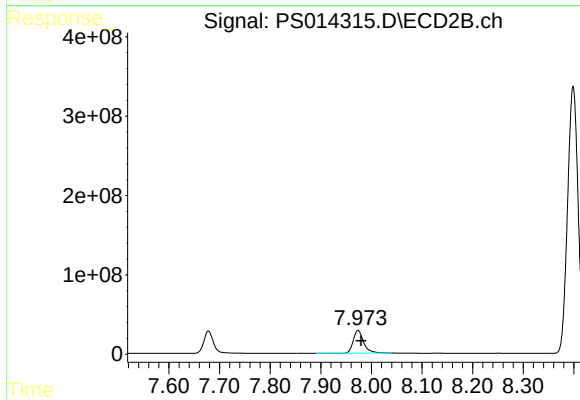


#39 AR-1262-4

R.T.: 7.973 min
Delta R.T.: -0.006 min
Response: 407592313
Conc: 1610.51 ng/ml

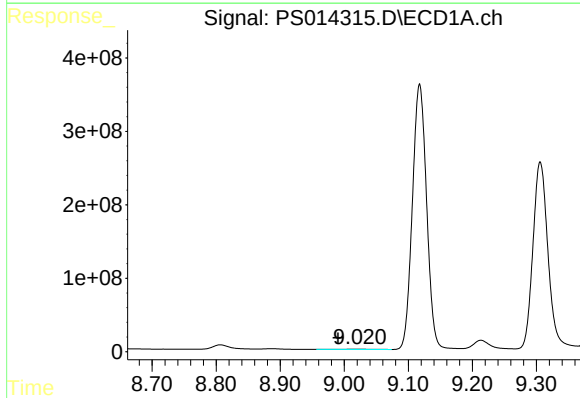


#41 AR-1268-1

R.T.: 9.020 min
Delta R.T.: 0.029 min
Response: 6680189
Conc: 9.76 ng/ml

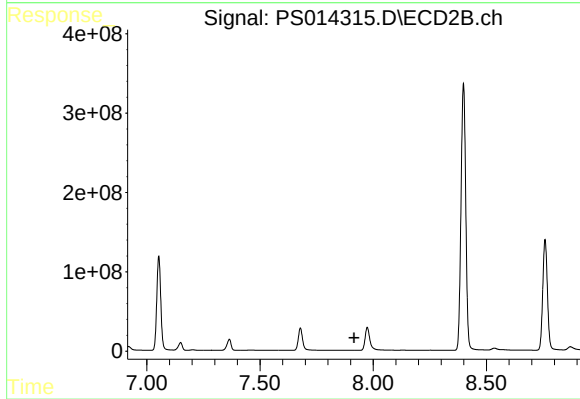

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 7.915 min
Response: 0
Conc: N.D.

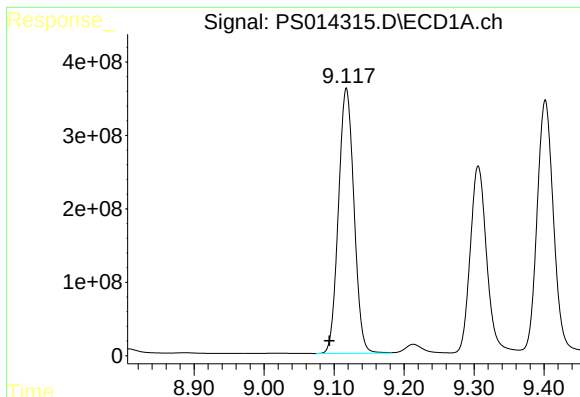

#42 AR-1268-2


R.T.: 9.118 min
Delta R.T.: 0.024 min
Response: 5562439120
Conc: 8972.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
HSTDCCC750

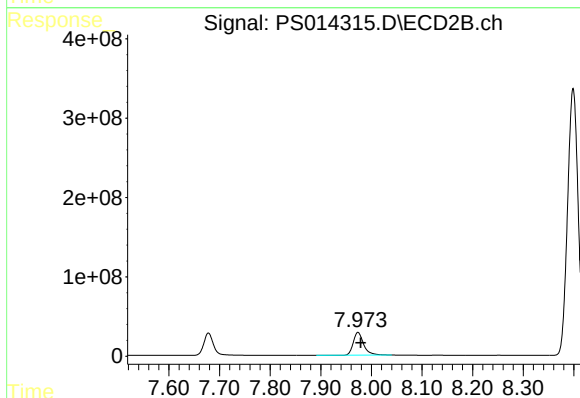


#42 AR-1268-2

R.T.: 7.973 min
Delta R.T.: -0.006 min
Response: 407592313
Conc: 1004.87 ng/ml

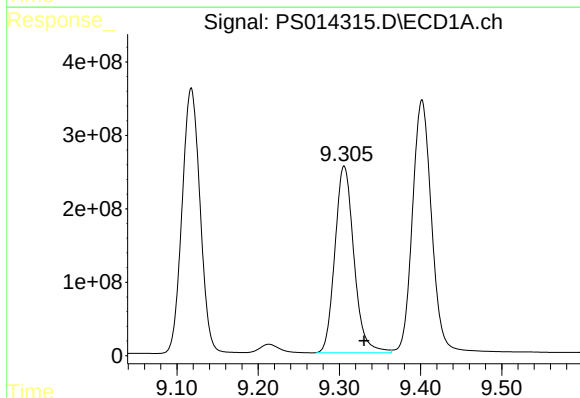

#43 AR-1268-3

R.T.: 9.306 min
Delta R.T.: -0.025 min
Response: 4133596053
Conc: 7873.87 ng/ml

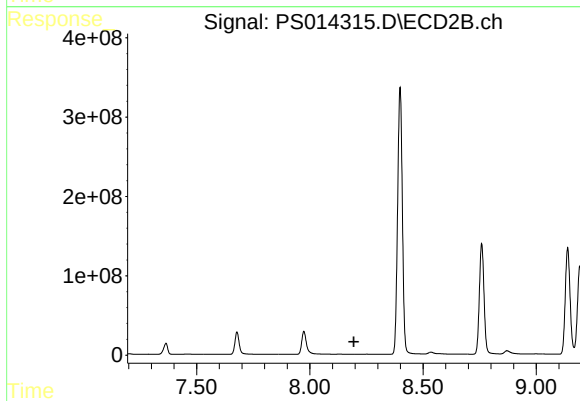

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.195 min
Response: 0
Conc: N.D.