

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032221\
 Data File : PS014320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2021 21:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:37:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 22 09:06:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8)	L2	AR-1221-1	4.857f	0.000	3415700	0	59.713 N.D. #
20)	L4	AR-1242-5	6.804f	0.000	926732	0	8.658 N.D. #
25)	L5	AR-1248-5	6.804f	0.000	926732	0	4.833 N.D. #
32)	L7	AR-1260-2	7.705f	0.000	245553	0	0.858 N.D. #
33)	L7	AR-1260-3	0.000	6.888f	0	255.1E6	N.D. 3198.404 #
34)	L7	AR-1260-4	8.341f	0.000	16633502	0	66.039 N.D. #
43)	L9	AR-1268-3	9.340	0.000	514887	0	0.981 N.D. #
45)	L9	AR-1268-5	10.260f	0.000	908688	0	0.477 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032221\
Data File : PS014320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2021 21:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:37:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 22 09:06:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

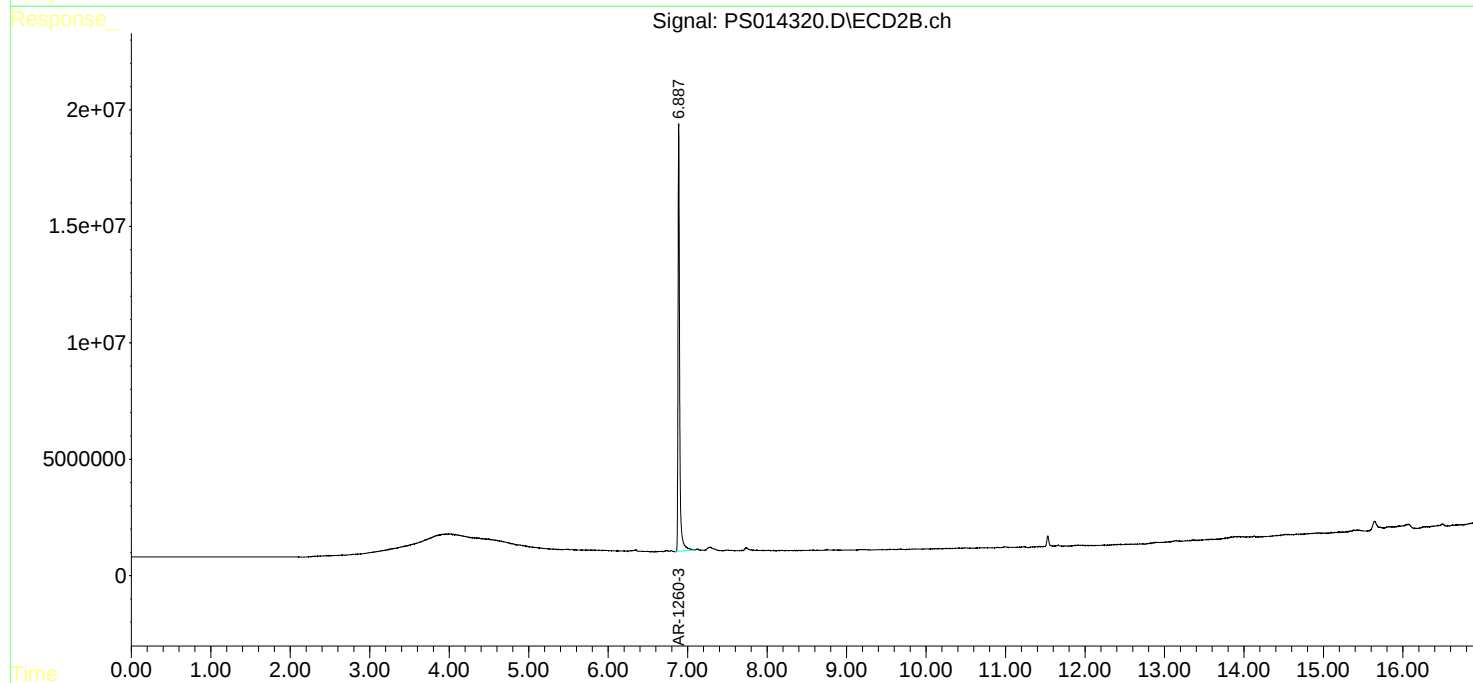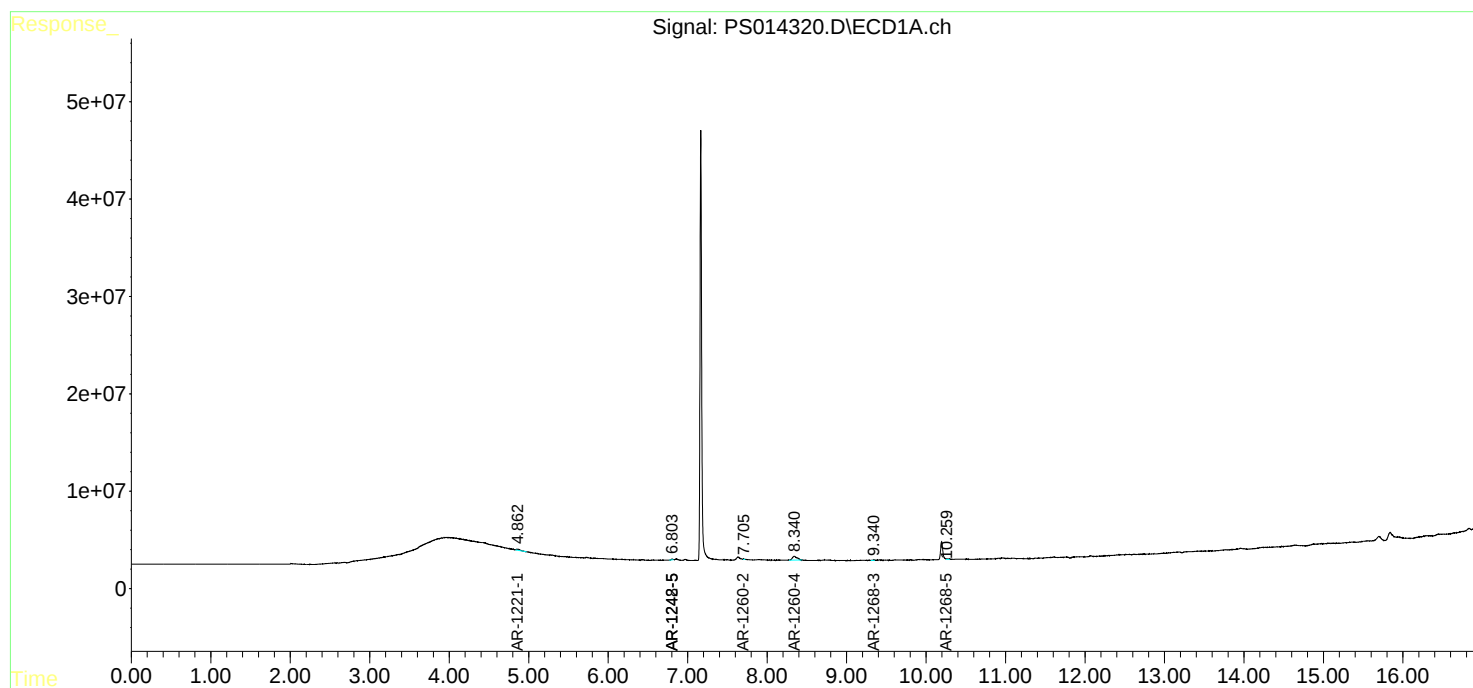


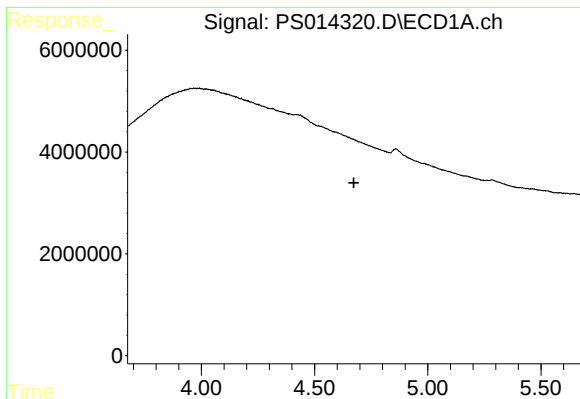

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

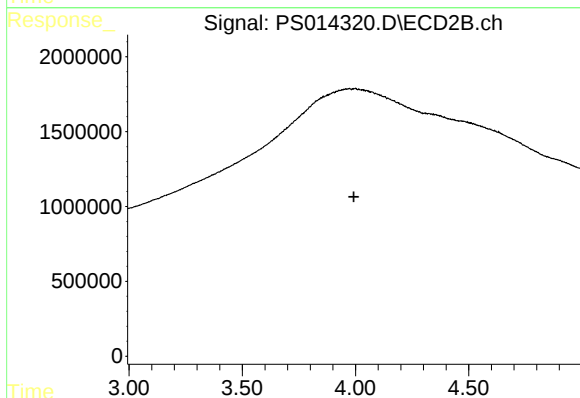


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.993 min
Response: 0
Conc: N.D.

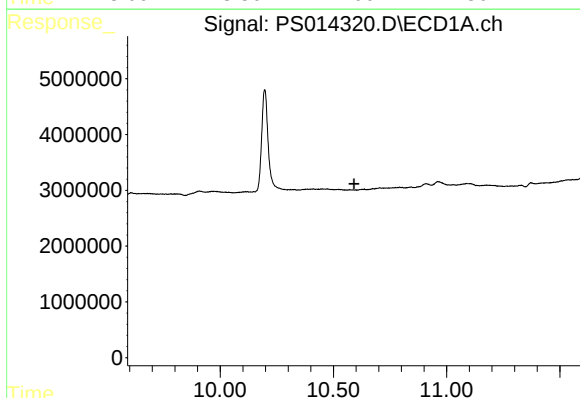


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.591 min
Response: 0
Conc: N.D.

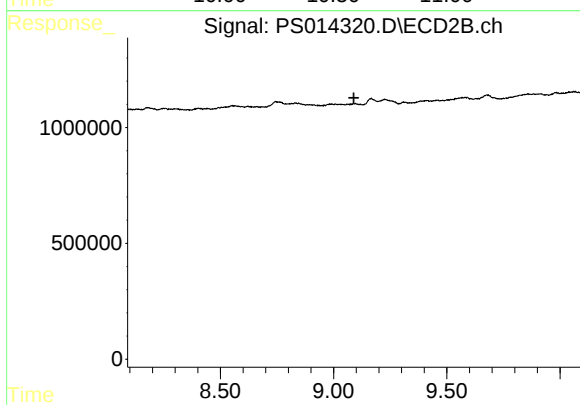

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.089 min
Response: 0
Conc: N.D.

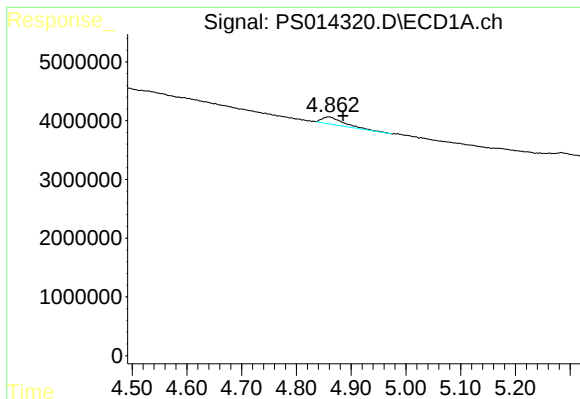

#8 AR-1221-1


R.T.: 4.857 min
Delta R.T.: -0.028 min
Response: 3415700
Conc: 59.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

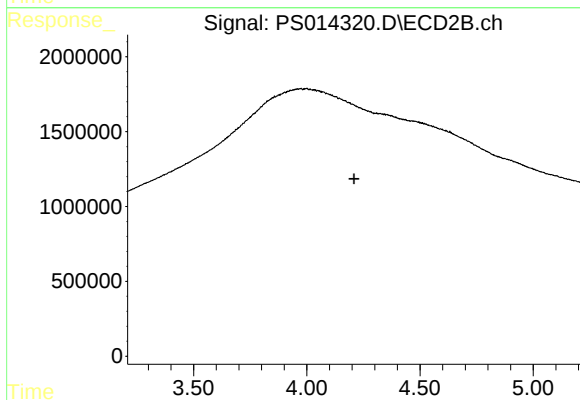


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.208 min
Response: 0
Conc: N.D.

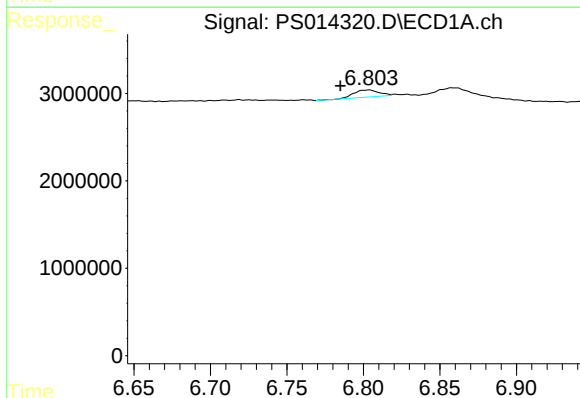


#20 AR-1242-5

R.T.: 6.804 min
Delta R.T.: 0.019 min
Response: 926732
Conc: 8.66 ng/ml

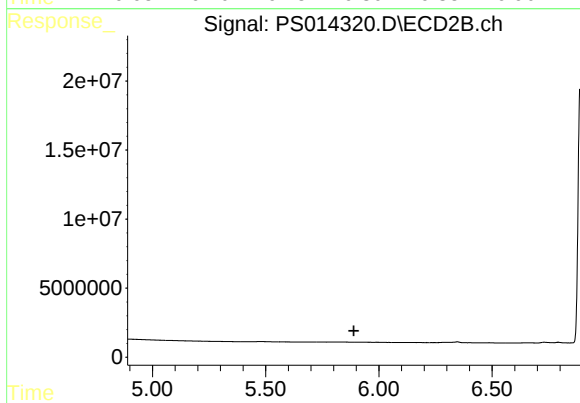

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.890 min
Response: 0
Conc: N.D.

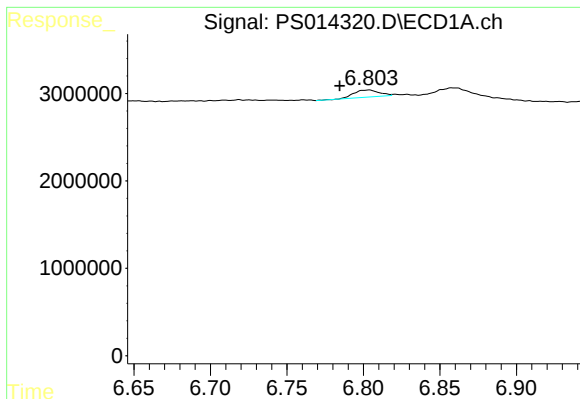

#25 AR-1248-5


R.T.: 6.804 min
Delta R.T.: 0.019 min
Response: 926732
Conc: 4.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

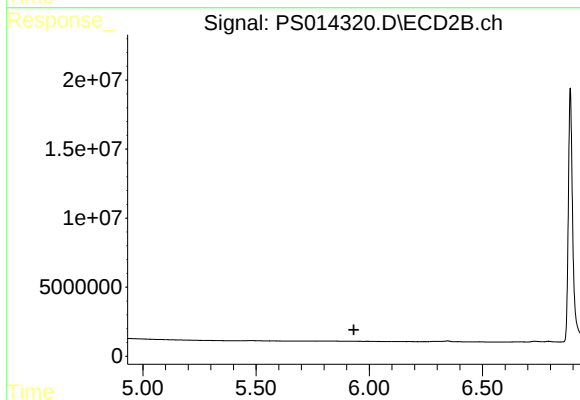


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.932 min
Response: 0
Conc: N.D.

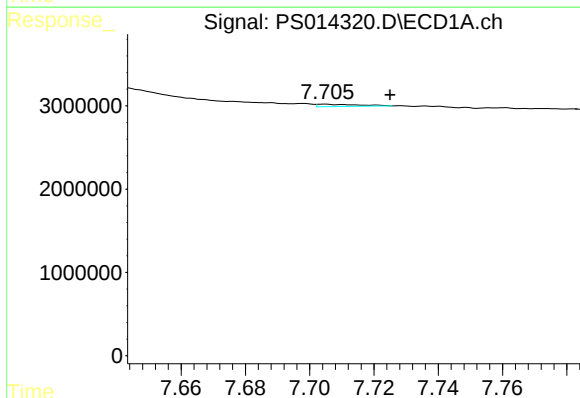


#32 AR-1260-2

R.T.: 7.705 min
Delta R.T.: -0.020 min
Response: 245553
Conc: 0.86 ng/ml

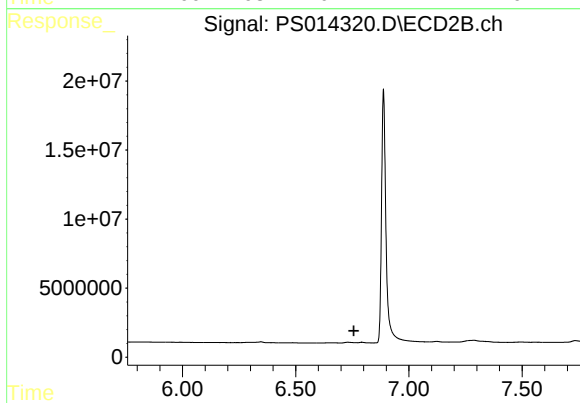

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.757 min
Response: 0
Conc: N.D.

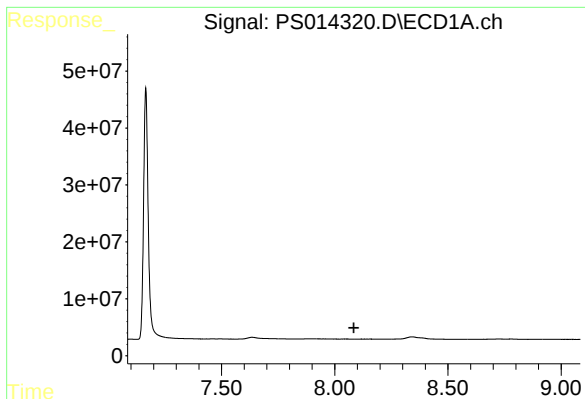

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

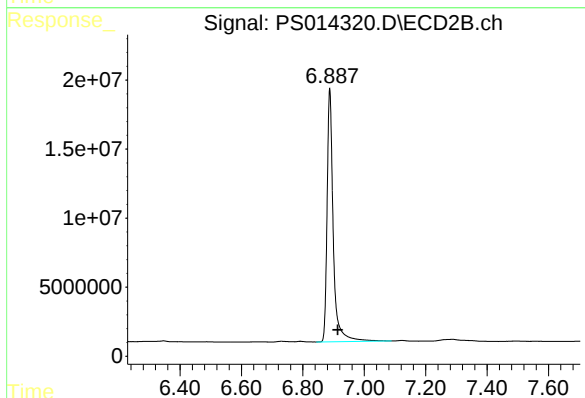


#33 AR-1260-3

R.T.: 6.888 min
Delta R.T.: -0.026 min
Response: 255051496
Conc: 3198.40 ng/ml

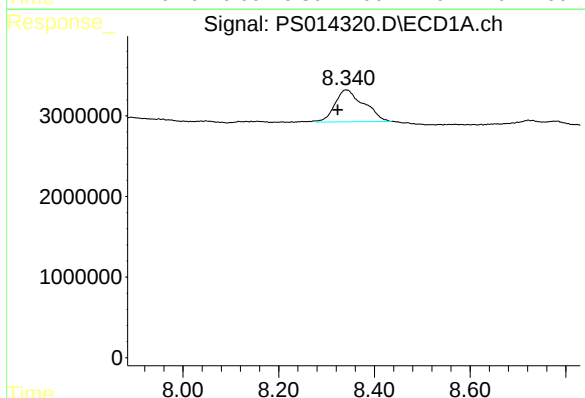


#34 AR-1260-4

R.T.: 8.341 min
Delta R.T.: 0.017 min
Response: 16633502
Conc: 66.04 ng/ml

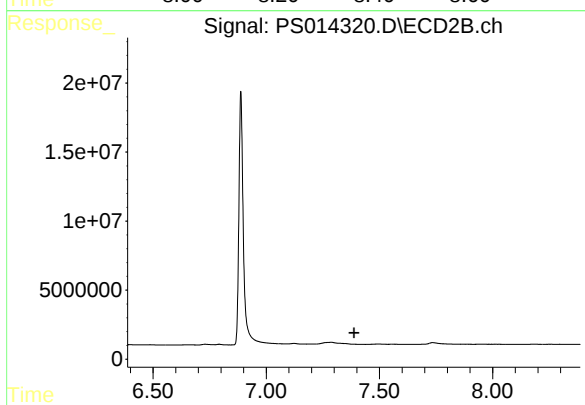

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

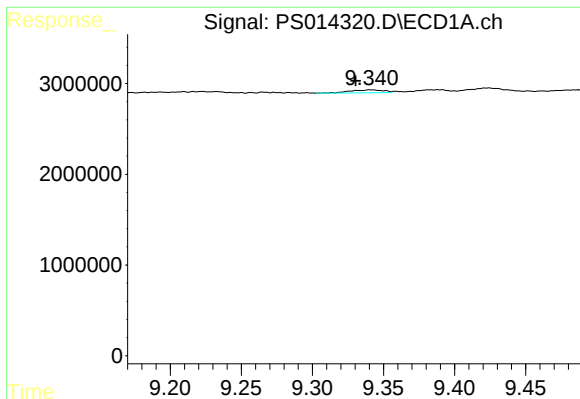

#43 AR-1268-3


R.T.: 9.340 min
Delta R.T.: 0.010 min
Response: 514887
Conc: 0.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

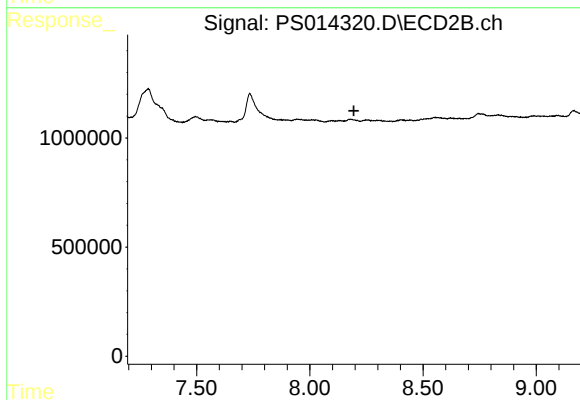


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.195 min
Response: 0
Conc: N.D.

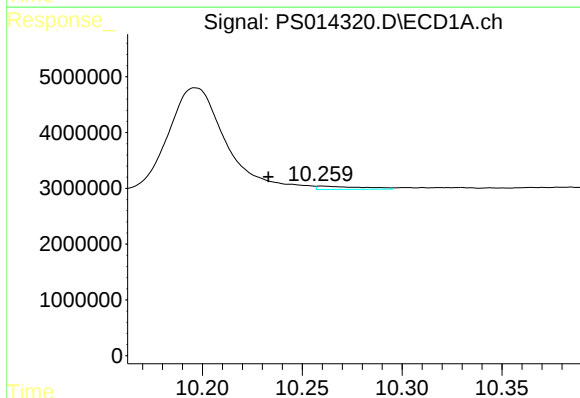

#45 AR-1268-5

R.T.: 10.260 min
Delta R.T.: 0.027 min
Response: 908688
Conc: 0.48 ng/ml

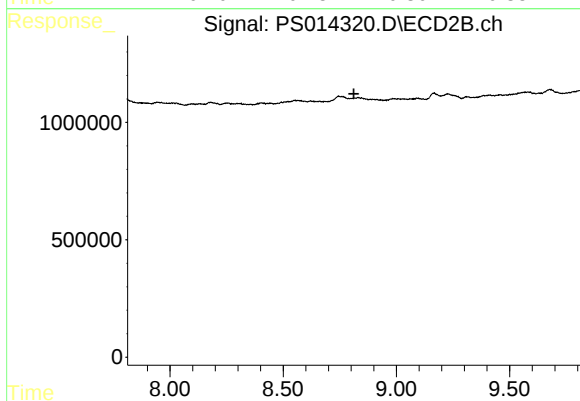

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.812 min
Response: 0
Conc: N.D.