

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 10:21
 Operator : DD\AJ
 Sample : PB135083BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB135083BL

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:40:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 15:40:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.917	3.928	1083276	753090	19.069	18.050
2) SA Decachlor...	10.910	9.190	733759	730868	19.077	19.034m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
Data File : P0076405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 10:21
Operator : DD\AJ
Sample : PB135083BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB135083BL


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 15:40:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

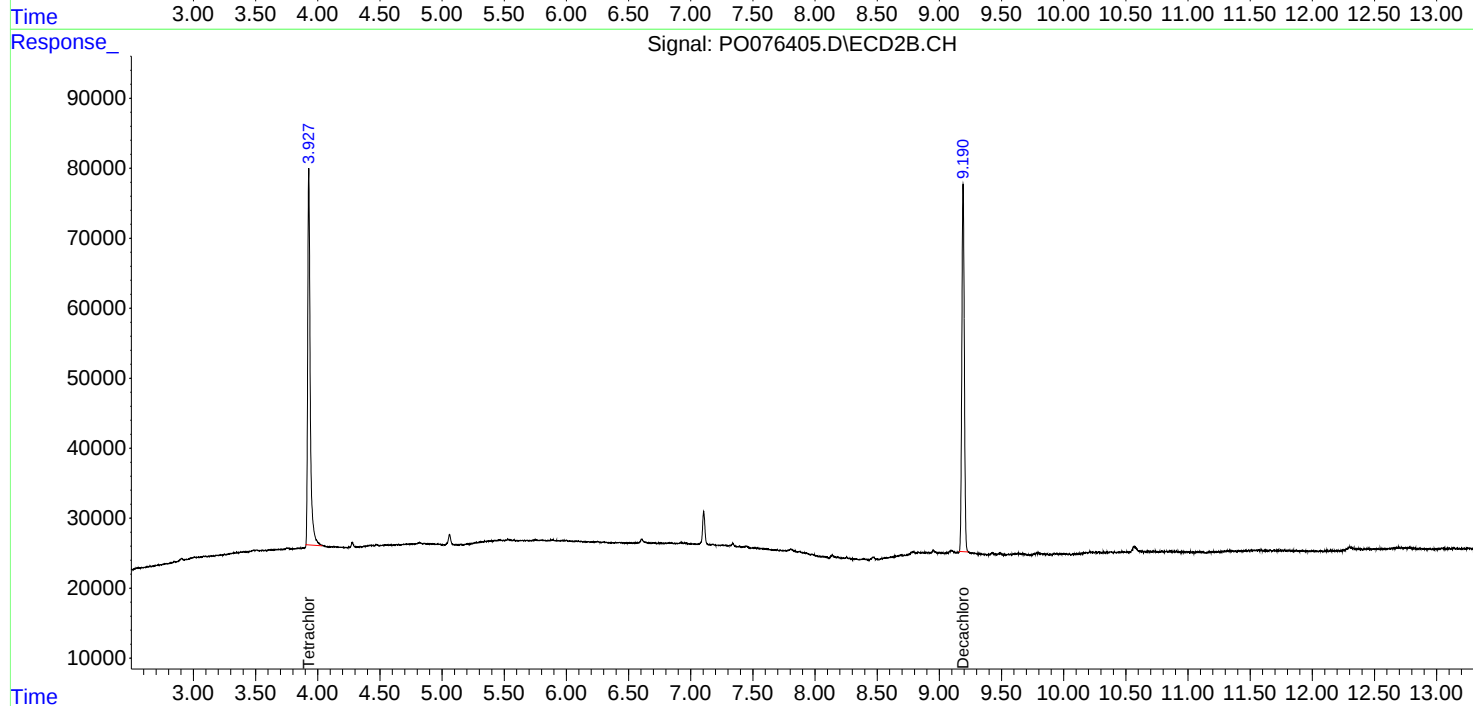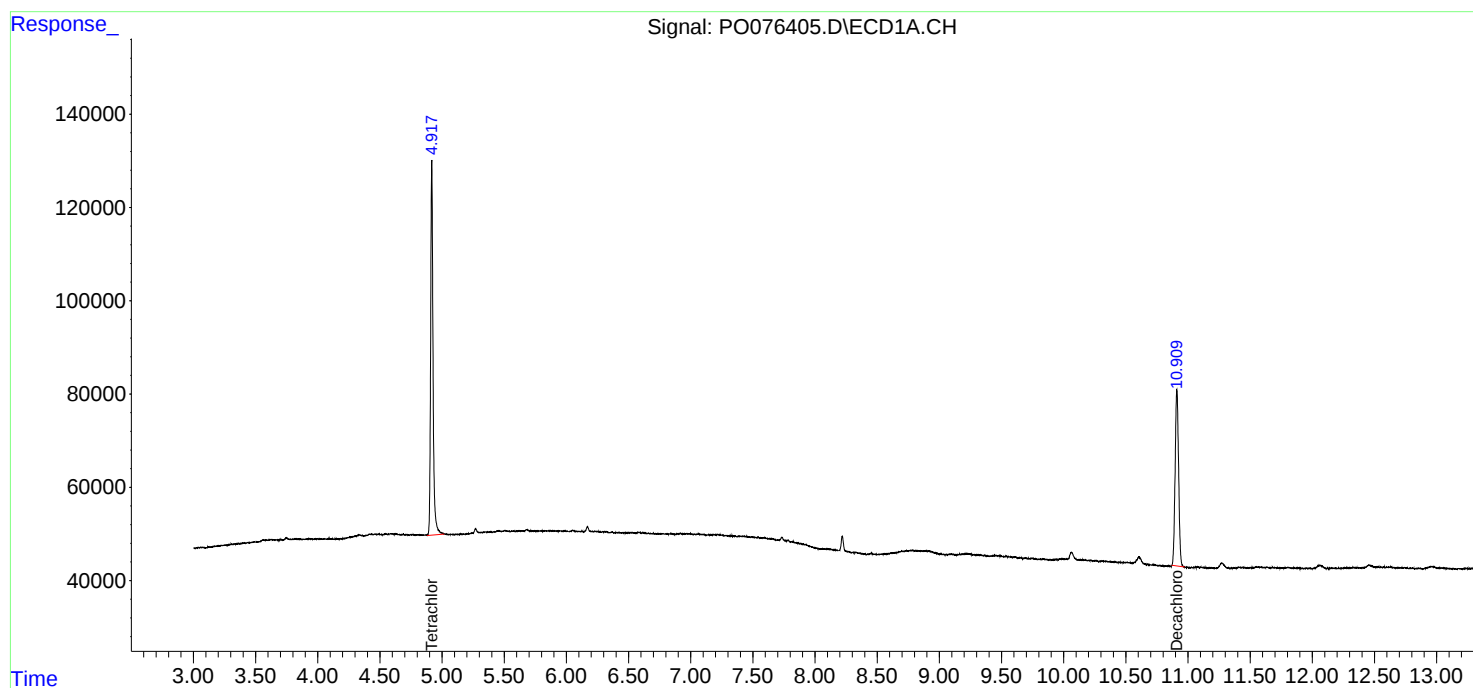

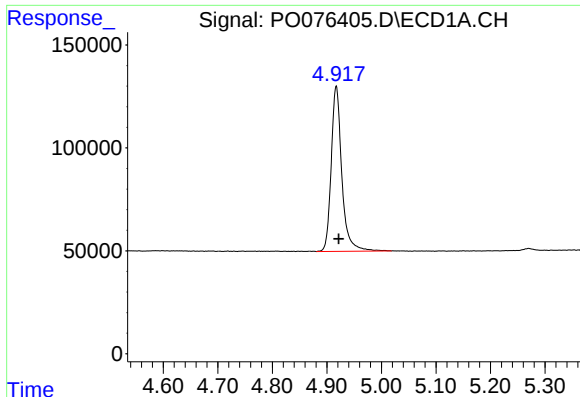


#1 Tetrachloro-m-xylene

R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 1083276
Conc: 19.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB135083BL


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:01 PM

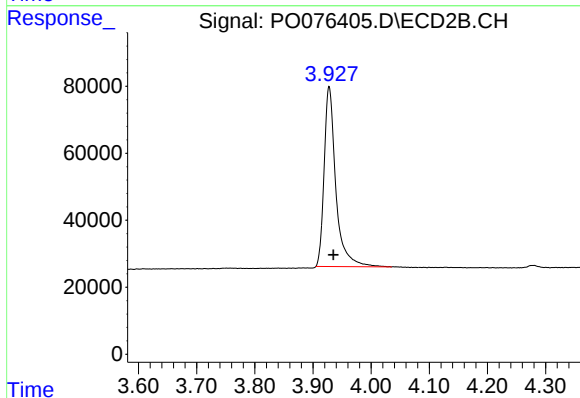


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.008 min
Response: 753090
Conc: 18.05 ng/ml

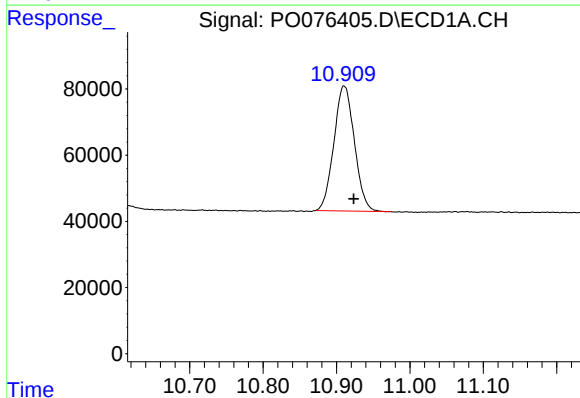

#2 Decachlorobiphenyl

R.T.: 10.910 min
Delta R.T.: -0.013 min
Response: 733759
Conc: 19.08 ng/ml

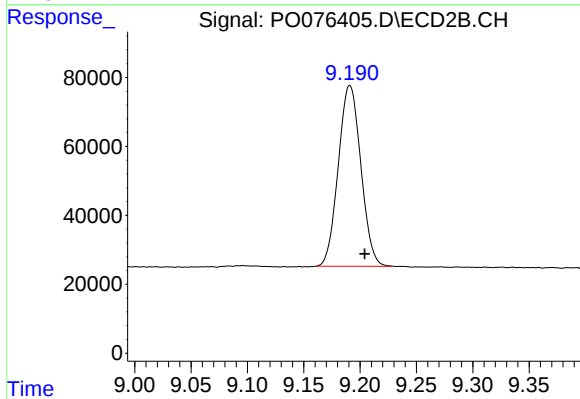

#2 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.014 min
Response: 730868
Conc: 19.03 ng/ml m