

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076427.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 16:37
 Operator : DD\AJ
 Sample : M1745-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:40:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 00:35:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.915	3.928	2249782	913890	39.602	21.905 #
2) SA Decachlor...	10.908f	9.189	1222165	998737	31.775	26.010m
Target Compounds						
26) L6 AR-1254-1	7.158	6.041	174671	139341	85.230	60.967 #
27) L6 AR-1254-2	7.382	6.199	212555	87899	68.400	44.381 #
28) L6 AR-1254-3	7.761	6.618	173115	159034	54.414	52.800
29) L6 AR-1254-4	8.057	6.857	125734	86363	60.012	48.940
30) L6 AR-1254-5	8.487	7.284	198074	289771	86.244	110.681 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032221\
Data File : PO076427.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 16:37
Operator : DD\AJ
Sample : M1745-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 00:35:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

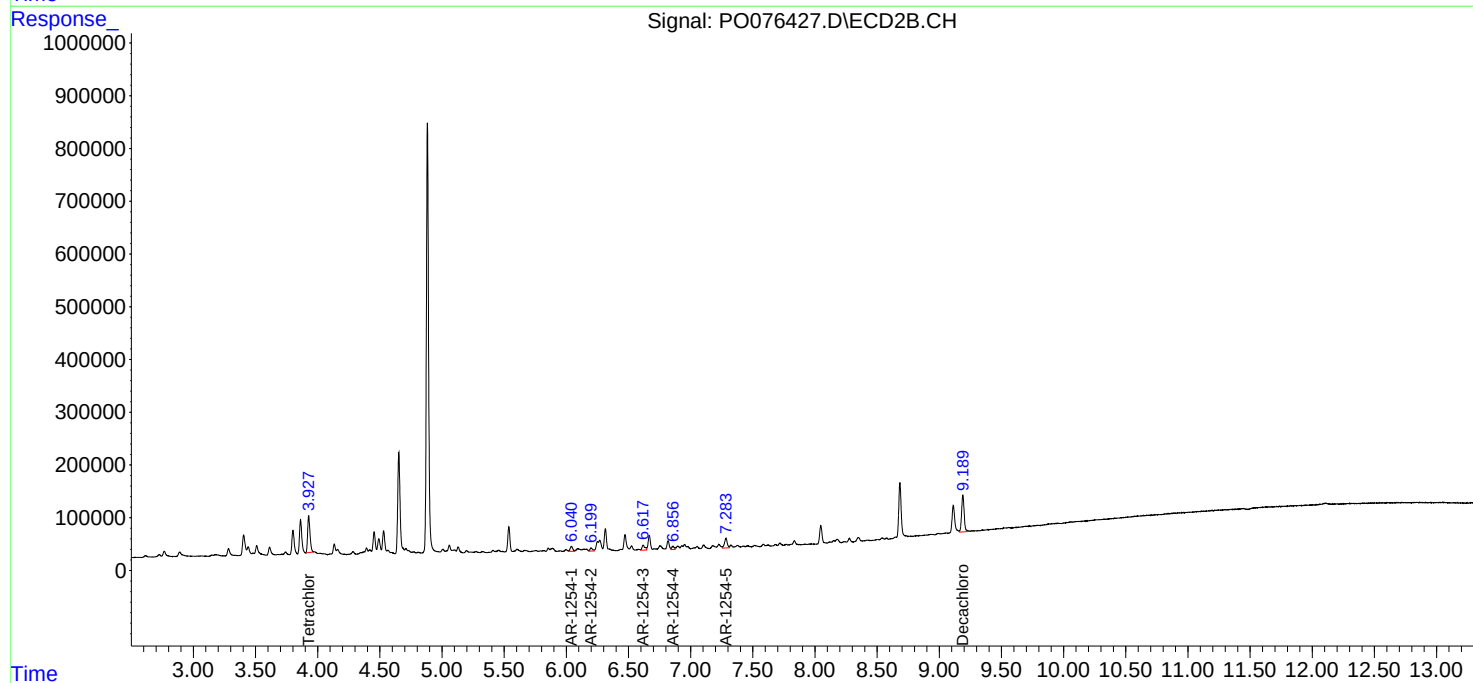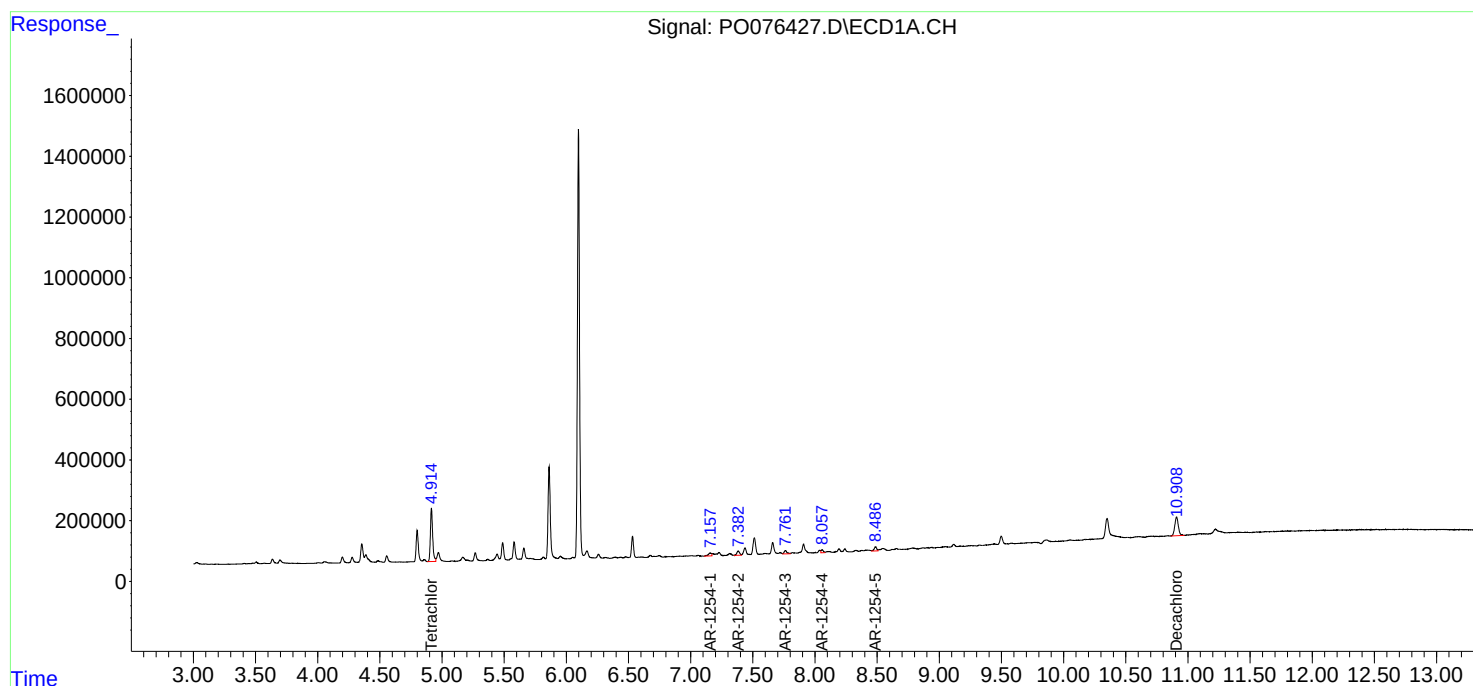

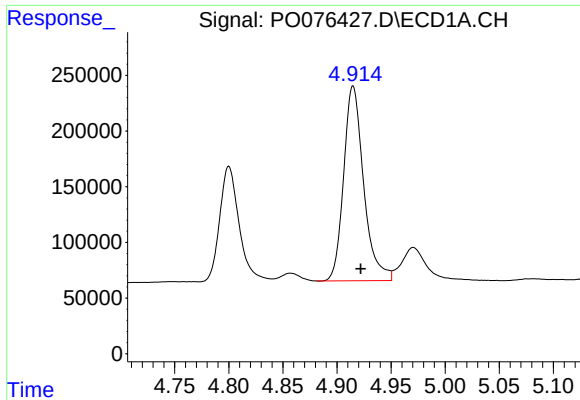


#1 Tetrachloro-m-xylene

R.T.: 4.915 min
Delta R.T.: -0.007 min
Response: 2249782
Conc: 39.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:43 PM

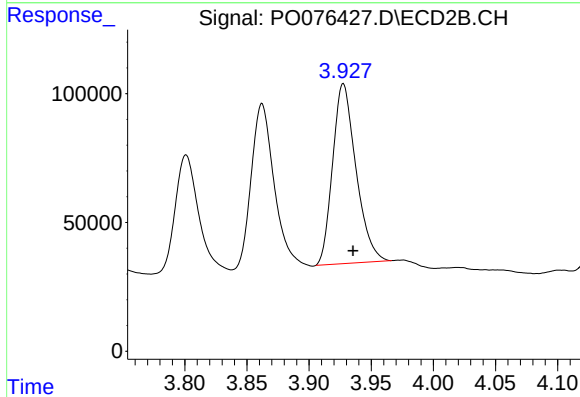


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.008 min
Response: 913890
Conc: 21.90 ng/ml

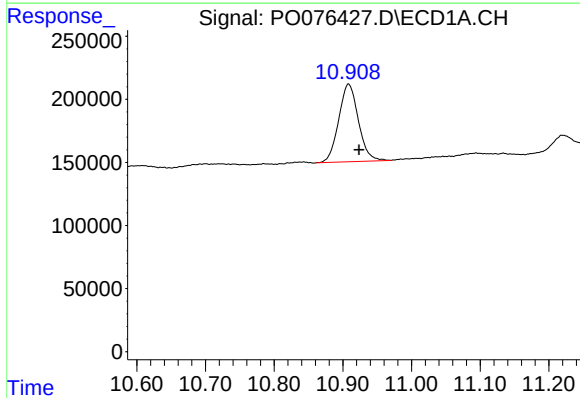


#2 Decachlorobiphenyl

R.T.: 10.908 min
Delta R.T.: -0.015 min
Response: 1222165
Conc: 31.77 ng/ml

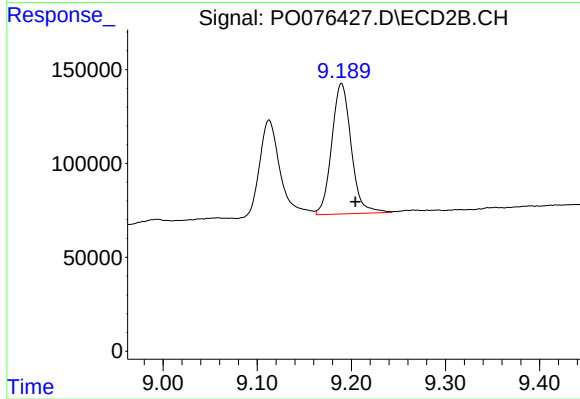

#2 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: -0.015 min
Response: 998737
Conc: 26.01 ng/ml m

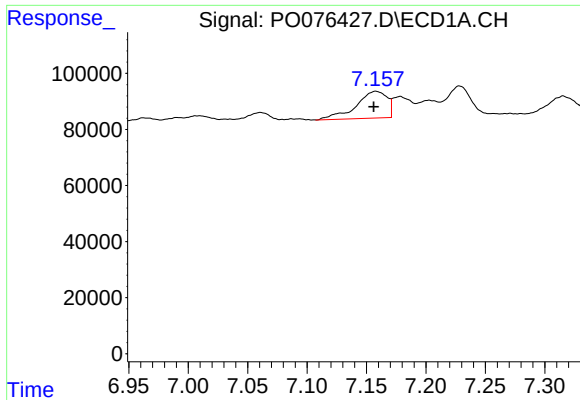


#26 AR-1254-1

R.T.: 7.158 min
Delta R.T.: 0.002 min
Response: 174671
Conc: 85.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:43 PM

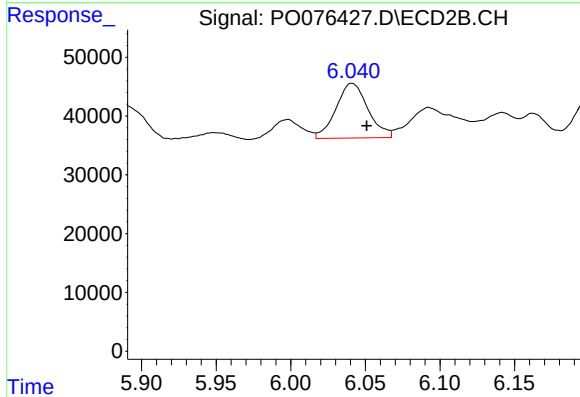


#26 AR-1254-1

R.T.: 6.041 min
Delta R.T.: -0.010 min
Response: 139341
Conc: 60.97 ng/ml

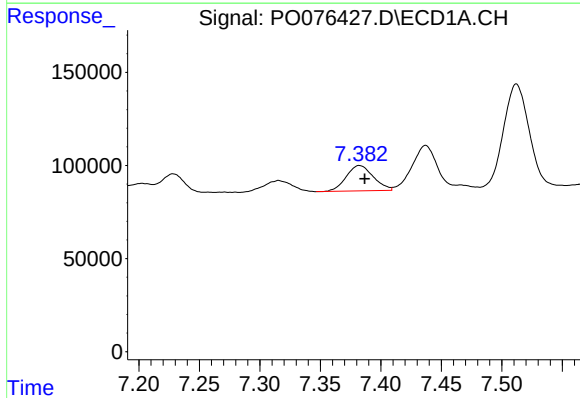


#27 AR-1254-2

R.T.: 7.382 min
Delta R.T.: -0.004 min
Response: 212555
Conc: 68.40 ng/ml

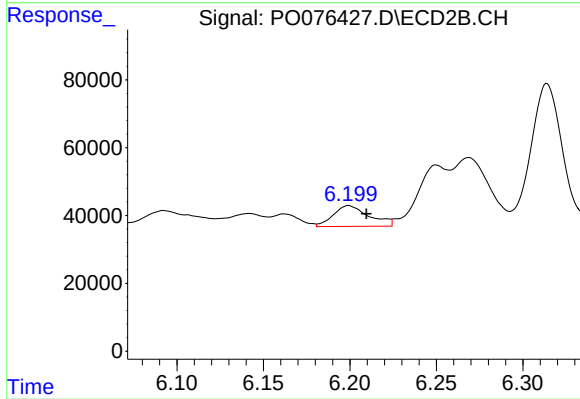

#27 AR-1254-2

R.T.: 6.199 min
Delta R.T.: -0.010 min
Response: 87899
Conc: 44.38 ng/ml

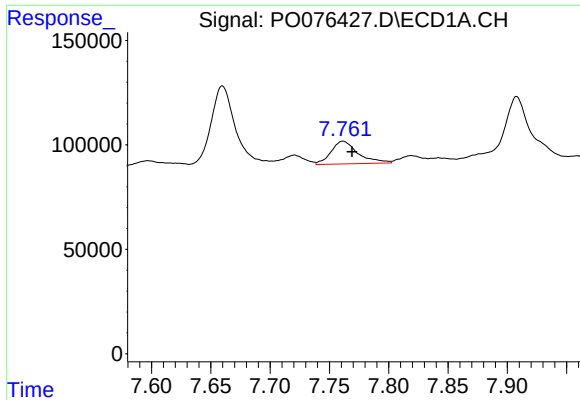


#28 AR-1254-3

R.T.: 7.761 min
Delta R.T.: -0.008 min
Response: 173115
Conc: 54.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:43 PM

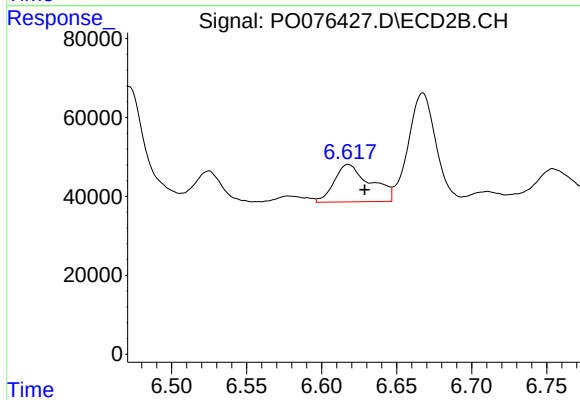


#28 AR-1254-3

R.T.: 6.618 min
Delta R.T.: -0.011 min
Response: 159034
Conc: 52.80 ng/ml

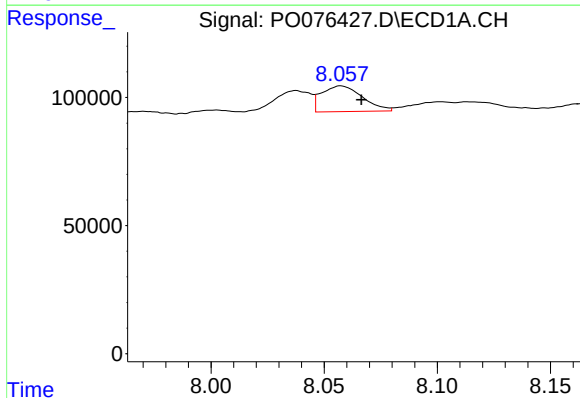


#29 AR-1254-4

R.T.: 8.057 min
Delta R.T.: -0.009 min
Response: 125734
Conc: 60.01 ng/ml

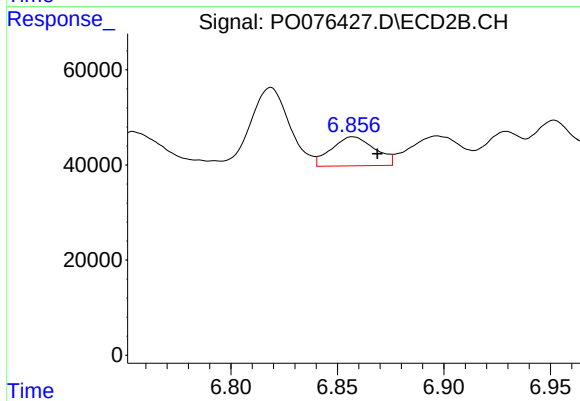

#29 AR-1254-4

R.T.: 6.857 min
Delta R.T.: -0.011 min
Response: 86363
Conc: 48.94 ng/ml

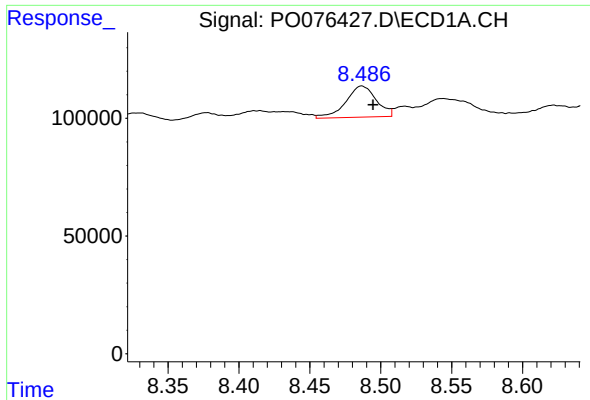


#30 AR-1254-5

R.T.: 8.487 min
Delta R.T.: -0.008 min
Response: 198074
Conc: 86.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C

Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:43 PM

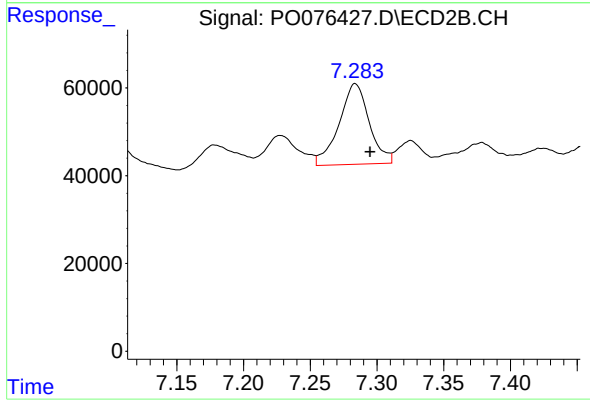

#30 AR-1254-5

R.T.: 7.284 min
Delta R.T.: -0.011 min
Response: 289771
Conc: 110.68 ng/ml