

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076428.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 16:54
 Operator : DD\AJ
 Sample : M1745-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:40:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 00:36:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.917	3.929	1827050	1030525	32.161	24.700
2) SA Decachlor...	10.909	9.191	3386837	1496999	88.053	38.987m#
Target Compounds						
26) L6 AR-1254-1	7.152	6.043	3591411	3256568	1752.419	1424.876
27) L6 AR-1254-2	7.382	6.202	3788381	1850876	1219.088	934.527
28) L6 AR-1254-3	7.764	6.620	2427044	2169159	762.879	720.164
29) L6 AR-1254-4	8.060	6.860	1015744	954074	484.809	540.648
30) L6 AR-1254-5	8.490	7.286	646232	1930214	281.377	737.265 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032221\
Data File : PO076428.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 16:54
Operator : DD\AJ
Sample : M1745-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 00:36:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

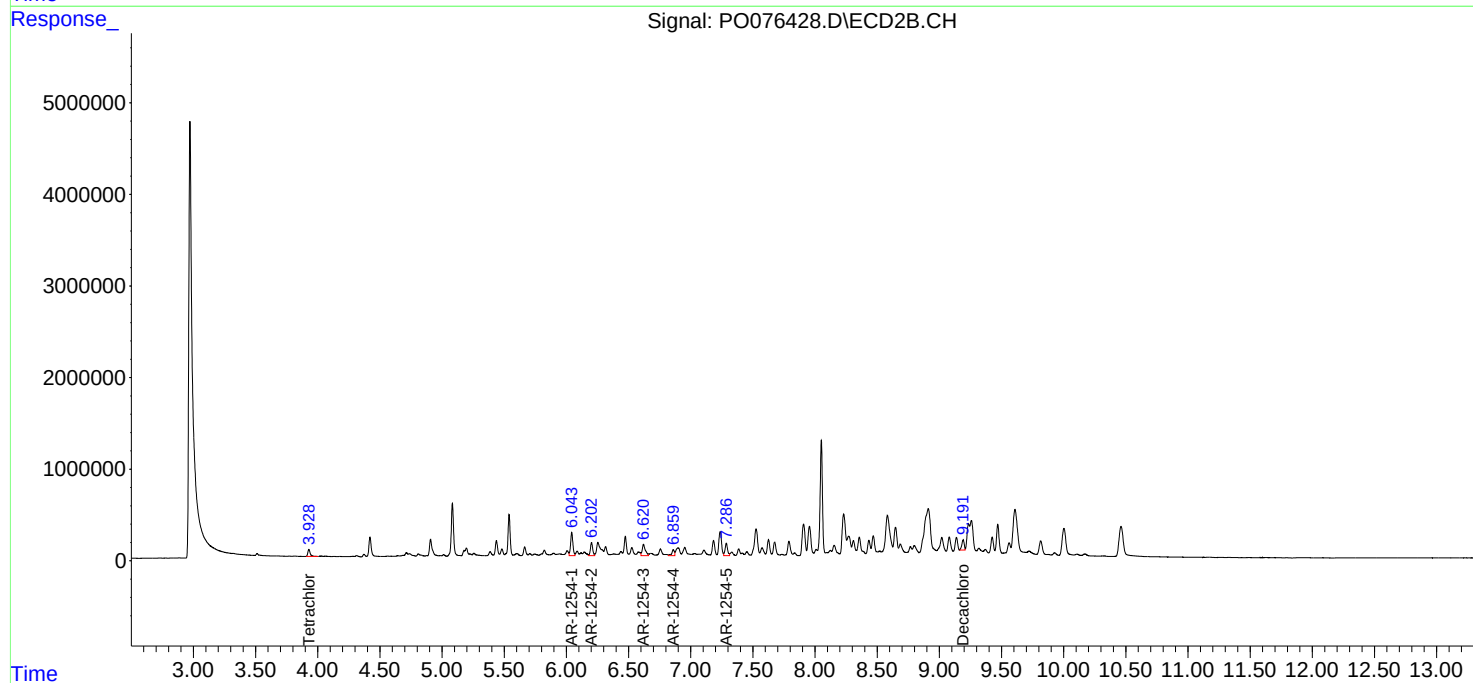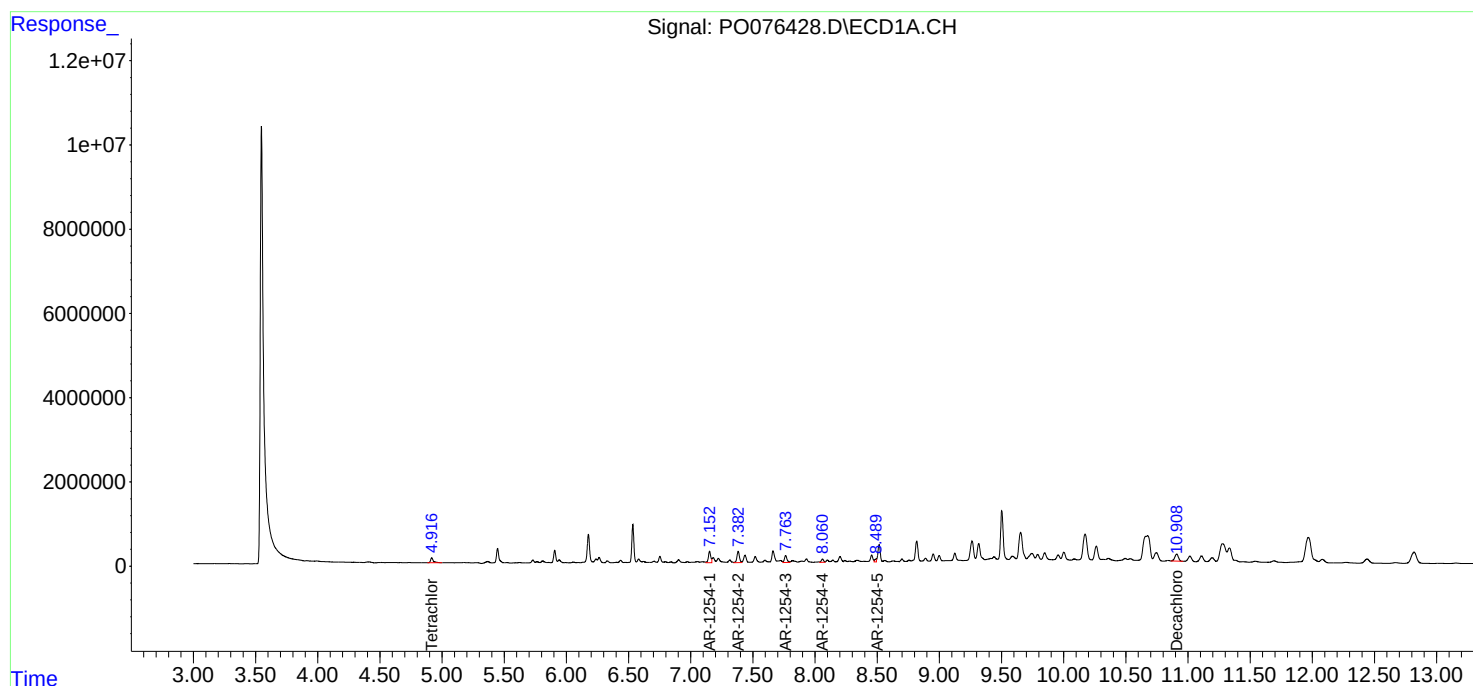

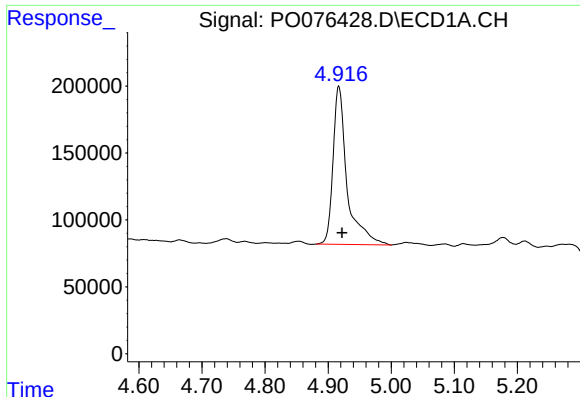


#1 Tetrachloro-m-xylene

R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 1827050
Conc: 32.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:45 PM

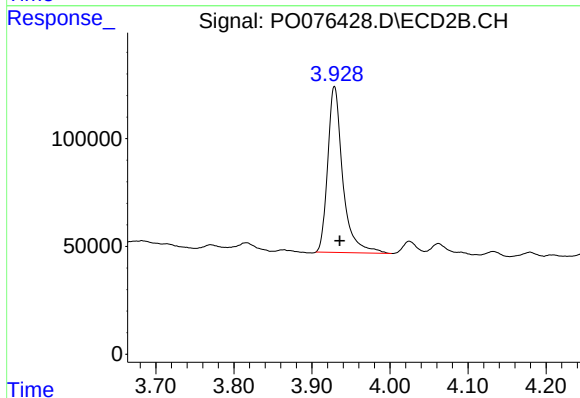


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.007 min
Response: 1030525
Conc: 24.70 ng/ml

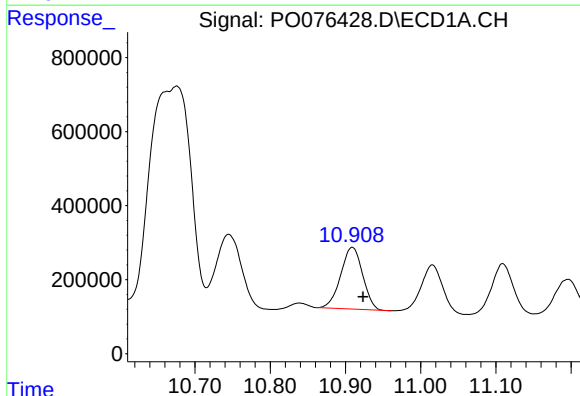


#2 Decachlorobiphenyl

R.T.: 10.909 min
Delta R.T.: -0.015 min
Response: 3386837
Conc: 88.05 ng/ml

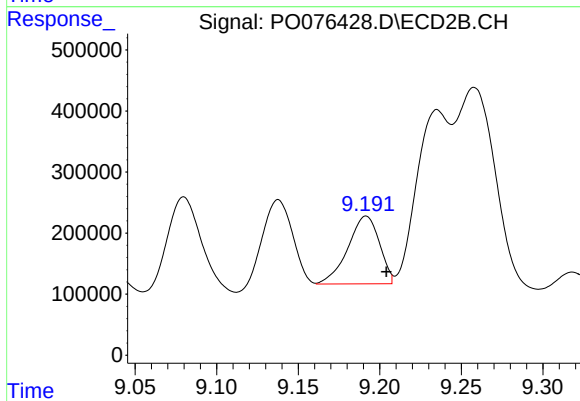

#2 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: -0.013 min
Response: 1496999
Conc: 38.99 ng/ml m

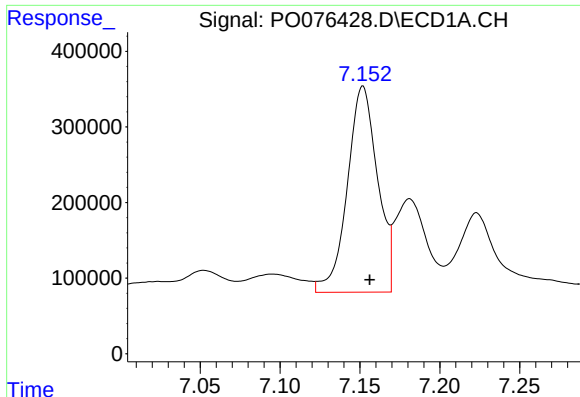


#26 AR-1254-1

R.T.: 7.152 min
Delta R.T.: -0.004 min
Response: 3591411
Conc: 1752.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:45 PM

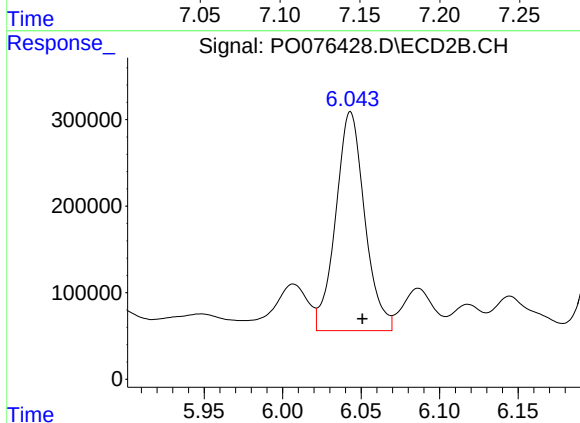


#26 AR-1254-1

R.T.: 6.043 min
Delta R.T.: -0.008 min
Response: 3256568
Conc: 1424.88 ng/ml

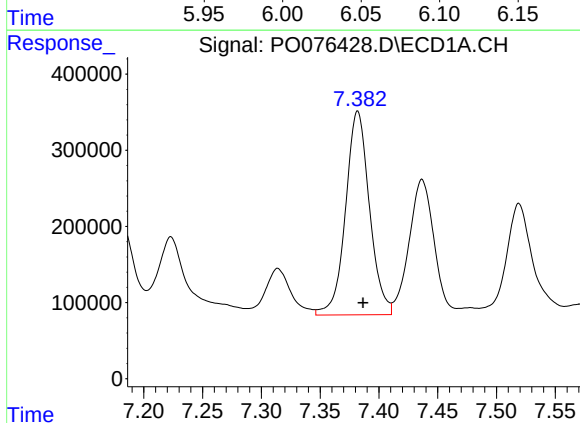


#27 AR-1254-2

R.T.: 7.382 min
Delta R.T.: -0.005 min
Response: 3788381
Conc: 1219.09 ng/ml

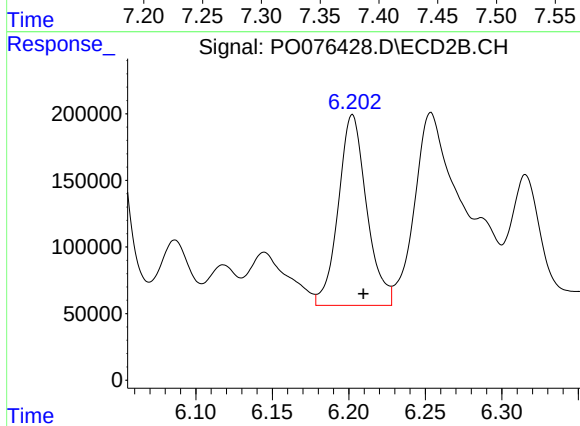

#27 AR-1254-2

R.T.: 6.202 min
Delta R.T.: -0.007 min
Response: 1850876
Conc: 934.53 ng/ml

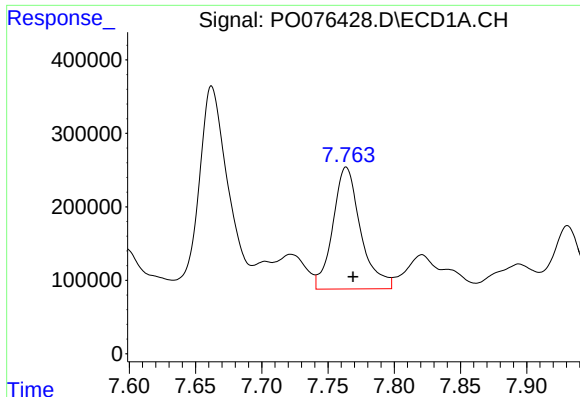


#28 AR-1254-3

R.T.: 7.764 min
Delta R.T.: -0.005 min
Response: 2427044
Conc: 762.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:45 PM

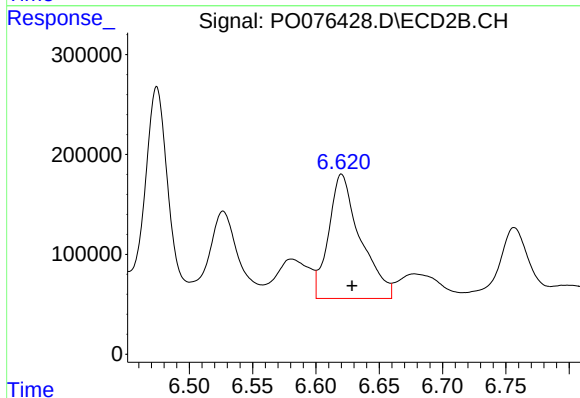


#28 AR-1254-3

R.T.: 6.620 min
Delta R.T.: -0.008 min
Response: 2169159
Conc: 720.16 ng/ml

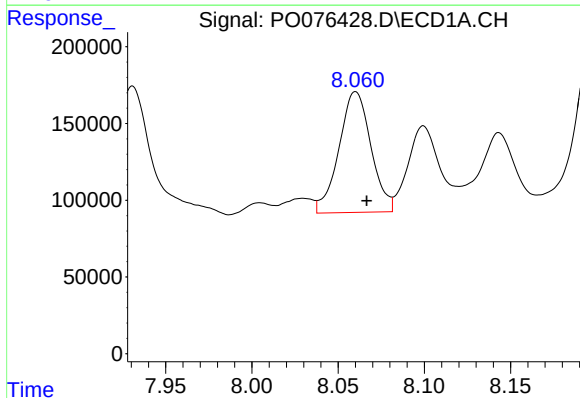


#29 AR-1254-4

R.T.: 8.060 min
Delta R.T.: -0.006 min
Response: 1015744
Conc: 484.81 ng/ml

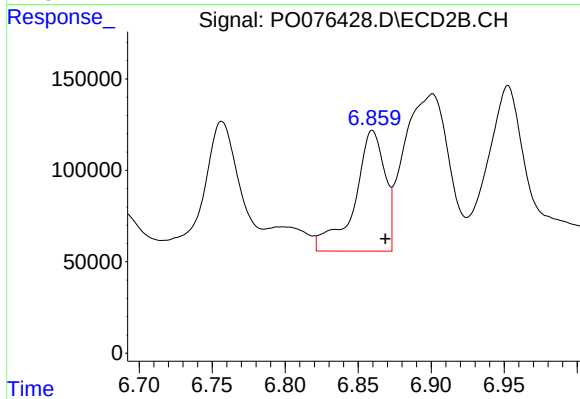

#29 AR-1254-4

R.T.: 6.860 min
Delta R.T.: -0.009 min
Response: 954074
Conc: 540.65 ng/ml

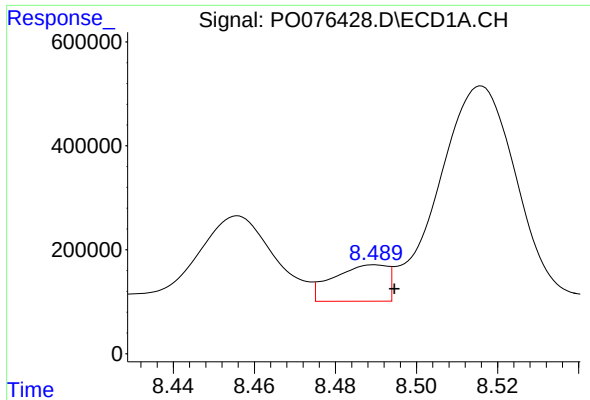


#30 AR-1254-5

R.T.: 8.490 min
Delta R.T.: -0.005 min
Response: 646232
Conc: 281.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C

Manual Integrations
APPROVED

Ankita
3/23/2021 1:40:45 PM

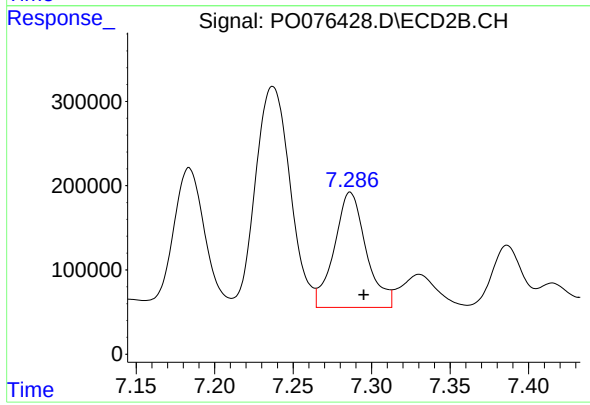

#30 AR-1254-5

R.T.: 7.286 min
Delta R.T.: -0.009 min
Response: 1930214
Conc: 737.27 ng/ml