

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
 Data File : P0076450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2021 23:28
 Operator : DD\AJ
 Sample : M1752-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP2-41720:23-41718

Manual Integrations
 APPROVED

Ankita
 3/23/2021 1:41:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 00:45:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.930	2056574	900624	36.201m	21.587 #
2) SA Decachlor...	10.910	9.190	806936	749043	20.979	19.508

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032221\
Data File : P0076450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2021 23:28
Operator : DD\AJ
Sample : M1752-07
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP2-41720:23-41718


Manual Integrations
APPROVED

Ankita
3/23/2021 1:41:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 00:45:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

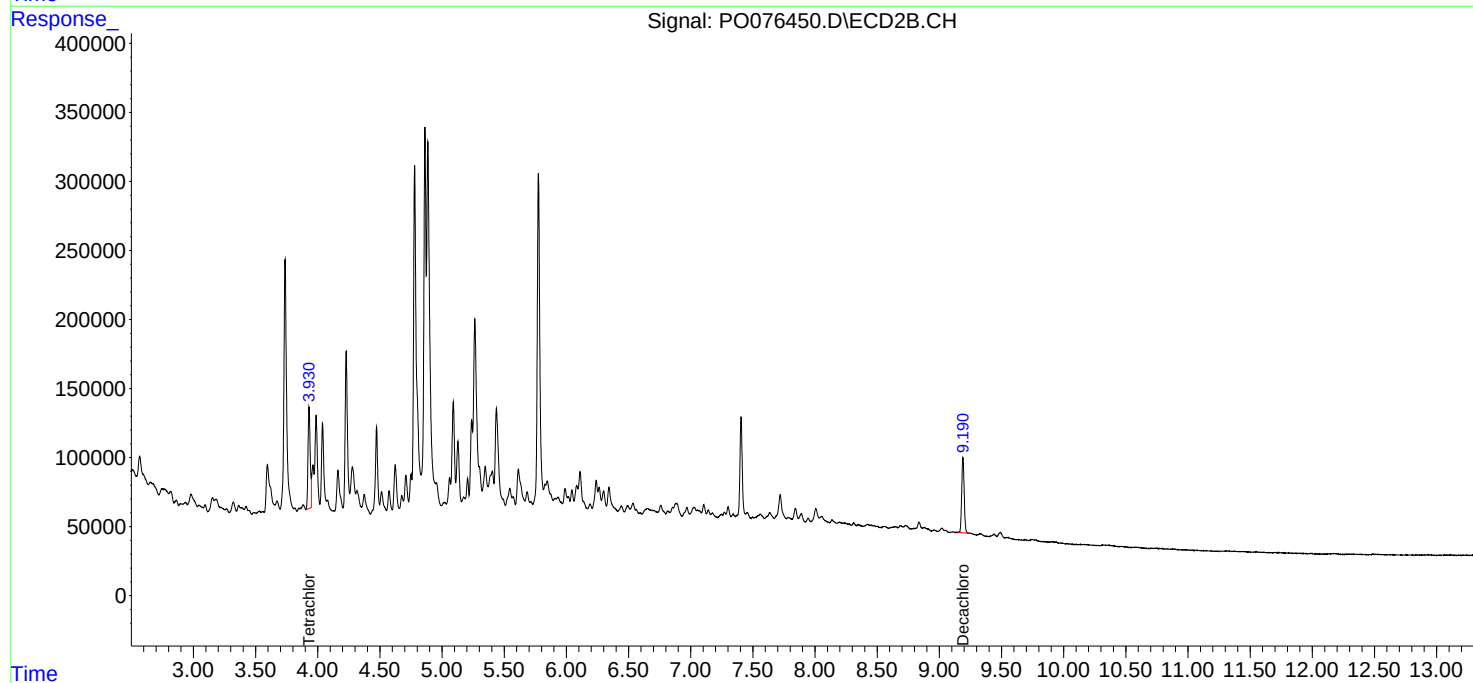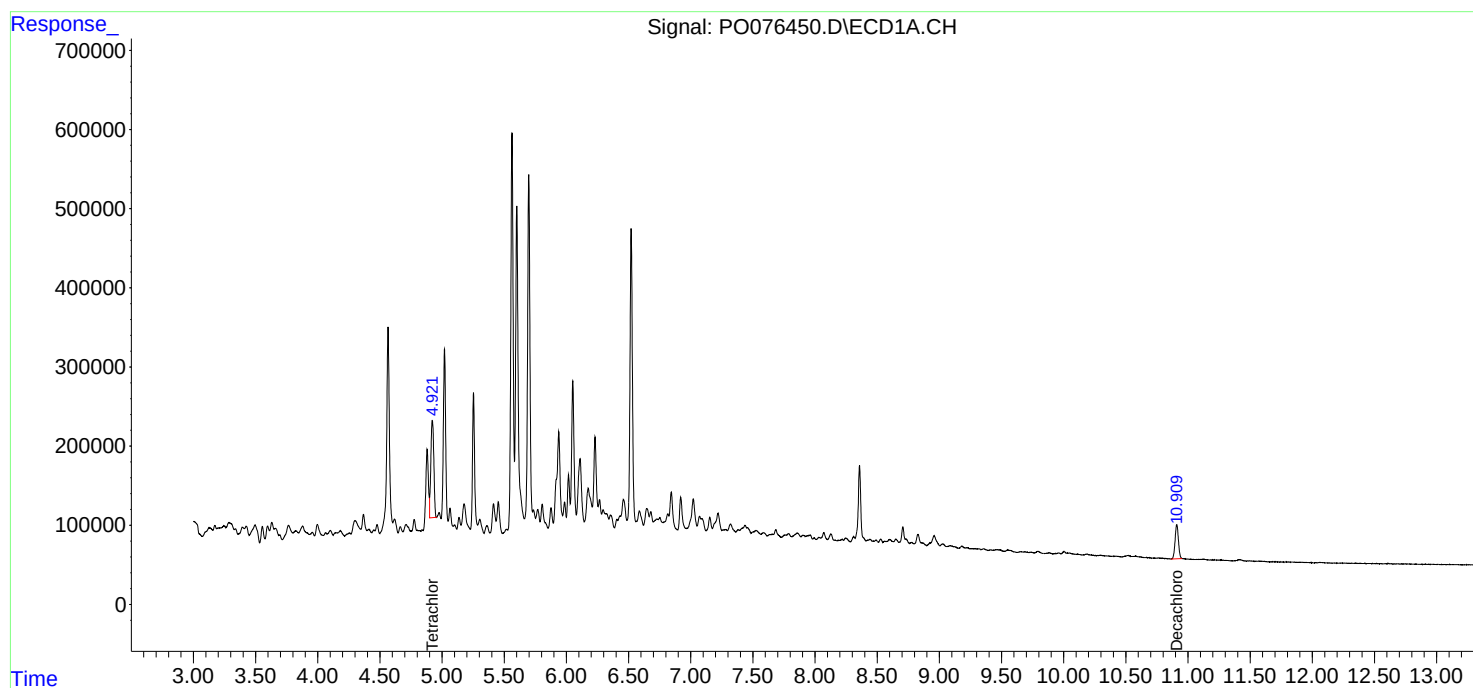

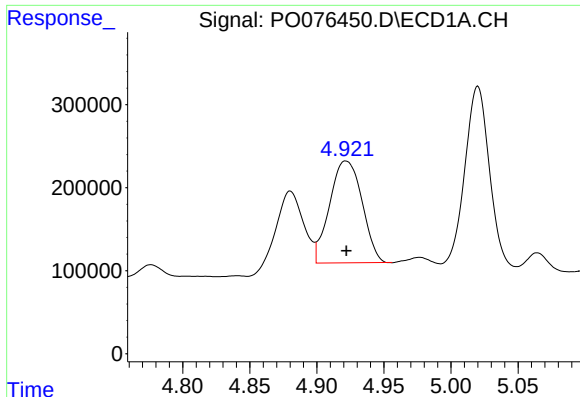


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 2056574
Conc: 36.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP2-41720:23-41718


Manual Integrations
APPROVED

Ankita
3/23/2021 1:41:12 PM

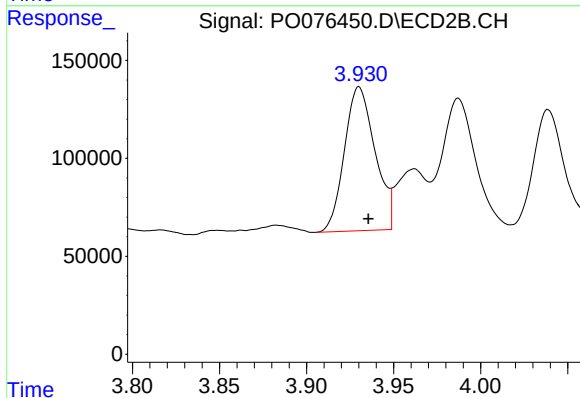


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 900624
Conc: 21.59 ng/ml

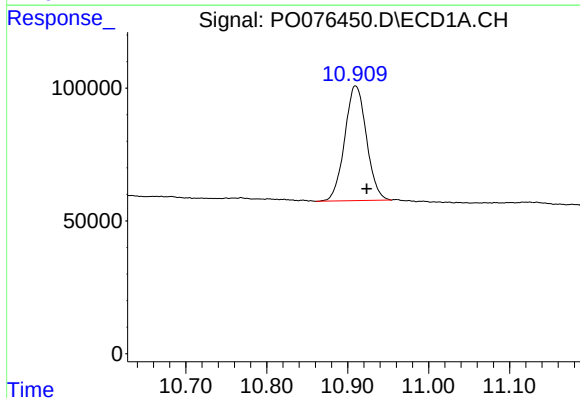

#2 Decachlorobiphenyl

R.T.: 10.910 min
Delta R.T.: -0.014 min
Response: 806936
Conc: 20.98 ng/ml

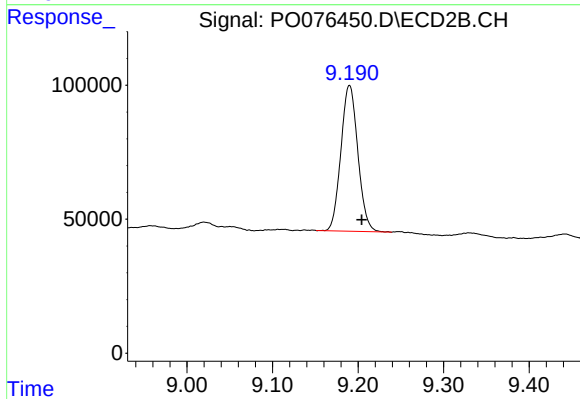

#2 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.014 min
Response: 749043
Conc: 19.51 ng/ml