

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032223\
 Data File : P0093424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 14:53
 Operator : YP/AJ
 Sample : 02023-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-12-TEST-PIT-ON-OCEAN

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:00:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.631	58728811	19066704	18.754	16.905
2) SA Decachlor...	10.254	8.657	32246203	13901248	14.899	14.197

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032223\
Data File : PO093424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 14:53
Operator : YP/AJ
Sample : 02023-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-12-TEST-PIT-ON-OCEAN

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:00:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

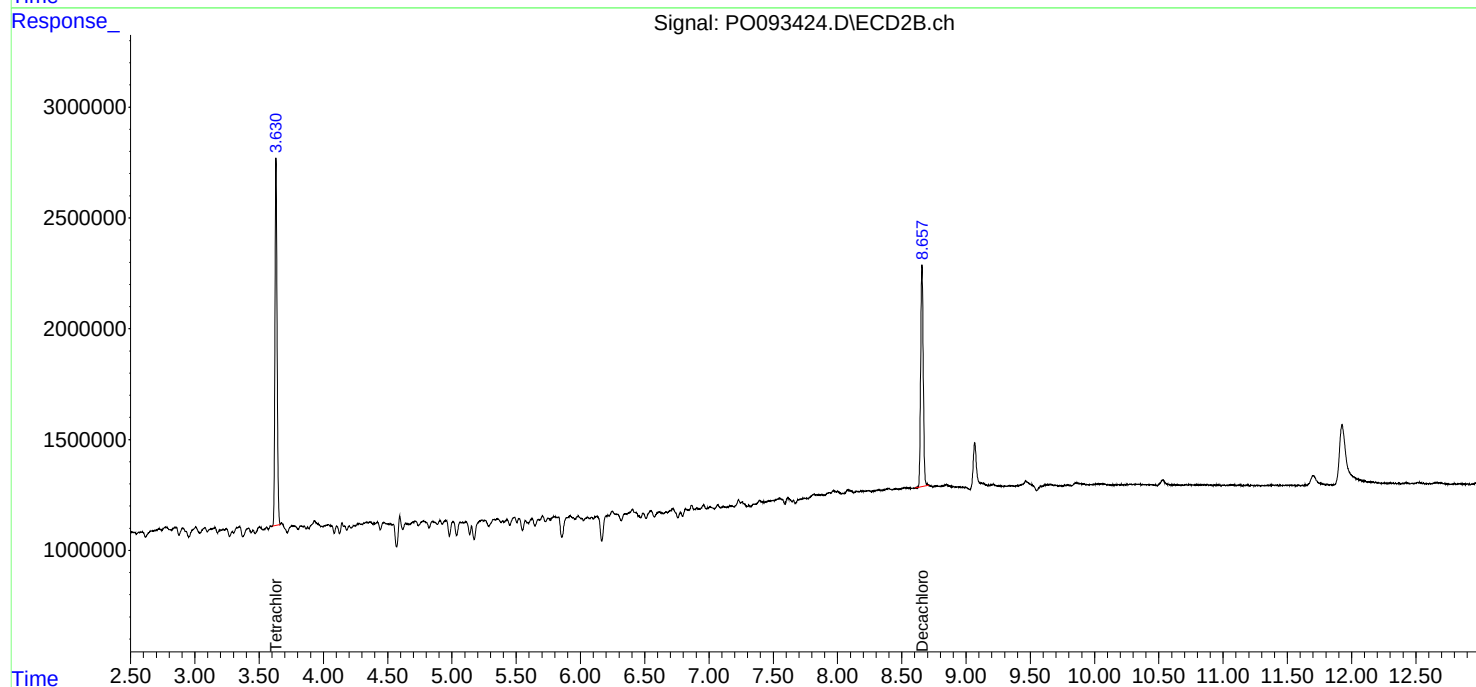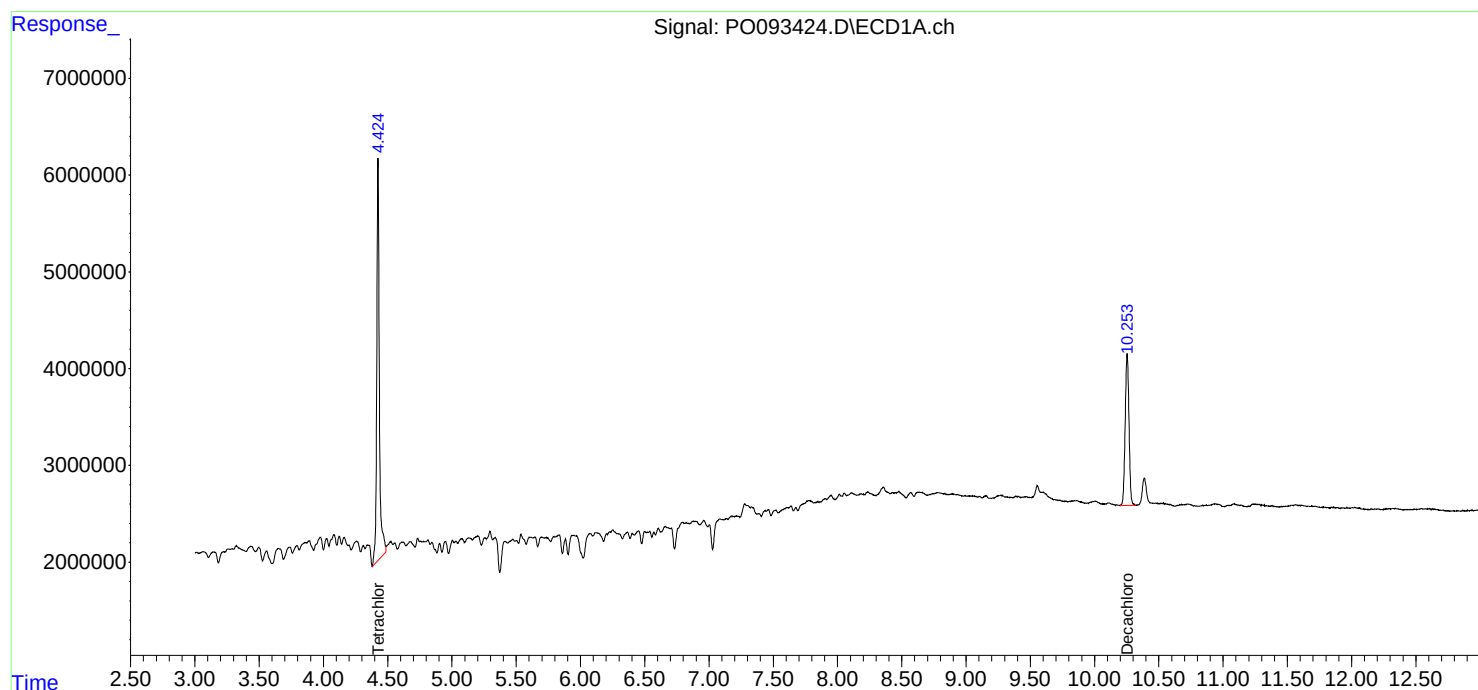


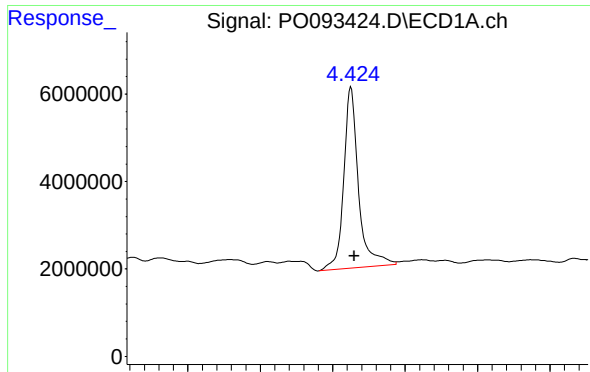

#1 Tetrachloro-m-xylene


R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 58728811
Conc: 18.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-12-TEST-PIT-ON-OCEAN

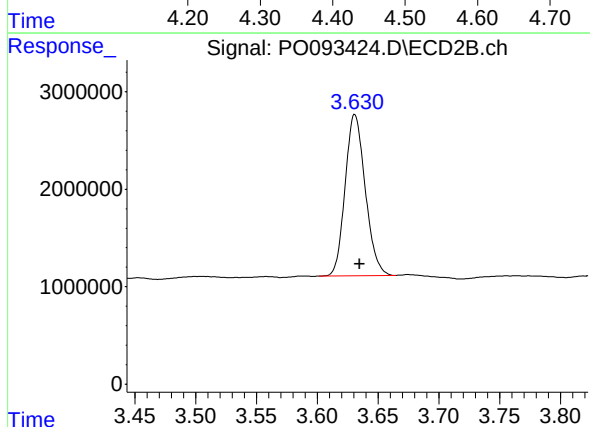


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 19066704
Conc: 16.91 ng/ml

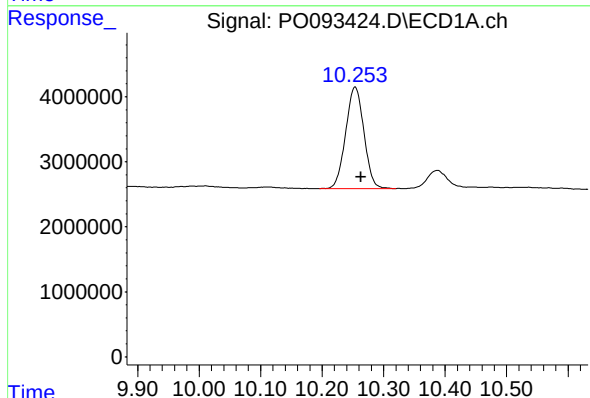

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: -0.010 min
Response: 32246203
Conc: 14.90 ng/ml

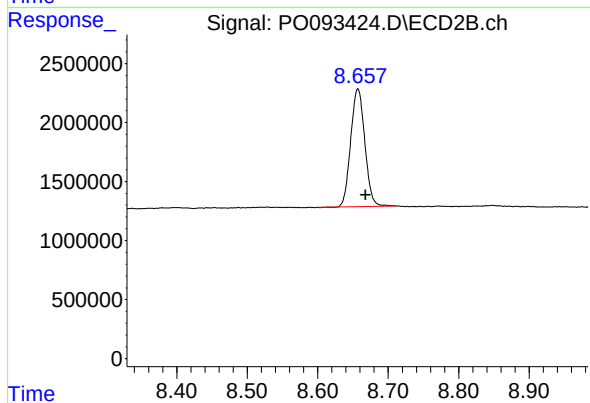

#2 Decachlorobiphenyl

R.T.: 8.657 min
Delta R.T.: -0.011 min
Response: 13901248
Conc: 14.20 ng/ml