

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032223\
 Data File : P0093425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 15:10
 Operator : YP/AJ
 Sample : 02023-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-13-TEST-PIT-ON-GRAVELLY

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:01:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.426	3.631	65692898	24206456	20.978	21.462
2) SA Decachlor...	10.253	8.657	45741429	19597545	21.135	20.015

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032223\
Data File : P0093425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 15:10
Operator : YP/AJ
Sample : 02023-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-13-TEST-PIT-ON-GRAVELLY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:01:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

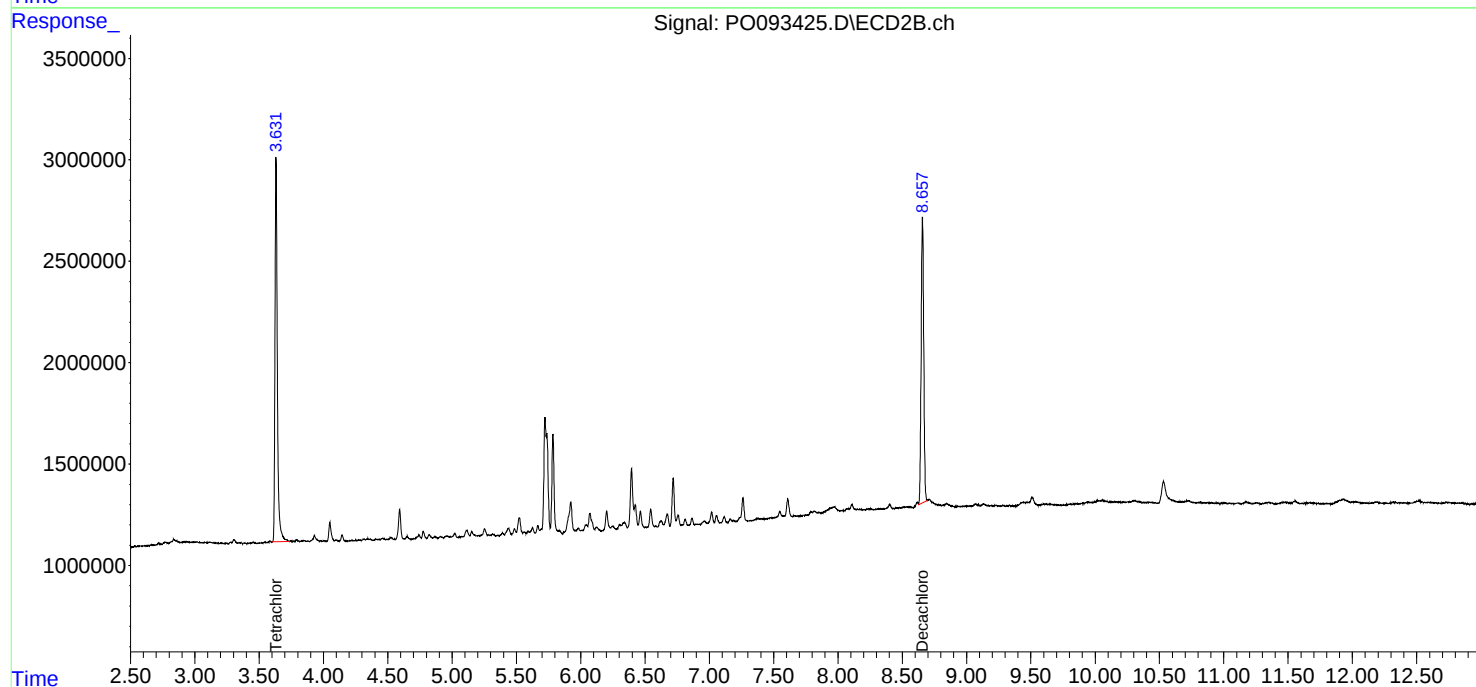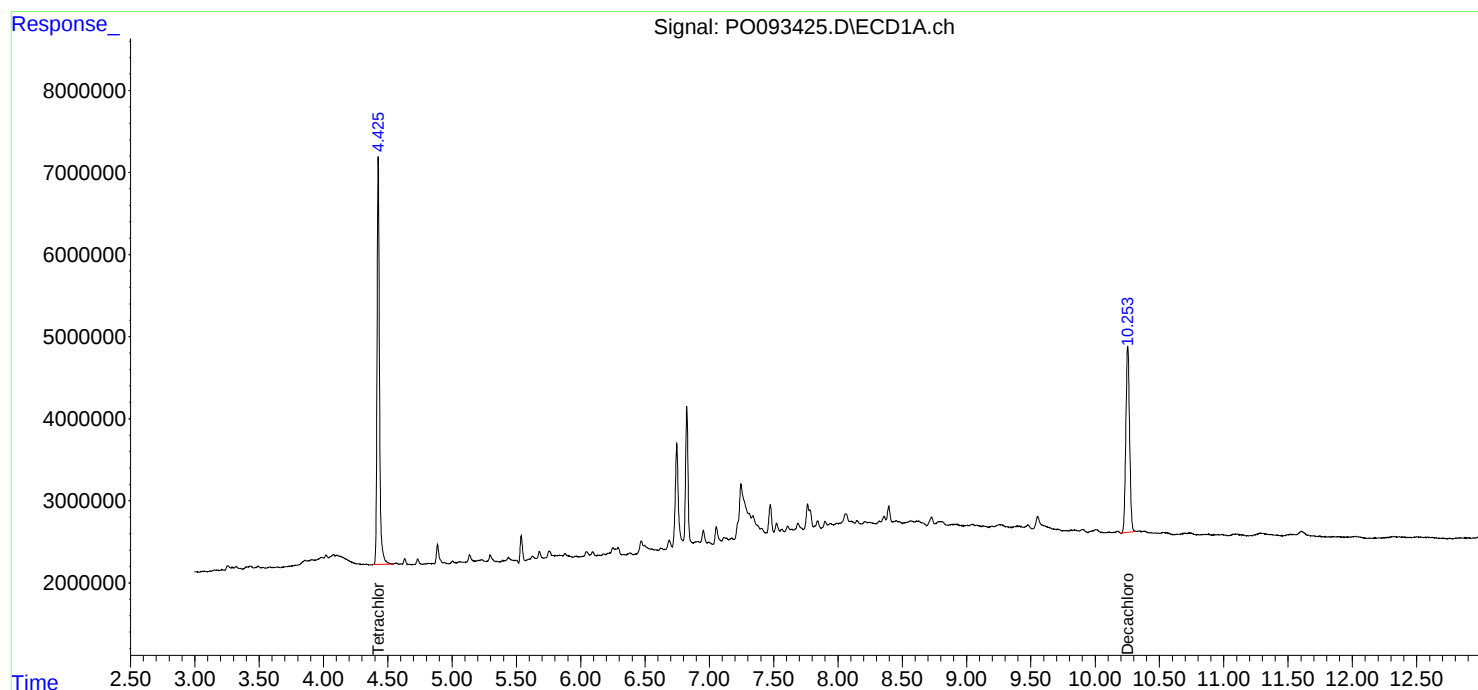


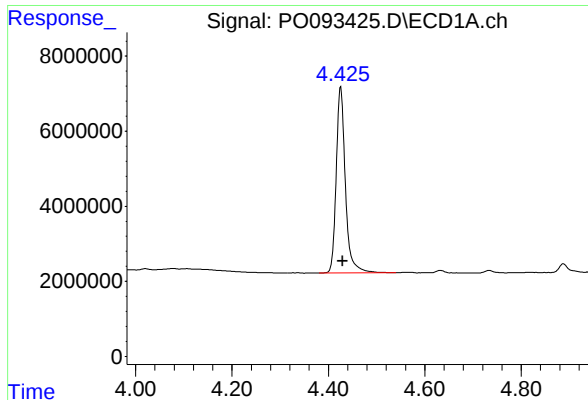

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.004 min
Response: 65692898
Conc: 20.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-13-TEST-PIT-ON-GRAVELLY

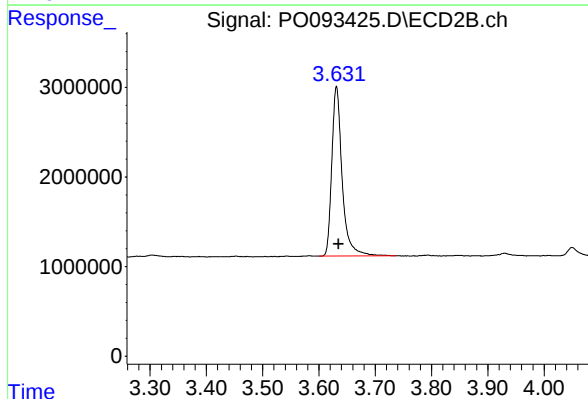


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 24206456
Conc: 21.46 ng/ml

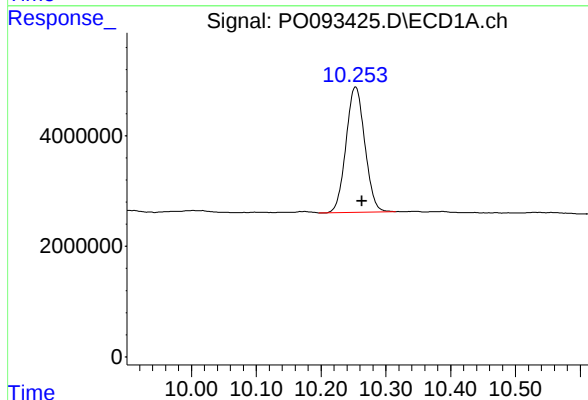

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: -0.010 min
Response: 45741429
Conc: 21.13 ng/ml

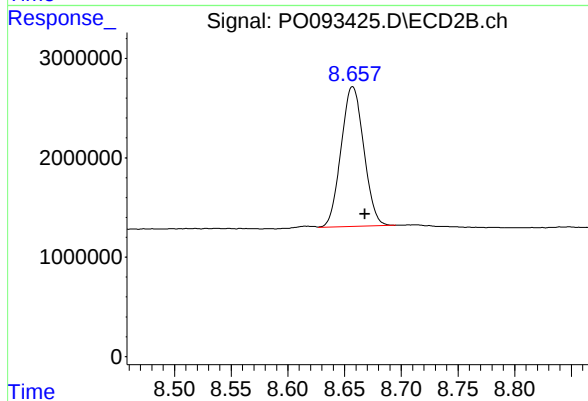

#2 Decachlorobiphenyl

R.T.: 8.657 min
Delta R.T.: -0.011 min
Response: 19597545
Conc: 20.02 ng/ml