

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032223\
 Data File : P0093449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 23:32
 Operator : YP/AJ
 Sample : 02026-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40205

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/23/2023
 Supervised By :Ankita Jodhani 03/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:07:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.424	3.631	55119980	21741664	17.602	19.277
2) SA Decachlor...	10.251	8.655	51847246	21942061	23.956	22.410
Target Compounds						
26) L6 AR-1254-1	6.462	5.509	486007	808229	4.159	12.877m#
27) L6 AR-1254-2	6.683	5.666	7921341	1096311	46.359m	19.455 #
28) L6 AR-1254-3	7.053	6.070	8357655	4119030	50.275	47.843m
29) L6 AR-1254-4	7.340	6.300	15372061	6330851	144.205	138.437
30) L6 AR-1254-5	7.763	6.718	25848813	13121604	190.895	177.674

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032223\
Data File : PO093449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 23:32
Operator : YP/AJ
Sample : 02026-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/23/2023
Supervised By :Ankita Jodhani 03/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:07:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

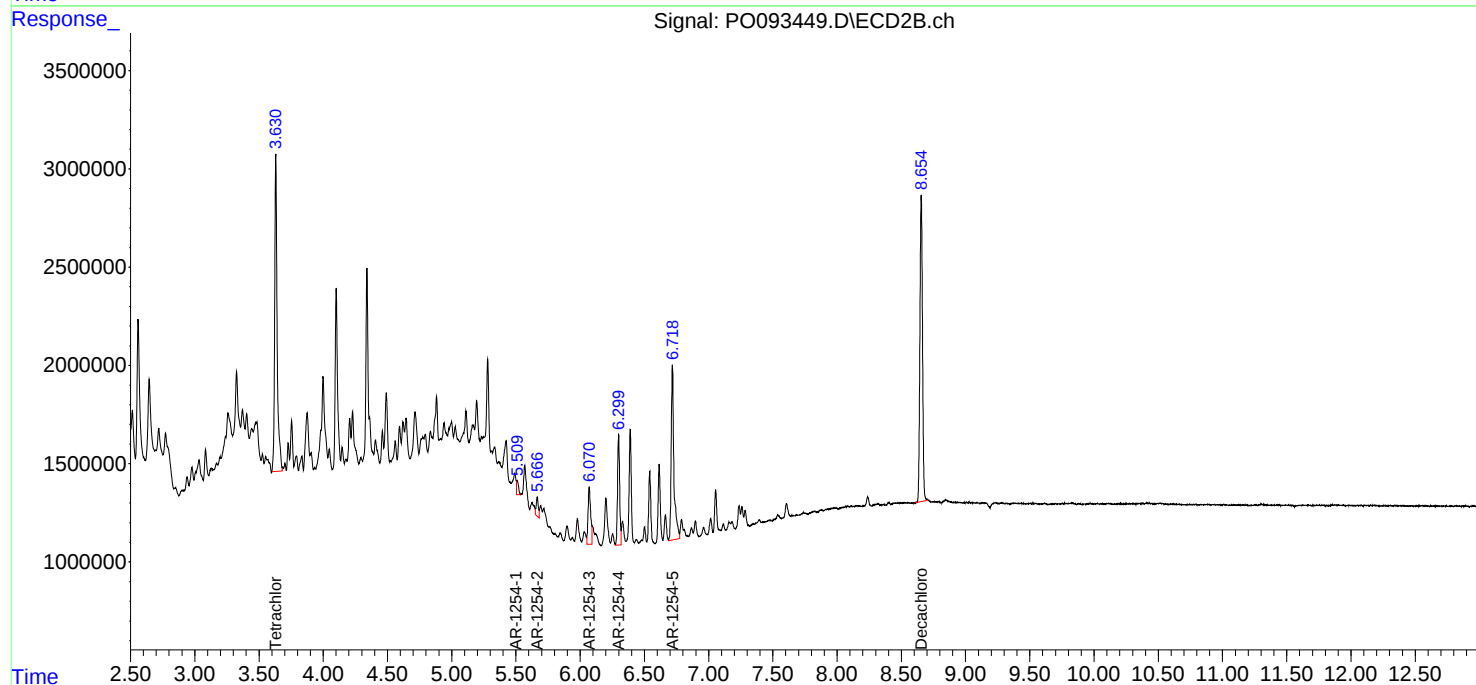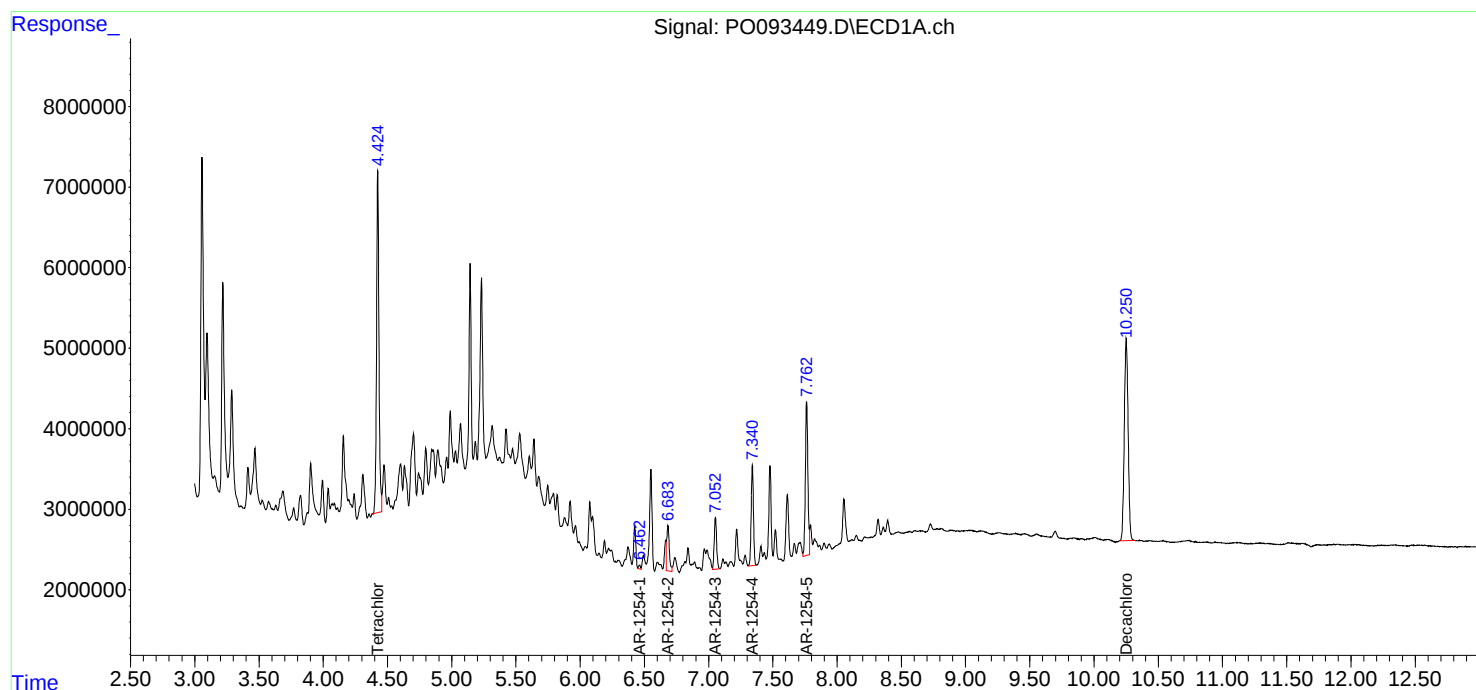

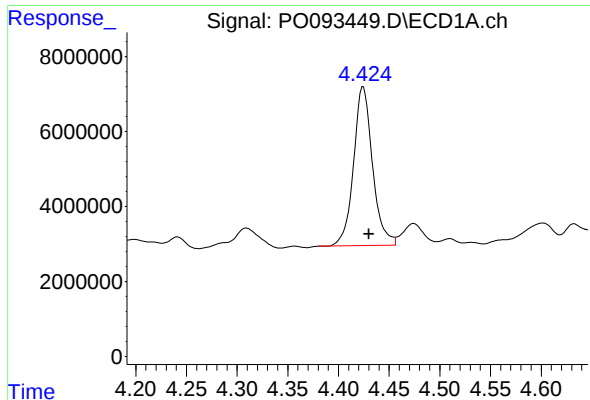


#1 Tetrachloro-m-xylene

R.T.: 4.424 min
Delta R.T.: -0.006 min
Response: 55119980
Conc: 17.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
40205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/23/2023
Supervised By :Ankita Jodhani 03/23/2023

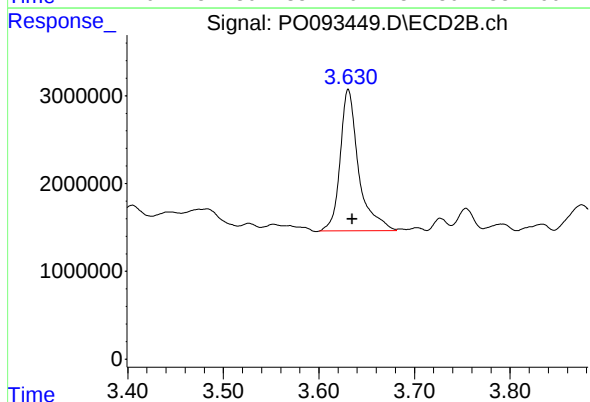


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 21741664
Conc: 19.28 ng/ml

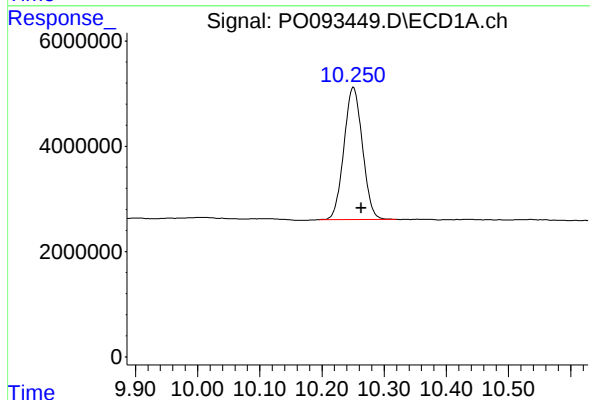


#2 Decachlorobiphenyl

R.T.: 10.251 min
Delta R.T.: -0.013 min
Response: 51847246
Conc: 23.96 ng/ml

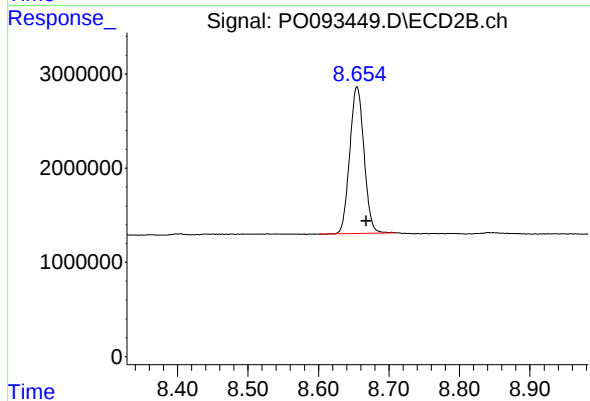

#2 Decachlorobiphenyl

R.T.: 8.655 min
Delta R.T.: -0.013 min
Response: 21942061
Conc: 22.41 ng/ml

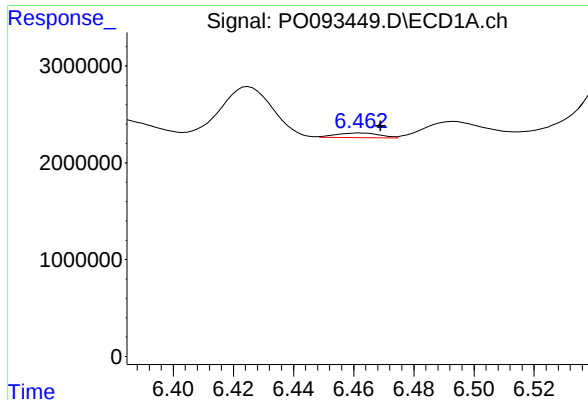


#26 AR-1254-1

R.T.: 6.462 min
Delta R.T.: -0.007 min
Response: 486007
Conc: 4.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
40205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/23/2023
Supervised By :Ankita Jodhani 03/23/2023

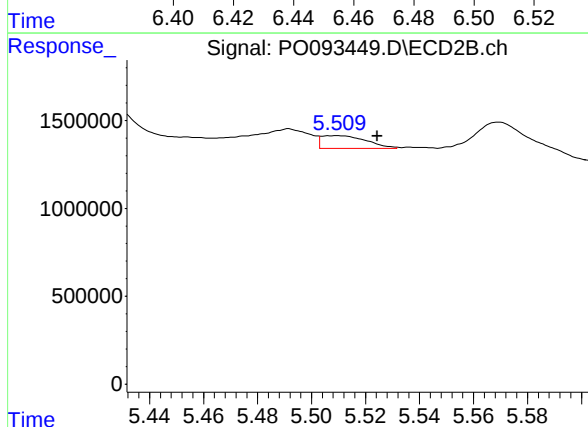


#26 AR-1254-1

R.T.: 5.509 min
Delta R.T.: -0.015 min
Response: 808229
Conc: 12.88 ng/ml

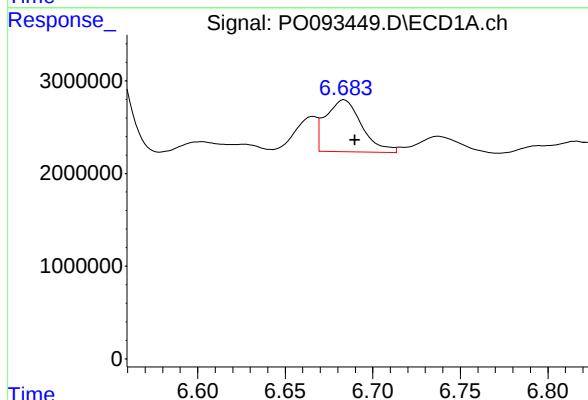


#27 AR-1254-2

R.T.: 6.683 min
Delta R.T.: -0.007 min
Response: 7921341
Conc: 46.36 ng/ml

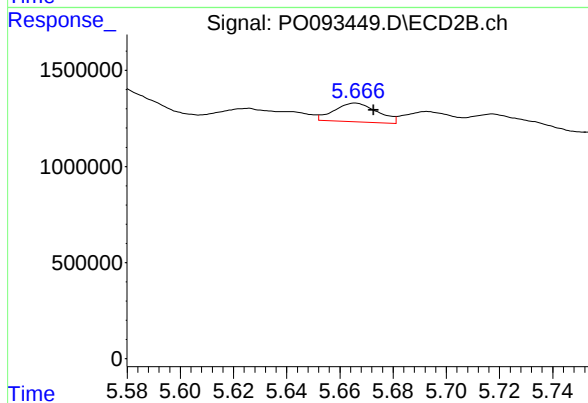

#27 AR-1254-2

R.T.: 5.666 min
Delta R.T.: -0.007 min
Response: 1096311
Conc: 19.45 ng/ml

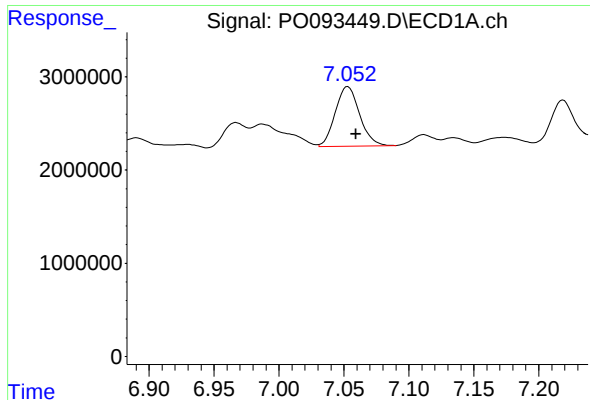


#28 AR-1254-3

R.T.: 7.053 min
Delta R.T.: -0.006 min
Response: 8357655
Conc: 50.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
40205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/23/2023
Supervised By :Ankita Jodhani 03/23/2023

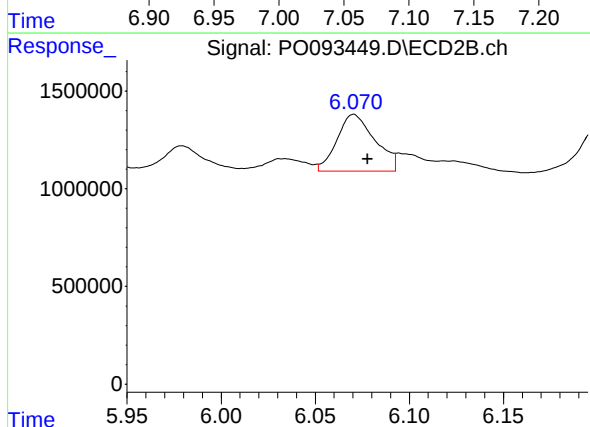


#28 AR-1254-3

R.T.: 6.070 min
Delta R.T.: -0.008 min
Response: 4119030
Conc: 47.84 ng/ml

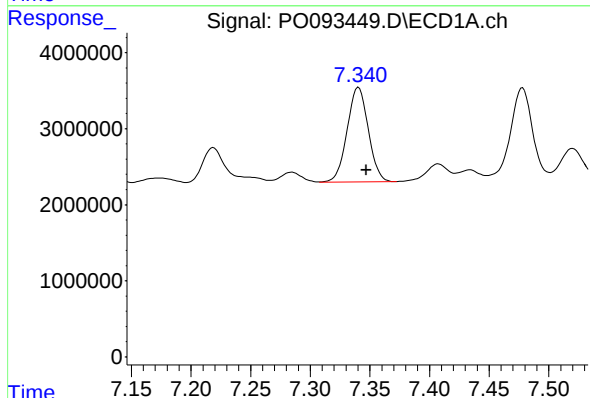


#29 AR-1254-4

R.T.: 7.340 min
Delta R.T.: -0.007 min
Response: 15372061
Conc: 144.21 ng/ml

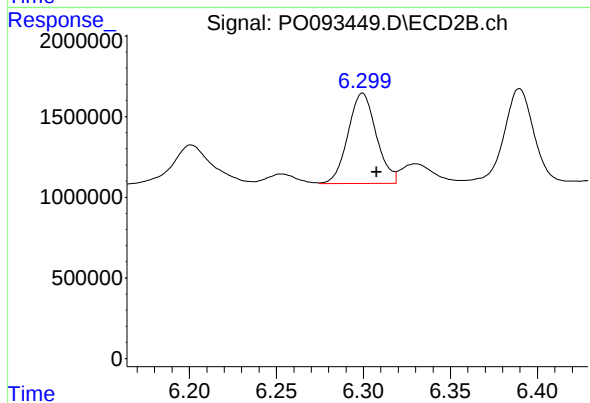

#29 AR-1254-4

R.T.: 6.300 min
Delta R.T.: -0.008 min
Response: 6330851
Conc: 138.44 ng/ml

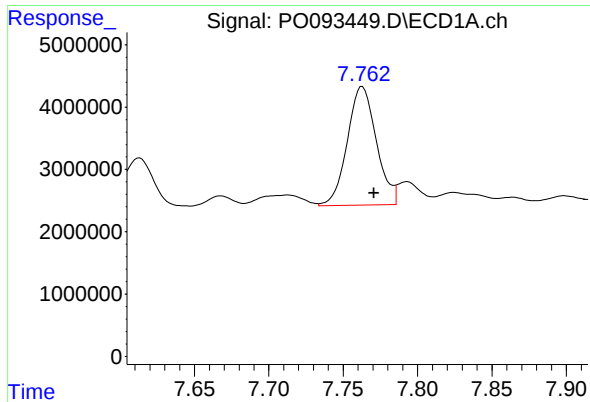


#30 AR-1254-5

R.T.: 7.763 min
Delta R.T.: -0.008 min
Response: 25848813
Conc: 190.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
40205

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/23/2023
Supervised By :Ankita Jodhani 03/23/2023

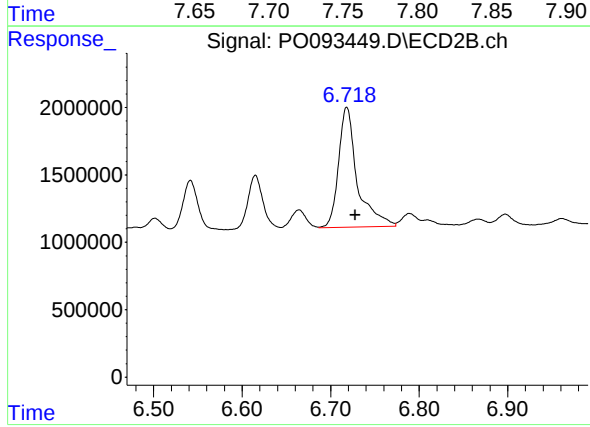

#30 AR-1254-5

R.T.: 6.718 min
Delta R.T.: -0.010 min
Response: 13121604
Conc: 177.67 ng/ml