

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032321\
 Data File : P0076457.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:00
 Operator : DD\AJ
 Sample : M1745-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-CRE

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:18:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 14:32:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.916	3.928	1879988	1055829	33.093	25.307
2) SA Decachlor...	10.904	9.188	3445968	1509246	89.590m	39.306m#
Target Compounds						
26) L6 AR-1254-1	7.150	6.041	3632842	3334053	1772.636	1458.778
27) L6 AR-1254-2	7.380	6.200	4049149	1893216	1303.002	955.905 #
28) L6 AR-1254-3	7.762	6.618	2821028	2253045	886.717	748.014
29) L6 AR-1254-4	8.057	6.858	1235134	995808	589.522	564.297
30) L6 AR-1254-5	8.485	7.284	777525	2060415	338.544m	786.997 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032321\
Data File : PO076457.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:00
Operator : DD\AJ
Sample : M1745-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 14:32:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

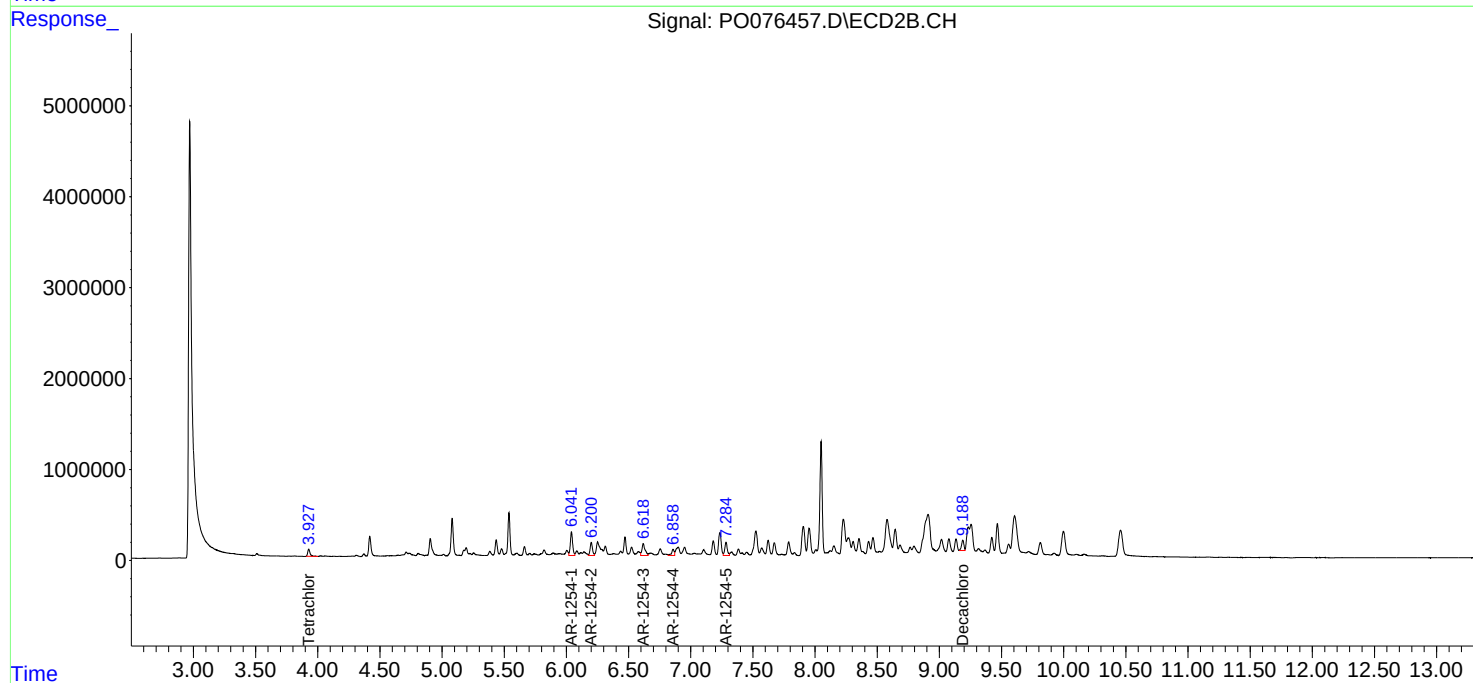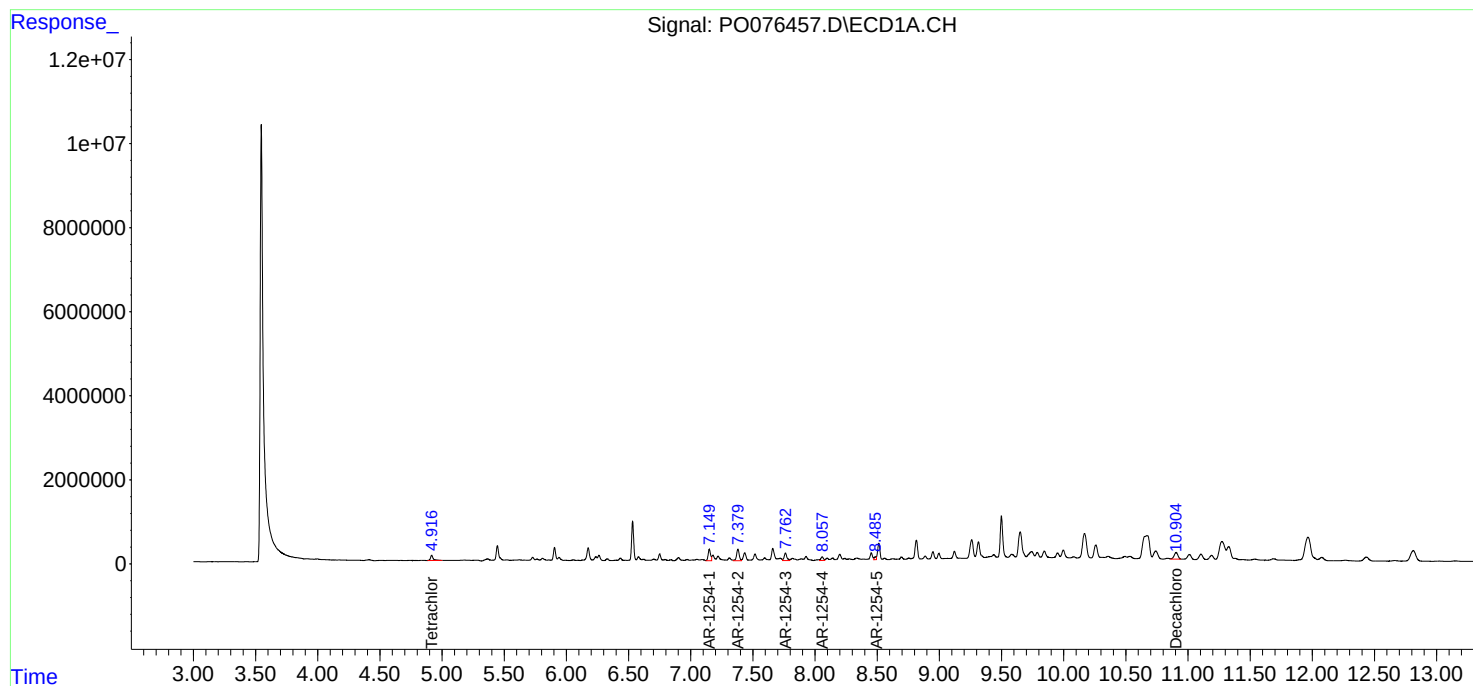

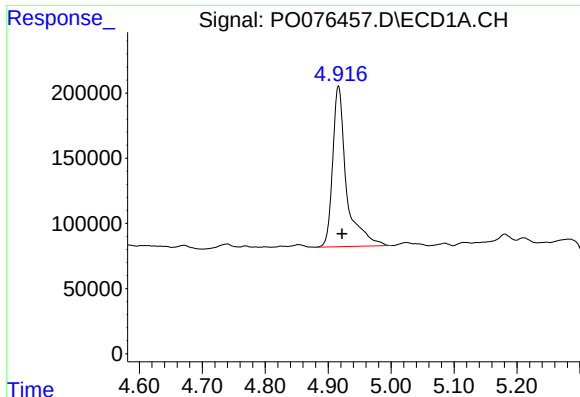


#1 Tetrachloro-m-xylene

R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 1879988
Conc: 33.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:19 PM

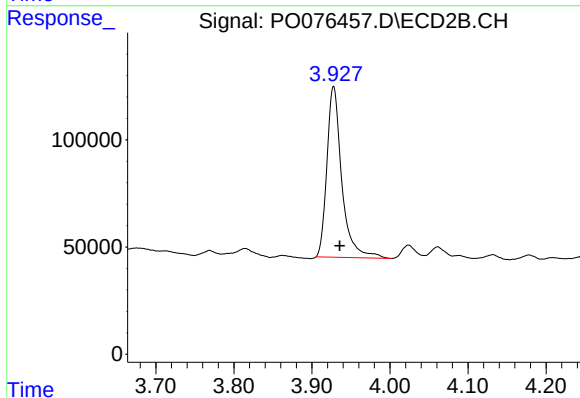


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.008 min
Response: 1055829
Conc: 25.31 ng/ml

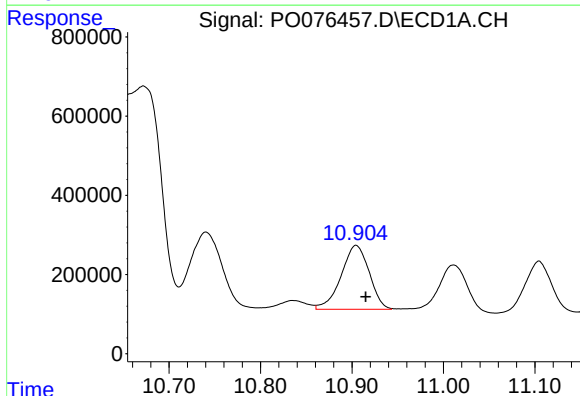


#2 Decachlorobiphenyl

R.T.: 10.904 min
Delta R.T.: -0.011 min
Response: 3445968
Conc: 89.59 ng/ml m

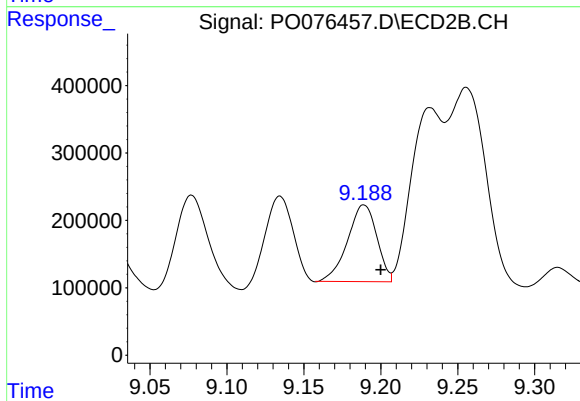

#2 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: -0.012 min
Response: 1509246
Conc: 39.31 ng/ml m

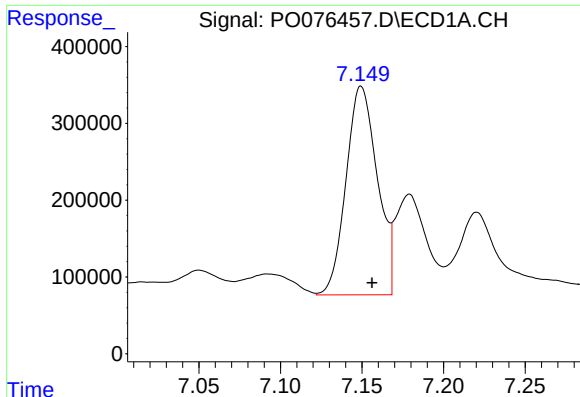


#26 AR-1254-1

R.T.: 7.150 min
Delta R.T.: -0.007 min
Response: 3632842
Conc: 1772.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:19 PM

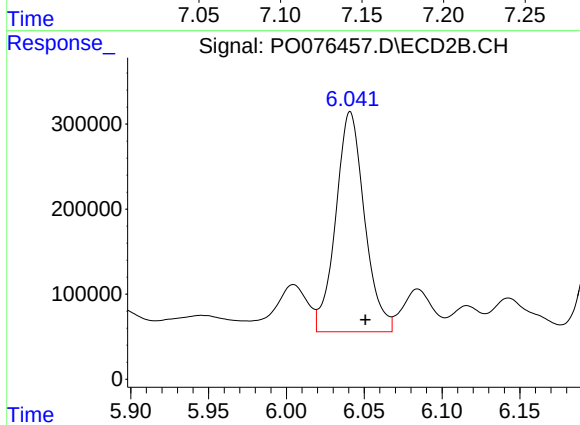


#26 AR-1254-1

R.T.: 6.041 min
Delta R.T.: -0.010 min
Response: 3334053
Conc: 1458.78 ng/ml

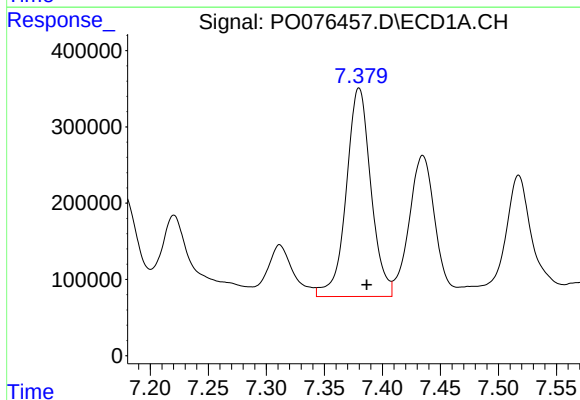


#27 AR-1254-2

R.T.: 7.380 min
Delta R.T.: -0.007 min
Response: 4049149
Conc: 1303.00 ng/ml

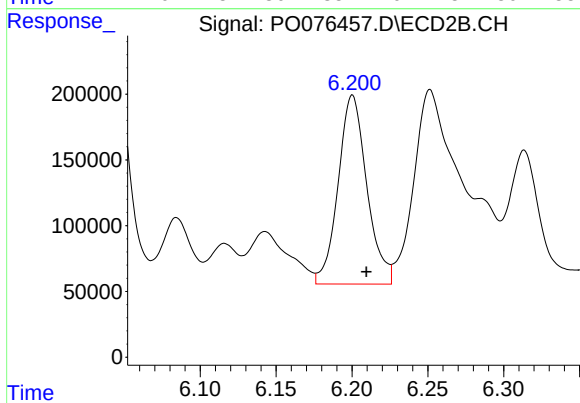

#27 AR-1254-2

R.T.: 6.200 min
Delta R.T.: -0.009 min
Response: 1893216
Conc: 955.90 ng/ml

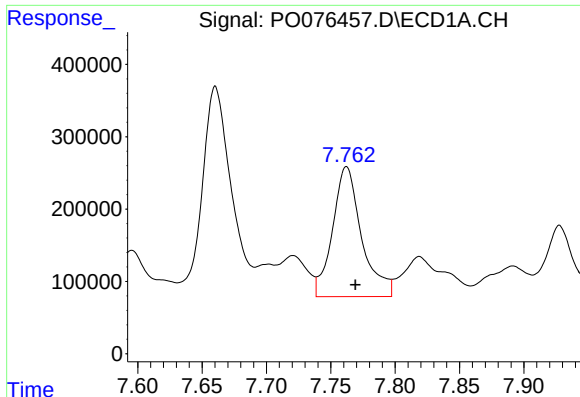


#28 AR-1254-3

R.T.: 7.762 min
Delta R.T.: -0.007 min
Response: 2821028
Conc: 886.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:19 PM

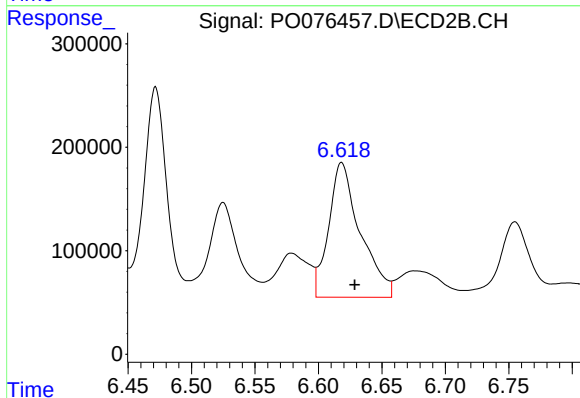


#28 AR-1254-3

R.T.: 6.618 min
Delta R.T.: -0.010 min
Response: 2253045
Conc: 748.01 ng/ml

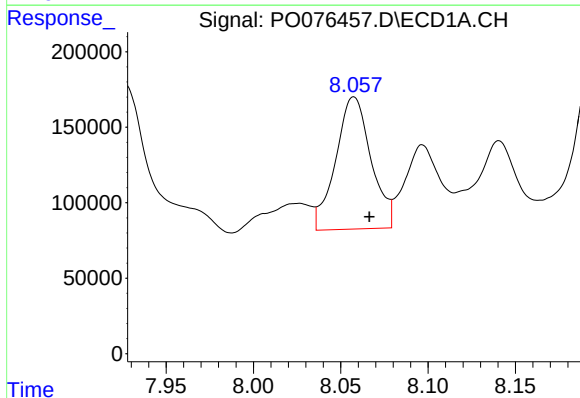


#29 AR-1254-4

R.T.: 8.057 min
Delta R.T.: -0.009 min
Response: 1235134
Conc: 589.52 ng/ml

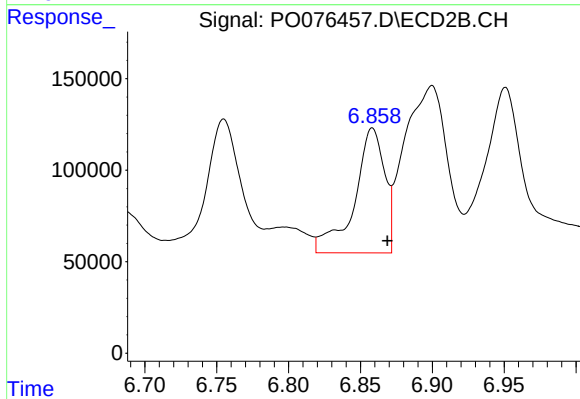

#29 AR-1254-4

R.T.: 6.858 min
Delta R.T.: -0.010 min
Response: 995808
Conc: 564.30 ng/ml

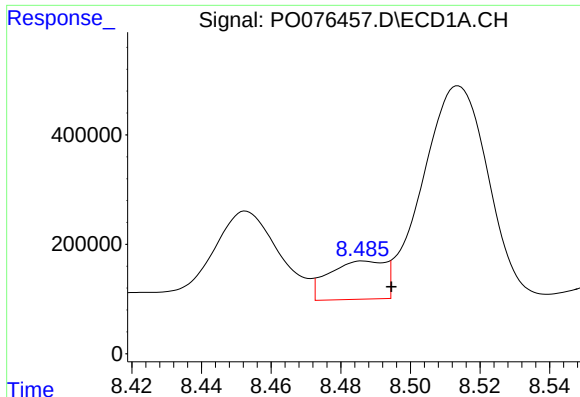


#30 AR-1254-5

R.T.: 8.485 min
Delta R.T.: -0.009 min
Response: 777525
Conc: 338.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE

Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:19 PM

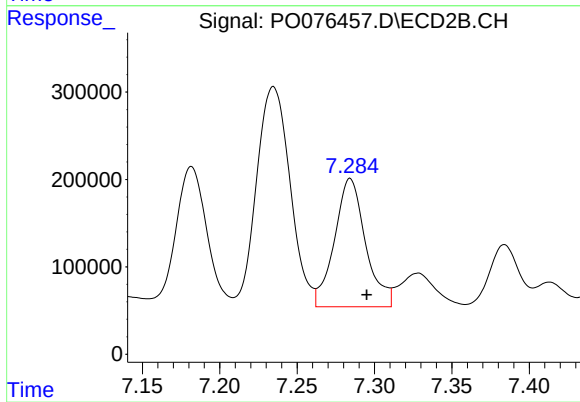

#30 AR-1254-5

R.T.: 7.284 min
Delta R.T.: -0.011 min
Response: 2060415
Conc: 787.00 ng/ml