

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032321\
 Data File : P0076458.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:17
 Operator : DD\AJ
 Sample : M1745-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:18:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 13:21:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.917	3.930	1084613	1324455	19.092	31.745 #
2) SA Decachlor...	10.912	9.191	967428	904472	25.152	23.555m
Target Compounds						
26) L6 AR-1254-1	7.151	6.042	656424	751421	320.300	328.776
27) L6 AR-1254-2	7.382	6.201	658239	378248	211.819	190.982
28) L6 AR-1254-3	7.763	6.625	606788	943562	190.728	313.264 #
29) L6 AR-1254-4	8.060	6.861	315359	244880	150.519	138.767
30) L6 AR-1254-5	8.488	7.286	455619	473202	198.382	180.745

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032321\
Data File : P0076458.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:17
Operator : DD\AJ
Sample : M1745-02
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 13:21:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

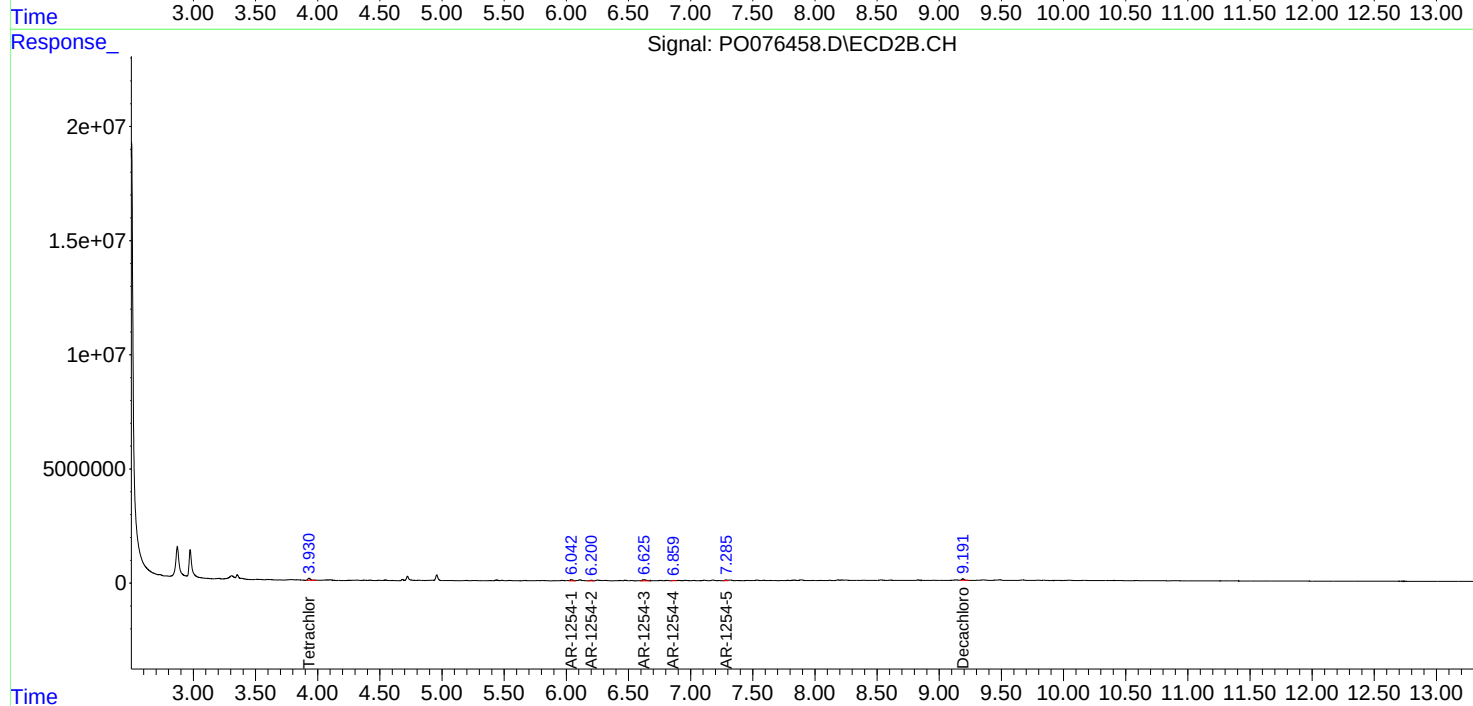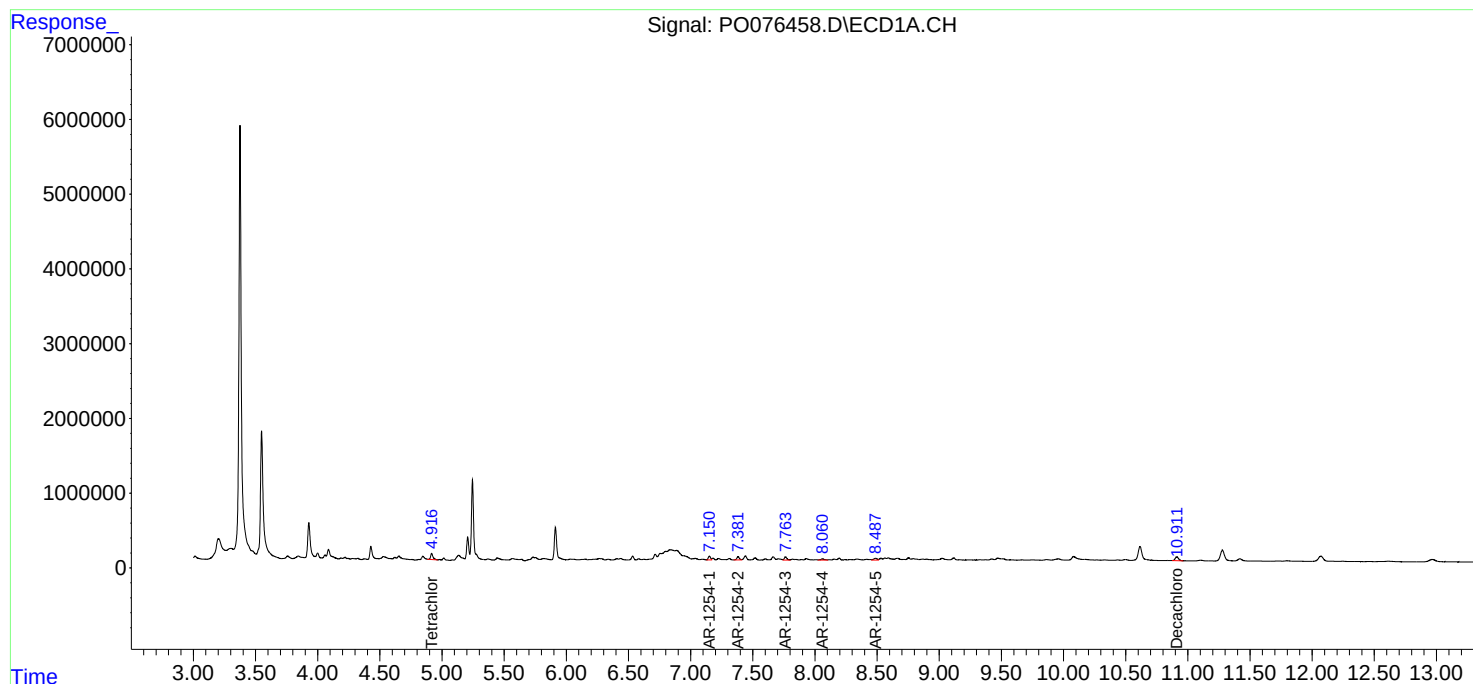

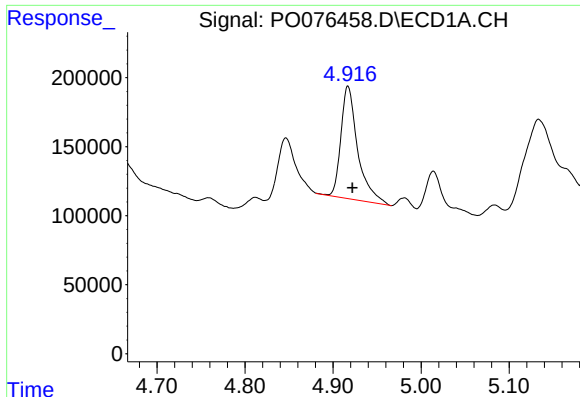


#1 Tetrachloro-m-xylene

R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 1084613
Conc: 19.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:21 PM

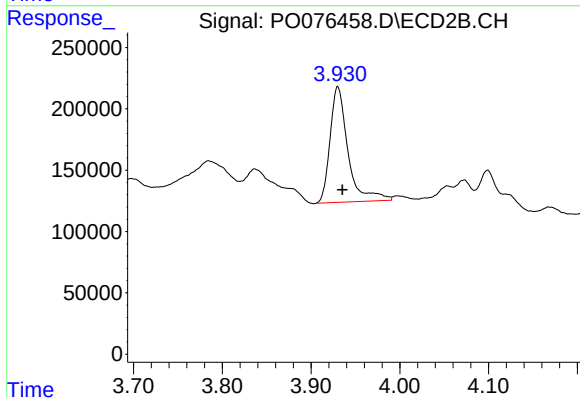


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 1324455
Conc: 31.75 ng/ml

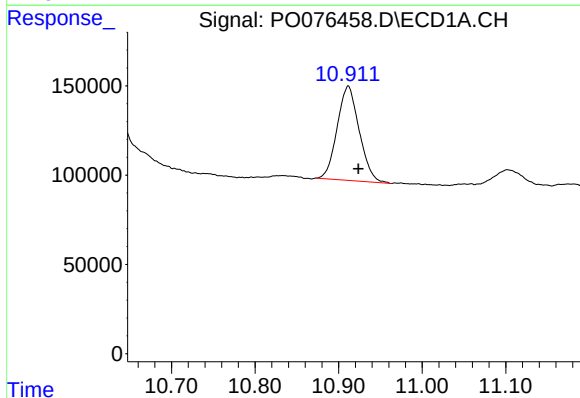


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.012 min
Response: 967428
Conc: 25.15 ng/ml

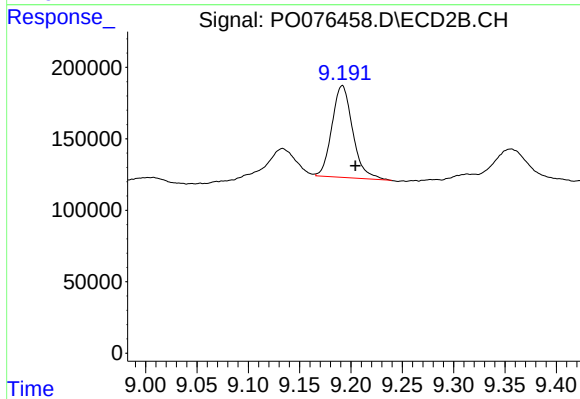

#2 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: -0.013 min
Response: 904472
Conc: 23.56 ng/ml m

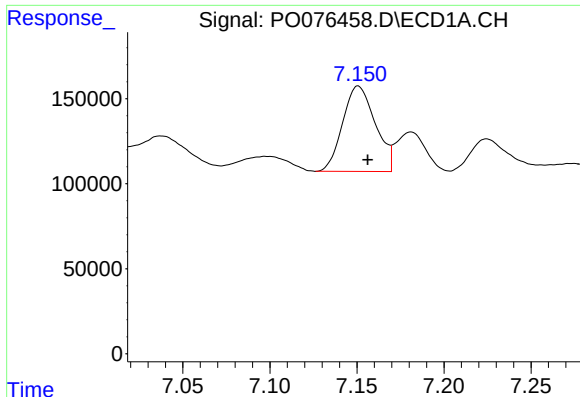


#26 AR-1254-1

R.T.: 7.151 min
Delta R.T.: -0.005 min
Response: 656424
Conc: 320.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:21 PM

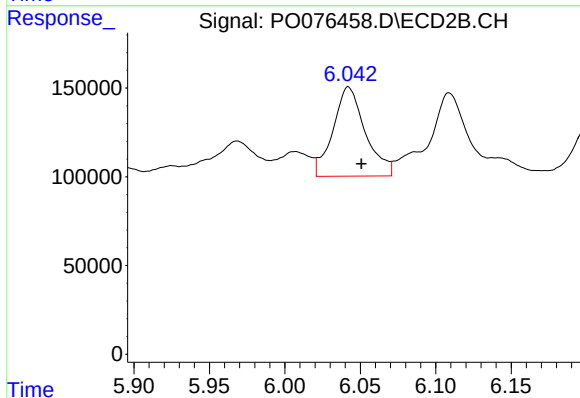


#26 AR-1254-1

R.T.: 6.042 min
Delta R.T.: -0.009 min
Response: 751421
Conc: 328.78 ng/ml

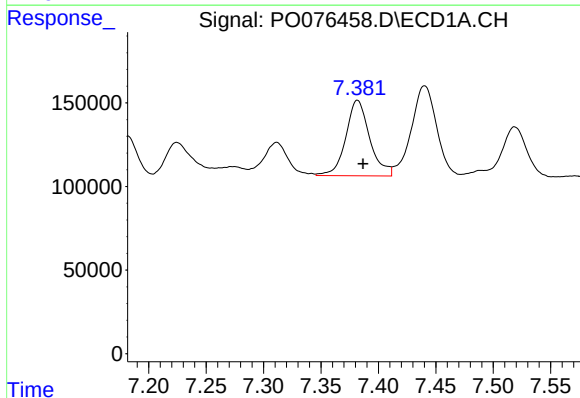


#27 AR-1254-2

R.T.: 7.382 min
Delta R.T.: -0.005 min
Response: 658239
Conc: 211.82 ng/ml

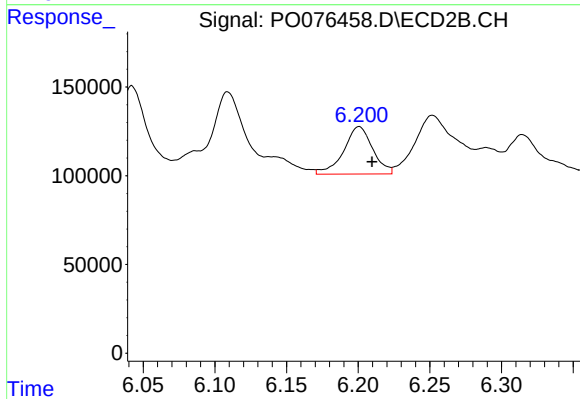

#27 AR-1254-2

R.T.: 6.201 min
Delta R.T.: -0.009 min
Response: 378248
Conc: 190.98 ng/ml

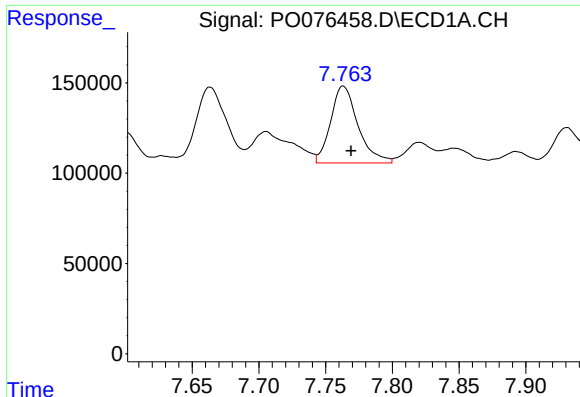


#28 AR-1254-3

R.T.: 7.763 min
Delta R.T.: -0.006 min
Response: 606788
Conc: 190.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:21 PM

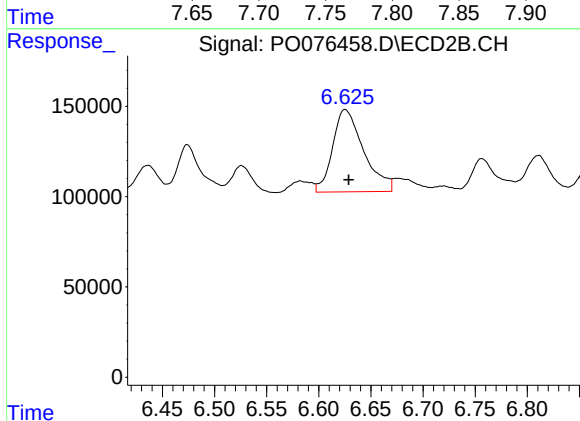


#28 AR-1254-3

R.T.: 6.625 min
Delta R.T.: -0.003 min
Response: 943562
Conc: 313.26 ng/ml

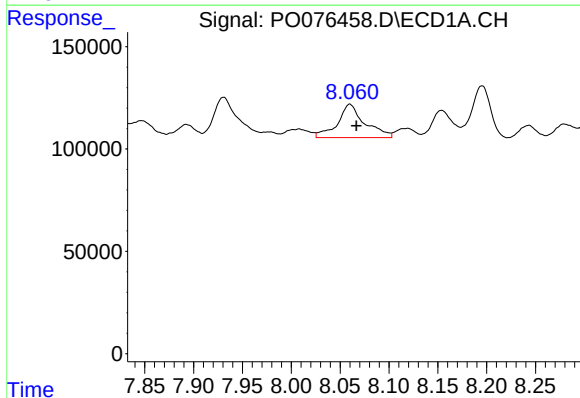


#29 AR-1254-4

R.T.: 8.060 min
Delta R.T.: -0.007 min
Response: 315359
Conc: 150.52 ng/ml

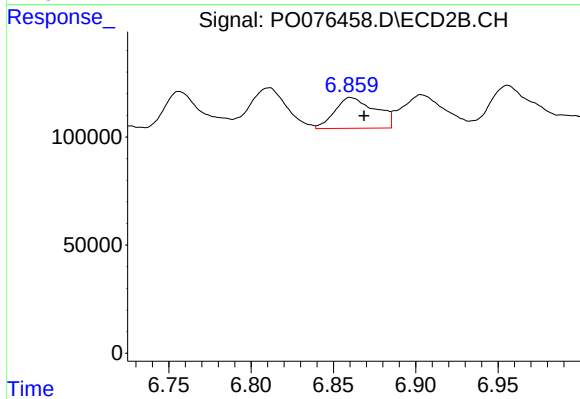

#29 AR-1254-4

R.T.: 6.861 min
Delta R.T.: -0.008 min
Response: 244880
Conc: 138.77 ng/ml

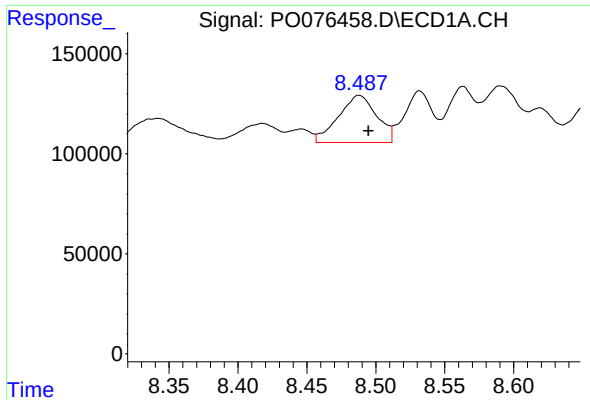


#30 AR-1254-5

R.T.: 8.488 min
Delta R.T.: -0.007 min
Response: 455619
Conc: 198.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C

Manual Integrations
APPROVED

Ankita
3/24/2021 2:18:21 PM

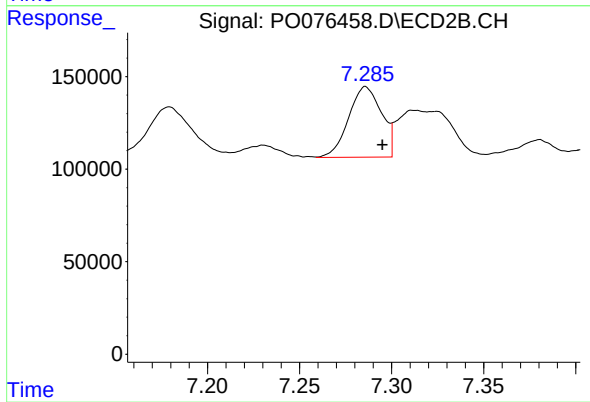

#30 AR-1254-5

R.T.: 7.286 min
Delta R.T.: -0.009 min
Response: 473202
Conc: 180.74 ng/ml