

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0032322\  
 Data File : P0085570.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Mar 2022 15:32  
 Operator : YP\AJ  
 Sample : N2055-13 10X  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 ECD\_0  
 ClientSampleId :  
 CLI-2022-36A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 24 01:13:42 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031522.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 16 04:43:31 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2   | Resp#1 | Resp#2 | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|--------|--------|--------|---------|
| -----                       |                 |        |        |        |        |        |         |
| System Monitoring Compounds |                 |        |        |        |        |        |         |
| 1)                          | SA Tetrachlo... | 4.489  | 3.588  | 206367 | 71467  | 1.009  | 1.668 # |
| 2)                          | SA Decachlor... | 10.392 | 8.603  | 228915 | 84592  | 1.904  | 2.203   |
| Target Compounds            |                 |        |        |        |        |        |         |
| 3)                          | L1 AR-1016-1    | 5.703  | 0.000  | 6964   | 0      | 1.107  | N.D. #  |
| 4)                          | L1 AR-1016-2    | 5.703  | 0.000  | 6964   | 0      | 0.760  | N.D. #  |
| 5)                          | L1 AR-1016-3    | 5.766  | 4.891  | 1889   | 2898   | 0.347  | 2.319 # |
| 6)                          | L1 AR-1016-4    | 5.859  | 4.891  | 21040  | 2898   | 4.770  | 2.655 # |
| 7)                          | L1 AR-1016-5    | 6.167  | 5.127  | 2398   | 1952   | 0.565  | 1.443 # |
| 8)                          | L2 AR-1221-1    | 4.667f | 0.000  | 932    | 0      | 0.422  | N.D. #  |
| 9)                          | L2 AR-1221-2    | 4.805  | 0.000  | 7762   | 0      | 4.765  | N.D. #  |
| 10)                         | L2 AR-1221-3    | 4.872  | 0.000  | 1485   | 0      | 0.289  | N.D. #  |
| 11)                         | L3 AR-1232-1    | 4.872  | 0.000  | 1485   | 0      | 0.316  | N.D. #  |
| 12)                         | L3 AR-1232-2    | 5.409  | 0.000  | 1104   | 0      | 0.479  | N.D. #  |
| 13)                         | L3 AR-1232-3    | 5.703  | 4.891  | 6964   | 2898   | 1.650  | 4.769 # |
| 14)                         | L3 AR-1232-4    | 5.859  | 4.891f | 21040  | 2898   | 10.478 | 5.200 # |
| 15)                         | L3 AR-1232-5    | 5.951  | 5.127  | 19154  | 1952   | 13.014 | 3.166 # |
| 16)                         | L4 AR-1242-1    | 5.703  | 0.000  | 6964   | 0      | 1.370  | N.D. #  |
| 17)                         | L4 AR-1242-2    | 5.703  | 0.000  | 6964   | 0      | 0.938  | N.D. #  |
| 18)                         | L4 AR-1242-3    | 5.766  | 4.891  | 1889   | 2898   | 0.430  | 2.866 # |
| 19)                         | L4 AR-1242-4    | 5.859  | 4.891f | 21040  | 2898   | 5.798  | 2.788 # |
| 20)                         | L4 AR-1242-5    | 6.615  | 0.000  | 4285   | 0      | 1.206  | N.D. #  |
| 21)                         | L5 AR-1248-1    | 5.703  | 0.000  | 6964   | 0      | 1.868  | N.D. #  |
| 22)                         | L5 AR-1248-2    | 5.951  | 4.891  | 19154  | 2898   | 3.614  | 1.979 # |
| 23)                         | L5 AR-1248-3    | 6.167  | 4.891f | 2398   | 2898   | 0.408  | 1.891 # |
| 24)                         | L5 AR-1248-4    | 6.581  | 5.127  | 12420  | 1952   | 1.926  | 1.111 # |
| 25)                         | L5 AR-1248-5    | 6.615  | 0.000  | 4285   | 0      | 0.692  | N.D. #  |
| 26)                         | L6 AR-1254-1    | 6.555  | 0.000  | 40666  | 0      | 6.136  | N.D. #  |
| 27)                         | L6 AR-1254-2    | 6.763  | 0.000  | 7085   | 0      | 0.708  | N.D. #  |
| 28)                         | L6 AR-1254-3    | 7.151  | 0.000  | 26145  | 0      | 2.540  | N.D. #  |
| 29)                         | L6 AR-1254-4    | 7.416  | 6.279  | 1116   | 967    | 0.159  | 0.436 # |
| 30)                         | L6 AR-1254-5    | 7.854  | 0.000  | 6544   | 0      | 0.855  | N.D. #  |
| 31)                         | L7 AR-1260-1    | 7.310  | 0.000  | 6842   | 0      | 0.992  | N.D. #  |
| 32)                         | L7 AR-1260-2    | 7.578  | 0.000  | 11765  | 0      | 1.504  | N.D. #  |
| 33)                         | L7 AR-1260-3    | 7.932  | 6.493  | 30346  | 2123   | 5.167  | 0.807 # |
| 34)                         | L7 AR-1260-4    | 8.155  | 0.000  | 15599  | 0      | 2.258  | N.D. #  |
| 35)                         | L7 AR-1260-5    | 8.492  | 0.000  | 9695   | 0      | 0.690  | N.D. #  |
| 36)                         | L8 AR-1262-1    | 7.932  | 0.000  | 30346  | 0      | 3.360  | N.D. #  |
| 37)                         | L8 AR-1262-2    | 8.492  | 0.000  | 9695   | 0      | 0.608  | N.D. #  |
| 38)                         | L8 AR-1262-3    | 8.822  | 0.000  | 3856   | 0      | 0.373  | N.D. #  |
| 39)                         | L8 AR-1262-4    | 8.886  | 0.000  | 4132   | 0      | 0.880  | N.D. #  |
| 40)                         | L8 AR-1262-5    | 9.595  | 0.000  | 437    | 0      | 0.082  | N.D. #  |
| 41)                         | L9 AR-1268-1    | 8.807  | 0.000  | 1694   | 0      | 0.088  | N.D. #  |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0032322\  
Data File : P0085570.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Mar 2022 15:32  
Operator : YP\AJ  
Sample : N2055-13 10X  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 24 01:13:42 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031522.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Mar 16 04:43:31 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|     | Compound     | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml |   |
|-----|--------------|--------|-------|--------|--------|-------|-------|---|
| 42) | L9 AR-1268-2 | 8.886  | 0.000 | 4132   | 0      | 0.238 | N.D.  | # |
| 43) | L9 AR-1268-3 | 9.149  | 0.000 | 1980   | 0      | 0.134 | N.D.  | # |
| 44) | L9 AR-1268-4 | 9.595  | 0.000 | 437    | 0      | 0.072 | N.D.  | # |
| 45) | L9 AR-1268-5 | 10.032 | 0.000 | 2235   | 0      | 0.046 | N.D.  | # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO032322\  
Data File : PO085570.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Mar 2022 15:32  
Operator : YP\AJ  
Sample : N2055-13 10X  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 24 01:13:42 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO031522.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Mar 16 04:43:31 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

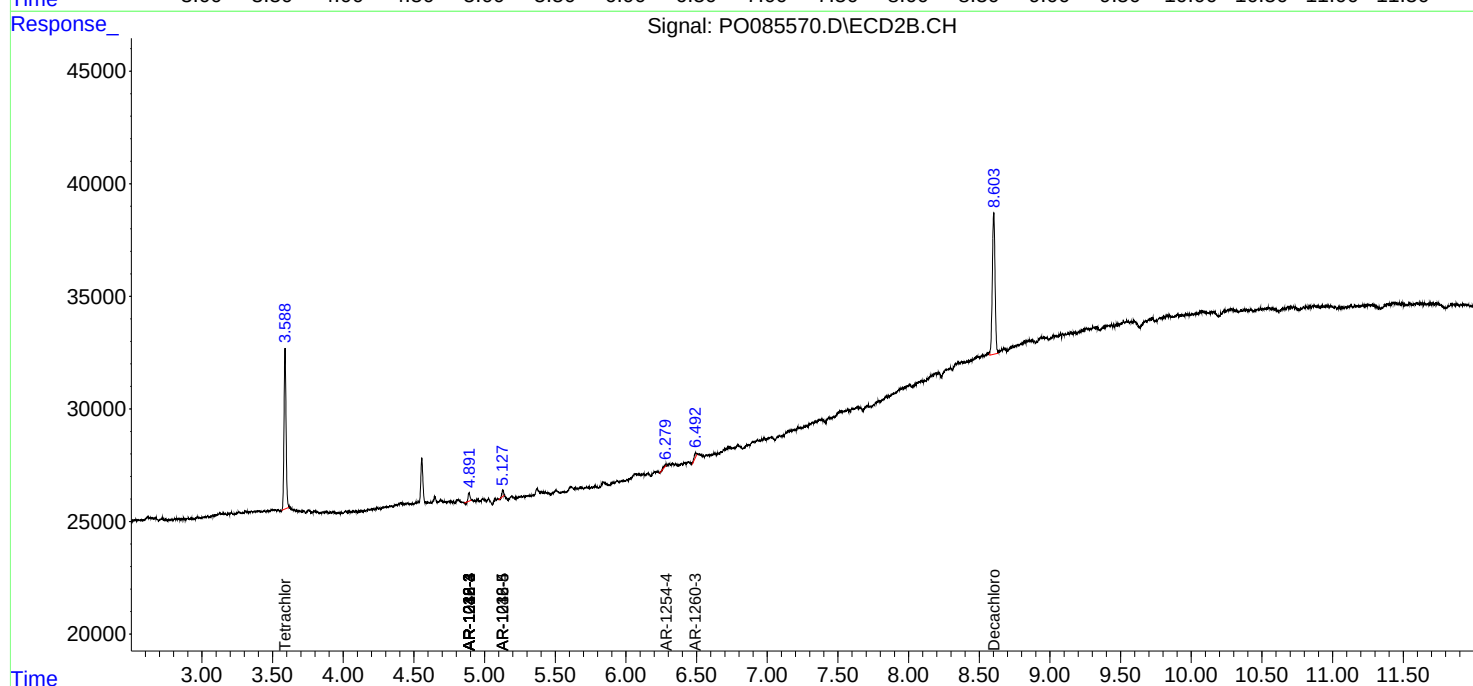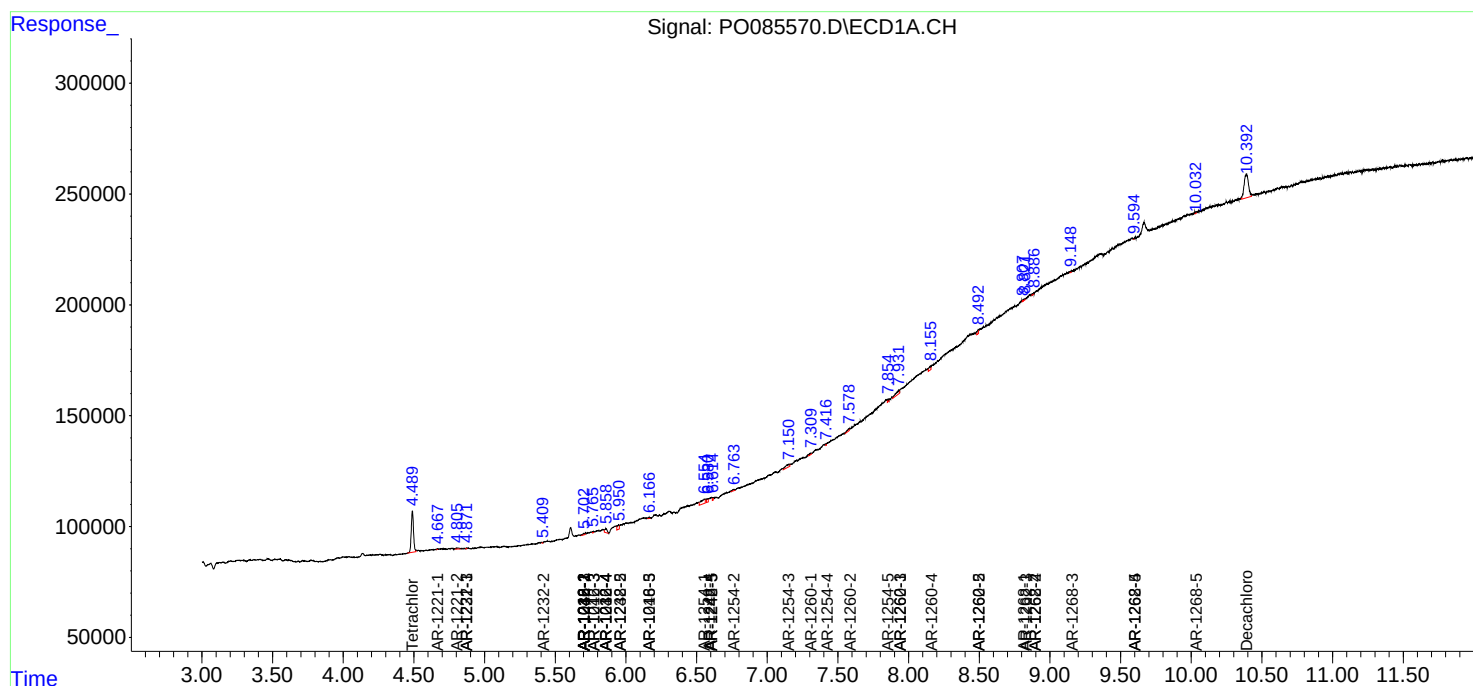


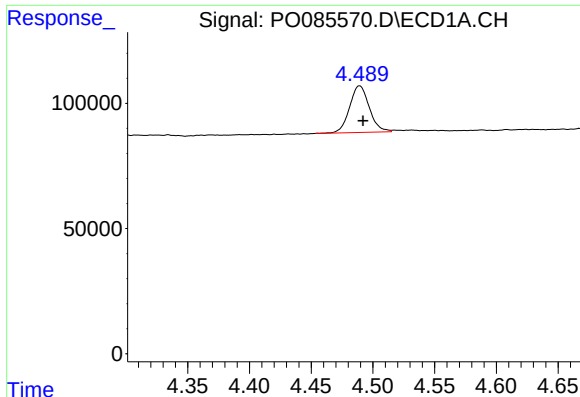

#1 Tetrachloro-m-xylene


R.T.: 4.489 min  
Delta R.T.: -0.003 min  
Response: 206367  
Conc: 1.01 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

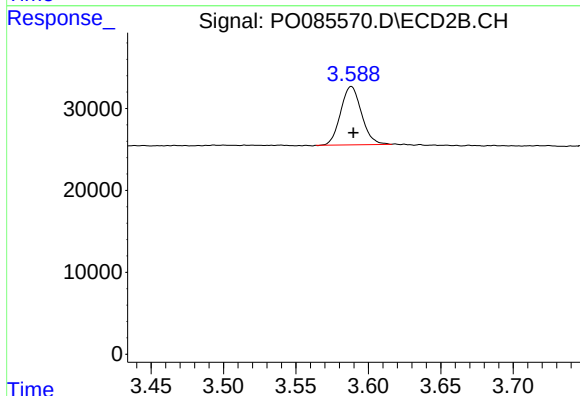


#1 Tetrachloro-m-xylene

R.T.: 3.588 min  
Delta R.T.: -0.001 min  
Response: 71467  
Conc: 1.67 ng/ml

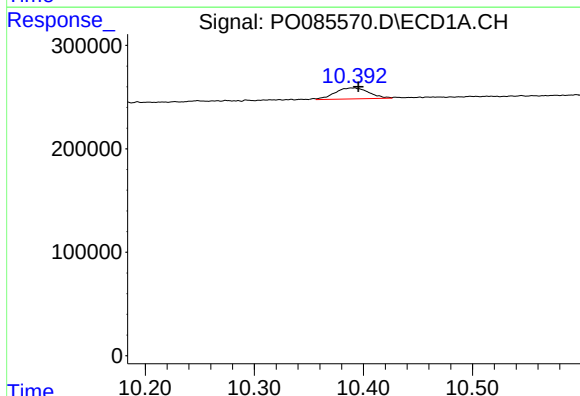


#2 Decachlorobiphenyl

R.T.: 10.392 min  
Delta R.T.: -0.003 min  
Response: 228915  
Conc: 1.90 ng/ml

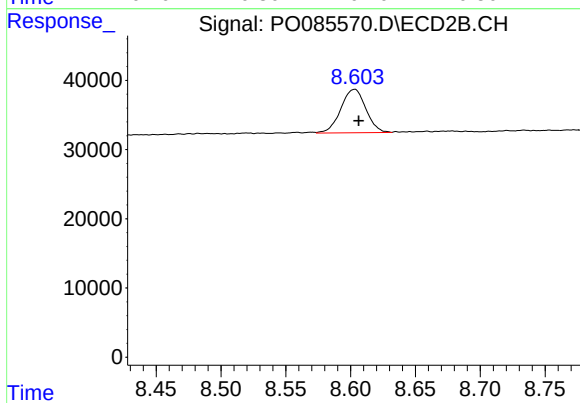

#2 Decachlorobiphenyl


R.T.: 8.603 min  
Delta R.T.: -0.003 min  
Response: 84592  
Conc: 2.20 ng/ml

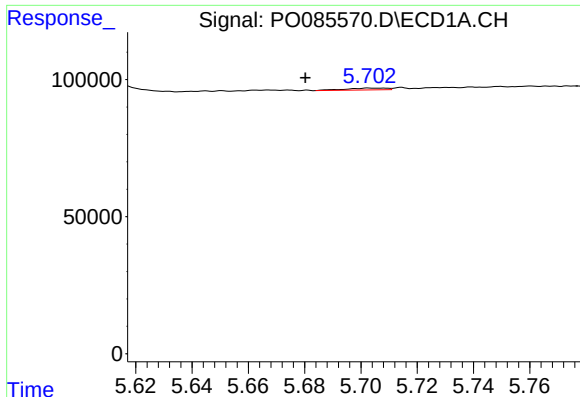

#3 AR-1016-1


R.T.: 5.703 min  
Delta R.T.: 0.022 min  
Response: 6964  
Conc: 1.11 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

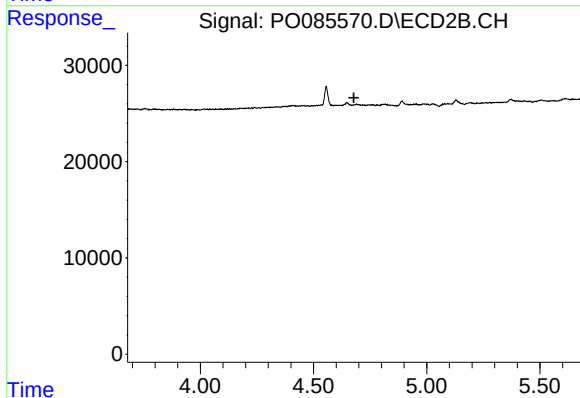


#3 AR-1016-1

R.T.: 0.000 min  
Exp R.T. : 4.679 min  
Response: 0  
Conc: N.D.

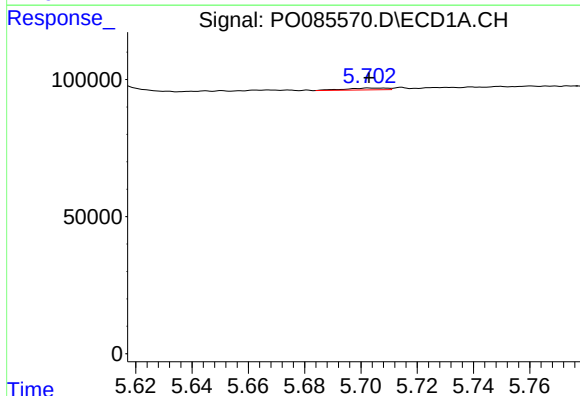


#4 AR-1016-2

R.T.: 5.703 min  
Delta R.T.: 0.000 min  
Response: 6964  
Conc: 0.76 ng/ml

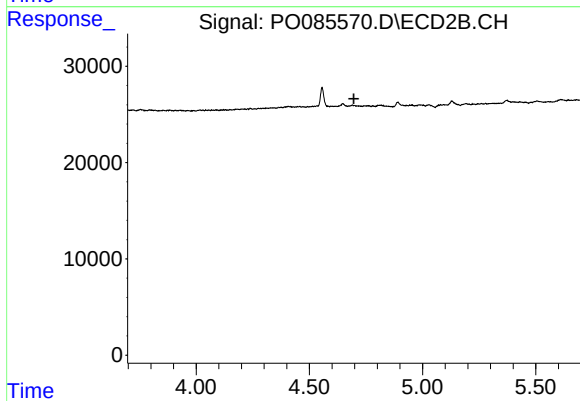

#4 AR-1016-2


R.T.: 0.000 min  
Exp R.T. : 4.697 min  
Response: 0  
Conc: N.D.

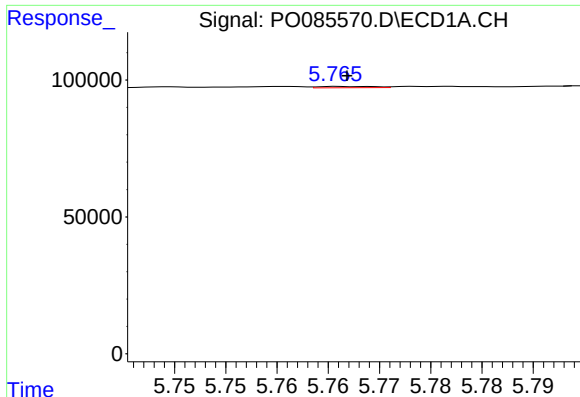

#5 AR-1016-3


R.T.: 5.766 min  
Delta R.T.: 0.000 min  
Response: 1889  
Conc: 0.35 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

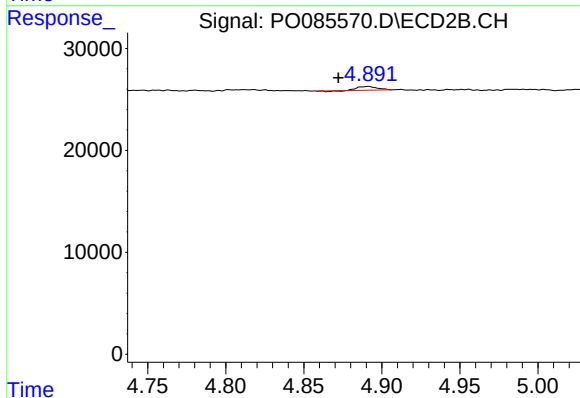


#5 AR-1016-3

R.T.: 4.891 min  
Delta R.T.: 0.019 min  
Response: 2898  
Conc: 2.32 ng/ml

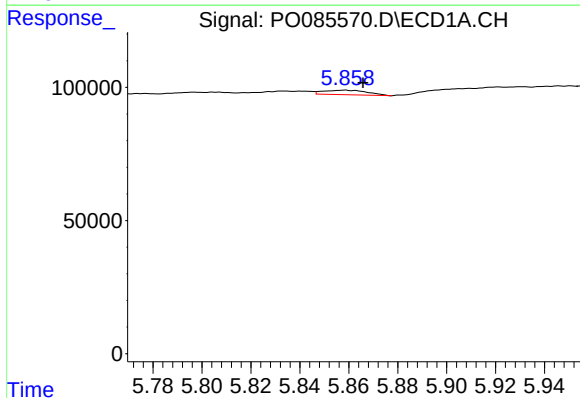


#6 AR-1016-4

R.T.: 5.859 min  
Delta R.T.: -0.007 min  
Response: 21040  
Conc: 4.77 ng/ml

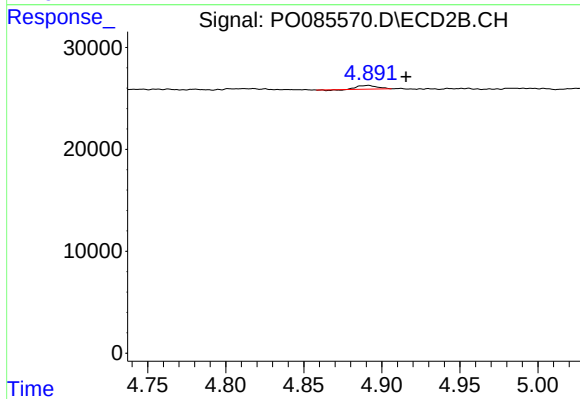

#6 AR-1016-4


R.T.: 4.891 min  
Delta R.T.: -0.024 min  
Response: 2898  
Conc: 2.65 ng/ml

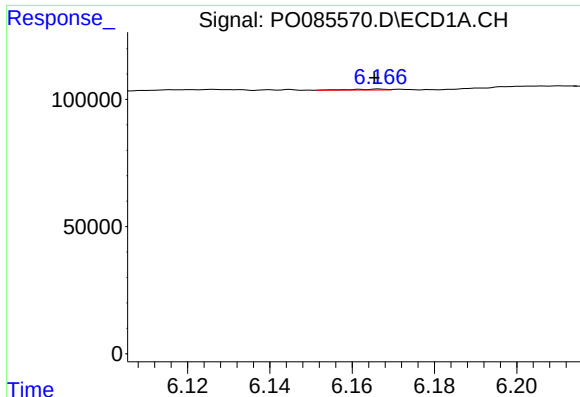

#7 AR-1016-5


R.T.: 6.167 min  
Delta R.T.: 0.001 min  
Response: 2398  
Conc: 0.56 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

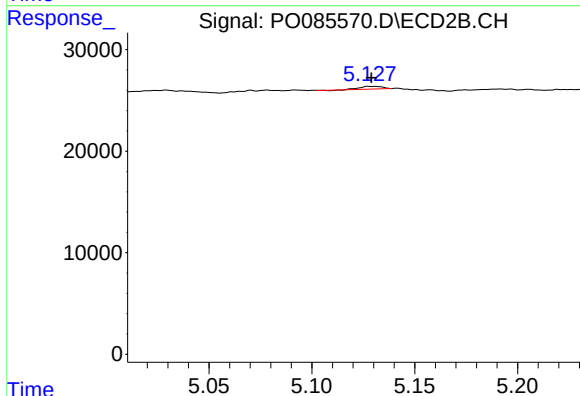


#7 AR-1016-5

R.T.: 5.127 min  
Delta R.T.: -0.001 min  
Response: 1952  
Conc: 1.44 ng/ml

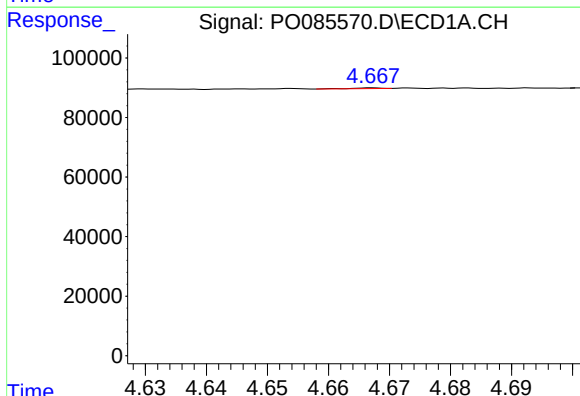


#8 AR-1221-1

R.T.: 4.667 min  
Delta R.T.: -0.036 min  
Response: 932  
Conc: 0.42 ng/ml

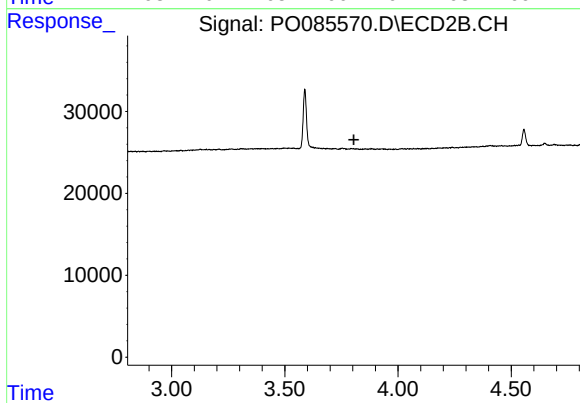

#8 AR-1221-1


R.T.: 0.000 min  
Exp R.T. : 3.805 min  
Response: 0  
Conc: N.D.

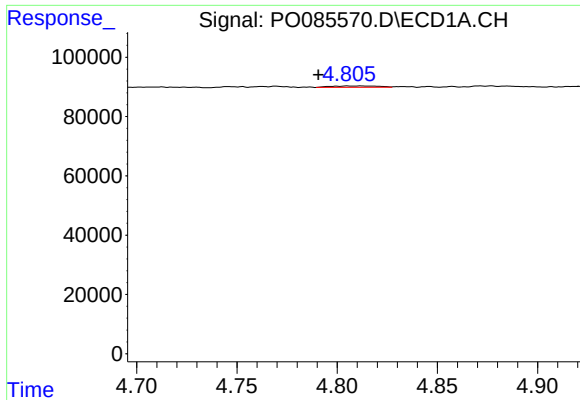

#9 AR-1221-2


R.T.: 4.805 min  
Delta R.T.: 0.014 min  
Response: 7762  
Conc: 4.77 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

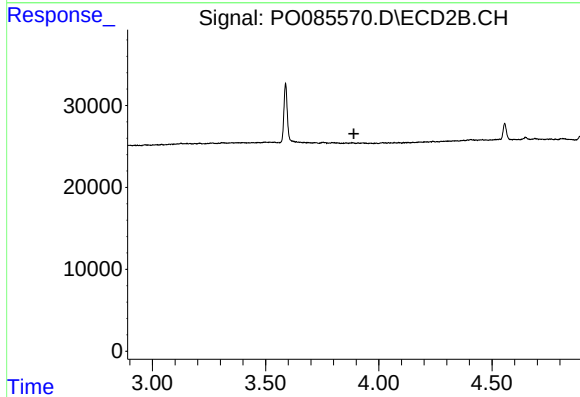


#9 AR-1221-2

R.T.: 0.000 min  
Exp R.T. : 3.890 min  
Response: 0  
Conc: N.D.

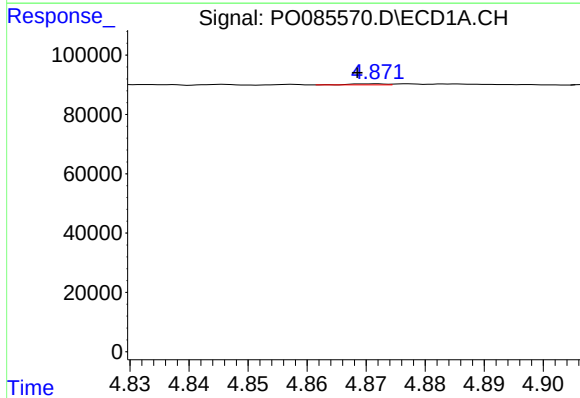

#10 AR-1221-3


R.T.: 4.872 min  
Delta R.T.: 0.003 min  
Response: 1485  
Conc: 0.29 ng/ml

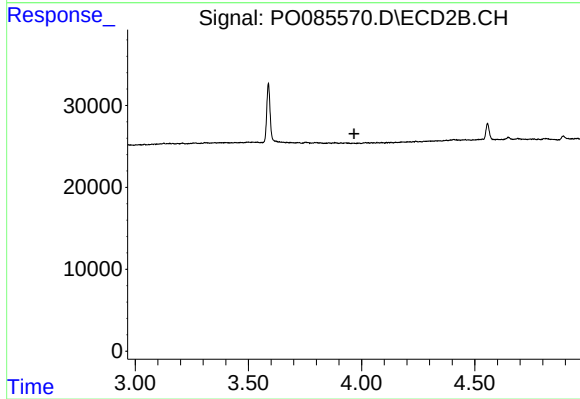

#10 AR-1221-3

R.T.: 0.000 min  
Exp R.T. : 3.966 min  
Response: 0  
Conc: N.D.




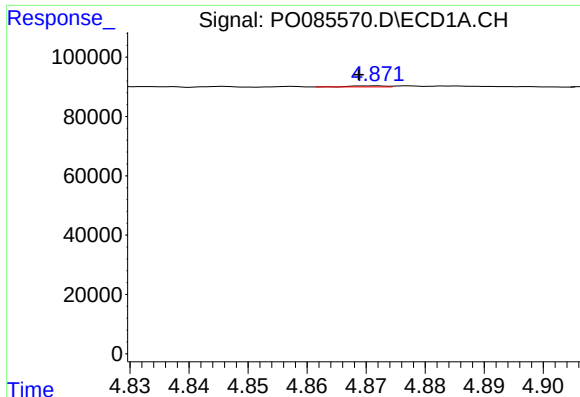

#11 AR-1232-1


R.T.: 4.872 min  
Delta R.T.: 0.003 min  
Response: 1485  
Conc: 0.32 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

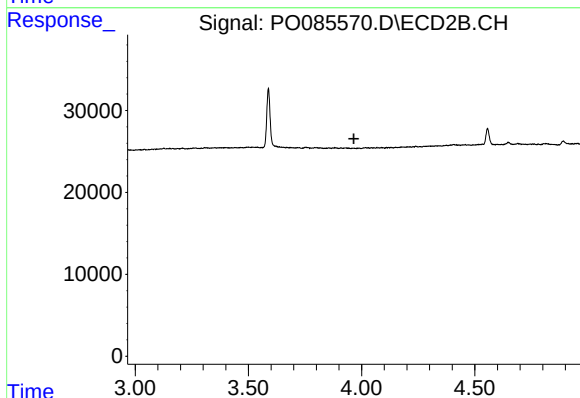


#11 AR-1232-1

R.T.: 0.000 min  
Exp R.T. : 3.966 min  
Response: 0  
Conc: N.D.

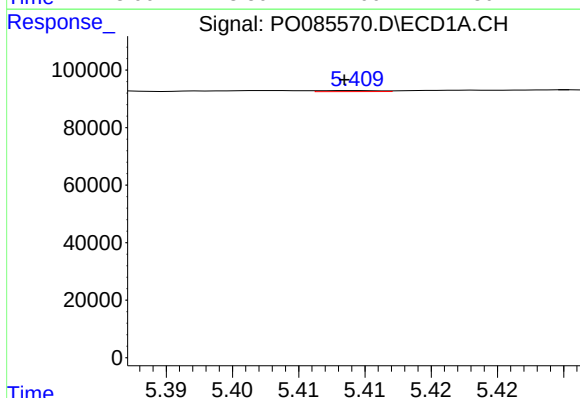


#12 AR-1232-2

R.T.: 5.409 min  
Delta R.T.: 0.000 min  
Response: 1104  
Conc: 0.48 ng/ml

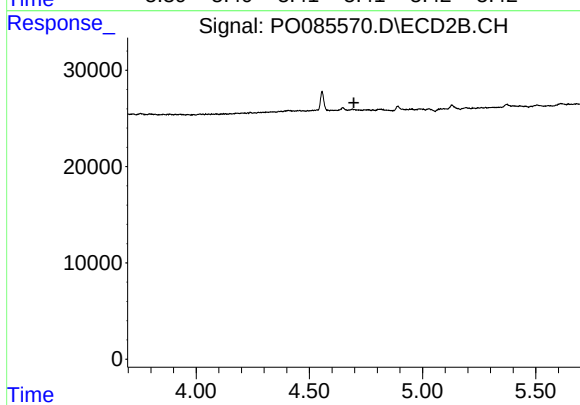

#12 AR-1232-2


R.T.: 0.000 min  
Exp R.T. : 4.697 min  
Response: 0  
Conc: N.D.

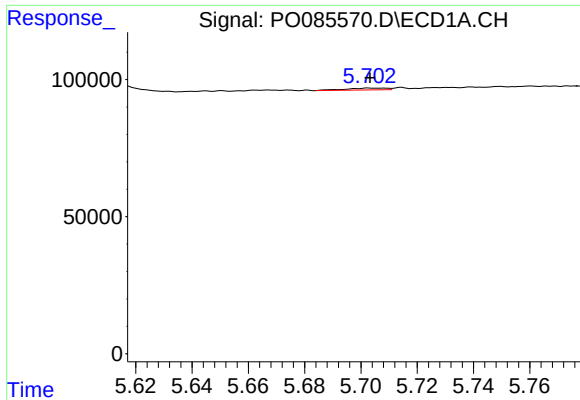

#13 AR-1232-3


R.T.: 5.703 min  
Delta R.T.: 0.000 min  
Response: 6964  
Conc: 1.65 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

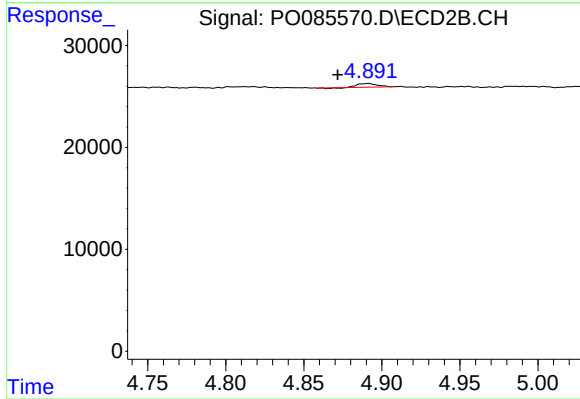


#13 AR-1232-3

R.T.: 4.891 min  
Delta R.T.: 0.020 min  
Response: 2898  
Conc: 4.77 ng/ml

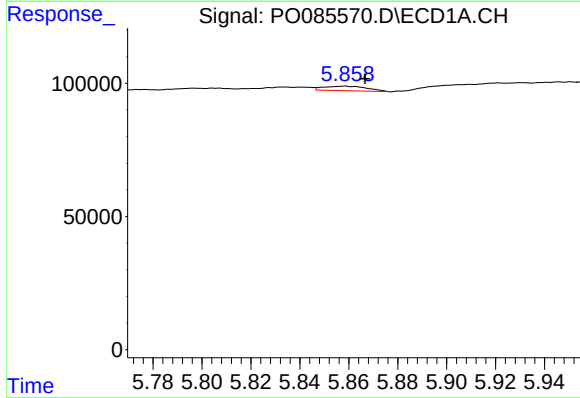


#14 AR-1232-4

R.T.: 5.859 min  
Delta R.T.: -0.008 min  
Response: 21040  
Conc: 10.48 ng/ml

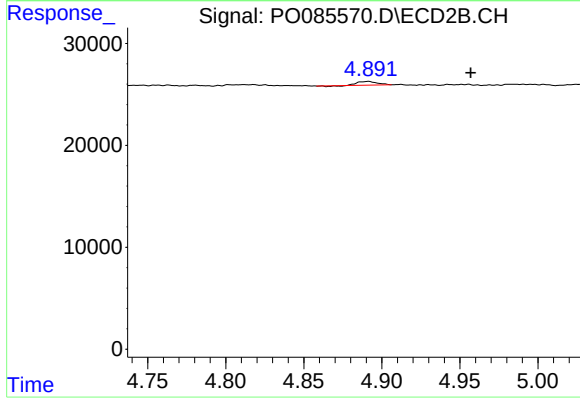

#14 AR-1232-4


R.T.: 4.891 min  
Delta R.T.: -0.066 min  
Response: 2898  
Conc: 5.20 ng/ml

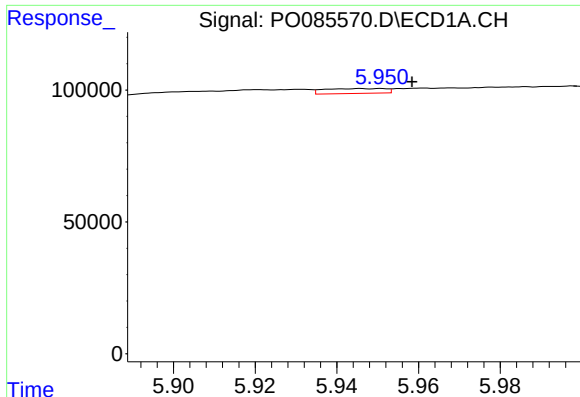

#15 AR-1232-5


R.T.: 5.951 min  
Delta R.T.: -0.008 min  
Response: 19154  
Conc: 13.01 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

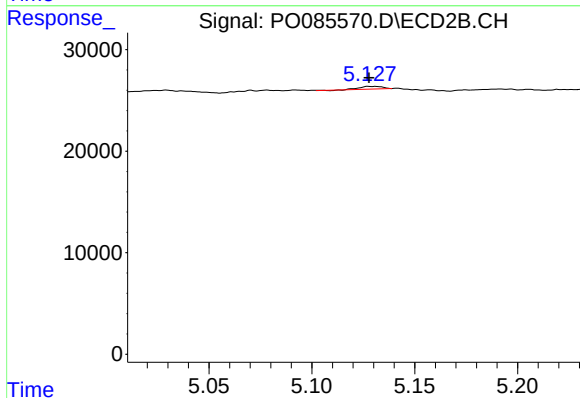


#15 AR-1232-5

R.T.: 5.127 min  
Delta R.T.: 0.000 min  
Response: 1952  
Conc: 3.17 ng/ml

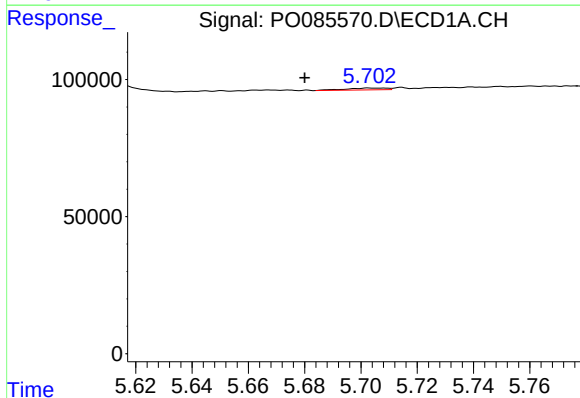


#16 AR-1242-1

R.T.: 5.703 min  
Delta R.T.: 0.023 min  
Response: 6964  
Conc: 1.37 ng/ml

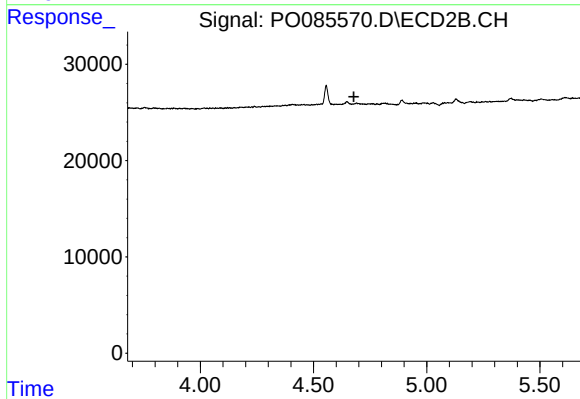

#16 AR-1242-1


R.T.: 0.000 min  
Exp R.T.: 4.678 min  
Response: 0  
Conc: N.D.

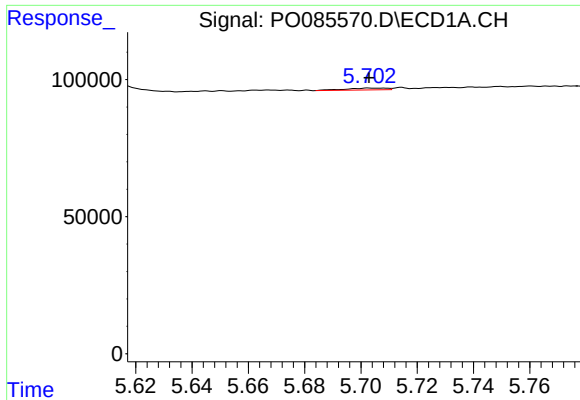

#17 AR-1242-2


R.T.: 5.703 min  
Delta R.T.: 0.000 min  
Response: 6964  
Conc: 0.94 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

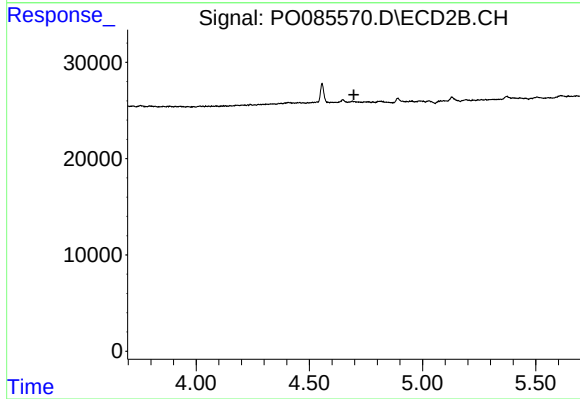


#17 AR-1242-2

R.T.: 0.000 min  
Exp R.T. : 4.696 min  
Response: 0  
Conc: N.D.

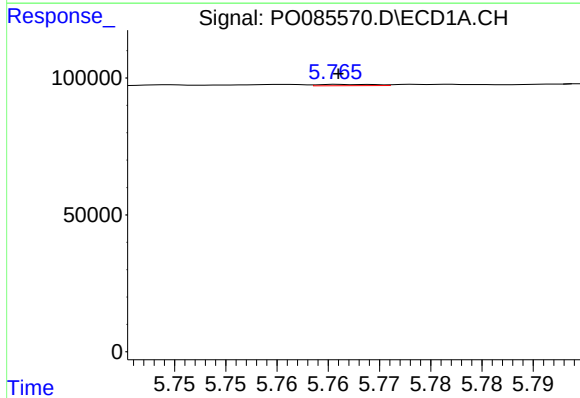


#18 AR-1242-3

R.T.: 5.766 min  
Delta R.T.: 0.000 min  
Response: 1889  
Conc: 0.43 ng/ml

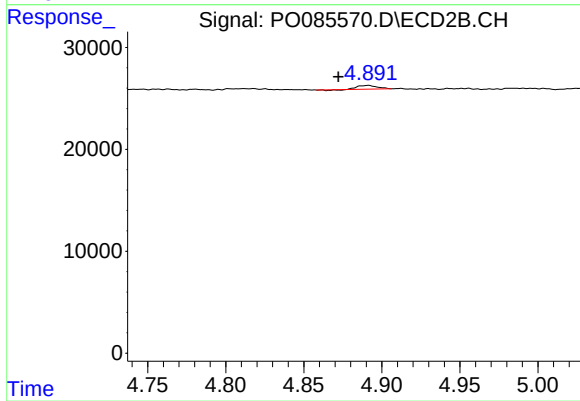

#18 AR-1242-3


R.T.: 4.891 min  
Delta R.T.: 0.019 min  
Response: 2898  
Conc: 2.87 ng/ml

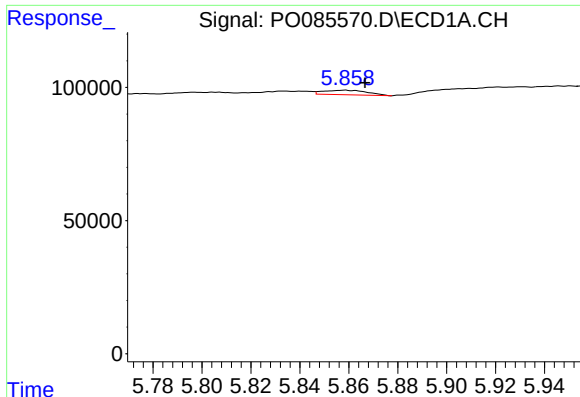

#19 AR-1242-4


R.T.: 5.859 min  
Delta R.T.: -0.008 min  
Response: 21040  
Conc: 5.80 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

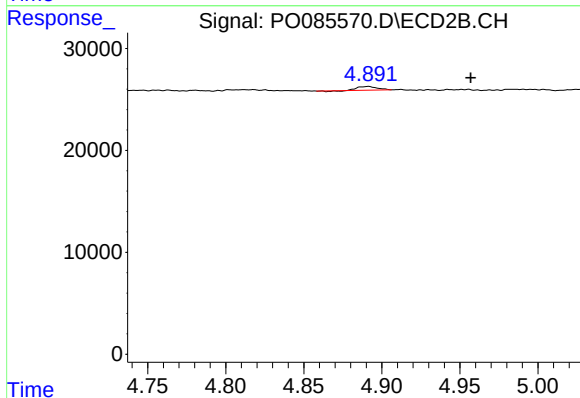


#19 AR-1242-4

R.T.: 4.891 min  
Delta R.T.: -0.065 min  
Response: 2898  
Conc: 2.79 ng/ml

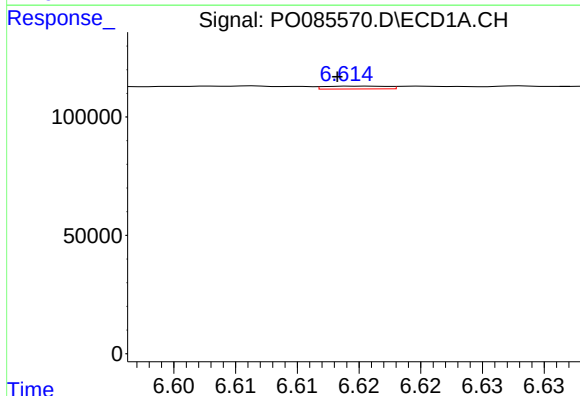


#20 AR-1242-5

R.T.: 6.615 min  
Delta R.T.: 0.002 min  
Response: 4285  
Conc: 1.21 ng/ml

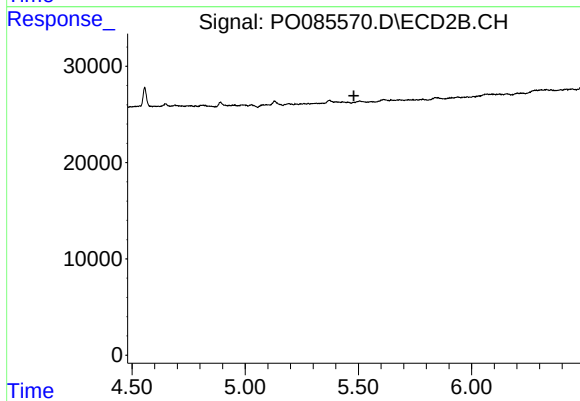

#20 AR-1242-5


R.T.: 0.000 min  
Exp R.T.: 5.480 min  
Response: 0  
Conc: N.D.

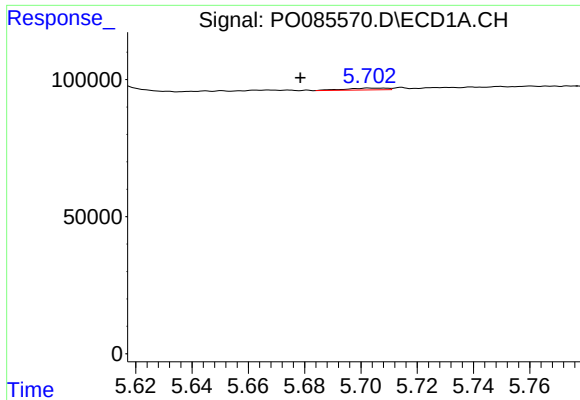

#21 AR-1248-1


R.T.: 5.703 min  
Delta R.T.: 0.024 min  
Response: 6964  
Conc: 1.87 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

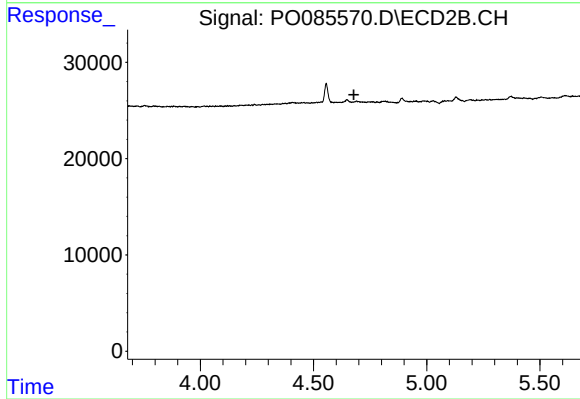


#21 AR-1248-1

R.T.: 0.000 min  
Exp R.T. : 4.678 min  
Response: 0  
Conc: N.D.

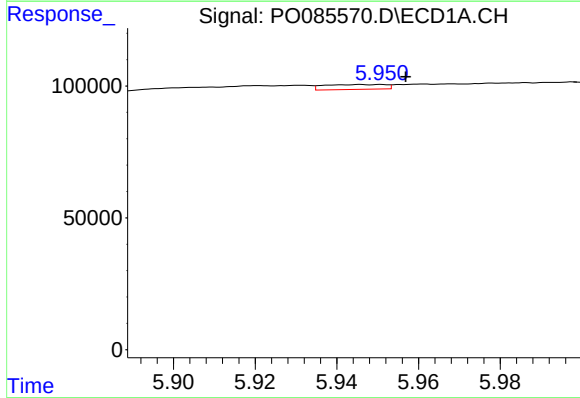


#22 AR-1248-2

R.T.: 5.951 min  
Delta R.T.: -0.006 min  
Response: 19154  
Conc: 3.61 ng/ml

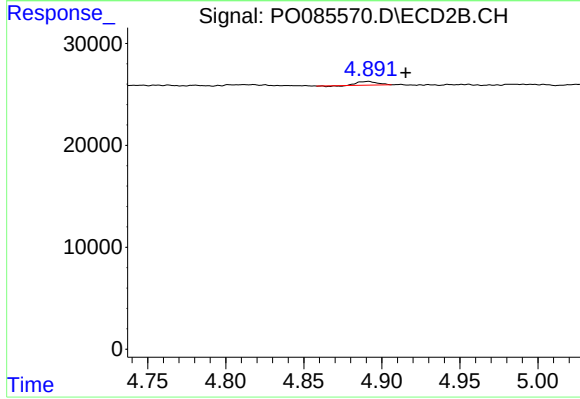

#22 AR-1248-2


R.T.: 4.891 min  
Delta R.T.: -0.024 min  
Response: 2898  
Conc: 1.98 ng/ml

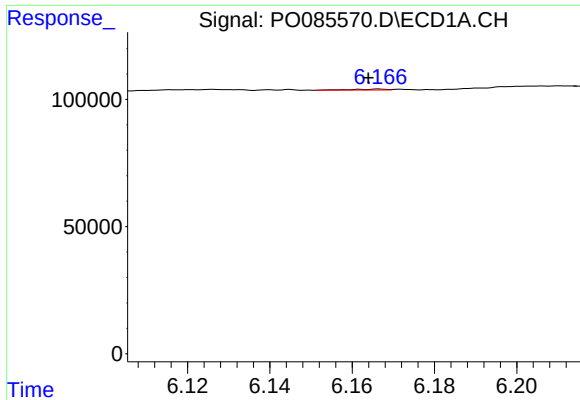

#23 AR-1248-3


R.T.: 6.167 min  
Delta R.T.: 0.003 min  
Response: 2398  
Conc: 0.41 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

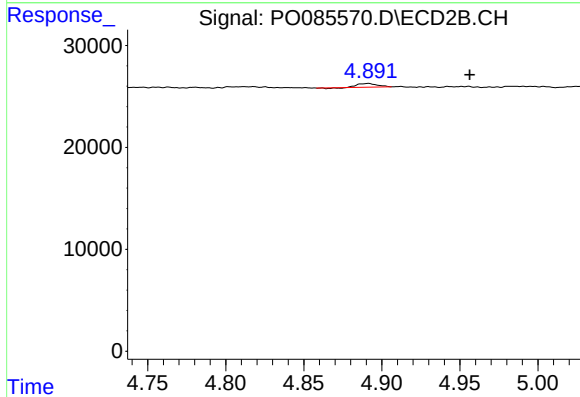


#23 AR-1248-3

R.T.: 4.891 min  
Delta R.T.: -0.065 min  
Response: 2898  
Conc: 1.89 ng/ml

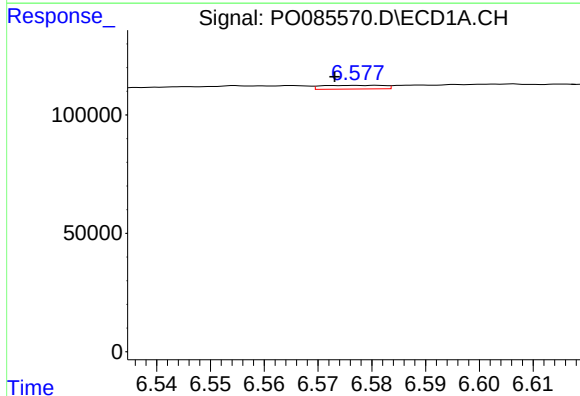


#24 AR-1248-4

R.T.: 6.581 min  
Delta R.T.: 0.008 min  
Response: 12420  
Conc: 1.93 ng/ml

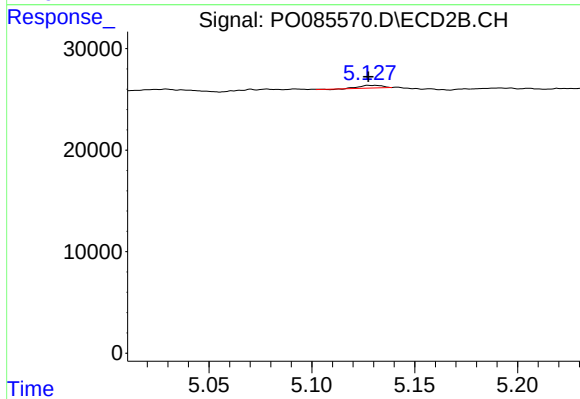

#24 AR-1248-4


R.T.: 5.127 min  
Delta R.T.: 0.000 min  
Response: 1952  
Conc: 1.11 ng/ml

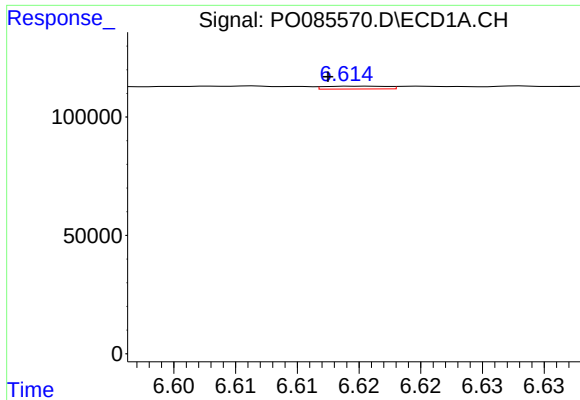

#25 AR-1248-5


R.T.: 6.615 min  
Delta R.T.: 0.003 min  
Response: 4285  
Conc: 0.69 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

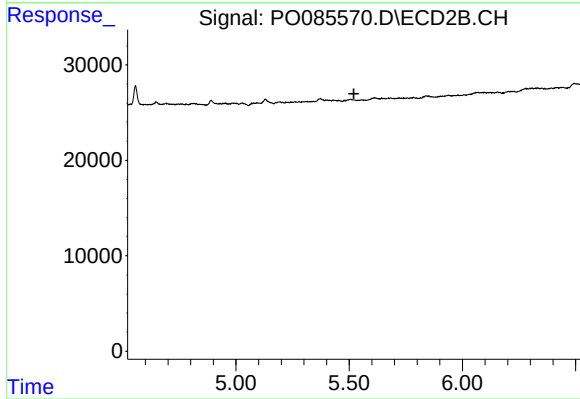


#25 AR-1248-5

R.T.: 0.000 min  
Exp R.T. : 5.521 min  
Response: 0  
Conc: N.D.

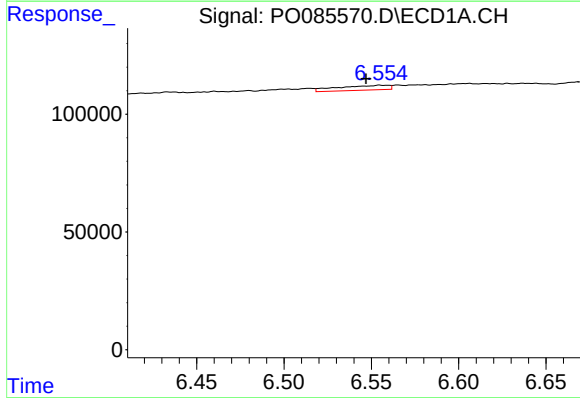

#26 AR-1254-1


R.T.: 6.555 min  
Delta R.T.: 0.008 min  
Response: 40666  
Conc: 6.14 ng/ml

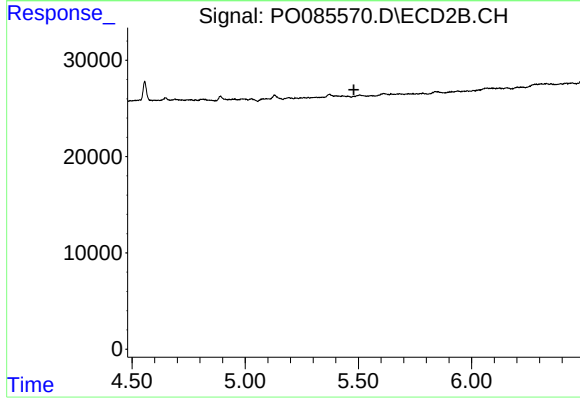

#26 AR-1254-1

R.T.: 0.000 min  
Exp R.T. : 5.480 min  
Response: 0  
Conc: N.D.




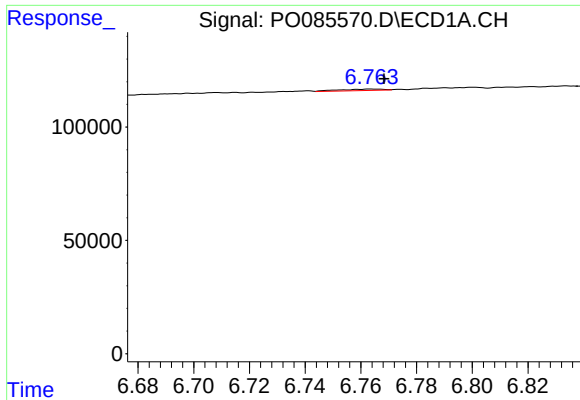

#27 AR-1254-2


R.T.: 6.763 min  
Delta R.T.: -0.005 min  
Response: 7085  
Conc: 0.71 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

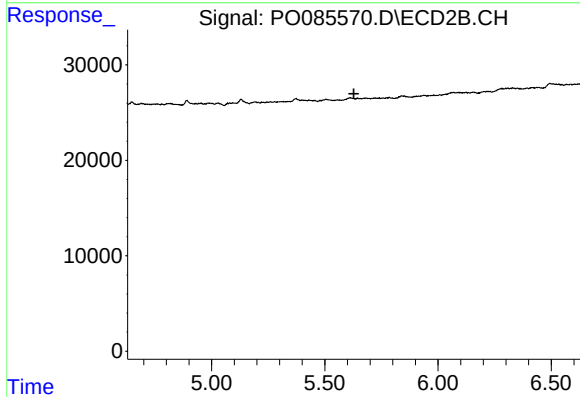


#27 AR-1254-2

R.T.: 0.000 min  
Exp R.T. : 5.628 min  
Response: 0  
Conc: N.D.

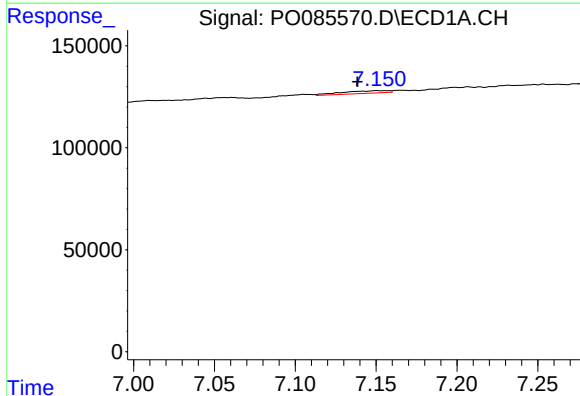


#28 AR-1254-3

R.T.: 7.151 min  
Delta R.T.: 0.012 min  
Response: 26145  
Conc: 2.54 ng/ml

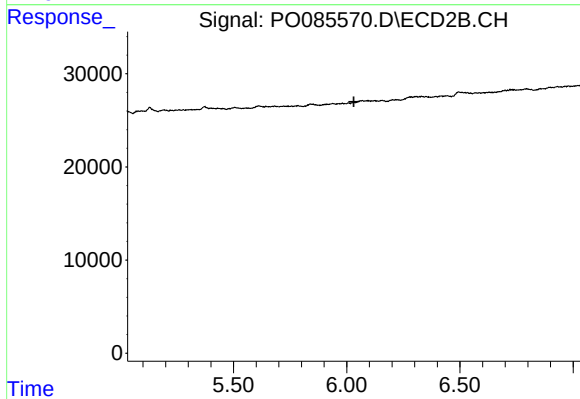

#28 AR-1254-3


R.T.: 0.000 min  
Exp R.T. : 6.032 min  
Response: 0  
Conc: N.D.

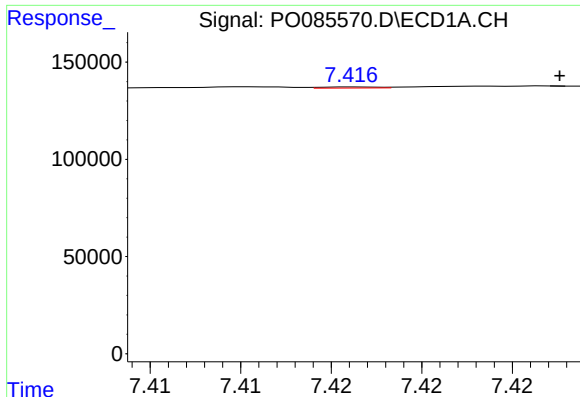

#29 AR-1254-4


R.T.: 7.416 min  
Delta R.T.: -0.011 min  
Response: 1116  
Conc: 0.16 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

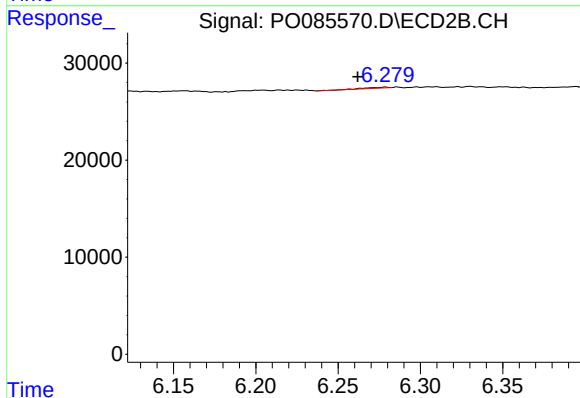


#29 AR-1254-4

R.T.: 6.279 min  
Delta R.T.: 0.017 min  
Response: 967  
Conc: 0.44 ng/ml

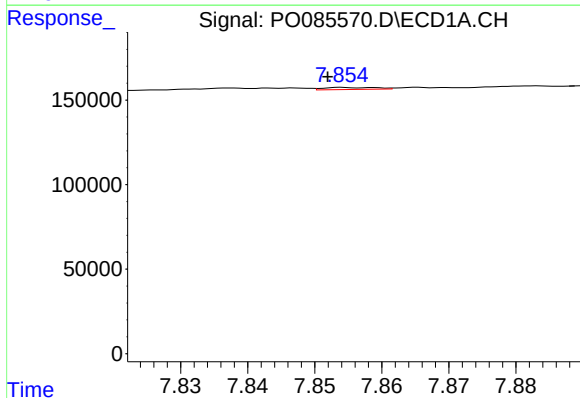


#30 AR-1254-5

R.T.: 7.854 min  
Delta R.T.: 0.002 min  
Response: 6544  
Conc: 0.86 ng/ml

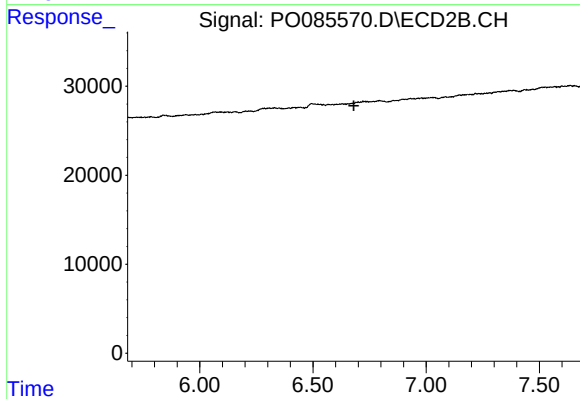

#30 AR-1254-5


R.T.: 0.000 min  
Exp R.T.: 6.680 min  
Response: 0  
Conc: N.D.

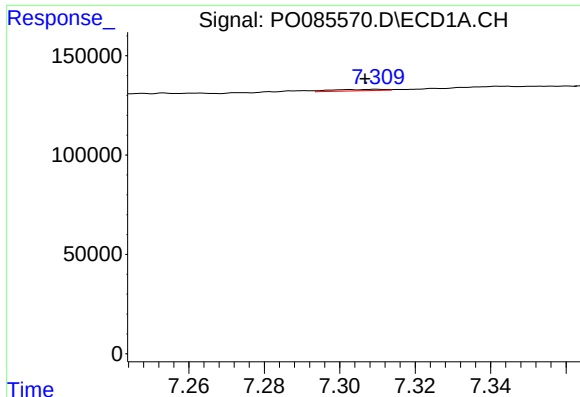

#31 AR-1260-1


R.T.: 7.310 min  
Delta R.T.: 0.003 min  
Response: 6842  
Conc: 0.99 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

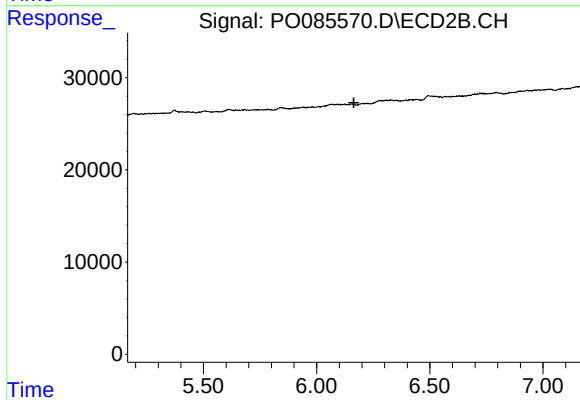


#31 AR-1260-1

R.T.: 0.000 min  
Exp R.T. : 6.165 min  
Response: 0  
Conc: N.D.

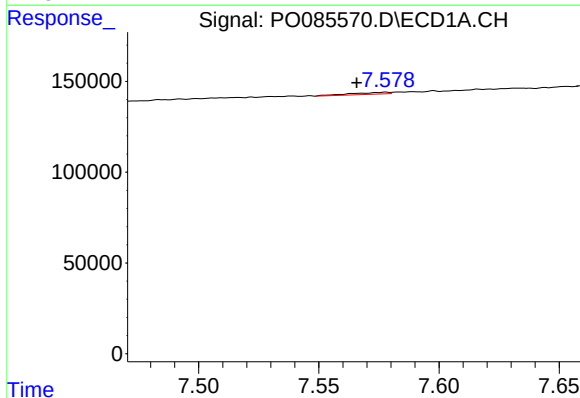


#32 AR-1260-2

R.T.: 7.578 min  
Delta R.T.: 0.012 min  
Response: 11765  
Conc: 1.50 ng/ml

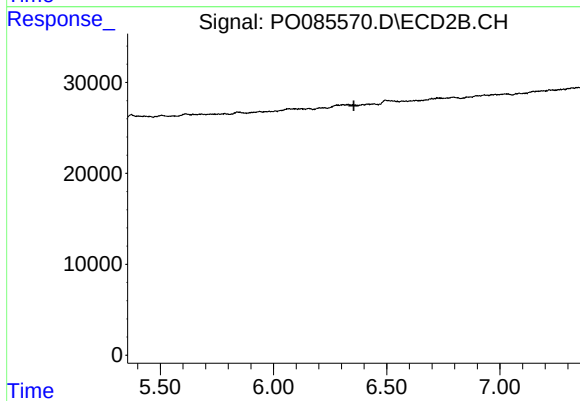

#32 AR-1260-2


R.T.: 0.000 min  
Exp R.T. : 6.355 min  
Response: 0  
Conc: N.D.

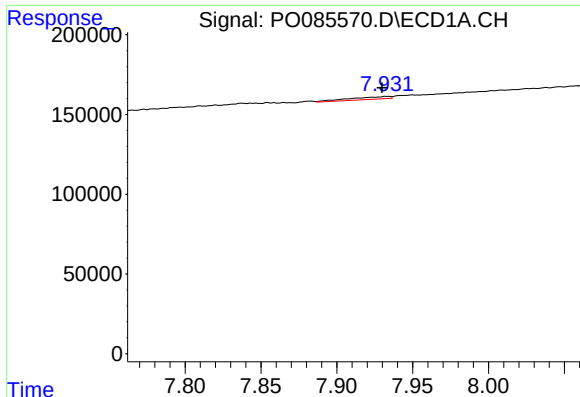

#33 AR-1260-3


R.T.: 7.932 min  
Delta R.T.: 0.002 min  
Response: 30346  
Conc: 5.17 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

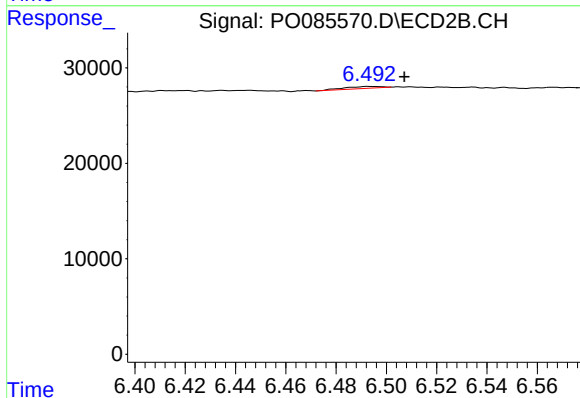


#33 AR-1260-3

R.T.: 6.493 min  
Delta R.T.: -0.015 min  
Response: 2123  
Conc: 0.81 ng/ml

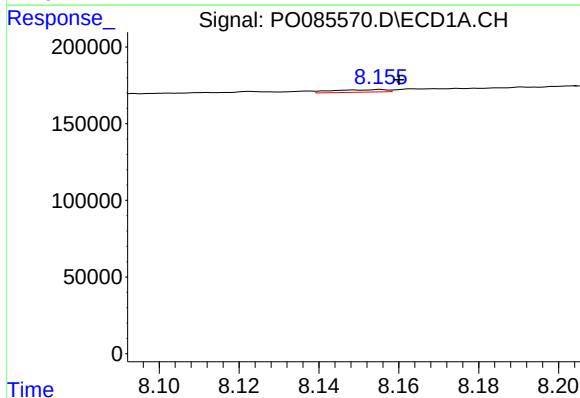


#34 AR-1260-4

R.T.: 8.155 min  
Delta R.T.: -0.005 min  
Response: 15599  
Conc: 2.26 ng/ml

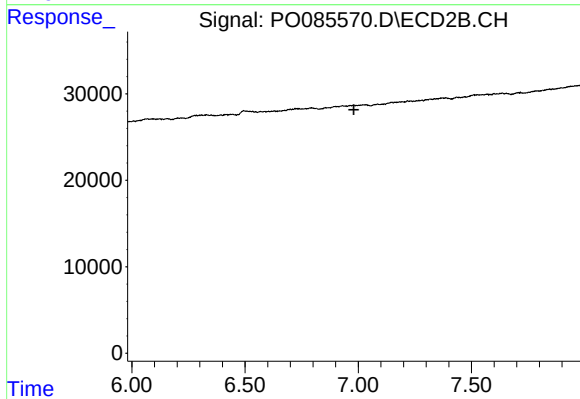

#34 AR-1260-4


R.T.: 0.000 min  
Exp R.T.: 6.981 min  
Response: 0  
Conc: N.D.

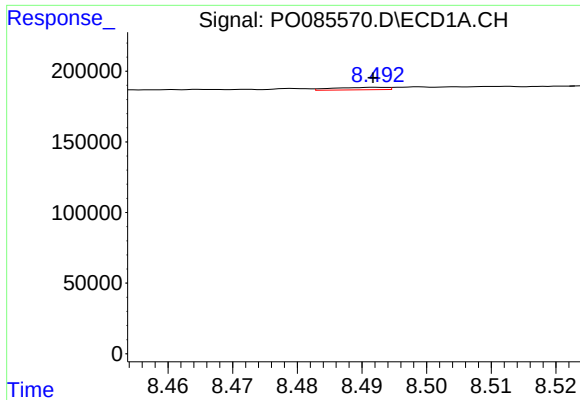

#35 AR-1260-5


R.T.: 8.492 min  
Delta R.T.: 0.000 min  
Response: 9695  
Conc: 0.69 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

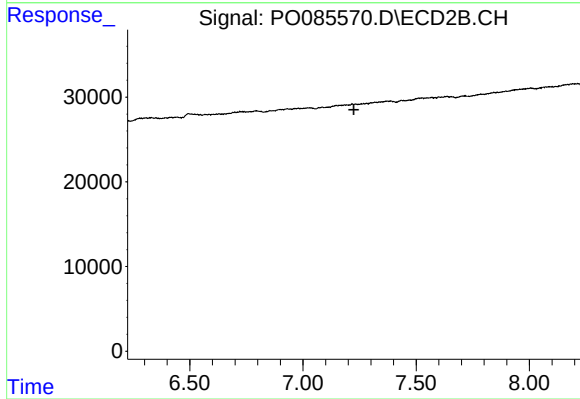


#35 AR-1260-5

R.T.: 0.000 min  
Exp R.T. : 7.225 min  
Response: 0  
Conc: N.D.

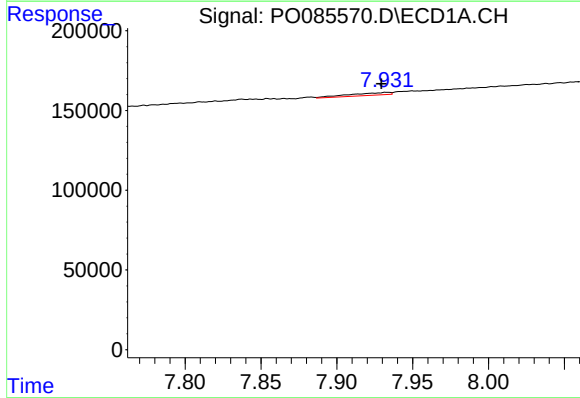


#36 AR-1262-1

R.T.: 7.932 min  
Delta R.T.: 0.003 min  
Response: 30346  
Conc: 3.36 ng/ml

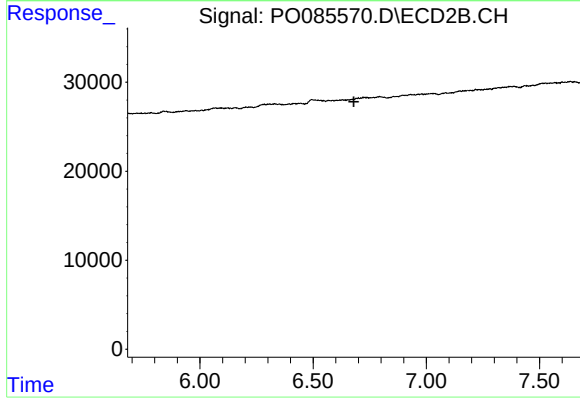

#36 AR-1262-1


R.T.: 0.000 min  
Exp R.T. : 6.680 min  
Response: 0  
Conc: N.D.

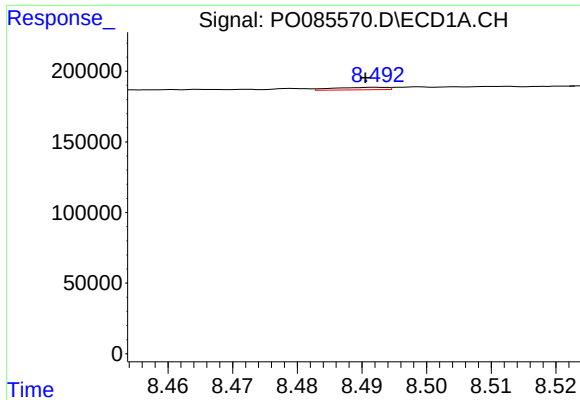

#37 AR-1262-2


R.T.: 8.492 min  
Delta R.T.: 0.002 min  
Response: 9695  
Conc: 0.61 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

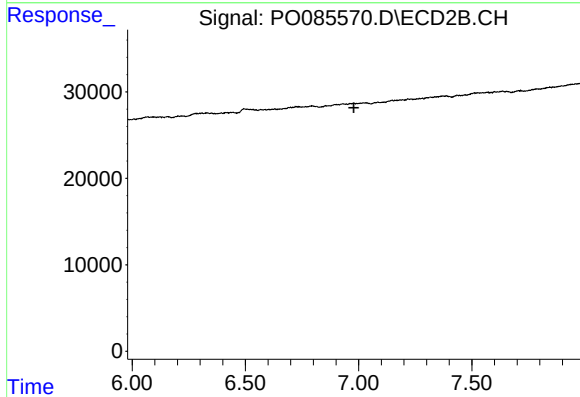


#37 AR-1262-2

R.T.: 0.000 min  
Exp R.T. : 6.979 min  
Response: 0  
Conc: N.D.

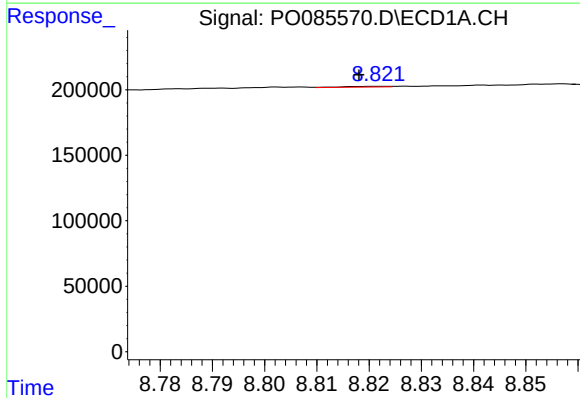


#38 AR-1262-3

R.T.: 8.822 min  
Delta R.T.: 0.004 min  
Response: 3856  
Conc: 0.37 ng/ml

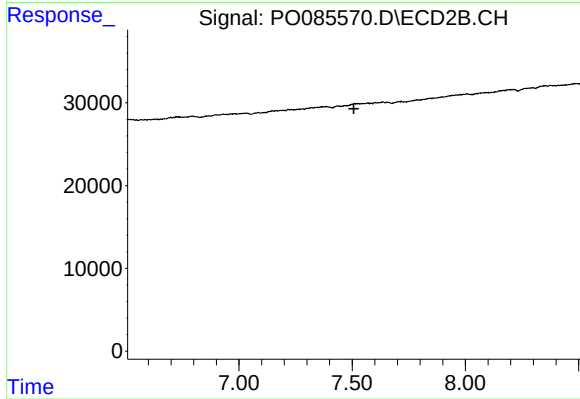

#38 AR-1262-3


R.T.: 0.000 min  
Exp R.T. : 7.508 min  
Response: 0  
Conc: N.D.

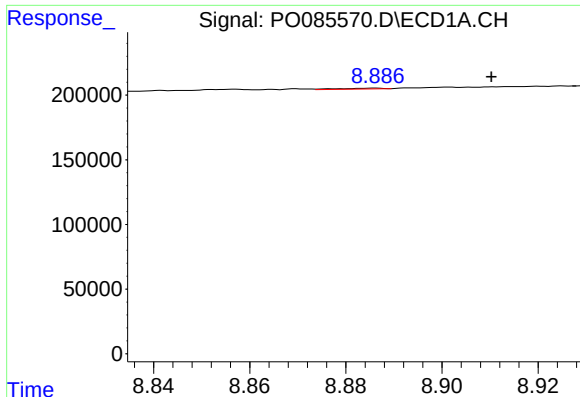

#39 AR-1262-4


R.T.: 8.886 min  
Delta R.T.: -0.024 min  
Response: 4132  
Conc: 0.88 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

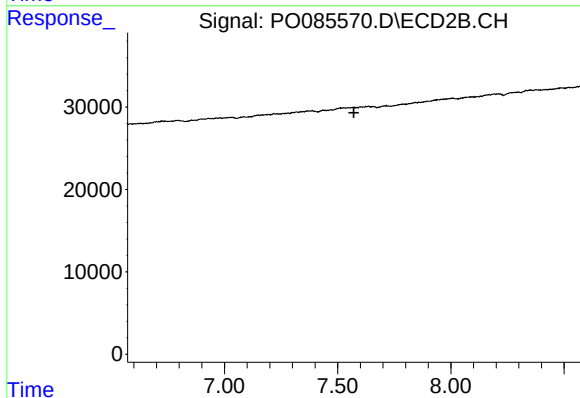


#39 AR-1262-4

R.T.: 0.000 min  
Exp R.T. : 7.571 min  
Response: 0  
Conc: N.D.

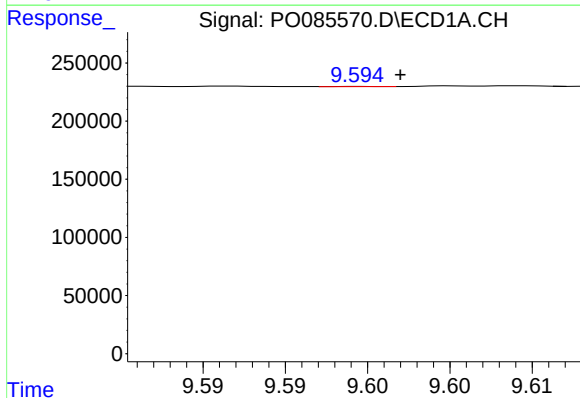


#40 AR-1262-5

R.T.: 9.595 min  
Delta R.T.: -0.002 min  
Response: 437  
Conc: 0.08 ng/ml

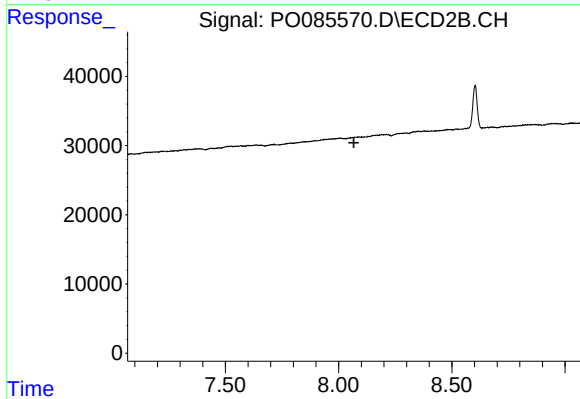

#40 AR-1262-5


R.T.: 0.000 min  
Exp R.T. : 8.067 min  
Response: 0  
Conc: N.D.

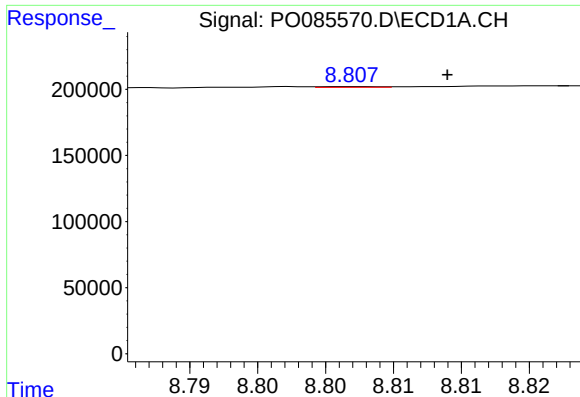

#41 AR-1268-1


R.T.: 8.807 min  
Delta R.T.: -0.007 min  
Response: 1694  
Conc: 0.09 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

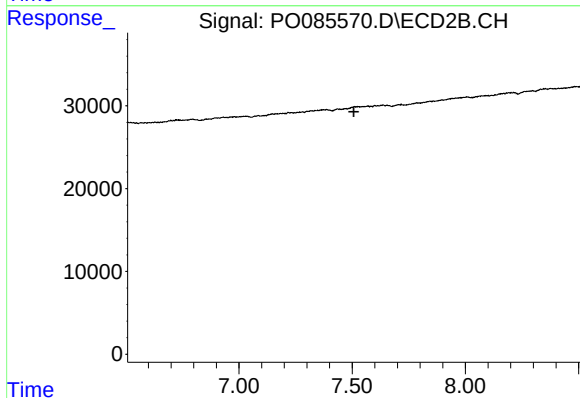


#41 AR-1268-1

R.T.: 0.000 min  
Exp R.T. : 7.508 min  
Response: 0  
Conc: N.D.

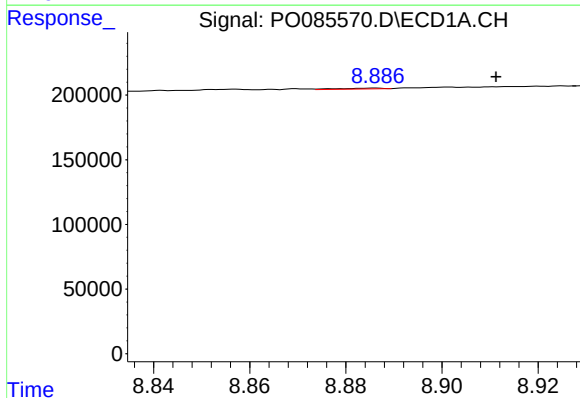

#42 AR-1268-2


R.T.: 8.886 min  
Delta R.T.: -0.025 min  
Response: 4132  
Conc: 0.24 ng/ml

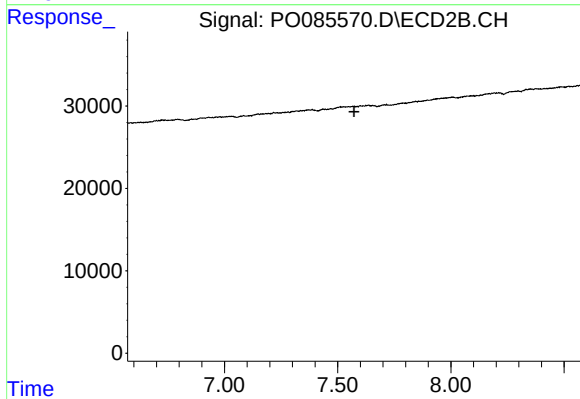

#42 AR-1268-2

R.T.: 0.000 min  
Exp R.T. : 7.572 min  
Response: 0  
Conc: N.D.




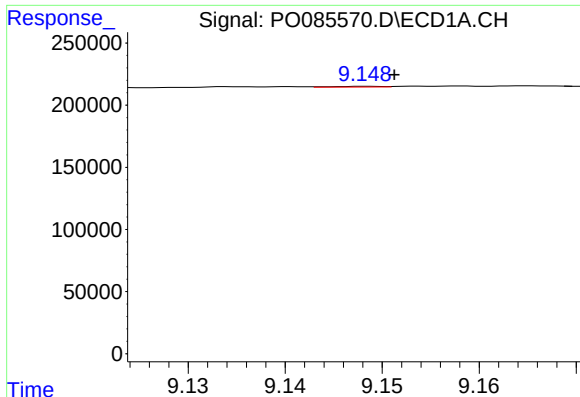

#43 AR-1268-3


R.T.: 9.149 min  
Delta R.T.: -0.003 min  
Response: 1980  
Conc: 0.13 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

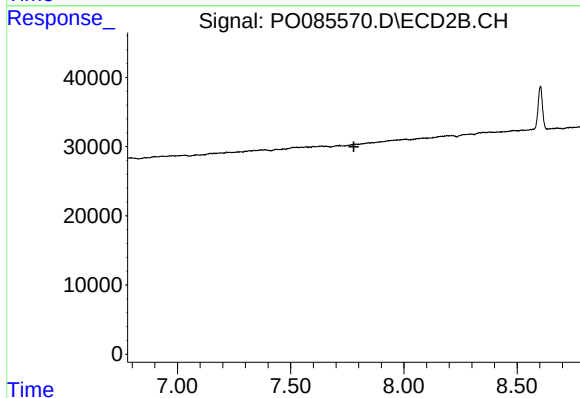


#43 AR-1268-3

R.T.: 0.000 min  
Exp R.T. : 7.779 min  
Response: 0  
Conc: N.D.

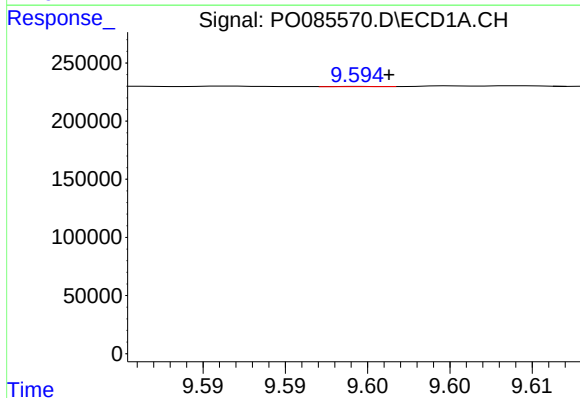


#44 AR-1268-4

R.T.: 9.595 min  
Delta R.T.: -0.002 min  
Response: 437  
Conc: 0.07 ng/ml

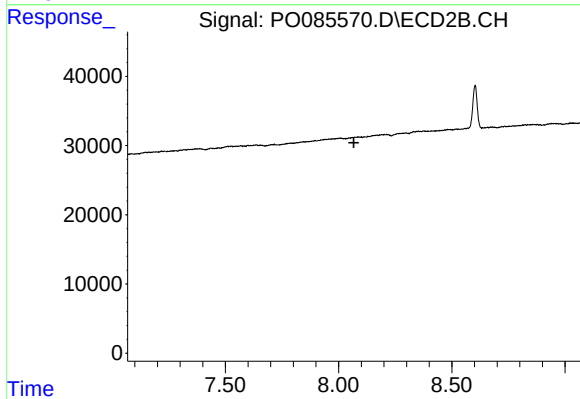

#44 AR-1268-4


R.T.: 0.000 min  
Exp R.T. : 8.068 min  
Response: 0  
Conc: N.D.

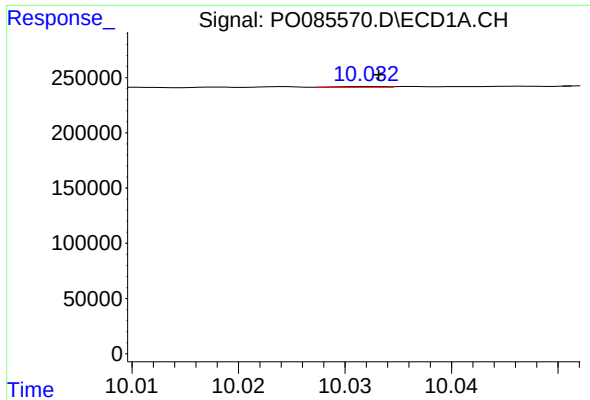

#45 AR-1268-5

R.T.: 10.032 min  
Delta R.T.: 0.000 min  
Response: 2235  
Conc: 0.05 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-36A

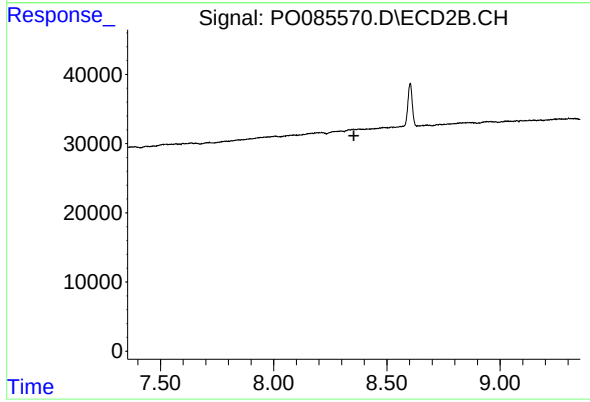

#45 AR-1268-5

R.T.: 0.000 min  
Exp R.T. : 8.354 min  
Response: 0  
Conc: N.D.