

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032322\
 Data File : P0085571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 15:48
 Operator : YP\AJ
 Sample : N2055-12 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CLI-2022-35B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:14:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.591	188565	66587	0.922	1.554 #
2)	SA Decachlor...	10.393	8.603	250009	81854	2.080	2.132
Target Compounds							
3)	L1 AR-1016-1	5.660	0.000	5782	0	0.919	N.D. #
4)	L1 AR-1016-2	5.710	0.000	9729	0	1.062	N.D. #
5)	L1 AR-1016-3	5.774	0.000	232	0	0.043	N.D. #
6)	L1 AR-1016-4	5.842	0.000	7266	0	1.647	N.D. #
7)	L1 AR-1016-5	6.174	0.000	2436	0	0.574	N.D. #
8)	L2 AR-1221-1	4.708	0.000	8780	0	3.980	N.D. #
9)	L2 AR-1221-2	4.803	0.000	3678	0	2.258	N.D. #
10)	L2 AR-1221-3	4.829f	0.000	5081	0	0.988	N.D. #
11)	L3 AR-1232-1	4.829f	0.000	5081	0	1.080	N.D. #
12)	L3 AR-1232-2	5.401	0.000	6323	0	2.744	N.D. #
13)	L3 AR-1232-3	5.710	0.000	9729	0	2.306	N.D. #
14)	L3 AR-1232-4	5.842	0.000	7266	0	3.618	N.D. #
15)	L3 AR-1232-5	5.967	0.000	5556	0	3.775	N.D. #
16)	L4 AR-1242-1	5.660	0.000	5782	0	1.137	N.D. #
17)	L4 AR-1242-2	5.710	0.000	9729	0	1.311	N.D. #
18)	L4 AR-1242-3	5.758	0.000	2983	0	0.679	N.D. #
19)	L4 AR-1242-4	5.842	0.000	7266	0	2.002	N.D. #
20)	L4 AR-1242-5	6.611	0.000	1496	0	0.421	N.D. #
21)	L5 AR-1248-1	5.660	0.000	5782	0	1.551	N.D. #
22)	L5 AR-1248-2	5.967	0.000	5556	0	1.048	N.D. #
23)	L5 AR-1248-3	6.174	0.000	2436	0	0.414	N.D. #
24)	L5 AR-1248-4	6.576	0.000	4958	0	0.769	N.D. #
25)	L5 AR-1248-5	6.611	0.000	1496	0	0.242	N.D. #
26)	L6 AR-1254-1	6.553	0.000	10477	0	1.581	N.D. #
27)	L6 AR-1254-2	6.766	0.000	4133	0	0.413	N.D. #
28)	L6 AR-1254-3	7.148	0.000	25737	0	2.501	N.D. #
29)	L6 AR-1254-4	7.433	0.000	12645	0	1.802	N.D. #
30)	L6 AR-1254-5	7.857	6.714	3307	6980	0.432	2.146 #
31)	L7 AR-1260-1	7.308	0.000	8507	0	1.233	N.D. #
32)	L7 AR-1260-2	7.551	0.000	6401	0	0.818	N.D. #
33)	L7 AR-1260-3	7.944	6.501	37614	5866	6.404	2.231 #
34)	L7 AR-1260-4	8.165	6.992	19150	4858	2.773	2.169
35)	L7 AR-1260-5	8.475	7.196	13004	15541	0.926	3.085 #
36)	L8 AR-1262-1	7.944	6.714	37614	6980	4.165	4.065
37)	L8 AR-1262-2	8.475	6.992	13004	4858	0.816	1.696 #
38)	L8 AR-1262-3	8.819	7.509	2448	4256	0.237	1.943 #
39)	L8 AR-1262-4	8.919	7.562	16227	1468	3.455	0.368 #
40)	L8 AR-1262-5	9.595	0.000	1920	0	0.361	N.D. #
41)	L9 AR-1268-1	8.815	7.509	4926	4256	0.255	0.641 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
 Data File : P0085571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 15:48
 Operator : YP\AJ
 Sample : N2055-12 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-35B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:14:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.919	7.562	16227	1468	0.934	0.249 #
43) L9	AR-1268-3	9.153	0.000	4782	0	0.324	N.D. #
44) L9	AR-1268-4	9.595	0.000	1920	0	0.315	N.D. #
45) L9	AR-1268-5	10.031	0.000	2882	0	0.060	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
Data File : P0085571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 15:48
Operator : YP\AJ
Sample : N2055-12 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:14:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

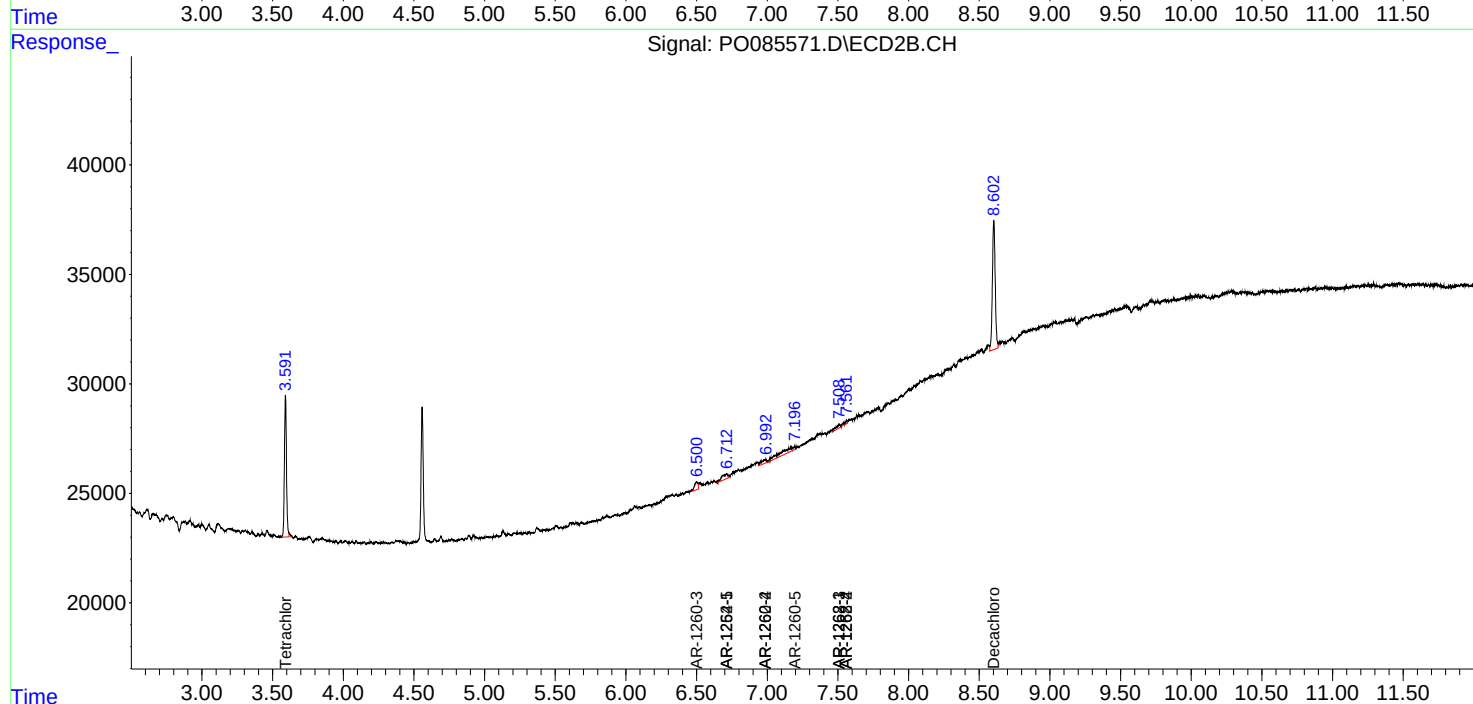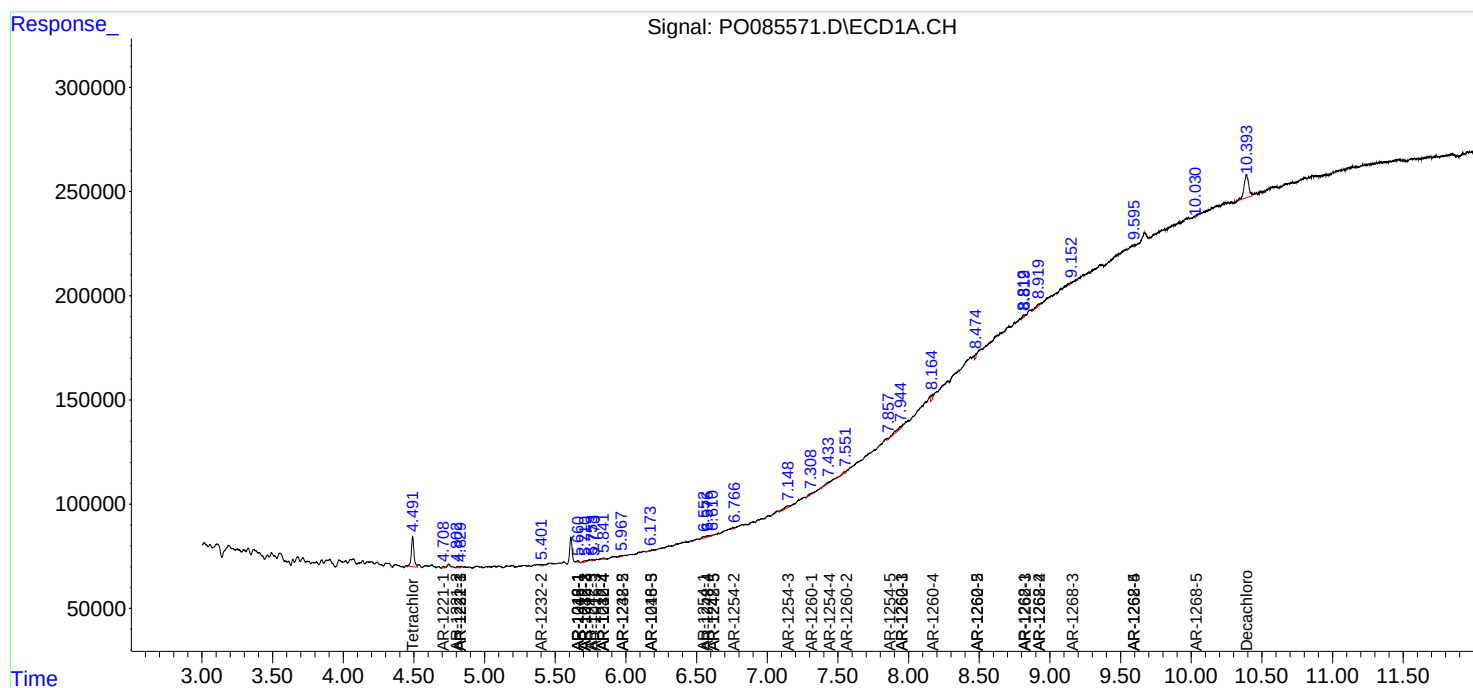


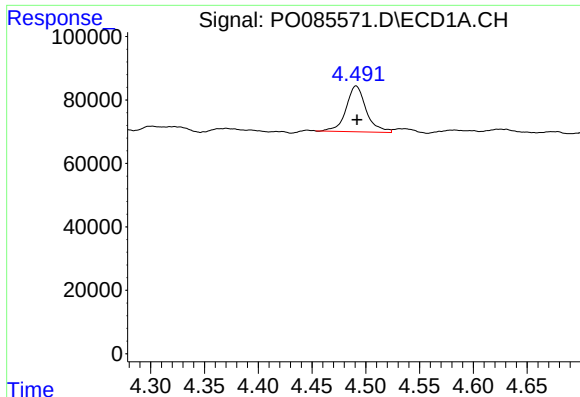

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: -0.001 min
Response: 188565
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

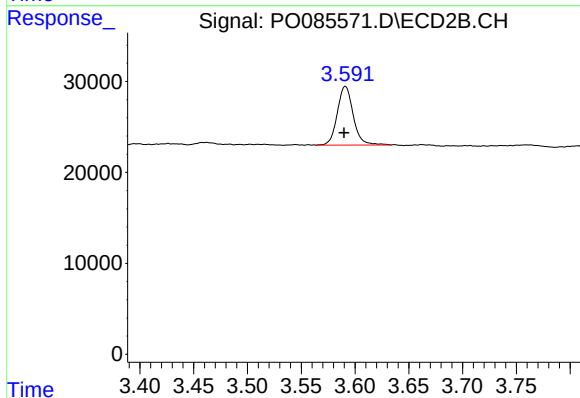


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: 0.001 min
Response: 66587
Conc: 1.55 ng/ml

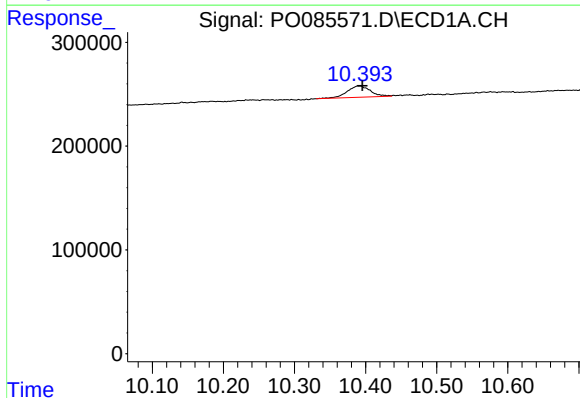


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.003 min
Response: 250009
Conc: 2.08 ng/ml

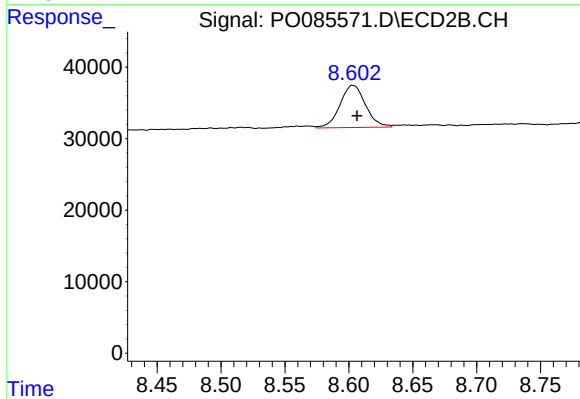

#2 Decachlorobiphenyl


R.T.: 8.603 min
Delta R.T.: -0.003 min
Response: 81854
Conc: 2.13 ng/ml

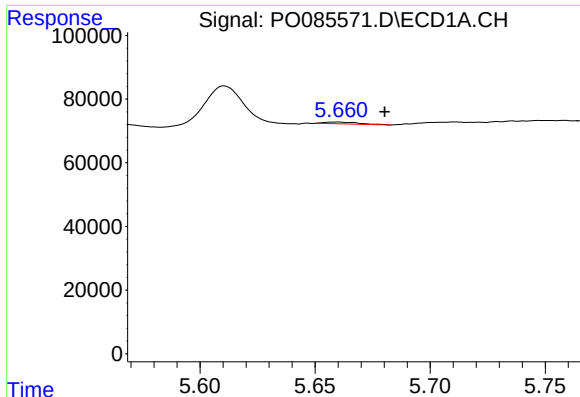

#3 AR-1016-1


R.T.: 5.660 min
Delta R.T.: -0.020 min
Response: 5782
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

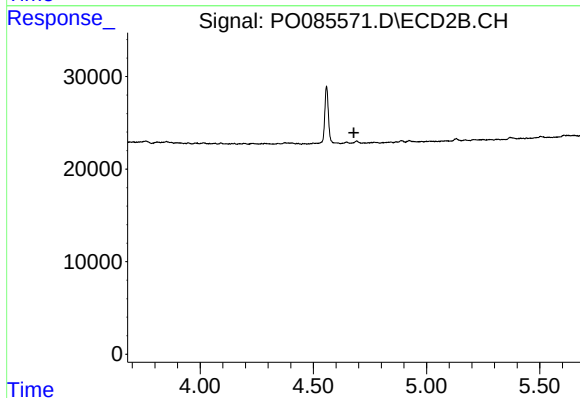


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

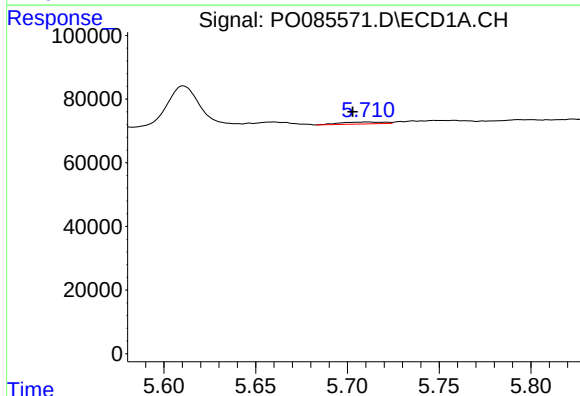


#4 AR-1016-2

R.T.: 5.710 min
Delta R.T.: 0.007 min
Response: 9729
Conc: 1.06 ng/ml

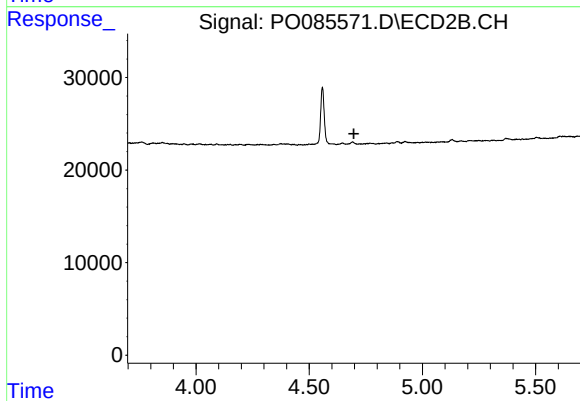

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.697 min
Response: 0
Conc: N.D.

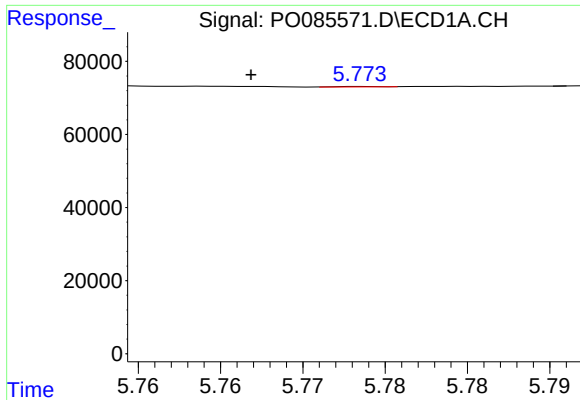

#5 AR-1016-3


R.T.: 5.774 min
Delta R.T.: 0.007 min
Response: 232
Conc: 0.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

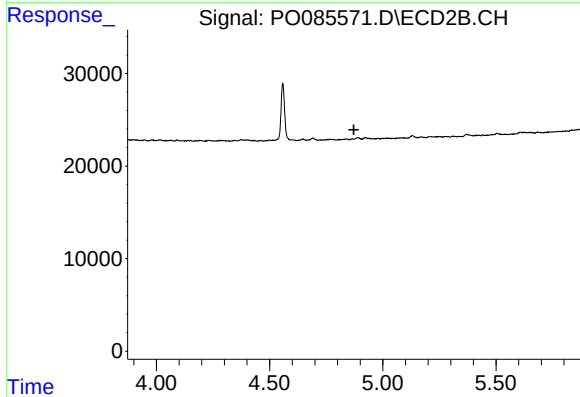


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

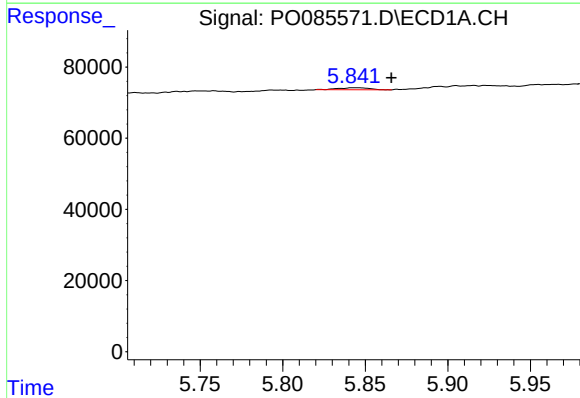


#6 AR-1016-4

R.T.: 5.842 min
Delta R.T.: -0.024 min
Response: 7266
Conc: 1.65 ng/ml

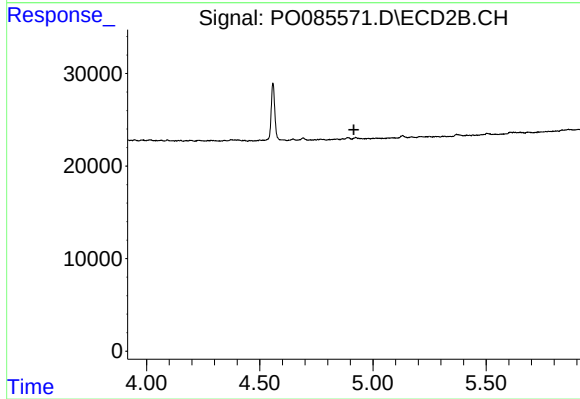

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

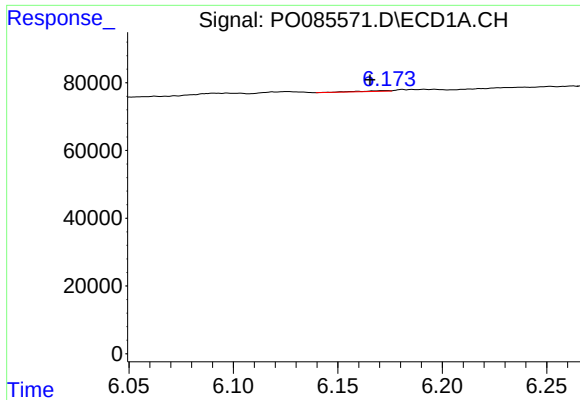

#7 AR-1016-5


R.T.: 6.174 min
Delta R.T.: 0.008 min
Response: 2436
Conc: 0.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

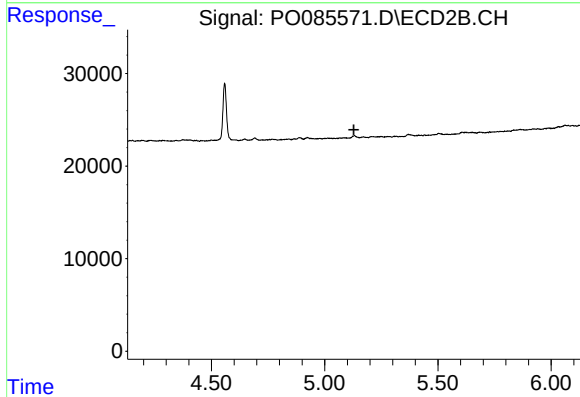


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

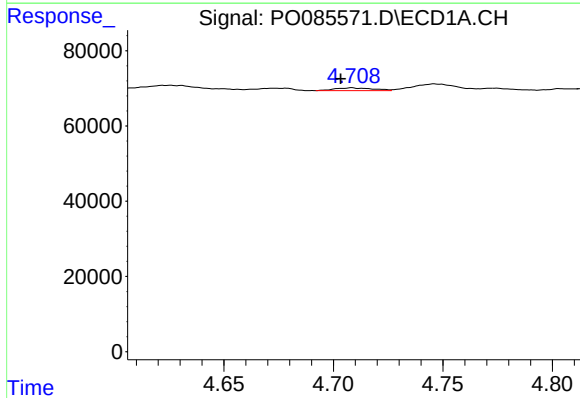


#8 AR-1221-1

R.T.: 4.708 min
Delta R.T.: 0.005 min
Response: 8780
Conc: 3.98 ng/ml

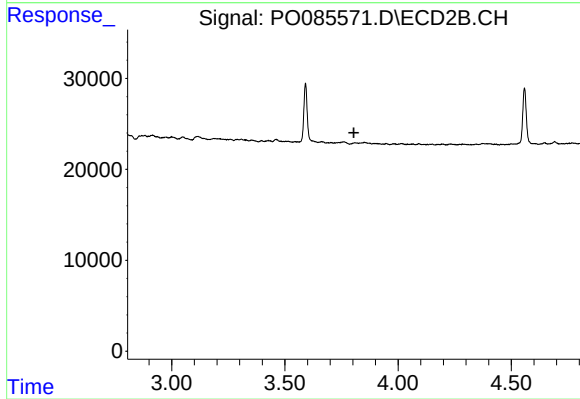

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.805 min
Response: 0
Conc: N.D.

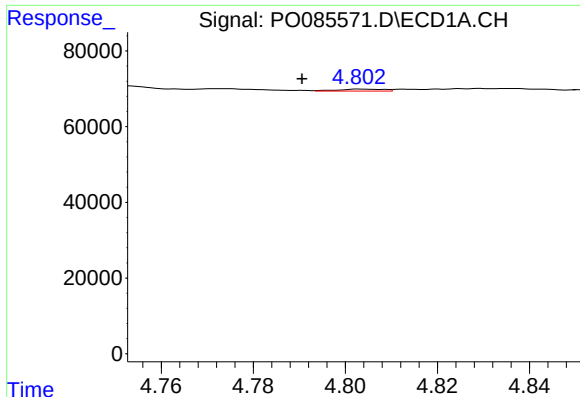

#9 AR-1221-2


R.T.: 4.803 min
Delta R.T.: 0.012 min
Response: 3678
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

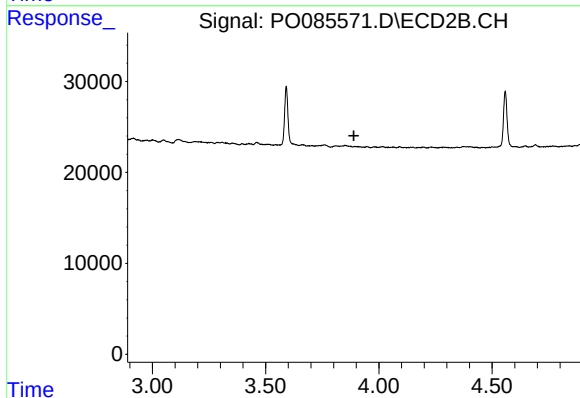


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

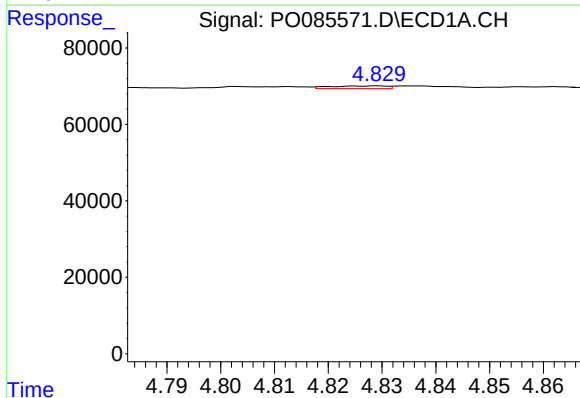


#10 AR-1221-3

R.T.: 4.829 min
Delta R.T.: -0.039 min
Response: 5081
Conc: 0.99 ng/ml

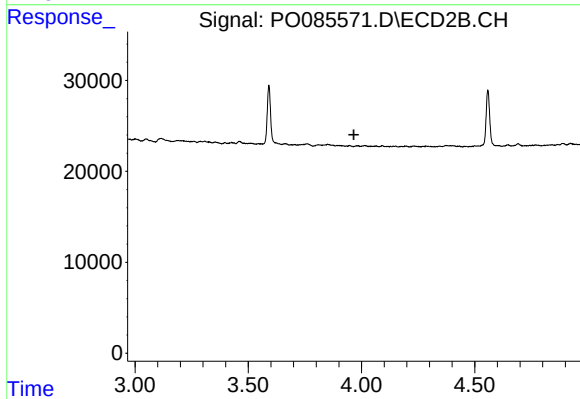

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

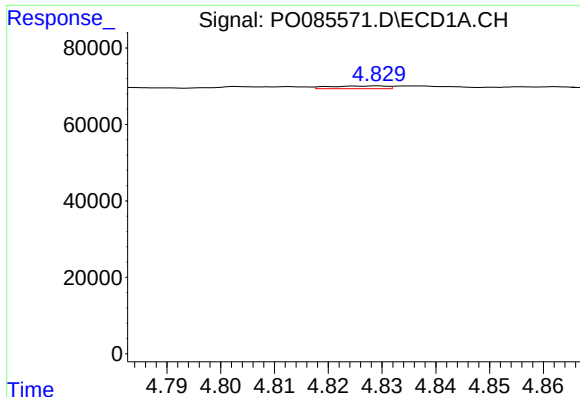

#11 AR-1232-1


R.T.: 4.829 min
Delta R.T.: -0.039 min
Response: 5081
Conc: 1.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

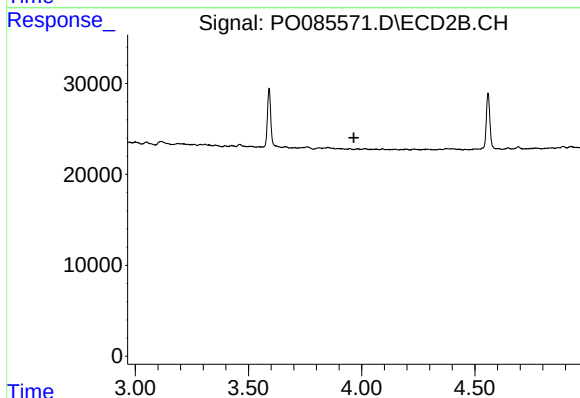


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

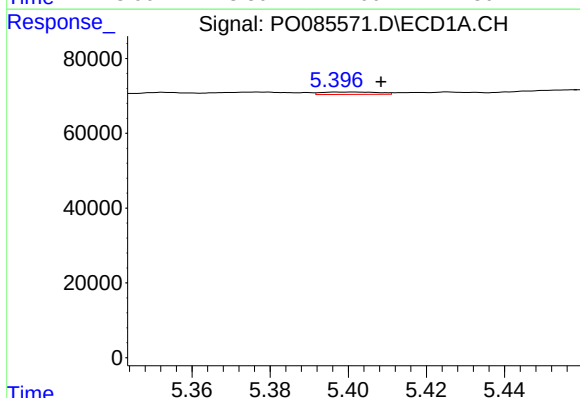


#12 AR-1232-2

R.T.: 5.401 min
Delta R.T.: -0.007 min
Response: 6323
Conc: 2.74 ng/ml

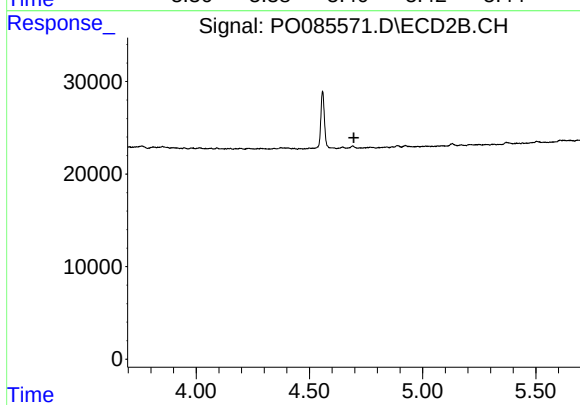

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.697 min
Response: 0
Conc: N.D.

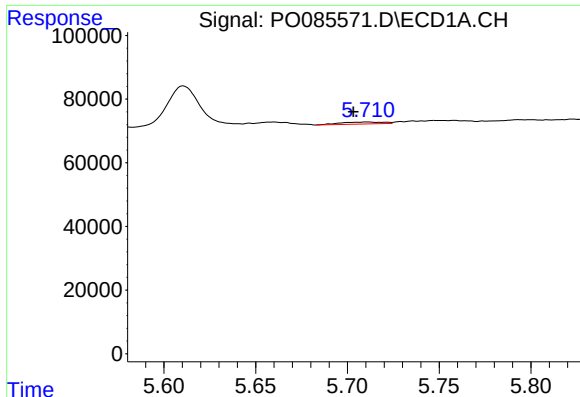

#13 AR-1232-3


R.T.: 5.710 min
Delta R.T.: 0.007 min
Response: 9729
Conc: 2.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

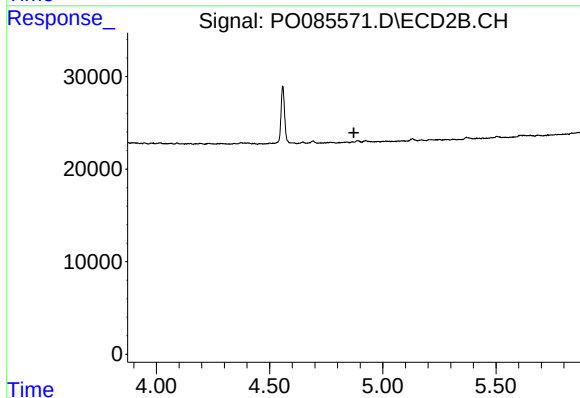


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

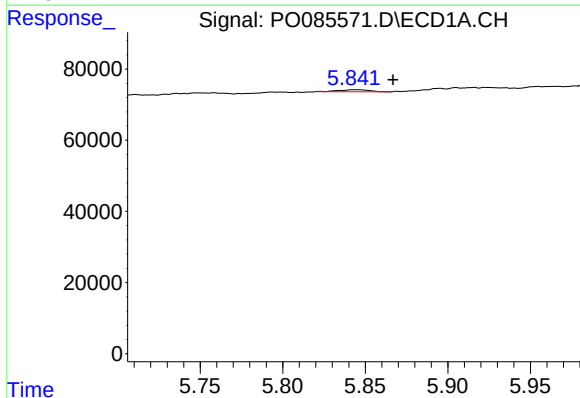


#14 AR-1232-4

R.T.: 5.842 min
Delta R.T.: -0.025 min
Response: 7266
Conc: 3.62 ng/ml

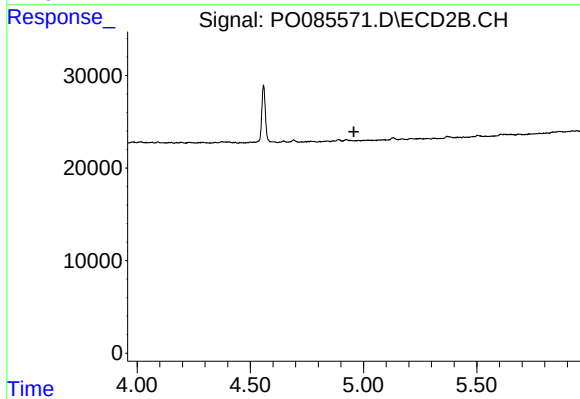

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

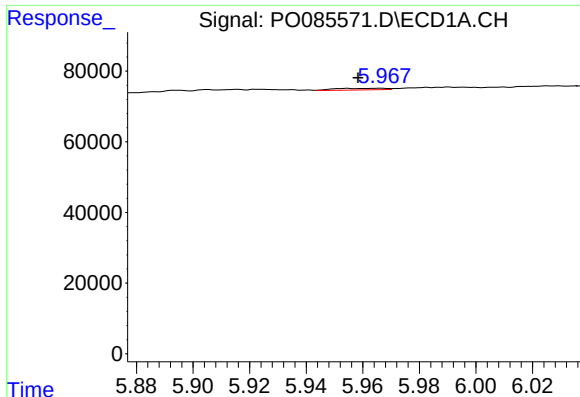

#15 AR-1232-5


R.T.: 5.967 min
Delta R.T.: 0.008 min
Response: 5556
Conc: 3.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

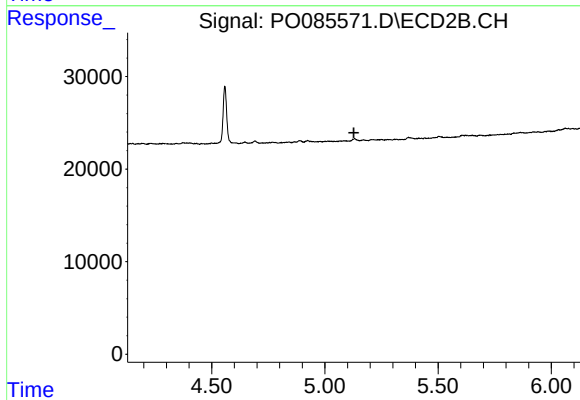


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.128 min
Response: 0
Conc: N.D.

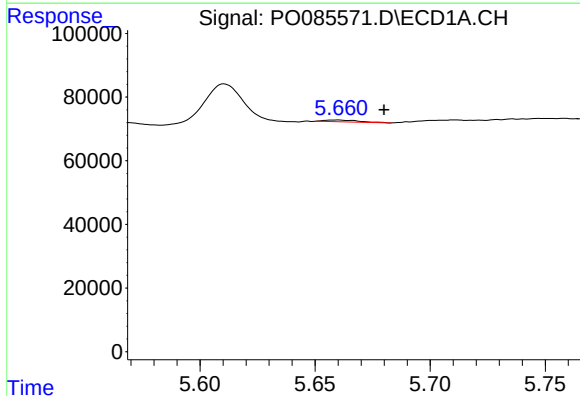


#16 AR-1242-1

R.T.: 5.660 min
Delta R.T.: -0.020 min
Response: 5782
Conc: 1.14 ng/ml

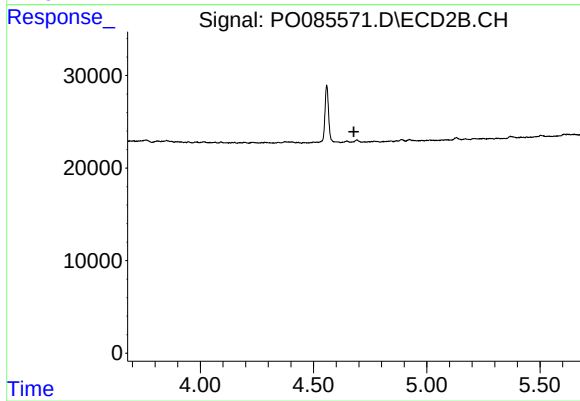

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.678 min
Response: 0
Conc: N.D.

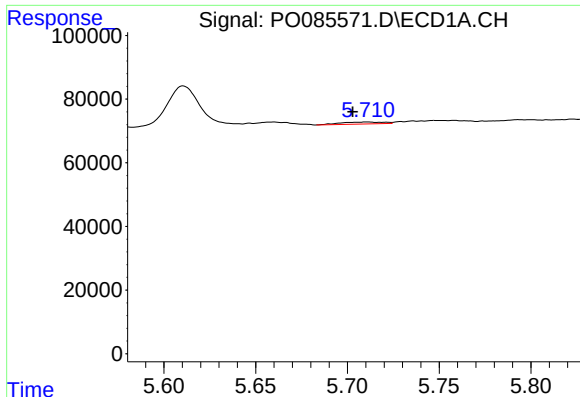

#17 AR-1242-2


R.T.: 5.710 min
Delta R.T.: 0.007 min
Response: 9729
Conc: 1.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

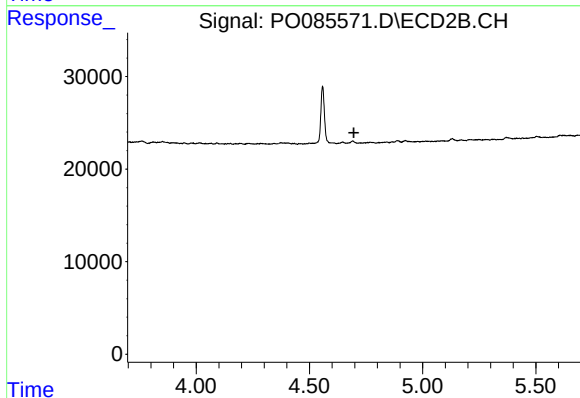


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.696 min
Response: 0
Conc: N.D.

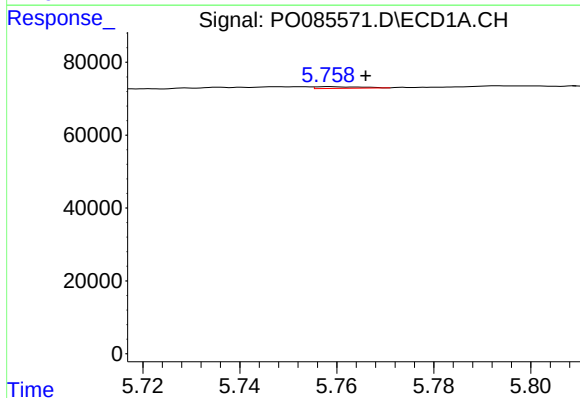


#18 AR-1242-3

R.T.: 5.758 min
Delta R.T.: -0.008 min
Response: 2983
Conc: 0.68 ng/ml

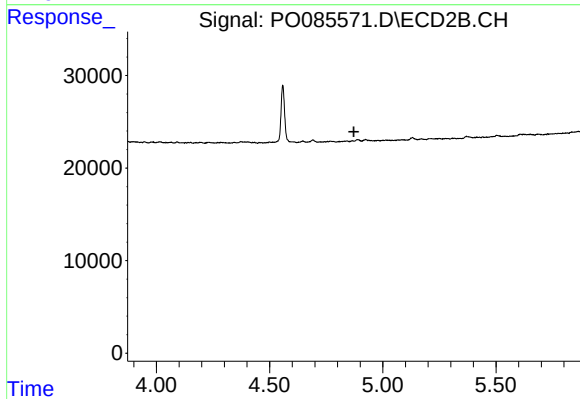

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

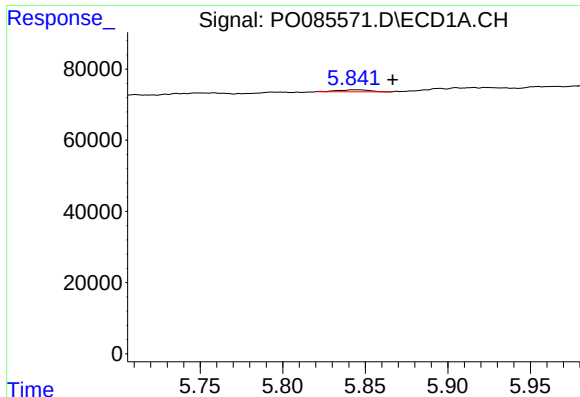

#19 AR-1242-4


R.T.: 5.842 min
Delta R.T.: -0.025 min
Response: 7266
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

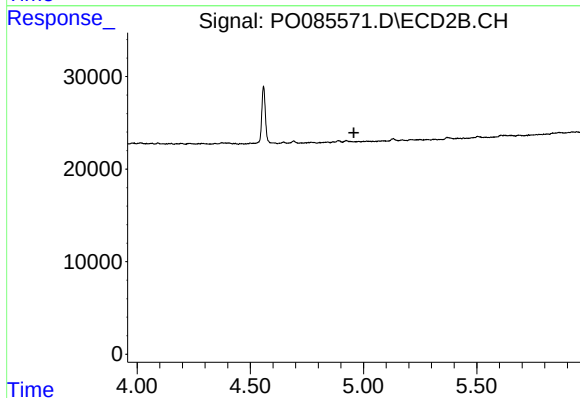


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

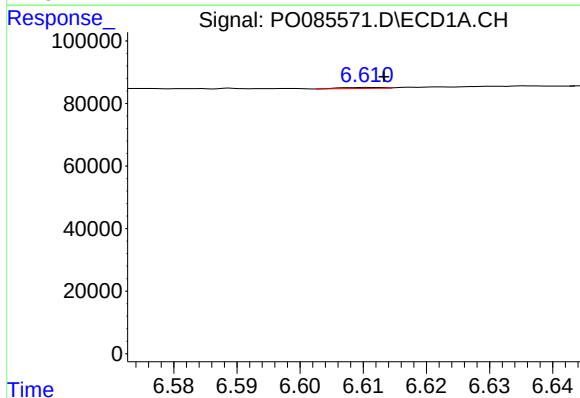


#20 AR-1242-5

R.T.: 6.611 min
Delta R.T.: -0.002 min
Response: 1496
Conc: 0.42 ng/ml

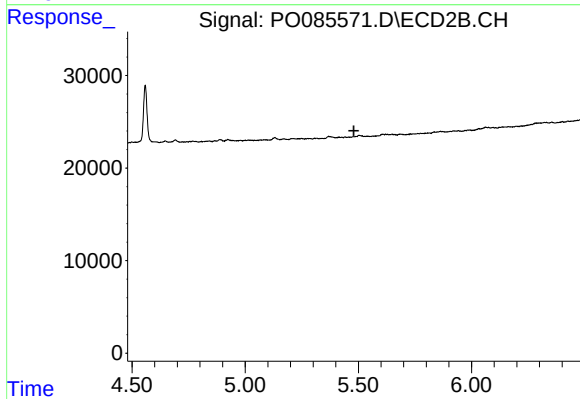

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

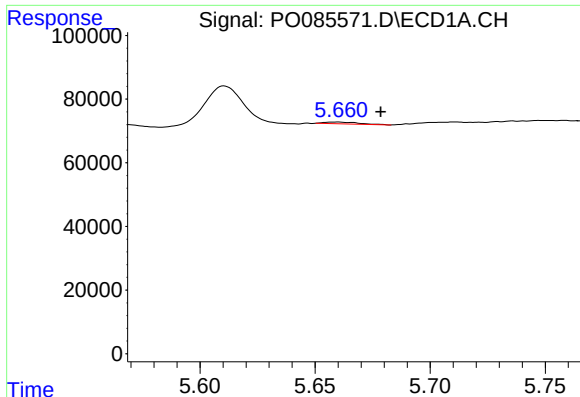

#21 AR-1248-1


R.T.: 5.660 min
Delta R.T.: -0.018 min
Response: 5782
Conc: 1.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

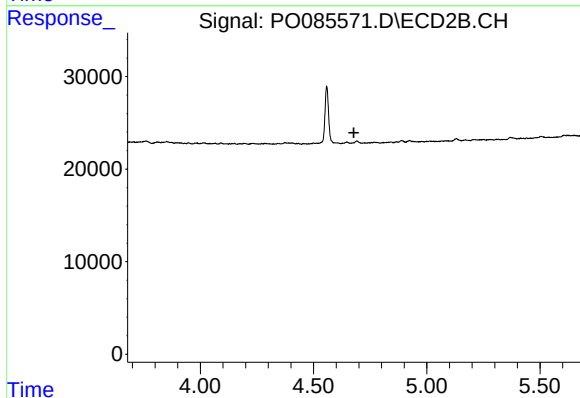


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.678 min
Response: 0
Conc: N.D.

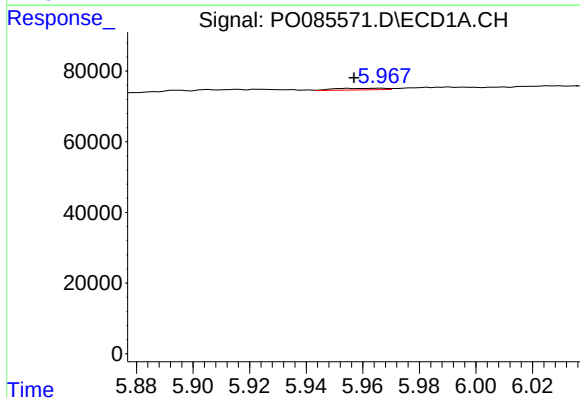


#22 AR-1248-2

R.T.: 5.967 min
Delta R.T.: 0.010 min
Response: 5556
Conc: 1.05 ng/ml

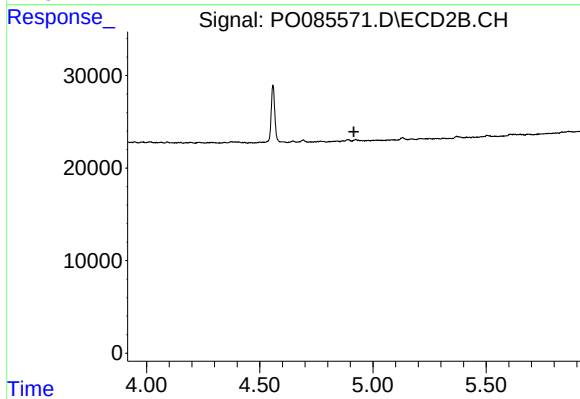

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

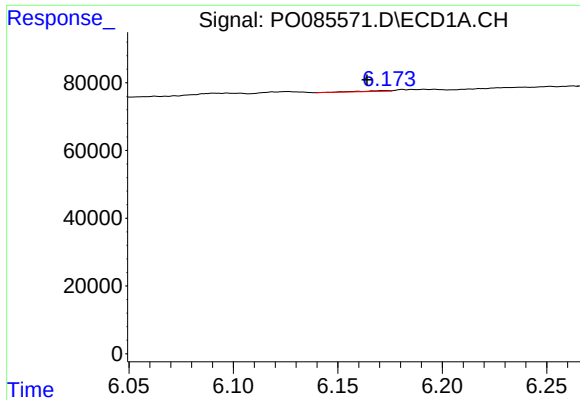

#23 AR-1248-3


R.T.: 6.174 min
Delta R.T.: 0.010 min
Response: 2436
Conc: 0.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

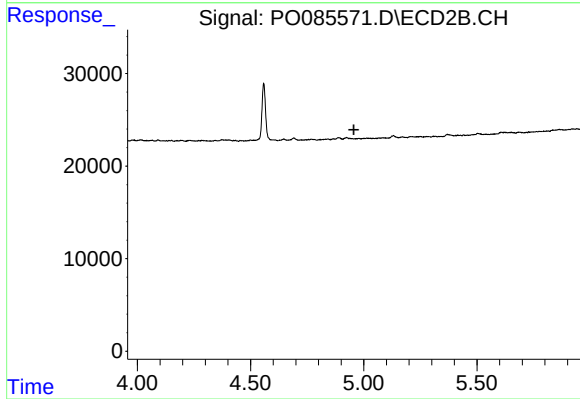


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

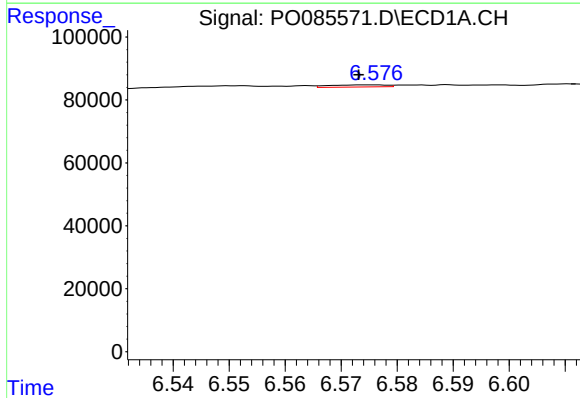


#24 AR-1248-4

R.T.: 6.576 min
Delta R.T.: 0.003 min
Response: 4958
Conc: 0.77 ng/ml

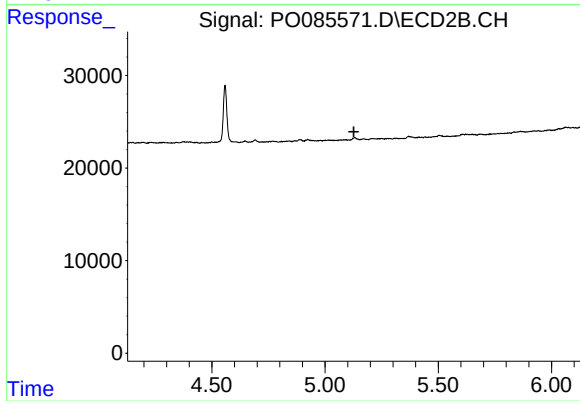

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.127 min
Response: 0
Conc: N.D.

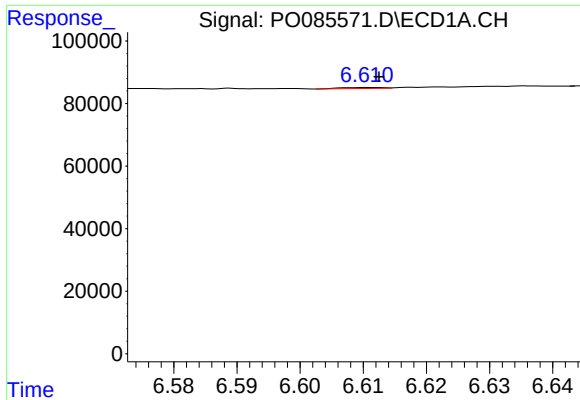

#25 AR-1248-5


R.T.: 6.611 min
Delta R.T.: -0.002 min
Response: 1496
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

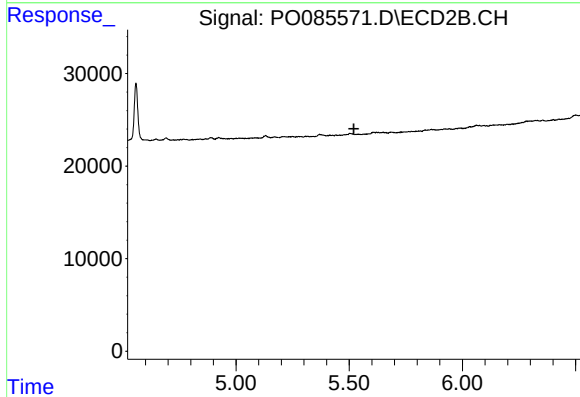


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.521 min
Response: 0
Conc: N.D.

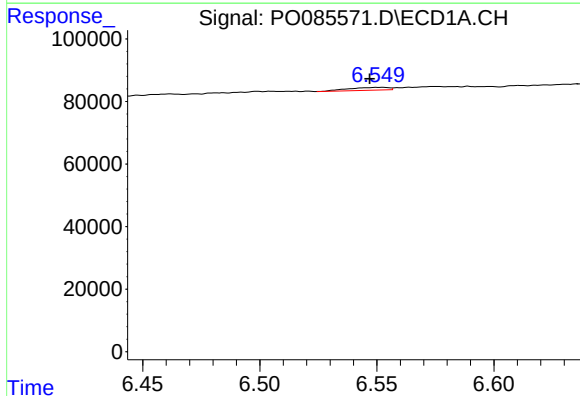


#26 AR-1254-1

R.T.: 6.553 min
Delta R.T.: 0.006 min
Response: 10477
Conc: 1.58 ng/ml

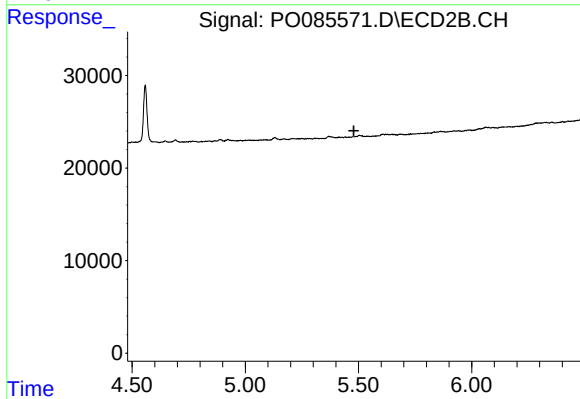

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

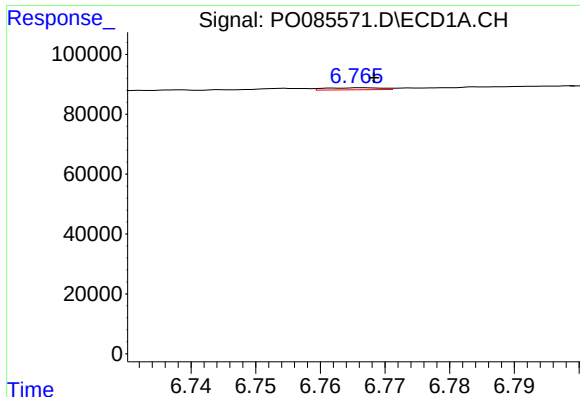

#27 AR-1254-2


R.T.: 6.766 min
Delta R.T.: -0.002 min
Response: 4133
Conc: 0.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

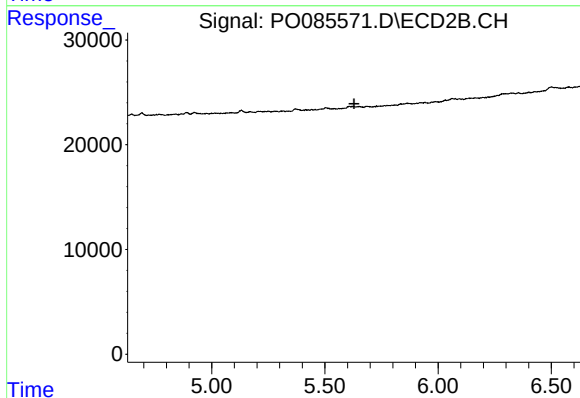


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.628 min
Response: 0
Conc: N.D.

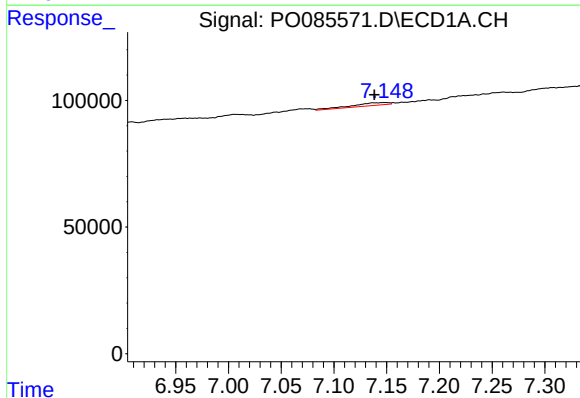


#28 AR-1254-3

R.T.: 7.148 min
Delta R.T.: 0.009 min
Response: 25737
Conc: 2.50 ng/ml

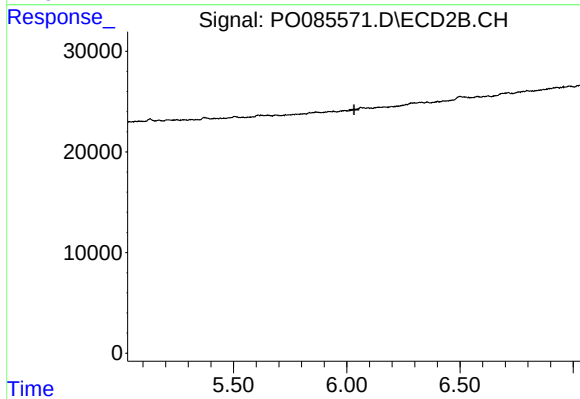

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.032 min
Response: 0
Conc: N.D.

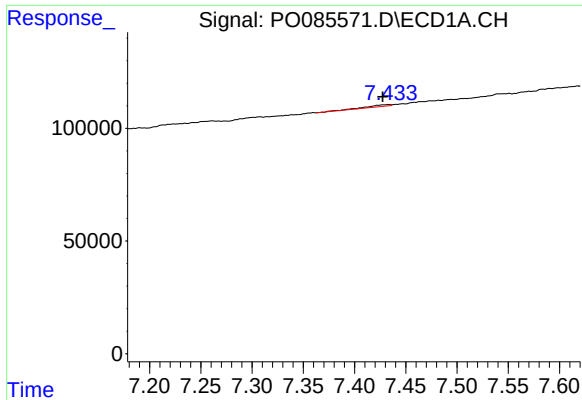

#29 AR-1254-4


R.T.: 7.433 min
Delta R.T.: 0.005 min
Response: 12645
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

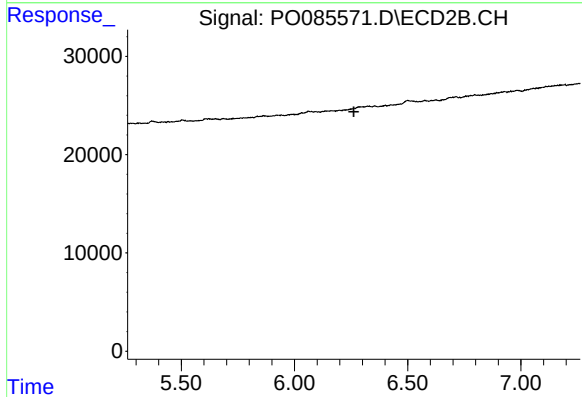


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.262 min
Response: 0
Conc: N.D.

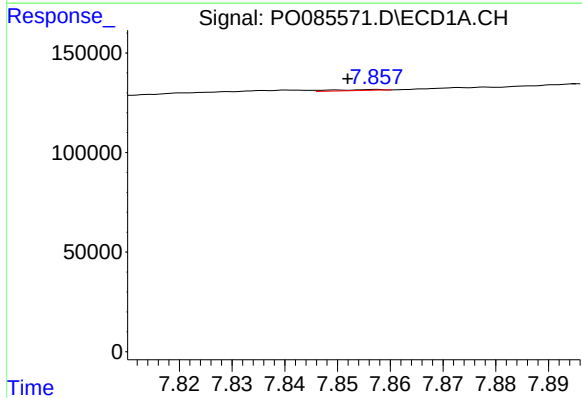


#30 AR-1254-5

R.T.: 7.857 min
Delta R.T.: 0.006 min
Response: 3307
Conc: 0.43 ng/ml

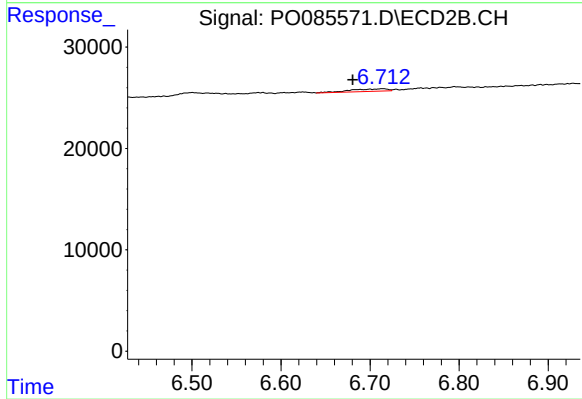

#30 AR-1254-5


R.T.: 6.714 min
Delta R.T.: 0.033 min
Response: 6980
Conc: 2.15 ng/ml

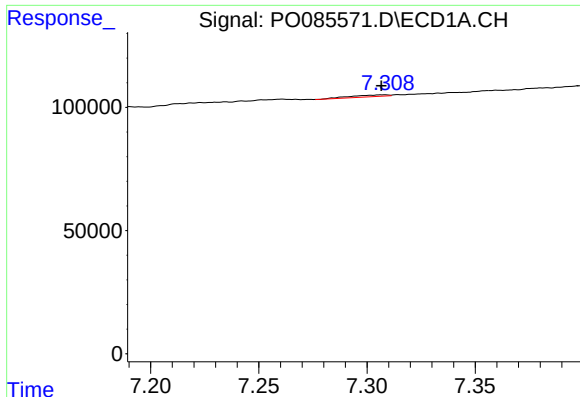

#31 AR-1260-1


R.T.: 7.308 min
Delta R.T.: 0.002 min
Response: 8507
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

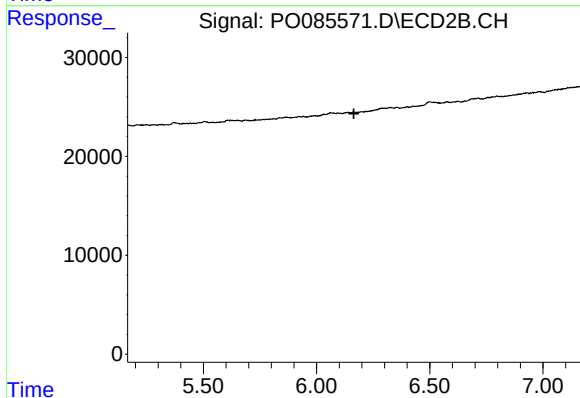


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.165 min
Response: 0
Conc: N.D.

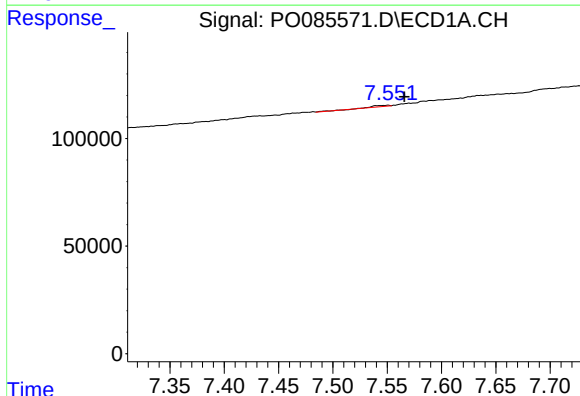


#32 AR-1260-2

R.T.: 7.551 min
Delta R.T.: -0.015 min
Response: 6401
Conc: 0.82 ng/ml

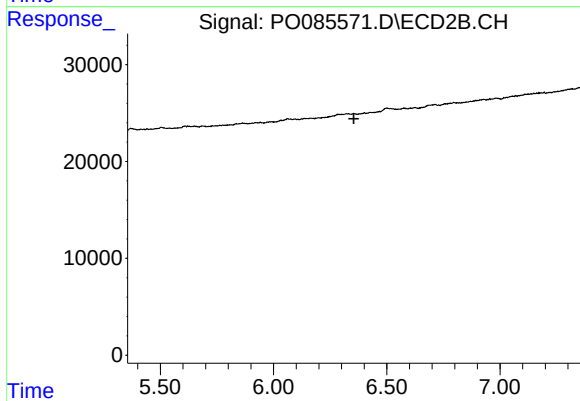

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

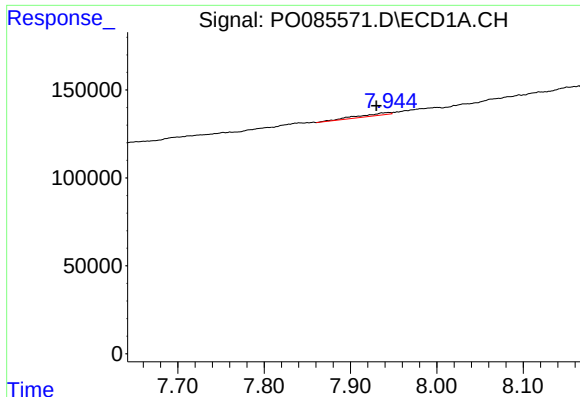

#33 AR-1260-3


R.T.: 7.944 min
Delta R.T.: 0.014 min
Response: 37614
Conc: 6.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

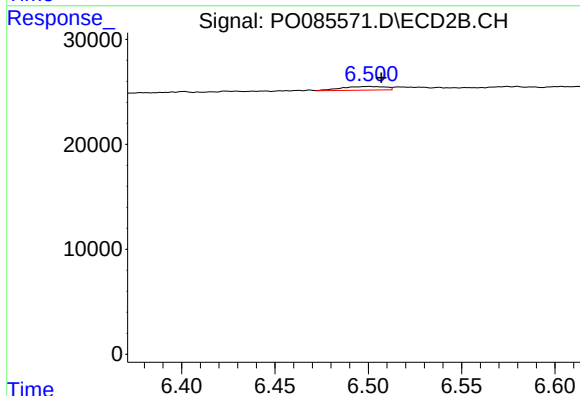


#33 AR-1260-3

R.T.: 6.501 min
Delta R.T.: -0.007 min
Response: 5866
Conc: 2.23 ng/ml

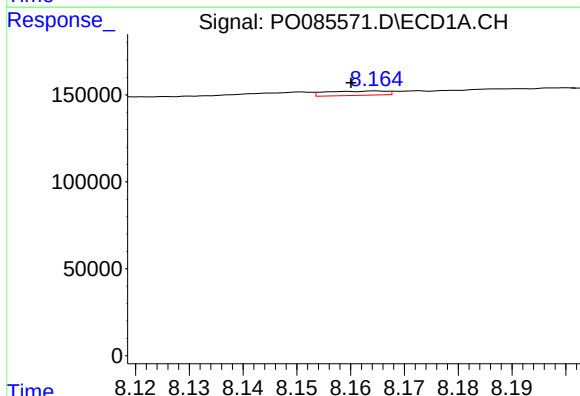


#34 AR-1260-4

R.T.: 8.165 min
Delta R.T.: 0.005 min
Response: 19150
Conc: 2.77 ng/ml

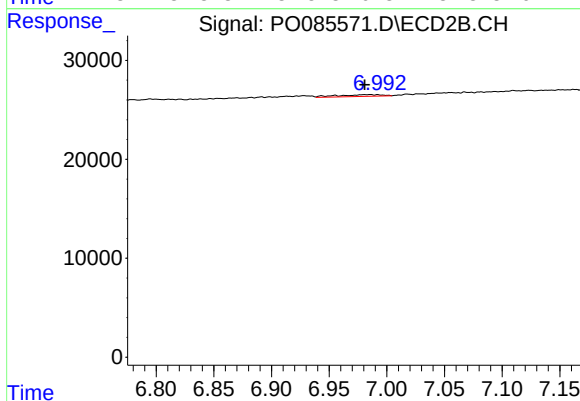

#34 AR-1260-4


R.T.: 6.992 min
Delta R.T.: 0.011 min
Response: 4858
Conc: 2.17 ng/ml

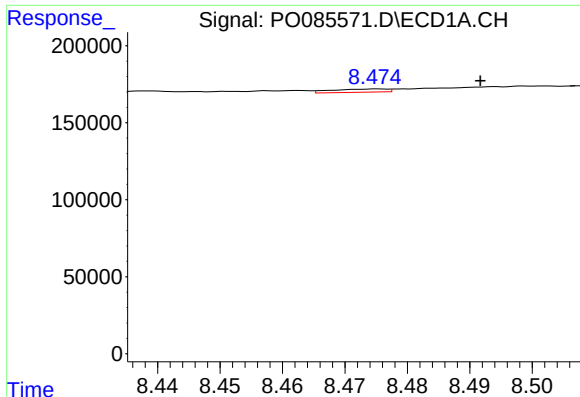

#35 AR-1260-5


R.T.: 8.475 min
Delta R.T.: -0.016 min
Response: 13004
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

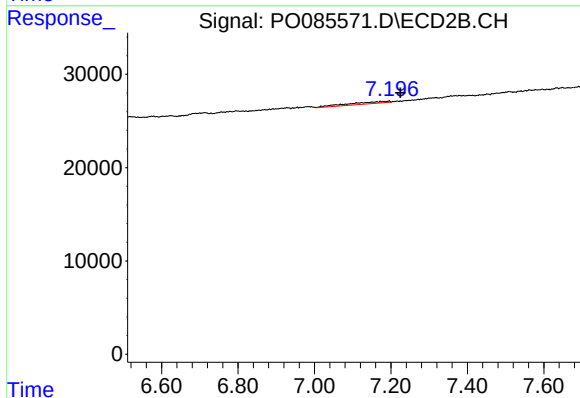


#35 AR-1260-5

R.T.: 7.196 min
Delta R.T.: -0.029 min
Response: 15541
Conc: 3.08 ng/ml

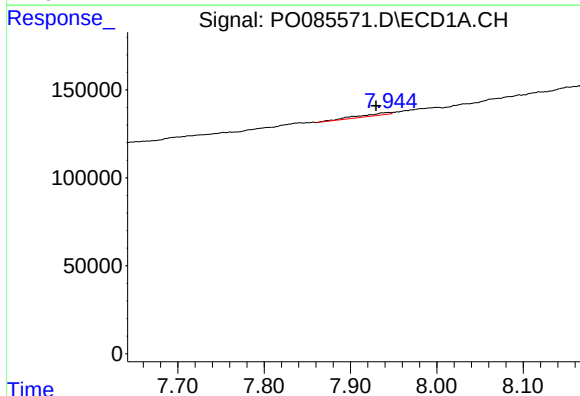


#36 AR-1262-1

R.T.: 7.944 min
Delta R.T.: 0.015 min
Response: 37614
Conc: 4.16 ng/ml

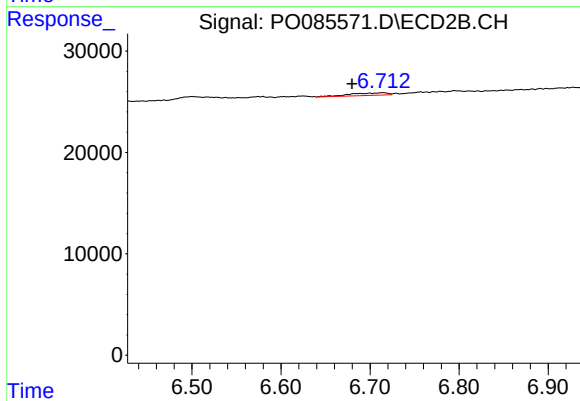

#36 AR-1262-1


R.T.: 6.714 min
Delta R.T.: 0.034 min
Response: 6980
Conc: 4.07 ng/ml

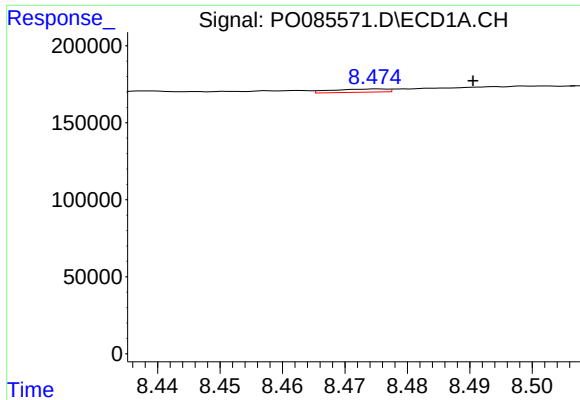

#37 AR-1262-2


R.T.: 8.475 min
Delta R.T.: -0.015 min
Response: 13004
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

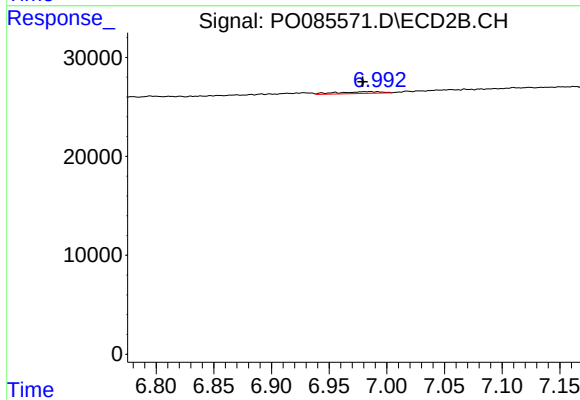


#37 AR-1262-2

R.T.: 6.992 min
Delta R.T.: 0.013 min
Response: 4858
Conc: 1.70 ng/ml

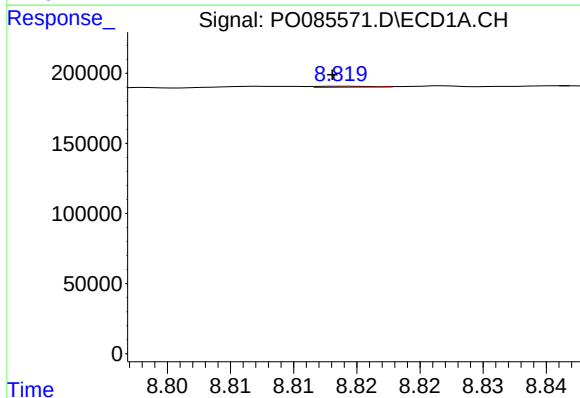


#38 AR-1262-3

R.T.: 8.819 min
Delta R.T.: 0.001 min
Response: 2448
Conc: 0.24 ng/ml

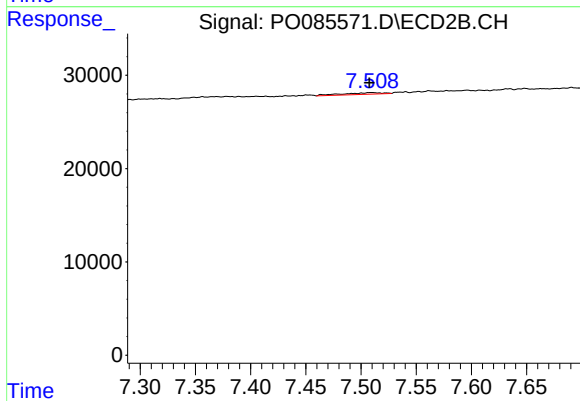

#38 AR-1262-3


R.T.: 7.509 min
Delta R.T.: 0.001 min
Response: 4256
Conc: 1.94 ng/ml

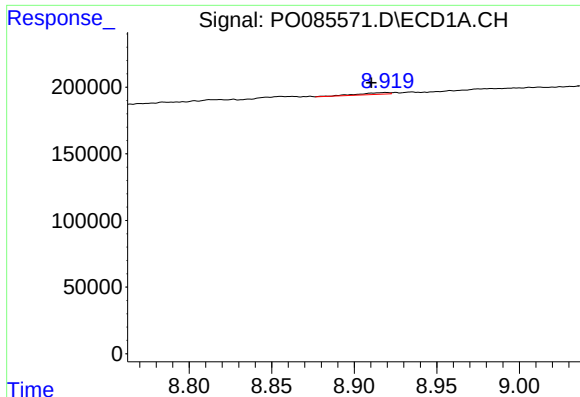

#39 AR-1262-4


R.T.: 8.919 min
Delta R.T.: 0.009 min
Response: 16227
Conc: 3.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

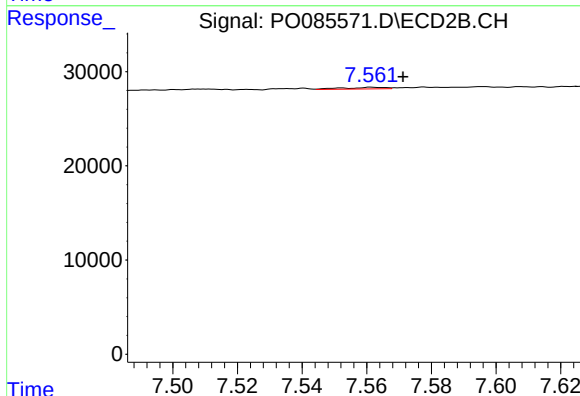


#39 AR-1262-4

R.T.: 7.562 min
Delta R.T.: -0.009 min
Response: 1468
Conc: 0.37 ng/ml

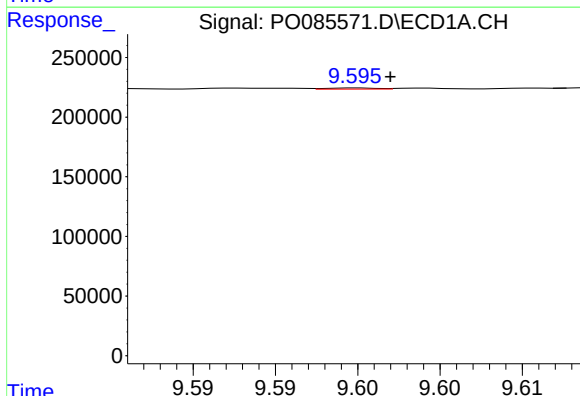


#40 AR-1262-5

R.T.: 9.595 min
Delta R.T.: -0.002 min
Response: 1920
Conc: 0.36 ng/ml

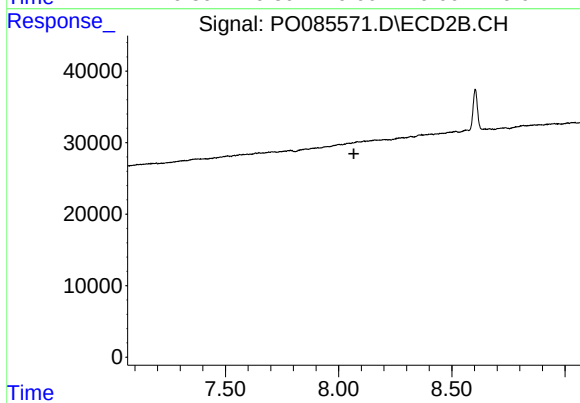

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.067 min
Response: 0
Conc: N.D.

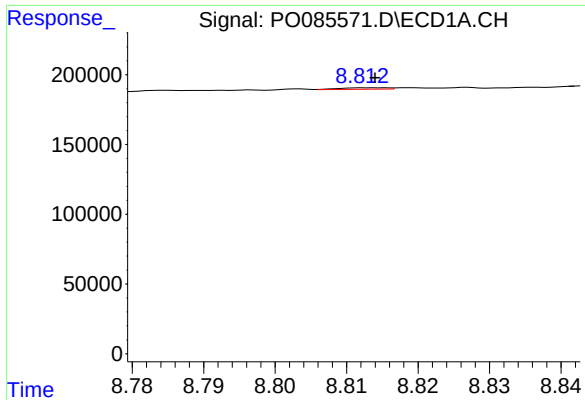

#41 AR-1268-1


R.T.: 8.815 min
Delta R.T.: 0.000 min
Response: 4926
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

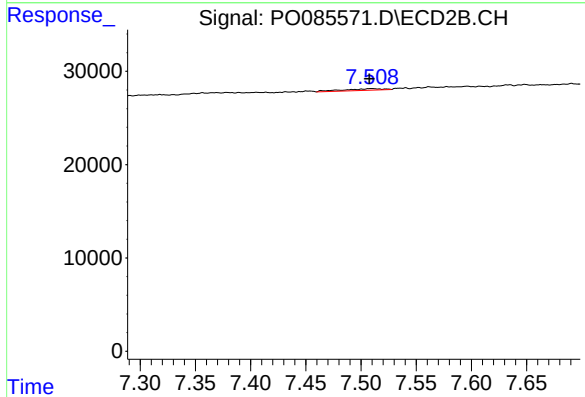


#41 AR-1268-1

R.T.: 7.509 min
Delta R.T.: 0.001 min
Response: 4256
Conc: 0.64 ng/ml

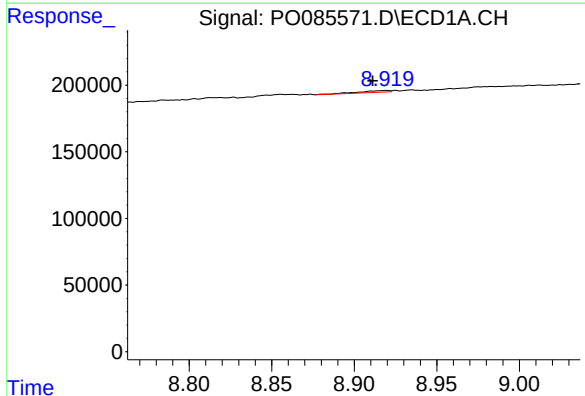


#42 AR-1268-2

R.T.: 8.919 min
Delta R.T.: 0.008 min
Response: 16227
Conc: 0.93 ng/ml

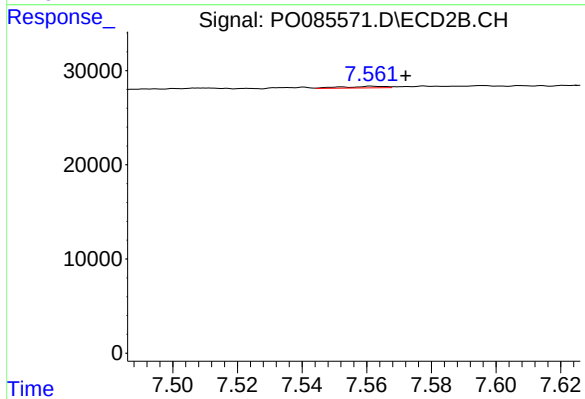

#42 AR-1268-2


R.T.: 7.562 min
Delta R.T.: -0.010 min
Response: 1468
Conc: 0.25 ng/ml

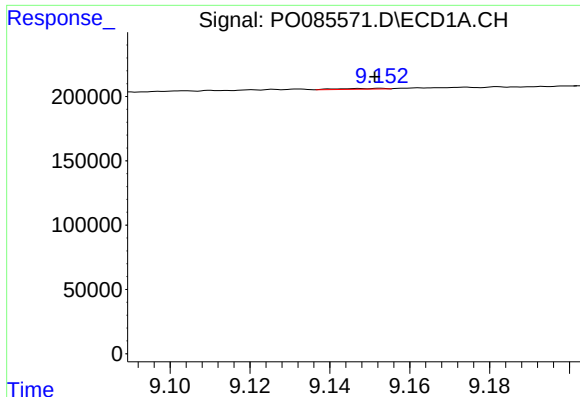

#43 AR-1268-3


R.T.: 9.153 min
Delta R.T.: 0.001 min
Response: 4782
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

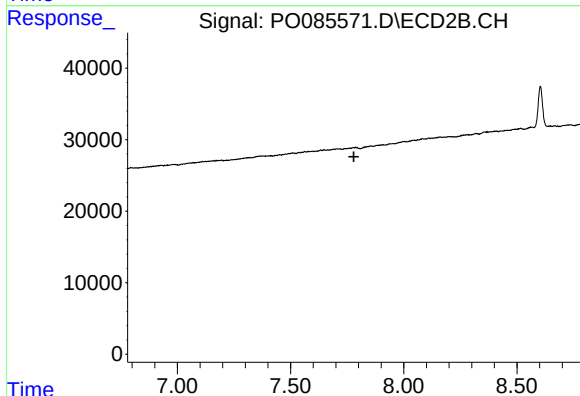


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

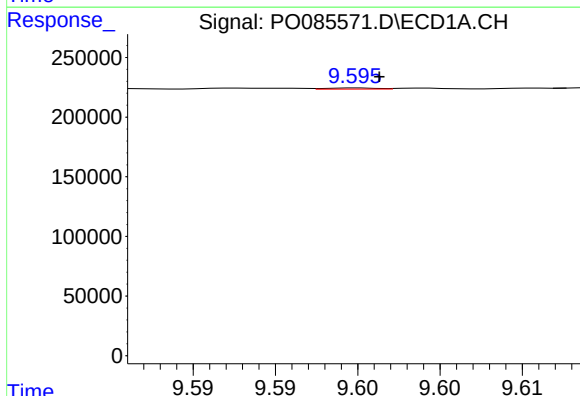


#44 AR-1268-4

R.T.: 9.595 min
Delta R.T.: -0.001 min
Response: 1920
Conc: 0.31 ng/ml

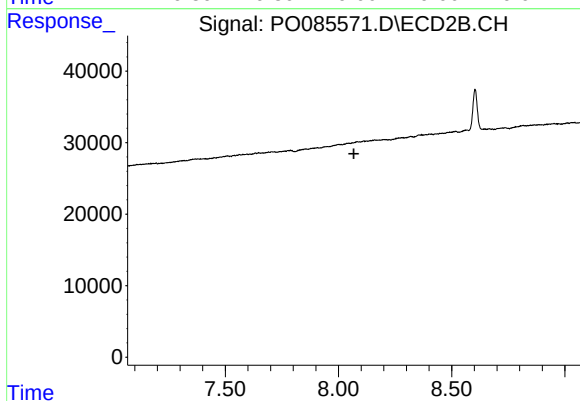

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.068 min
Response: 0
Conc: N.D.

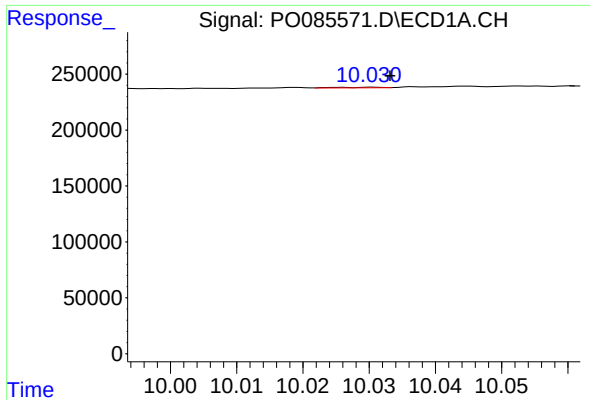

#45 AR-1268-5

R.T.: 10.031 min
Delta R.T.: -0.003 min
Response: 2882
Conc: 0.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-35B

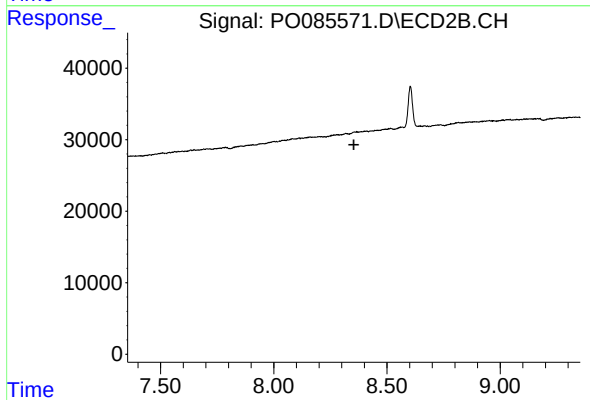

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.