

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
 Data File : P0085573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 16:20
 Operator : YP\AJ
 Sample : N2055-10 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-34B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:15:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.490	3.590	253477	67100	1.240	1.566 #
2)	SA Decachlor...	10.390	8.604	226736	83414	1.886	2.173
Target Compounds							
3)	L1 AR-1016-1	5.707	0.000	4937	0	0.785	N.D. #
4)	L1 AR-1016-2	5.707	0.000	4937	0	0.539	N.D. #
5)	L1 AR-1016-3	5.764	4.866	2510	4282	0.461	3.427 #
6)	L1 AR-1016-4	5.856	4.866f	6165	4282	1.398	3.923 #
7)	L1 AR-1016-5	6.210f	0.000	43203	0	10.175	N.D. #
8)	L2 AR-1221-1	4.711	3.742f	9298	5794	4.215	11.234 #
9)	L2 AR-1221-2	4.798	0.000	4878	0	2.995	N.D. #
10)	L2 AR-1221-3	4.863	0.000	2233	0	0.434	N.D. #
11)	L3 AR-1232-1	4.863	0.000	2233	0	0.475	N.D. #
12)	L3 AR-1232-2	5.410	0.000	1761	0	0.764	N.D. #
13)	L3 AR-1232-3	5.707	4.866	4937	4282	1.170	7.047 #
14)	L3 AR-1232-4	5.856	0.000	6165	0	3.070	N.D. #
15)	L3 AR-1232-5	5.957	0.000	21614	0	14.685	N.D. #
16)	L4 AR-1242-1	5.707	0.000	4937	0	0.971	N.D. #
17)	L4 AR-1242-2	5.707	0.000	4937	0	0.665	N.D. #
18)	L4 AR-1242-3	5.764	4.866	2510	4282	0.571	4.235 #
19)	L4 AR-1242-4	5.856	0.000	6165	0	1.699	N.D. #
20)	L4 AR-1242-5	6.616	0.000	1944	0	0.547	N.D. #
21)	L5 AR-1248-1	5.707	0.000	4937	0	1.324	N.D. #
22)	L5 AR-1248-2	5.957	4.866f	21614	4282	4.078	2.925 #
23)	L5 AR-1248-3	6.210f	0.000	43203	0	7.343	N.D. #
24)	L5 AR-1248-4	6.571	0.000	2186	0	0.339	N.D. #
25)	L5 AR-1248-5	6.616	5.557f	1944	12905	0.314	7.514 #
26)	L6 AR-1254-1	6.543	0.000	8750	0	1.320	N.D. #
27)	L6 AR-1254-2	6.769	5.613	2248	5078	0.225	2.176 #
28)	L6 AR-1254-3	7.151	6.036	28321	4031	2.752	1.098 #
29)	L6 AR-1254-4	7.431	0.000	13832	0	1.972	N.D. #
30)	L6 AR-1254-5	7.856	0.000	2554	0	0.334	N.D. #
31)	L7 AR-1260-1	7.309	0.000	3785	0	0.549	N.D. #
32)	L7 AR-1260-2	7.576	0.000	9935	0	1.270	N.D. #
33)	L7 AR-1260-3	7.945	6.500	48216	5516	8.209	2.098 #
34)	L7 AR-1260-4	8.159	0.000	51007	0	7.385	N.D. #
35)	L7 AR-1260-5	8.497	0.000	16851	0	1.199	N.D. #
36)	L8 AR-1262-1	7.945	0.000	48216	0	5.338	N.D. #
37)	L8 AR-1262-2	8.497	0.000	16851	0	1.058	N.D. #
38)	L8 AR-1262-3	8.810	0.000	1926	0	0.186	N.D. #
39)	L8 AR-1262-4	8.912	0.000	3843	0	0.818	N.D. #
40)	L8 AR-1262-5	9.602	0.000	3474	0	0.653	N.D. #
41)	L9 AR-1268-1	8.810	0.000	1926	0	0.100	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
Data File : P0085573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 16:20
Operator : YP\AJ
Sample : N2055-10 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	8.912	0.000	3843	0	0.221	N.D.	#
43)	L9 AR-1268-3	9.156	0.000	3546	0	0.240	N.D.	#
44)	L9 AR-1268-4	9.602	0.000	3474	0	0.569	N.D.	#
45)	L9 AR-1268-5	10.029	0.000	1538	0	0.032	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
Data File : P0085573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 16:20
Operator : YP\AJ
Sample : N2055-10 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

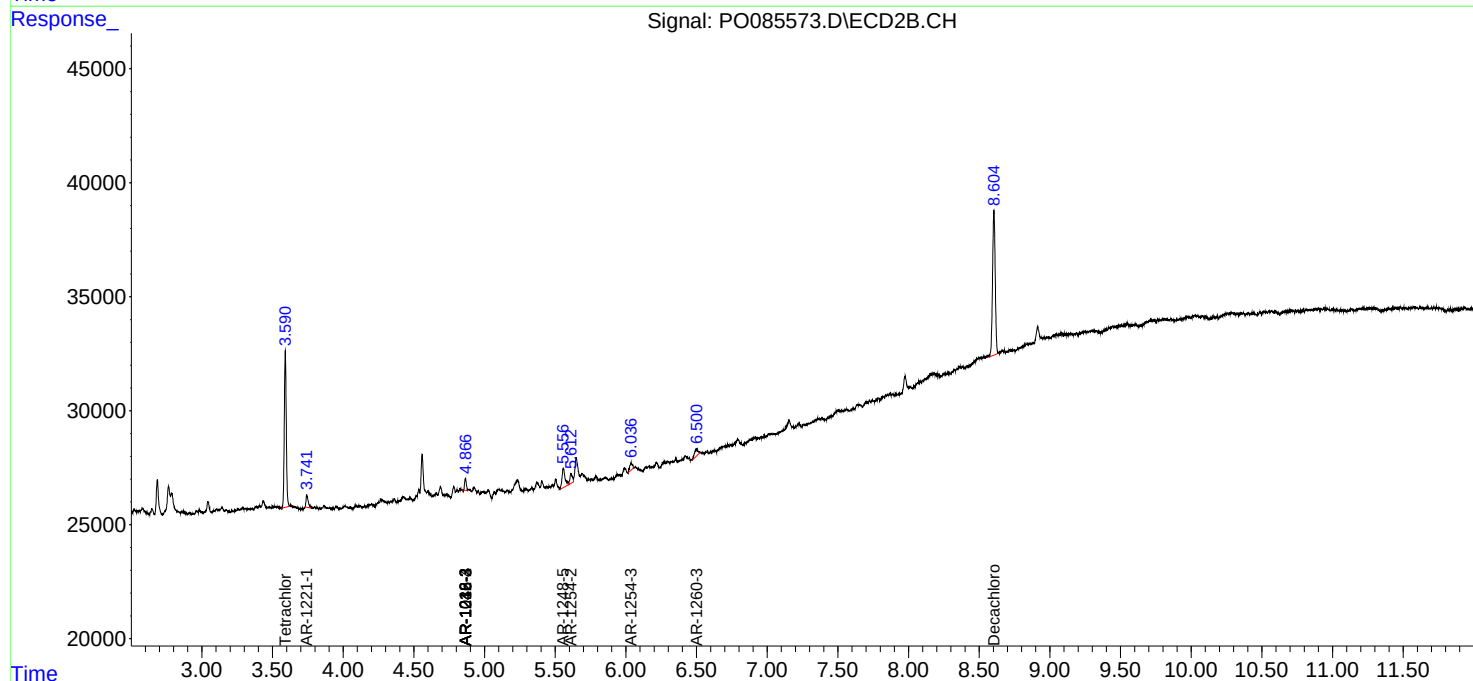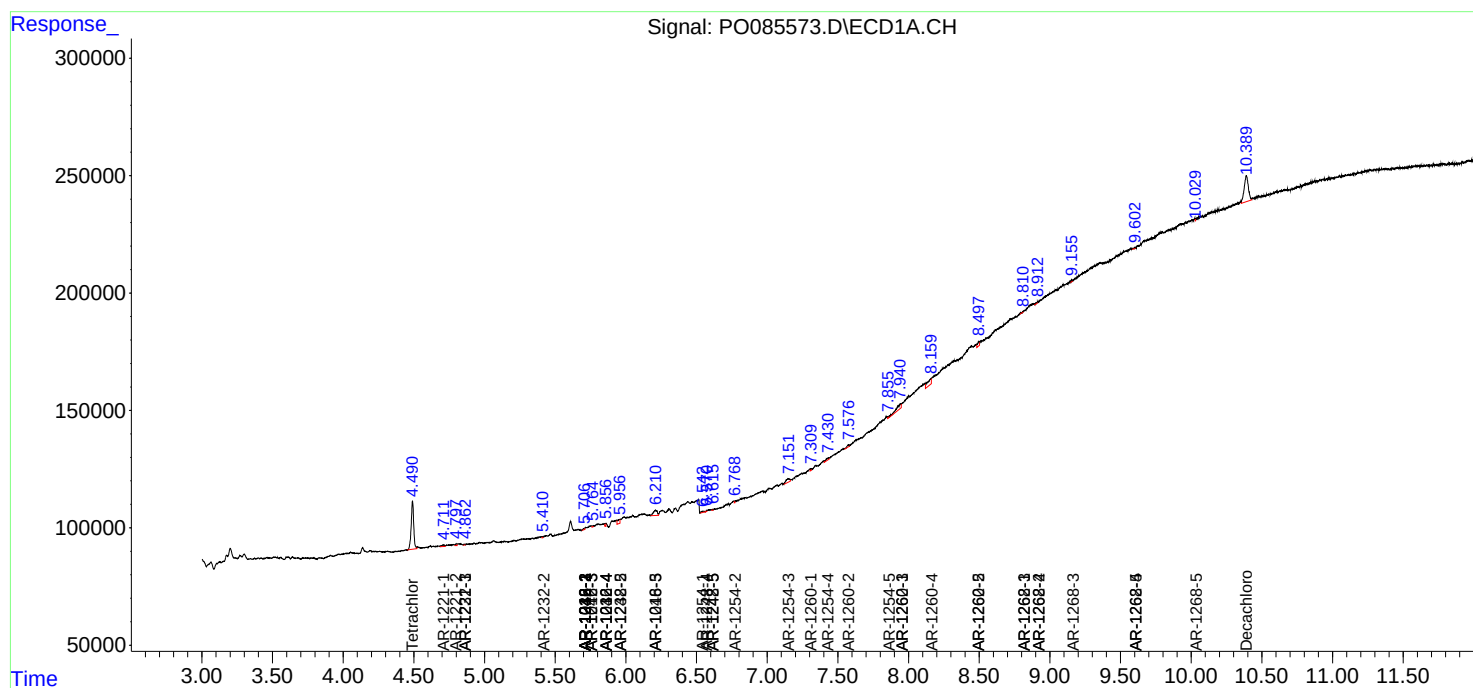


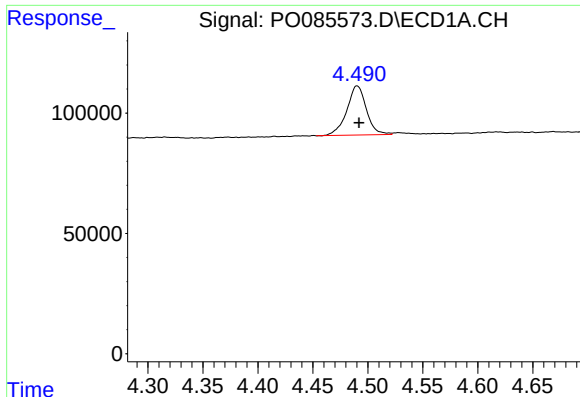

#1 Tetrachloro-m-xylene


R.T.: 4.490 min
Delta R.T.: -0.002 min
Response: 253477
Conc: 1.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

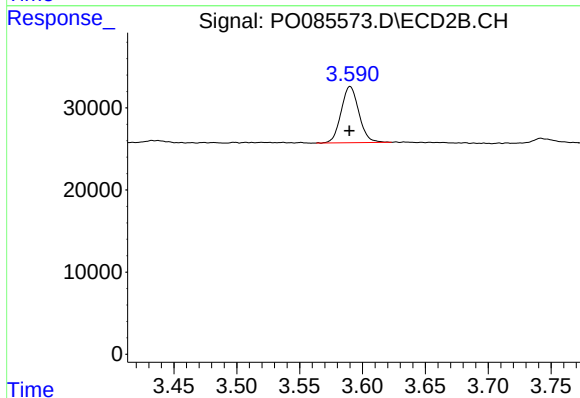


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: 0.000 min
Response: 67100
Conc: 1.57 ng/ml

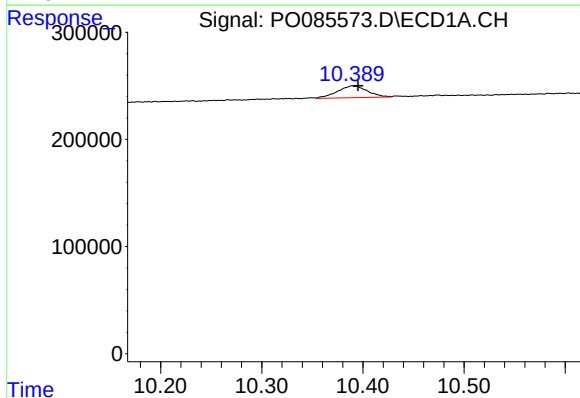


#2 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.006 min
Response: 226736
Conc: 1.89 ng/ml

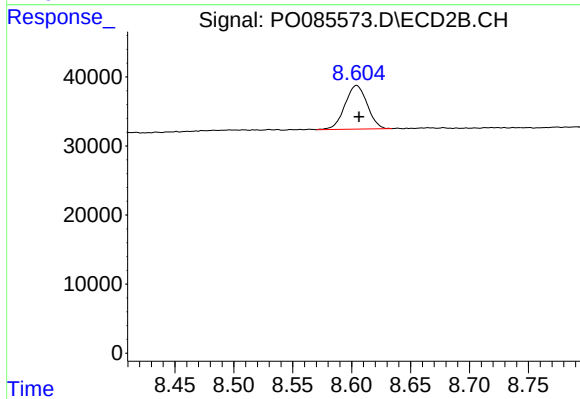

#2 Decachlorobiphenyl


R.T.: 8.604 min
Delta R.T.: -0.002 min
Response: 83414
Conc: 2.17 ng/ml

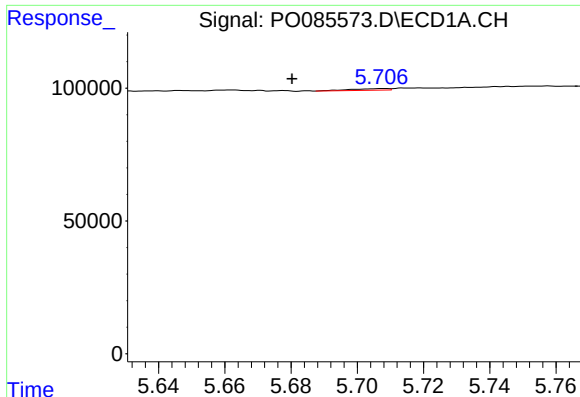

#3 AR-1016-1


R.T.: 5.707 min
Delta R.T.: 0.027 min
Response: 4937
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

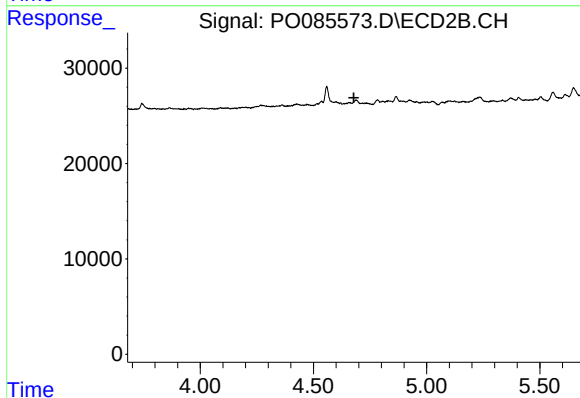


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

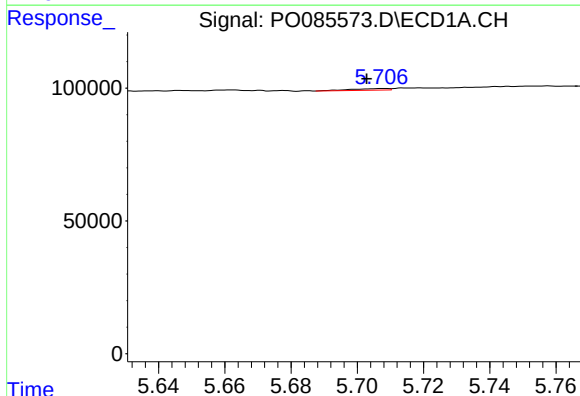


#4 AR-1016-2

R.T.: 5.707 min
Delta R.T.: 0.005 min
Response: 4937
Conc: 0.54 ng/ml

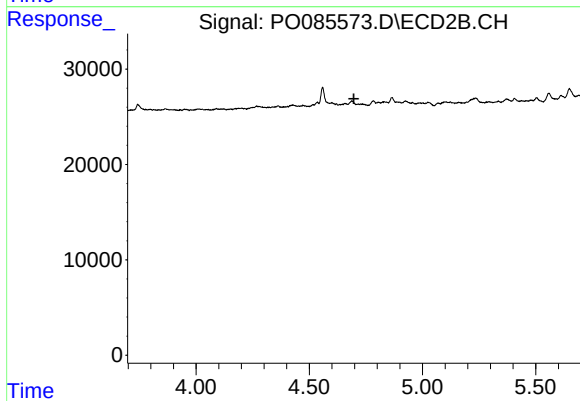

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.697 min
Response: 0
Conc: N.D.

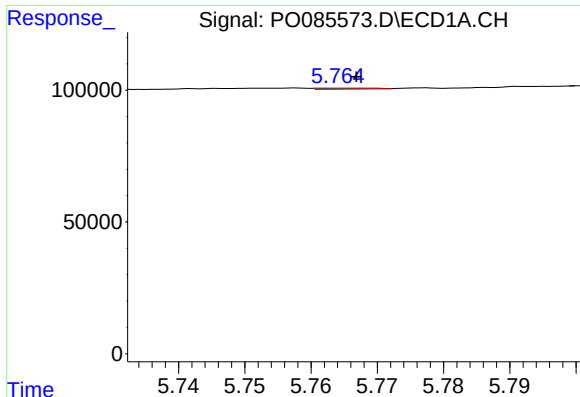

#5 AR-1016-3


R.T.: 5.764 min
Delta R.T.: -0.003 min
Response: 2510
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

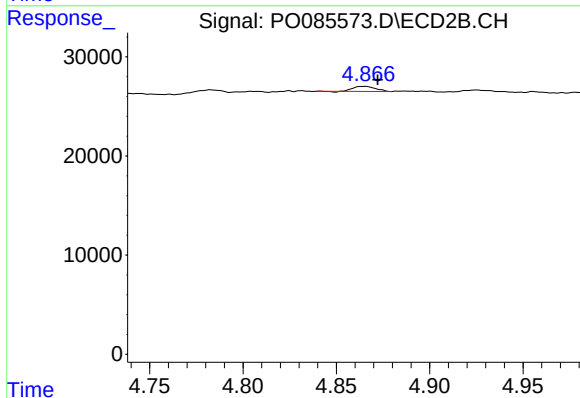


#5 AR-1016-3

R.T.: 4.866 min
Delta R.T.: -0.006 min
Response: 4282
Conc: 3.43 ng/ml

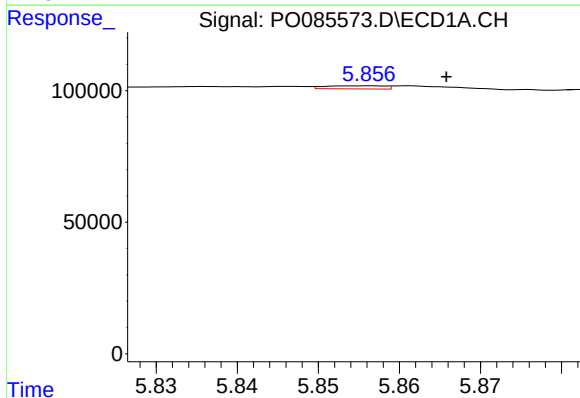


#6 AR-1016-4

R.T.: 5.856 min
Delta R.T.: -0.009 min
Response: 6165
Conc: 1.40 ng/ml

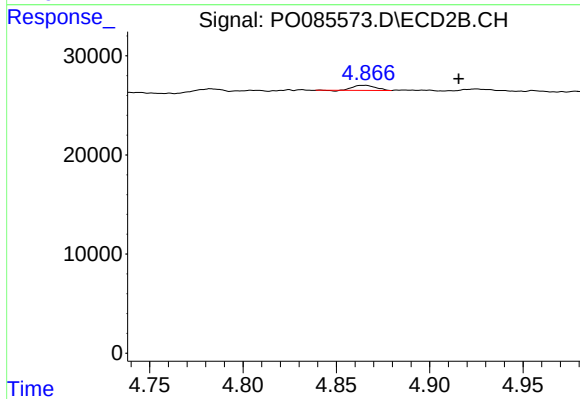

#6 AR-1016-4


R.T.: 4.866 min
Delta R.T.: -0.050 min
Response: 4282
Conc: 3.92 ng/ml

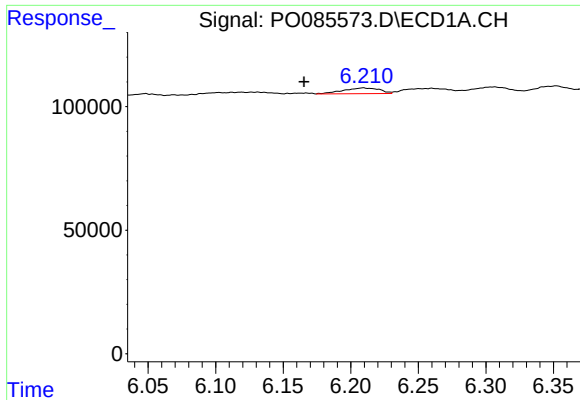

#7 AR-1016-5


R.T.: 6.210 min
Delta R.T.: 0.044 min
Response: 43203
Conc: 10.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

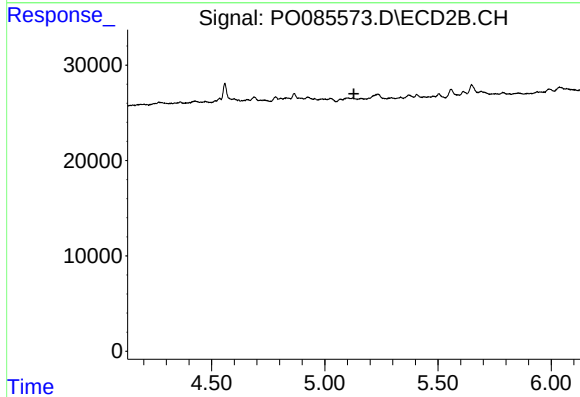


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

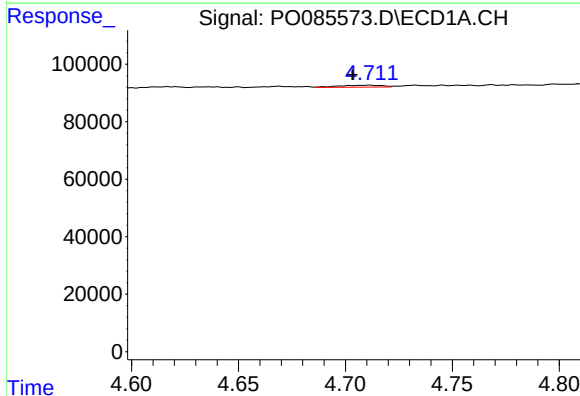


#8 AR-1221-1

R.T.: 4.711 min
Delta R.T.: 0.008 min
Response: 9298
Conc: 4.22 ng/ml

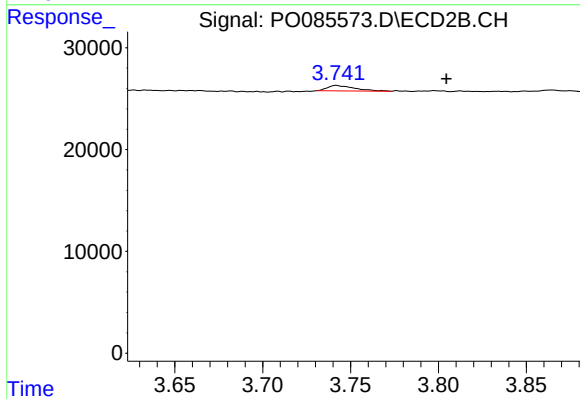

#8 AR-1221-1


R.T.: 3.742 min
Delta R.T.: -0.063 min
Response: 5794
Conc: 11.23 ng/ml

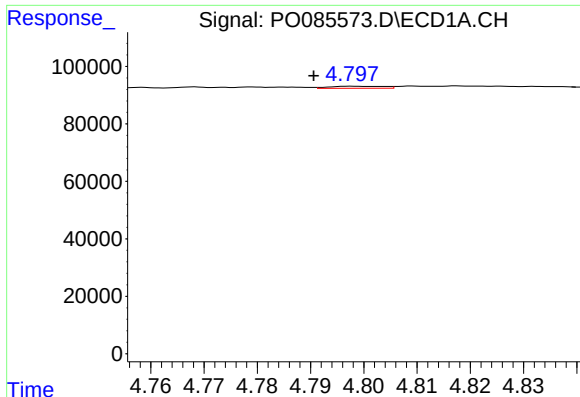

#9 AR-1221-2


R.T.: 4.798 min
Delta R.T.: 0.007 min
Response: 4878
Conc: 2.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

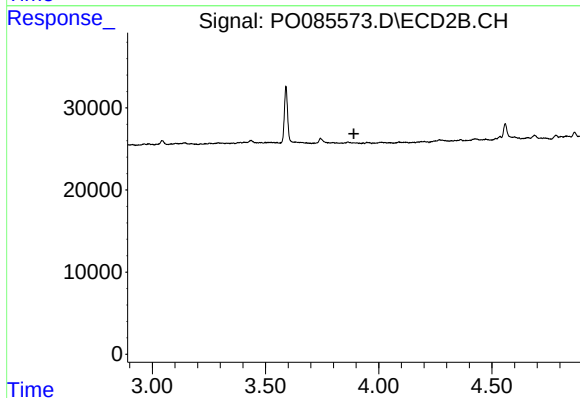


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

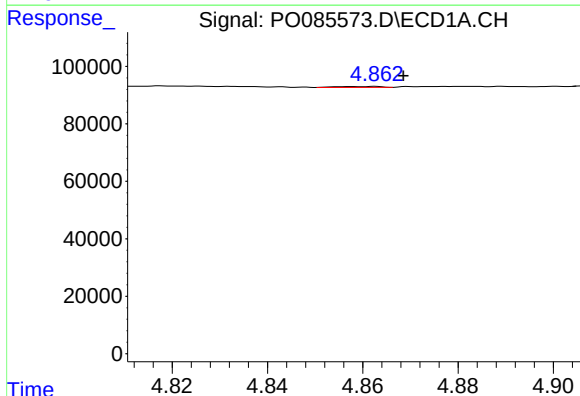


#10 AR-1221-3

R.T.: 4.863 min
Delta R.T.: -0.006 min
Response: 2233
Conc: 0.43 ng/ml

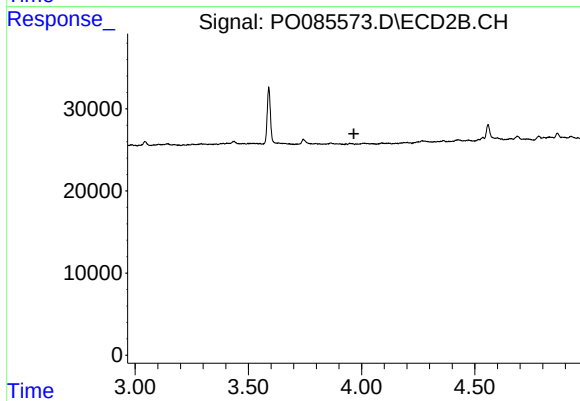

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

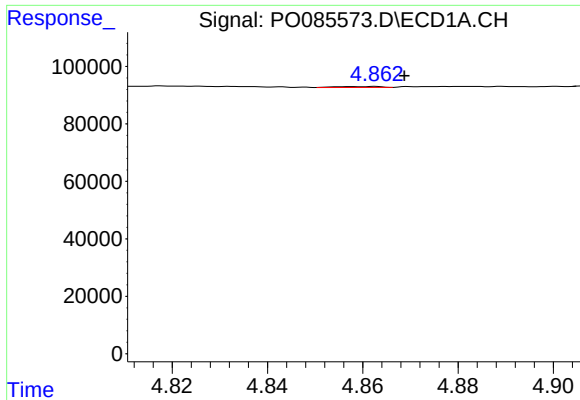

#11 AR-1232-1


R.T.: 4.863 min
Delta R.T.: -0.006 min
Response: 2233
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

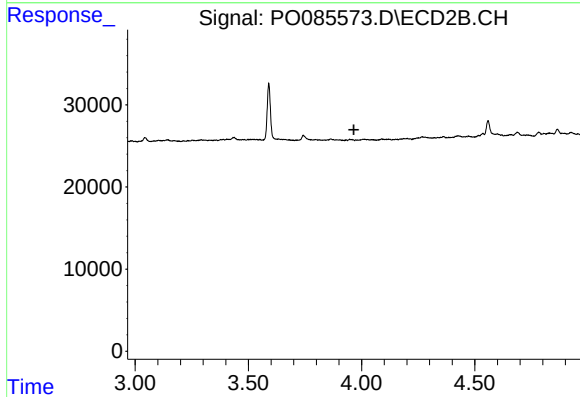


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

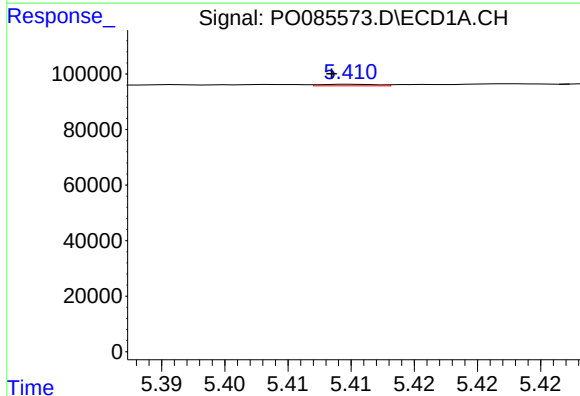


#12 AR-1232-2

R.T.: 5.410 min
Delta R.T.: 0.002 min
Response: 1761
Conc: 0.76 ng/ml

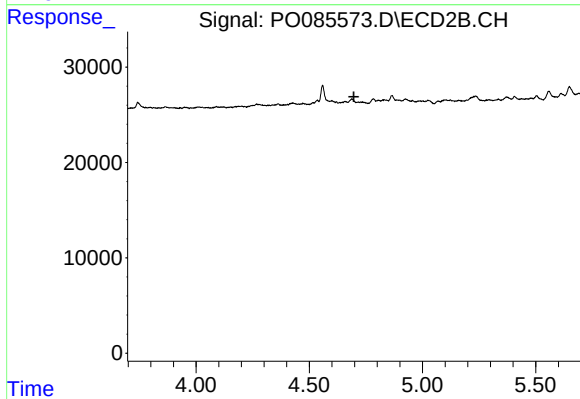

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.697 min
Response: 0
Conc: N.D.

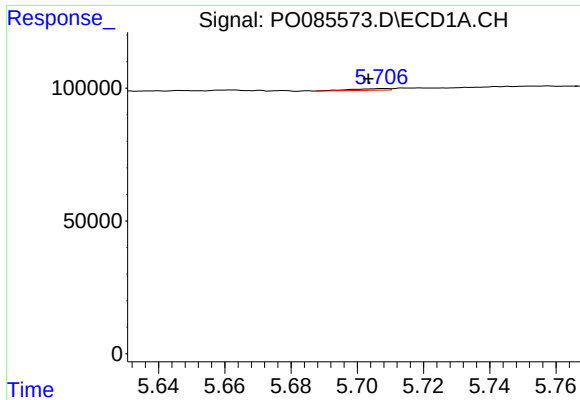

#13 AR-1232-3


R.T.: 5.707 min
Delta R.T.: 0.004 min
Response: 4937
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

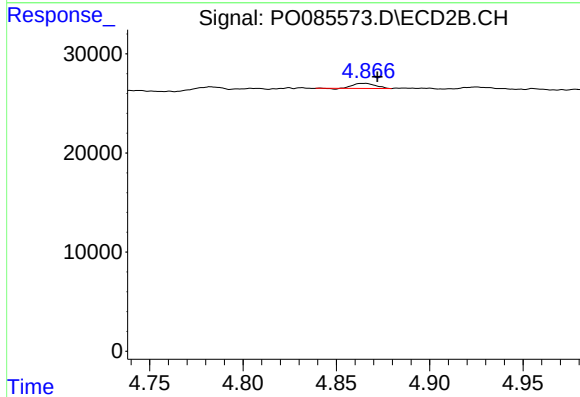


#13 AR-1232-3

R.T.: 4.866 min
Delta R.T.: -0.006 min
Response: 4282
Conc: 7.05 ng/ml

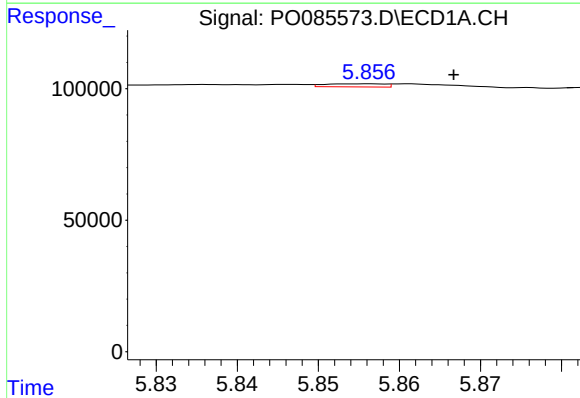


#14 AR-1232-4

R.T.: 5.856 min
Delta R.T.: -0.010 min
Response: 6165
Conc: 3.07 ng/ml

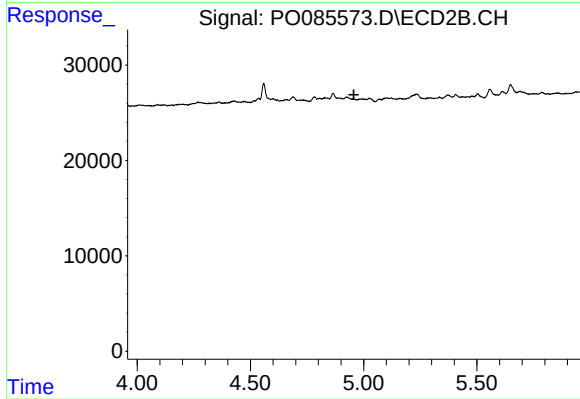

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

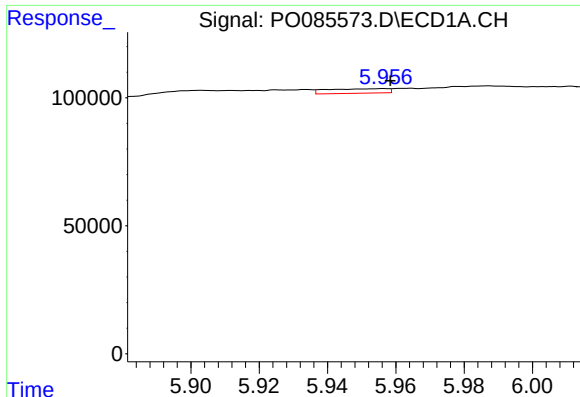

#15 AR-1232-5


R.T.: 5.957 min
Delta R.T.: -0.002 min
Response: 21614
Conc: 14.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

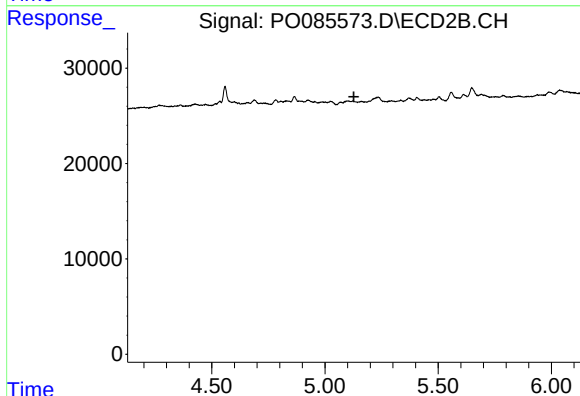


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.128 min
Response: 0
Conc: N.D.

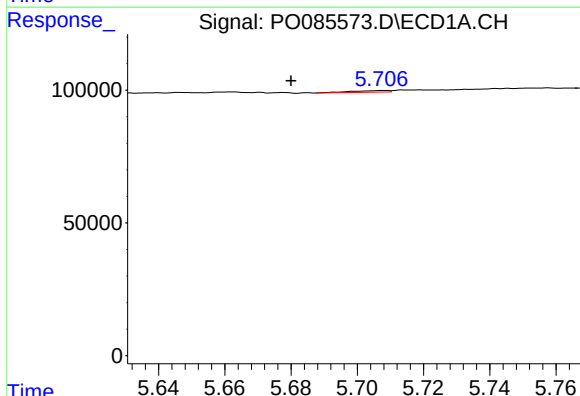


#16 AR-1242-1

R.T.: 5.707 min
Delta R.T.: 0.027 min
Response: 4937
Conc: 0.97 ng/ml

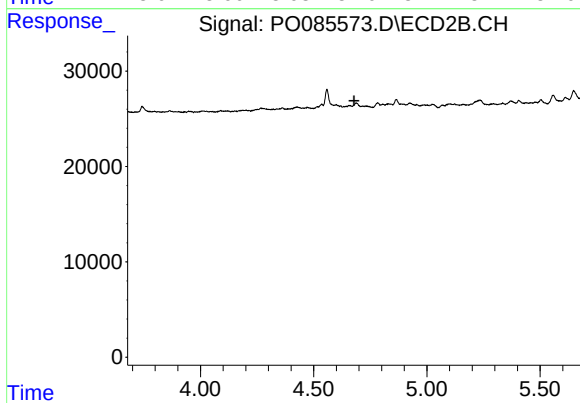

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.678 min
Response: 0
Conc: N.D.

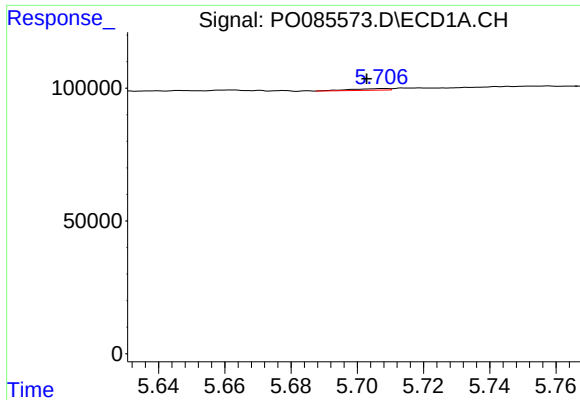

#17 AR-1242-2


R.T.: 5.707 min
Delta R.T.: 0.005 min
Response: 4937
Conc: 0.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

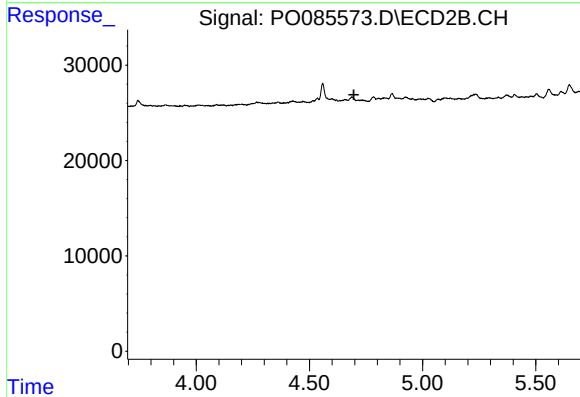


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.696 min
Response: 0
Conc: N.D.

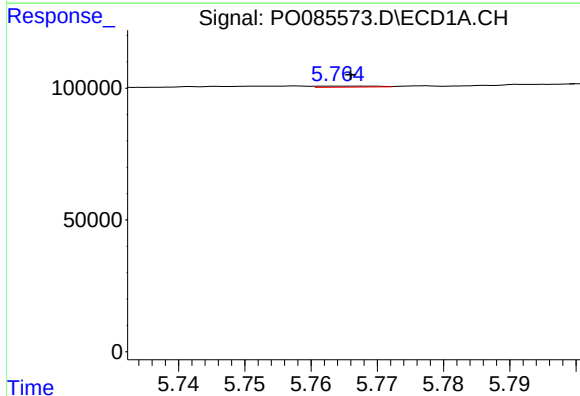


#18 AR-1242-3

R.T.: 5.764 min
Delta R.T.: -0.002 min
Response: 2510
Conc: 0.57 ng/ml

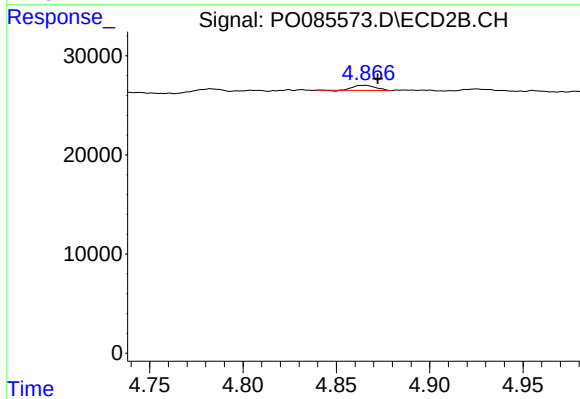

#18 AR-1242-3


R.T.: 4.866 min
Delta R.T.: -0.006 min
Response: 4282
Conc: 4.24 ng/ml

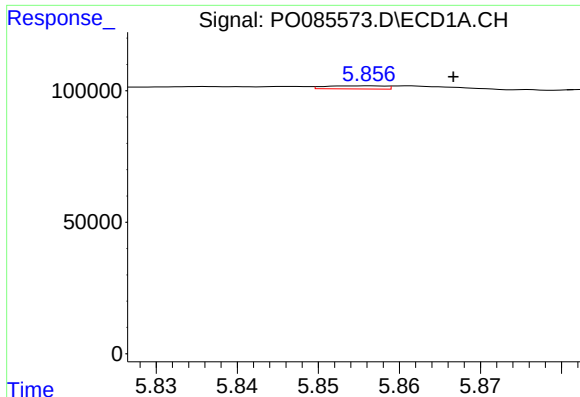

#19 AR-1242-4


R.T.: 5.856 min
Delta R.T.: -0.010 min
Response: 6165
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

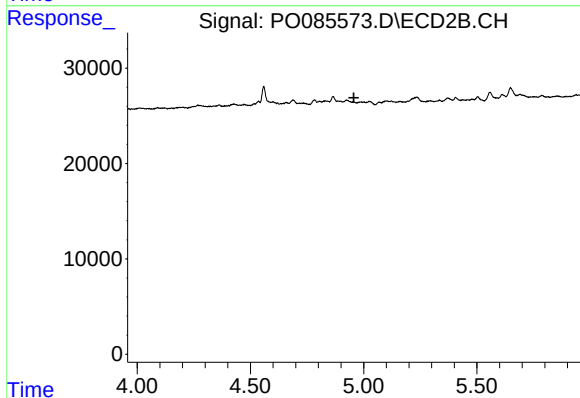


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

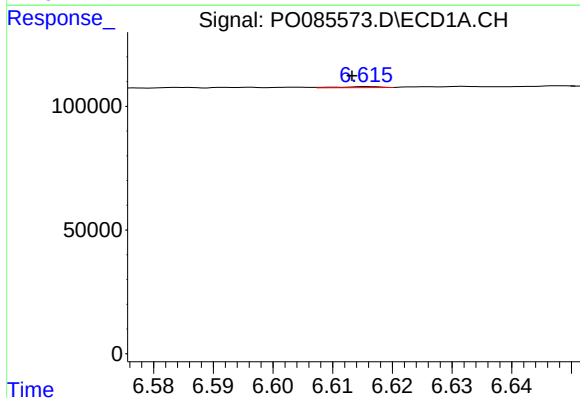


#20 AR-1242-5

R.T.: 6.616 min
Delta R.T.: 0.003 min
Response: 1944
Conc: 0.55 ng/ml

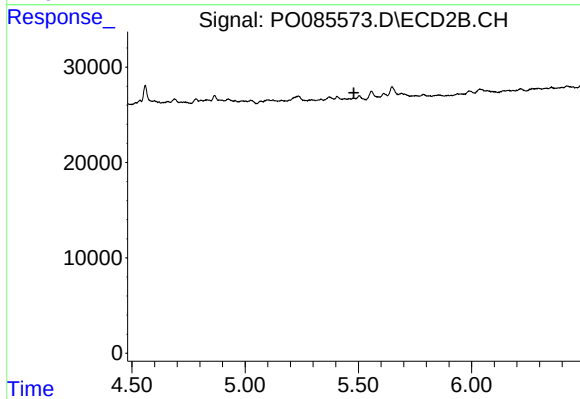

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

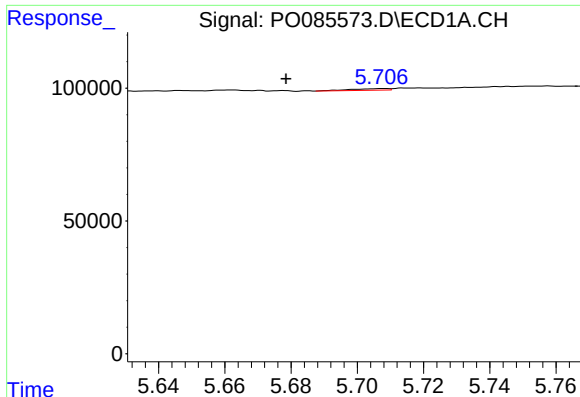

#21 AR-1248-1


R.T.: 5.707 min
Delta R.T.: 0.029 min
Response: 4937
Conc: 1.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

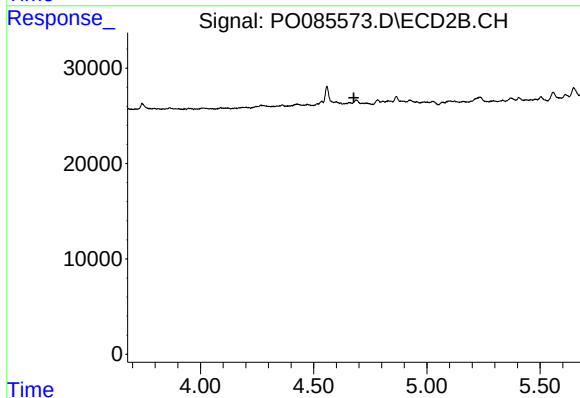


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.678 min
Response: 0
Conc: N.D.

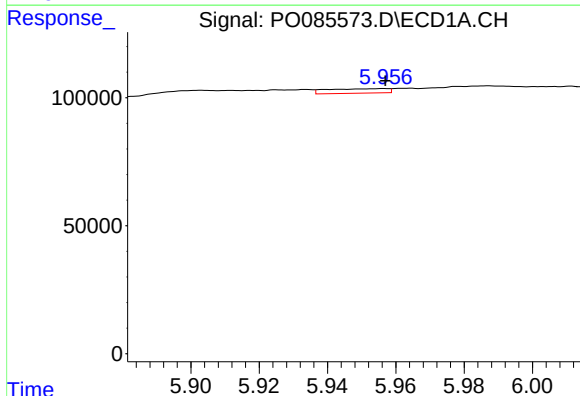


#22 AR-1248-2

R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 21614
Conc: 4.08 ng/ml

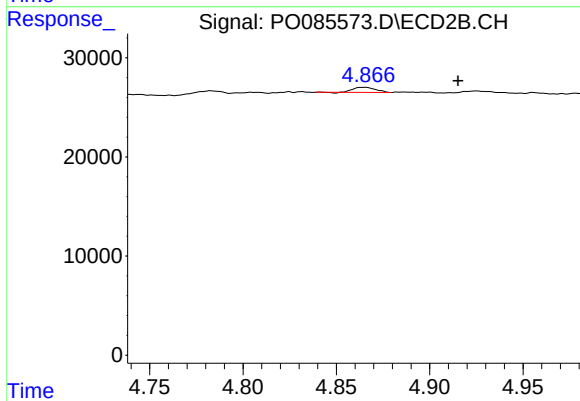

#22 AR-1248-2


R.T.: 4.866 min
Delta R.T.: -0.049 min
Response: 4282
Conc: 2.92 ng/ml

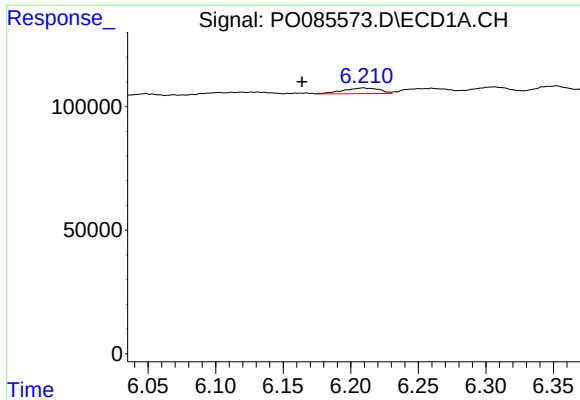

#23 AR-1248-3


R.T.: 6.210 min
Delta R.T.: 0.046 min
Response: 43203
Conc: 7.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

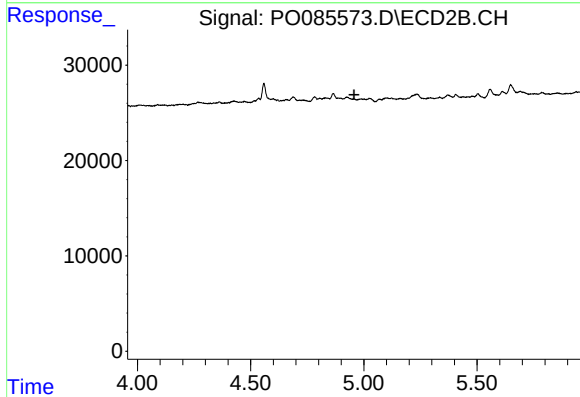


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

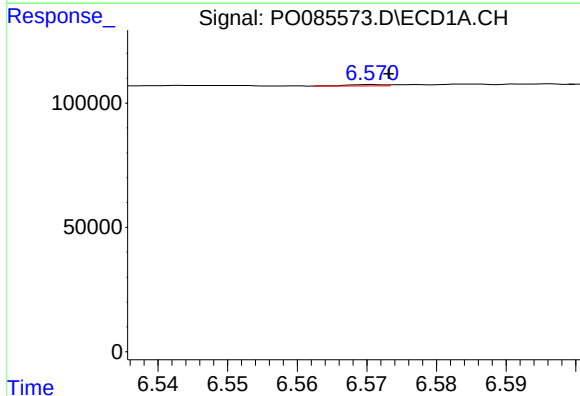


#24 AR-1248-4

R.T.: 6.571 min
Delta R.T.: -0.002 min
Response: 2186
Conc: 0.34 ng/ml

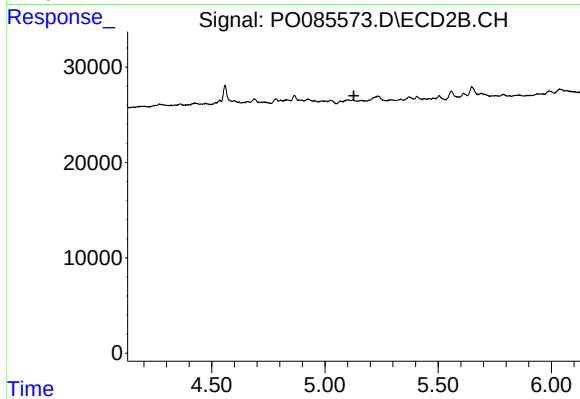

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.127 min
Response: 0
Conc: N.D.

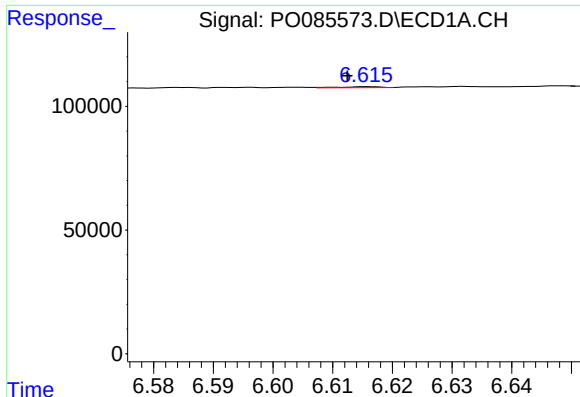

#25 AR-1248-5


R.T.: 6.616 min
Delta R.T.: 0.003 min
Response: 1944
Conc: 0.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

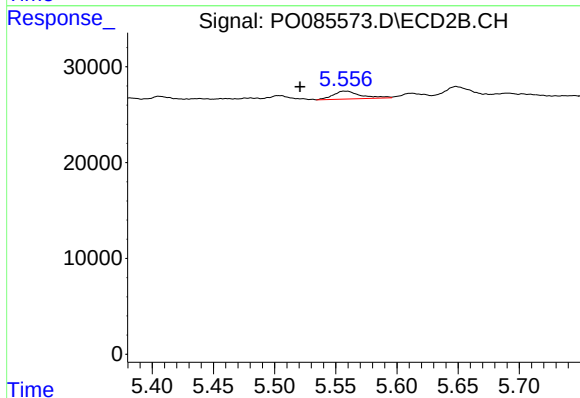


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: 0.036 min
Response: 12905
Conc: 7.51 ng/ml

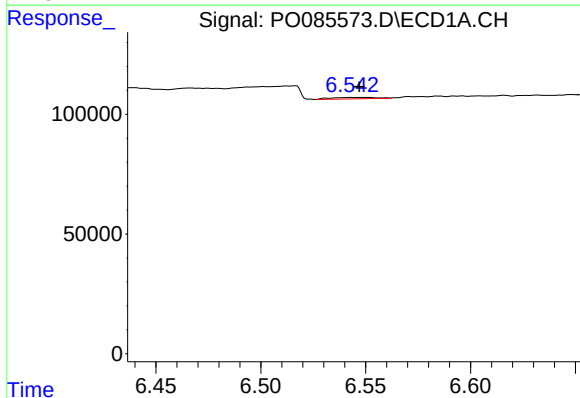


#26 AR-1254-1

R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 8750
Conc: 1.32 ng/ml

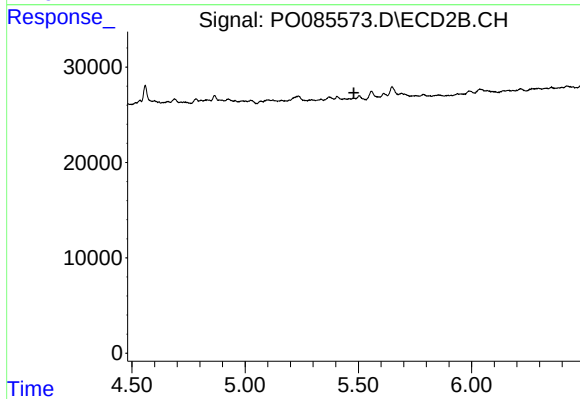

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 5.480 min
Response: 0
Conc: N.D.

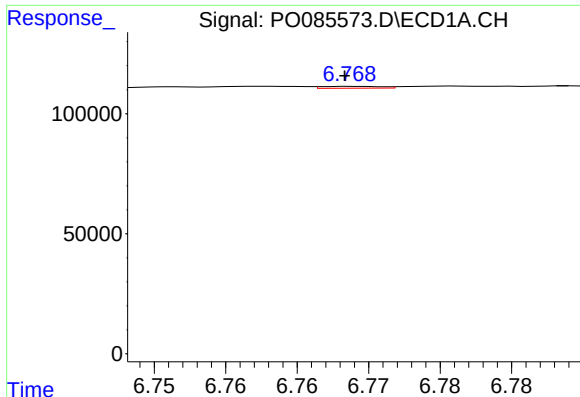

#27 AR-1254-2


R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 2248
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

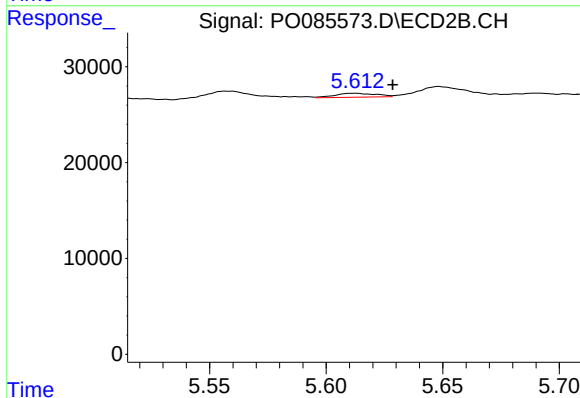


#27 AR-1254-2

R.T.: 5.613 min
Delta R.T.: -0.016 min
Response: 5078
Conc: 2.18 ng/ml

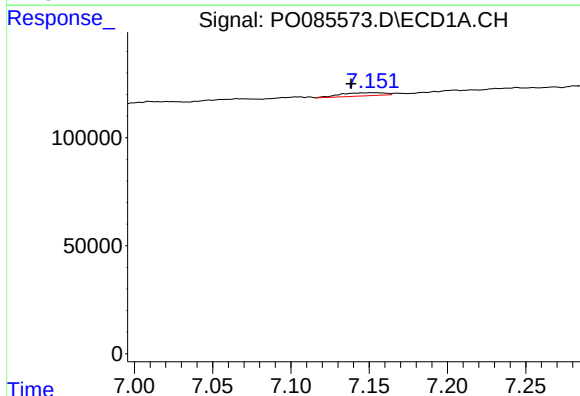


#28 AR-1254-3

R.T.: 7.151 min
Delta R.T.: 0.013 min
Response: 28321
Conc: 2.75 ng/ml

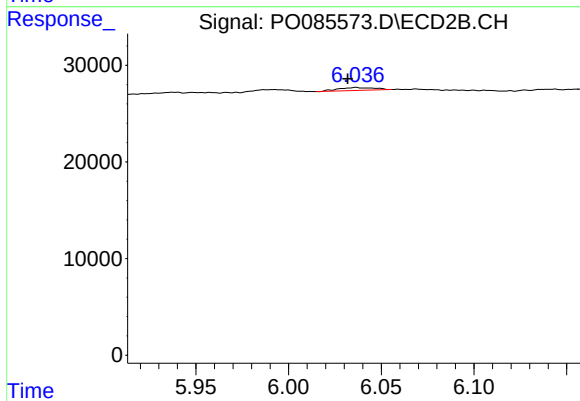

#28 AR-1254-3


R.T.: 6.036 min
Delta R.T.: 0.005 min
Response: 4031
Conc: 1.10 ng/ml

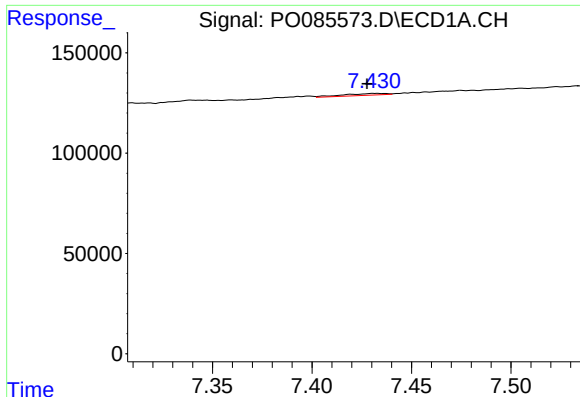

#29 AR-1254-4


R.T.: 7.431 min
Delta R.T.: 0.003 min
Response: 13832
Conc: 1.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

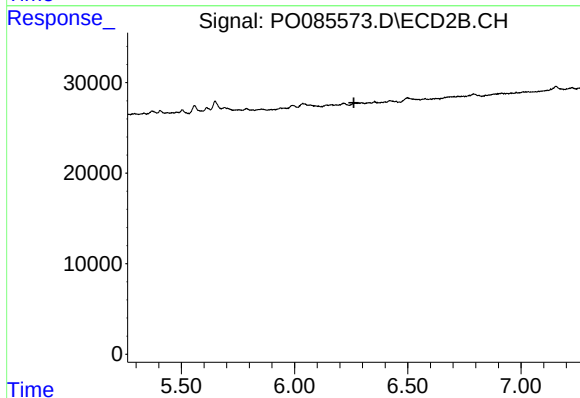


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.262 min
Response: 0
Conc: N.D.

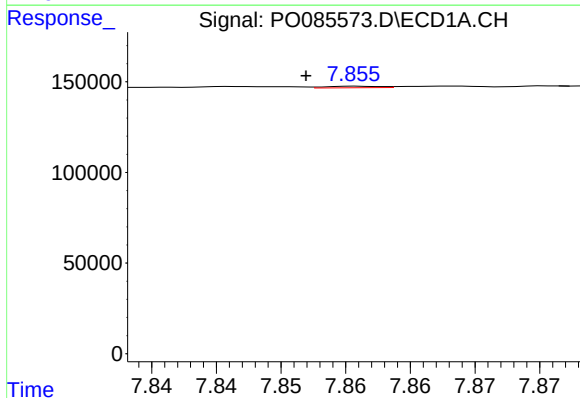


#30 AR-1254-5

R.T.: 7.856 min
Delta R.T.: 0.004 min
Response: 2554
Conc: 0.33 ng/ml

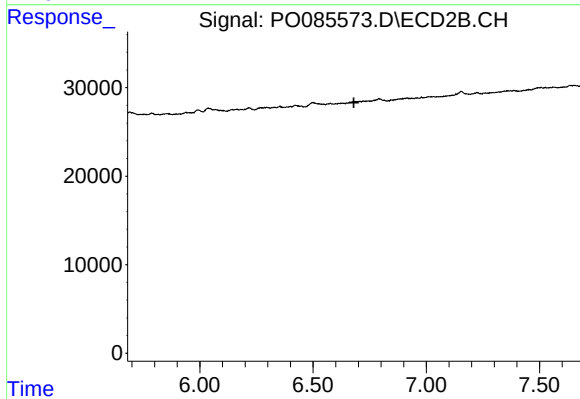

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

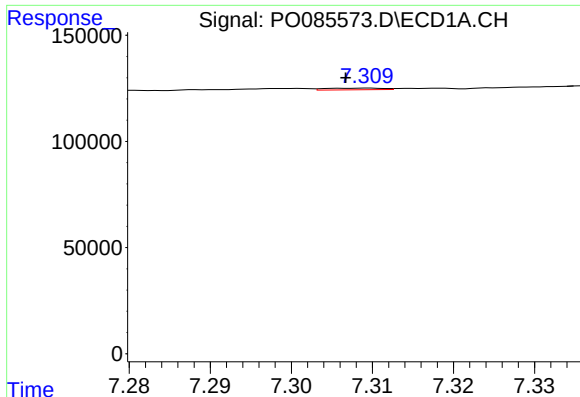

#31 AR-1260-1


R.T.: 7.309 min
Delta R.T.: 0.003 min
Response: 3785
Conc: 0.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

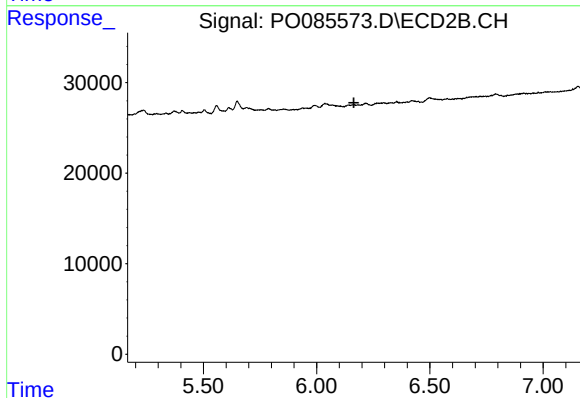


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.165 min
Response: 0
Conc: N.D.

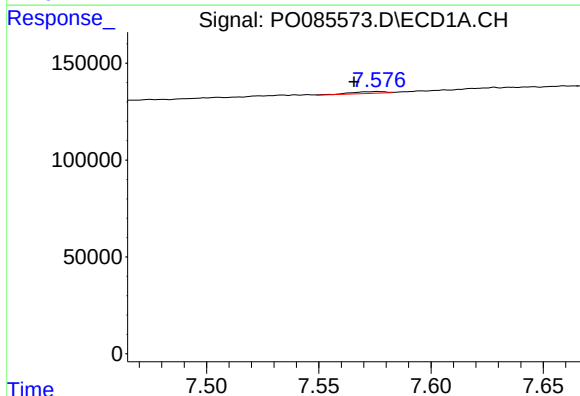


#32 AR-1260-2

R.T.: 7.576 min
Delta R.T.: 0.011 min
Response: 9935
Conc: 1.27 ng/ml

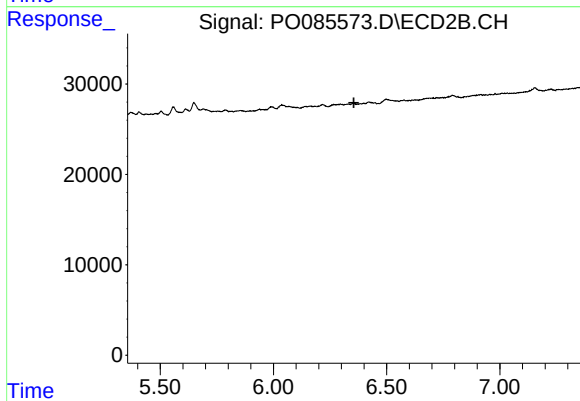

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

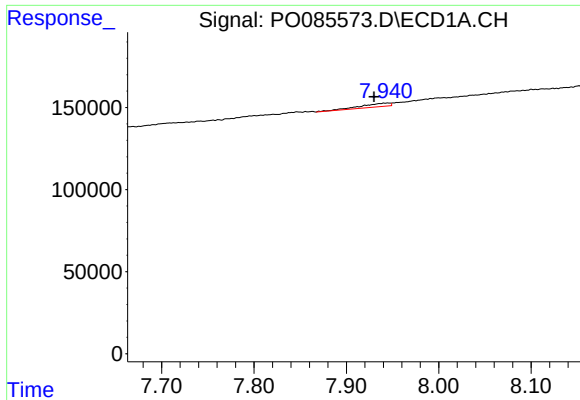

#33 AR-1260-3


R.T.: 7.945 min
Delta R.T.: 0.015 min
Response: 48216
Conc: 8.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

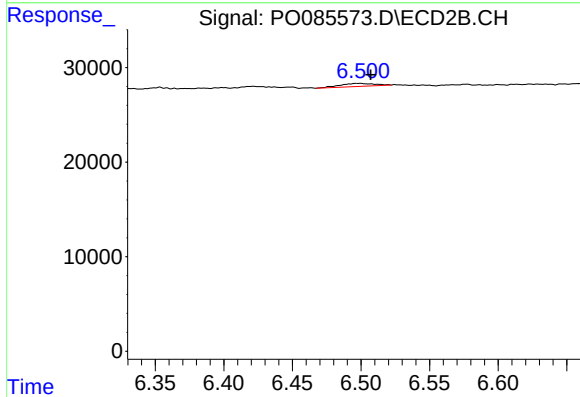


#33 AR-1260-3

R.T.: 6.500 min
Delta R.T.: -0.007 min
Response: 5516
Conc: 2.10 ng/ml

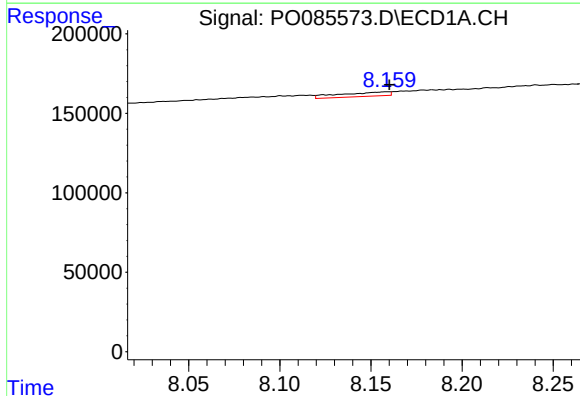


#34 AR-1260-4

R.T.: 8.159 min
Delta R.T.: -0.001 min
Response: 51007
Conc: 7.38 ng/ml

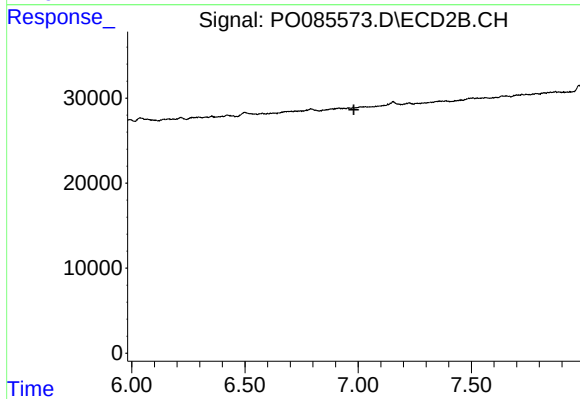

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 6.981 min
Response: 0
Conc: N.D.

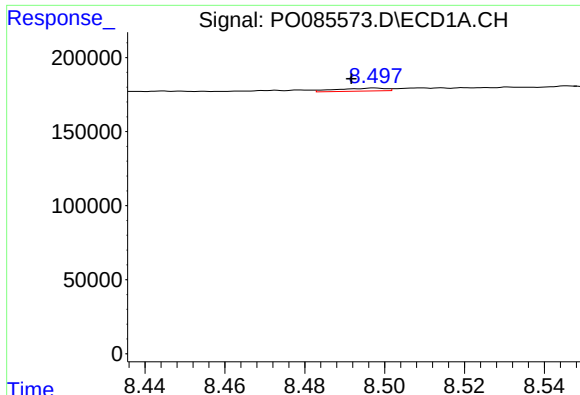

#35 AR-1260-5


R.T.: 8.497 min
Delta R.T.: 0.006 min
Response: 16851
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

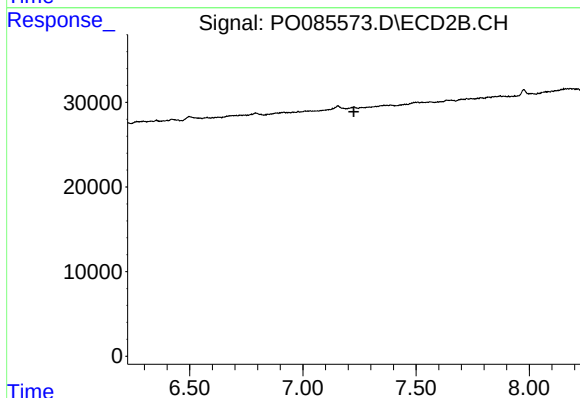


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.225 min
Response: 0
Conc: N.D.

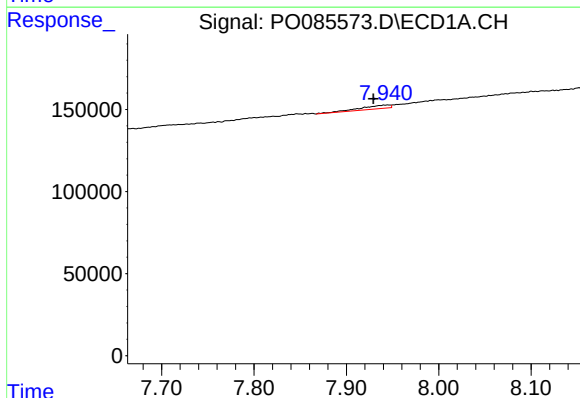


#36 AR-1262-1

R.T.: 7.945 min
Delta R.T.: 0.015 min
Response: 48216
Conc: 5.34 ng/ml

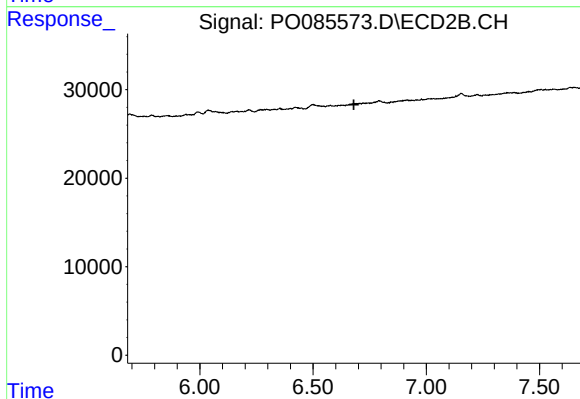

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

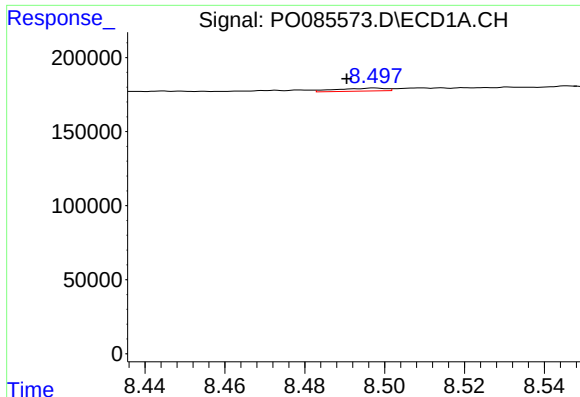

#37 AR-1262-2


R.T.: 8.497 min
Delta R.T.: 0.007 min
Response: 16851
Conc: 1.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

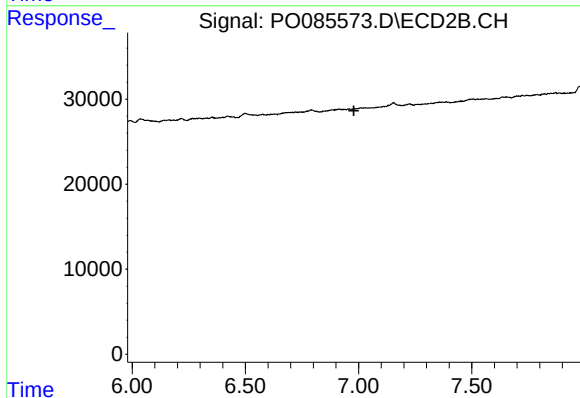


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

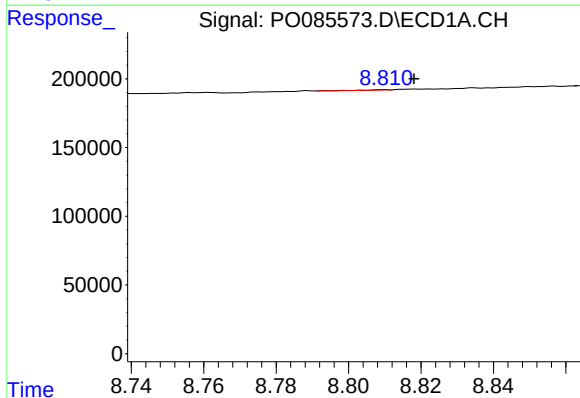


#38 AR-1262-3

R.T.: 8.810 min
Delta R.T.: -0.008 min
Response: 1926
Conc: 0.19 ng/ml

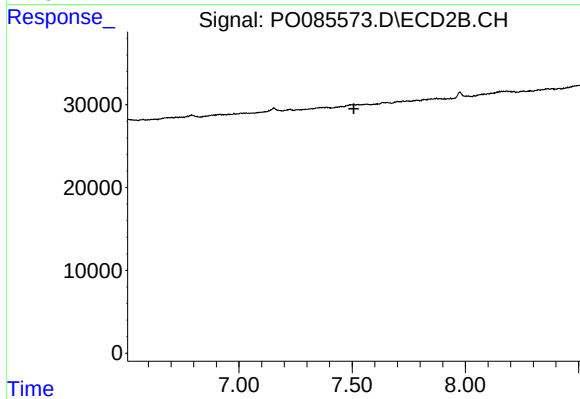

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.508 min
Response: 0
Conc: N.D.

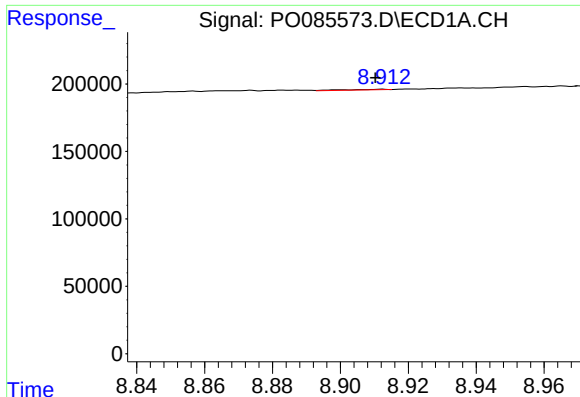

#39 AR-1262-4


R.T.: 8.912 min
Delta R.T.: 0.002 min
Response: 3843
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

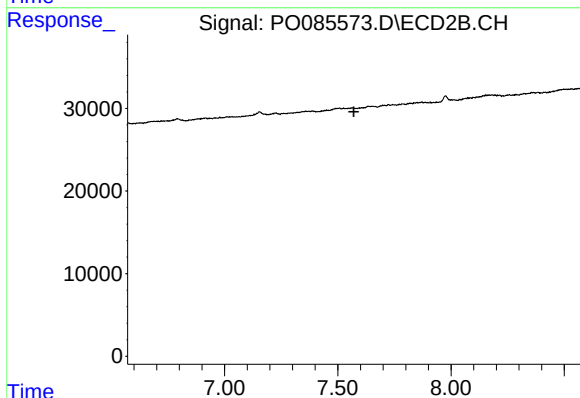


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.571 min
Response: 0
Conc: N.D.

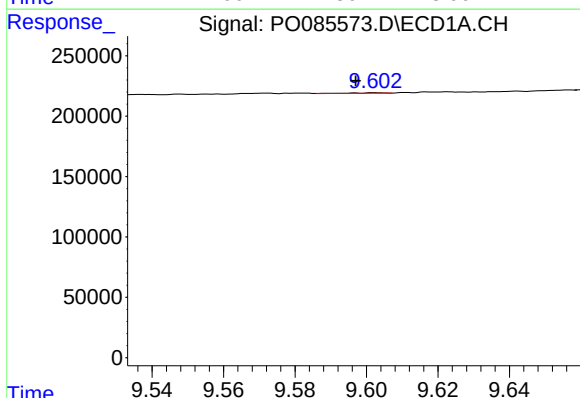


#40 AR-1262-5

R.T.: 9.602 min
Delta R.T.: 0.005 min
Response: 3474
Conc: 0.65 ng/ml

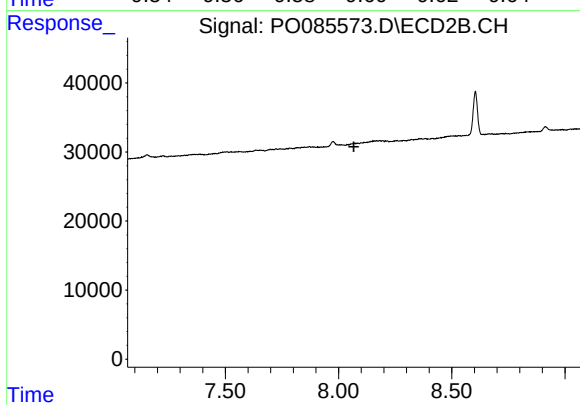

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.067 min
Response: 0
Conc: N.D.

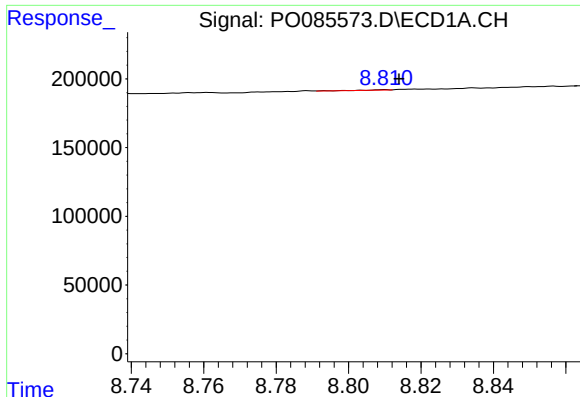

#41 AR-1268-1


R.T.: 8.810 min
Delta R.T.: -0.004 min
Response: 1926
Conc: 0.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

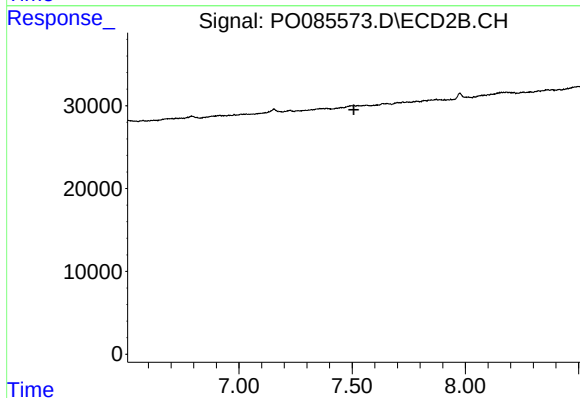


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.508 min
Response: 0
Conc: N.D.

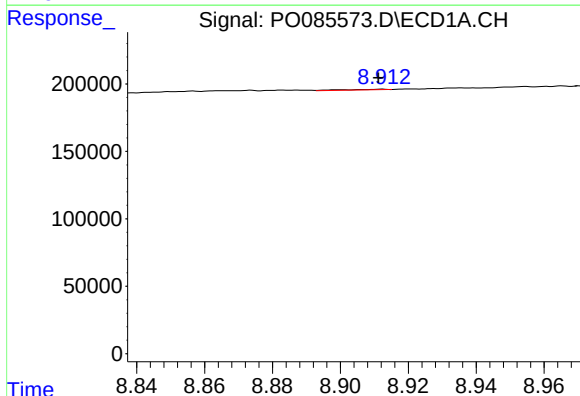


#42 AR-1268-2

R.T.: 8.912 min
Delta R.T.: 0.001 min
Response: 3843
Conc: 0.22 ng/ml

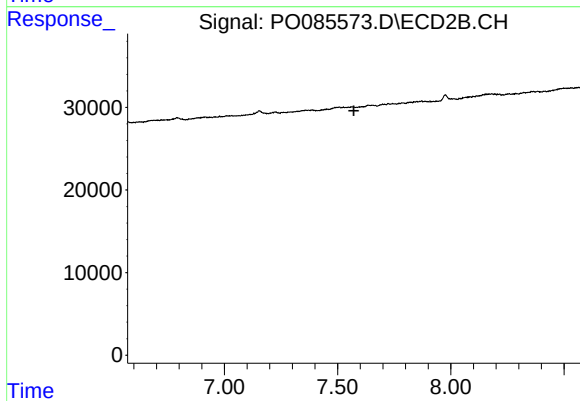

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

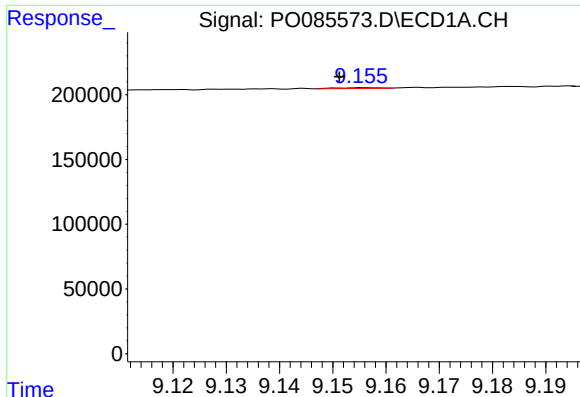

#43 AR-1268-3


R.T.: 9.156 min
Delta R.T.: 0.005 min
Response: 3546
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

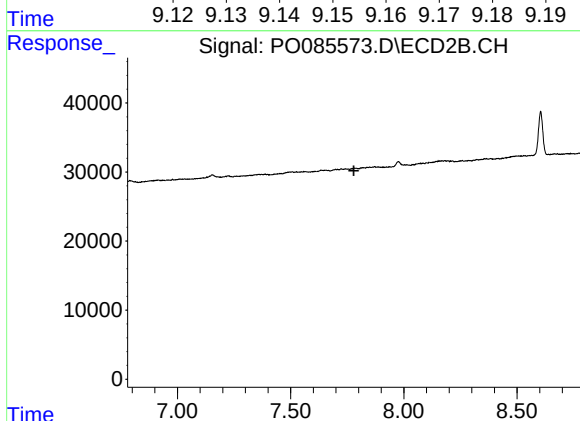


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

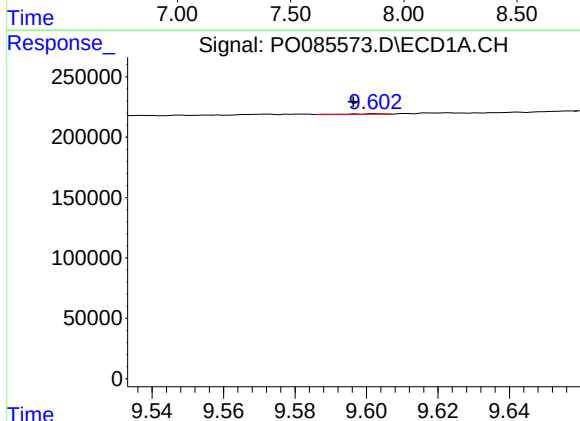


#44 AR-1268-4

R.T.: 9.602 min
Delta R.T.: 0.006 min
Response: 3474
Conc: 0.57 ng/ml

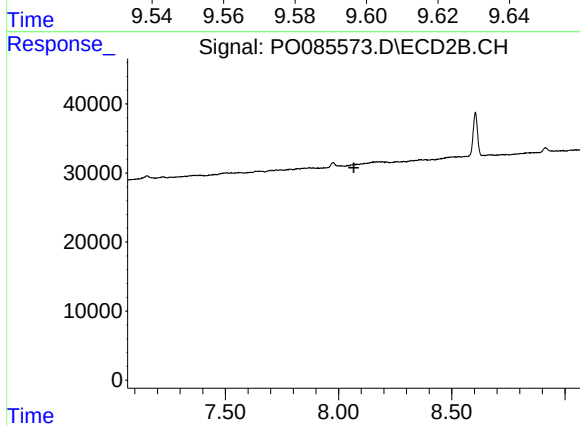

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.068 min
Response: 0
Conc: N.D.

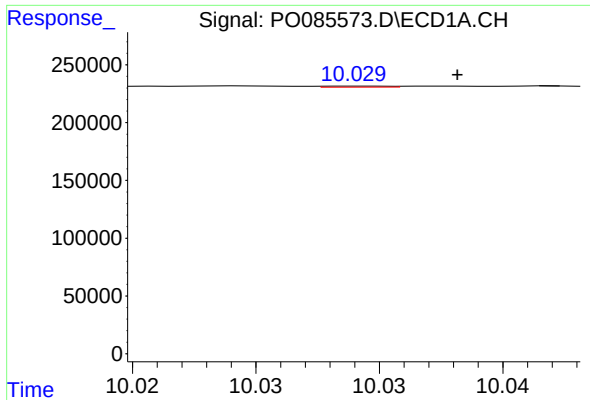

#45 AR-1268-5

R.T.: 10.029 min
Delta R.T.: -0.004 min
Response: 1538
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34B

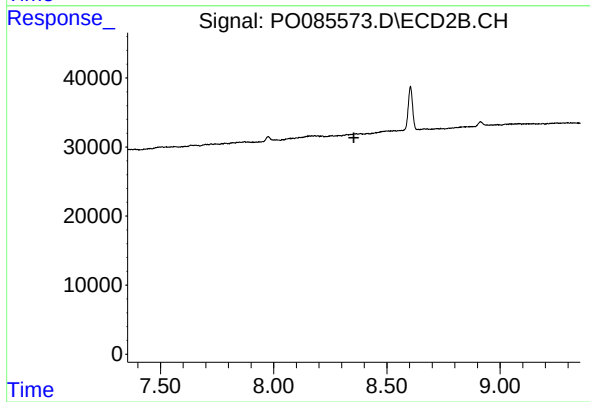

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.