

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032322\
 Data File : P0085574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 16:36
 Operator : YP\AJ
 Sample : N2055-09-10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CLI-2022-34A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:15:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.589	326616	97305	1.597	2.271 #
2)	SA Decachlor...	10.391	8.604	274588	78250	2.284	2.038
Target Compounds							
3)	L1 AR-1016-1	5.673	4.693	22463	4713	3.569	2.953
4)	L1 AR-1016-2	5.713	4.693	26838	4713	2.930	2.037 #
5)	L1 AR-1016-3	5.772	4.861	1394	3282	0.256	2.626 #
6)	L1 AR-1016-4	5.856	4.919	9049	4798	2.052	4.395 #
7)	L1 AR-1016-5	6.169	5.127	25290	9479	5.956	7.008
8)	L2 AR-1221-1	4.759f	3.742f	2039	3820	0.924	7.406 #
9)	L2 AR-1221-2	4.780	0.000	1526	0	0.937	N.D. #
10)	L2 AR-1221-3	4.832f	0.000	1529	0	0.297	N.D. #
11)	L3 AR-1232-1	4.832f	0.000	1529	0	0.325	N.D. #
12)	L3 AR-1232-2	5.401	4.693	61067	4713	26.500	4.326 #
13)	L3 AR-1232-3	5.713	4.861	26838	3282	6.360	5.400
14)	L3 AR-1232-4	5.856	4.919f	9049	4798	4.507	8.610 #
15)	L3 AR-1232-5	5.933	5.127	6665	9479	4.528	15.373 #
16)	L4 AR-1242-1	5.673	4.693	22463	4713	4.419	3.607
17)	L4 AR-1242-2	5.713	4.693	26838	4713	3.615	2.550 #
18)	L4 AR-1242-3	5.772	4.861	1394	3282	0.317	3.245 #
19)	L4 AR-1242-4	5.856	4.919f	9049	4798	2.494	4.616 #
20)	L4 AR-1242-5	6.617	5.478	27701	5827	7.796	4.721 #
21)	L5 AR-1248-1	5.673	4.693	22463	4713	6.026	4.875
22)	L5 AR-1248-2	5.933	4.919	6665	4798	1.257	3.277 #
23)	L5 AR-1248-3	6.169	4.919f	25290	4798	4.299	3.130 #
24)	L5 AR-1248-4	6.575	5.127	27157	9479	4.212	5.393 #
25)	L5 AR-1248-5	6.617	5.478f	27701	5827	4.474	3.392
26)	L6 AR-1254-1	6.547	5.478	69758	5827	10.526	2.217 #
27)	L6 AR-1254-2	6.772	5.626	30680	6229	3.066	2.669
28)	L6 AR-1254-3	7.142	6.028	222435	14951	21.613	4.071 #
29)	L6 AR-1254-4	7.426	6.260	132447	5334	18.878	2.408 #
30)	L6 AR-1254-5	7.852	6.681	147495	8569	19.276	2.634 #
31)	L7 AR-1260-1	7.304	0.000	138015	0	20.002	N.D. #
32)	L7 AR-1260-2	7.577	0.000	131564	0	16.818	N.D. #
33)	L7 AR-1260-3	7.937	6.502	51453	15362	8.760	5.843 #
34)	L7 AR-1260-4	8.161	0.000	129319	0	18.723	N.D. #
35)	L7 AR-1260-5	8.494	0.000	19843	0	1.412	N.D. #
36)	L8 AR-1262-1	7.937	6.681	51453	8569	5.697	4.991
37)	L8 AR-1262-2	8.494	0.000	19843	0	1.245	N.D. #
38)	L8 AR-1262-3	8.819	0.000	5298	0	0.513	N.D. #
39)	L8 AR-1262-4	8.911	0.000	7360	0	1.567	N.D. #
40)	L8 AR-1262-5	9.589	0.000	20118	0	3.783	N.D. #
41)	L9 AR-1268-1	8.819	0.000	5298	0	0.275	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
 Data File : P0085574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 16:36
 Operator : YP\AJ
 Sample : N2055-09-10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-34A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:15:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	8.911	0.000	7360	0	0.424	N.D.	#
43)	L9 AR-1268-3	9.151	0.000	24464	0	1.657	N.D.	#
44)	L9 AR-1268-4	9.589	0.000	20118	0	3.297	N.D.	#
45)	L9 AR-1268-5	10.034	0.000	4116	0	0.085	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032322\
Data File : PO085574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 16:36
Operator : YP\AJ
Sample : N2055-09-10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:15:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

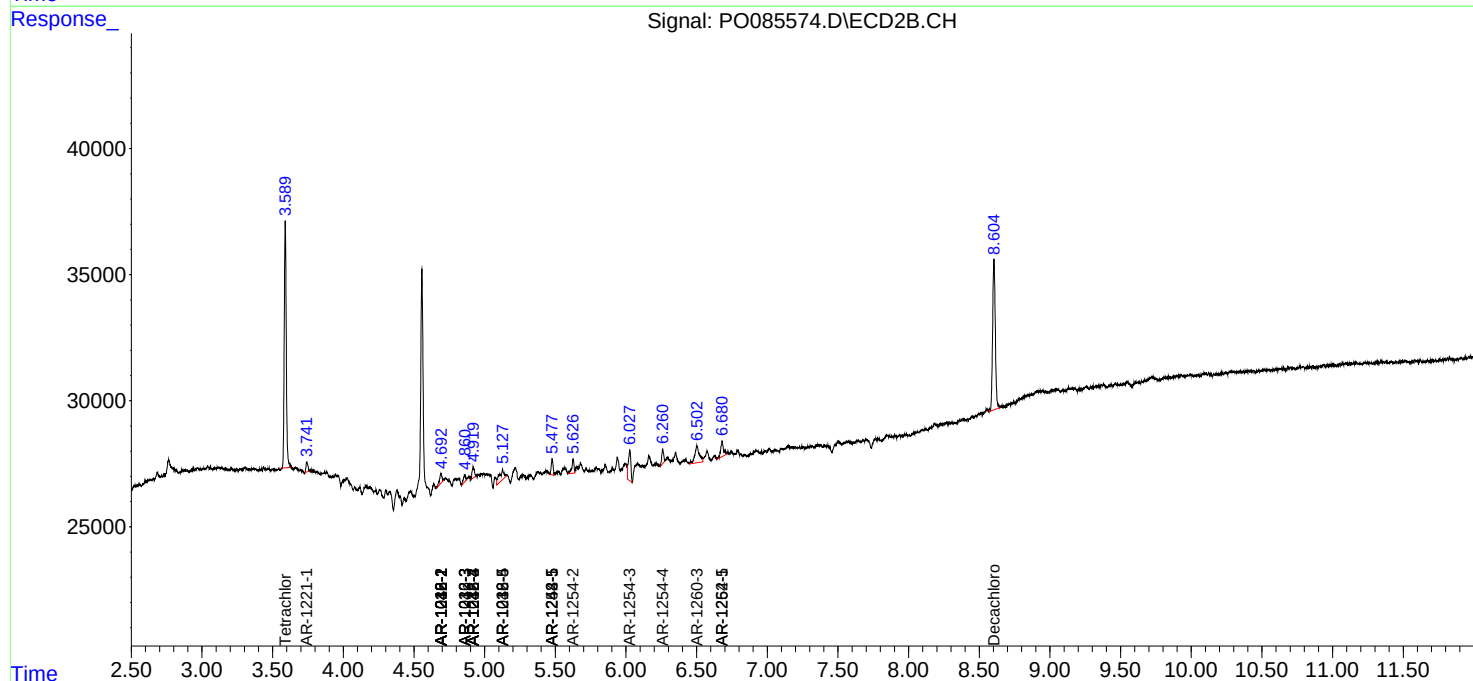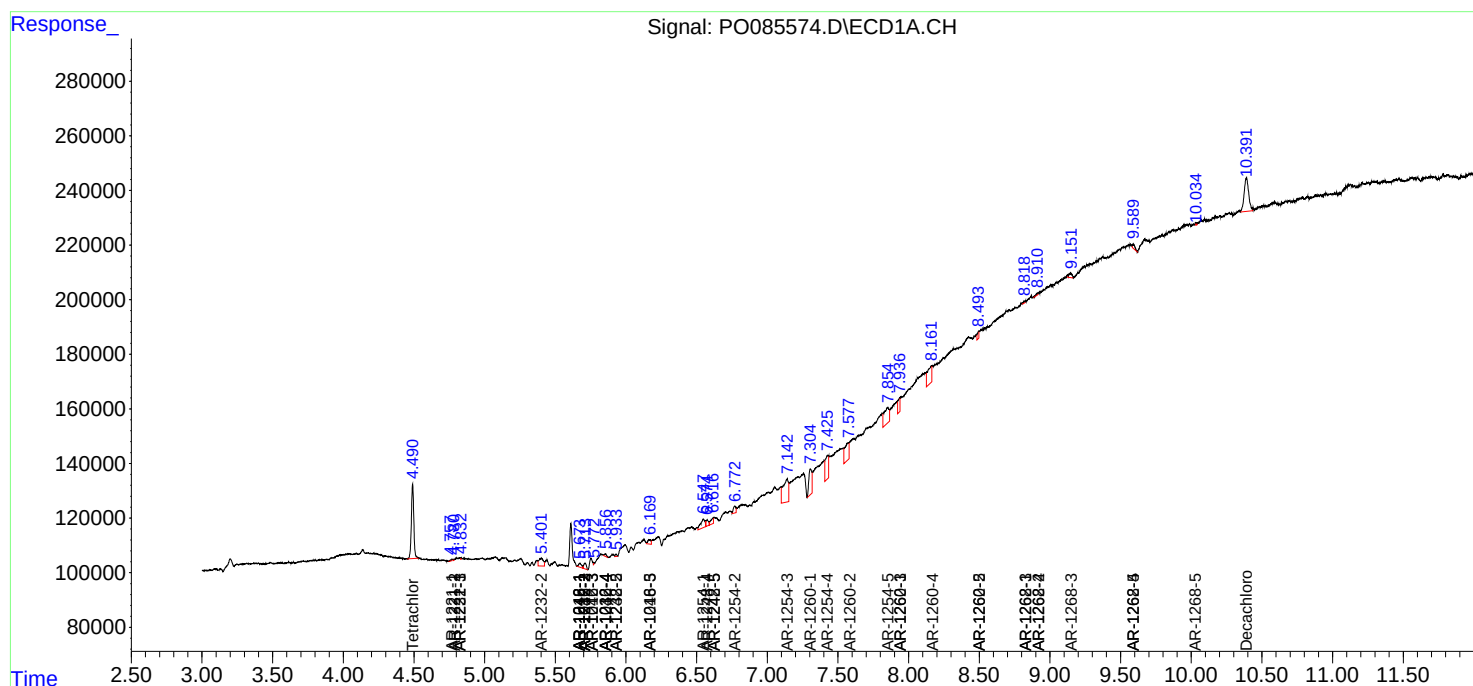


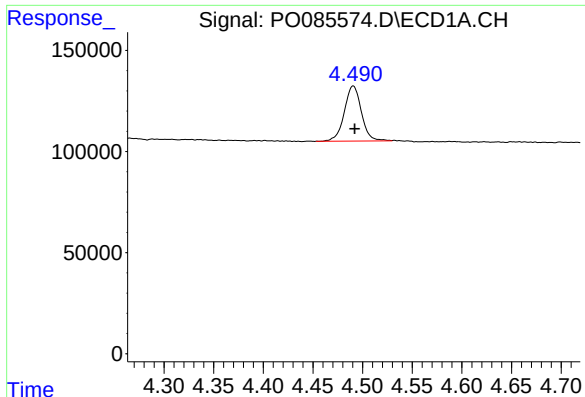

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: -0.001 min
Response: 326616
Conc: 1.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

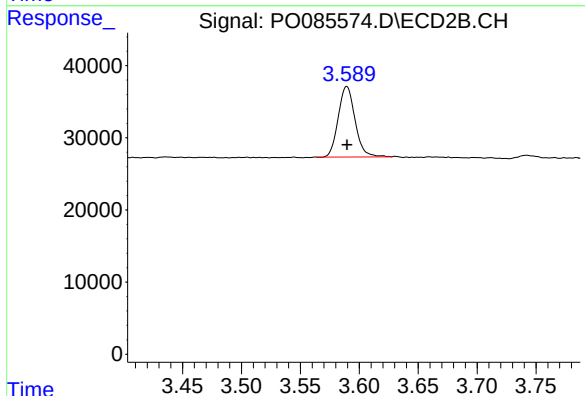


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: 0.000 min
Response: 97305
Conc: 2.27 ng/ml

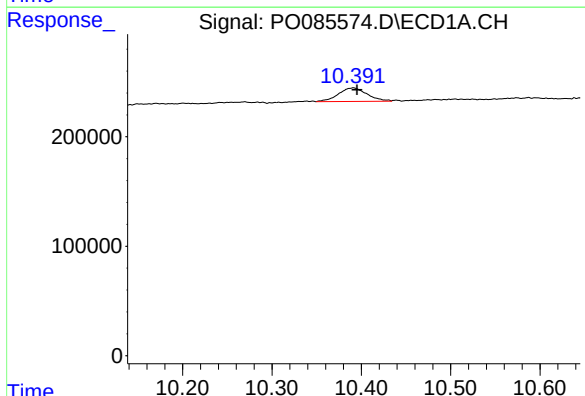


#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.004 min
Response: 274588
Conc: 2.28 ng/ml

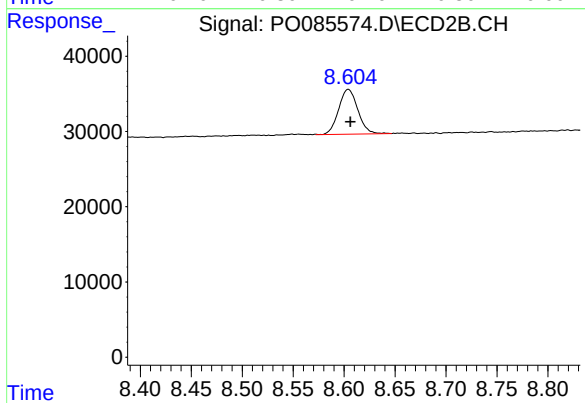

#2 Decachlorobiphenyl


R.T.: 8.604 min
Delta R.T.: -0.002 min
Response: 78250
Conc: 2.04 ng/ml

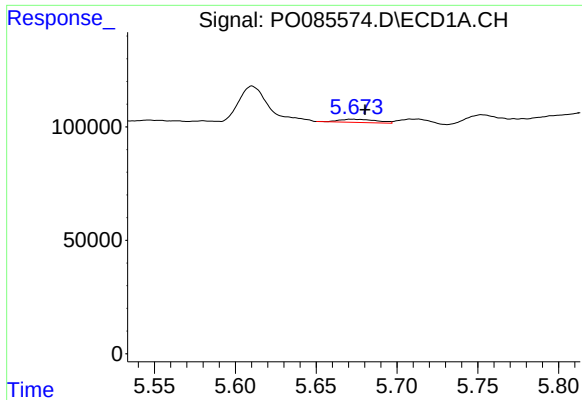

#3 AR-1016-1


R.T.: 5.673 min
Delta R.T.: -0.007 min
Response: 22463
Conc: 3.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

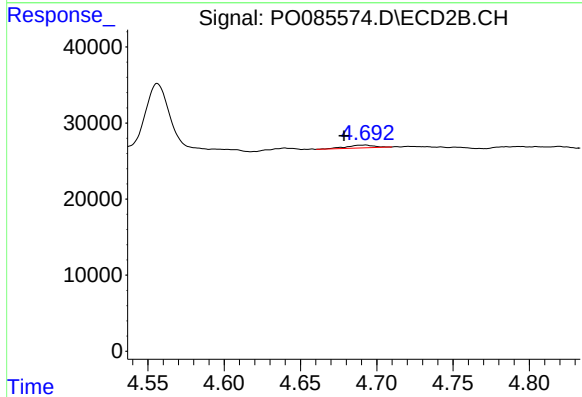


#3 AR-1016-1

R.T.: 4.693 min
Delta R.T.: 0.014 min
Response: 4713
Conc: 2.95 ng/ml

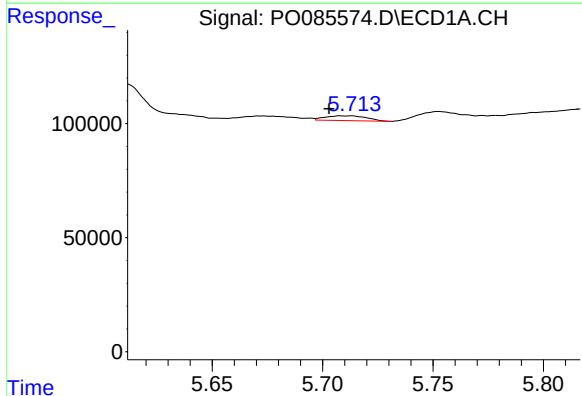


#4 AR-1016-2

R.T.: 5.713 min
Delta R.T.: 0.010 min
Response: 26838
Conc: 2.93 ng/ml

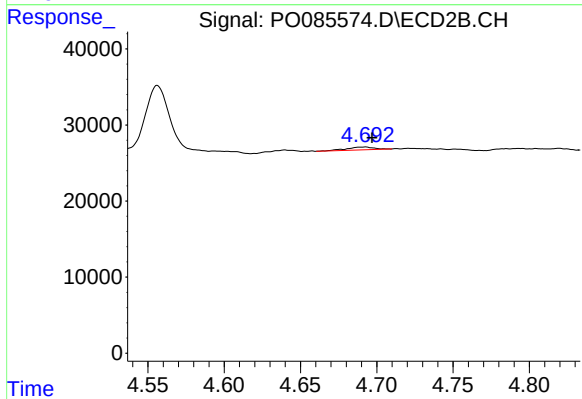

#4 AR-1016-2


R.T.: 4.693 min
Delta R.T.: -0.004 min
Response: 4713
Conc: 2.04 ng/ml

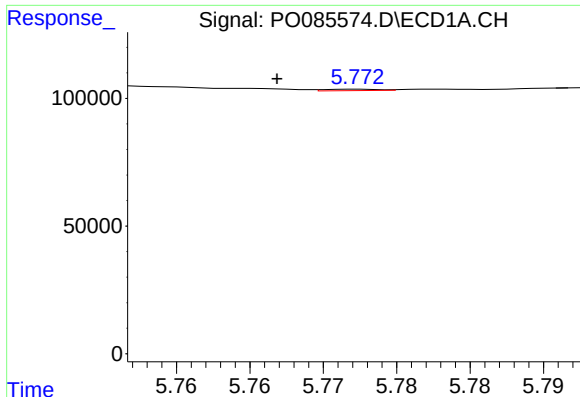

#5 AR-1016-3


R.T.: 5.772 min
Delta R.T.: 0.006 min
Response: 1394
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

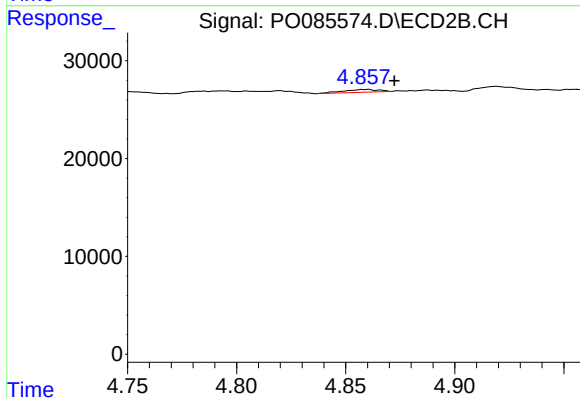


#5 AR-1016-3

R.T.: 4.861 min
Delta R.T.: -0.012 min
Response: 3282
Conc: 2.63 ng/ml

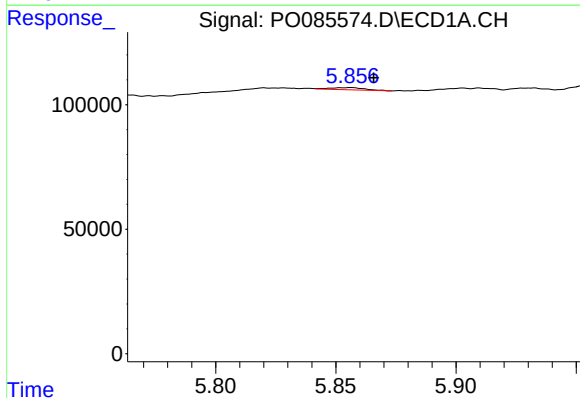


#6 AR-1016-4

R.T.: 5.856 min
Delta R.T.: -0.009 min
Response: 9049
Conc: 2.05 ng/ml

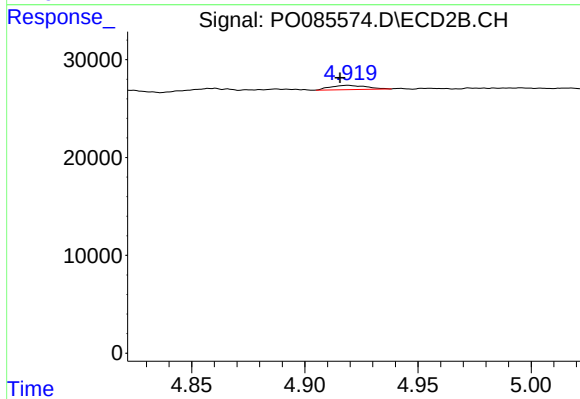

#6 AR-1016-4


R.T.: 4.919 min
Delta R.T.: 0.003 min
Response: 4798
Conc: 4.40 ng/ml

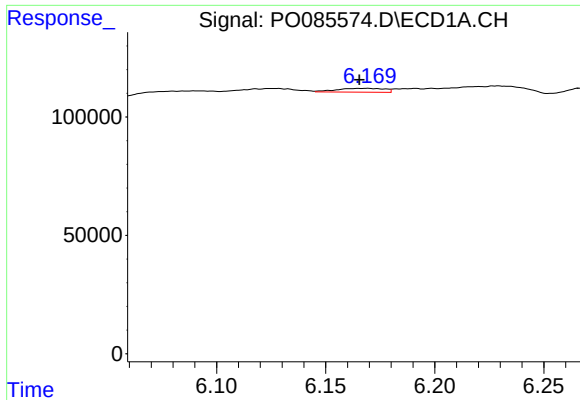

#7 AR-1016-5


R.T.: 6.169 min
Delta R.T.: 0.004 min
Response: 25290
Conc: 5.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

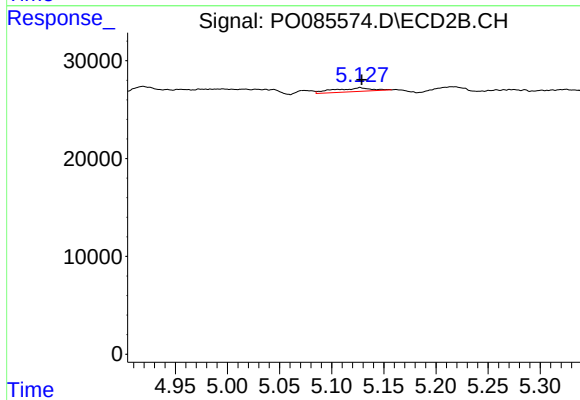


#7 AR-1016-5

R.T.: 5.127 min
Delta R.T.: -0.002 min
Response: 9479
Conc: 7.01 ng/ml

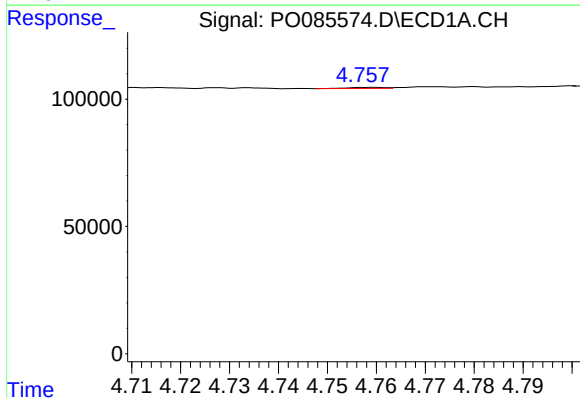


#8 AR-1221-1

R.T.: 4.759 min
Delta R.T.: 0.056 min
Response: 2039
Conc: 0.92 ng/ml

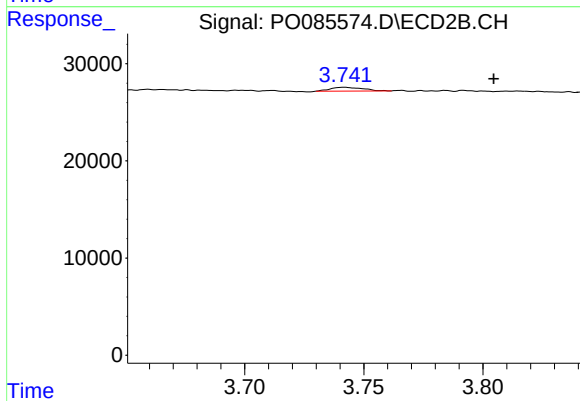

#8 AR-1221-1


R.T.: 3.742 min
Delta R.T.: -0.063 min
Response: 3820
Conc: 7.41 ng/ml

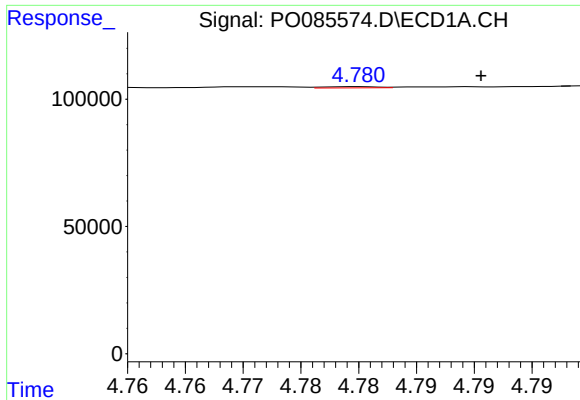

#9 AR-1221-2


R.T.: 4.780 min
Delta R.T.: -0.011 min
Response: 1526
Conc: 0.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

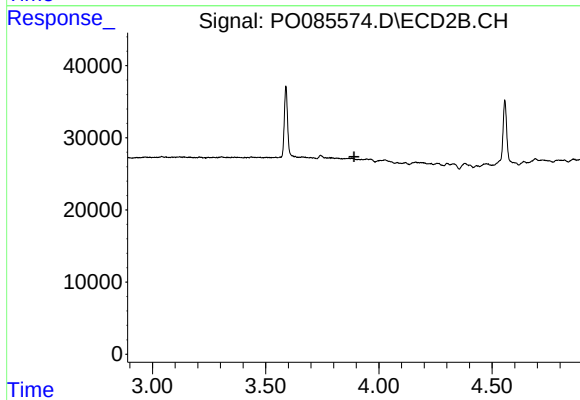


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

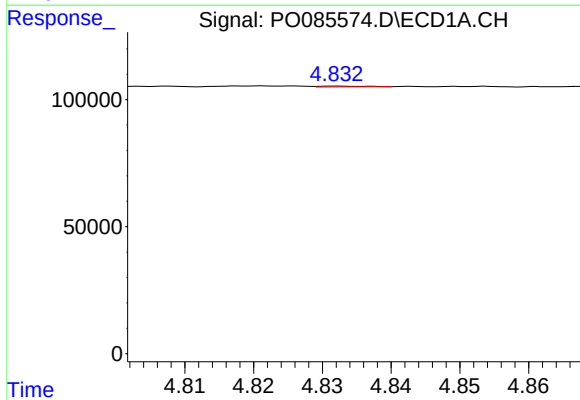


#10 AR-1221-3

R.T.: 4.832 min
Delta R.T.: -0.036 min
Response: 1529
Conc: 0.30 ng/ml

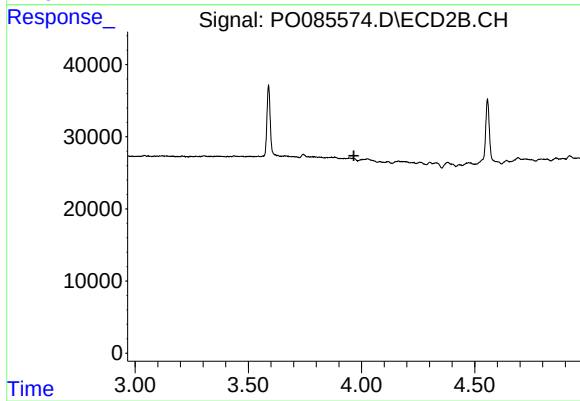

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

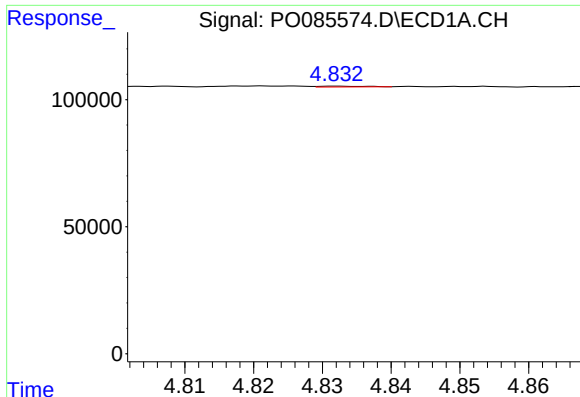

#11 AR-1232-1


R.T.: 4.832 min
Delta R.T.: -0.037 min
Response: 1529
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

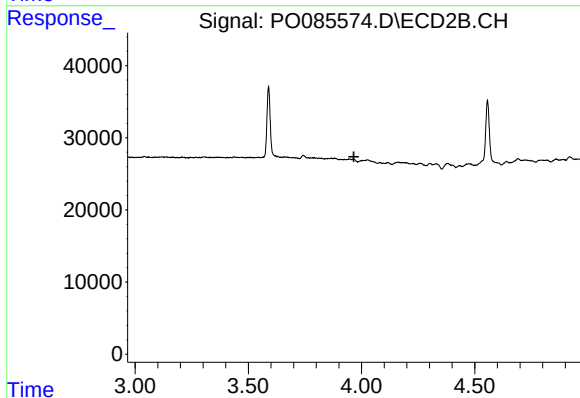


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

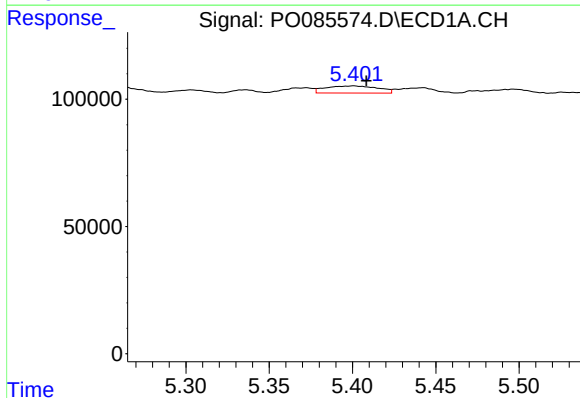


#12 AR-1232-2

R.T.: 5.401 min
Delta R.T.: -0.007 min
Response: 61067
Conc: 26.50 ng/ml

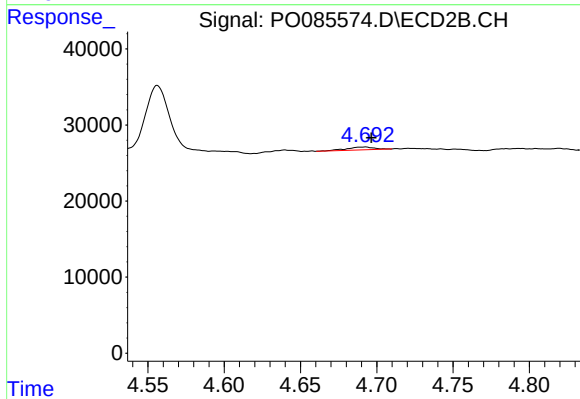

#12 AR-1232-2


R.T.: 4.693 min
Delta R.T.: -0.004 min
Response: 4713
Conc: 4.33 ng/ml

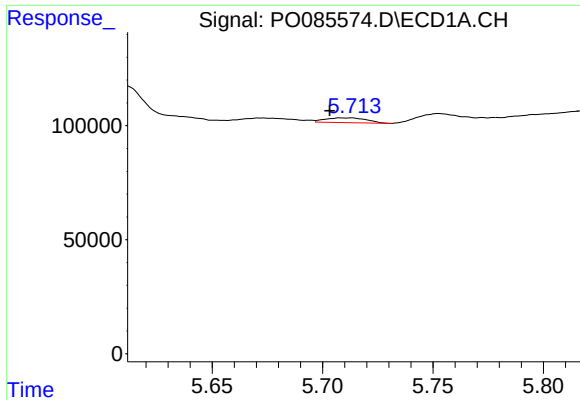

#13 AR-1232-3


R.T.: 5.713 min
Delta R.T.: 0.010 min
Response: 26838
Conc: 6.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

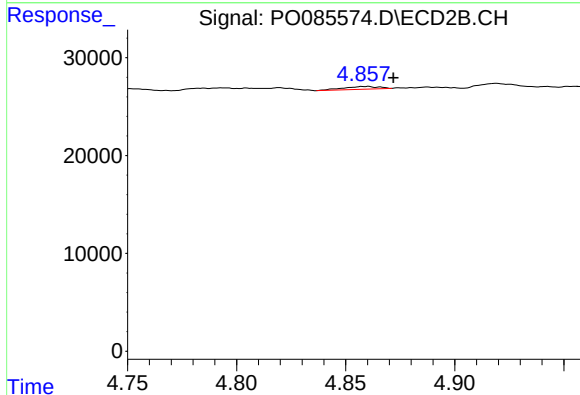


#13 AR-1232-3

R.T.: 4.861 min
Delta R.T.: -0.011 min
Response: 3282
Conc: 5.40 ng/ml

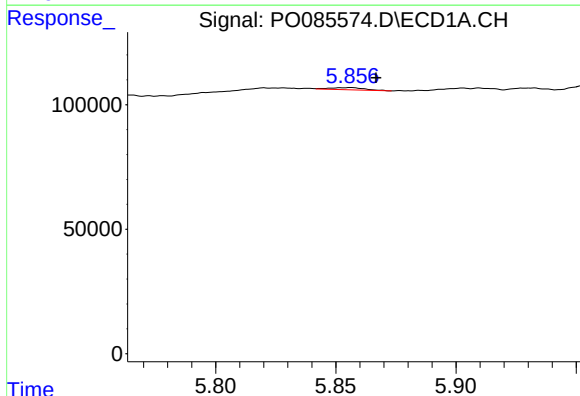


#14 AR-1232-4

R.T.: 5.856 min
Delta R.T.: -0.010 min
Response: 9049
Conc: 4.51 ng/ml

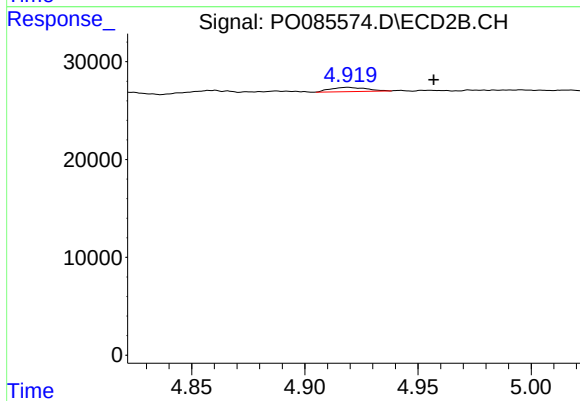

#14 AR-1232-4


R.T.: 4.919 min
Delta R.T.: -0.038 min
Response: 4798
Conc: 8.61 ng/ml

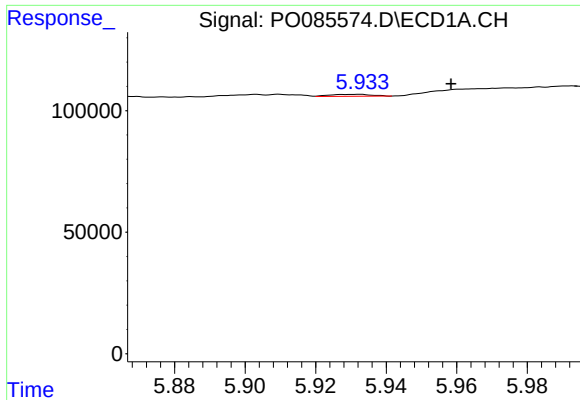

#15 AR-1232-5


R.T.: 5.933 min
Delta R.T.: -0.026 min
Response: 6665
Conc: 4.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

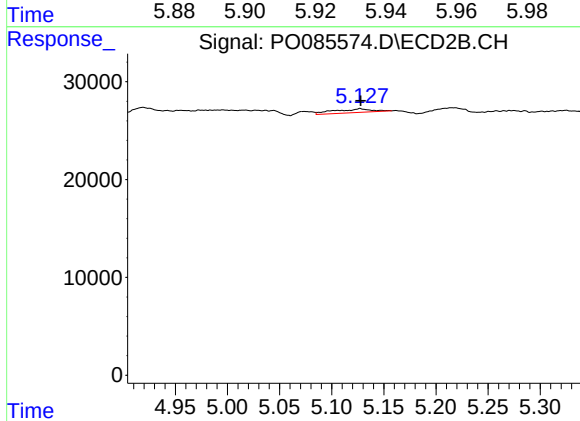


#15 AR-1232-5

R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 9479
Conc: 15.37 ng/ml

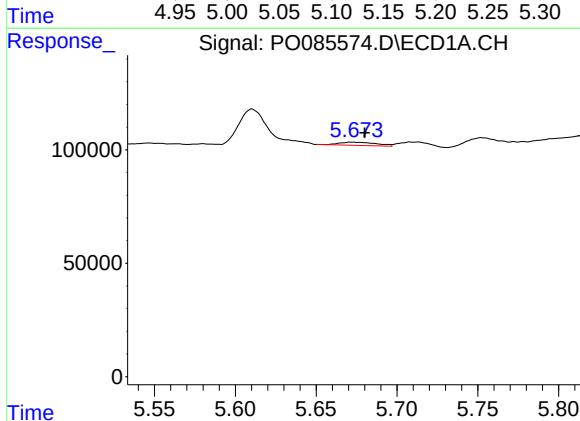


#16 AR-1242-1

R.T.: 5.673 min
Delta R.T.: -0.007 min
Response: 22463
Conc: 4.42 ng/ml

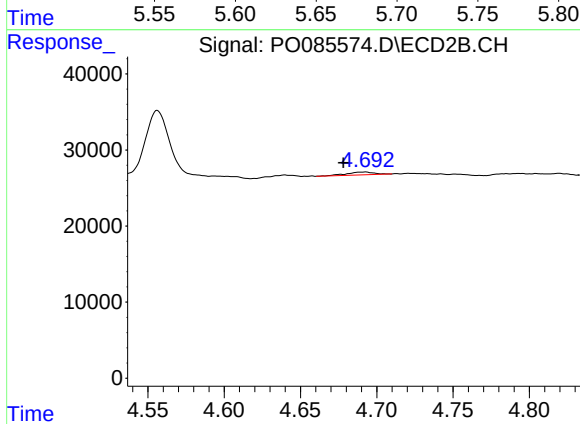

#16 AR-1242-1


R.T.: 4.693 min
Delta R.T.: 0.015 min
Response: 4713
Conc: 3.61 ng/ml

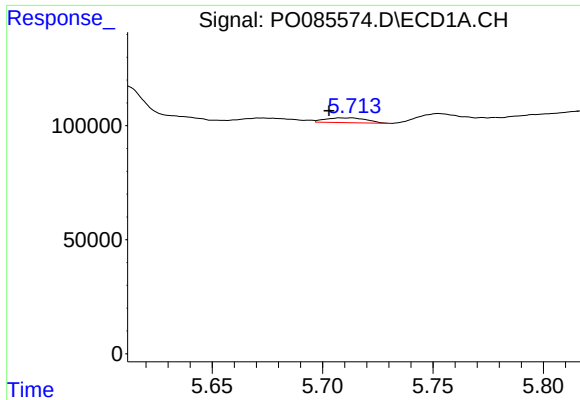

#17 AR-1242-2


R.T.: 5.713 min
Delta R.T.: 0.010 min
Response: 26838
Conc: 3.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

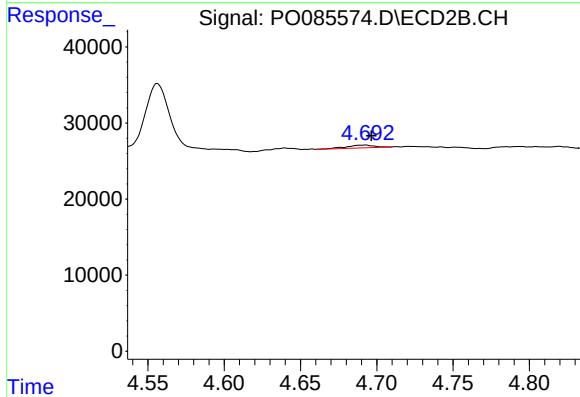


#17 AR-1242-2

R.T.: 4.693 min
Delta R.T.: -0.004 min
Response: 4713
Conc: 2.55 ng/ml

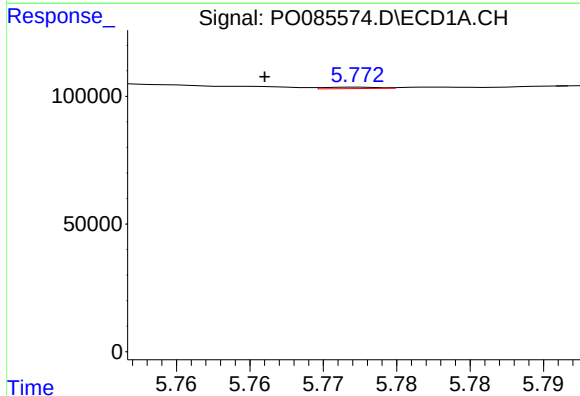


#18 AR-1242-3

R.T.: 5.772 min
Delta R.T.: 0.006 min
Response: 1394
Conc: 0.32 ng/ml

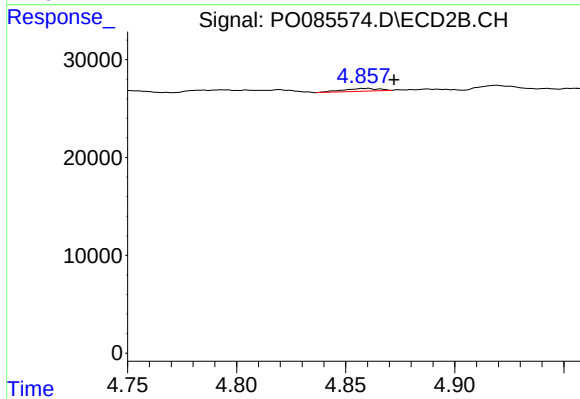

#18 AR-1242-3


R.T.: 4.861 min
Delta R.T.: -0.012 min
Response: 3282
Conc: 3.25 ng/ml

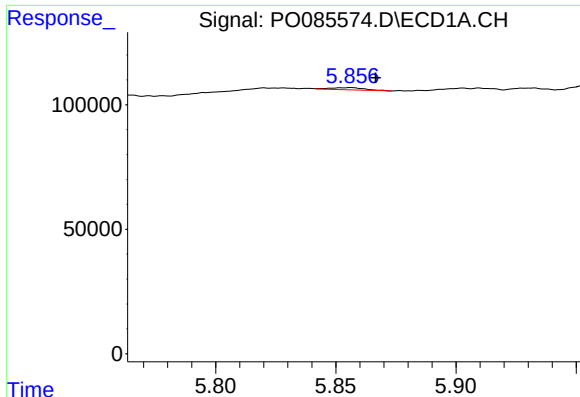

#19 AR-1242-4


R.T.: 5.856 min
Delta R.T.: -0.010 min
Response: 9049
Conc: 2.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

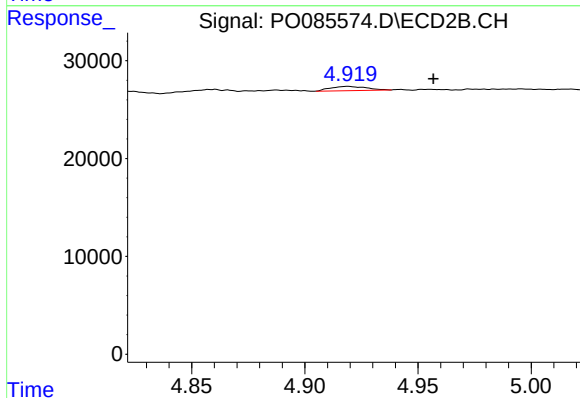


#19 AR-1242-4

R.T.: 4.919 min
Delta R.T.: -0.038 min
Response: 4798
Conc: 4.62 ng/ml

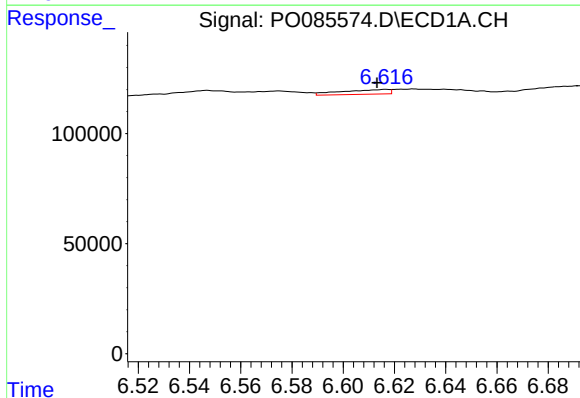


#20 AR-1242-5

R.T.: 6.617 min
Delta R.T.: 0.003 min
Response: 27701
Conc: 7.80 ng/ml

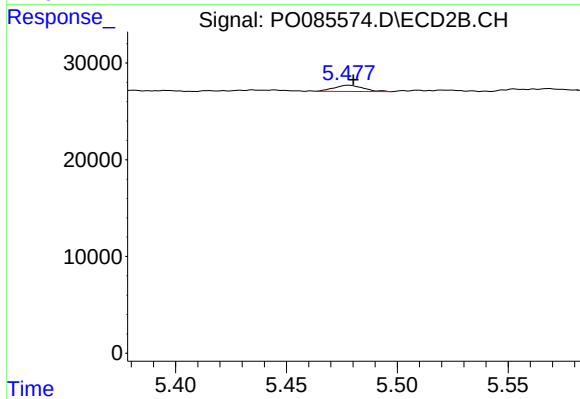

#20 AR-1242-5


R.T.: 5.478 min
Delta R.T.: -0.002 min
Response: 5827
Conc: 4.72 ng/ml

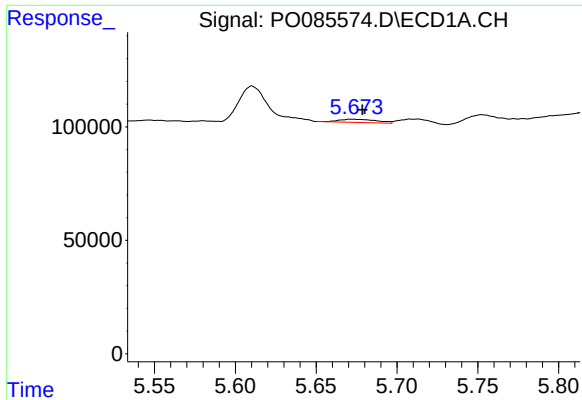

#21 AR-1248-1


R.T.: 5.673 min
Delta R.T.: -0.006 min
Response: 22463
Conc: 6.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

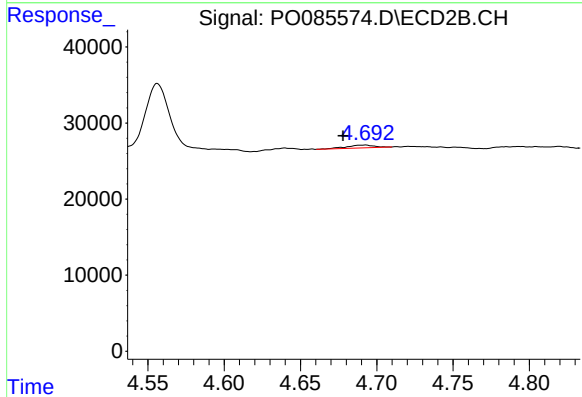


#21 AR-1248-1

R.T.: 4.693 min
Delta R.T.: 0.015 min
Response: 4713
Conc: 4.88 ng/ml

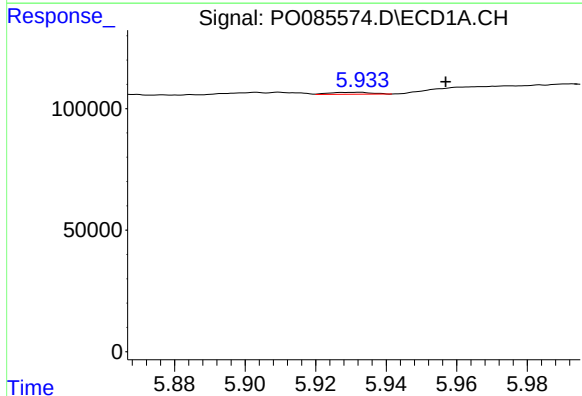


#22 AR-1248-2

R.T.: 5.933 min
Delta R.T.: -0.024 min
Response: 6665
Conc: 1.26 ng/ml

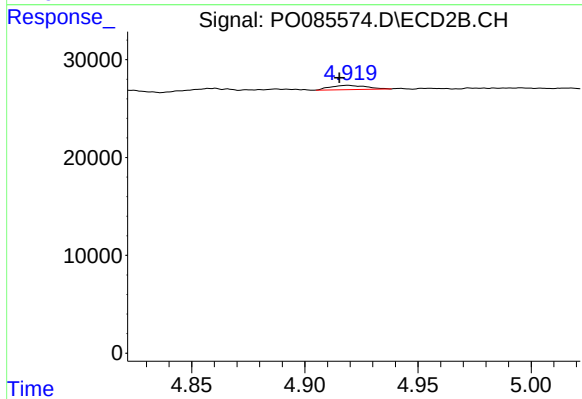

#22 AR-1248-2


R.T.: 4.919 min
Delta R.T.: 0.004 min
Response: 4798
Conc: 3.28 ng/ml

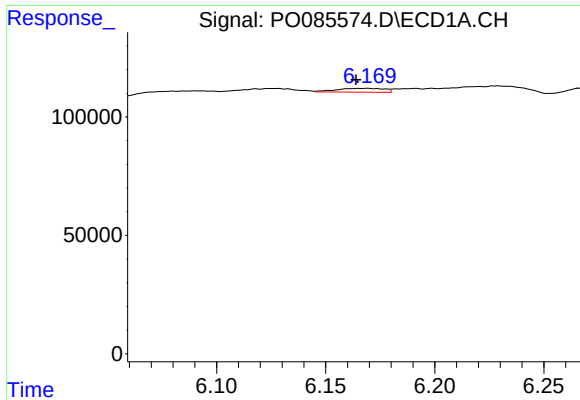

#23 AR-1248-3


R.T.: 6.169 min
Delta R.T.: 0.005 min
Response: 25290
Conc: 4.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

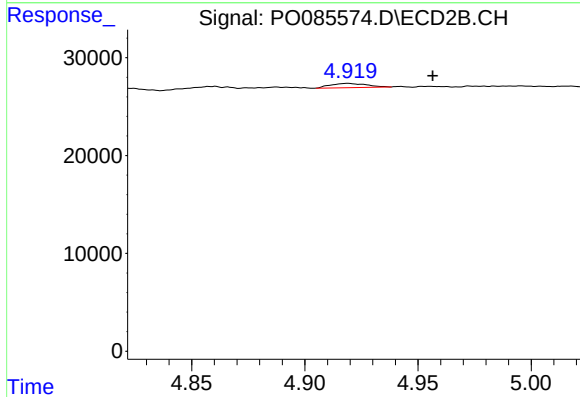


#23 AR-1248-3

R.T.: 4.919 min
Delta R.T.: -0.037 min
Response: 4798
Conc: 3.13 ng/ml

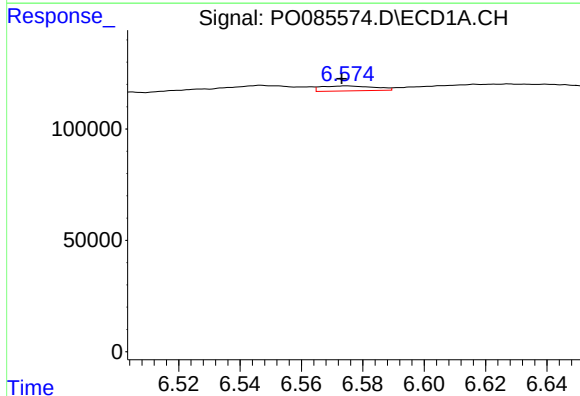


#24 AR-1248-4

R.T.: 6.575 min
Delta R.T.: 0.002 min
Response: 27157
Conc: 4.21 ng/ml

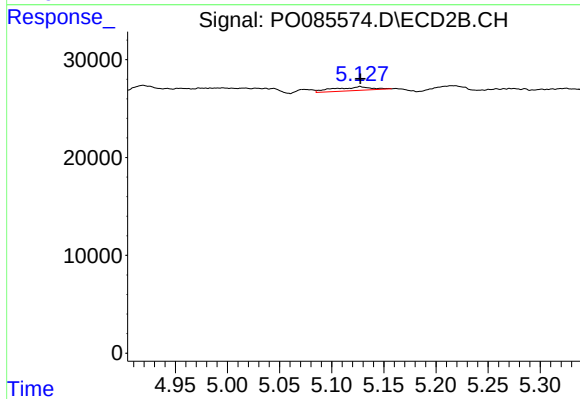

#24 AR-1248-4


R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 9479
Conc: 5.39 ng/ml

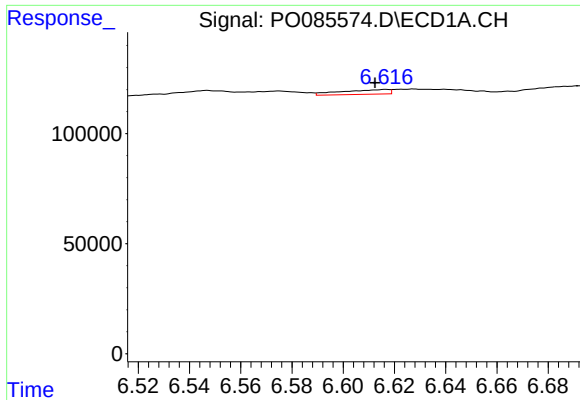

#25 AR-1248-5


R.T.: 6.617 min
Delta R.T.: 0.004 min
Response: 27701
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

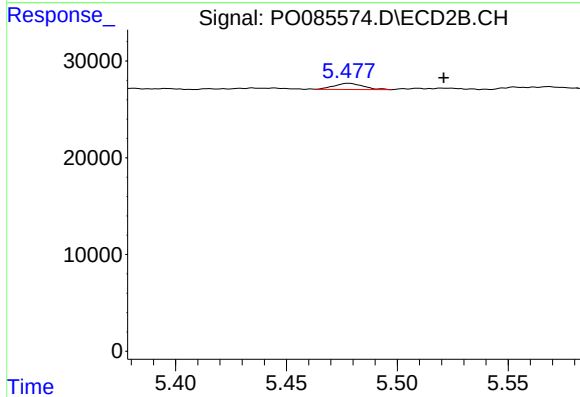


#25 AR-1248-5

R.T.: 5.478 min
Delta R.T.: -0.043 min
Response: 5827
Conc: 3.39 ng/ml

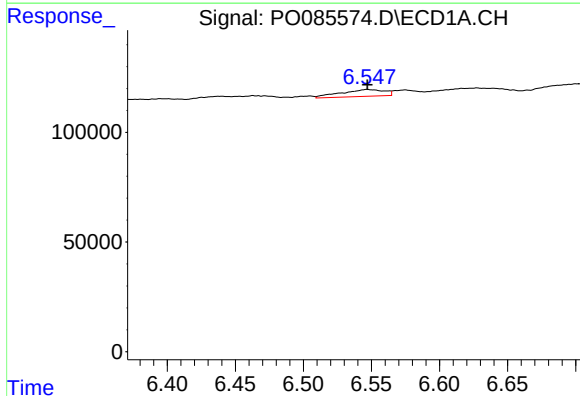


#26 AR-1254-1

R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 69758
Conc: 10.53 ng/ml

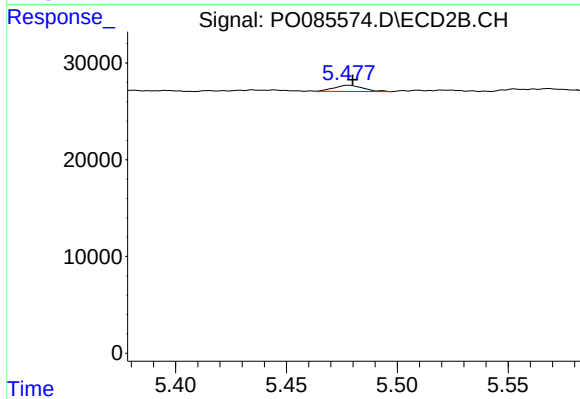

#26 AR-1254-1


R.T.: 5.478 min
Delta R.T.: -0.002 min
Response: 5827
Conc: 2.22 ng/ml

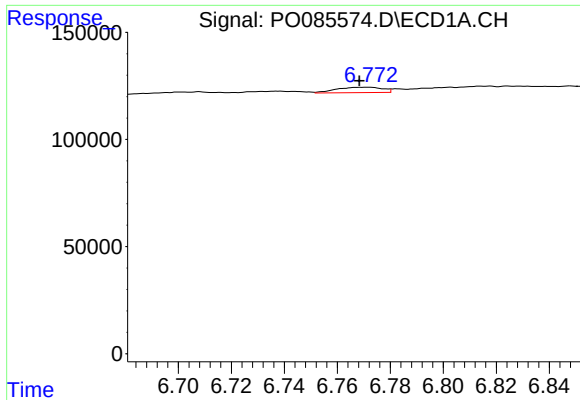

#27 AR-1254-2


R.T.: 6.772 min
Delta R.T.: 0.003 min
Response: 30680
Conc: 3.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

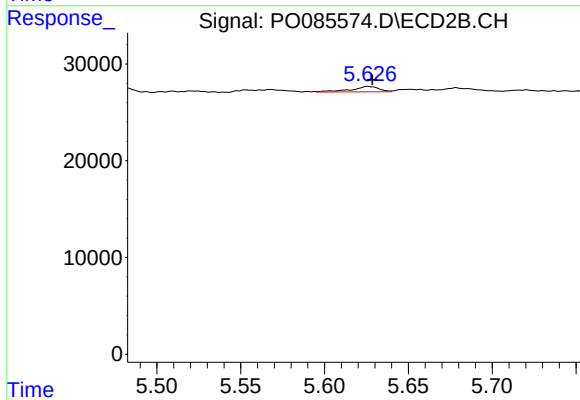


#27 AR-1254-2

R.T.: 5.626 min
Delta R.T.: -0.002 min
Response: 6229
Conc: 2.67 ng/ml

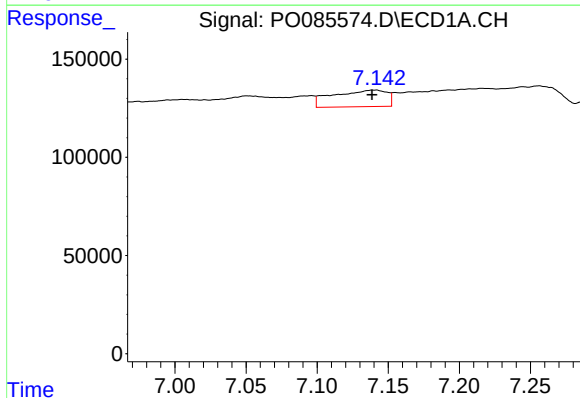


#28 AR-1254-3

R.T.: 7.142 min
Delta R.T.: 0.003 min
Response: 222435
Conc: 21.61 ng/ml

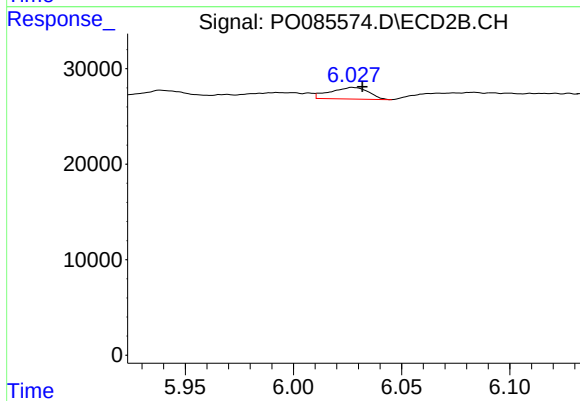

#28 AR-1254-3


R.T.: 6.028 min
Delta R.T.: -0.004 min
Response: 14951
Conc: 4.07 ng/ml

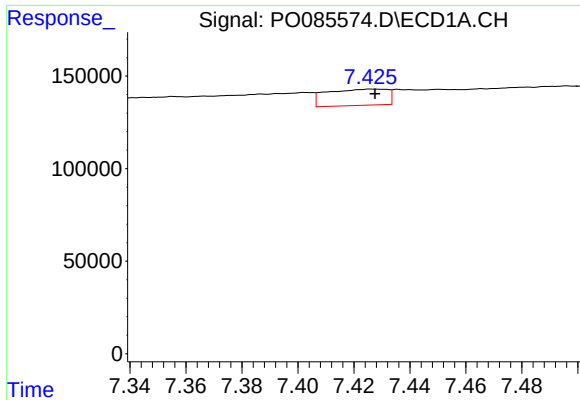

#29 AR-1254-4


R.T.: 7.426 min
Delta R.T.: -0.002 min
Response: 132447
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

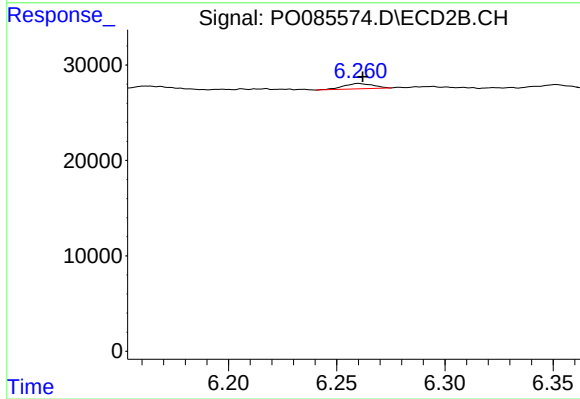


#29 AR-1254-4

R.T.: 6.260 min
Delta R.T.: -0.002 min
Response: 5334
Conc: 2.41 ng/ml

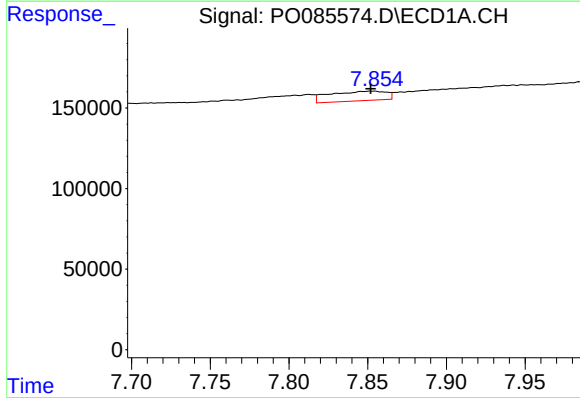


#30 AR-1254-5

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 147495
Conc: 19.28 ng/ml

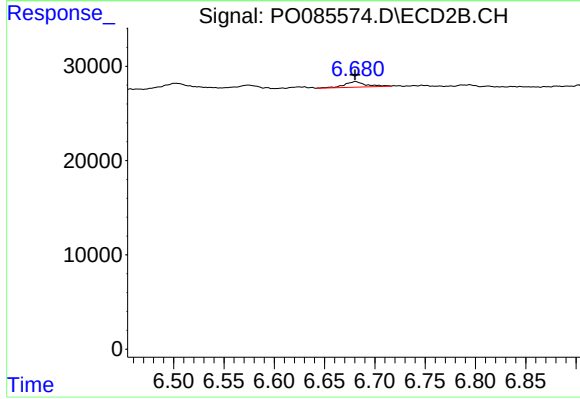

#30 AR-1254-5


R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 8569
Conc: 2.63 ng/ml

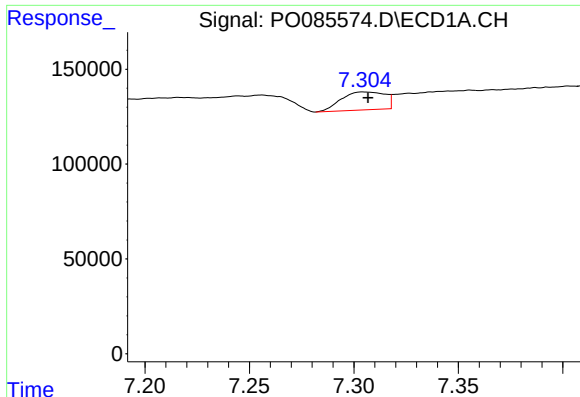

#31 AR-1260-1


R.T.: 7.304 min
Delta R.T.: -0.002 min
Response: 138015
Conc: 20.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

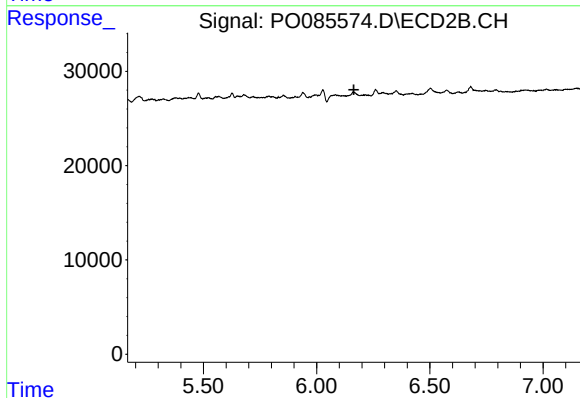


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.165 min
Response: 0
Conc: N.D.

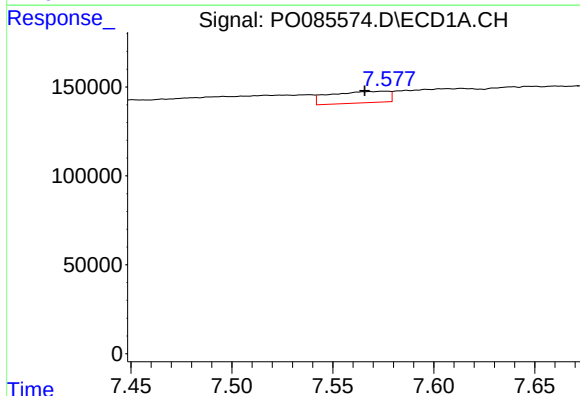


#32 AR-1260-2

R.T.: 7.577 min
Delta R.T.: 0.011 min
Response: 131564
Conc: 16.82 ng/ml

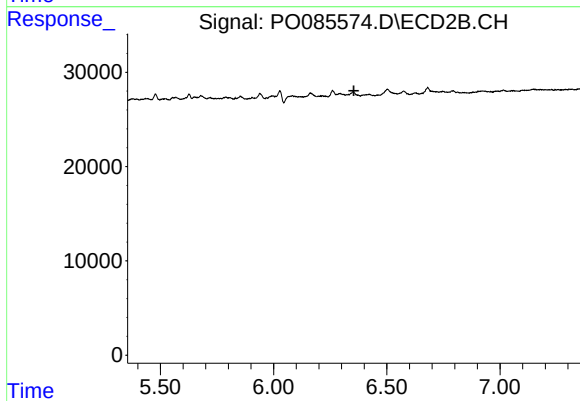

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

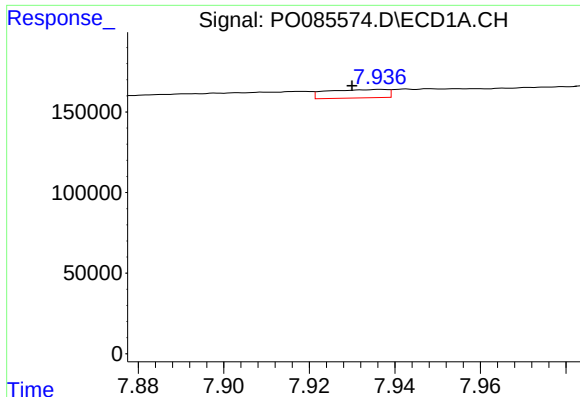

#33 AR-1260-3


R.T.: 7.937 min
Delta R.T.: 0.007 min
Response: 51453
Conc: 8.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

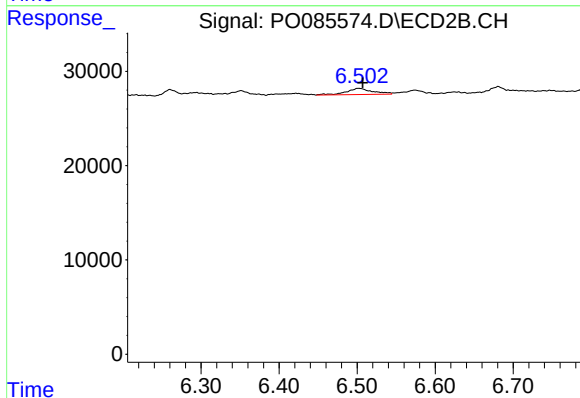


#33 AR-1260-3

R.T.: 6.502 min
Delta R.T.: -0.005 min
Response: 15362
Conc: 5.84 ng/ml

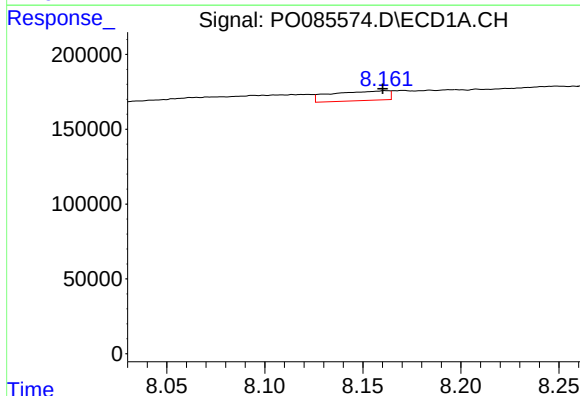


#34 AR-1260-4

R.T.: 8.161 min
Delta R.T.: 0.001 min
Response: 129319
Conc: 18.72 ng/ml

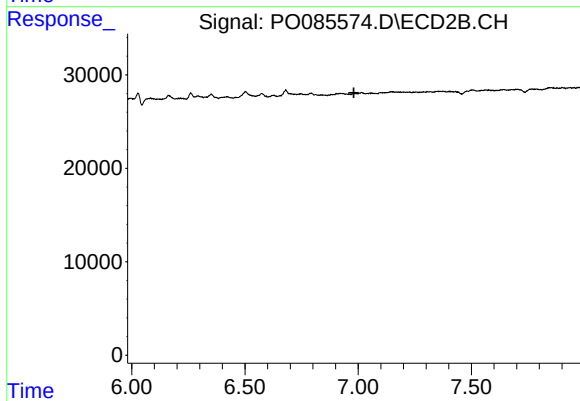

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.981 min
Response: 0
Conc: N.D.

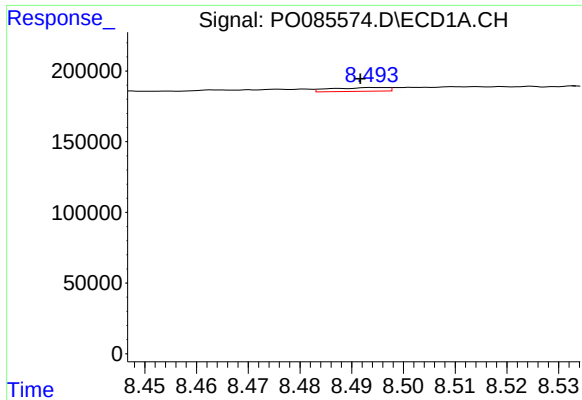

#35 AR-1260-5


R.T.: 8.494 min
Delta R.T.: 0.002 min
Response: 19843
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

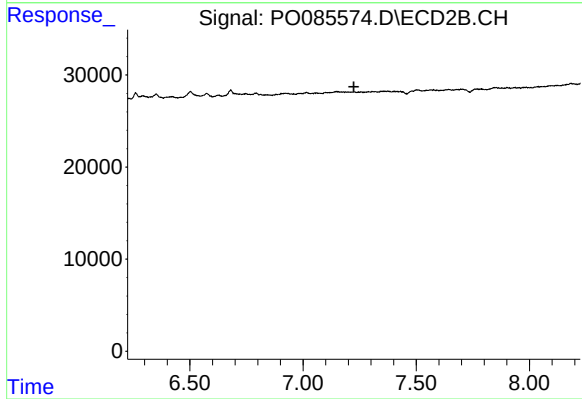


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.225 min
Response: 0
Conc: N.D.

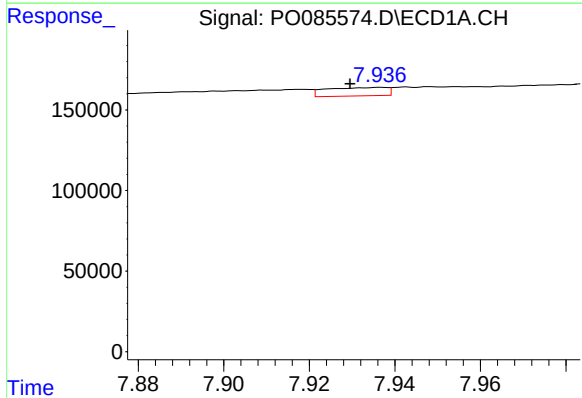


#36 AR-1262-1

R.T.: 7.937 min
Delta R.T.: 0.007 min
Response: 51453
Conc: 5.70 ng/ml

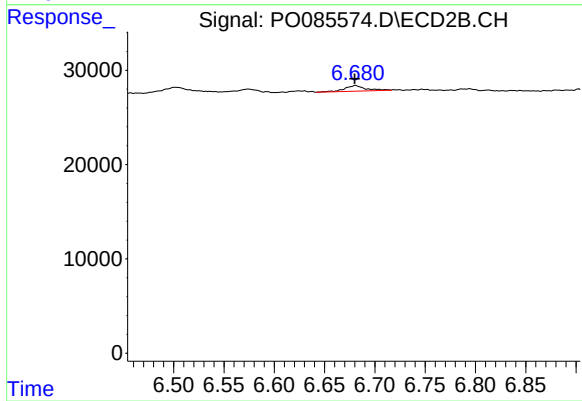

#36 AR-1262-1


R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 8569
Conc: 4.99 ng/ml

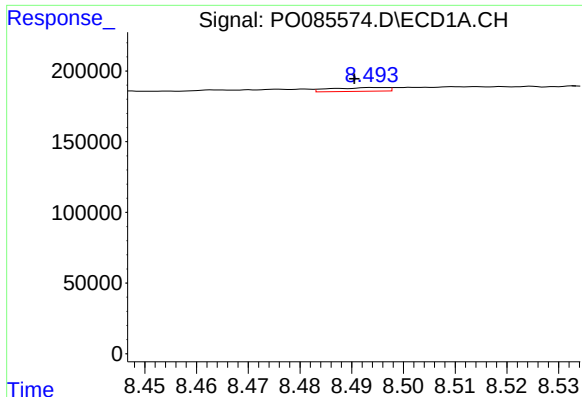

#37 AR-1262-2


R.T.: 8.494 min
Delta R.T.: 0.004 min
Response: 19843
Conc: 1.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

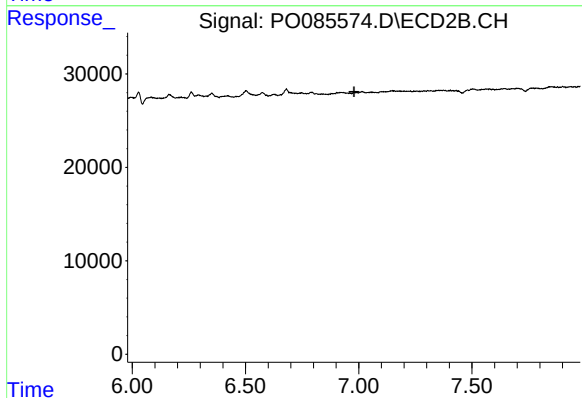


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

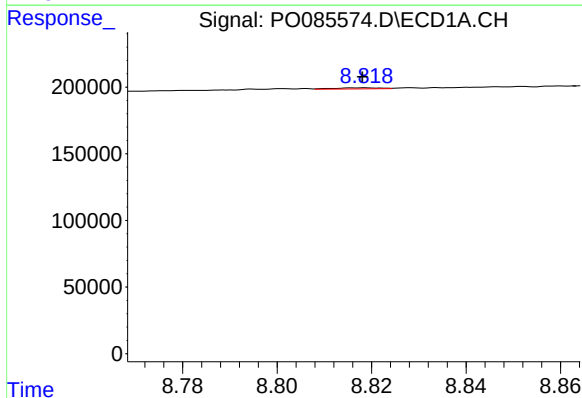


#38 AR-1262-3

R.T.: 8.819 min
Delta R.T.: 0.000 min
Response: 5298
Conc: 0.51 ng/ml

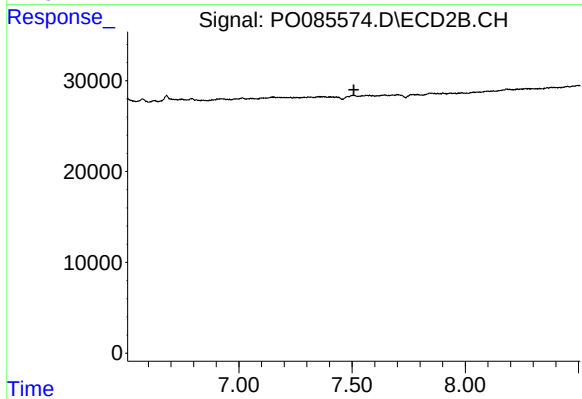

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.508 min
Response: 0
Conc: N.D.

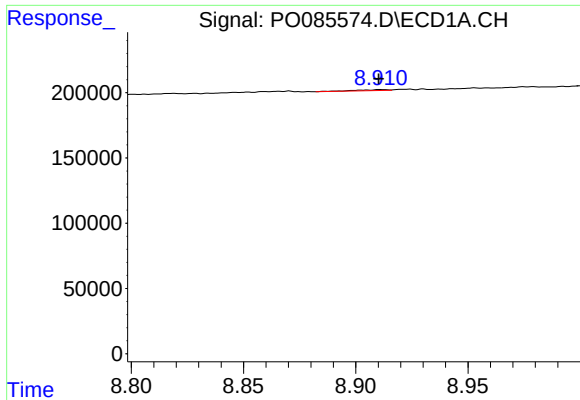

#39 AR-1262-4


R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 7360
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

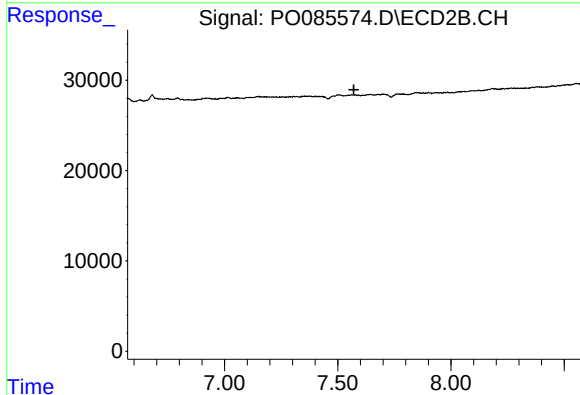


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.571 min
Response: 0
Conc: N.D.

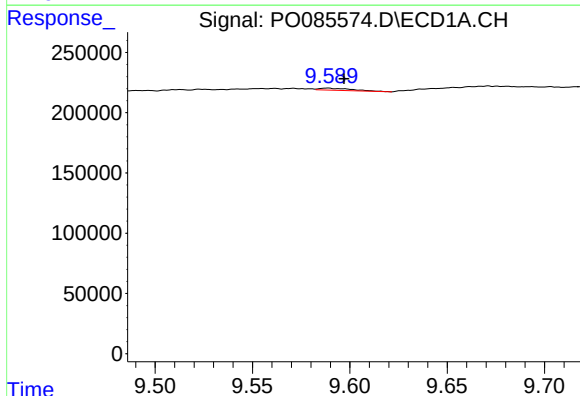


#40 AR-1262-5

R.T.: 9.589 min
Delta R.T.: -0.008 min
Response: 20118
Conc: 3.78 ng/ml

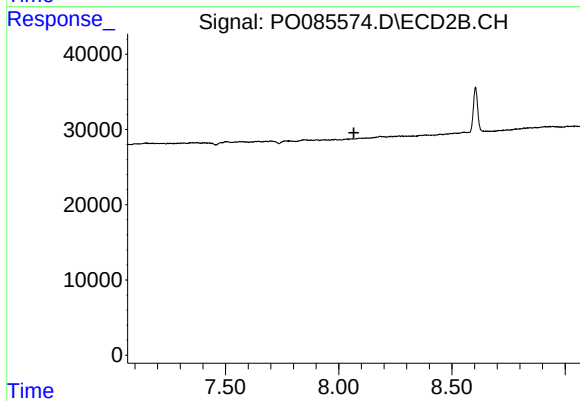

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.067 min
Response: 0
Conc: N.D.

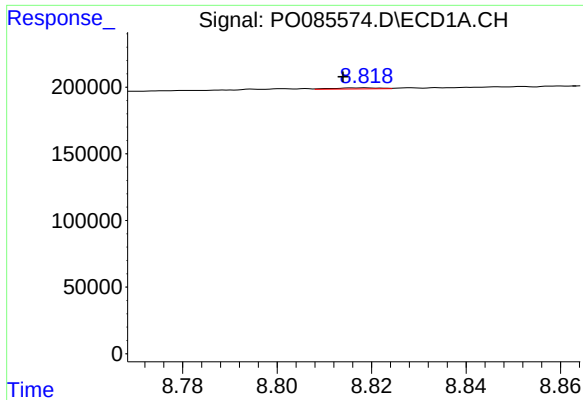

#41 AR-1268-1


R.T.: 8.819 min
Delta R.T.: 0.005 min
Response: 5298
Conc: 0.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

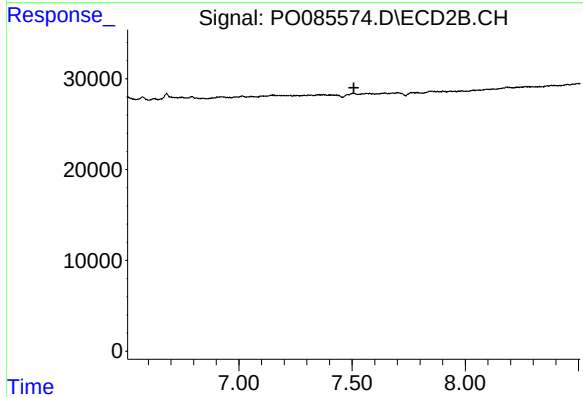


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.508 min
Response: 0
Conc: N.D.

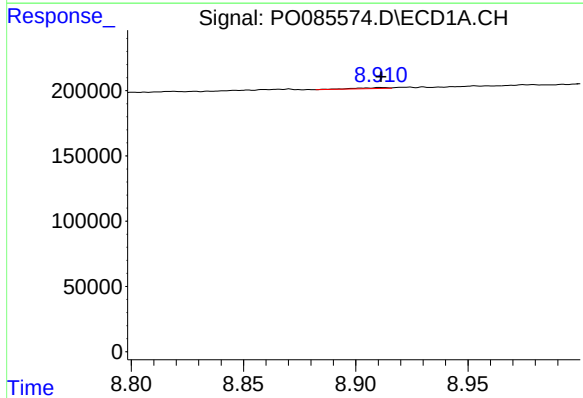


#42 AR-1268-2

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 7360
Conc: 0.42 ng/ml

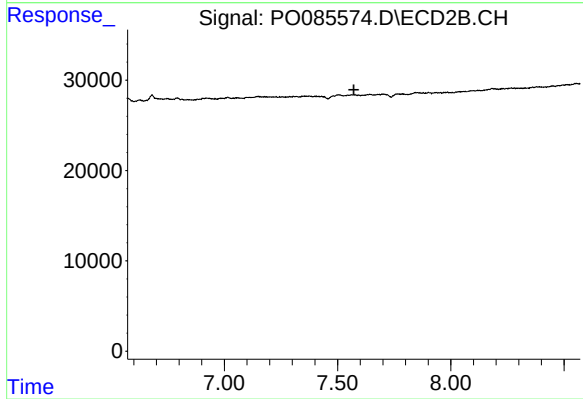

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

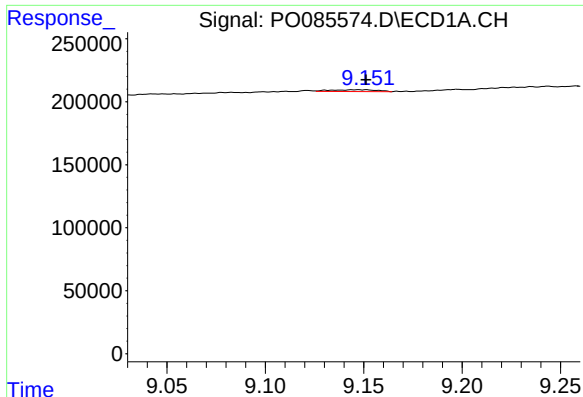

#43 AR-1268-3


R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 24464
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

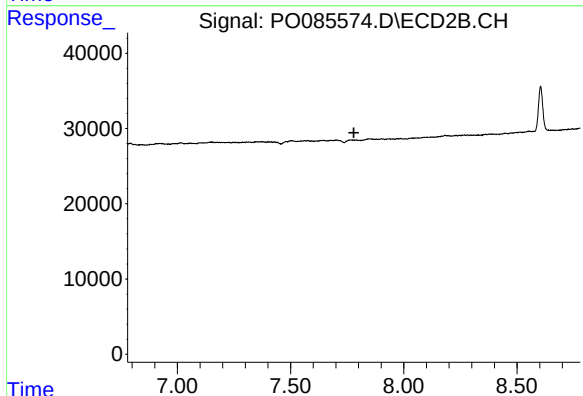


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

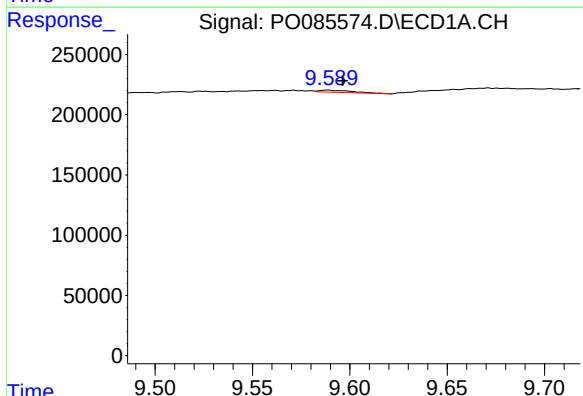


#44 AR-1268-4

R.T.: 9.589 min
Delta R.T.: -0.007 min
Response: 20118
Conc: 3.30 ng/ml

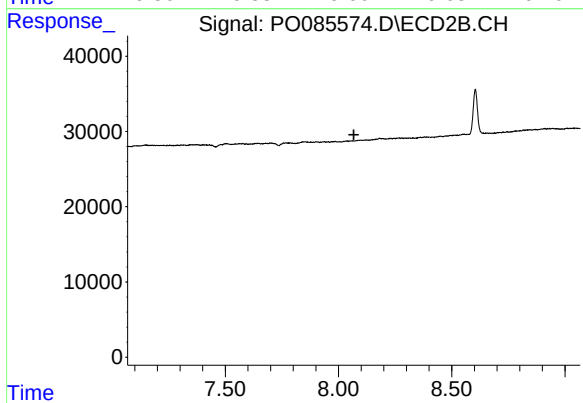

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.068 min
Response: 0
Conc: N.D.

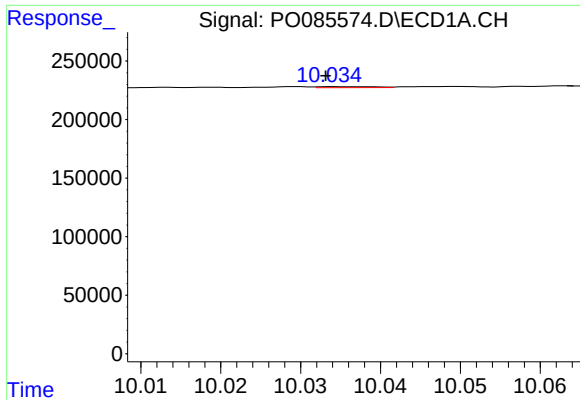

#45 AR-1268-5

R.T.: 10.034 min
Delta R.T.: 0.001 min
Response: 4116
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-34A

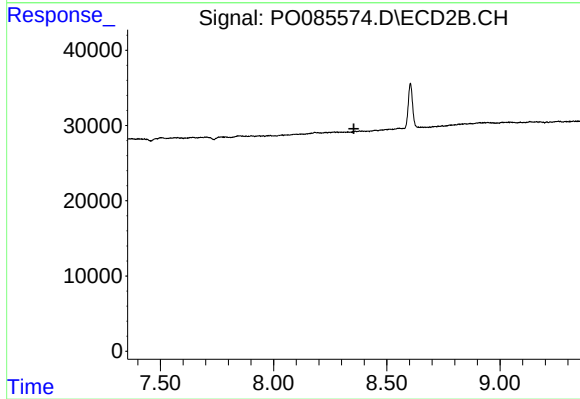

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.