

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032322\
 Data File : P0085585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 21:45
 Operator : YP\AJ
 Sample : N2053-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AUD-1285

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:25:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.589	3327335	945662	16.272	22.073 #
2) SA Decachlor...	10.394	8.607	2571853	688159	21.395	17.924
Target Compounds						
31) L7 AR-1260-1	7.304	6.163	83106	42647	12.044m	17.988 #
32) L7 AR-1260-2	7.557	6.353	592257	50262	75.711	18.005m#
33) L7 AR-1260-3	7.934	6.504	430845	49446	73.353m	18.807m#
34) L7 AR-1260-4	8.158	6.979	127719	31079	18.491m	13.876m
35) L7 AR-1260-5	8.491	7.222	138266	55970	9.842m	11.110m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
Data File : P0085585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 21:45
Operator : YP\AJ
Sample : N2053-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1285


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:25:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

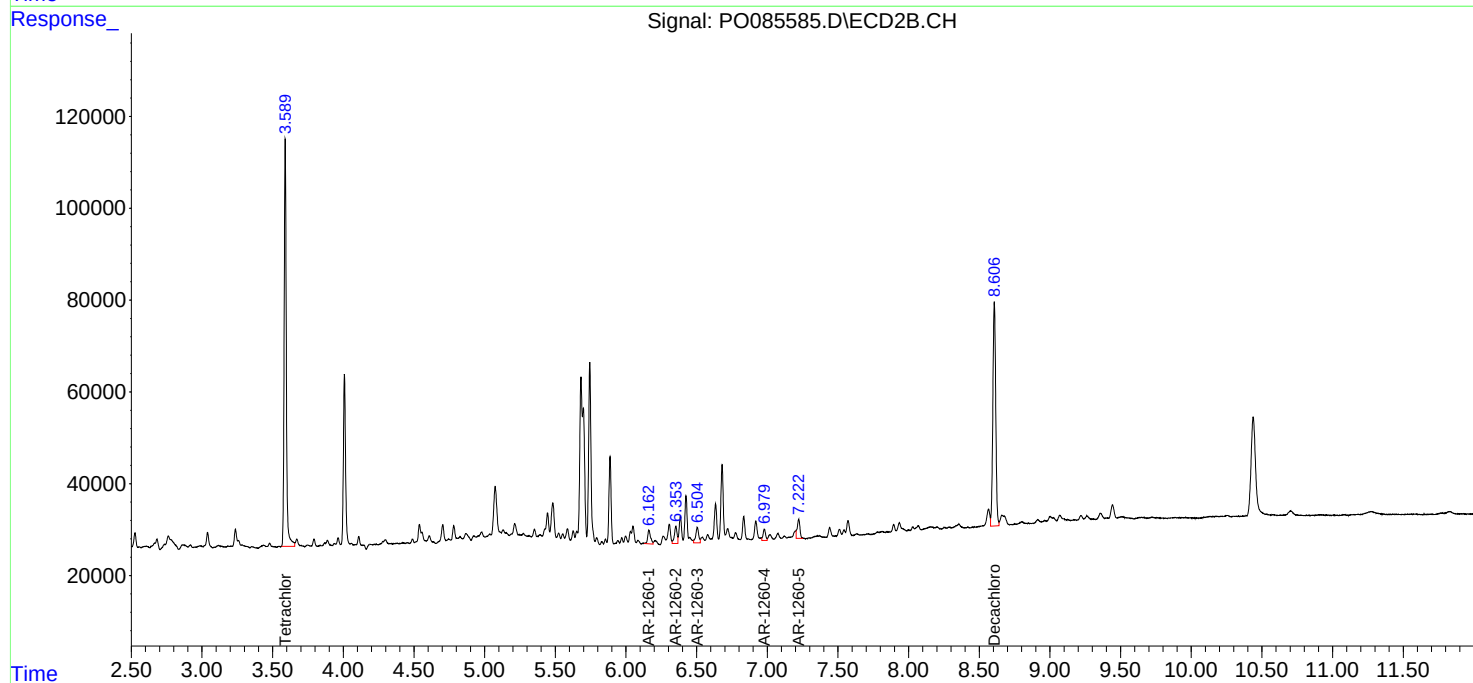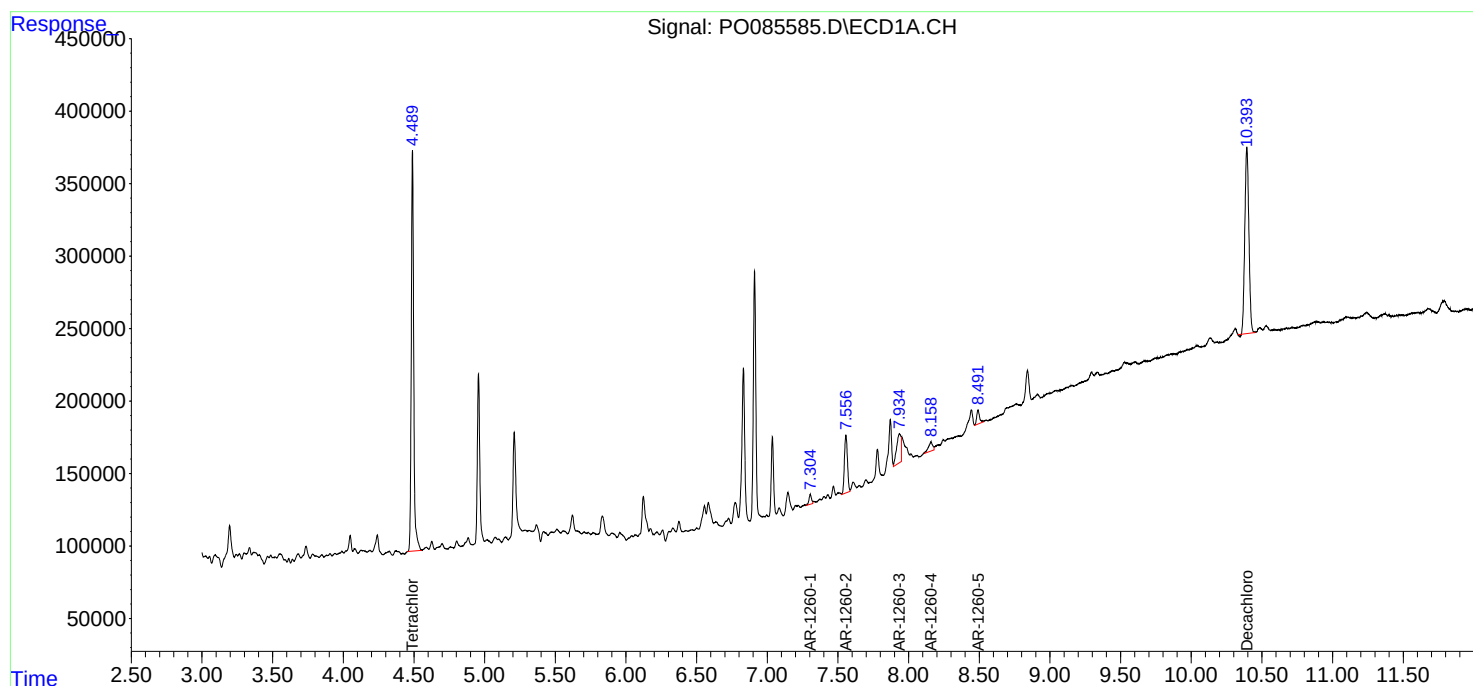

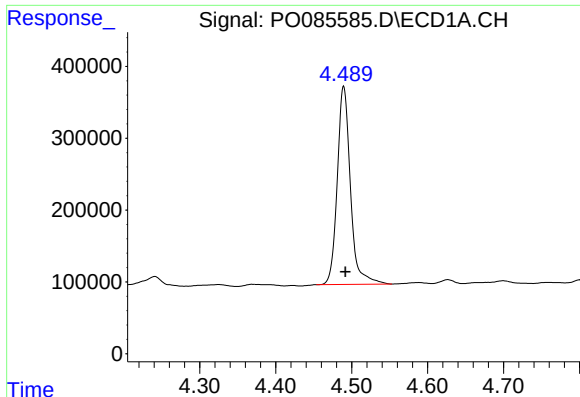


#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: -0.002 min
Response: 3327335
Conc: 16.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1285


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

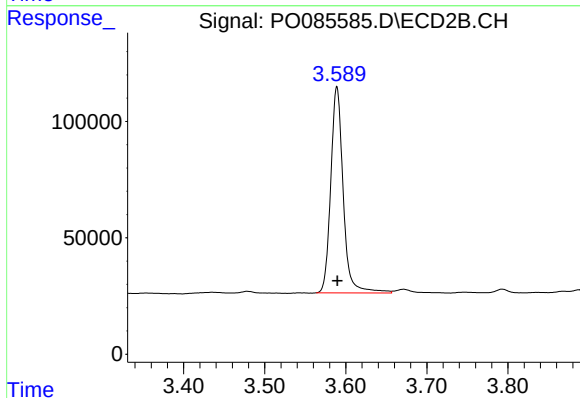


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: 0.000 min
Response: 945662
Conc: 22.07 ng/ml

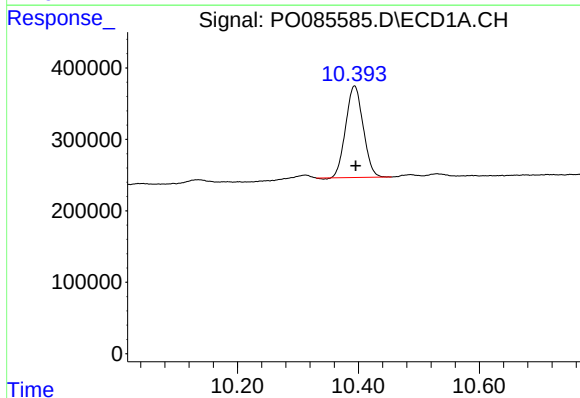


#2 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: -0.002 min
Response: 2571853
Conc: 21.40 ng/ml

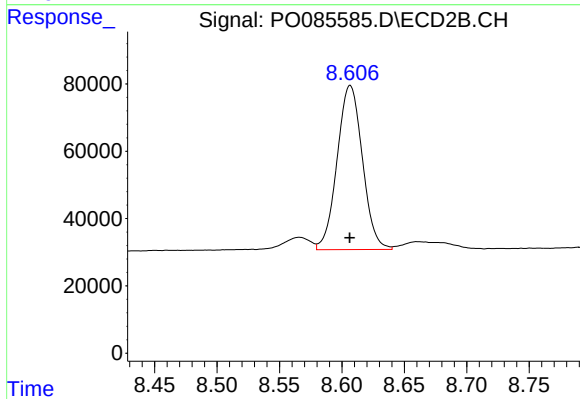

#2 Decachlorobiphenyl

R.T.: 8.607 min
Delta R.T.: 0.000 min
Response: 688159
Conc: 17.92 ng/ml

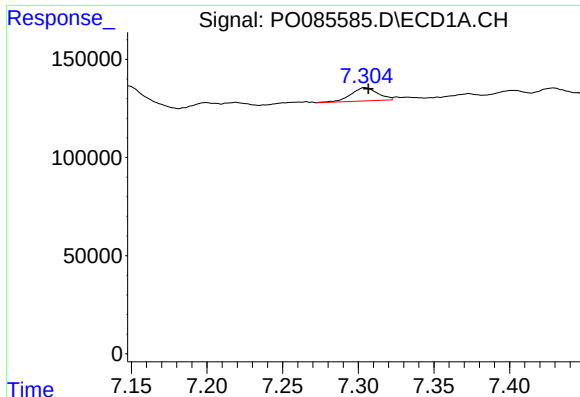


#31 AR-1260-1

R.T.: 7.304 min
Delta R.T.: -0.003 min
Response: 83106
Conc: 12.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1285


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

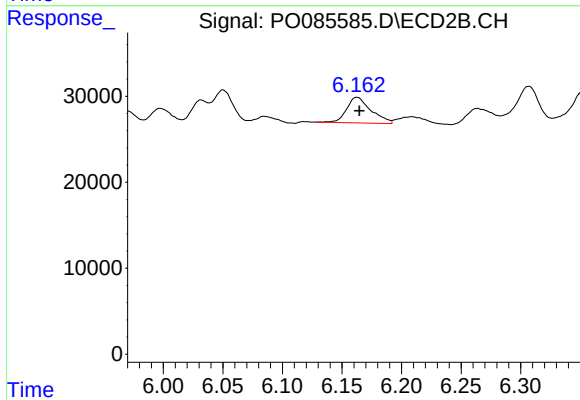


#31 AR-1260-1

R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 42647
Conc: 17.99 ng/ml

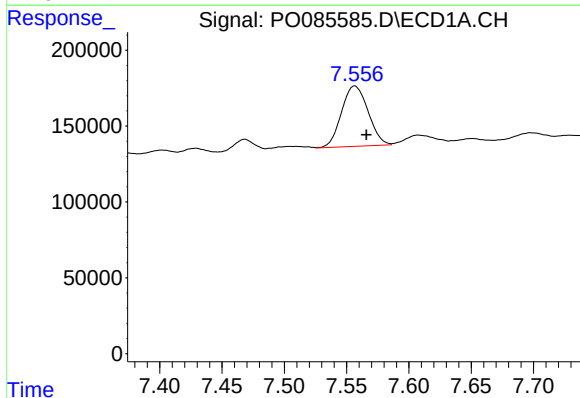


#32 AR-1260-2

R.T.: 7.557 min
Delta R.T.: -0.009 min
Response: 592257
Conc: 75.71 ng/ml

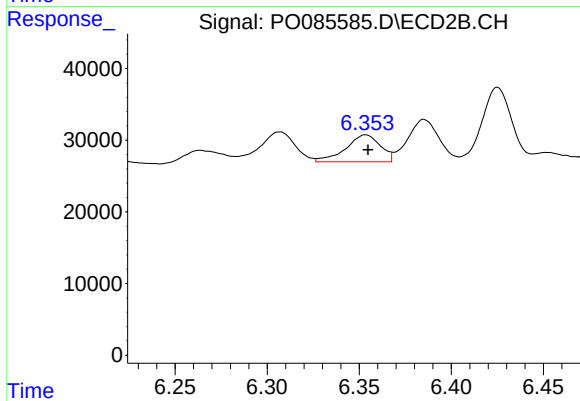

#32 AR-1260-2

R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 50262
Conc: 18.00 ng/ml m

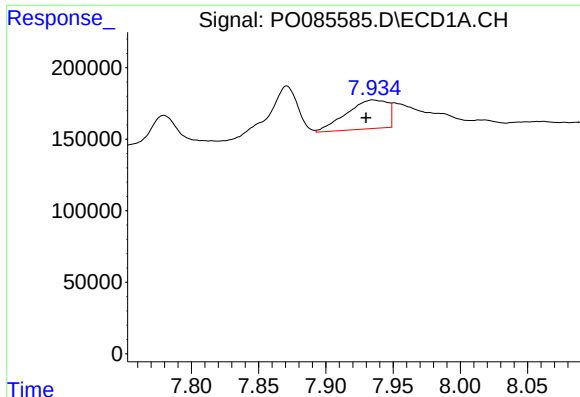


#33 AR-1260-3

R.T.: 7.934 min
Delta R.T.: 0.004 min
Response: 430845
Conc: 73.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1285


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

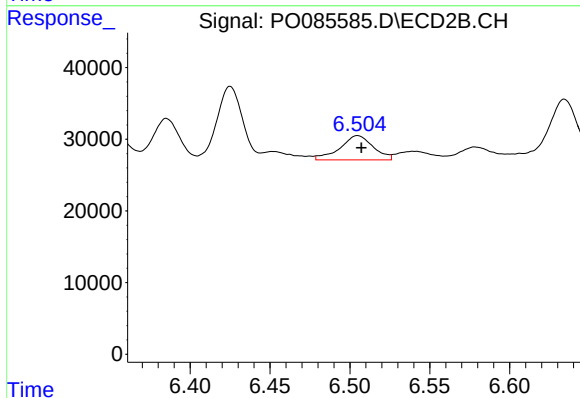


#33 AR-1260-3

R.T.: 6.504 min
Delta R.T.: -0.003 min
Response: 49446
Conc: 18.81 ng/ml m

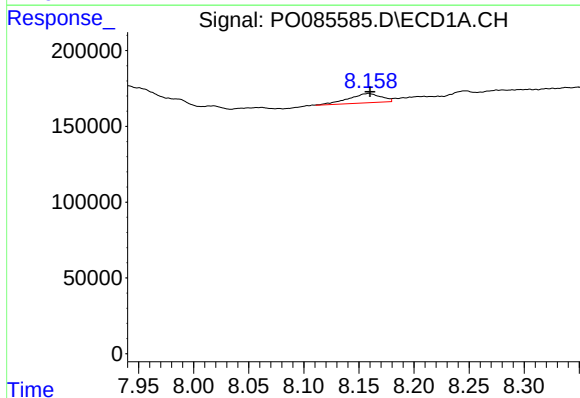


#34 AR-1260-4

R.T.: 8.158 min
Delta R.T.: -0.002 min
Response: 127719
Conc: 18.49 ng/ml m

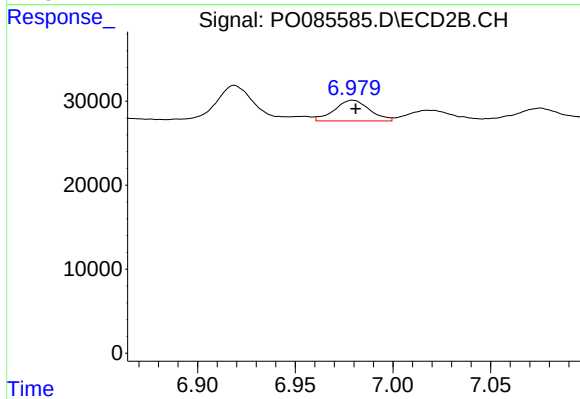

#34 AR-1260-4

R.T.: 6.979 min
Delta R.T.: -0.002 min
Response: 31079
Conc: 13.88 ng/ml m

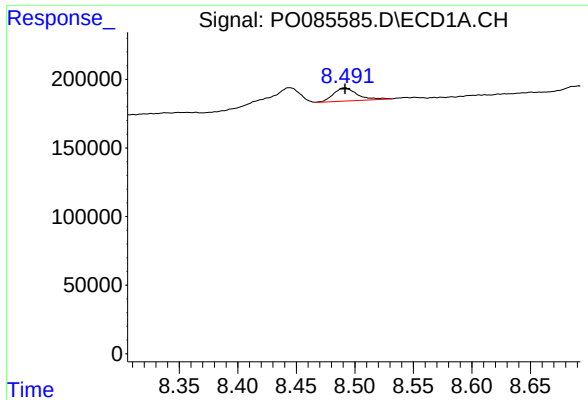


#35 AR-1260-5

R.T.: 8.491 min
Delta R.T.: 0.000 min
Response: 138266
Conc: 9.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1285

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

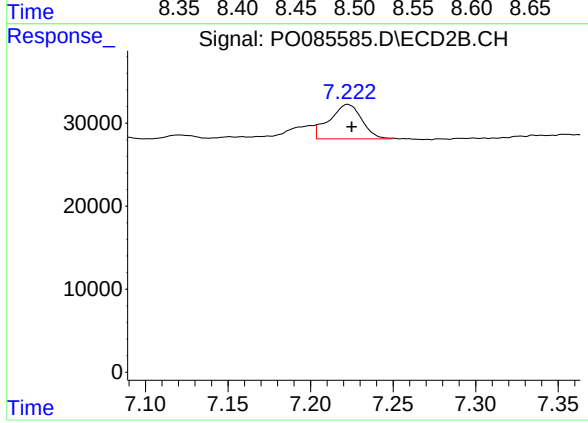

#35 AR-1260-5

R.T.: 7.222 min
Delta R.T.: -0.003 min
Response: 55970
Conc: 11.11 ng/ml m