

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
 Data File : P0085586.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2022 22:01
 Operator : YP\AJ
 Sample : N2053-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1286

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 01:25:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.589	2429352	793619	11.881	18.524 #
2) SA Decachlor...	10.393	8.606	2371010	640414	19.725m	16.680
Target Compounds						
31) L7 AR-1260-1	7.303	6.163	137856	74021	19.979	31.222 #
32) L7 AR-1260-2	7.557	6.352	514054	76550	65.714	27.422m#
33) L7 AR-1260-3	7.948	6.505	1225022	93014	208.563m	35.378m#
34) L7 AR-1260-4	8.156	6.979	165019	41416	23.892m	18.491m
35) L7 AR-1260-5	8.490	7.224	212213	77857	15.105m	15.454m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032322\
Data File : P0085586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2022 22:01
Operator : YP\AJ
Sample : N2053-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1286


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 01:25:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

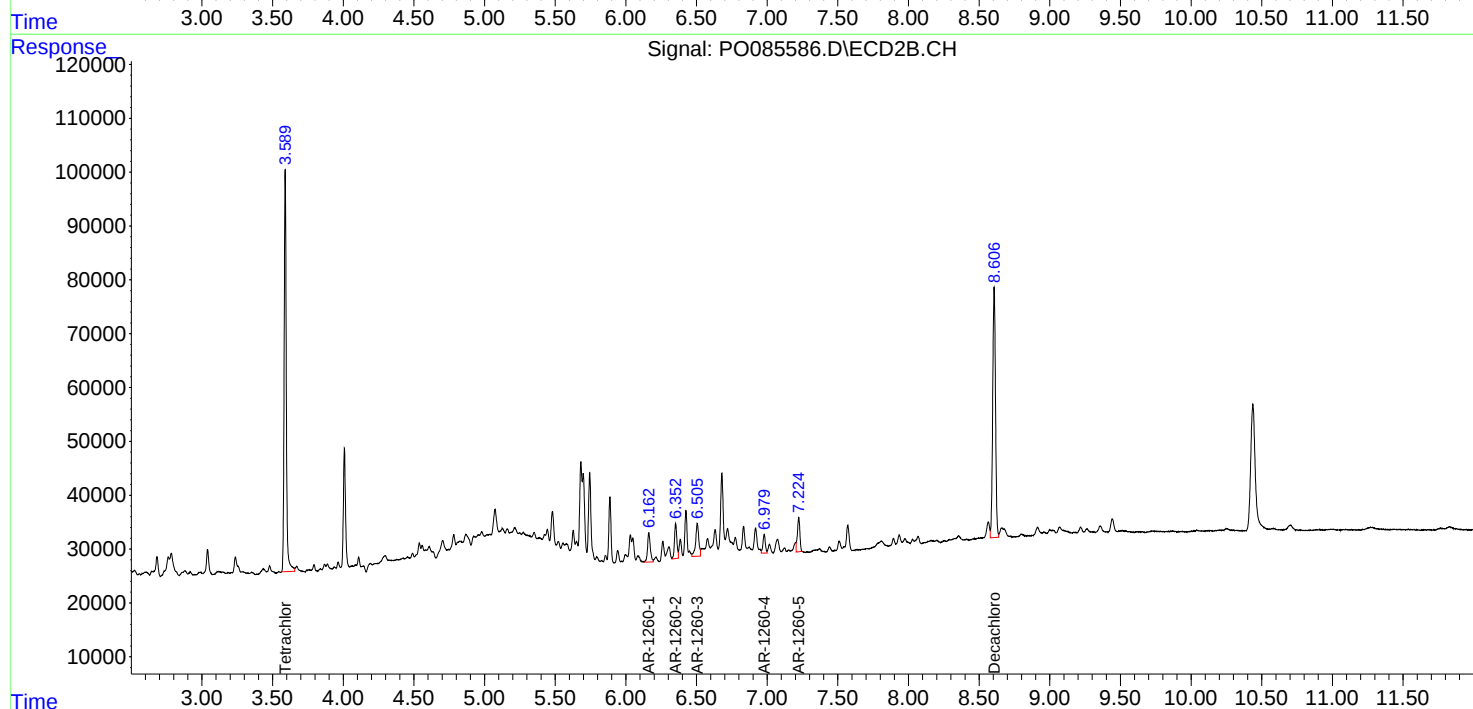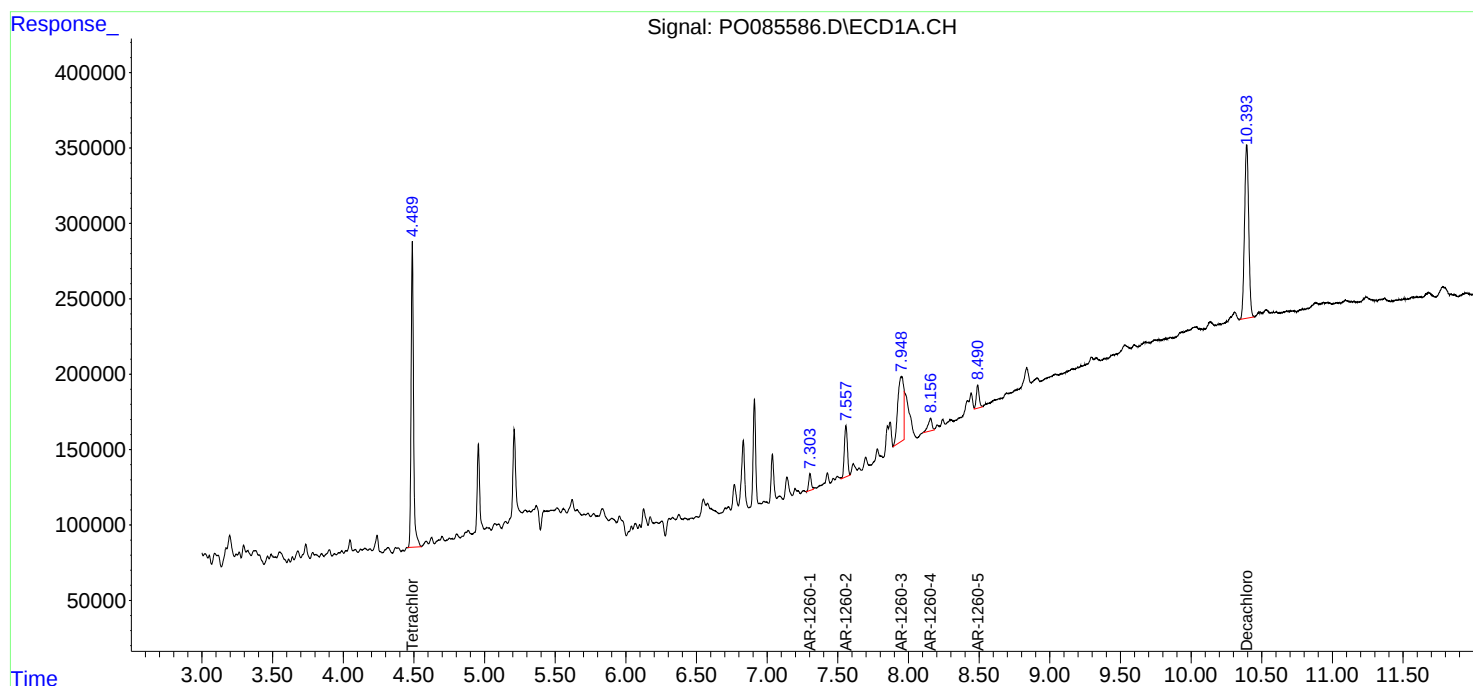

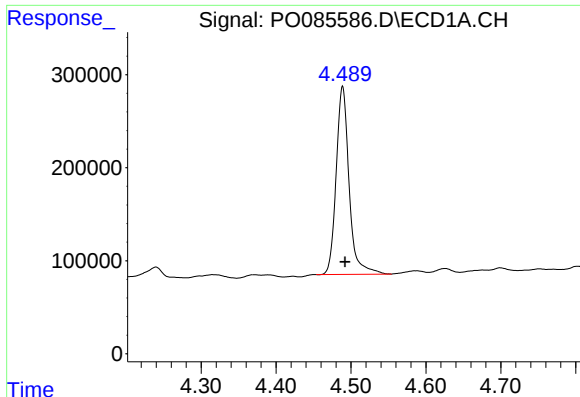


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.003 min
Response: 2429352
Conc: 11.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1286


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

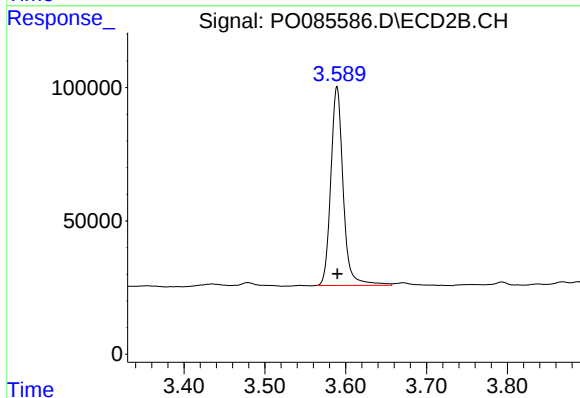


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: 0.000 min
Response: 793619
Conc: 18.52 ng/ml

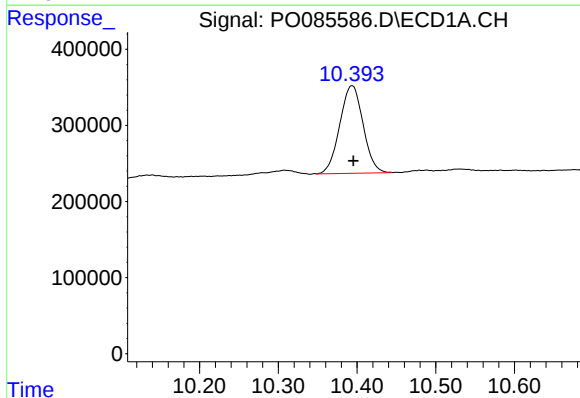


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.002 min
Response: 2371010
Conc: 19.72 ng/ml m

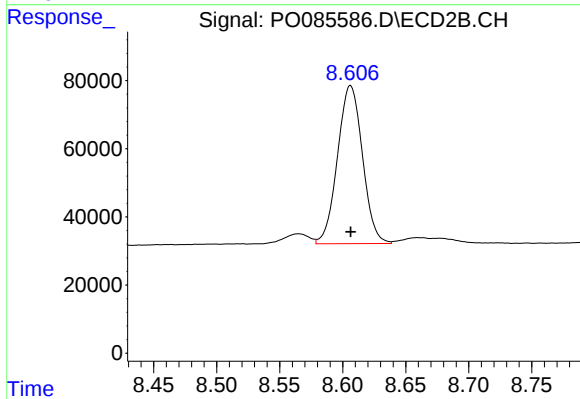

#2 Decachlorobiphenyl

R.T.: 8.606 min
Delta R.T.: 0.000 min
Response: 640414
Conc: 16.68 ng/ml

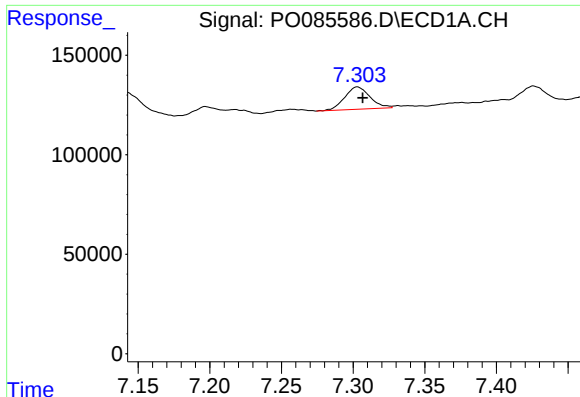


#31 AR-1260-1

R.T.: 7.303 min
Delta R.T.: -0.004 min
Response: 137856
Conc: 19.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1286


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

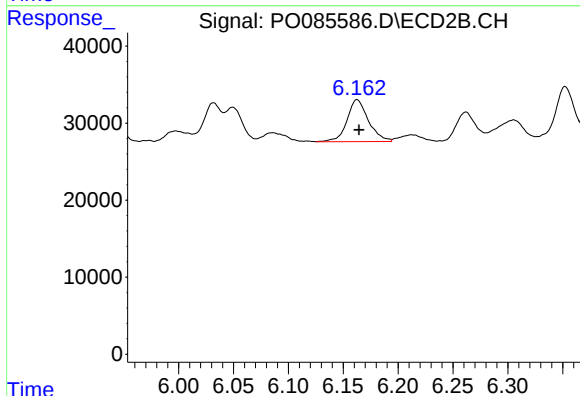


#31 AR-1260-1

R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 74021
Conc: 31.22 ng/ml

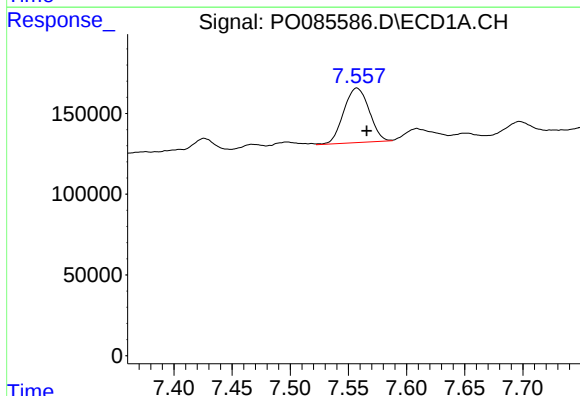


#32 AR-1260-2

R.T.: 7.557 min
Delta R.T.: -0.009 min
Response: 514054
Conc: 65.71 ng/ml

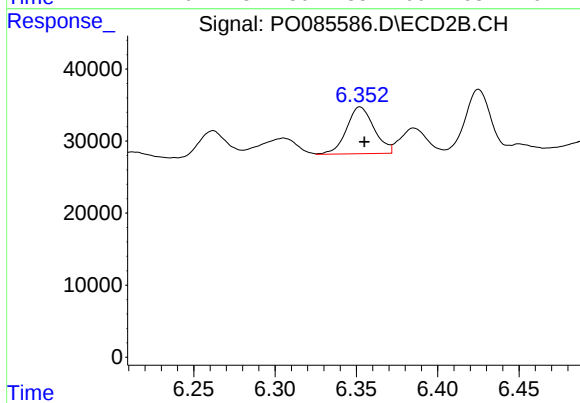

#32 AR-1260-2

R.T.: 6.352 min
Delta R.T.: -0.003 min
Response: 76550
Conc: 27.42 ng/ml m

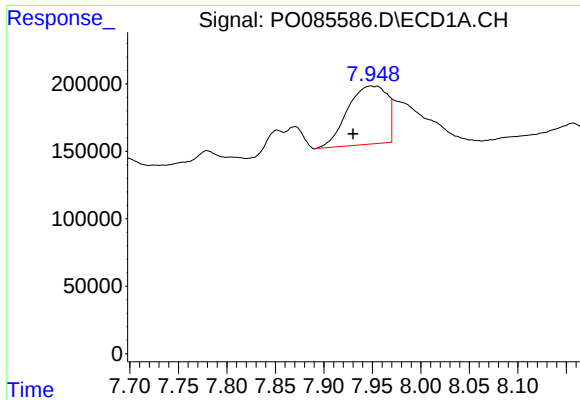


#33 AR-1260-3

R.T.: 7.948 min
Delta R.T.: 0.018 min
Response: 1225022
Conc: 208.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1286


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

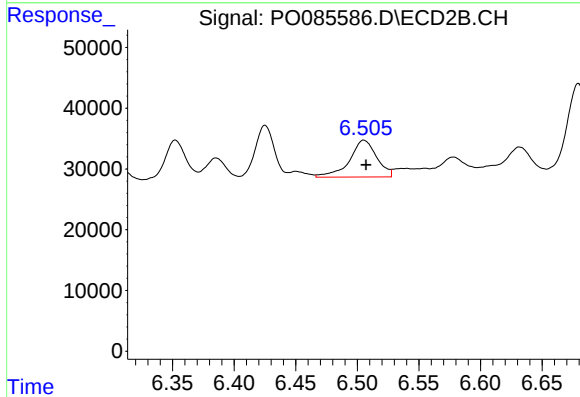


#33 AR-1260-3

R.T.: 6.505 min
Delta R.T.: -0.003 min
Response: 93014
Conc: 35.38 ng/ml m

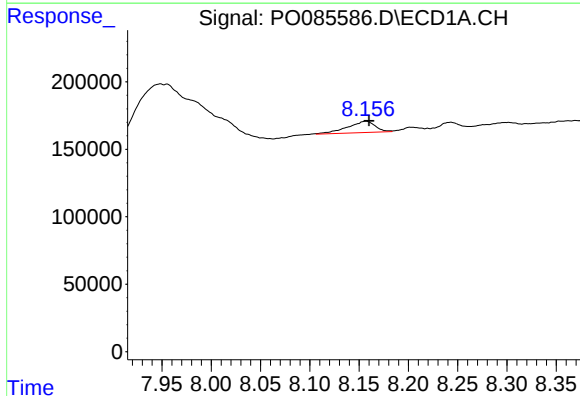


#34 AR-1260-4

R.T.: 8.156 min
Delta R.T.: -0.004 min
Response: 165019
Conc: 23.89 ng/ml m

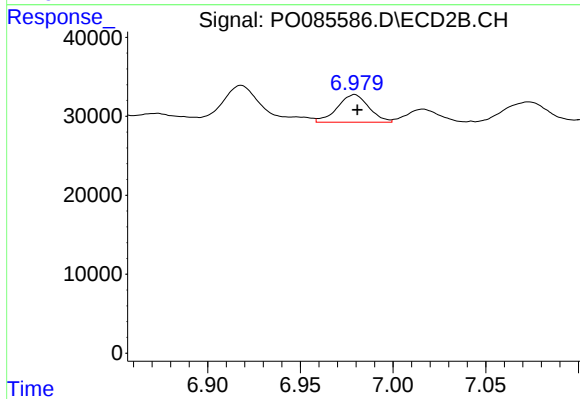

#34 AR-1260-4

R.T.: 6.979 min
Delta R.T.: -0.002 min
Response: 41416
Conc: 18.49 ng/ml m

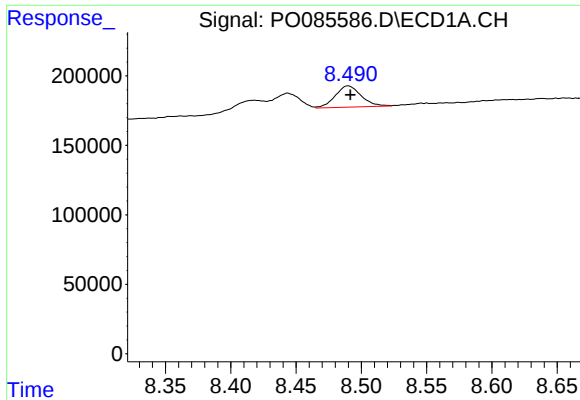


#35 AR-1260-5

R.T.: 8.490 min
Delta R.T.: -0.002 min
Response: 212213
Conc: 15.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1286

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

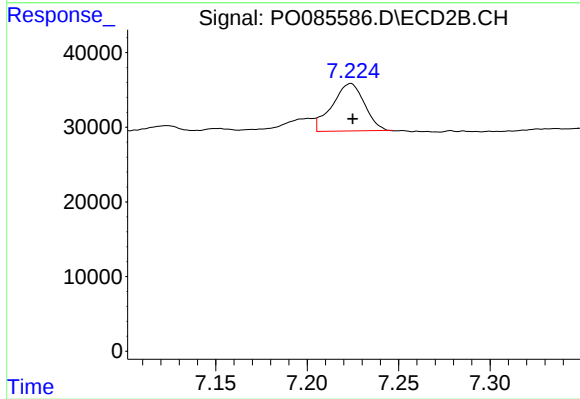

#35 AR-1260-5

R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 77857
Conc: 15.45 ng/ml m