

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032323\
 Data File : P0093468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 10:34
 Operator : YP/AJ
 Sample : 02026-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40208

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2023
 Supervised By :Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 11:14:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.632	41323452	17013757	13.196m	15.085
2) SA Decachlor...	10.254	8.658	43789773	18119456	20.233	18.506
Target Compounds						
26) L6 AR-1254-1	6.465	5.516	2236532	1407313	19.139	22.422
27) L6 AR-1254-2	6.686	5.667	16064735	4036447	94.019	71.629m
28) L6 AR-1254-3	7.055	6.072	20191012	10360831	121.459	120.343
29) L6 AR-1254-4	7.343	6.301	40957594	16093006	384.223	351.907
30) L6 AR-1254-5	7.765	6.721	58641302	28709984	433.069m	388.750

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032323\
Data File : PO093468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 10:34
Operator : YP/AJ
Sample : 02026-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40208


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 11:14:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

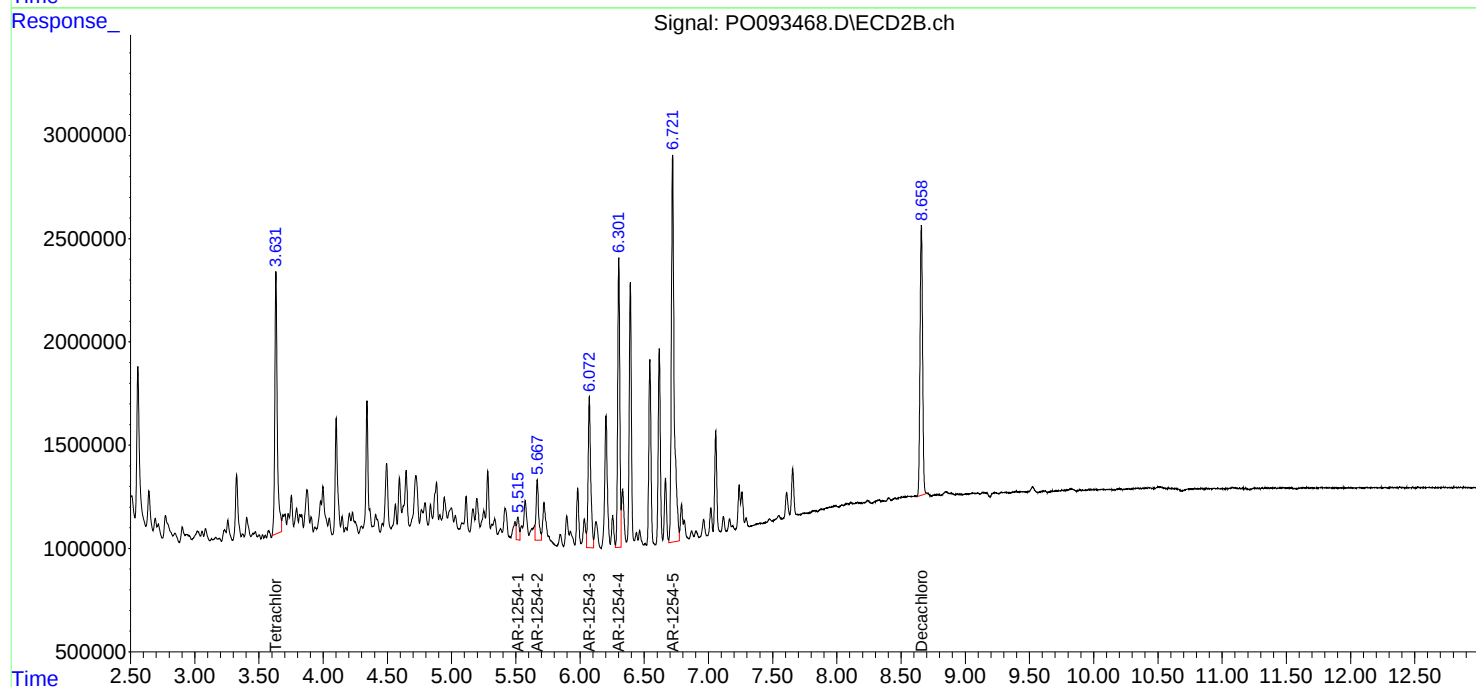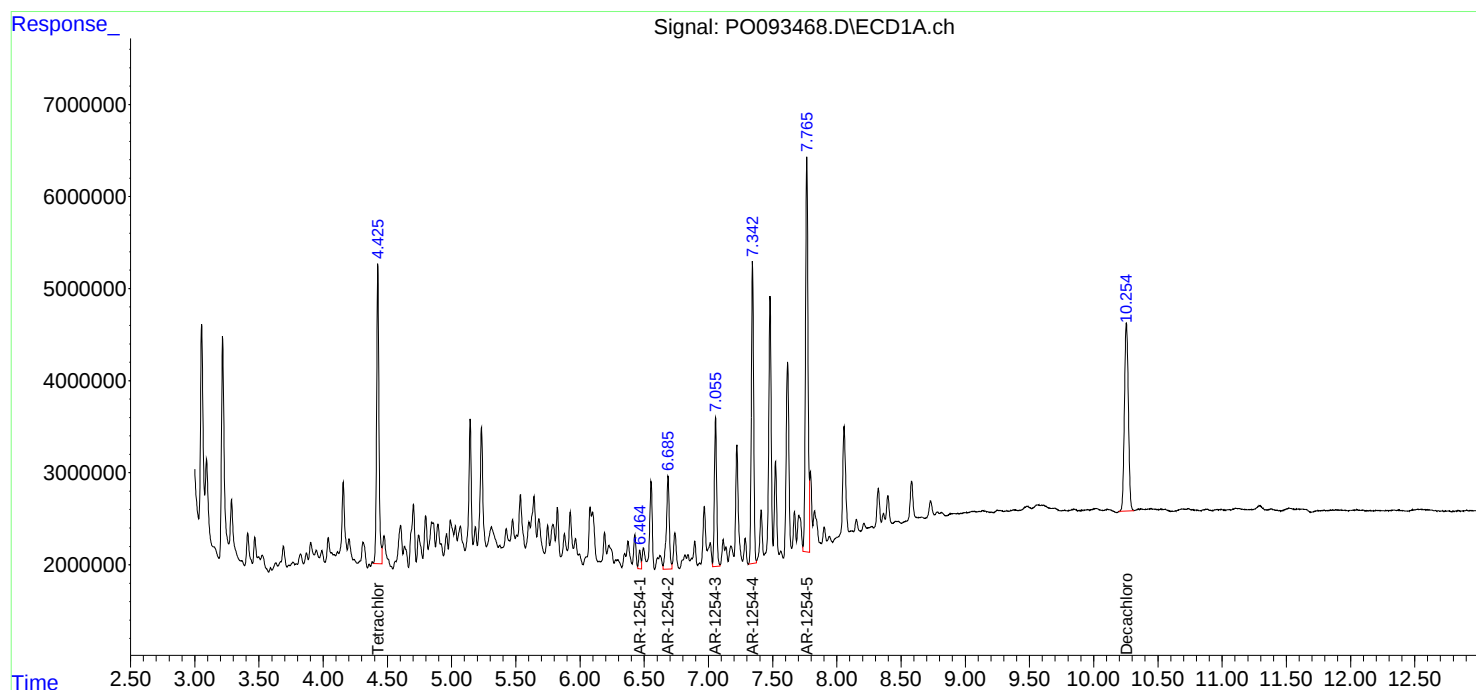

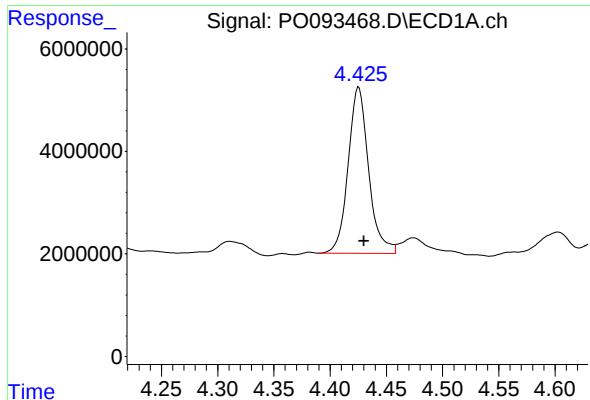


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 41323452
Conc: 13.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
40208


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

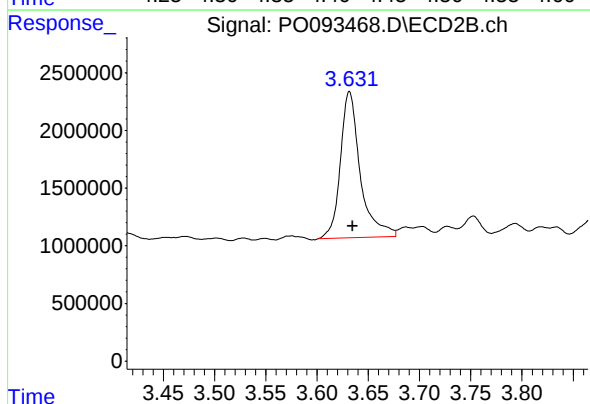


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.003 min
Response: 17013757
Conc: 15.08 ng/ml

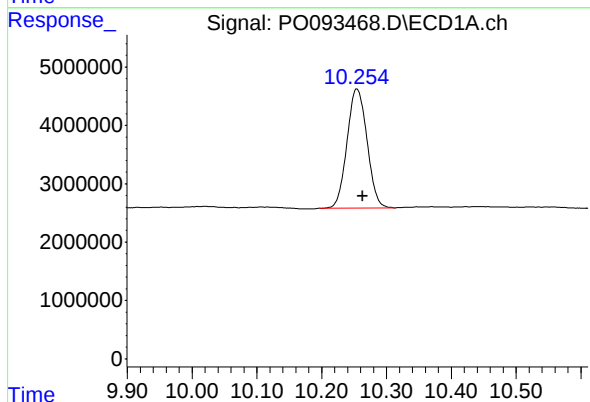


#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: -0.009 min
Response: 43789773
Conc: 20.23 ng/ml

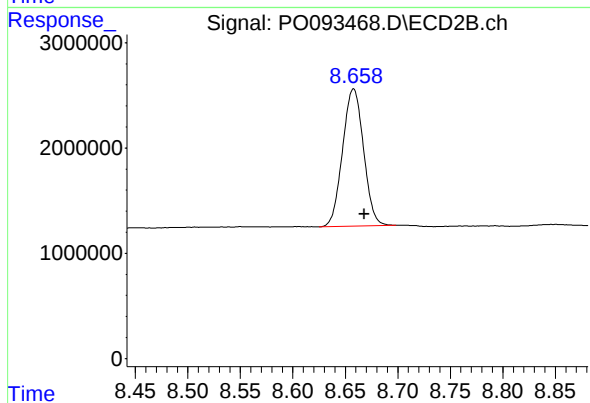

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.010 min
Response: 18119456
Conc: 18.51 ng/ml

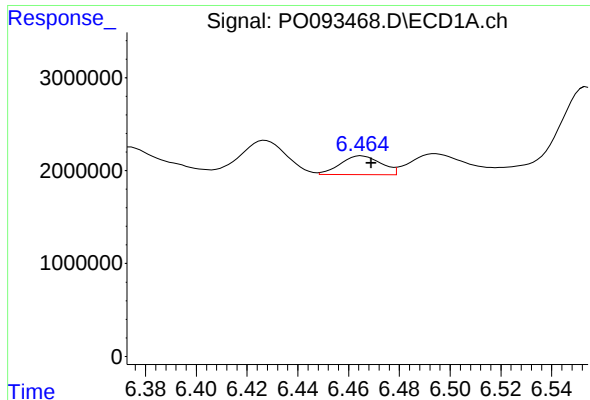


#26 AR-1254-1

R.T.: 6.465 min
Delta R.T.: -0.004 min
Response: 2236532
Conc: 19.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
40208


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

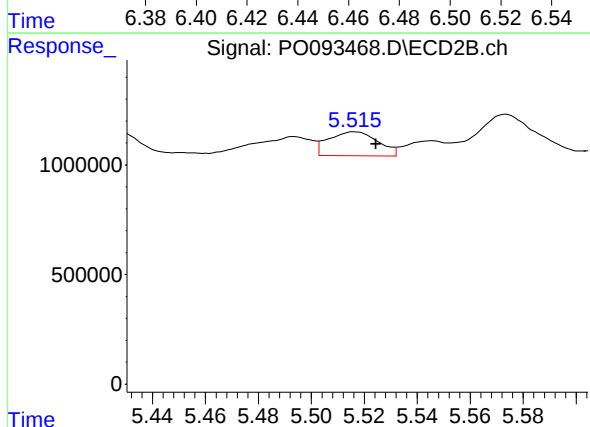


#26 AR-1254-1

R.T.: 5.516 min
Delta R.T.: -0.008 min
Response: 1407313
Conc: 22.42 ng/ml

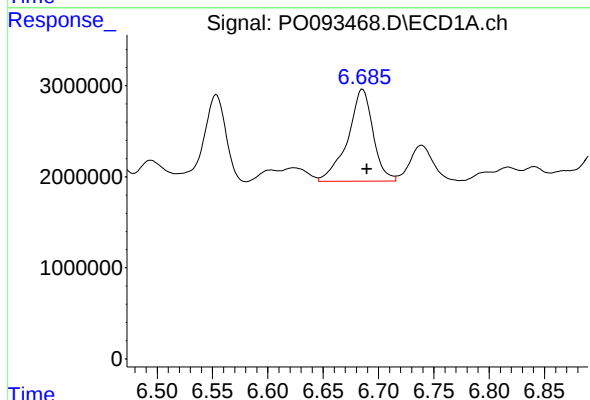


#27 AR-1254-2

R.T.: 6.686 min
Delta R.T.: -0.004 min
Response: 16064735
Conc: 94.02 ng/ml

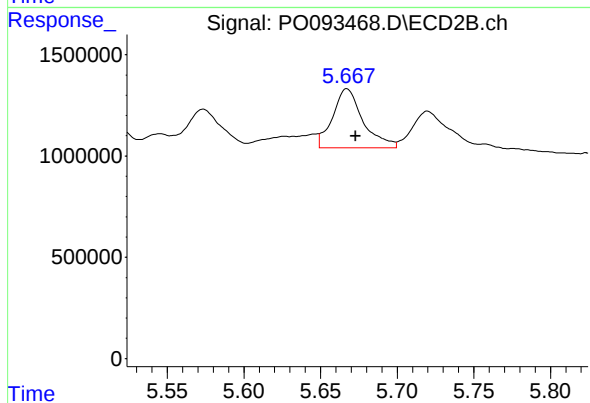

#27 AR-1254-2

R.T.: 5.667 min
Delta R.T.: -0.006 min
Response: 4036447
Conc: 71.63 ng/ml m

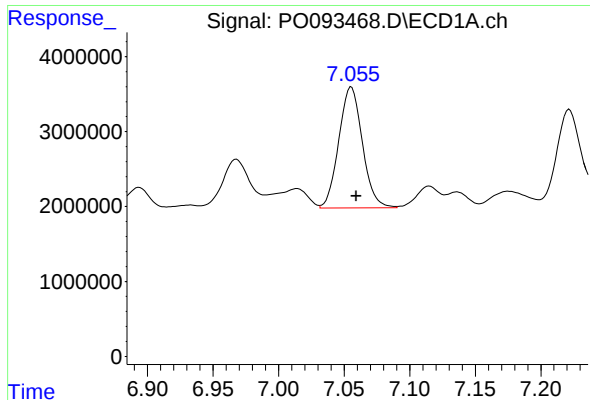


#28 AR-1254-3

R.T.: 7.055 min
Delta R.T.: -0.004 min
Response: 20191012
Conc: 121.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
40208


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

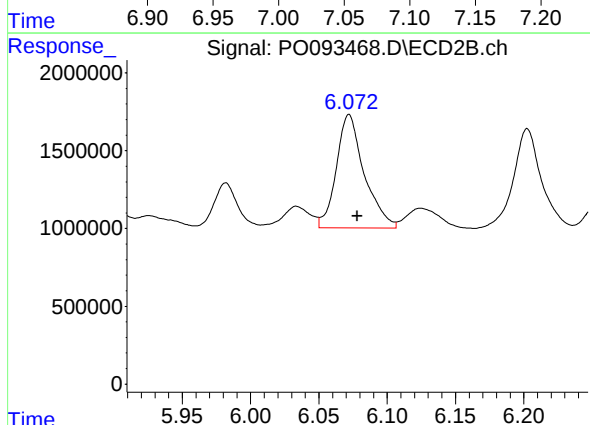


#28 AR-1254-3

R.T.: 6.072 min
Delta R.T.: -0.006 min
Response: 10360831
Conc: 120.34 ng/ml

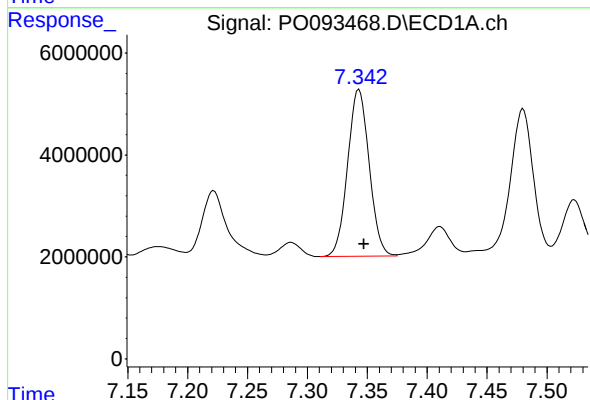


#29 AR-1254-4

R.T.: 7.343 min
Delta R.T.: -0.004 min
Response: 40957594
Conc: 384.22 ng/ml

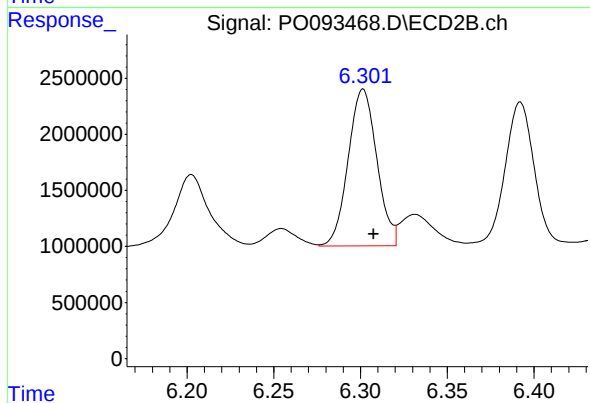

#29 AR-1254-4

R.T.: 6.301 min
Delta R.T.: -0.006 min
Response: 16093006
Conc: 351.91 ng/ml

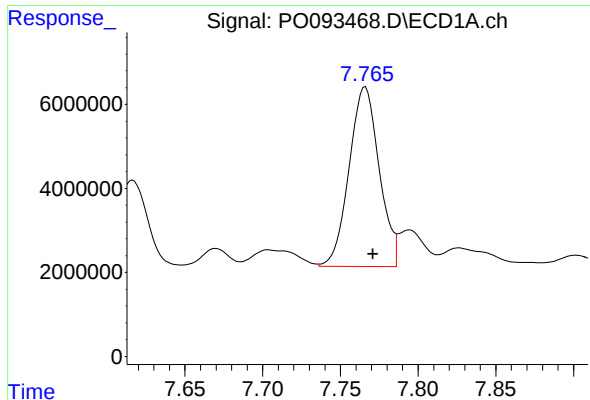


#30 AR-1254-5

R.T.: 7.765 min
Delta R.T.: -0.005 min
Response: 58641302
Conc: 433.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
40208

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

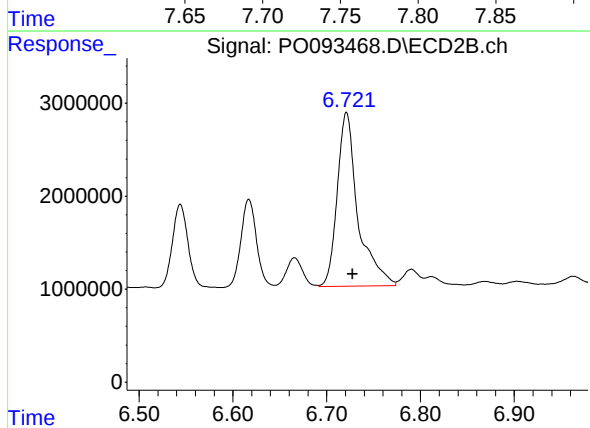

#30 AR-1254-5

R.T.: 6.721 min
Delta R.T.: -0.007 min
Response: 28709984
Conc: 388.75 ng/ml