

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076513.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 8:36
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 14:19:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.914	3.928	1553845	930179	17.742	16.957
2)	SA Decachlor...	10.887	9.185	1203826	855081	18.493	18.146
Target Compounds							
3)	L1 AR-1016-1	6.236	5.177	124240	55093	45.972	33.450 #
4)	L1 AR-1016-2	6.261	5.197	173662	113351	42.244	39.060
5)	L1 AR-1016-3	6.325	5.386	112291	44412	46.539	33.263 #
6)	L1 AR-1016-4	6.433	5.437	78923	41049	40.720	36.569
7)	L1 AR-1016-5	6.746	5.663	80435	54121	41.297	39.304
8)	L2 AR-1221-1	5.165	0.000	11425	0	12.985	N.D. #
9)	L2 AR-1221-2	5.266	0.000	35345	0	52.193	N.D. #
10)	L2 AR-1221-3	5.352	4.373	73708	33256	34.063	24.784 #
11)	L3 AR-1232-1	5.352	4.373	73708	33256	41.668	30.442 #
12)	L3 AR-1232-2	5.940	5.197	111261	113351	125.443	94.835
13)	L3 AR-1232-3	6.261	5.386	173662	44412	102.841	81.338
14)	L3 AR-1232-4	6.433	5.480	78923	42735	100.799	83.239
15)	L3 AR-1232-5	6.529	5.663	70573	54121	128.020	99.212
16)	L4 AR-1242-1	6.236	5.177	124240	55093	55.574	42.775
17)	L4 AR-1242-2	6.261	5.197	173662	113351	51.113	48.368
18)	L4 AR-1242-3	6.325	5.386	112291	44412	55.565	41.016 #
19)	L4 AR-1242-4	6.433	5.480	78923	42735	49.003	38.572
20)	L4 AR-1242-5	7.216	6.040	14113	39409	8.080	29.710 #
21)	L5 AR-1248-1	6.236	5.177	124240	55093	75.056	54.970 #
22)	L5 AR-1248-2	6.529	5.437	70573	41049	28.911	25.211
23)	L5 AR-1248-3	6.746	5.480	80435	42735	28.076	25.890
24)	L5 AR-1248-4	7.175	5.663	18902	54121	6.053	27.838 #
25)	L5 AR-1248-5	7.216	0.000	14113	0	4.532	N.D. #
26)	L6 AR-1254-1	7.144	6.040	62606	39409	18.849	13.305 #
27)	L6 AR-1254-2	7.372	6.199	71550	37202	13.902	14.318
28)	L6 AR-1254-3	7.755	6.634	46564	78532	8.754	19.607 #
29)	L6 AR-1254-4	8.048	6.889f	23675	20831	6.564	8.792 #
30)	L6 AR-1254-5	8.477	7.282	176252	146683	44.964	41.617
31)	L7 AR-1260-1	7.921	6.752	157621	115241	45.868	44.966
32)	L7 AR-1260-2	8.186	6.950	182298	137555	44.961	44.354
33)	L7 AR-1260-3	8.551	7.103	129608	138039	42.900	46.988
34)	L7 AR-1260-4	8.781	7.584	146006	101876	41.898	42.745
35)	L7 AR-1260-5	9.104	7.831	284604	234778	42.115	41.383
36)	L8 AR-1262-1	8.551	7.282	129608	146683	25.050	74.591 #
37)	L8 AR-1262-2	9.104	7.831	284604	234778	33.025	34.922
38)	L8 AR-1262-3	9.431f	8.116	171764	54712	30.297	20.313 #
39)	L8 AR-1262-4	9.485	8.179	114120	178406	26.509	35.850 #
40)	L8 AR-1262-5	10.158	8.676	88918	63786	30.603	29.358
41)	L9 AR-1268-1	9.431f	8.116	171764	54712	16.555	7.018 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076513.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 8:36
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 14:19:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.485f	8.179	114120	178406	12.264	25.152 #
44) L9	AR-1268-4	10.158	8.676	88918	63786	27.363	26.414
45) L9	AR-1268-5	10.562	8.948	42188	19309	1.594	1.067 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032421\
Data File : PO076513.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 8:36
Operator : DD\AJ
Sample : M1458-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 14:19:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

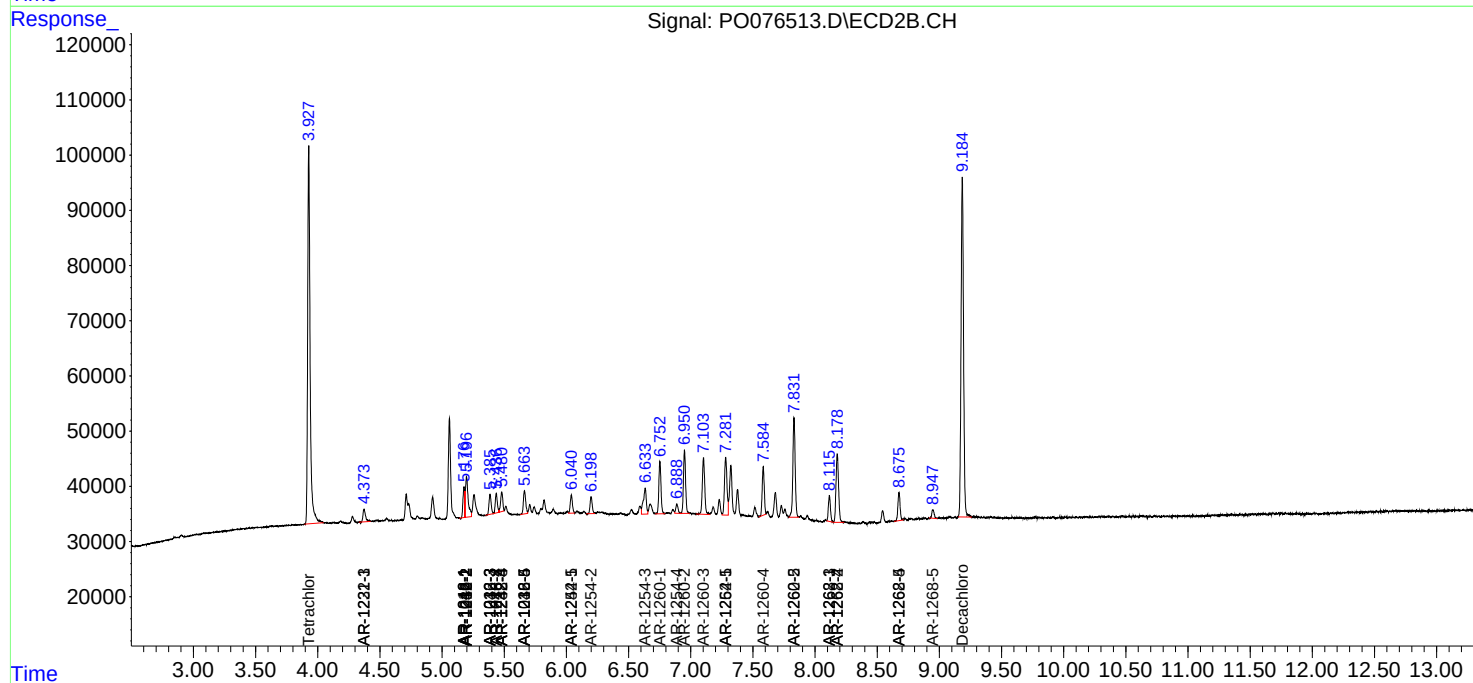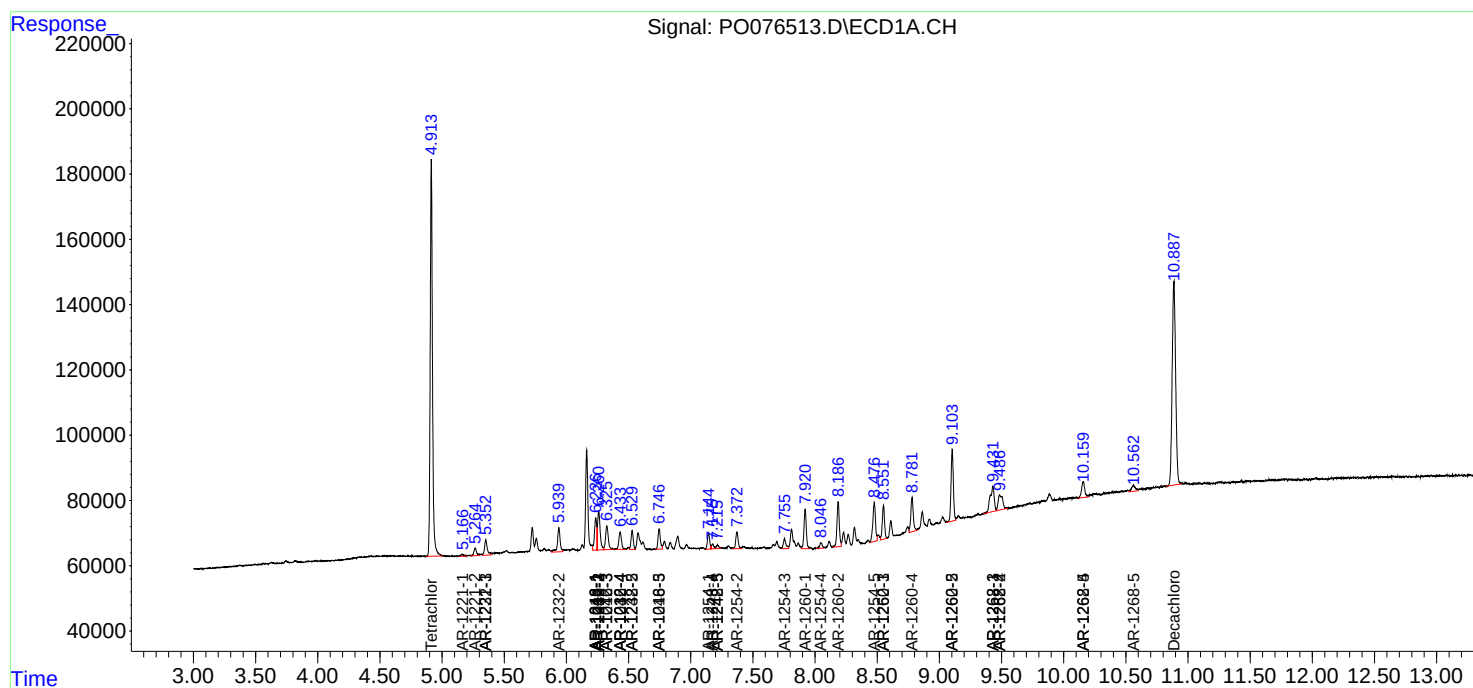


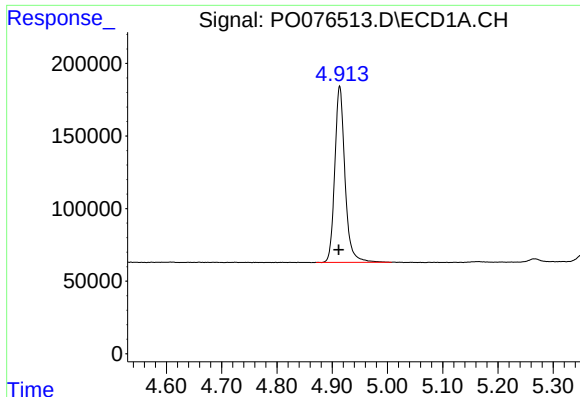

#1 Tetrachloro-m-xylene


R.T.: 4.914 min
Delta R.T.: 0.002 min
Response: 1553845
Conc: 17.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

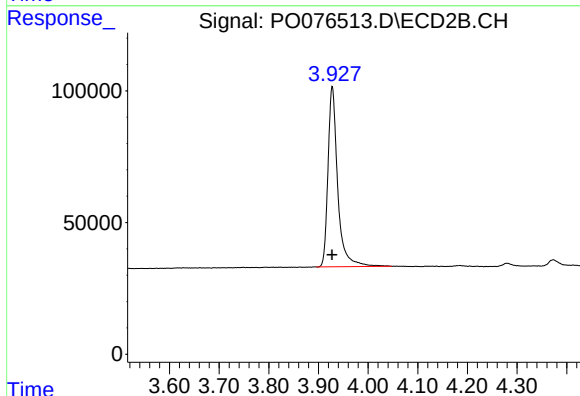


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 930179
Conc: 16.96 ng/ml

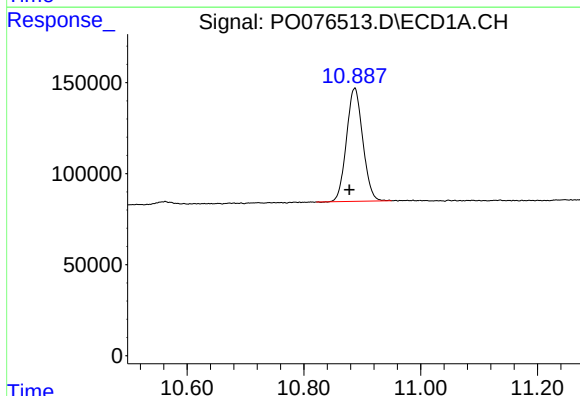


#2 Decachlorobiphenyl

R.T.: 10.887 min
Delta R.T.: 0.009 min
Response: 1203826
Conc: 18.49 ng/ml

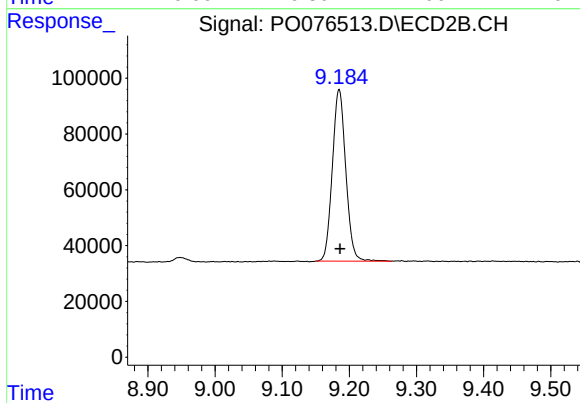

#2 Decachlorobiphenyl


R.T.: 9.185 min
Delta R.T.: -0.001 min
Response: 855081
Conc: 18.15 ng/ml

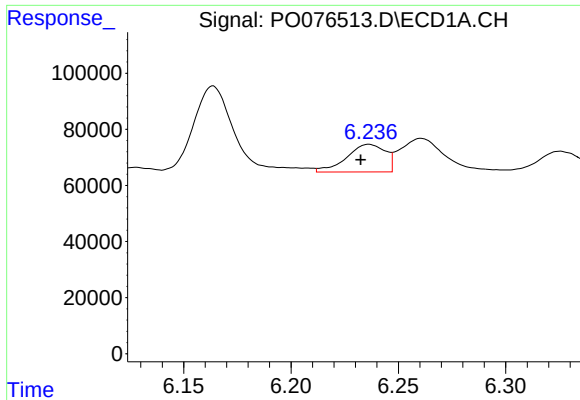

#3 AR-1016-1


R.T.: 6.236 min
Delta R.T.: 0.004 min
Response: 124240
Conc: 45.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

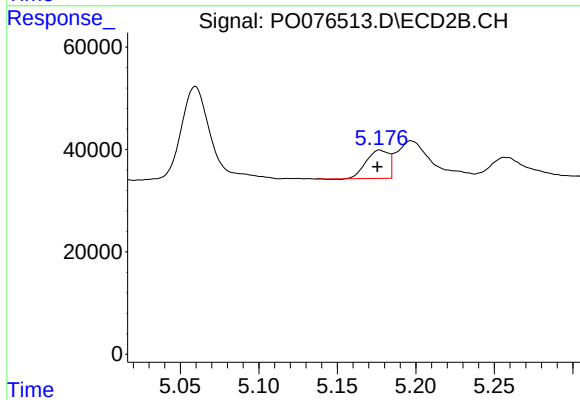


#3 AR-1016-1

R.T.: 5.177 min
Delta R.T.: 0.002 min
Response: 55093
Conc: 33.45 ng/ml

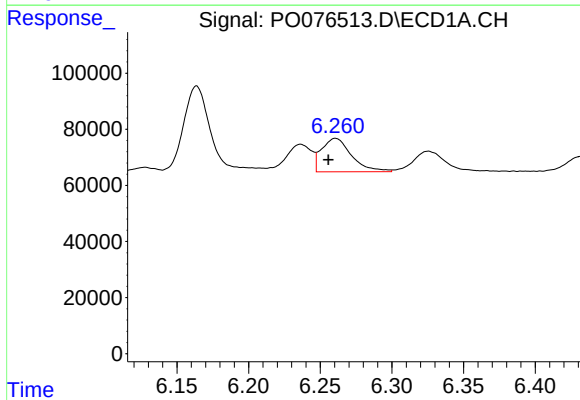


#4 AR-1016-2

R.T.: 6.261 min
Delta R.T.: 0.005 min
Response: 173662
Conc: 42.24 ng/ml

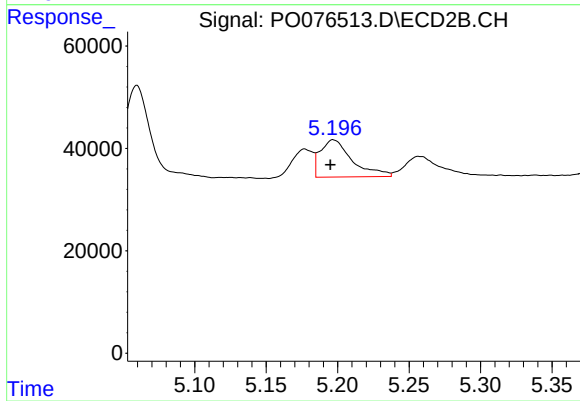

#4 AR-1016-2


R.T.: 5.197 min
Delta R.T.: 0.002 min
Response: 113351
Conc: 39.06 ng/ml

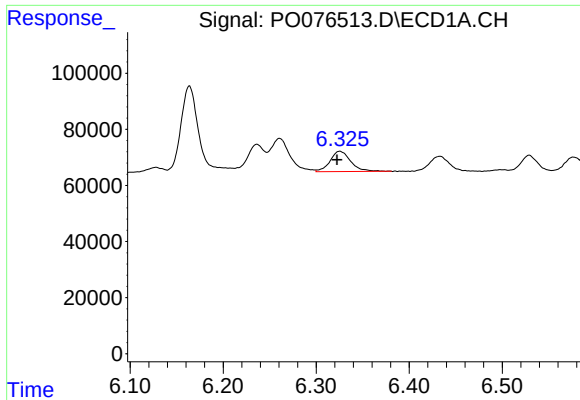

#5 AR-1016-3


R.T.: 6.325 min
Delta R.T.: 0.003 min
Response: 112291
Conc: 46.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

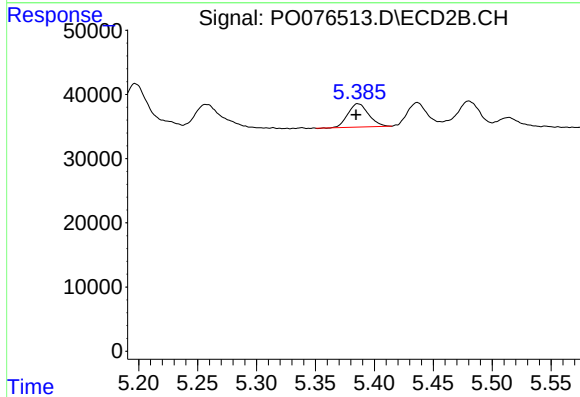


#5 AR-1016-3

R.T.: 5.386 min
Delta R.T.: 0.002 min
Response: 44412
Conc: 33.26 ng/ml

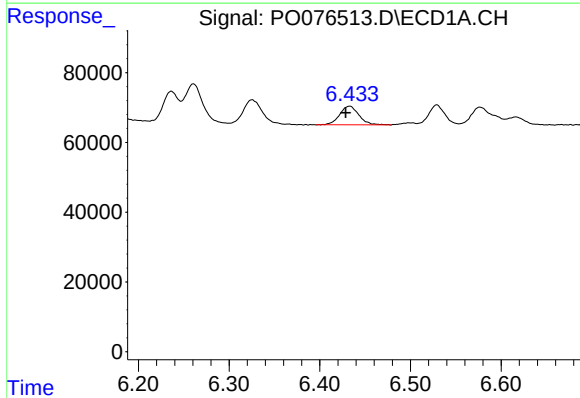


#6 AR-1016-4

R.T.: 6.433 min
Delta R.T.: 0.004 min
Response: 78923
Conc: 40.72 ng/ml

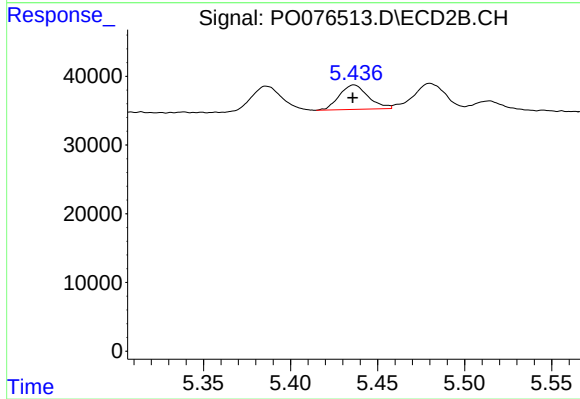

#6 AR-1016-4


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 41049
Conc: 36.57 ng/ml

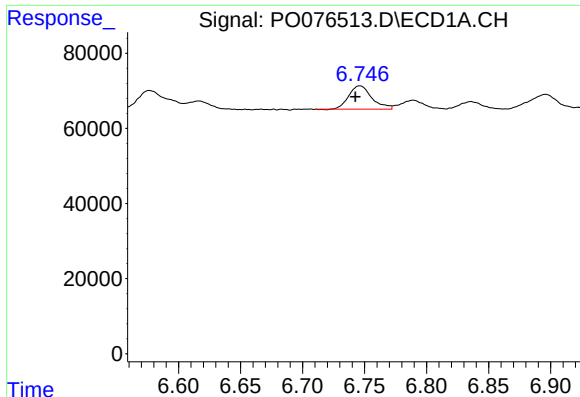

#7 AR-1016-5


R.T.: 6.746 min
Delta R.T.: 0.004 min
Response: 80435
Conc: 41.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

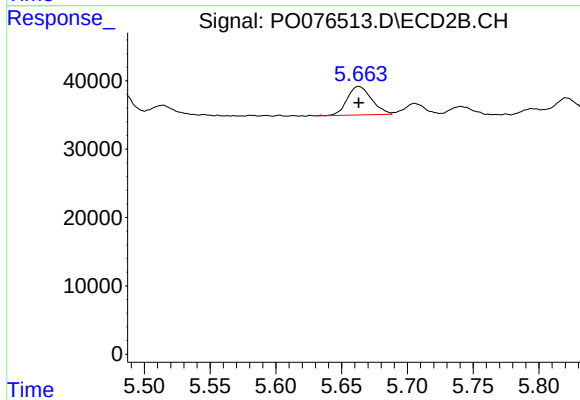


#7 AR-1016-5

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 54121
Conc: 39.30 ng/ml

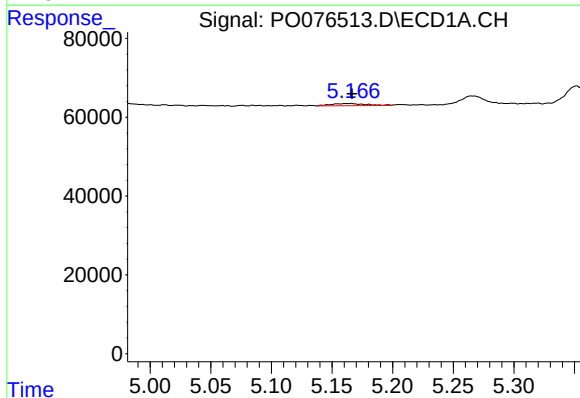


#8 AR-1221-1

R.T.: 5.165 min
Delta R.T.: -0.001 min
Response: 11425
Conc: 12.98 ng/ml

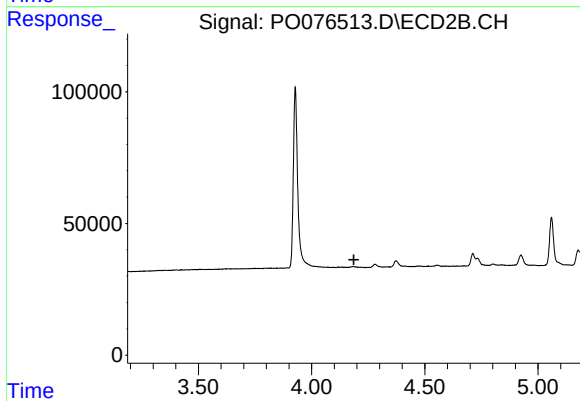

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

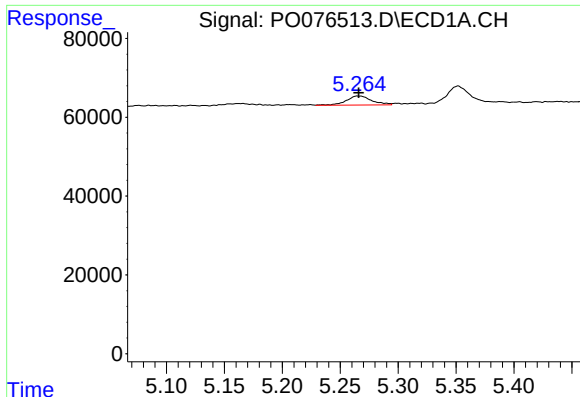

#9 AR-1221-2


R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 35345
Conc: 52.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

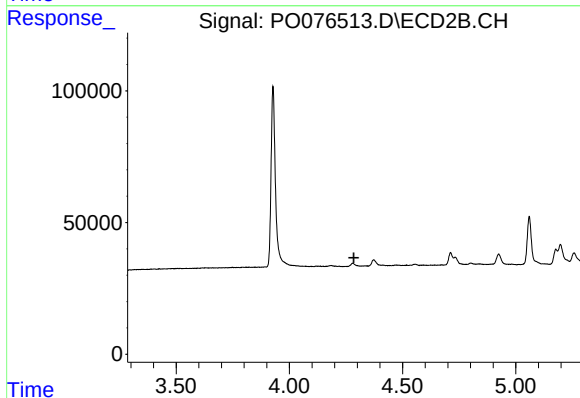


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

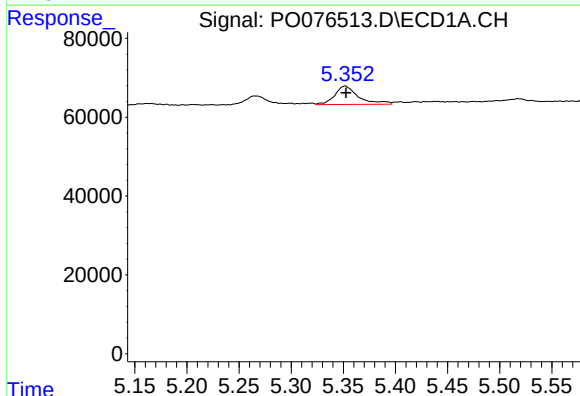


#10 AR-1221-3

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 73708
Conc: 34.06 ng/ml

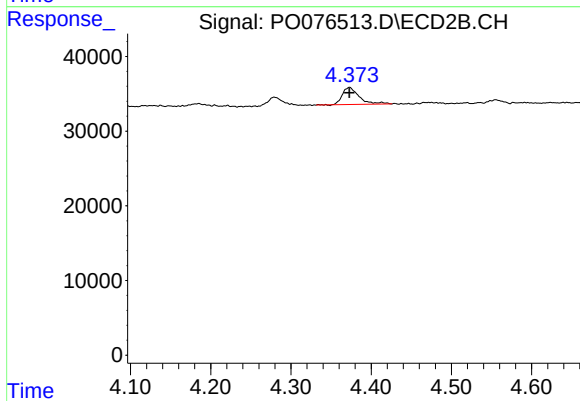

#10 AR-1221-3


R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 33256
Conc: 24.78 ng/ml

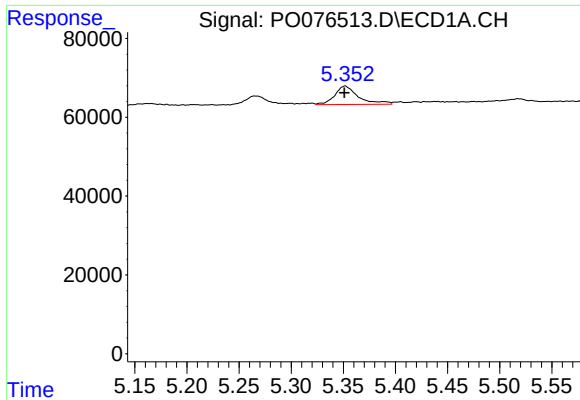

#11 AR-1232-1


R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 73708
Conc: 41.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

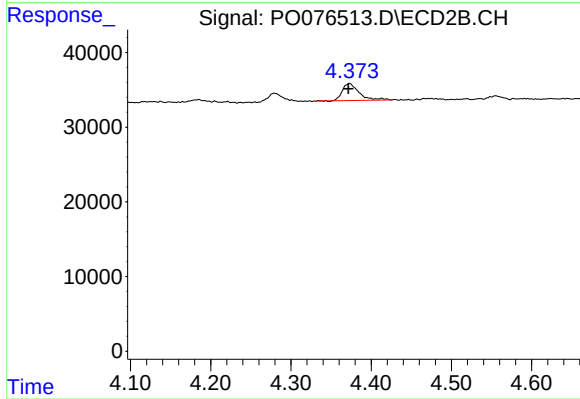


#11 AR-1232-1

R.T.: 4.373 min
Delta R.T.: 0.001 min
Response: 33256
Conc: 30.44 ng/ml

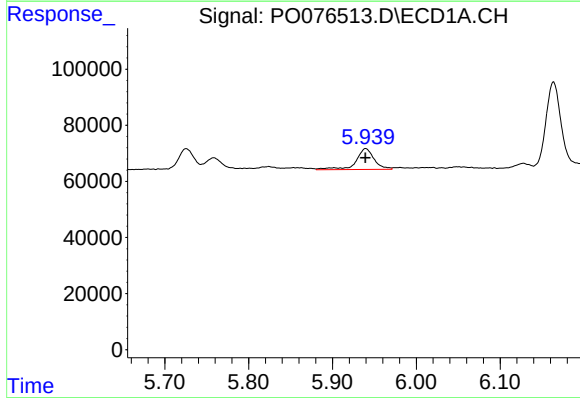


#12 AR-1232-2

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 111261
Conc: 125.44 ng/ml

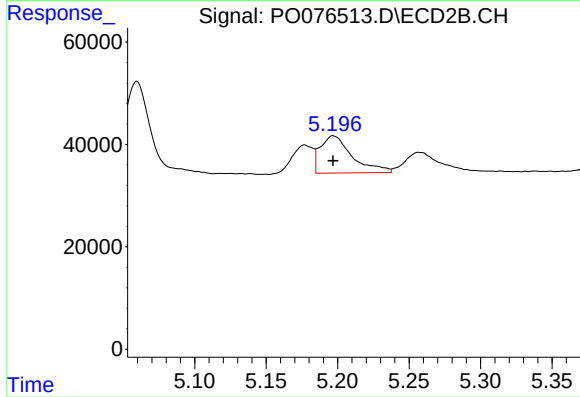

#12 AR-1232-2


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 113351
Conc: 94.83 ng/ml

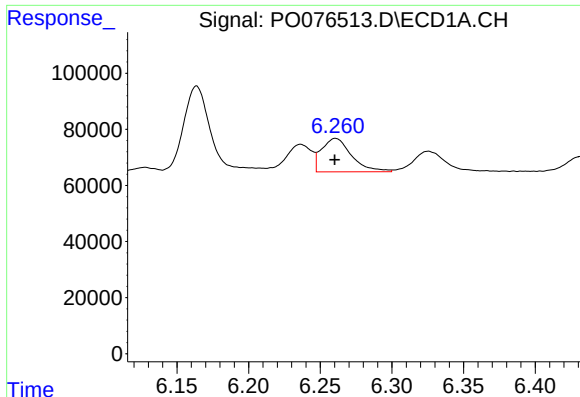

#13 AR-1232-3


R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 173662
Conc: 102.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

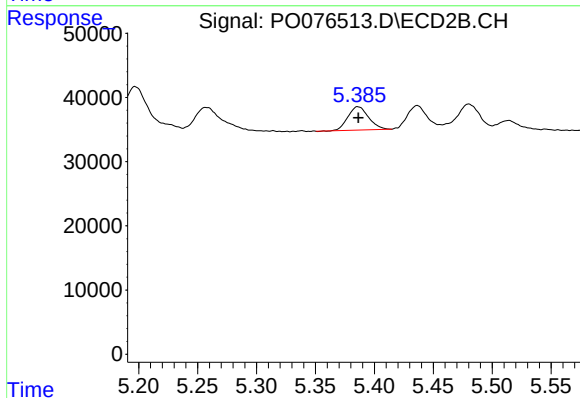


#13 AR-1232-3

R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 44412
Conc: 81.34 ng/ml

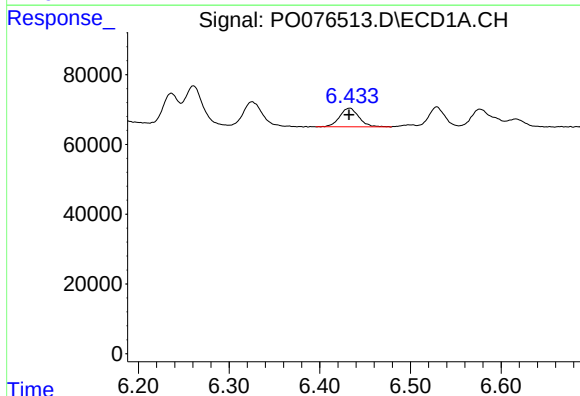


#14 AR-1232-4

R.T.: 6.433 min
Delta R.T.: 0.000 min
Response: 78923
Conc: 100.80 ng/ml

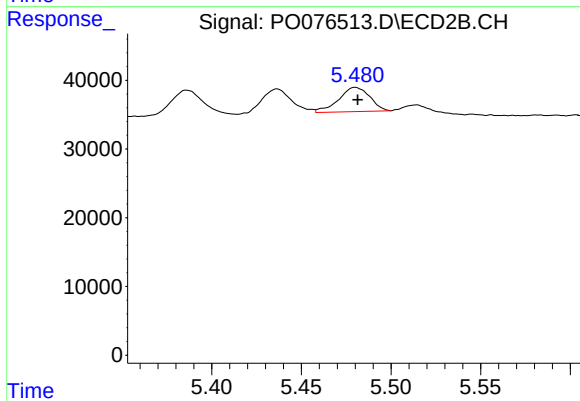

#14 AR-1232-4


R.T.: 5.480 min
Delta R.T.: -0.001 min
Response: 42735
Conc: 83.24 ng/ml

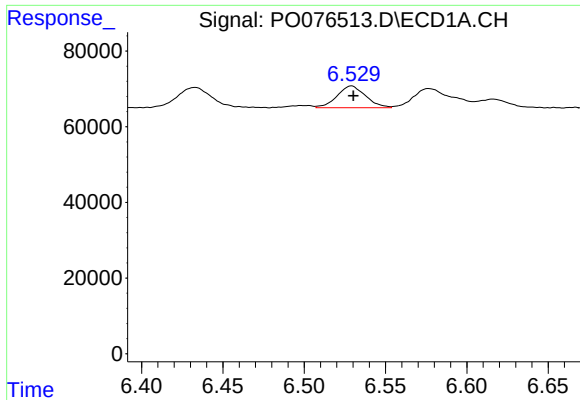

#15 AR-1232-5


R.T.: 6.529 min
Delta R.T.: -0.001 min
Response: 70573
Conc: 128.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

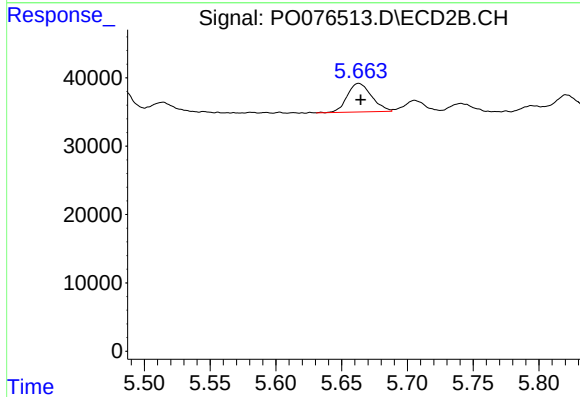


#15 AR-1232-5

R.T.: 5.663 min
Delta R.T.: -0.002 min
Response: 54121
Conc: 99.21 ng/ml

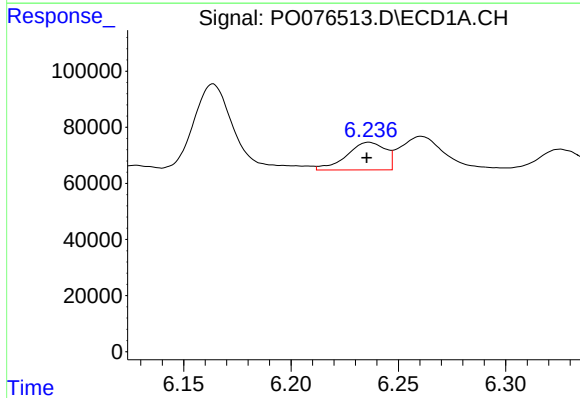


#16 AR-1242-1

R.T.: 6.236 min
Delta R.T.: 0.001 min
Response: 124240
Conc: 55.57 ng/ml

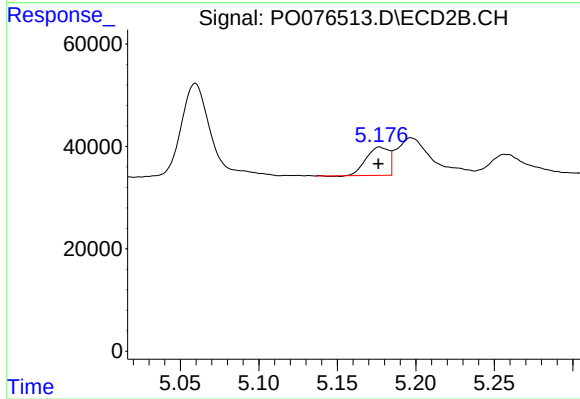

#16 AR-1242-1


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 55093
Conc: 42.78 ng/ml

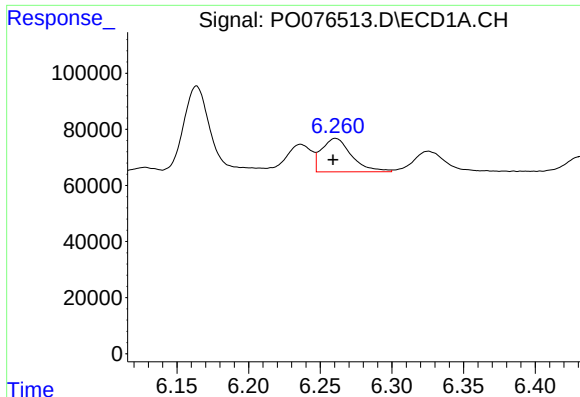

#17 AR-1242-2


R.T.: 6.261 min
Delta R.T.: 0.002 min
Response: 173662
Conc: 51.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

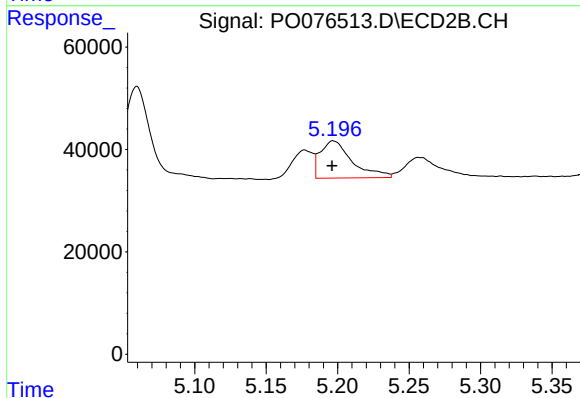


#17 AR-1242-2

R.T.: 5.197 min
Delta R.T.: 0.001 min
Response: 113351
Conc: 48.37 ng/ml

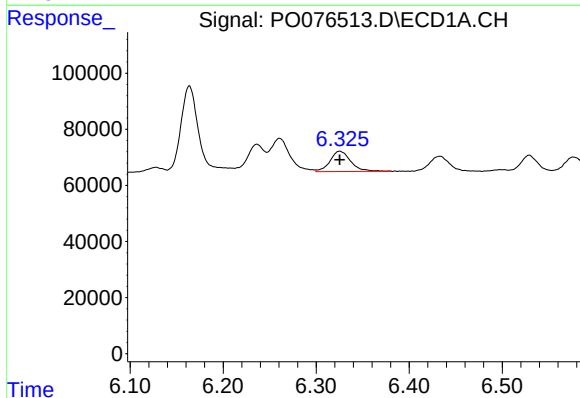


#18 AR-1242-3

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 112291
Conc: 55.56 ng/ml

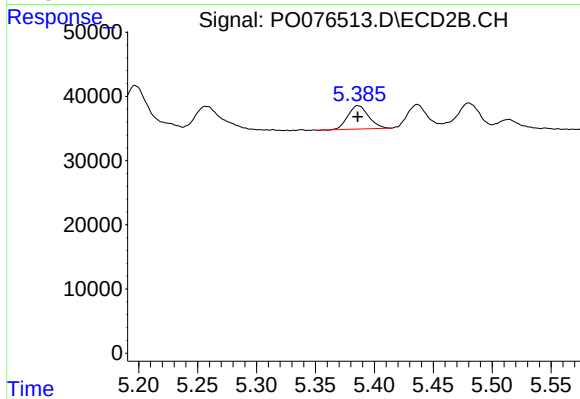

#18 AR-1242-3


R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 44412
Conc: 41.02 ng/ml

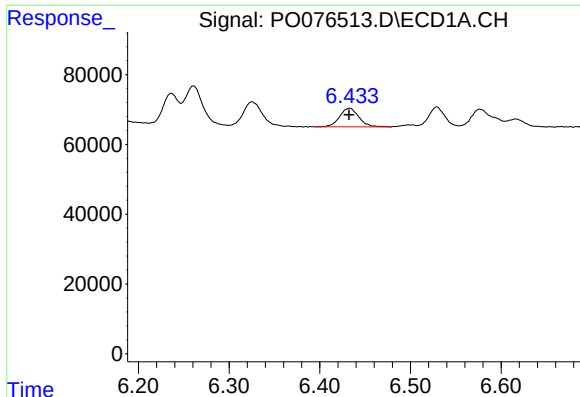

#19 AR-1242-4


R.T.: 6.433 min
Delta R.T.: 0.000 min
Response: 78923
Conc: 49.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

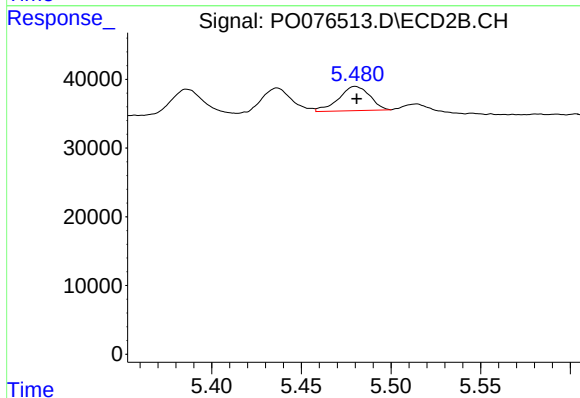


#19 AR-1242-4

R.T.: 5.480 min
Delta R.T.: 0.000 min
Response: 42735
Conc: 38.57 ng/ml

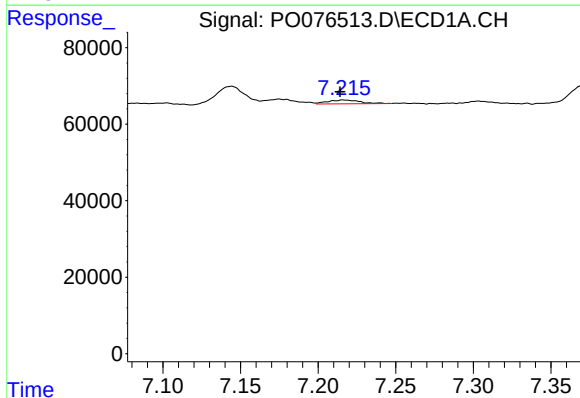


#20 AR-1242-5

R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 14113
Conc: 8.08 ng/ml

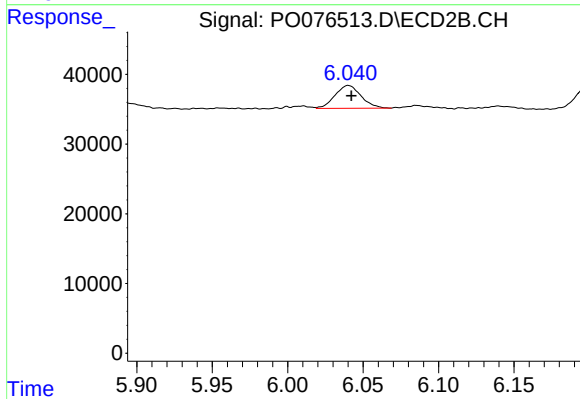

#20 AR-1242-5


R.T.: 6.040 min
Delta R.T.: -0.002 min
Response: 39409
Conc: 29.71 ng/ml

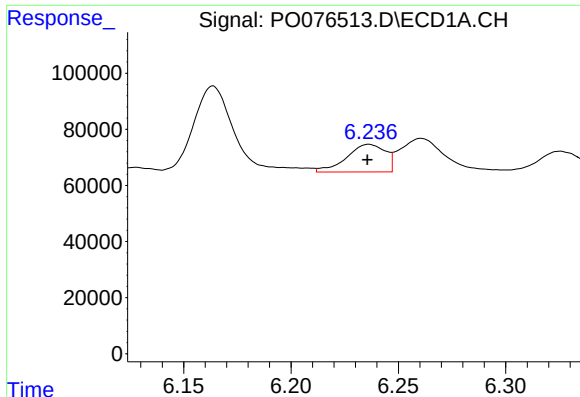

#21 AR-1248-1


R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 124240
Conc: 75.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

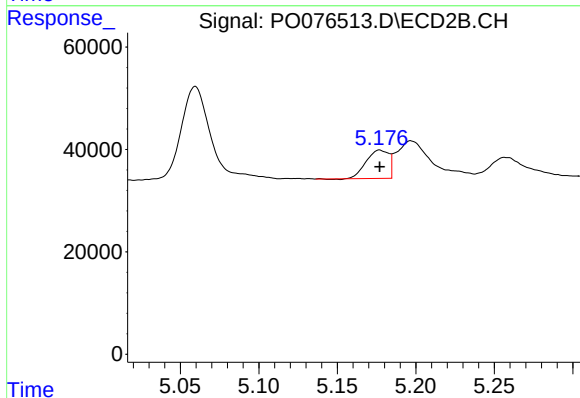


#21 AR-1248-1

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 55093
Conc: 54.97 ng/ml

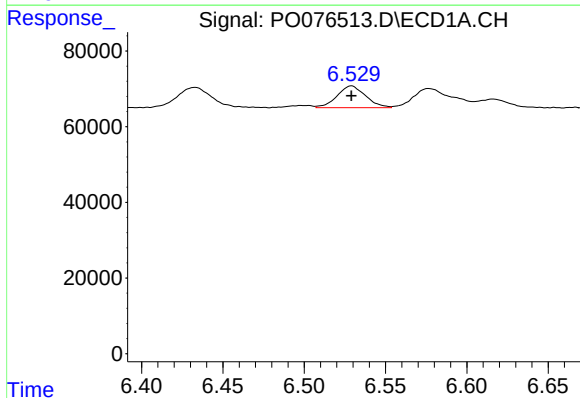


#22 AR-1248-2

R.T.: 6.529 min
Delta R.T.: 0.000 min
Response: 70573
Conc: 28.91 ng/ml

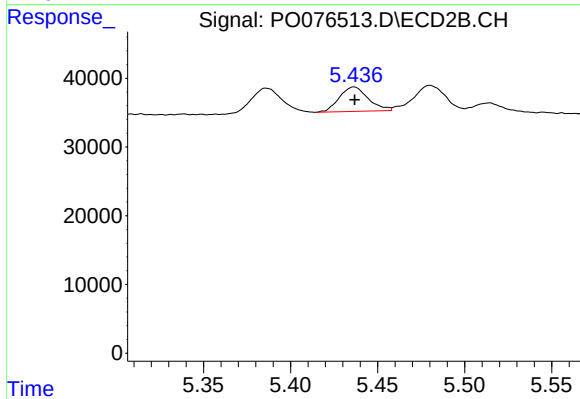

#22 AR-1248-2


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 41049
Conc: 25.21 ng/ml

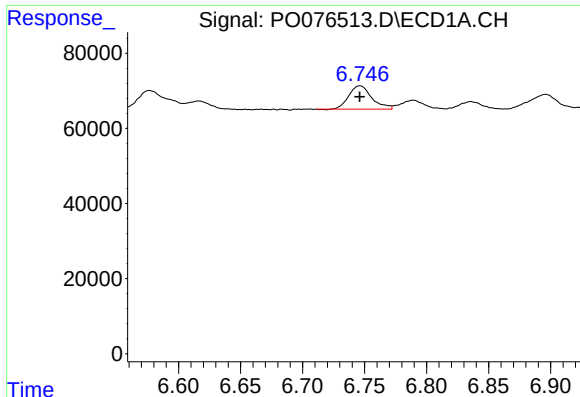

#23 AR-1248-3


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 80435
Conc: 28.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

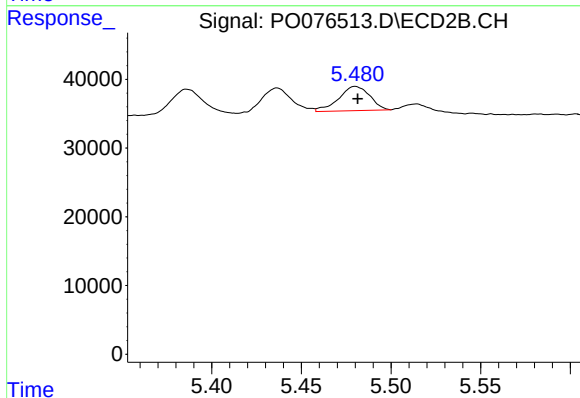


#23 AR-1248-3

R.T.: 5.480 min
Delta R.T.: -0.001 min
Response: 42735
Conc: 25.89 ng/ml

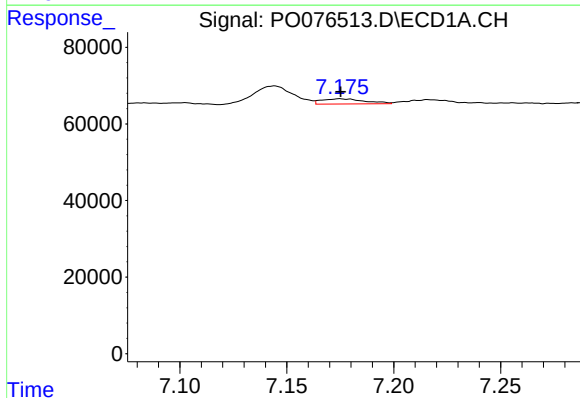


#24 AR-1248-4

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 18902
Conc: 6.05 ng/ml

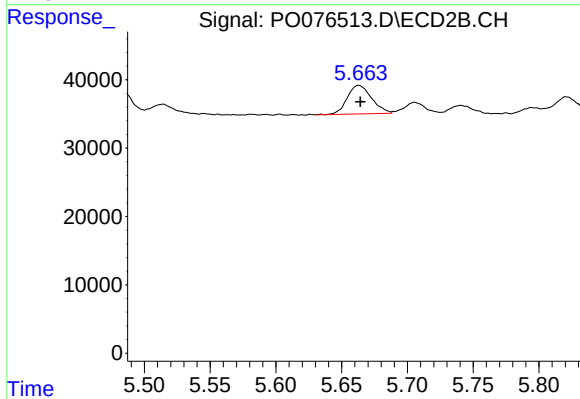

#24 AR-1248-4


R.T.: 5.663 min
Delta R.T.: -0.001 min
Response: 54121
Conc: 27.84 ng/ml

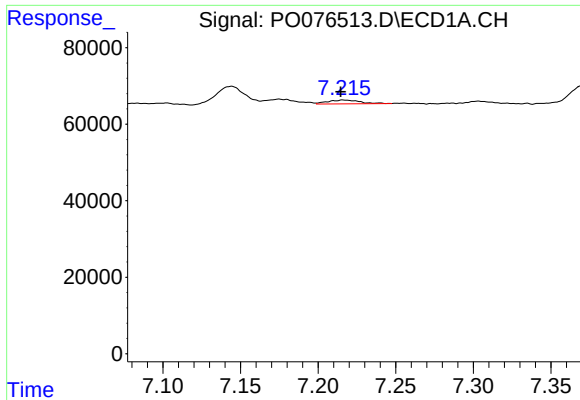

#25 AR-1248-5


R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 14113
Conc: 4.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

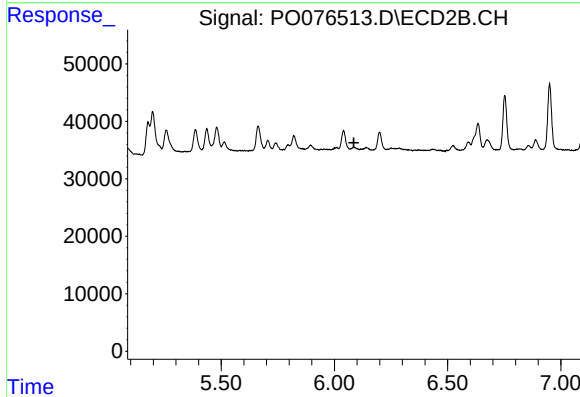


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.086 min
Response: 0
Conc: N.D.

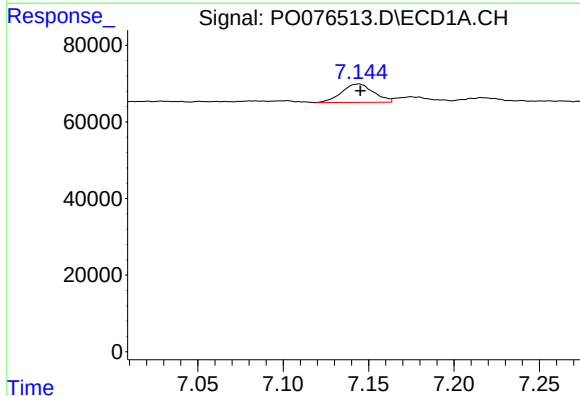


#26 AR-1254-1

R.T.: 7.144 min
Delta R.T.: -0.001 min
Response: 62606
Conc: 18.85 ng/ml

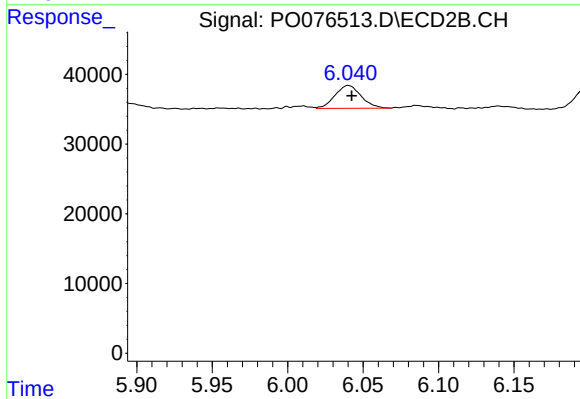

#26 AR-1254-1


R.T.: 6.040 min
Delta R.T.: -0.002 min
Response: 39409
Conc: 13.31 ng/ml

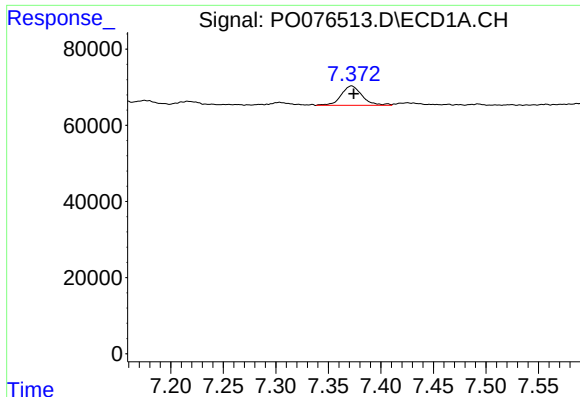

#27 AR-1254-2


R.T.: 7.372 min
Delta R.T.: -0.002 min
Response: 71550
Conc: 13.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

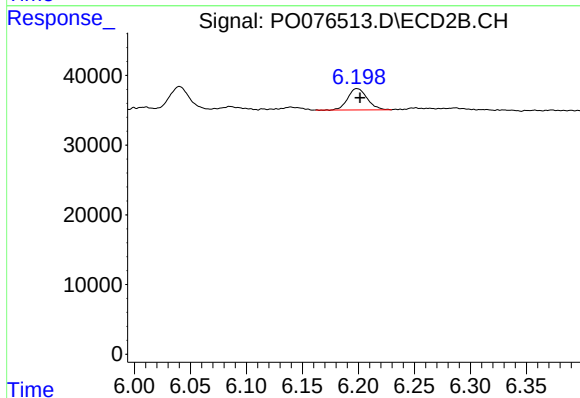


#27 AR-1254-2

R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 37202
Conc: 14.32 ng/ml

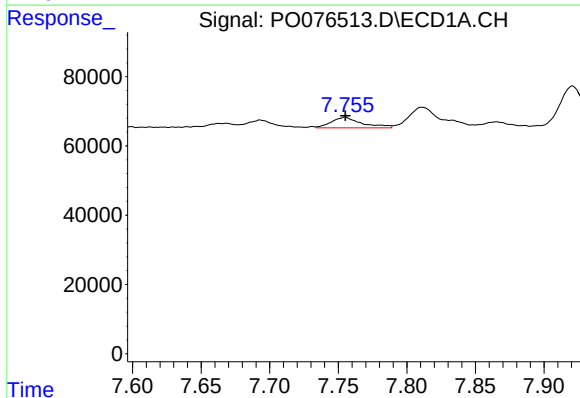


#28 AR-1254-3

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 46564
Conc: 8.75 ng/ml

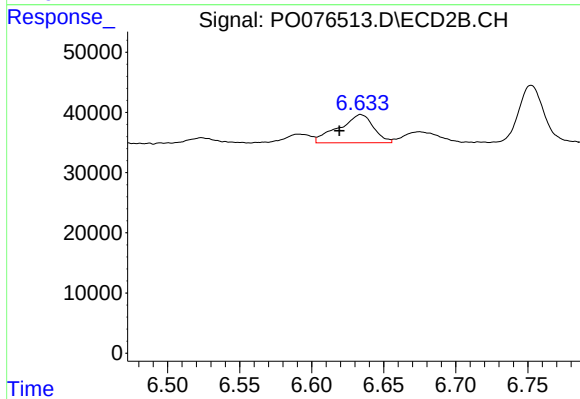

#28 AR-1254-3


R.T.: 6.634 min
Delta R.T.: 0.015 min
Response: 78532
Conc: 19.61 ng/ml

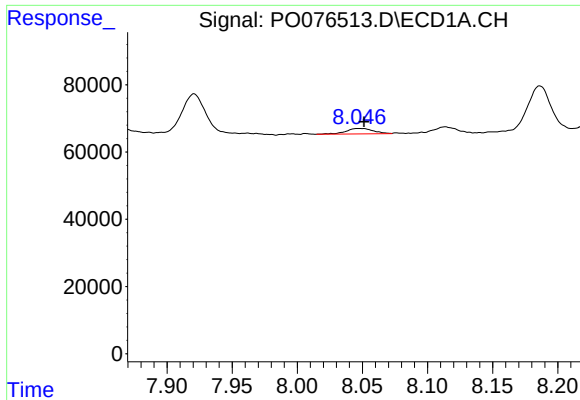

#29 AR-1254-4


R.T.: 8.048 min
Delta R.T.: -0.003 min
Response: 23675
Conc: 6.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

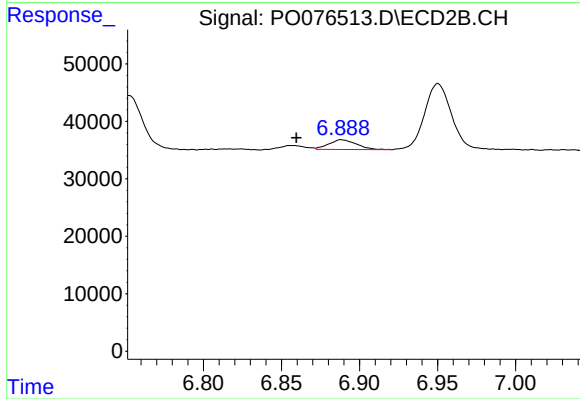


#29 AR-1254-4

R.T.: 6.889 min
Delta R.T.: 0.029 min
Response: 20831
Conc: 8.79 ng/ml

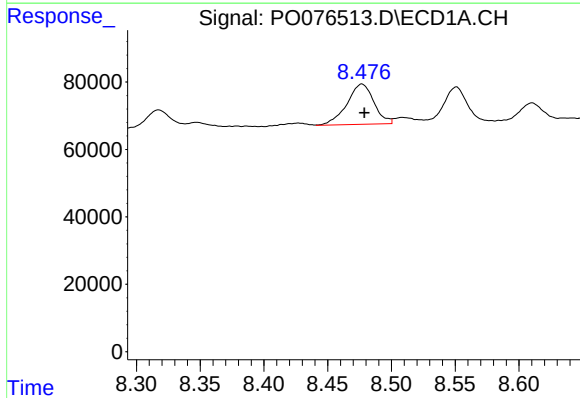


#30 AR-1254-5

R.T.: 8.477 min
Delta R.T.: -0.002 min
Response: 176252
Conc: 44.96 ng/ml

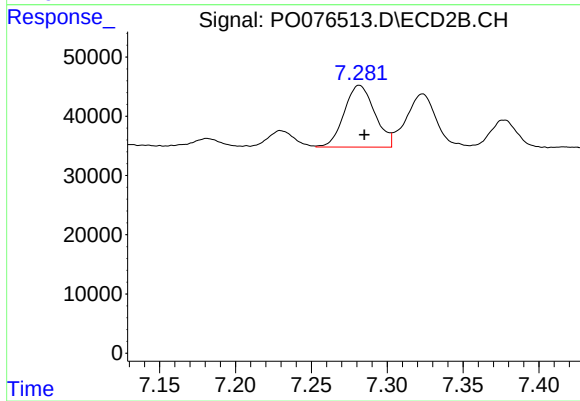

#30 AR-1254-5


R.T.: 7.282 min
Delta R.T.: -0.003 min
Response: 146683
Conc: 41.62 ng/ml

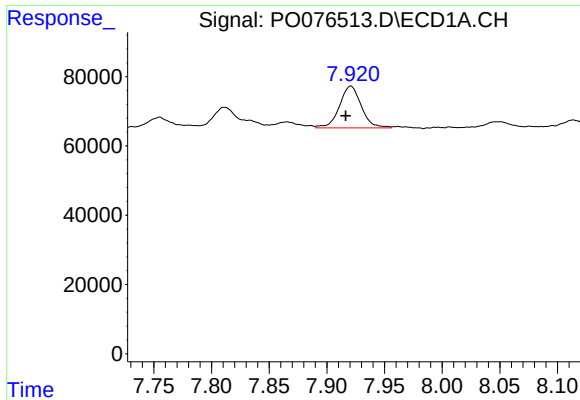

#31 AR-1260-1


R.T.: 7.921 min
Delta R.T.: 0.004 min
Response: 157621
Conc: 45.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

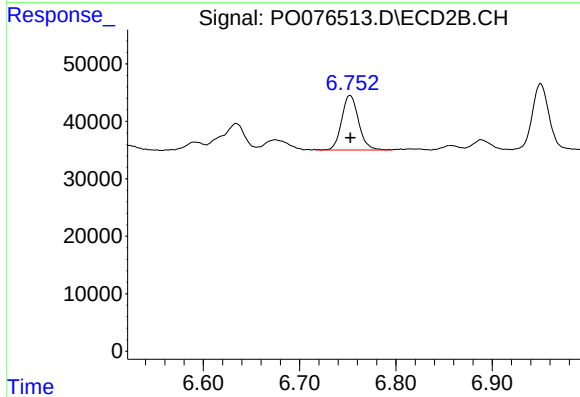


#31 AR-1260-1

R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 115241
Conc: 44.97 ng/ml

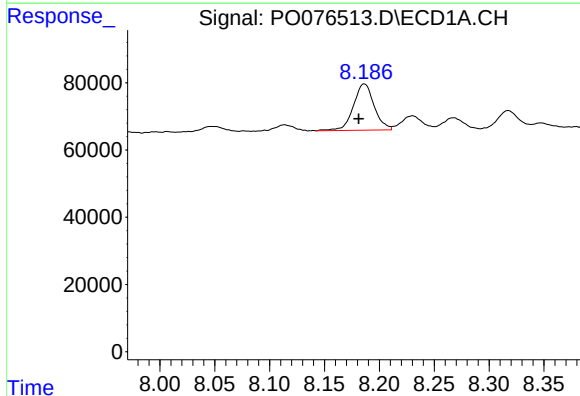


#32 AR-1260-2

R.T.: 8.186 min
Delta R.T.: 0.005 min
Response: 182298
Conc: 44.96 ng/ml

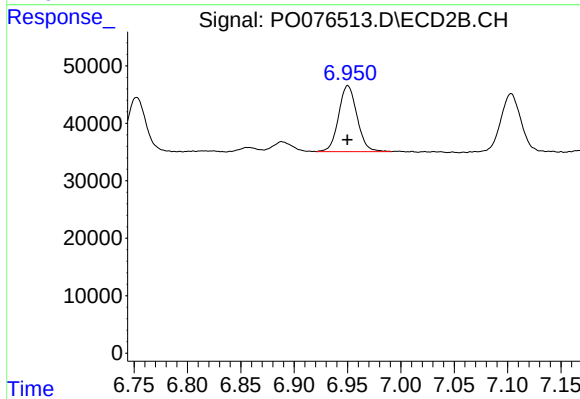

#32 AR-1260-2


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 137555
Conc: 44.35 ng/ml

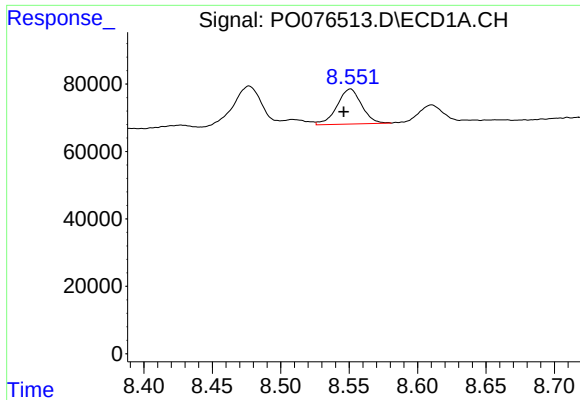

#33 AR-1260-3


R.T.: 8.551 min
Delta R.T.: 0.005 min
Response: 129608
Conc: 42.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

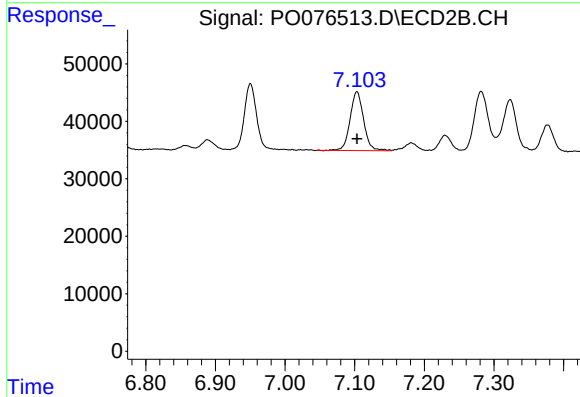


#33 AR-1260-3

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 138039
Conc: 46.99 ng/ml

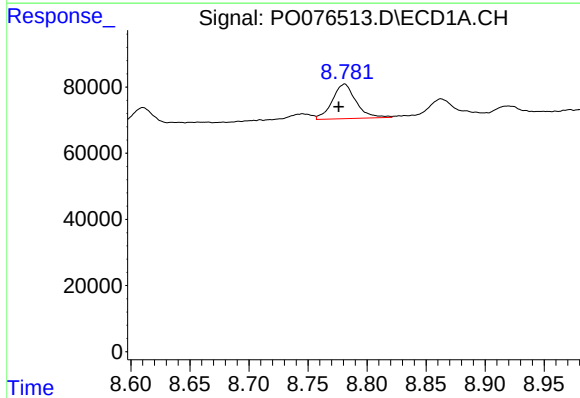


#34 AR-1260-4

R.T.: 8.781 min
Delta R.T.: 0.005 min
Response: 146006
Conc: 41.90 ng/ml

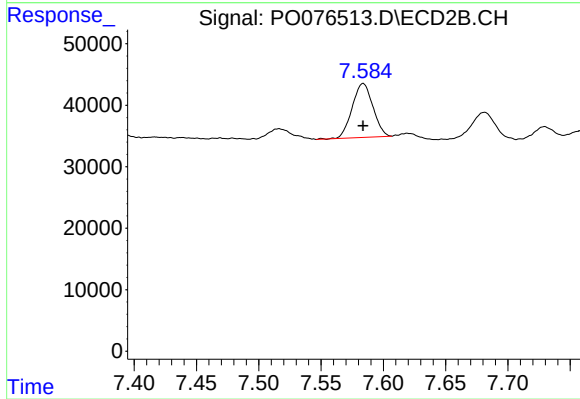

#34 AR-1260-4


R.T.: 7.584 min
Delta R.T.: 0.000 min
Response: 101876
Conc: 42.75 ng/ml

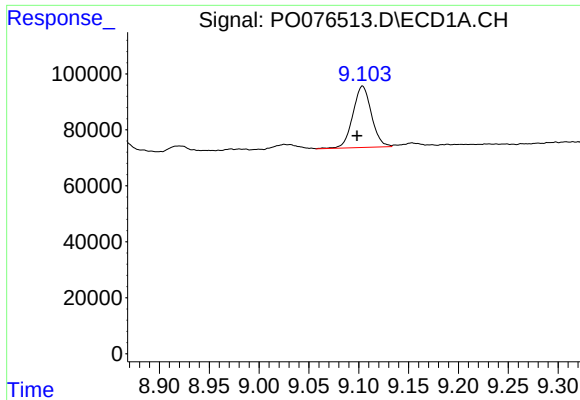

#35 AR-1260-5


R.T.: 9.104 min
Delta R.T.: 0.006 min
Response: 284604
Conc: 42.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

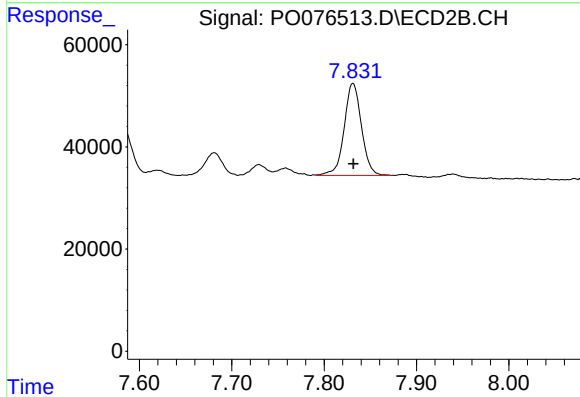


#35 AR-1260-5

R.T.: 7.831 min
Delta R.T.: 0.000 min
Response: 234778
Conc: 41.38 ng/ml

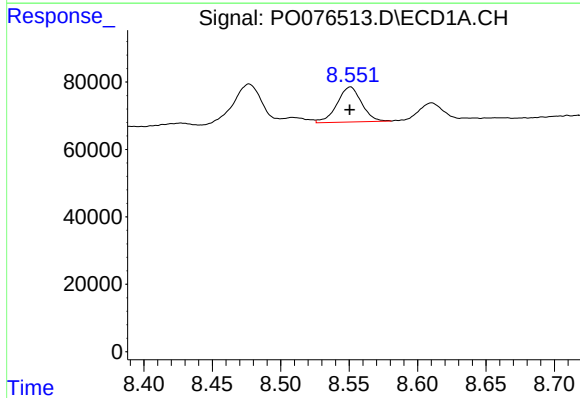


#36 AR-1262-1

R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 129608
Conc: 25.05 ng/ml

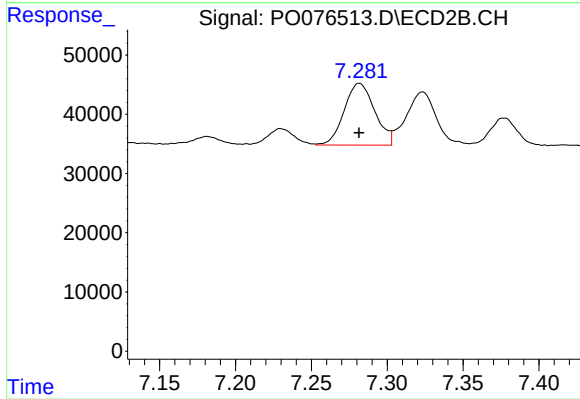

#36 AR-1262-1


R.T.: 7.282 min
Delta R.T.: 0.000 min
Response: 146683
Conc: 74.59 ng/ml

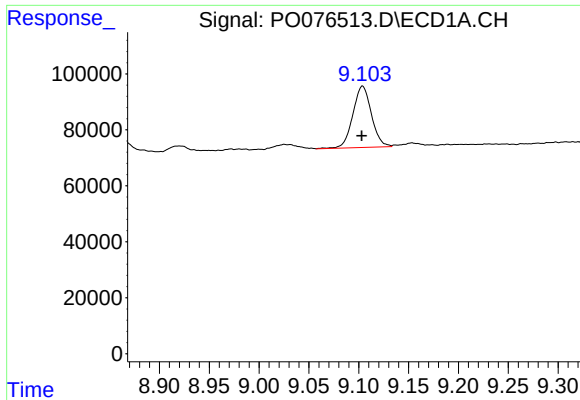

#37 AR-1262-2


R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 284604
Conc: 33.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

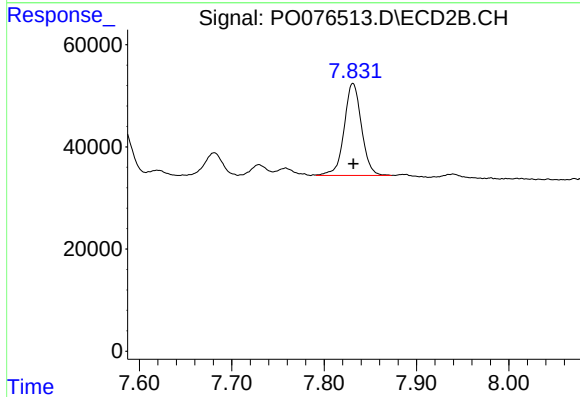


#37 AR-1262-2

R.T.: 7.831 min
Delta R.T.: 0.000 min
Response: 234778
Conc: 34.92 ng/ml

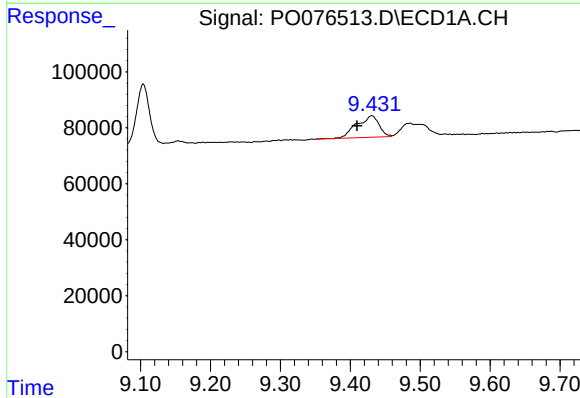


#38 AR-1262-3

R.T.: 9.431 min
Delta R.T.: 0.021 min
Response: 171764
Conc: 30.30 ng/ml

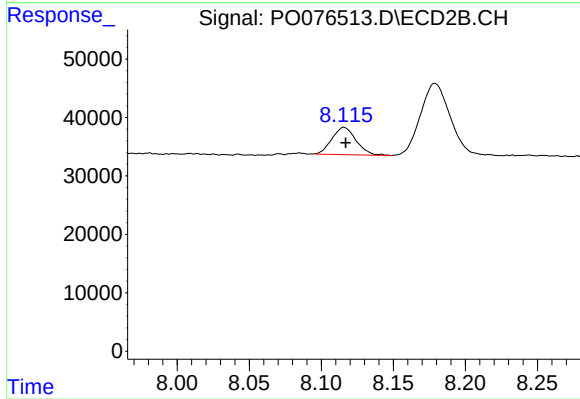

#38 AR-1262-3


R.T.: 8.116 min
Delta R.T.: -0.001 min
Response: 54712
Conc: 20.31 ng/ml

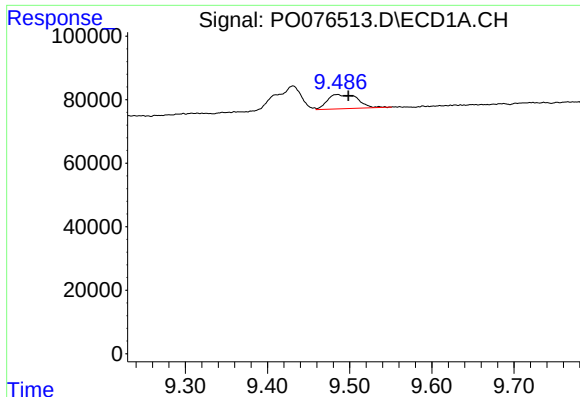

#39 AR-1262-4


R.T.: 9.485 min
Delta R.T.: -0.014 min
Response: 114120
Conc: 26.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

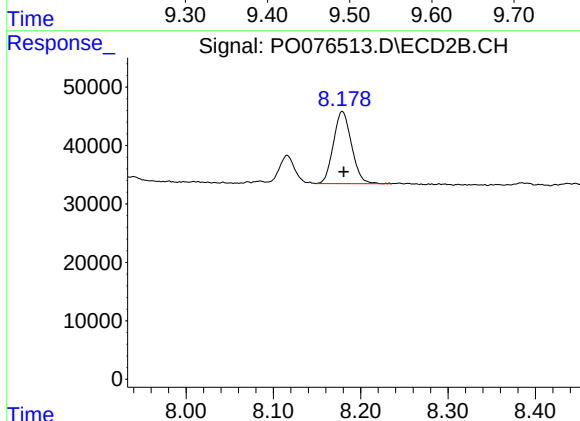


#39 AR-1262-4

R.T.: 8.179 min
Delta R.T.: -0.002 min
Response: 178406
Conc: 35.85 ng/ml

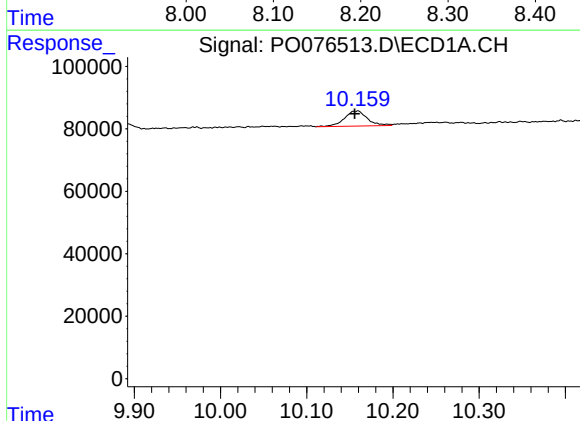


#40 AR-1262-5

R.T.: 10.158 min
Delta R.T.: 0.002 min
Response: 88918
Conc: 30.60 ng/ml

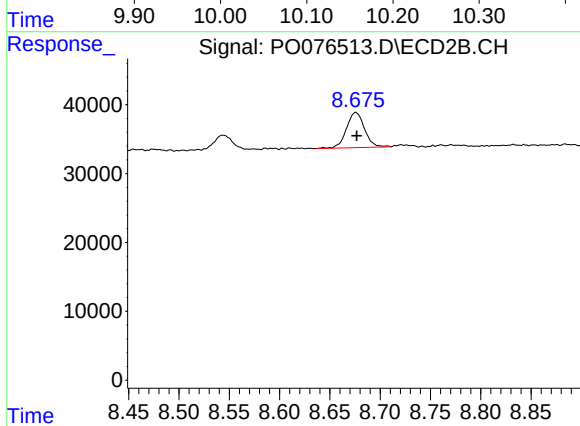

#40 AR-1262-5


R.T.: 8.676 min
Delta R.T.: 0.000 min
Response: 63786
Conc: 29.36 ng/ml

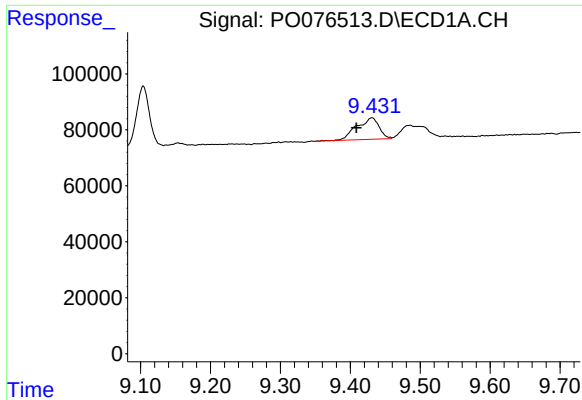

#41 AR-1268-1


R.T.: 9.431 min
Delta R.T.: 0.022 min
Response: 171764
Conc: 16.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

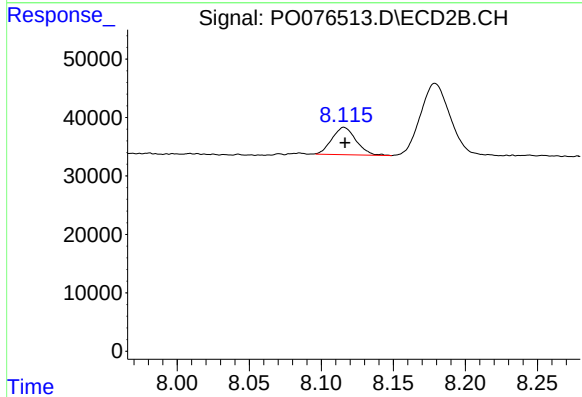


#41 AR-1268-1

R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 54712
Conc: 7.02 ng/ml

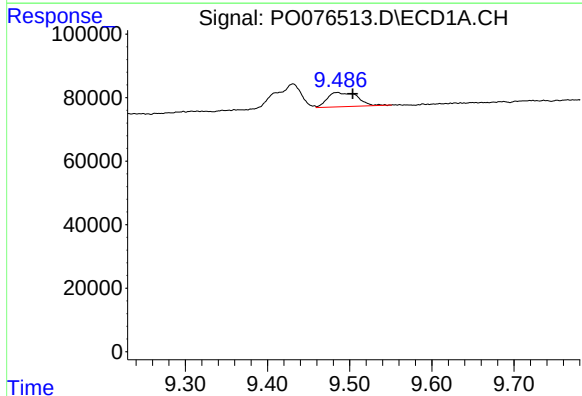


#42 AR-1268-2

R.T.: 9.485 min
Delta R.T.: -0.019 min
Response: 114120
Conc: 12.26 ng/ml

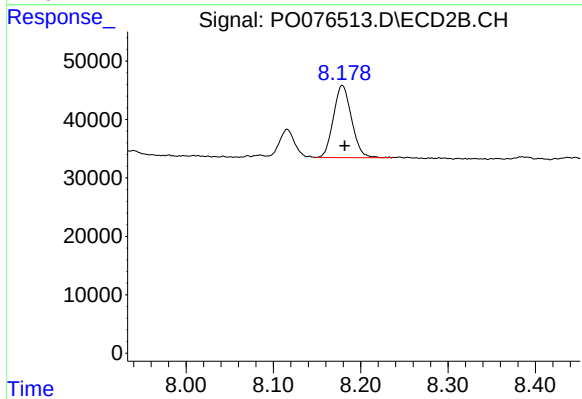

#42 AR-1268-2


R.T.: 8.179 min
Delta R.T.: -0.003 min
Response: 178406
Conc: 25.15 ng/ml

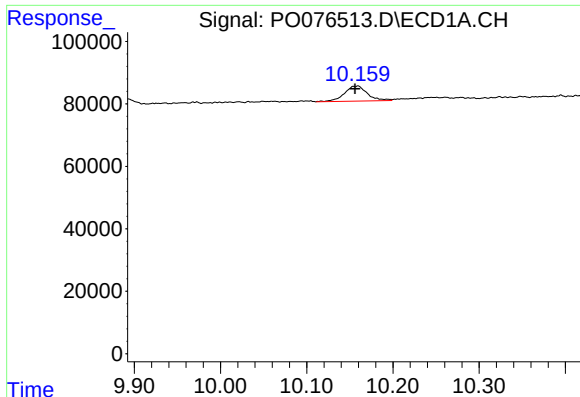

#44 AR-1268-4


R.T.: 10.158 min
Delta R.T.: 0.002 min
Response: 88918
Conc: 27.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

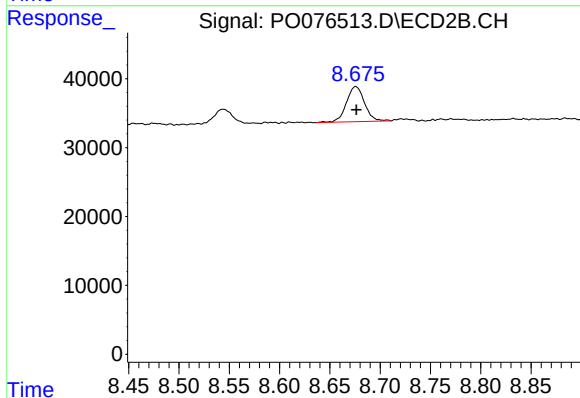


#44 AR-1268-4

R.T.: 8.676 min
Delta R.T.: 0.000 min
Response: 63786
Conc: 26.41 ng/ml

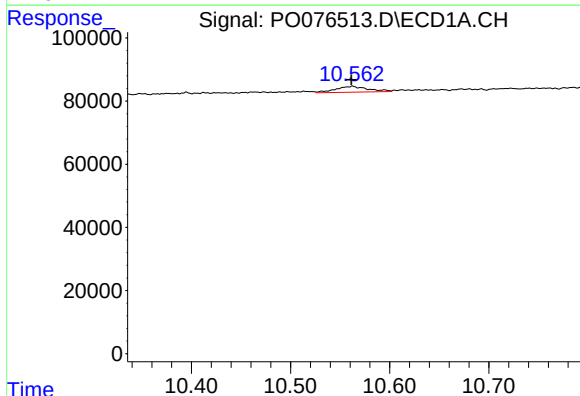

#45 AR-1268-5

R.T.: 10.562 min
Delta R.T.: 0.000 min
Response: 42188
Conc: 1.59 ng/ml

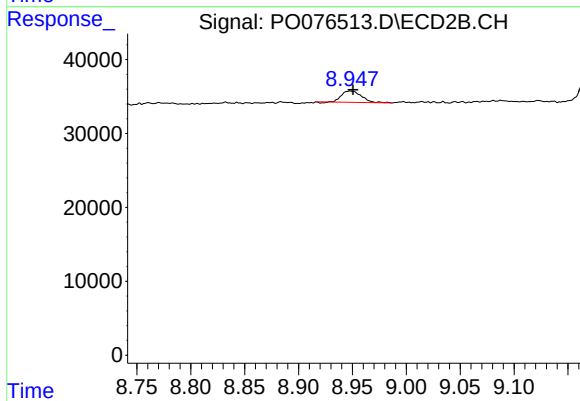

#45 AR-1268-5

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 19309
Conc: 1.07 ng/ml