

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 9:12
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 14:20:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.915	3.929	1614985	962506	18.440	17.547
2)	SA Decachlor...	10.888	9.187	1264236	895371	19.421	19.001
Target Compounds							
3)	L1 AR-1016-1	6.238	5.178	50501	26131	18.687	15.866
4)	L1 AR-1016-2	6.262	5.200	75336	49683	18.326	17.120
5)	L1 AR-1016-3	6.327	5.388	48089	18100	19.930	13.556 #
6)	L1 AR-1016-4	6.434	5.437	32365	13874	16.699	12.360 #
7)	L1 AR-1016-5	6.747	5.665	34241	19144	17.580	13.903
8)	L2 AR-1221-1	5.167	0.000	22069	0	25.083	N.D. #
9)	L2 AR-1221-2	5.267	4.283	39880	20753	58.889	48.161
10)	L2 AR-1221-3	5.354	4.373	82221	45420	37.998	33.849
11)	L3 AR-1232-1	5.354	4.373	82221	45420	46.481	41.577
12)	L3 AR-1232-2	5.942	5.200	54148	49683	61.050	41.567 #
13)	L3 AR-1232-3	6.262	5.388	75336	18100	44.613	33.149 #
14)	L3 AR-1232-4	6.434	5.481	32365	18832	41.336	36.682
15)	L3 AR-1232-5	6.531	5.665	30317	19144	54.995	35.094 #
16)	L4 AR-1242-1	6.238	5.178	50501	26131	22.590	20.289
17)	L4 AR-1242-2	6.262	5.200	75336	49683	22.173	21.201
18)	L4 AR-1242-3	6.327	5.388	48089	18100	23.796	16.716 #
19)	L4 AR-1242-4	6.434	5.481	32365	18832	20.095	16.998
20)	L4 AR-1242-5	7.217	6.044	51442	25077	29.451	18.906 #
21)	L5 AR-1248-1	6.238	5.178	50501	26131	30.509	26.073
22)	L5 AR-1248-2	6.531	5.437	30317	13874	12.420	8.521 #
23)	L5 AR-1248-3	6.747	5.481	34241	18832	11.952	11.409
24)	L5 AR-1248-4	7.177	5.665	41278	19144	13.219	9.847 #
25)	L5 AR-1248-5	7.217	6.087	51442	24360	16.520	13.147
26)	L6 AR-1254-1	7.145	6.044	31267	25077	9.414	8.466
27)	L6 AR-1254-2	7.380	0.000	36042	0	7.003	N.D. #
28)	L6 AR-1254-3	7.758	0.000	23957	0	4.504	N.D. #
29)	L6 AR-1254-4	8.054	0.000	9653	0	2.676	N.D. #
30)	L6 AR-1254-5	8.486	0.000	6732	0	1.717	N.D. #
31)	L7 AR-1260-1	7.890f	0.000	8722	0	2.538	N.D. #
32)	L7 AR-1260-2	8.189	0.000	13047	0	3.218	N.D. #
33)	L7 AR-1260-3	8.554	0.000	5814	0	1.924	N.D. #
34)	L7 AR-1260-4	8.789	0.000	18430	0	5.289	N.D. #
35)	L7 AR-1260-5	9.122f	0.000	17028	0	2.520	N.D. #
36)	L8 AR-1262-1	8.554	0.000	5814	0	1.124	N.D. #
37)	L8 AR-1262-2	9.122f	0.000	17028	0	1.976	N.D. #
38)	L8 AR-1262-3	9.415	0.000	867	0	0.153	N.D. #
39)	L8 AR-1262-4	9.499	0.000	3496	0	0.812	N.D. #
40)	L8 AR-1262-5	10.160	0.000	12485	0	4.297	N.D. #
41)	L9 AR-1268-1	9.415	0.000	867	0	0.084	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 9:12
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 14:20:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
42)	L9 AR-1268-2	9.499	0.000	3496	0	0.376	N.D.	#
43)	L9 AR-1268-3	9.754f	0.000	20101	0	2.420	N.D.	#
44)	L9 AR-1268-4	10.160	0.000	12485	0	3.842	N.D.	#
45)	L9 AR-1268-5	10.574	0.000	24238	0	0.916	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
Data File : P0076515.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 9:12
Operator : DD\AJ
Sample : M1458-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 14:20:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

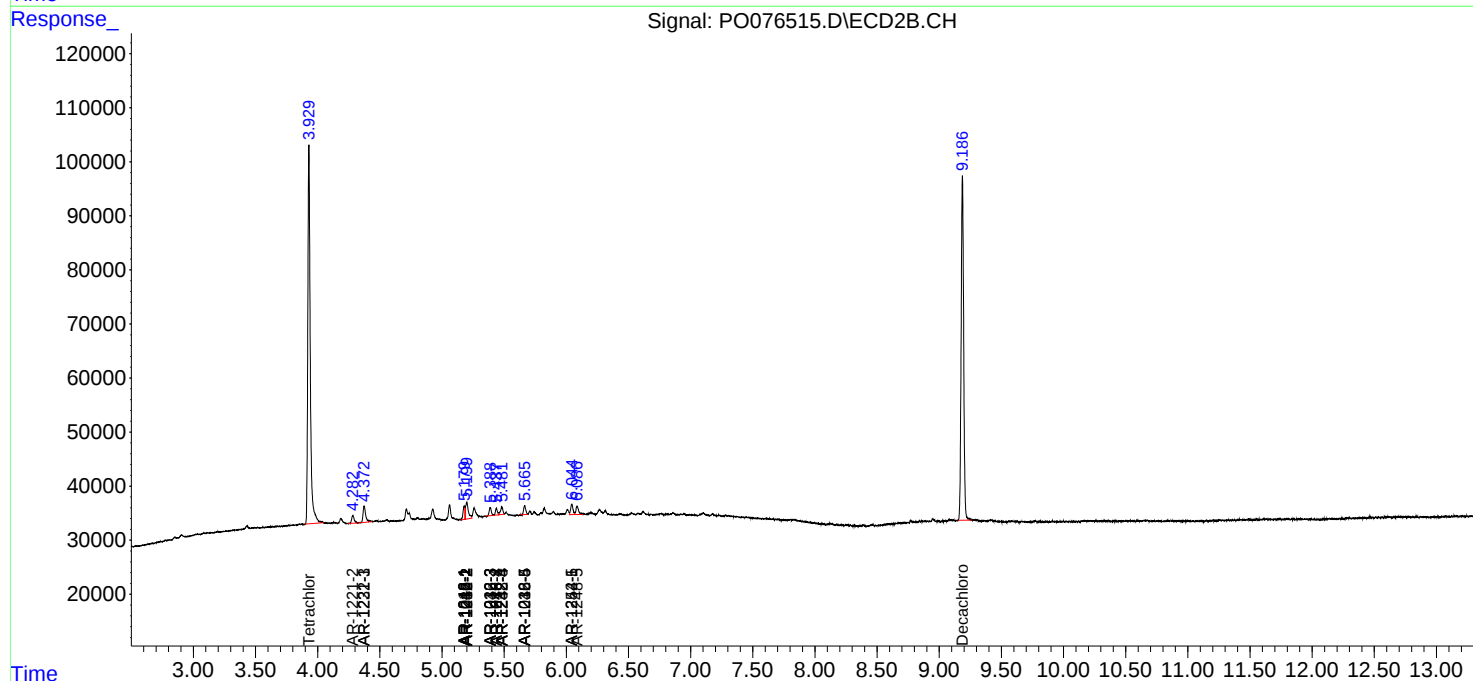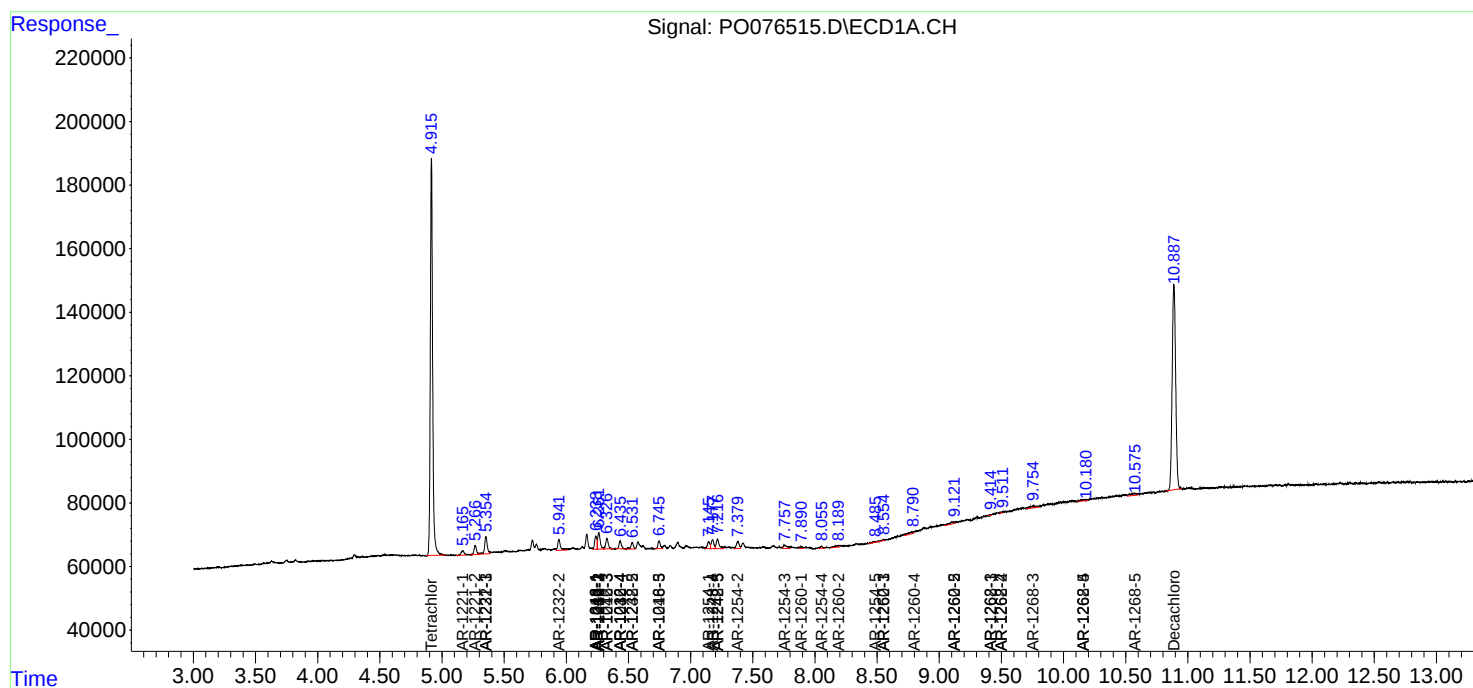


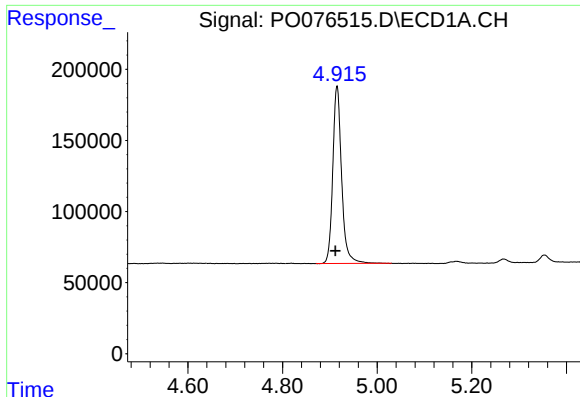

#1 Tetrachloro-m-xylene


R.T.: 4.915 min
Delta R.T.: 0.003 min
Response: 1614985
Conc: 18.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

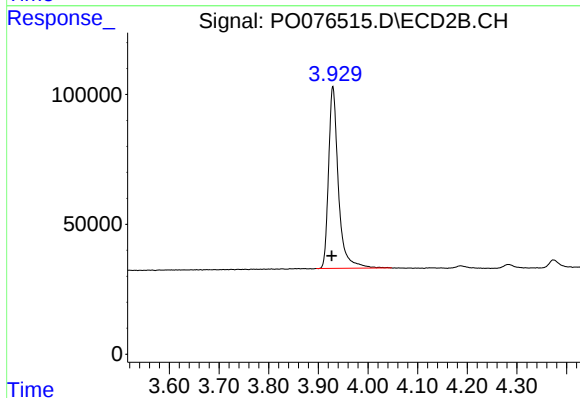


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: 0.002 min
Response: 962506
Conc: 17.55 ng/ml

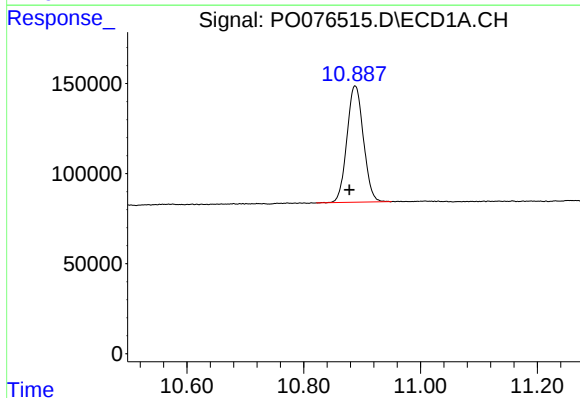


#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.010 min
Response: 1264236
Conc: 19.42 ng/ml

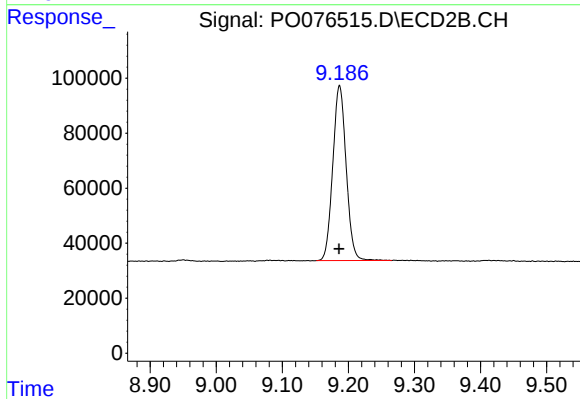

#2 Decachlorobiphenyl


R.T.: 9.187 min
Delta R.T.: 0.000 min
Response: 895371
Conc: 19.00 ng/ml

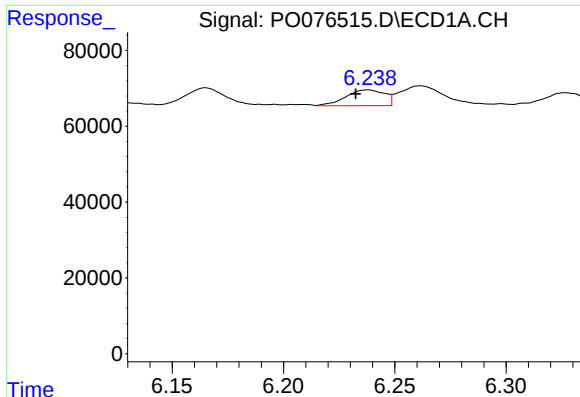

#3 AR-1016-1


R.T.: 6.238 min
Delta R.T.: 0.005 min
Response: 50501
Conc: 18.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

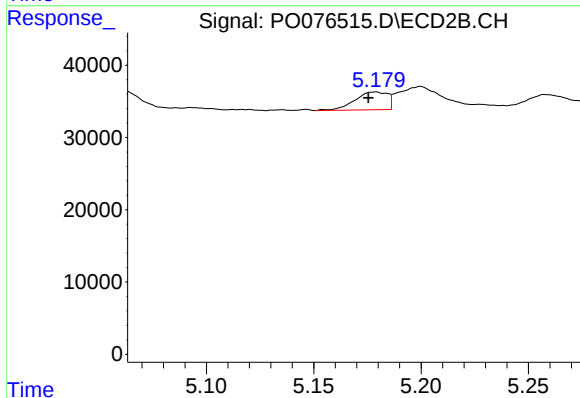


#3 AR-1016-1

R.T.: 5.178 min
Delta R.T.: 0.003 min
Response: 26131
Conc: 15.87 ng/ml

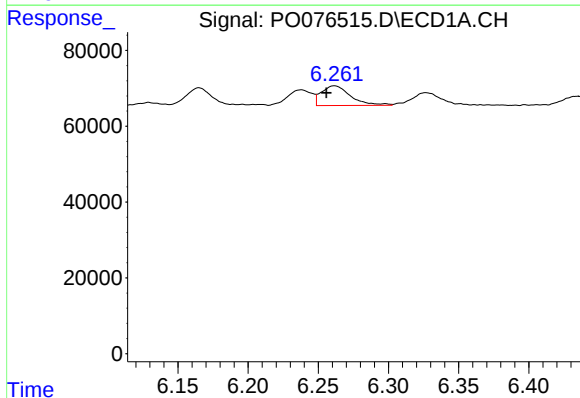


#4 AR-1016-2

R.T.: 6.262 min
Delta R.T.: 0.006 min
Response: 75336
Conc: 18.33 ng/ml

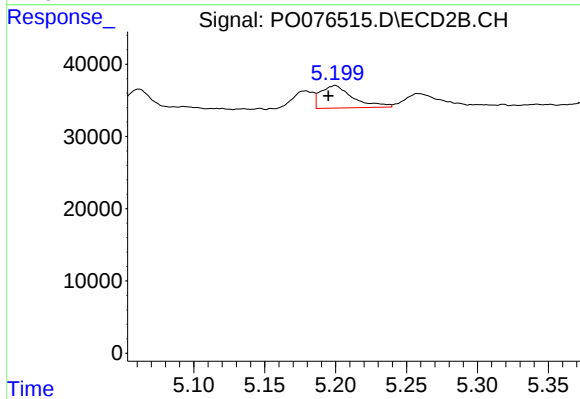

#4 AR-1016-2


R.T.: 5.200 min
Delta R.T.: 0.005 min
Response: 49683
Conc: 17.12 ng/ml

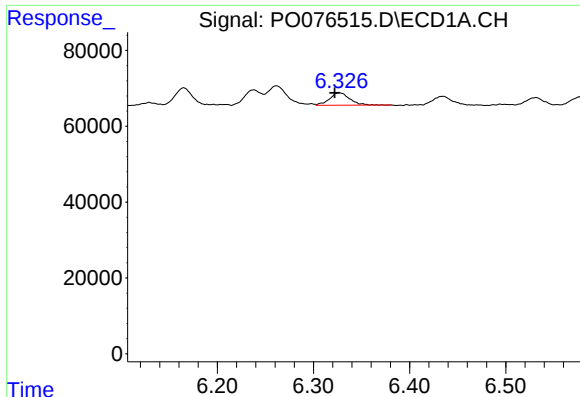

#5 AR-1016-3


R.T.: 6.327 min
Delta R.T.: 0.004 min
Response: 48089
Conc: 19.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

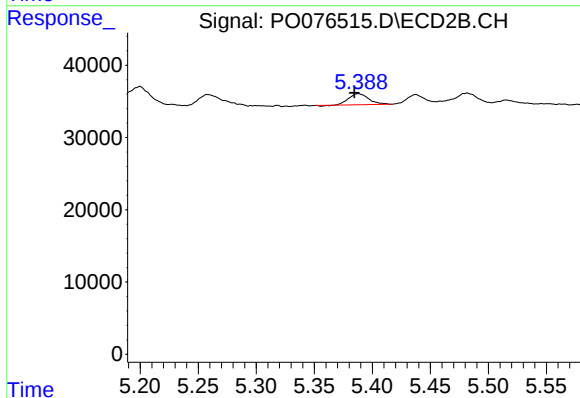


#5 AR-1016-3

R.T.: 5.388 min
Delta R.T.: 0.003 min
Response: 18100
Conc: 13.56 ng/ml

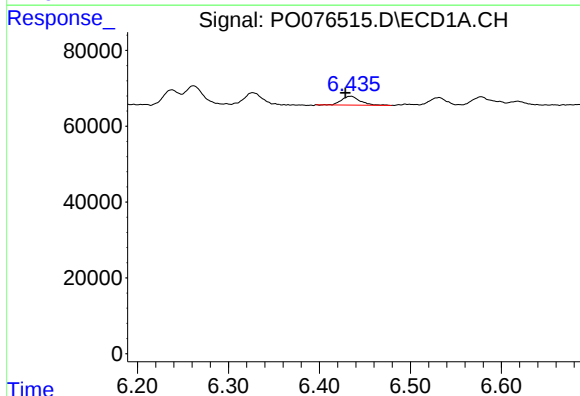


#6 AR-1016-4

R.T.: 6.434 min
Delta R.T.: 0.006 min
Response: 32365
Conc: 16.70 ng/ml

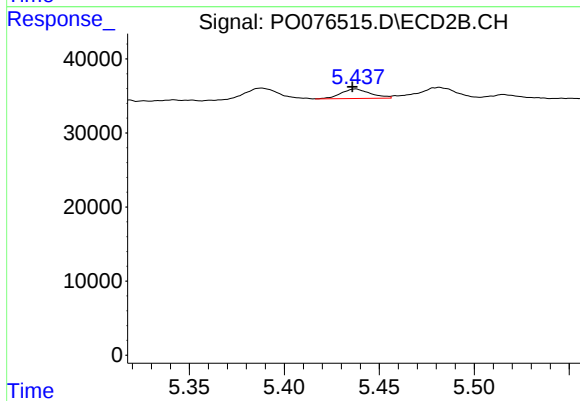

#6 AR-1016-4


R.T.: 5.437 min
Delta R.T.: 0.002 min
Response: 13874
Conc: 12.36 ng/ml

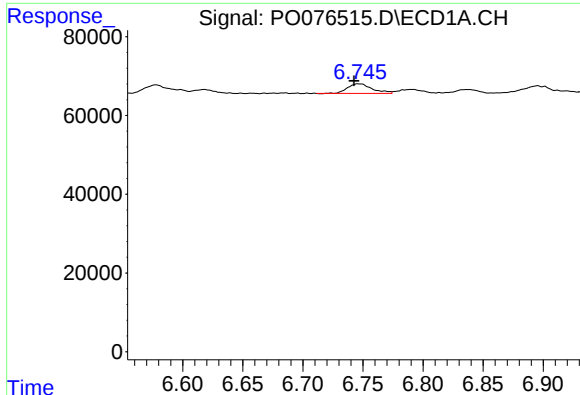

#7 AR-1016-5


R.T.: 6.747 min
Delta R.T.: 0.004 min
Response: 34241
Conc: 17.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

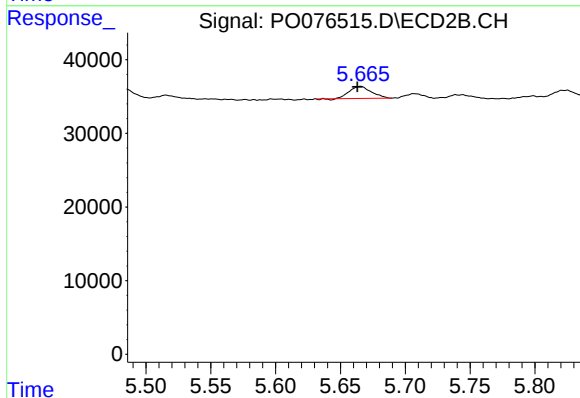


#7 AR-1016-5

R.T.: 5.665 min
Delta R.T.: 0.002 min
Response: 19144
Conc: 13.90 ng/ml

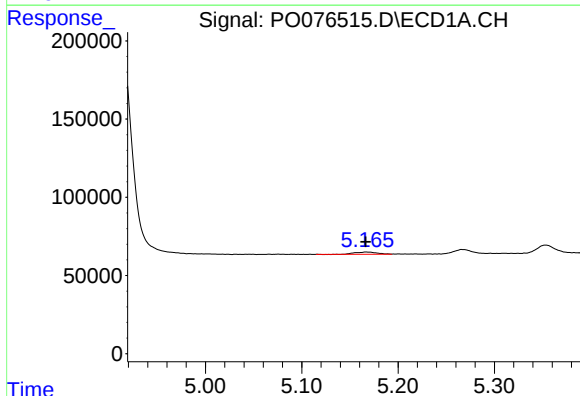


#8 AR-1221-1

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 22069
Conc: 25.08 ng/ml

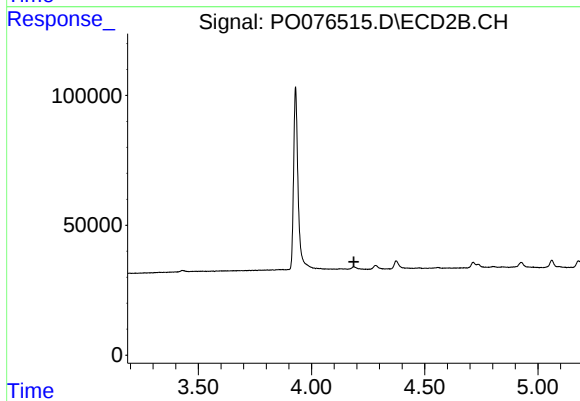

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

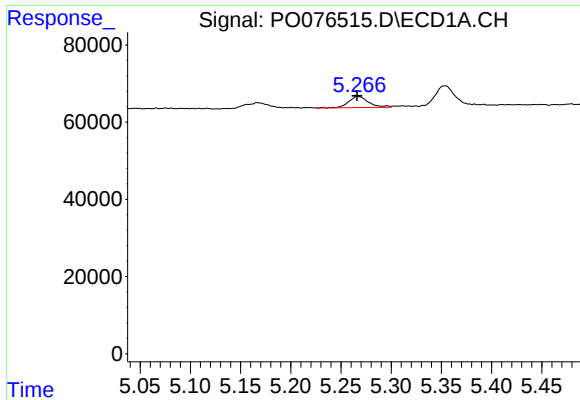

#9 AR-1221-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 39880
Conc: 58.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

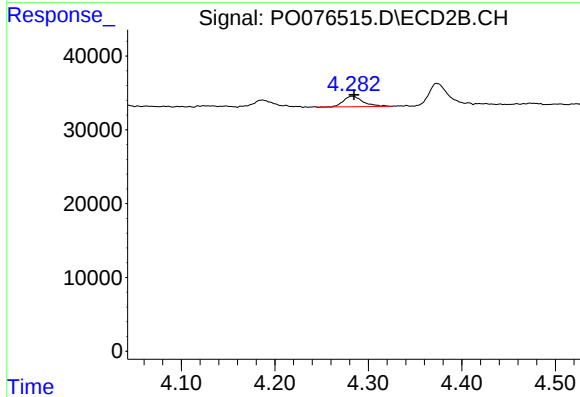


#9 AR-1221-2

R.T.: 4.283 min
Delta R.T.: -0.002 min
Response: 20753
Conc: 48.16 ng/ml

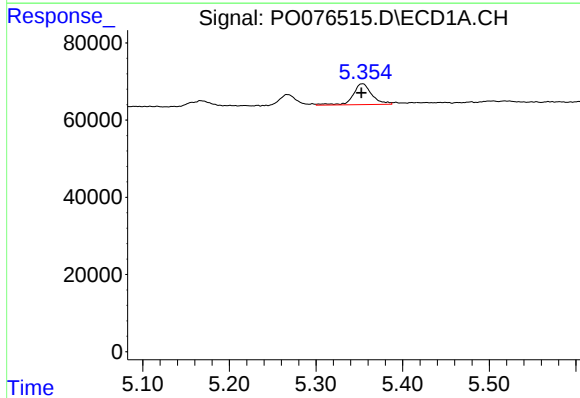


#10 AR-1221-3

R.T.: 5.354 min
Delta R.T.: 0.001 min
Response: 82221
Conc: 38.00 ng/ml

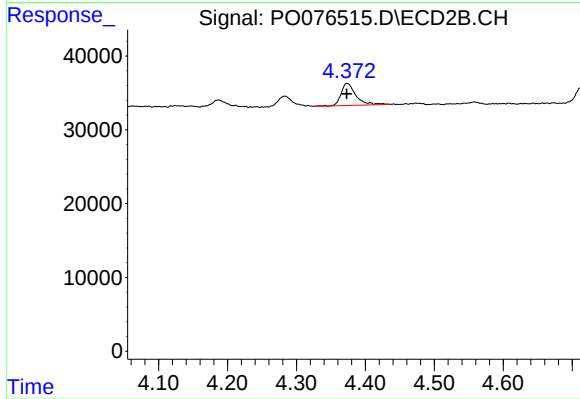

#10 AR-1221-3


R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 45420
Conc: 33.85 ng/ml

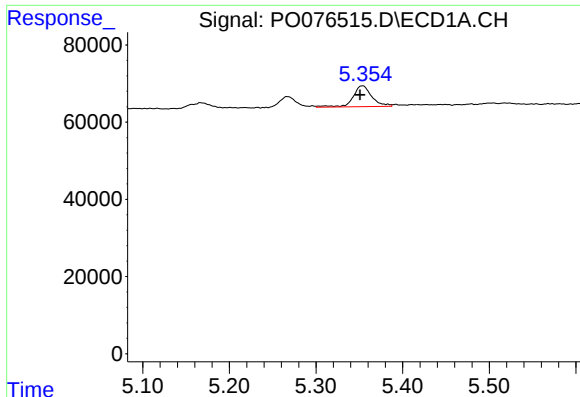

#11 AR-1232-1


R.T.: 5.354 min
Delta R.T.: 0.003 min
Response: 82221
Conc: 46.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

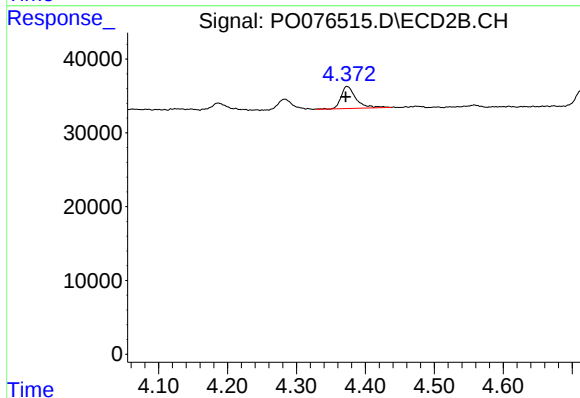


#11 AR-1232-1

R.T.: 4.373 min
Delta R.T.: 0.002 min
Response: 45420
Conc: 41.58 ng/ml

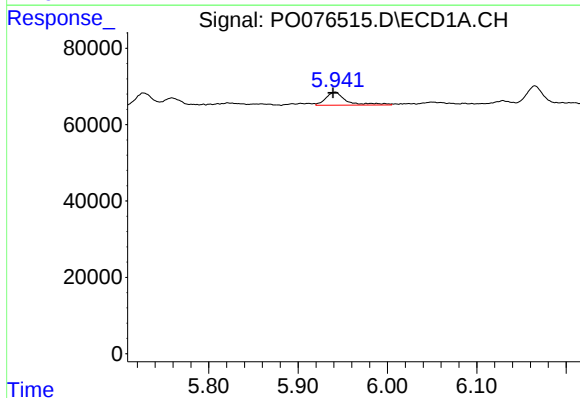


#12 AR-1232-2

R.T.: 5.942 min
Delta R.T.: 0.002 min
Response: 54148
Conc: 61.05 ng/ml

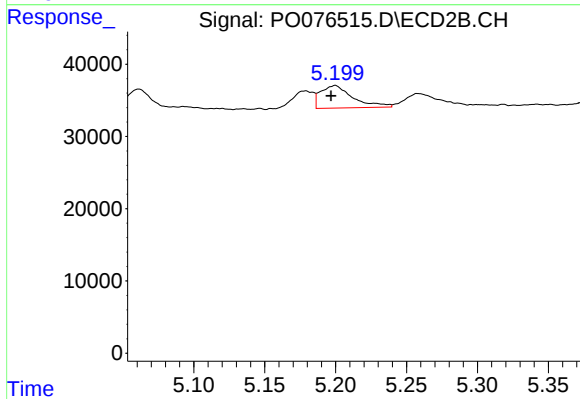

#12 AR-1232-2


R.T.: 5.200 min
Delta R.T.: 0.003 min
Response: 49683
Conc: 41.57 ng/ml

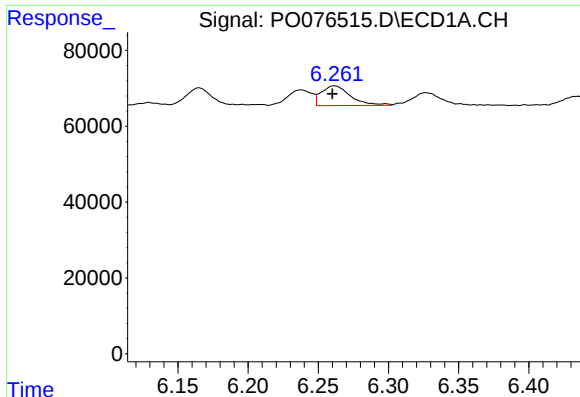

#13 AR-1232-3


R.T.: 6.262 min
Delta R.T.: 0.001 min
Response: 75336
Conc: 44.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

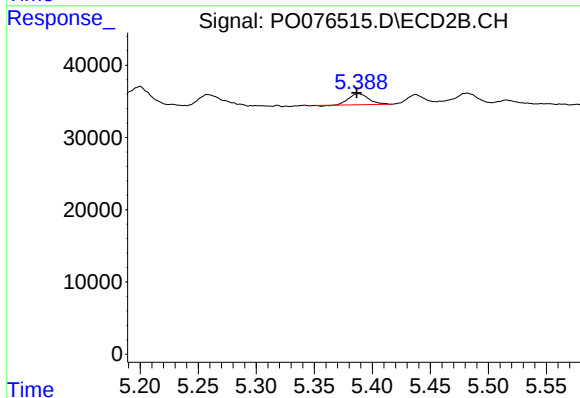


#13 AR-1232-3

R.T.: 5.388 min
Delta R.T.: 0.001 min
Response: 18100
Conc: 33.15 ng/ml

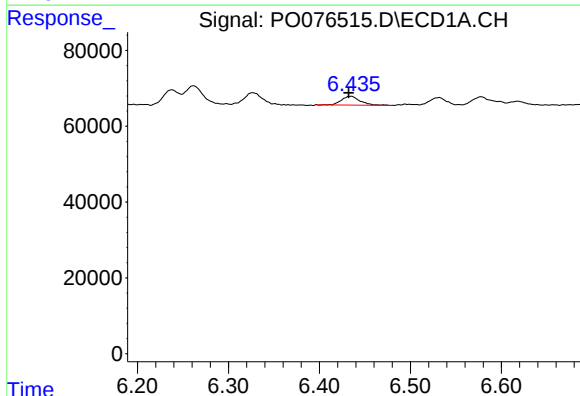


#14 AR-1232-4

R.T.: 6.434 min
Delta R.T.: 0.002 min
Response: 32365
Conc: 41.34 ng/ml

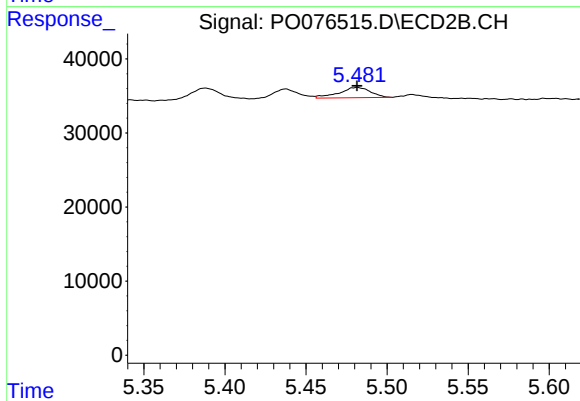

#14 AR-1232-4


R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 18832
Conc: 36.68 ng/ml

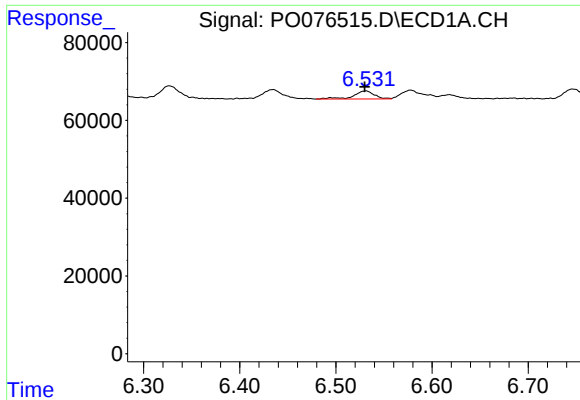

#15 AR-1232-5


R.T.: 6.531 min
Delta R.T.: 0.001 min
Response: 30317
Conc: 55.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

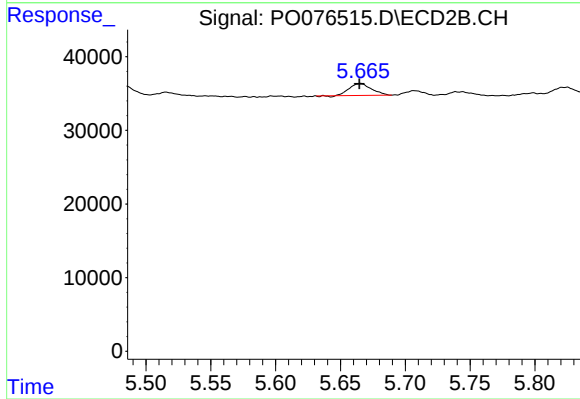


#15 AR-1232-5

R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 19144
Conc: 35.09 ng/ml

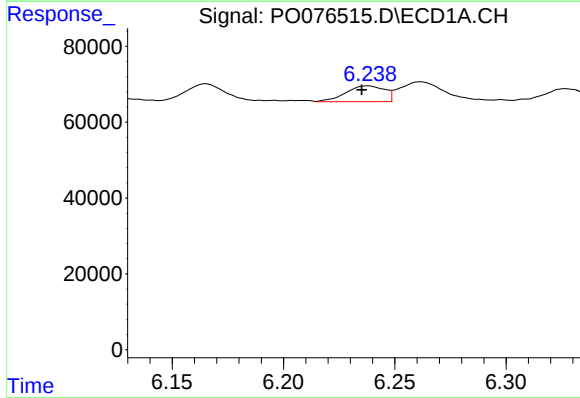


#16 AR-1242-1

R.T.: 6.238 min
Delta R.T.: 0.003 min
Response: 50501
Conc: 22.59 ng/ml

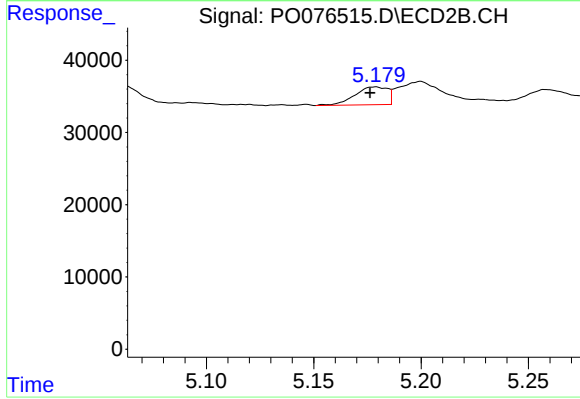

#16 AR-1242-1


R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 26131
Conc: 20.29 ng/ml

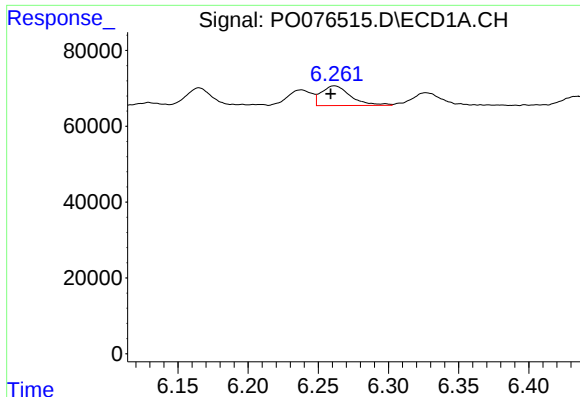

#17 AR-1242-2


R.T.: 6.262 min
Delta R.T.: 0.003 min
Response: 75336
Conc: 22.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

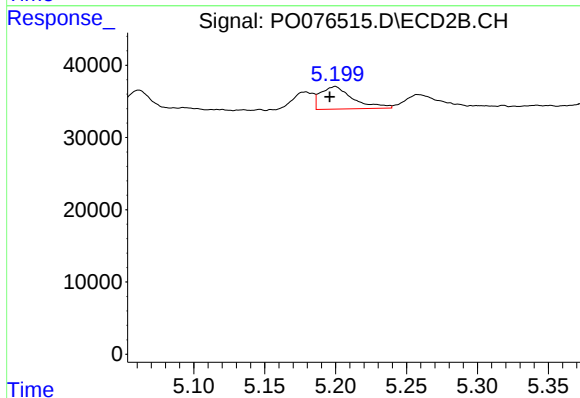


#17 AR-1242-2

R.T.: 5.200 min
Delta R.T.: 0.004 min
Response: 49683
Conc: 21.20 ng/ml

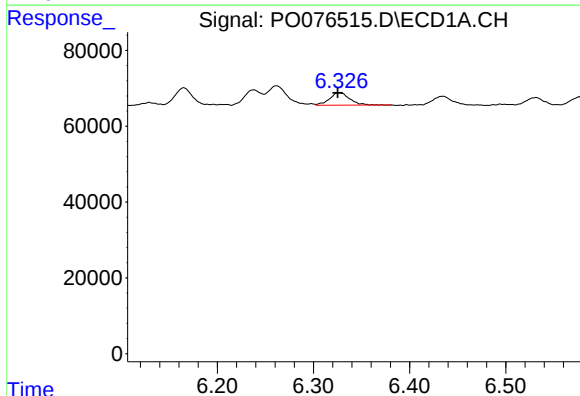


#18 AR-1242-3

R.T.: 6.327 min
Delta R.T.: 0.001 min
Response: 48089
Conc: 23.80 ng/ml

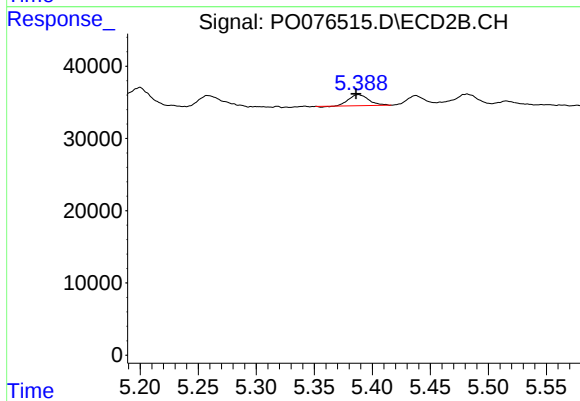

#18 AR-1242-3


R.T.: 5.388 min
Delta R.T.: 0.002 min
Response: 18100
Conc: 16.72 ng/ml

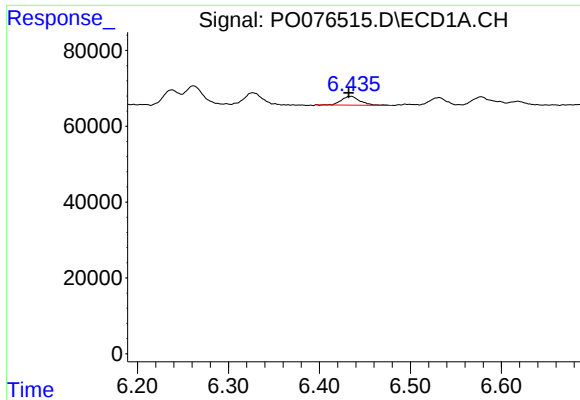

#19 AR-1242-4


R.T.: 6.434 min
Delta R.T.: 0.002 min
Response: 32365
Conc: 20.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

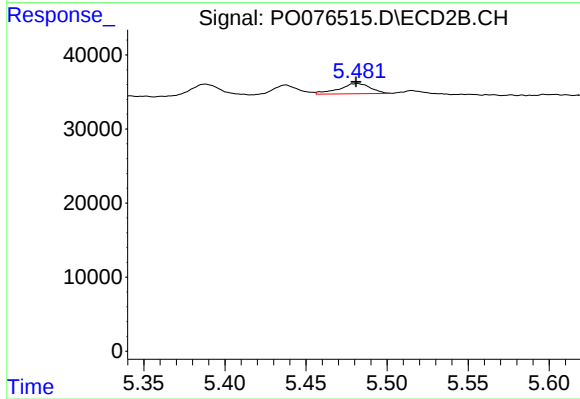


#19 AR-1242-4

R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 18832
Conc: 17.00 ng/ml

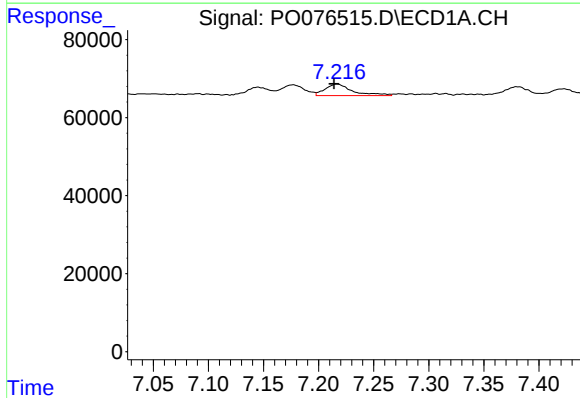


#20 AR-1242-5

R.T.: 7.217 min
Delta R.T.: 0.003 min
Response: 51442
Conc: 29.45 ng/ml

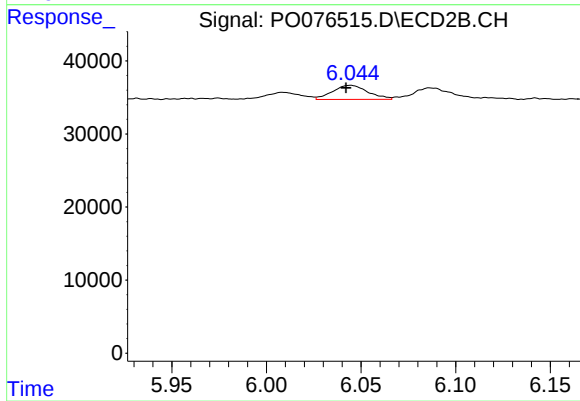

#20 AR-1242-5


R.T.: 6.044 min
Delta R.T.: 0.002 min
Response: 25077
Conc: 18.91 ng/ml

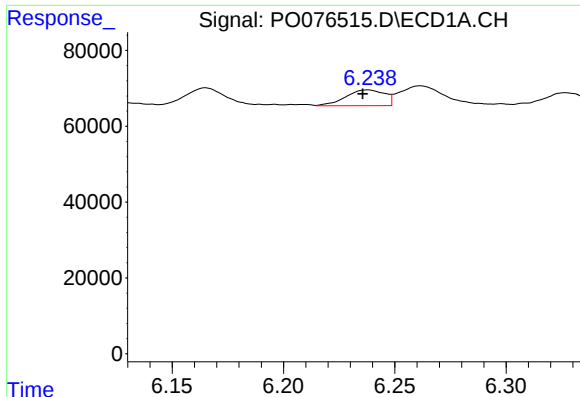

#21 AR-1248-1


R.T.: 6.238 min
Delta R.T.: 0.002 min
Response: 50501
Conc: 30.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

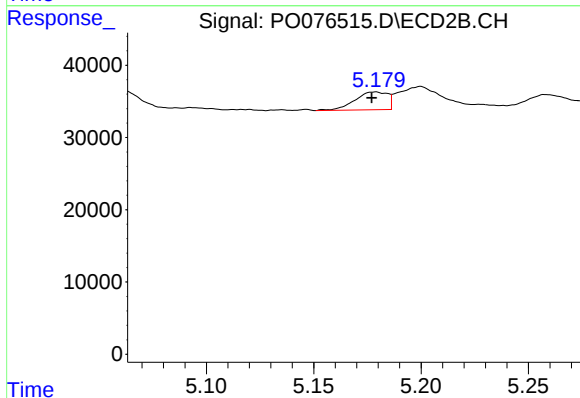


#21 AR-1248-1

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 26131
Conc: 26.07 ng/ml

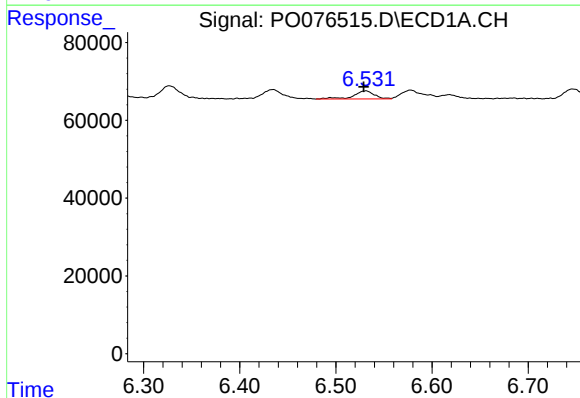


#22 AR-1248-2

R.T.: 6.531 min
Delta R.T.: 0.002 min
Response: 30317
Conc: 12.42 ng/ml

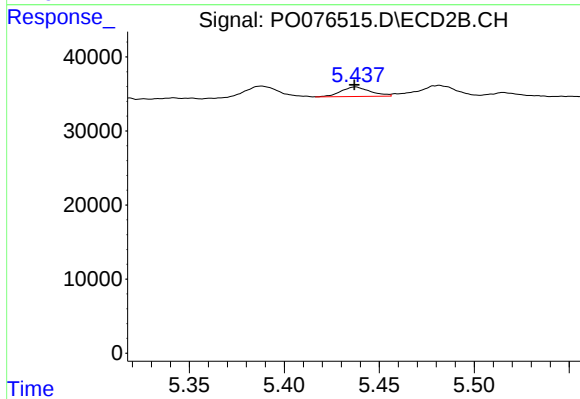

#22 AR-1248-2


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 13874
Conc: 8.52 ng/ml

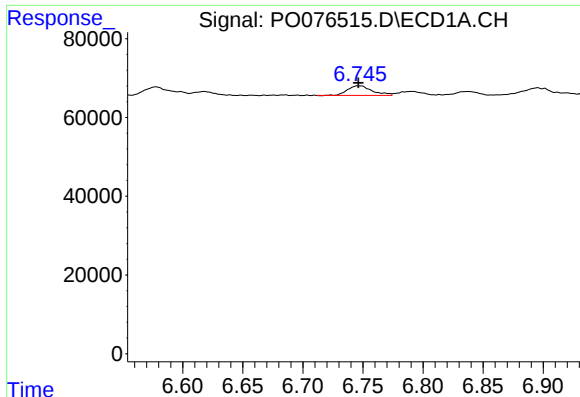

#23 AR-1248-3


R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 34241
Conc: 11.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

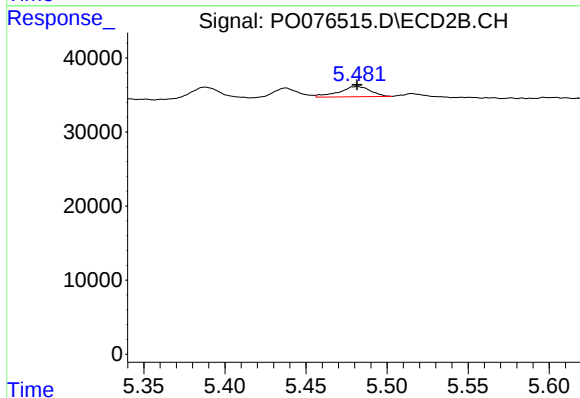


#23 AR-1248-3

R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 18832
Conc: 11.41 ng/ml

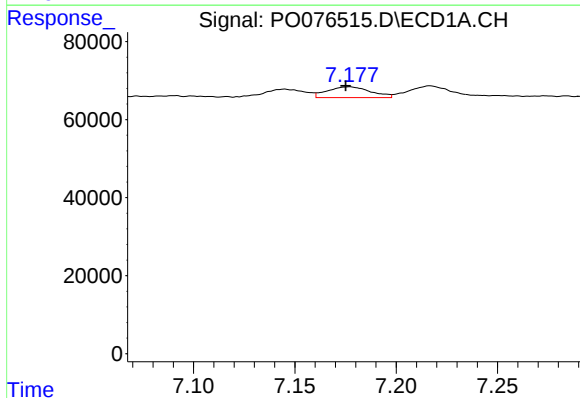


#24 AR-1248-4

R.T.: 7.177 min
Delta R.T.: 0.001 min
Response: 41278
Conc: 13.22 ng/ml

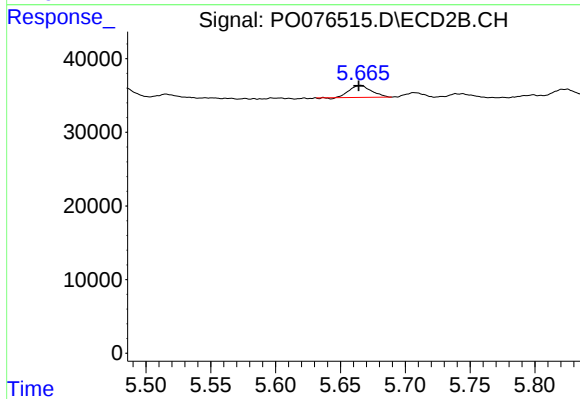

#24 AR-1248-4


R.T.: 5.665 min
Delta R.T.: 0.001 min
Response: 19144
Conc: 9.85 ng/ml

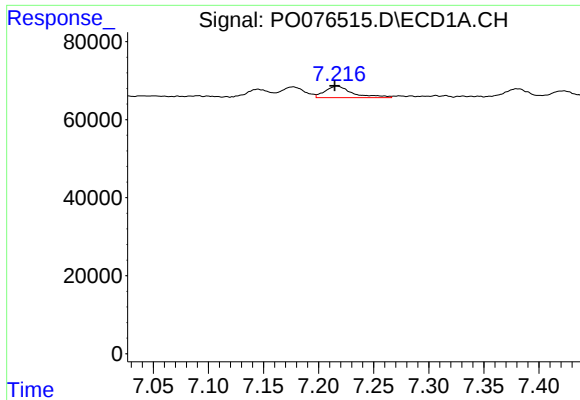

#25 AR-1248-5


R.T.: 7.217 min
Delta R.T.: 0.002 min
Response: 51442
Conc: 16.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

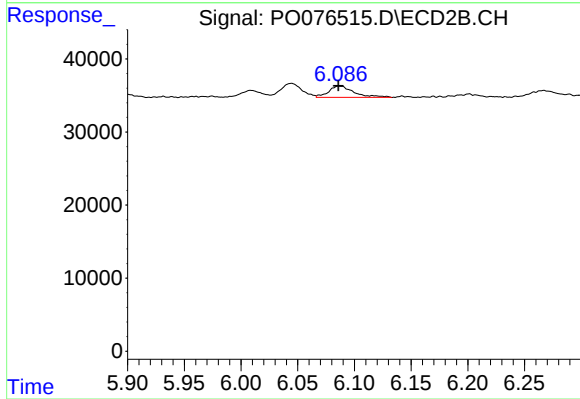


#25 AR-1248-5

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 24360
Conc: 13.15 ng/ml

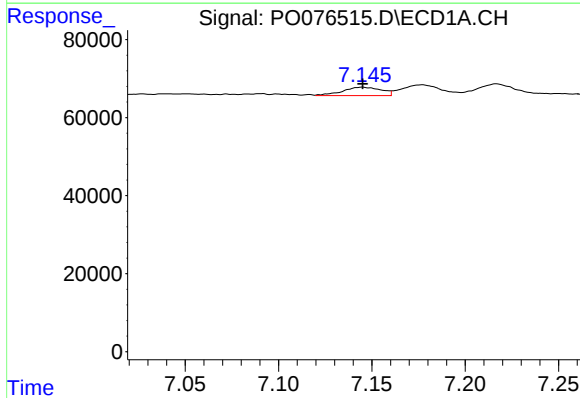


#26 AR-1254-1

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 31267
Conc: 9.41 ng/ml

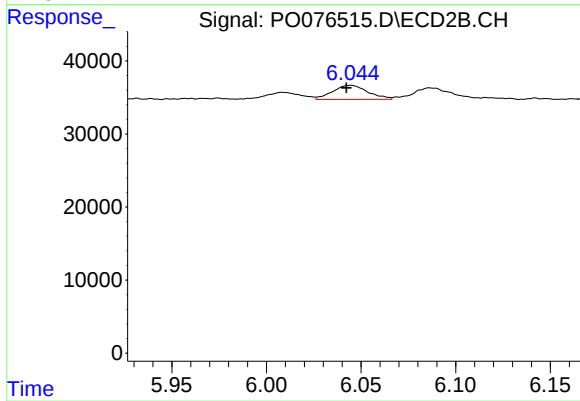

#26 AR-1254-1


R.T.: 6.044 min
Delta R.T.: 0.002 min
Response: 25077
Conc: 8.47 ng/ml

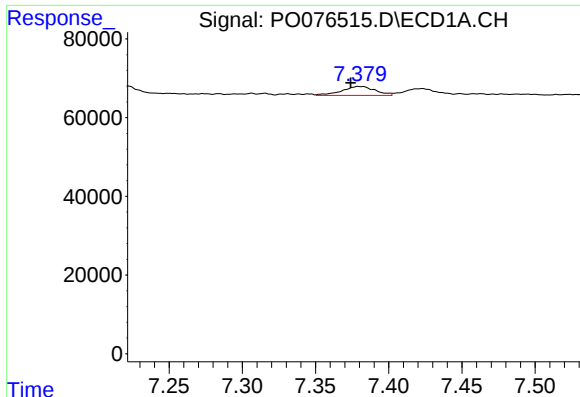

#27 AR-1254-2


R.T.: 7.380 min
Delta R.T.: 0.006 min
Response: 36042
Conc: 7.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

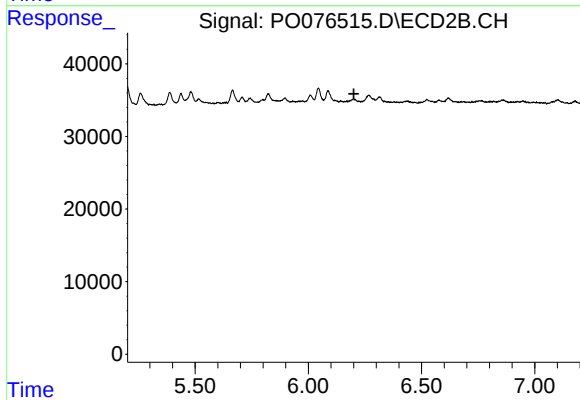


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.201 min
Response: 0
Conc: N.D.

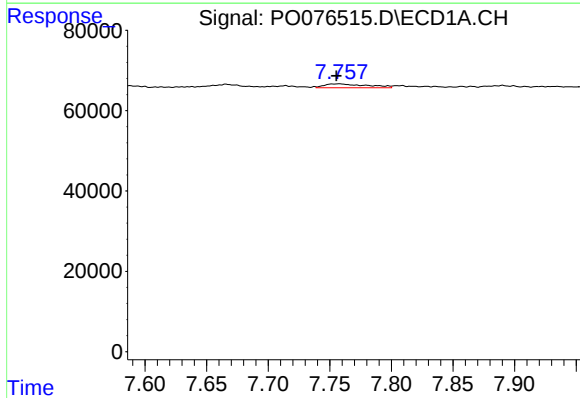


#28 AR-1254-3

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 23957
Conc: 4.50 ng/ml

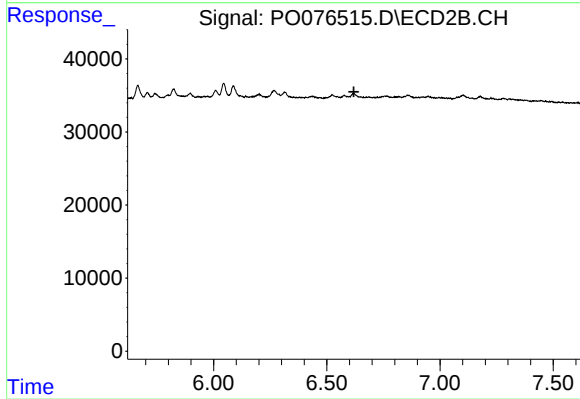

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.619 min
Response: 0
Conc: N.D.

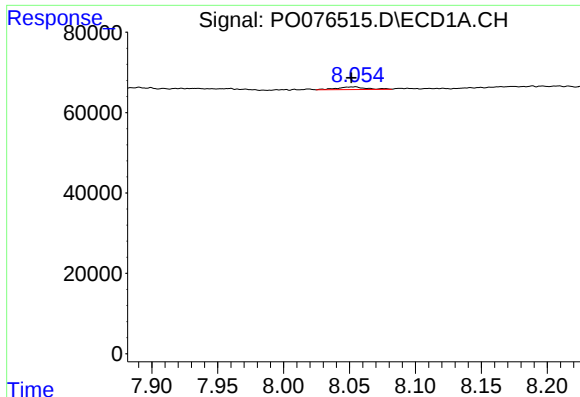

#29 AR-1254-4


R.T.: 8.054 min
Delta R.T.: 0.003 min
Response: 9653
Conc: 2.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

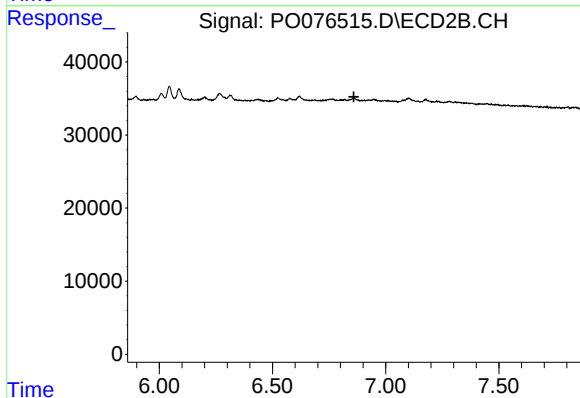


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

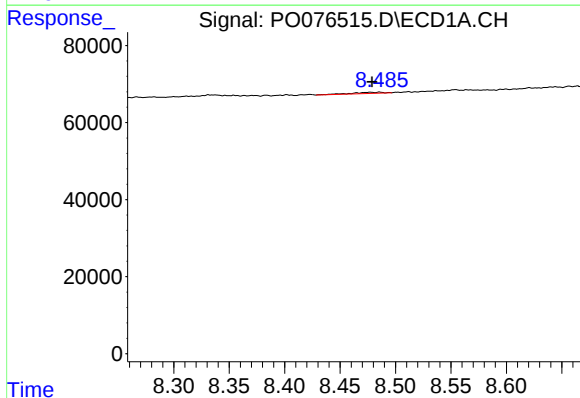


#30 AR-1254-5

R.T.: 8.486 min
Delta R.T.: 0.007 min
Response: 6732
Conc: 1.72 ng/ml

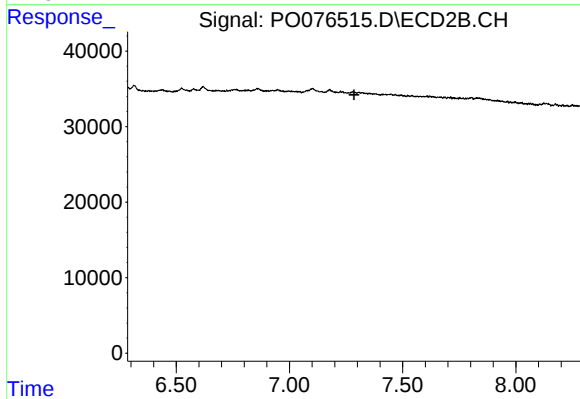

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

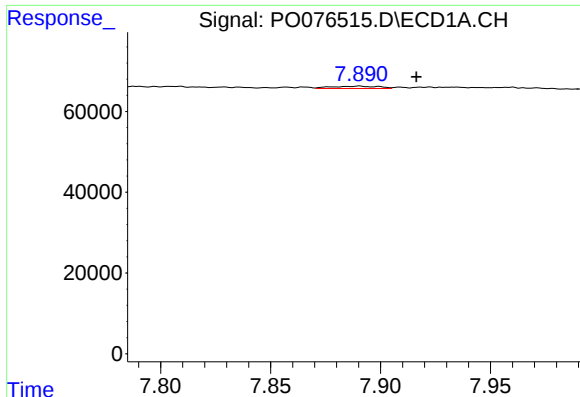

#31 AR-1260-1


R.T.: 7.890 min
Delta R.T.: -0.026 min
Response: 8722
Conc: 2.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

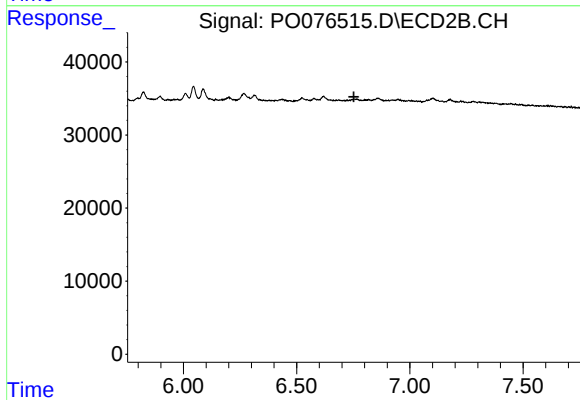


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.753 min
Response: 0
Conc: N.D.

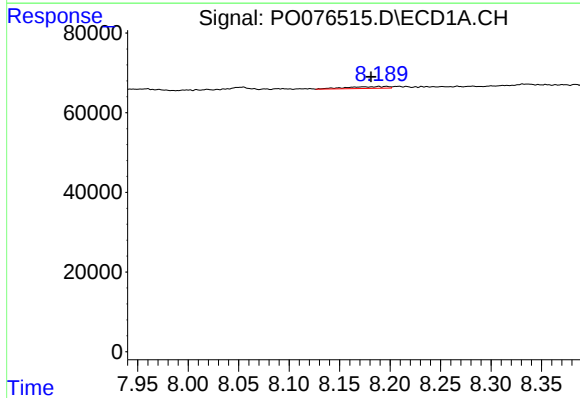


#32 AR-1260-2

R.T.: 8.189 min
Delta R.T.: 0.007 min
Response: 13047
Conc: 3.22 ng/ml

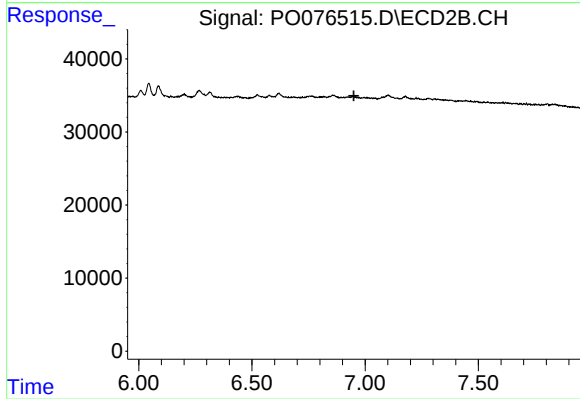

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.950 min
Response: 0
Conc: N.D.

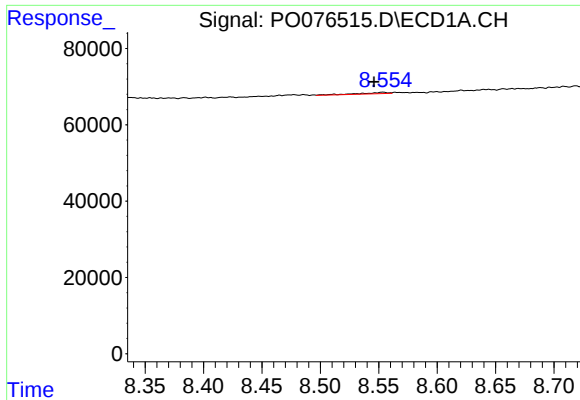

#33 AR-1260-3


R.T.: 8.554 min
Delta R.T.: 0.008 min
Response: 5814
Conc: 1.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

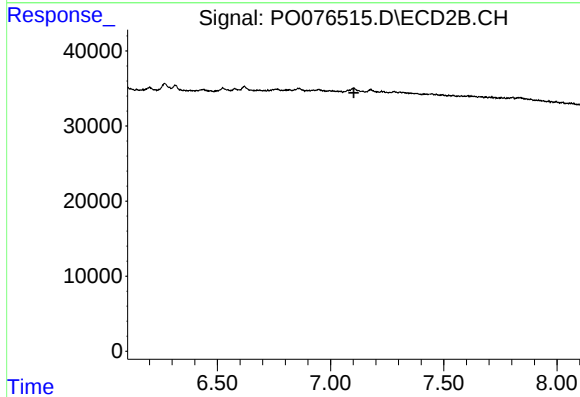


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.103 min
Response: 0
Conc: N.D.

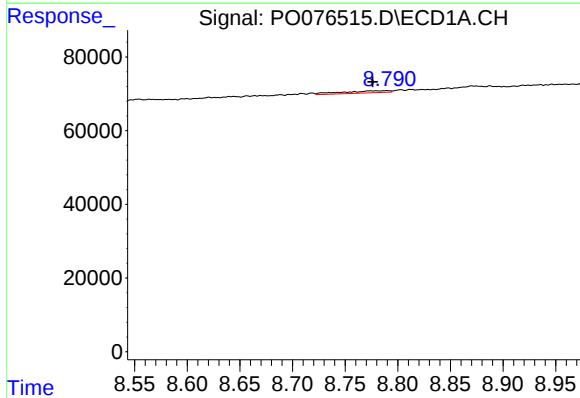


#34 AR-1260-4

R.T.: 8.789 min
Delta R.T.: 0.013 min
Response: 18430
Conc: 5.29 ng/ml

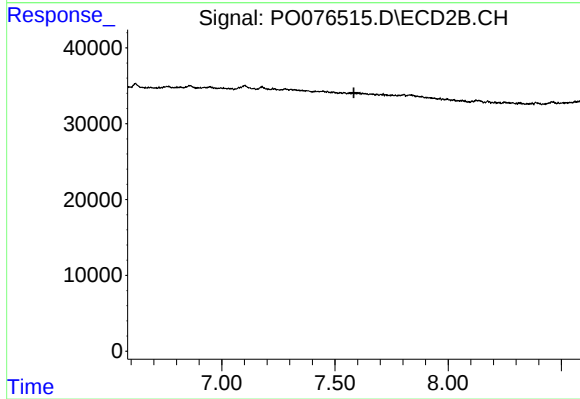

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.584 min
Response: 0
Conc: N.D.

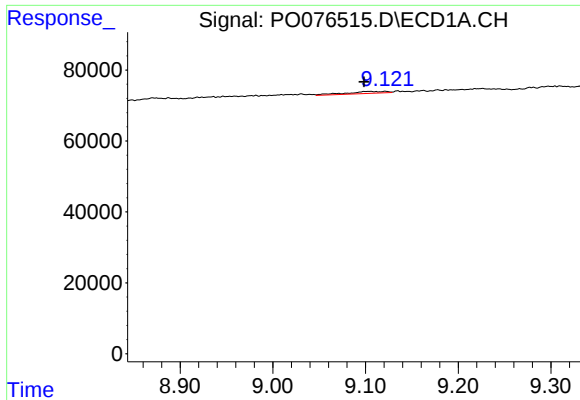

#35 AR-1260-5


R.T.: 9.122 min
Delta R.T.: 0.023 min
Response: 17028
Conc: 2.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

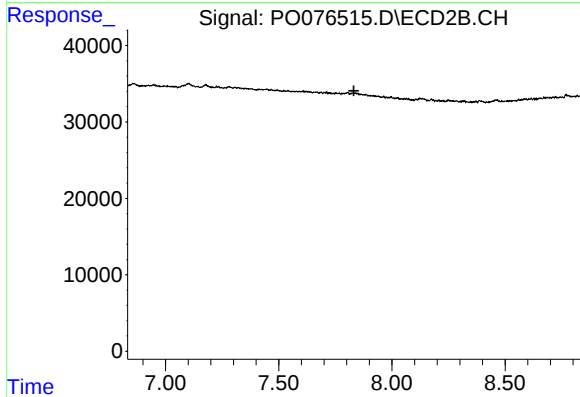


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.832 min
Response: 0
Conc: N.D.

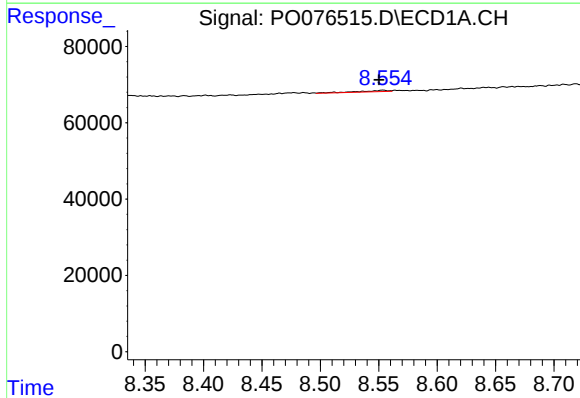


#36 AR-1262-1

R.T.: 8.554 min
Delta R.T.: 0.003 min
Response: 5814
Conc: 1.12 ng/ml

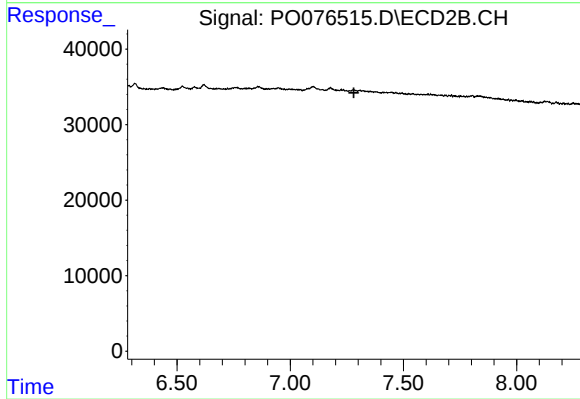

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

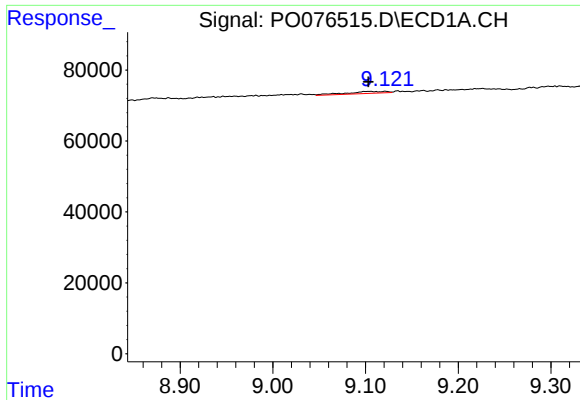

#37 AR-1262-2


R.T.: 9.122 min
Delta R.T.: 0.019 min
Response: 17028
Conc: 1.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

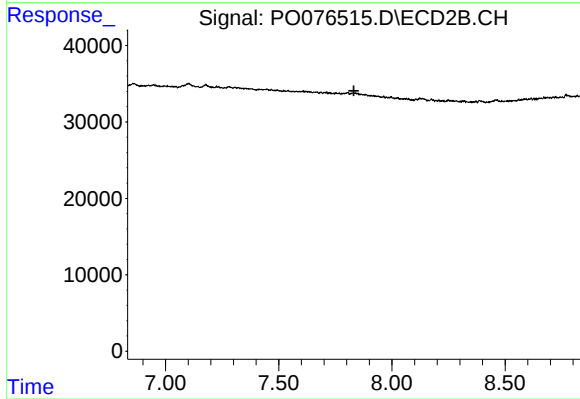


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.832 min
Response: 0
Conc: N.D.

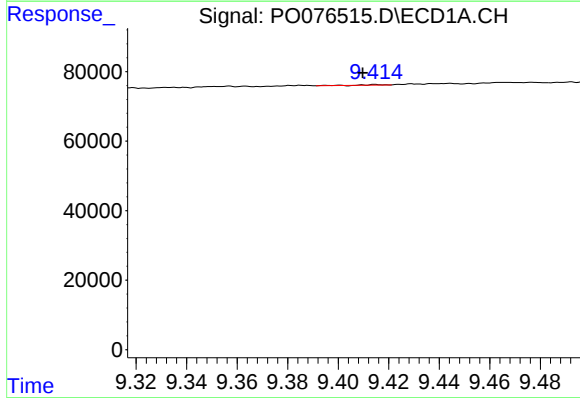


#38 AR-1262-3

R.T.: 9.415 min
Delta R.T.: 0.005 min
Response: 867
Conc: 0.15 ng/ml

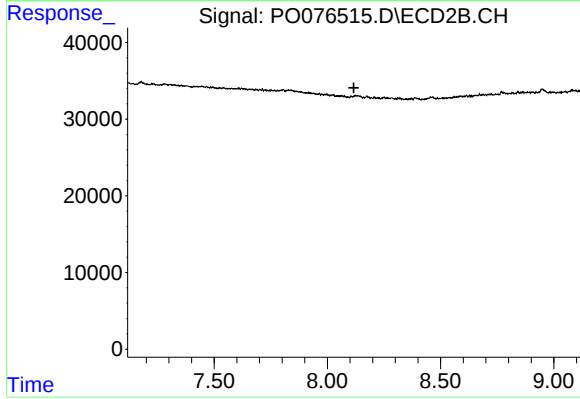

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

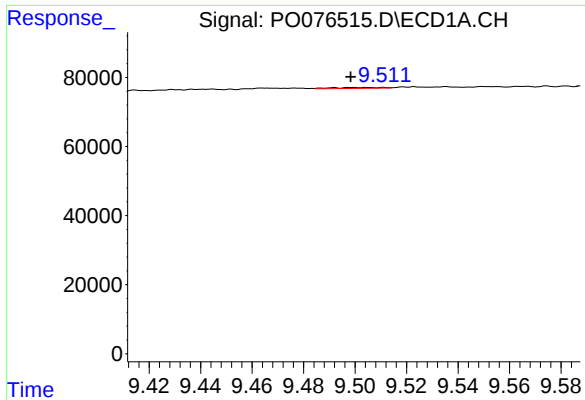

#39 AR-1262-4


R.T.: 9.499 min
Delta R.T.: 0.000 min
Response: 3496
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

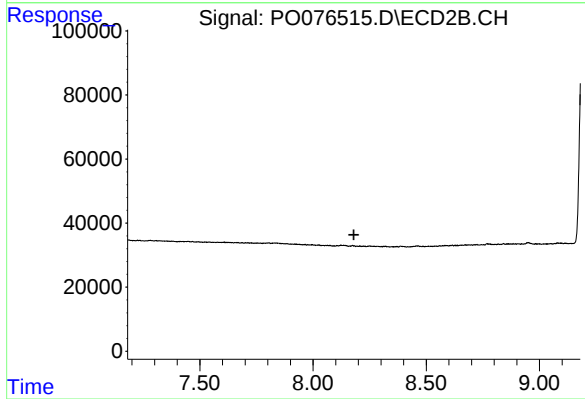


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.180 min
Response: 0
Conc: N.D.

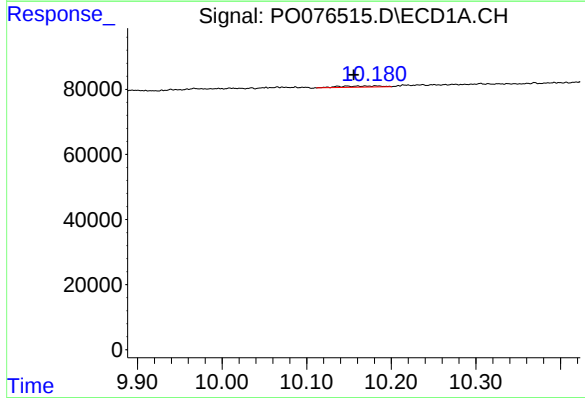


#40 AR-1262-5

R.T.: 10.160 min
Delta R.T.: 0.005 min
Response: 12485
Conc: 4.30 ng/ml

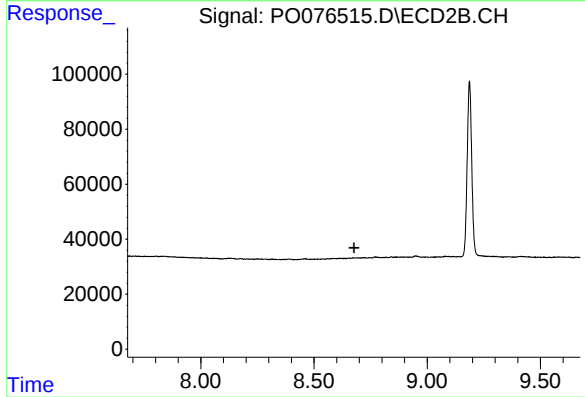

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.677 min
Response: 0
Conc: N.D.

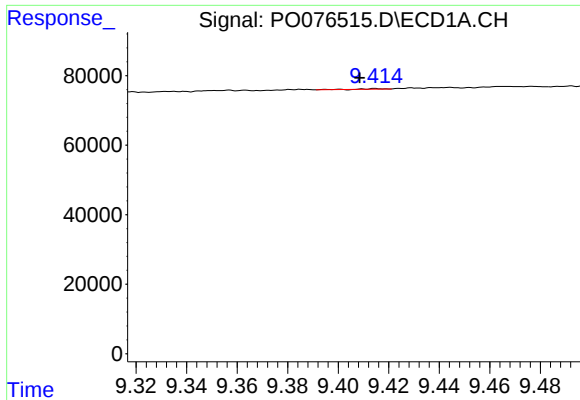

#41 AR-1268-1


R.T.: 9.415 min
Delta R.T.: 0.006 min
Response: 867
Conc: 0.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

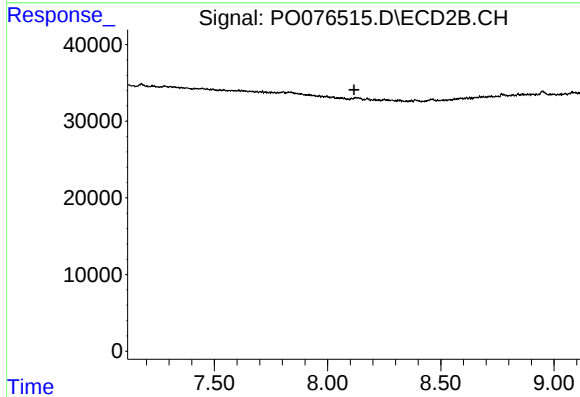


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

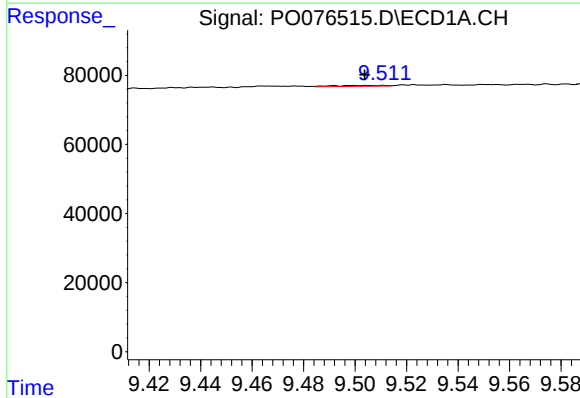


#42 AR-1268-2

R.T.: 9.499 min
Delta R.T.: -0.004 min
Response: 3496
Conc: 0.38 ng/ml

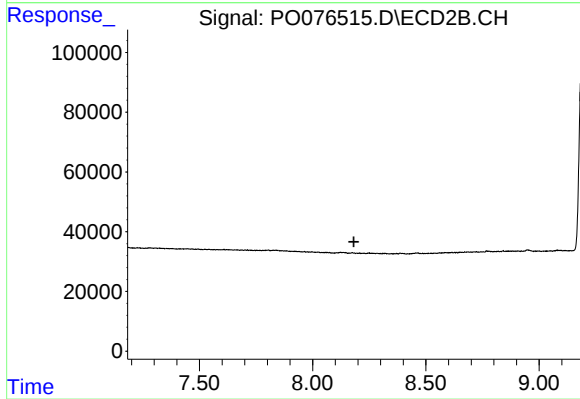

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.182 min
Response: 0
Conc: N.D.

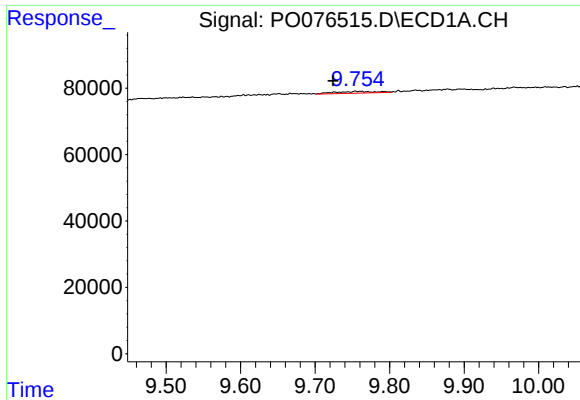

#43 AR-1268-3


R.T.: 9.754 min
Delta R.T.: 0.030 min
Response: 20101
Conc: 2.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

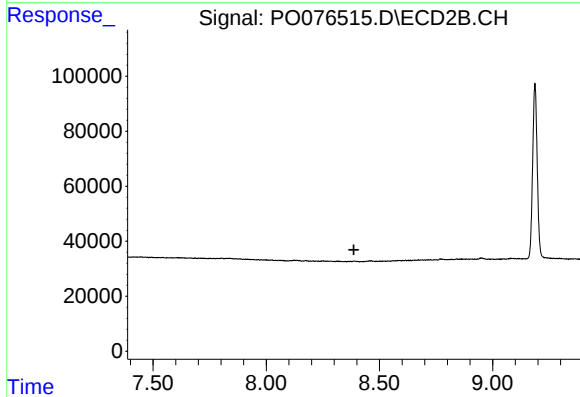


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.387 min
Response: 0
Conc: N.D.

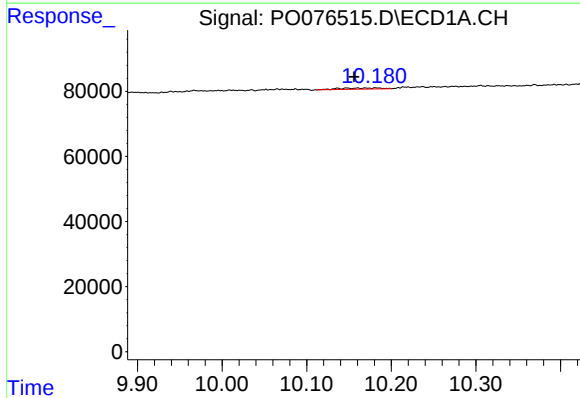


#44 AR-1268-4

R.T.: 10.160 min
Delta R.T.: 0.005 min
Response: 12485
Conc: 3.84 ng/ml

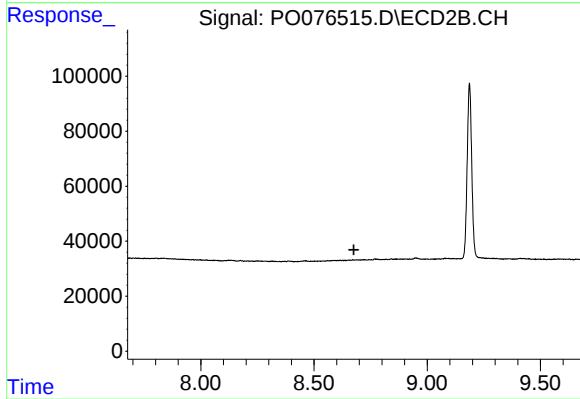

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.676 min
Response: 0
Conc: N.D.

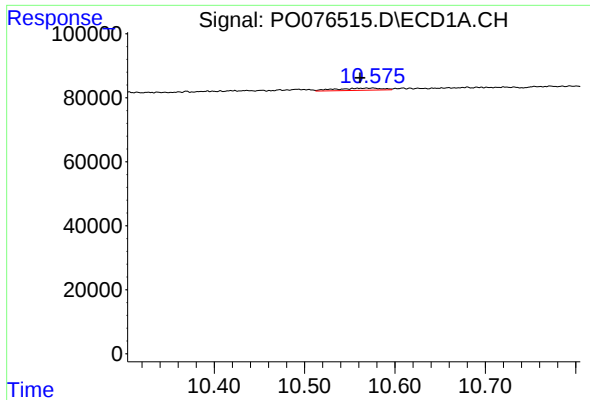

#45 AR-1268-5

R.T.: 10.574 min
Delta R.T.: 0.013 min
Response: 24238
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

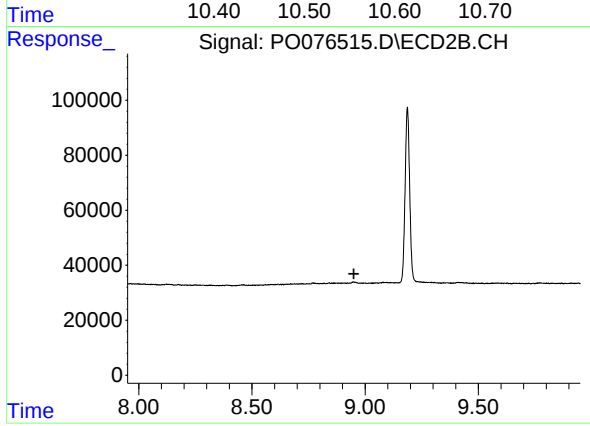

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.950 min
Response: 0
Conc: N.D.