

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076495.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 3:28
 Operator : DD\AJ
 Sample : P0032421ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO032421

Manual Integrations
 APPROVED

Ankita
 3/24/2021 4:00:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:02:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 04:01:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.913	3.928	4968842	2886422	56.735	52.620
2)	SA Decachlor...	10.887	9.186	3544027	2421520	54.444	51.389
Target Compounds							
3)	L1 AR-1016-1	6.235	5.177	1487578	819172	550.442	497.364
4)	L1 AR-1016-2	6.259	5.196	2341110	1506625	569.490	519.168
5)	L1 AR-1016-3	6.324	5.387	1375278	687549	569.980m	514.940
6)	L1 AR-1016-4	6.432	5.437	1109251	628320	572.312	559.756
7)	L1 AR-1016-5	6.745	5.664	1109265	759733	569.523m	551.733
31)	L7 AR-1260-1	7.920	6.754	1952076	1390163	568.062m	542.423
32)	L7 AR-1260-2	8.185	6.951	2293855	1705959	565.744	550.079
33)	L7 AR-1260-3	8.551	7.104	1730674	1579529	572.855m	537.666
34)	L7 AR-1260-4	8.782	7.585	1976447	1311080	567.159	550.105
35)	L7 AR-1260-5	9.104	7.832	3797246	3029185	561.902	533.934

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032421\
Data File : PO076495.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 3:28
Operator : DD\AJ
Sample : PO032421ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:02:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 04:01:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

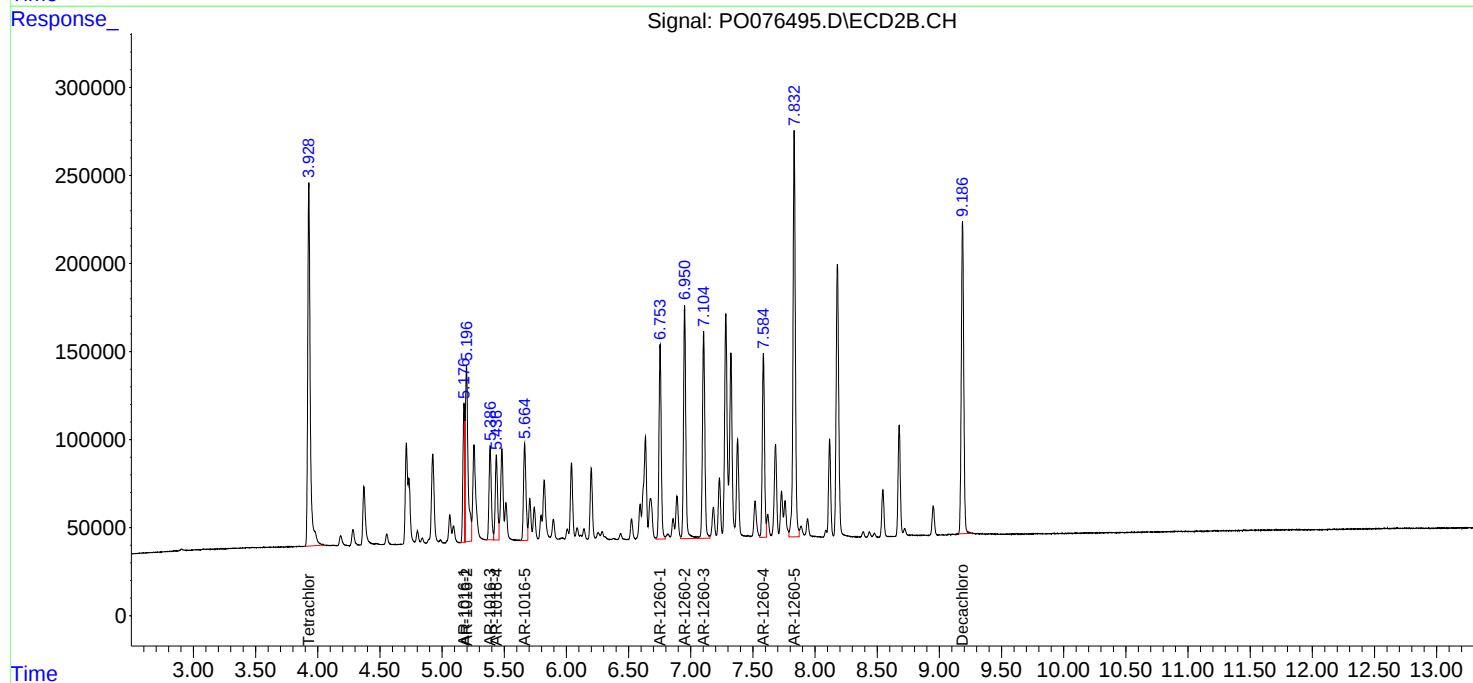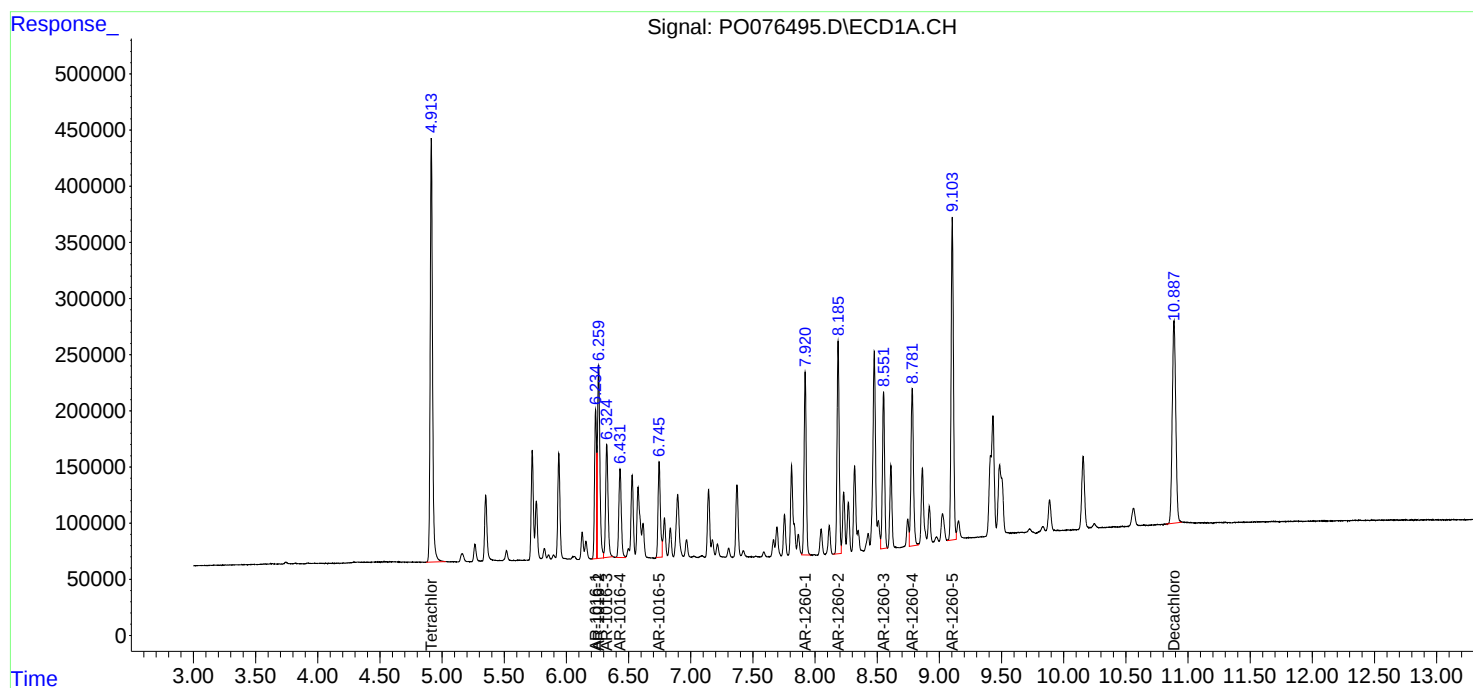

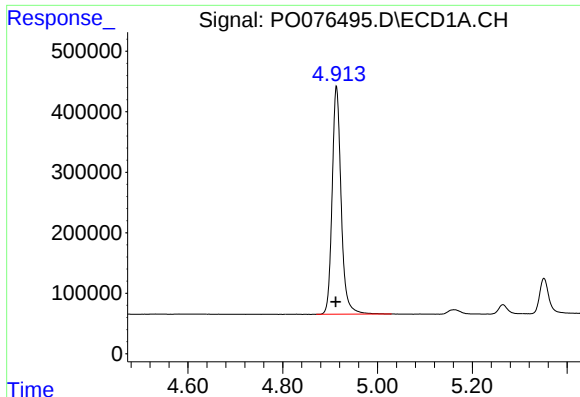


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.001 min
Response: 4968842
Conc: 56.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

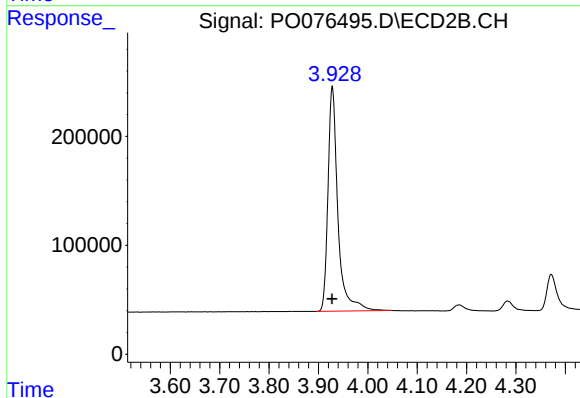


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 2886422
Conc: 52.62 ng/ml

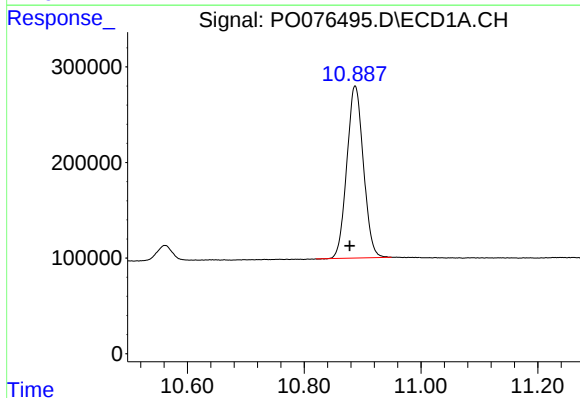


#2 Decachlorobiphenyl

R.T.: 10.887 min
Delta R.T.: 0.009 min
Response: 3544027
Conc: 54.44 ng/ml

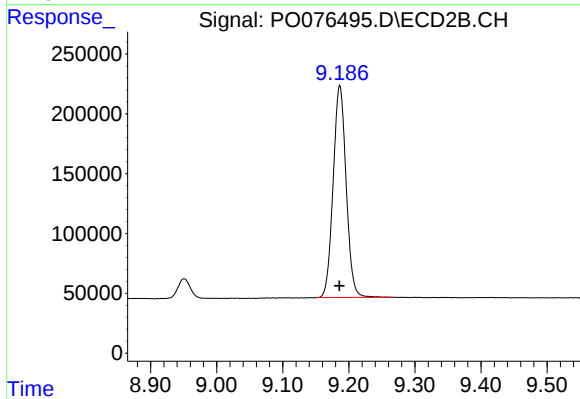

#2 Decachlorobiphenyl

R.T.: 9.186 min
Delta R.T.: 0.000 min
Response: 2421520
Conc: 51.39 ng/ml

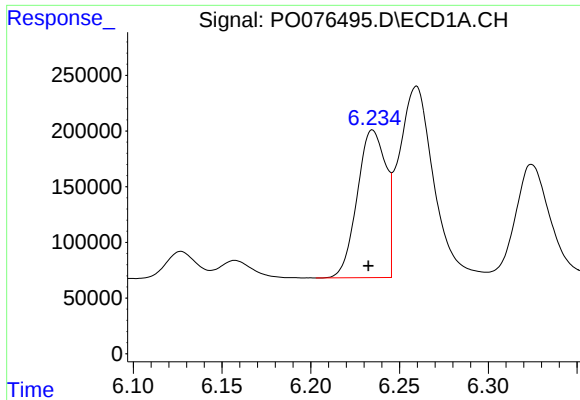


#3 AR-1016-1

R.T.: 6.235 min
Delta R.T.: 0.003 min
Response: 1487578
Conc: 550.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

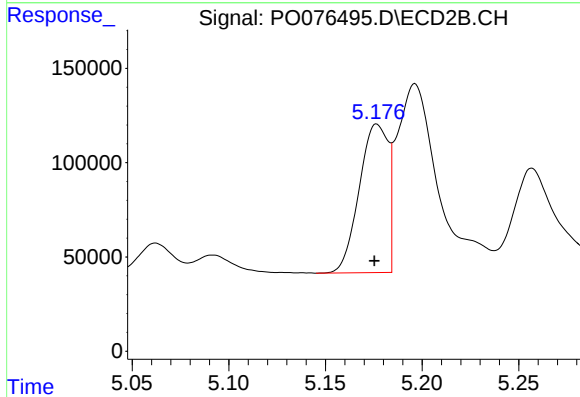


#3 AR-1016-1

R.T.: 5.177 min
Delta R.T.: 0.001 min
Response: 819172
Conc: 497.36 ng/ml

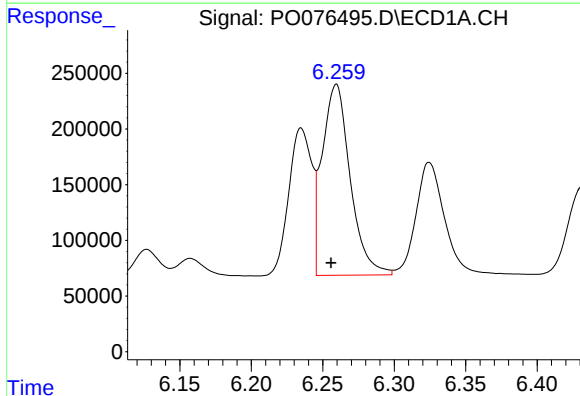


#4 AR-1016-2

R.T.: 6.259 min
Delta R.T.: 0.004 min
Response: 2341110
Conc: 569.49 ng/ml

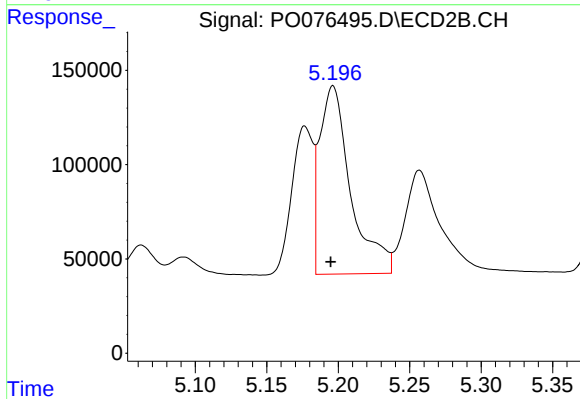

#4 AR-1016-2

R.T.: 5.196 min
Delta R.T.: 0.001 min
Response: 1506625
Conc: 519.17 ng/ml

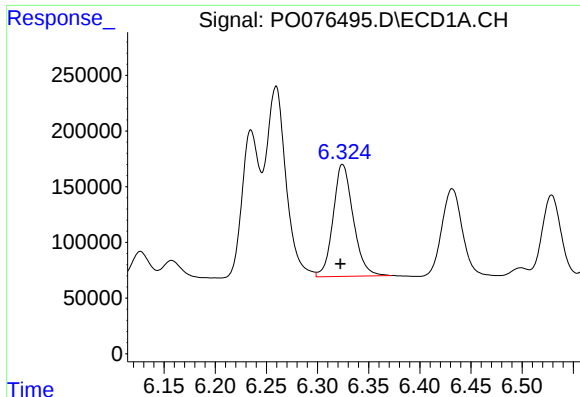


#5 AR-1016-3

R.T.: 6.324 min
Delta R.T.: 0.002 min
Response: 1375278
Conc: 569.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

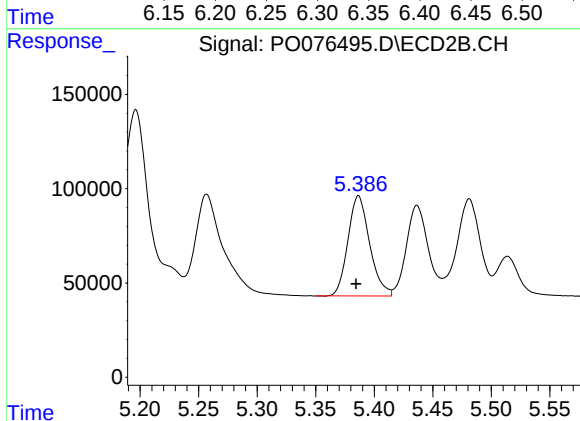


#5 AR-1016-3

R.T.: 5.387 min
Delta R.T.: 0.002 min
Response: 687549
Conc: 514.94 ng/ml

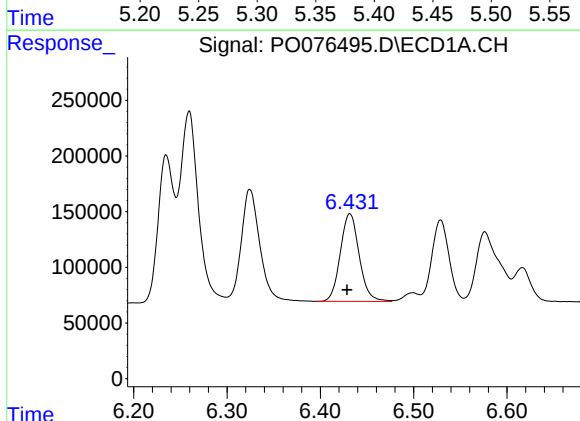


#6 AR-1016-4

R.T.: 6.432 min
Delta R.T.: 0.003 min
Response: 1109251
Conc: 572.31 ng/ml

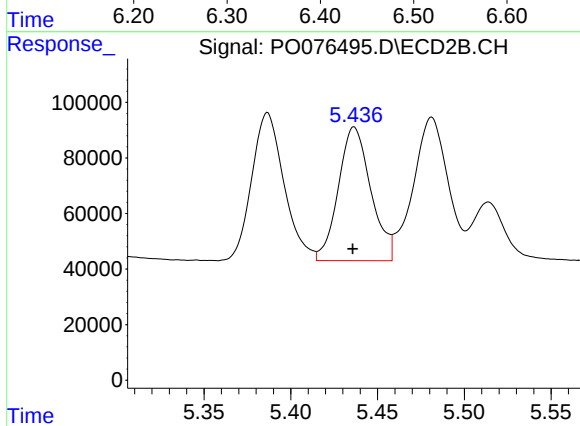

#6 AR-1016-4

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 628320
Conc: 559.76 ng/ml

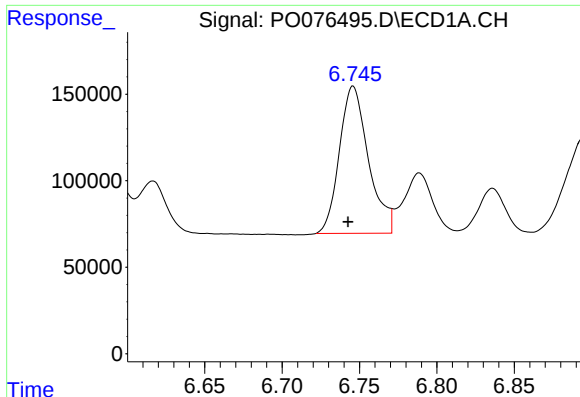


#7 AR-1016-5

R.T.: 6.745 min
Delta R.T.: 0.003 min
Response: 1109265
Conc: 569.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

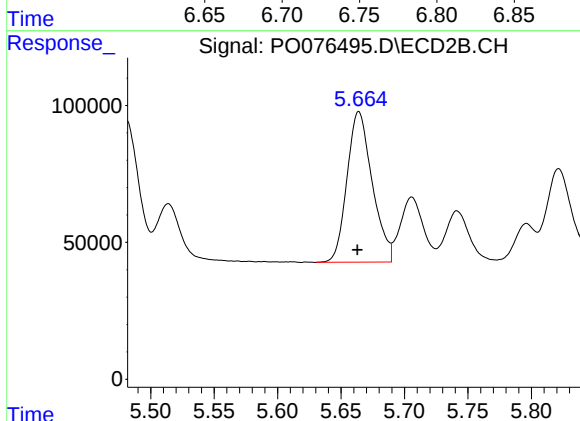


#7 AR-1016-5

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 759733
Conc: 551.73 ng/ml

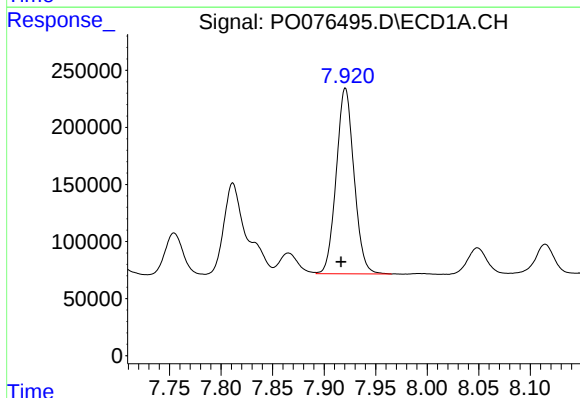


#31 AR-1260-1

R.T.: 7.920 min
Delta R.T.: 0.004 min
Response: 1952076
Conc: 568.06 ng/ml m

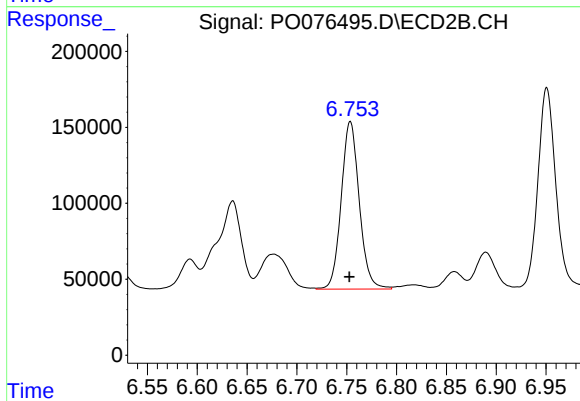

#31 AR-1260-1

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 1390163
Conc: 542.42 ng/ml

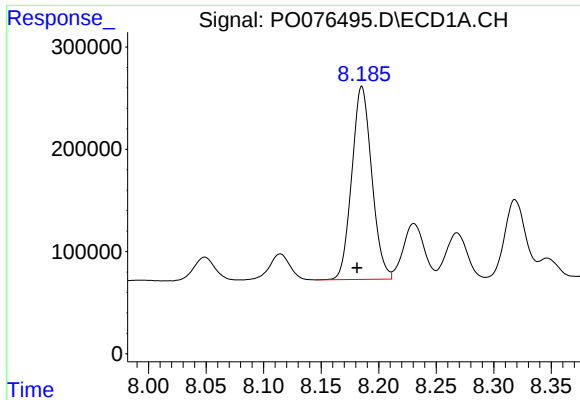


#32 AR-1260-2

R.T.: 8.185 min
Delta R.T.: 0.004 min
Response: 2293855
Conc: 565.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

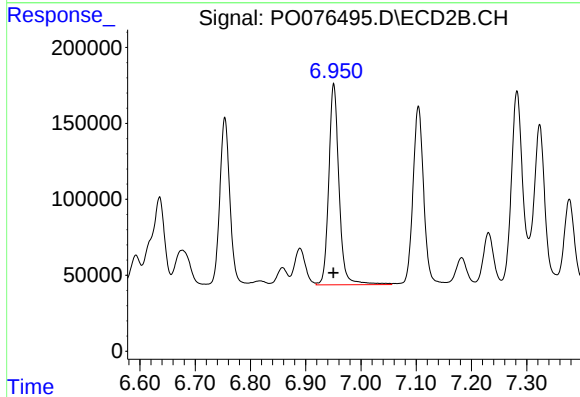


#32 AR-1260-2

R.T.: 6.951 min
Delta R.T.: 0.000 min
Response: 1705959
Conc: 550.08 ng/ml

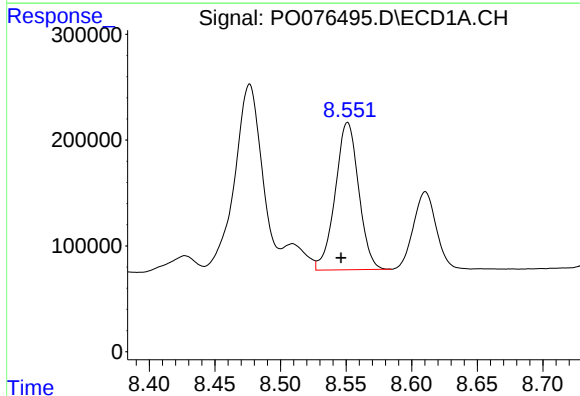


#33 AR-1260-3

R.T.: 8.551 min
Delta R.T.: 0.005 min
Response: 1730674
Conc: 572.86 ng/ml m

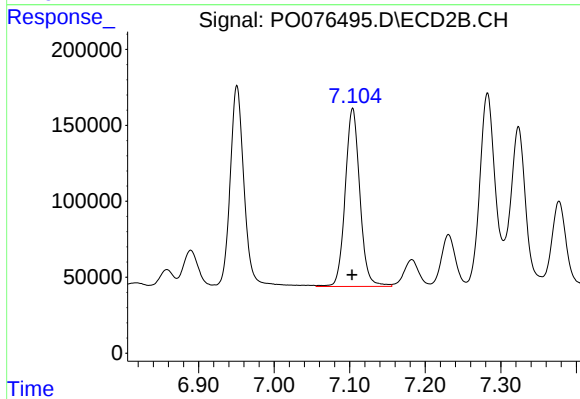

#33 AR-1260-3

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 1579529
Conc: 537.67 ng/ml

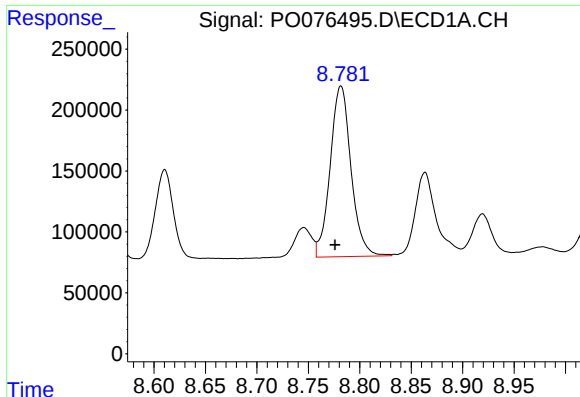


#34 AR-1260-4

R.T.: 8.782 min
Delta R.T.: 0.006 min
Response: 1976447
Conc: 567.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:25 PM

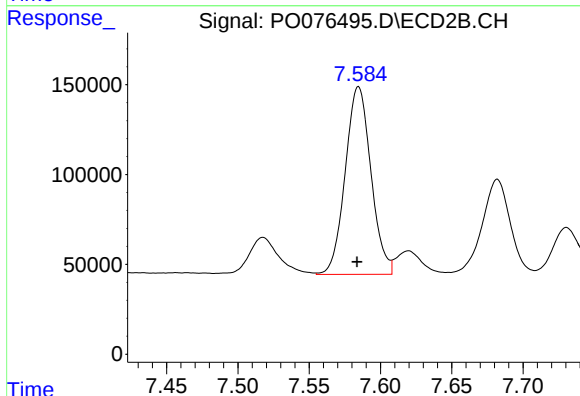


#34 AR-1260-4

R.T.: 7.585 min
Delta R.T.: 0.000 min
Response: 1311080
Conc: 550.11 ng/ml

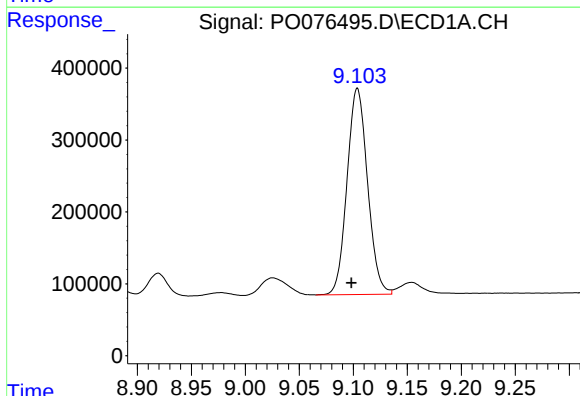

#35 AR-1260-5

R.T.: 9.104 min
Delta R.T.: 0.006 min
Response: 3797246
Conc: 561.90 ng/ml

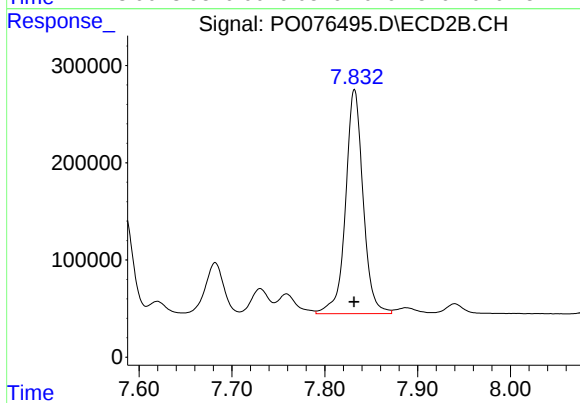

#35 AR-1260-5

R.T.: 7.832 min
Delta R.T.: 0.000 min
Response: 3029185
Conc: 533.93 ng/ml