

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076499.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 4:36
 Operator : DD\AJ
 Sample : AR1262ICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO032421AR1262

Manual Integrations
 APPROVED

Ankita
 3/24/2021 3:59:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 05:32:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:31:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.928	5200453	2982359	53.305	51.473
2) SA Decachlor...	10.889	9.187	3666495	2506324	51.896	50.794
Target Compounds						
36) L8 AR-1262-1	8.551	7.282	2686127	999748	519.167	508.392
37) L8 AR-1262-2	9.104	7.833	4524243	3459197	524.980	514.539
38) L8 AR-1262-3	9.410	8.117	2999295	1377047	529.033	511.264
39) L8 AR-1262-4	9.501	8.181	2243619	2553475	521.165m	513.105
40) L8 AR-1262-5	10.157	8.677	1519924	1141091	523.106	525.192

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032421\
Data File : P0076499.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 4:36
Operator : DD\AJ
Sample : AR1262ICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO032421AR1262


Manual Integrations
APPROVED

Ankita
3/24/2021 3:59:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 05:32:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:31:56 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

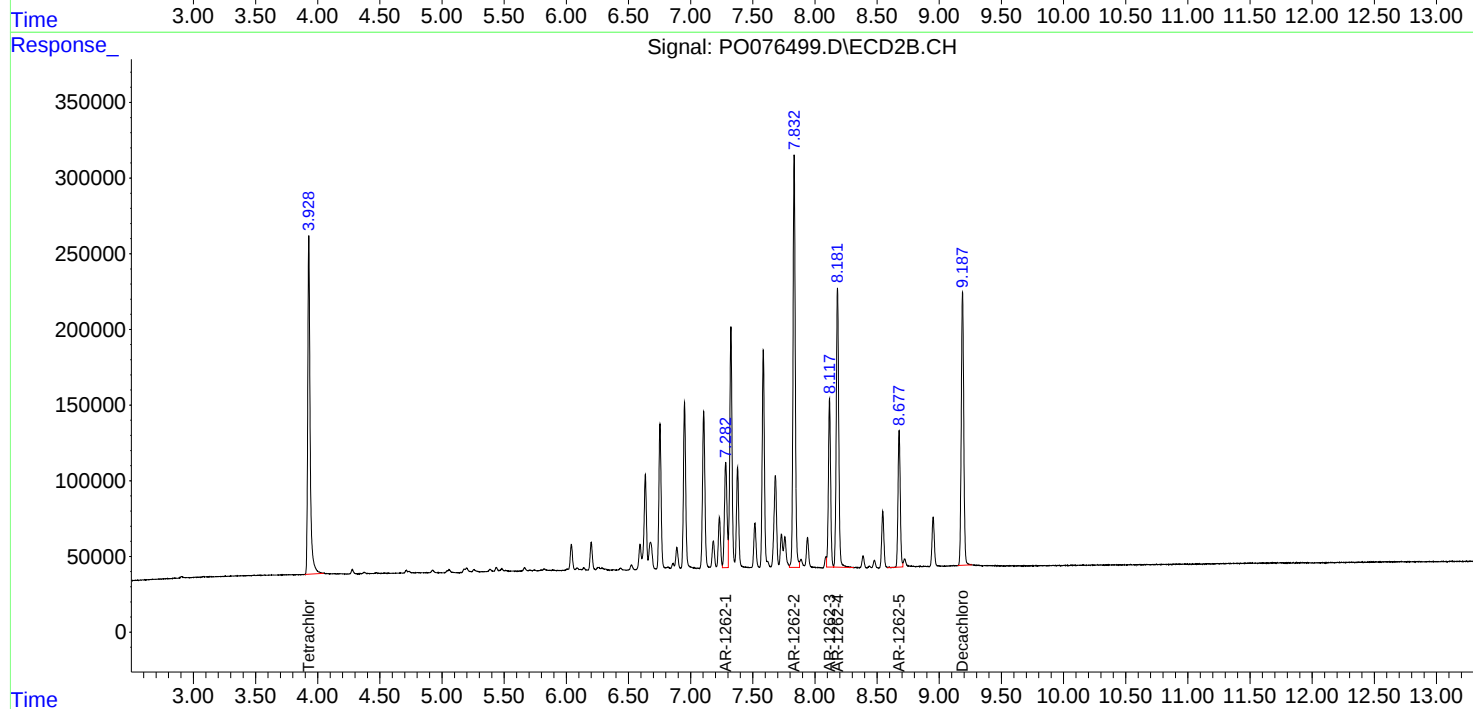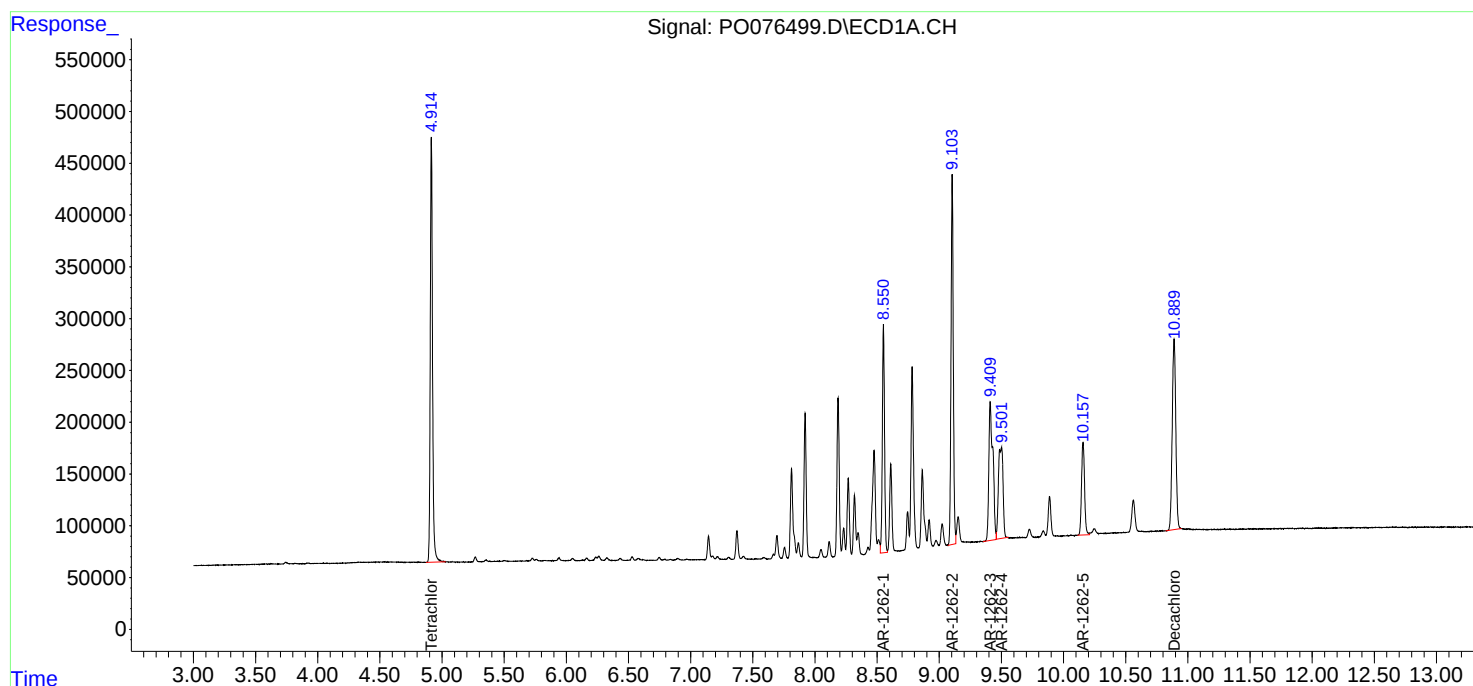

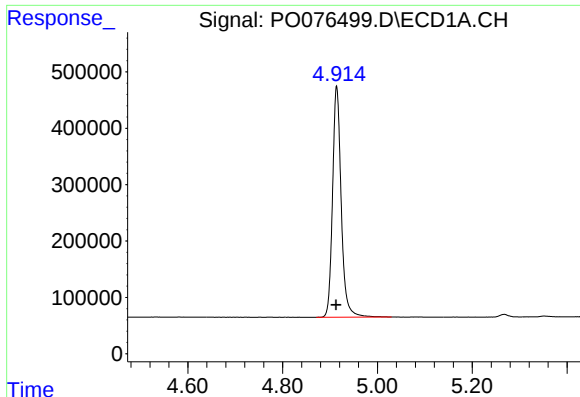


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 5200453
Conc: 53.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421AR1262


Manual Integrations
APPROVED

Ankita
3/24/2021 3:59:48 PM

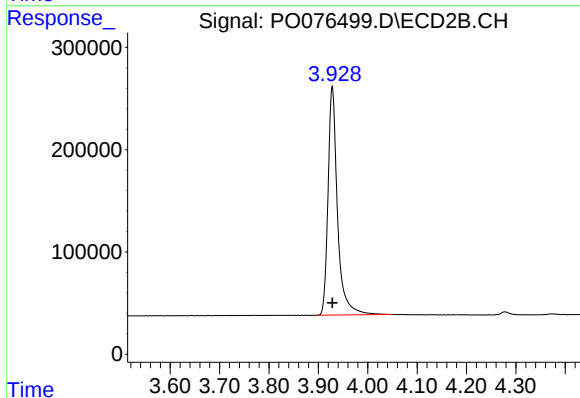


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 2982359
Conc: 51.47 ng/ml

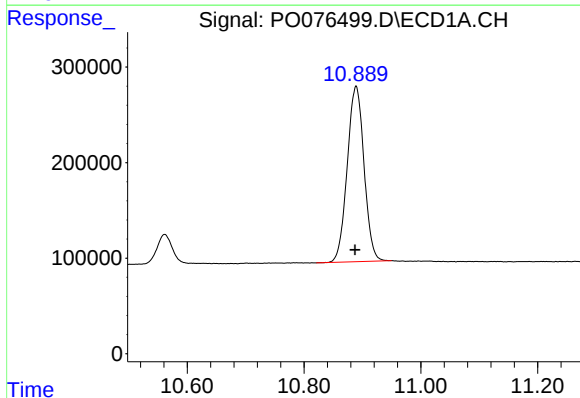


#2 Decachlorobiphenyl

R.T.: 10.889 min
Delta R.T.: 0.002 min
Response: 3666495
Conc: 51.90 ng/ml

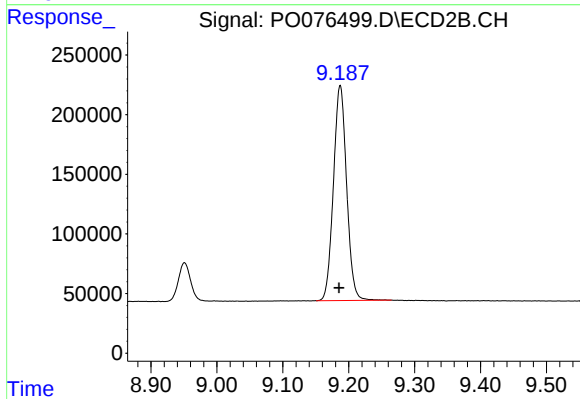

#2 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: 0.002 min
Response: 2506324
Conc: 50.79 ng/ml

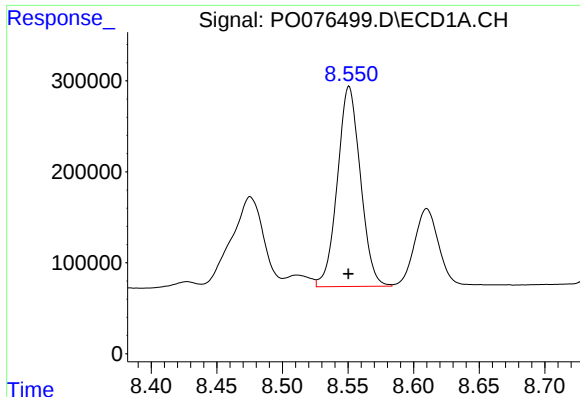


#36 AR-1262-1

R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 2686127
Conc: 519.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421AR1262


Manual Integrations
APPROVED

Ankita
3/24/2021 3:59:48 PM

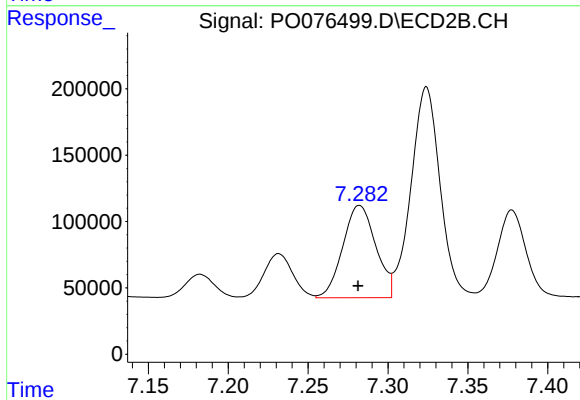


#36 AR-1262-1

R.T.: 7.282 min
Delta R.T.: 0.000 min
Response: 999748
Conc: 508.39 ng/ml

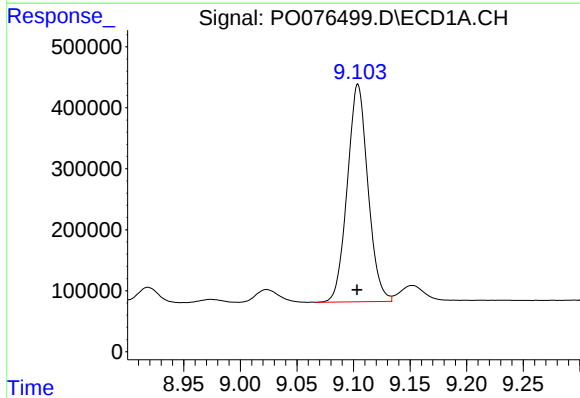


#37 AR-1262-2

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 4524243
Conc: 524.98 ng/ml

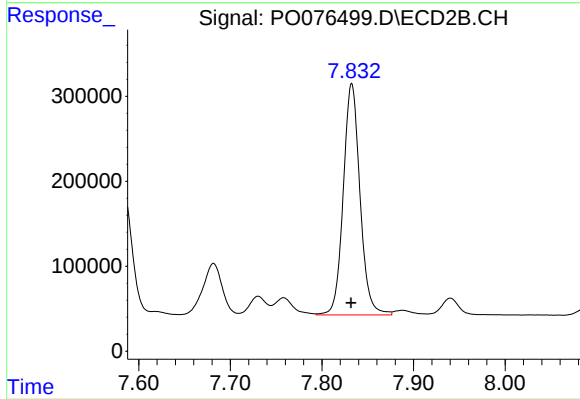

#37 AR-1262-2

R.T.: 7.833 min
Delta R.T.: 0.000 min
Response: 3459197
Conc: 514.54 ng/ml

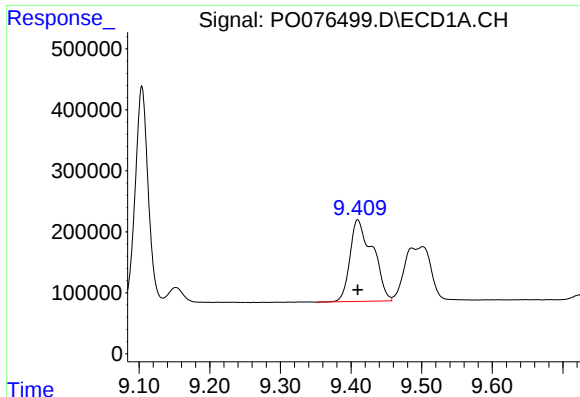


#38 AR-1262-3

R.T.: 9.410 min
Delta R.T.: 0.000 min
Response: 2999295
Conc: 529.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421AR1262


Manual Integrations
APPROVED

Ankita
3/24/2021 3:59:48 PM

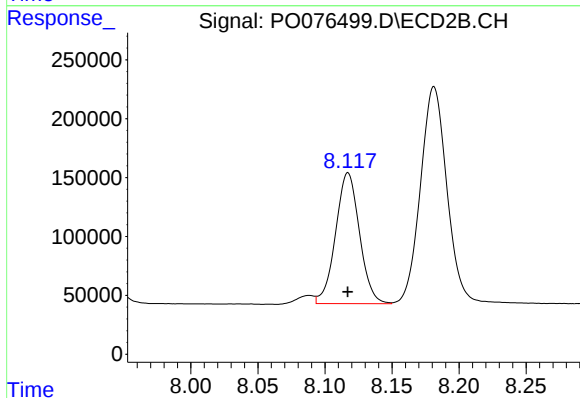


#38 AR-1262-3

R.T.: 8.117 min
Delta R.T.: 0.000 min
Response: 1377047
Conc: 511.26 ng/ml

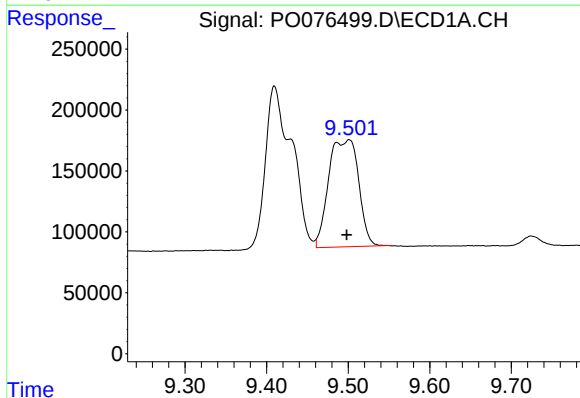


#39 AR-1262-4

R.T.: 9.501 min
Delta R.T.: 0.002 min
Response: 2243619
Conc: 521.17 ng/ml m

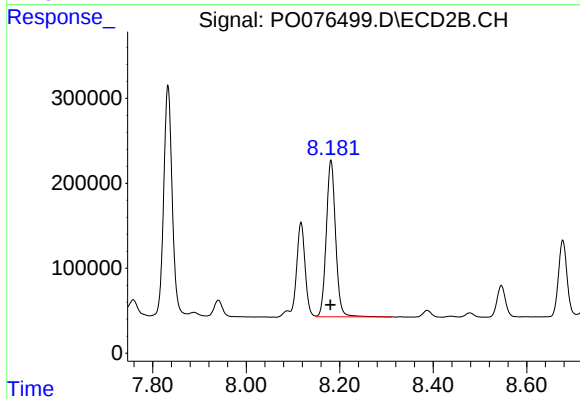

#39 AR-1262-4

R.T.: 8.181 min
Delta R.T.: 0.000 min
Response: 2553475
Conc: 513.10 ng/ml

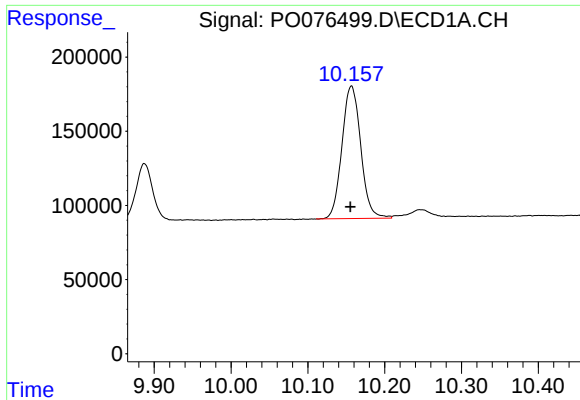


#40 AR-1262-5

R.T.: 10.157 min
Delta R.T.: 0.001 min
Response: 1519924
Conc: 523.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO032421AR1262

Manual Integrations
APPROVED

Ankita
3/24/2021 3:59:48 PM

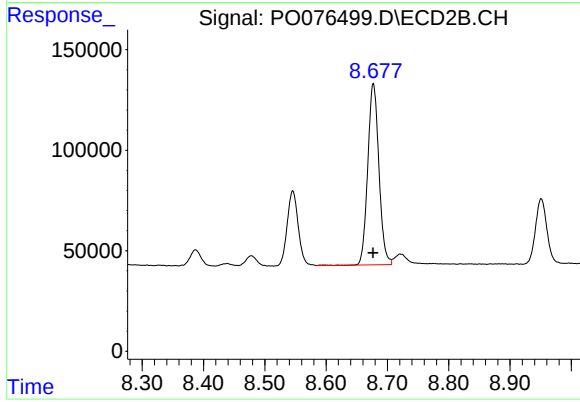

#40 AR-1262-5

R.T.: 8.677 min
Delta R.T.: 0.000 min
Response: 1141091
Conc: 525.19 ng/ml