

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032421\
 Data File : P0076518.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 10:03
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Manual Integrations
 APPROVED

Ankita
 3/24/2021 4:00:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 14:21:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.915	3.930	1589378	944385	18.148	17.216
2)	SA Decachlor...	10.888	9.186	1270136	904333	19.512	19.191
Target Compounds							
26)	L6 AR-1254-1	7.145	6.041	148948	129538	44.844	43.734
27)	L6 AR-1254-2	7.374	6.201	230533	115176	44.790	44.330
28)	L6 AR-1254-3	7.756	6.618	229602	170145	43.164	42.481
29)	L6 AR-1254-4	8.052	6.859	149403	90849	41.423	38.342m
30)	L6 AR-1254-5	8.479	7.283	181196	145479	46.226	41.276

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032421\
Data File : PO076518.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 10:03
Operator : DD\AJ
Sample : M1458-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 14:21:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

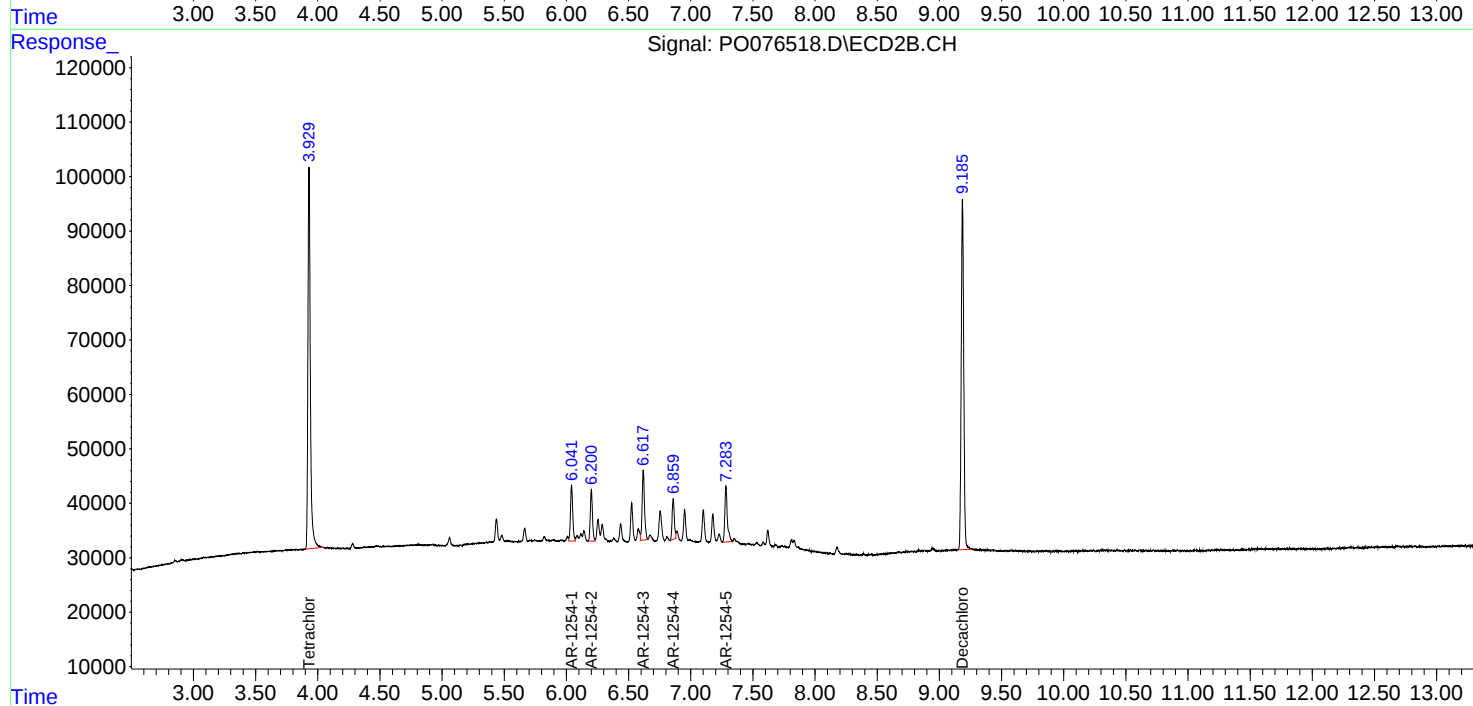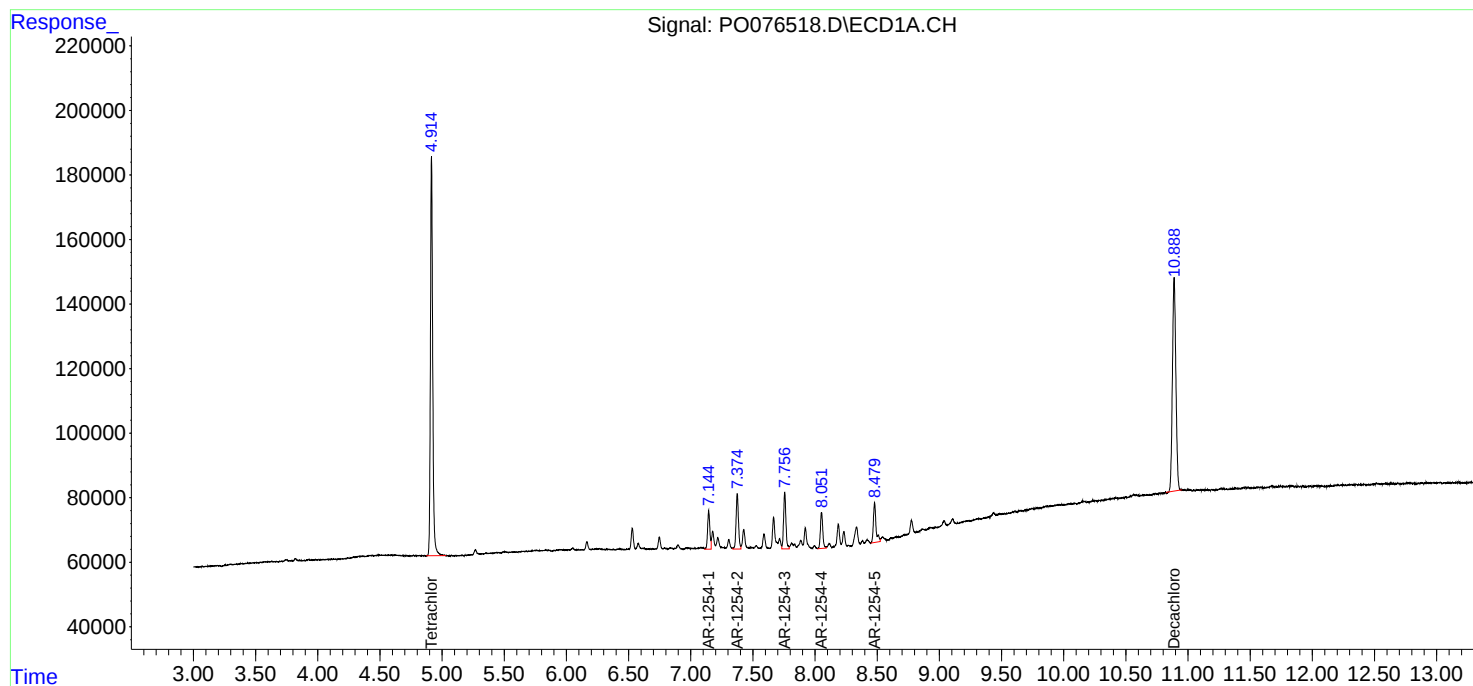

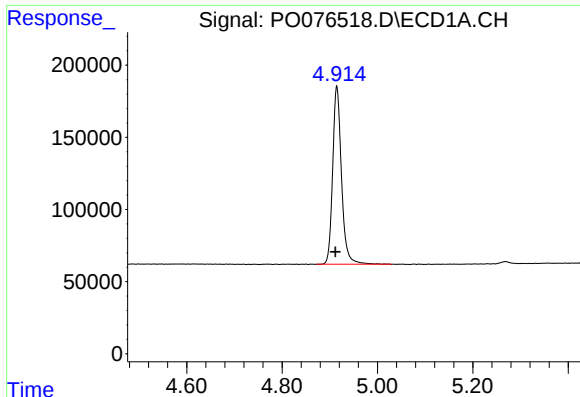


#1 Tetrachloro-m-xylene

R.T.: 4.915 min
Delta R.T.: 0.003 min
Response: 1589378
Conc: 18.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:11 PM

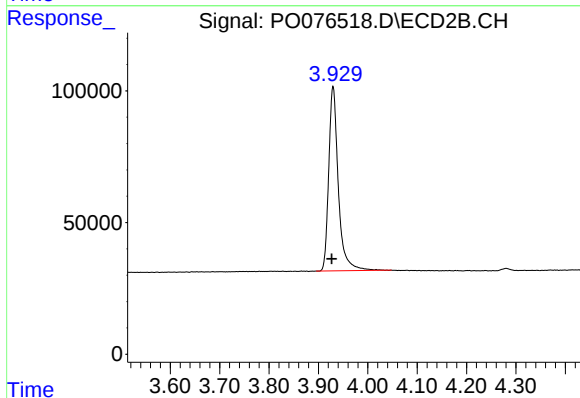


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.002 min
Response: 944385
Conc: 17.22 ng/ml

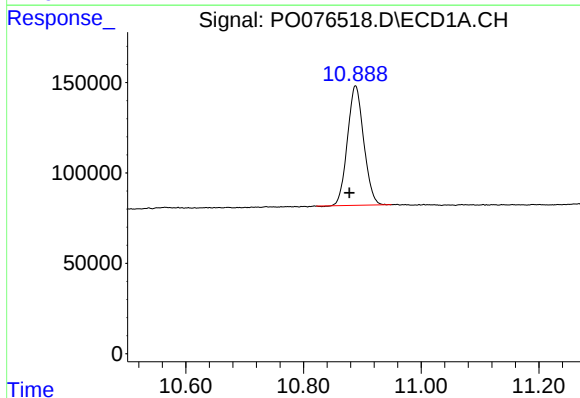


#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.010 min
Response: 1270136
Conc: 19.51 ng/ml

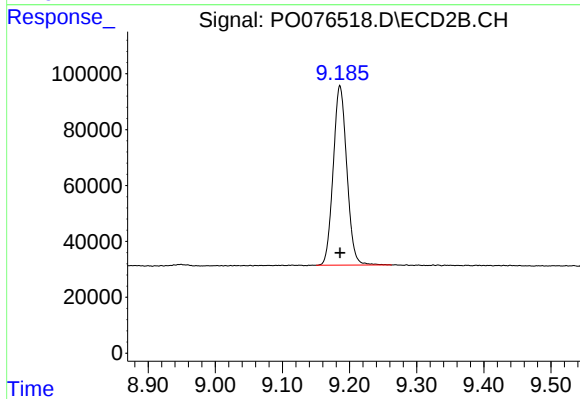

#2 Decachlorobiphenyl

R.T.: 9.186 min
Delta R.T.: 0.000 min
Response: 904333
Conc: 19.19 ng/ml

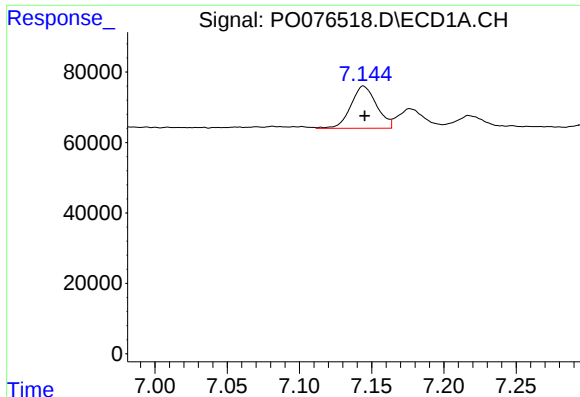


#26 AR-1254-1

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 148948
Conc: 44.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:11 PM

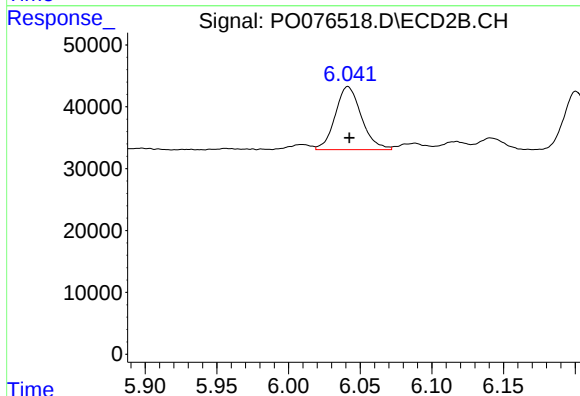


#26 AR-1254-1

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 129538
Conc: 43.73 ng/ml

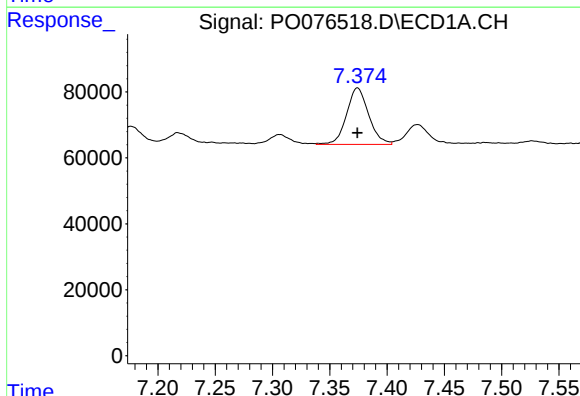


#27 AR-1254-2

R.T.: 7.374 min
Delta R.T.: 0.000 min
Response: 230533
Conc: 44.79 ng/ml

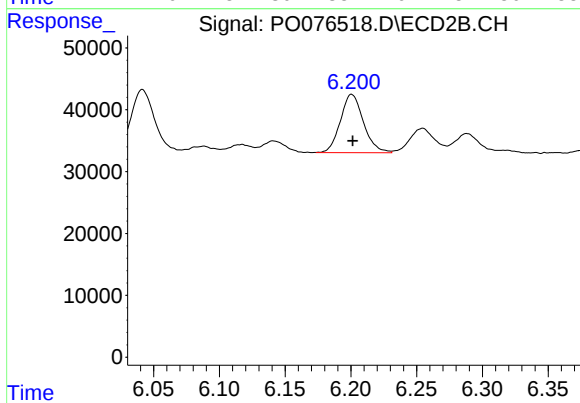

#27 AR-1254-2

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 115176
Conc: 44.33 ng/ml

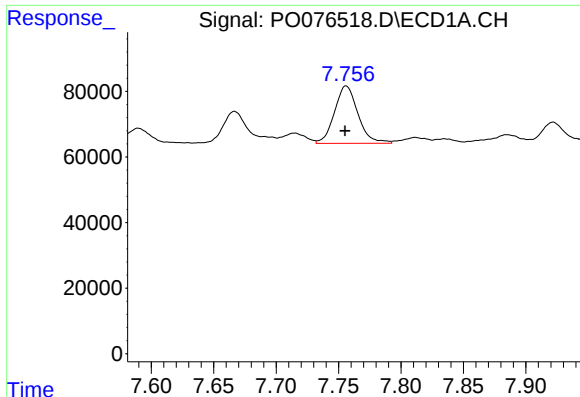


#28 AR-1254-3

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 229602
Conc: 43.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:11 PM

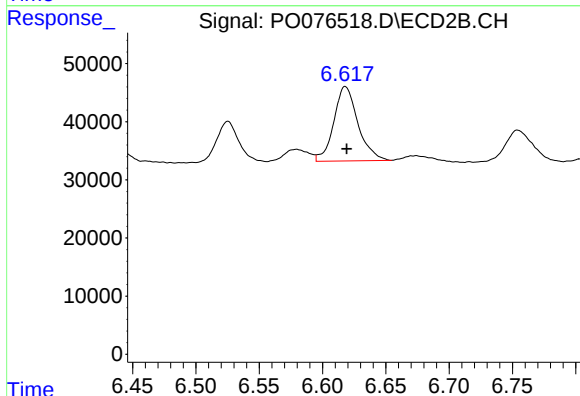


#28 AR-1254-3

R.T.: 6.618 min
Delta R.T.: -0.001 min
Response: 170145
Conc: 42.48 ng/ml

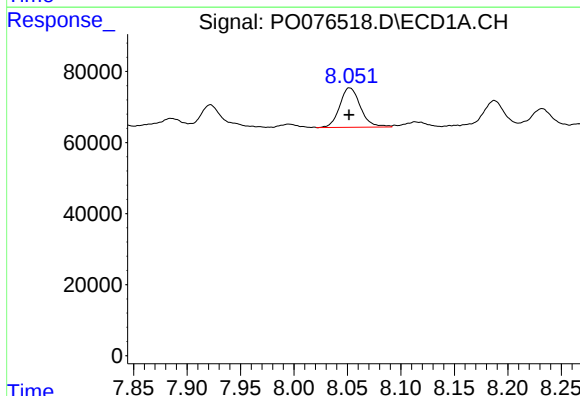


#29 AR-1254-4

R.T.: 8.052 min
Delta R.T.: 0.000 min
Response: 149403
Conc: 41.42 ng/ml

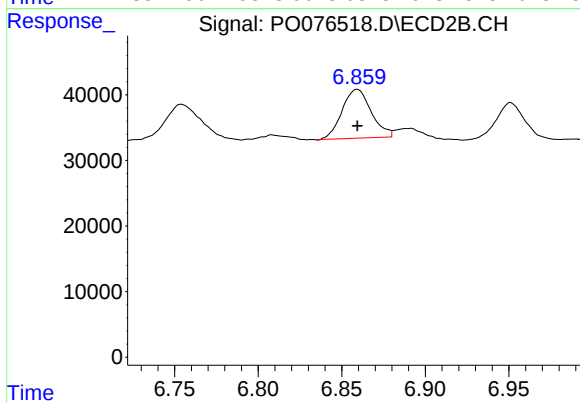

#29 AR-1254-4

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 90849
Conc: 38.34 ng/ml m

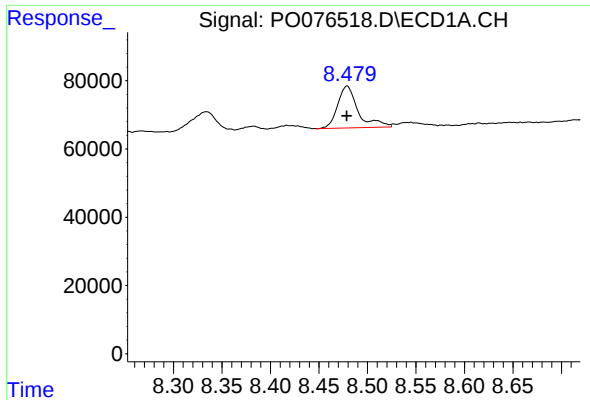


#30 AR-1254-5

R.T.: 8.479 min
Delta R.T.: 0.000 min
Response: 181196
Conc: 46.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Manual Integrations
APPROVED

Ankita
3/24/2021 4:00:11 PM

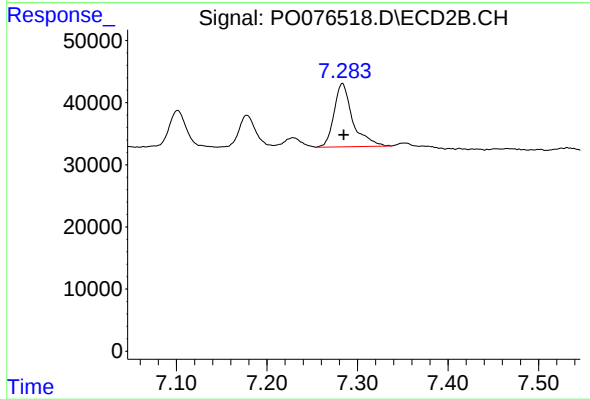

#30 AR-1254-5

R.T.: 7.283 min
Delta R.T.: -0.002 min
Response: 145479
Conc: 41.28 ng/ml