

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032422\
 Data File : P0085600.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2022 14:14
 Operator : YP\AJ
 Sample : N2084-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 BLDG-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:26:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.499	3.591	3065056	806642	14.990m	18.828 #
2) SA Decachlor...	10.411	8.612	2856770	692289	23.766	18.032
Target Compounds						
41) L9 AR-1268-1	8.827	7.513	620288	207515	32.140m	31.246
42) L9 AR-1268-2	8.925	7.577	611445	200451	35.190	34.010
43) L9 AR-1268-3	9.166	7.784	182541	54742	12.368	11.018
44) L9 AR-1268-4	9.613	8.073	445299	116553	72.982	54.923
45) L9 AR-1268-5	10.052	8.360	784318	200005	16.247	14.281

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032422\
Data File : PO085600.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2022 14:14
Operator : YP\AJ
Sample : N2084-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BLDG-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:26:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

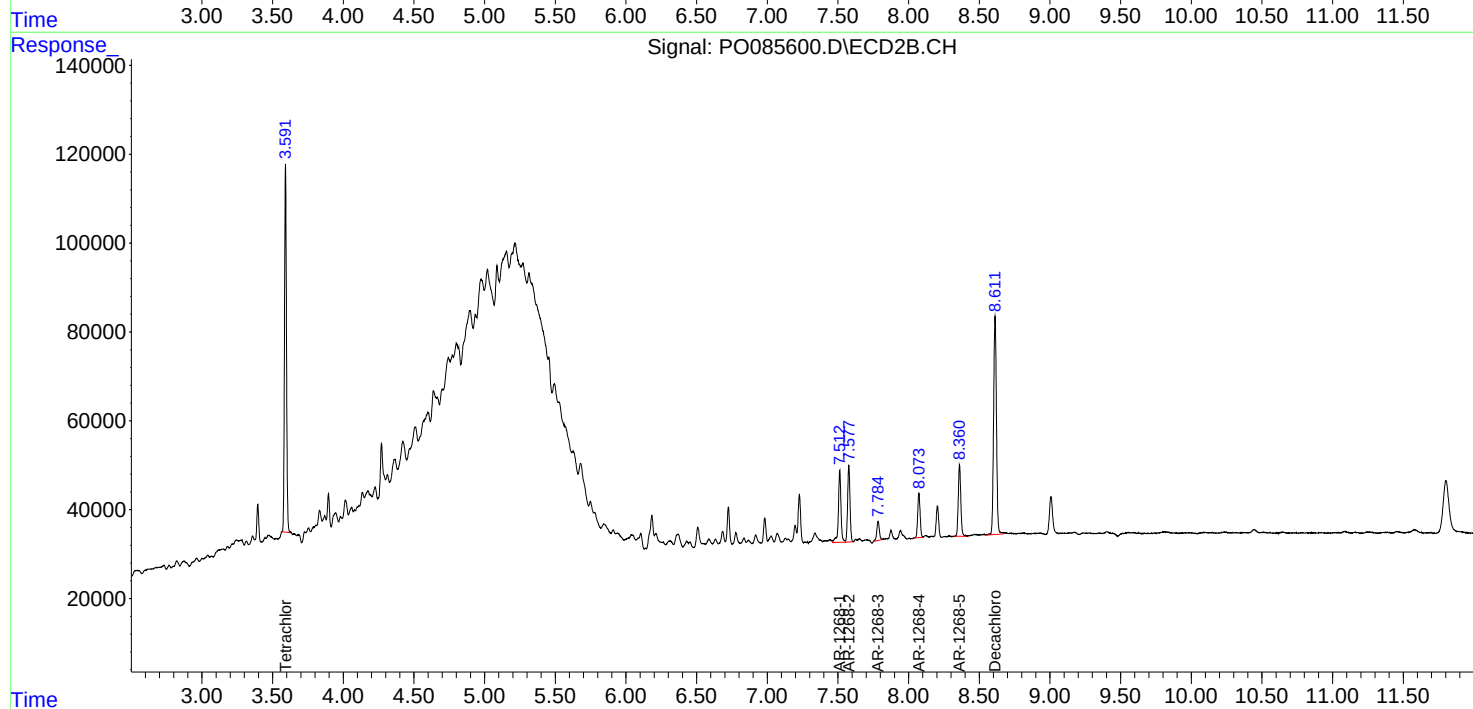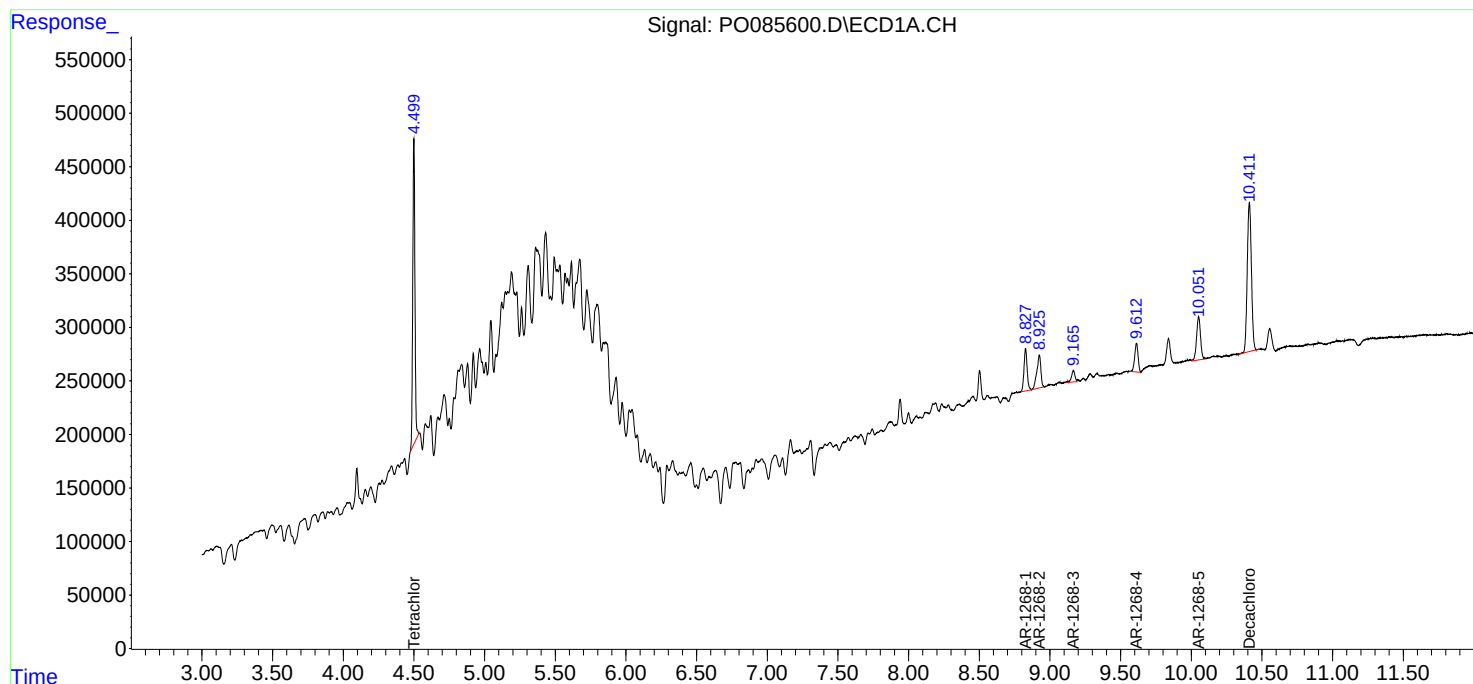

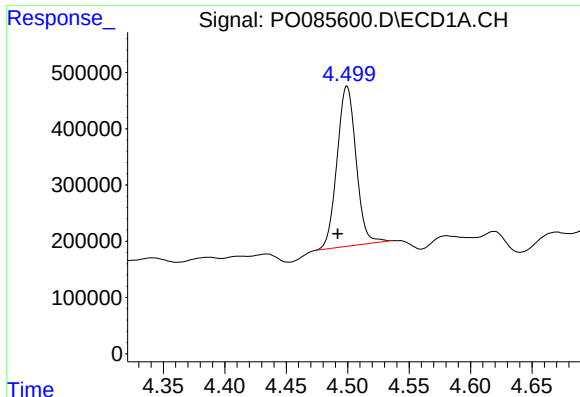


#1 Tetrachloro-m-xylene

R.T.: 4.499 min
Delta R.T.: 0.007 min
Response: 3065056
Conc: 14.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLDG-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

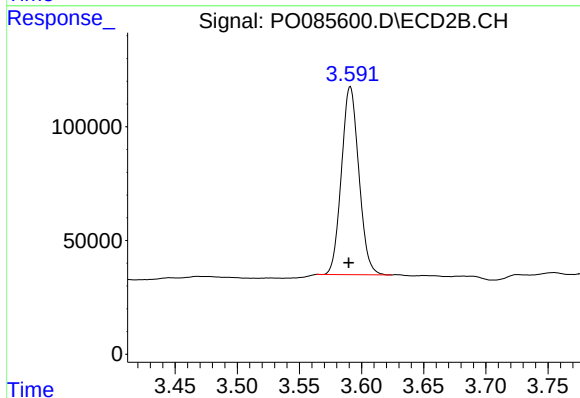


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: 0.001 min
Response: 806642
Conc: 18.83 ng/ml

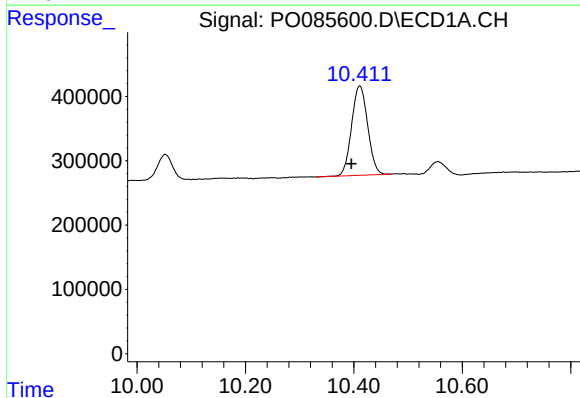


#2 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: 0.015 min
Response: 2856770
Conc: 23.77 ng/ml

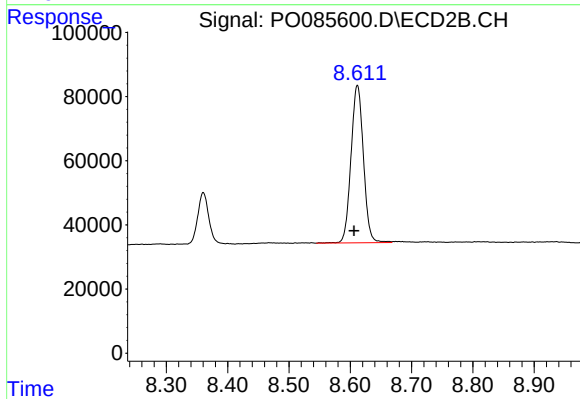

#2 Decachlorobiphenyl

R.T.: 8.612 min
Delta R.T.: 0.005 min
Response: 692289
Conc: 18.03 ng/ml

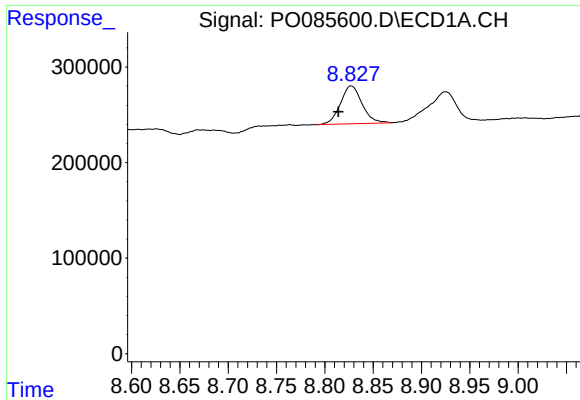


#41 AR-1268-1

R.T.: 8.827 min
Delta R.T.: 0.013 min
Response: 620288
Conc: 32.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLDG-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

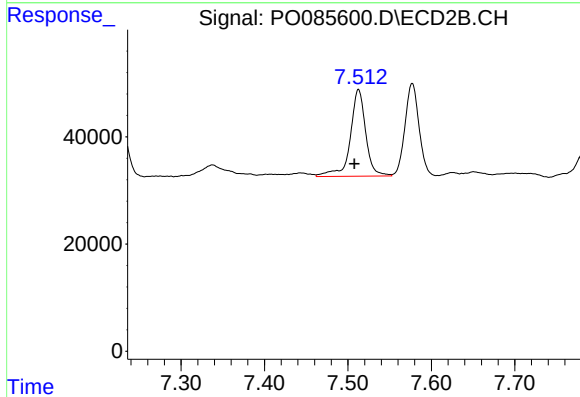


#41 AR-1268-1

R.T.: 7.513 min
Delta R.T.: 0.005 min
Response: 207515
Conc: 31.25 ng/ml

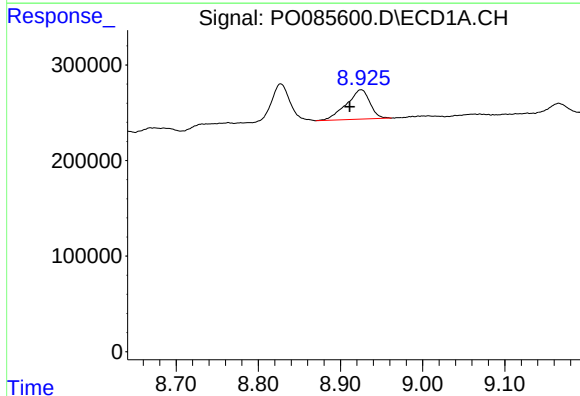


#42 AR-1268-2

R.T.: 8.925 min
Delta R.T.: 0.014 min
Response: 611445
Conc: 35.19 ng/ml

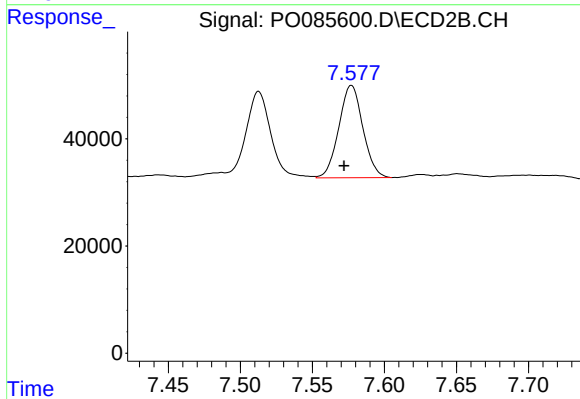

#42 AR-1268-2

R.T.: 7.577 min
Delta R.T.: 0.005 min
Response: 200451
Conc: 34.01 ng/ml

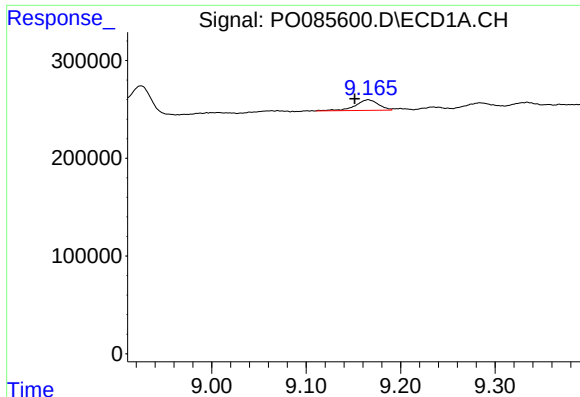


#43 AR-1268-3

R.T.: 9.166 min
Delta R.T.: 0.014 min
Response: 182541
Conc: 12.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLDG-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

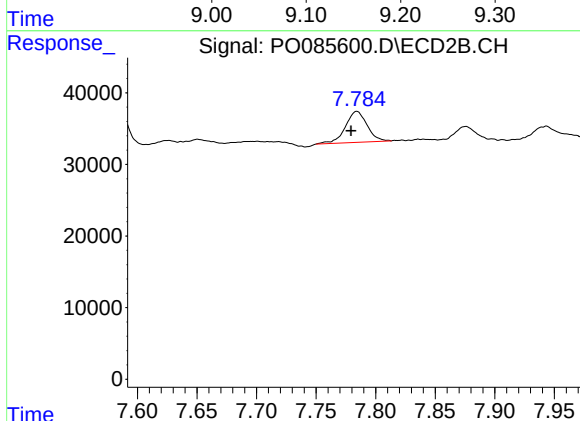


#43 AR-1268-3

R.T.: 7.784 min
Delta R.T.: 0.005 min
Response: 54742
Conc: 11.02 ng/ml

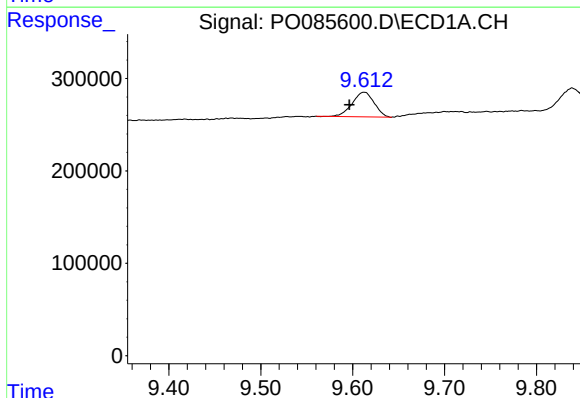


#44 AR-1268-4

R.T.: 9.613 min
Delta R.T.: 0.016 min
Response: 445299
Conc: 72.98 ng/ml

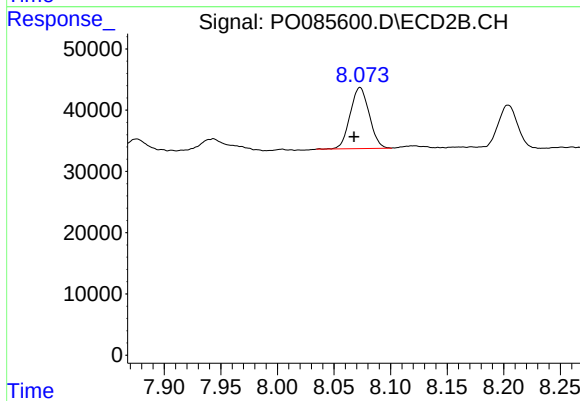

#44 AR-1268-4

R.T.: 8.073 min
Delta R.T.: 0.005 min
Response: 116553
Conc: 54.92 ng/ml

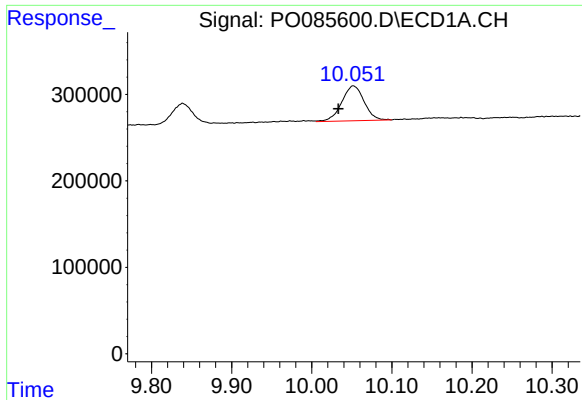


#45 AR-1268-5

R.T.: 10.052 min
Delta R.T.: 0.019 min
Response: 784318
Conc: 16.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLDG-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

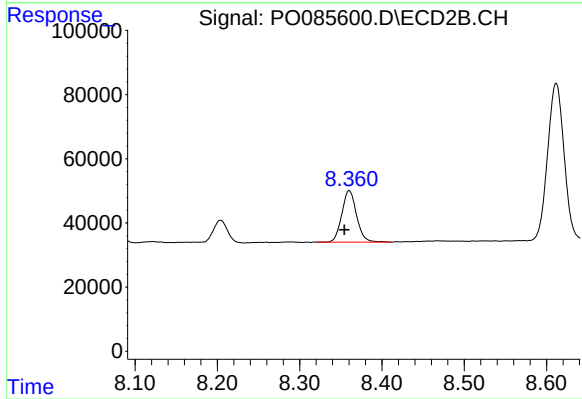

#45 AR-1268-5

R.T.: 8.360 min
Delta R.T.: 0.006 min
Response: 200005
Conc: 14.28 ng/ml