

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0032422\  
 Data File : P0085607.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 24 Mar 2022 16:05  
 Operator : YP\AJ  
 Sample : N2055-01 10X  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 CLI-2022-30A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 25 06:32:56 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031522.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 16 04:43:31 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml   |
|-----------------------------|--------|-------|--------|--------|-------|---------|
| -----                       |        |       |        |        |       |         |
| System Monitoring Compounds |        |       |        |        |       |         |
| 1) SA Tetrachlo...          | 4.490  | 3.589 | 270012 | 79903  | 1.320 | 1.865 # |
| 2) SA Decachlor...          | 10.394 | 8.606 | 305737 | 79527  | 2.543 | 2.071   |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0032422\  
Data File : P0085607.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 24 Mar 2022 16:05  
Operator : YP\AJ  
Sample : N2055-01 10X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-30A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 25 06:32:56 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031522.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Mar 16 04:43:31 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

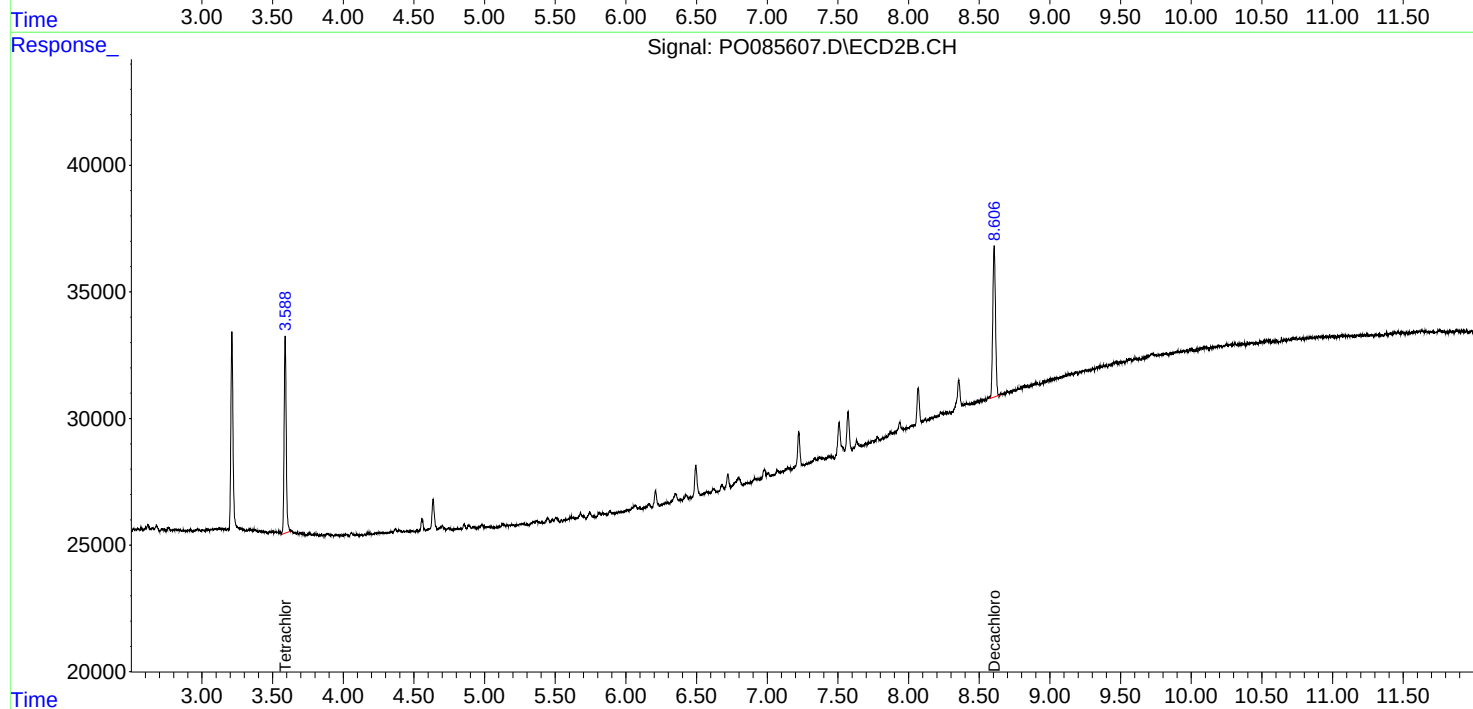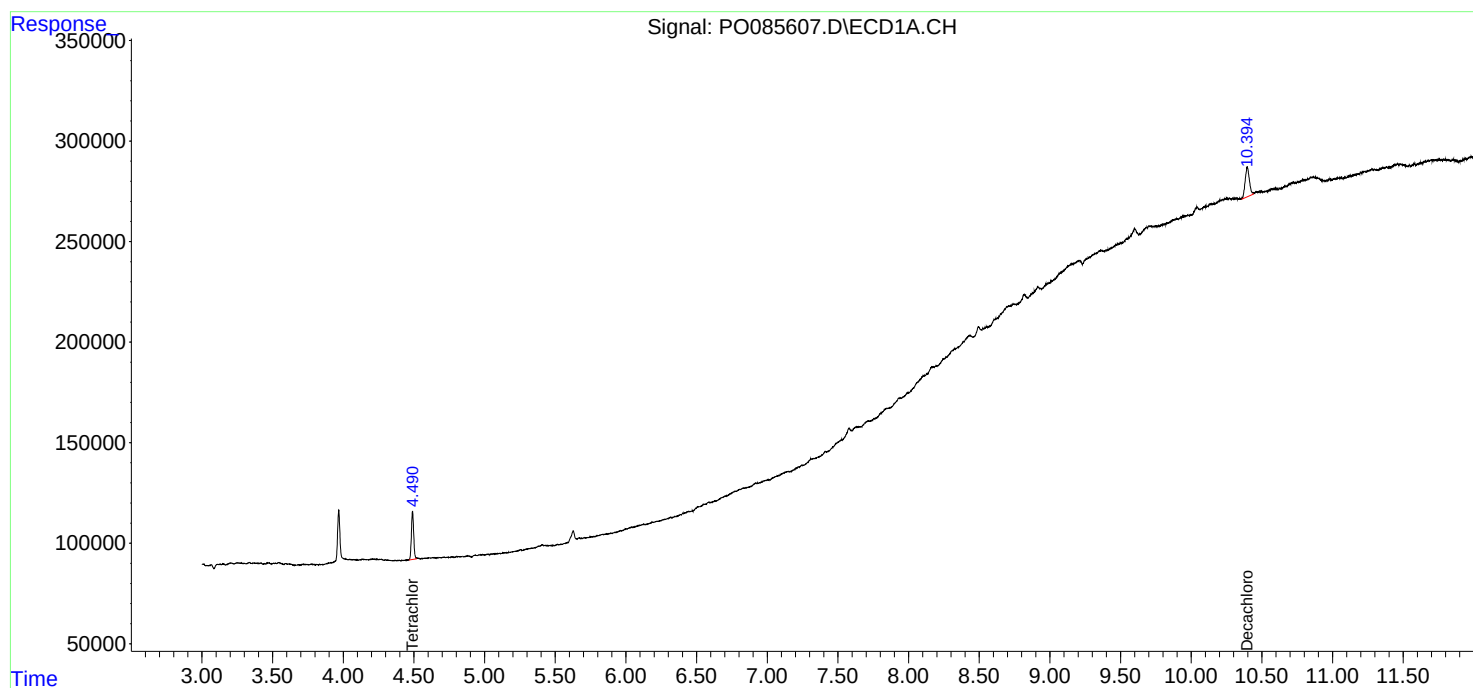


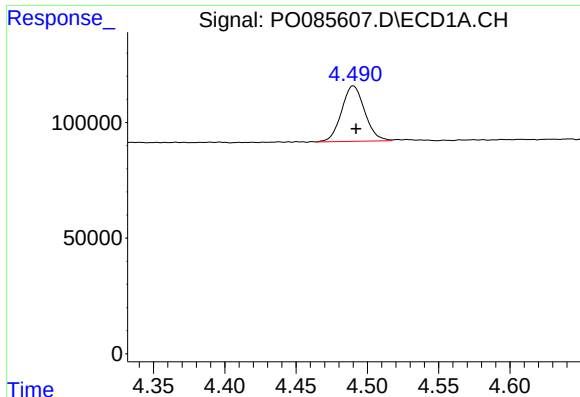

#1 Tetrachloro-m-xylene


R.T.: 4.490 min  
Delta R.T.: -0.002 min  
Response: 270012  
Conc: 1.32 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CLI-2022-30A

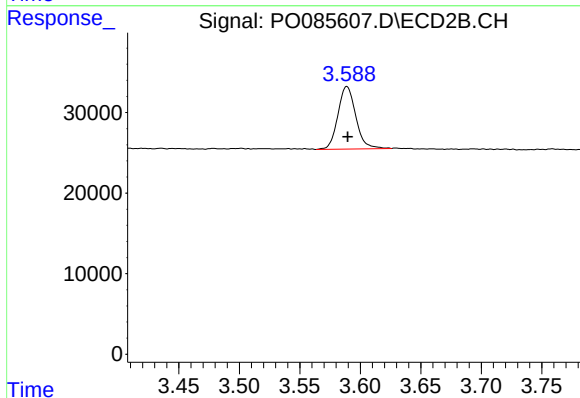


#1 Tetrachloro-m-xylene

R.T.: 3.589 min  
Delta R.T.: 0.000 min  
Response: 79903  
Conc: 1.87 ng/ml

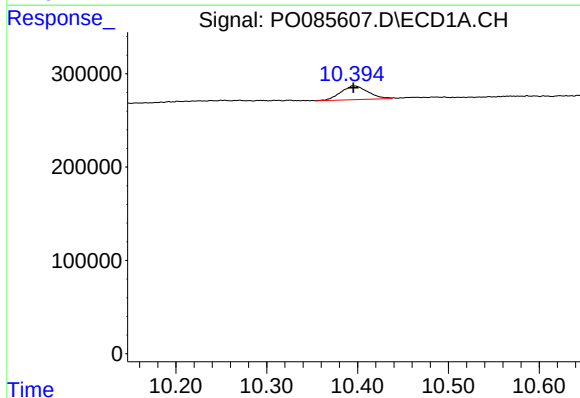

#2 Decachlorobiphenyl

R.T.: 10.394 min  
Delta R.T.: 0.000 min  
Response: 305737  
Conc: 2.54 ng/ml

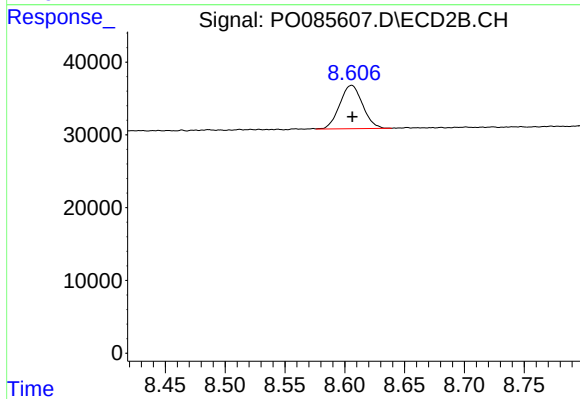

#2 Decachlorobiphenyl

R.T.: 8.606 min  
Delta R.T.: 0.000 min  
Response: 79527  
Conc: 2.07 ng/ml