

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032422\
 Data File : P0085616.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2022 19:21
 Operator : YP\AJ
 Sample : N2055-05 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-32A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:48:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.588	311913	88845	1.525m	2.074 #
2) SA Decachlor...	10.397	8.609	260130	76670	2.164	1.997
Target Compounds						
26) L6 AR-1254-1	6.546	5.479	7218176	2760653	1089.164	1050.389
27) L6 AR-1254-2	6.767	5.628	11542062	2473161	1153.318	1059.903
28) L6 AR-1254-3	7.139	6.031	11684399	3898528	1135.340	1061.454
29) L6 AR-1254-4	7.427	6.261	7912653	2282585	1127.817	1030.474
30) L6 AR-1254-5	7.852	6.681	8454090	3079516	1104.884	946.733

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032422\
Data File : P0085616.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2022 19:21
Operator : YP\AJ
Sample : N2055-05 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CLI-2022-32A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:48:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

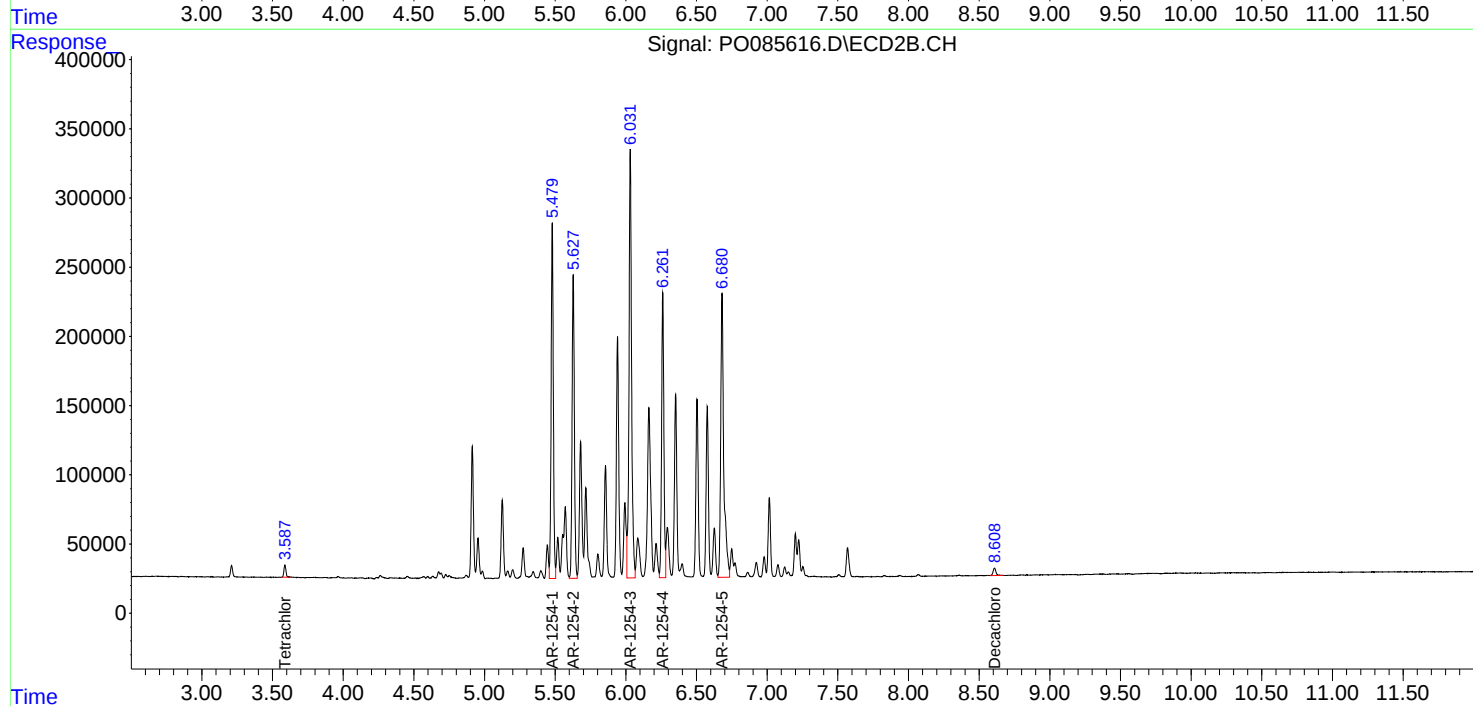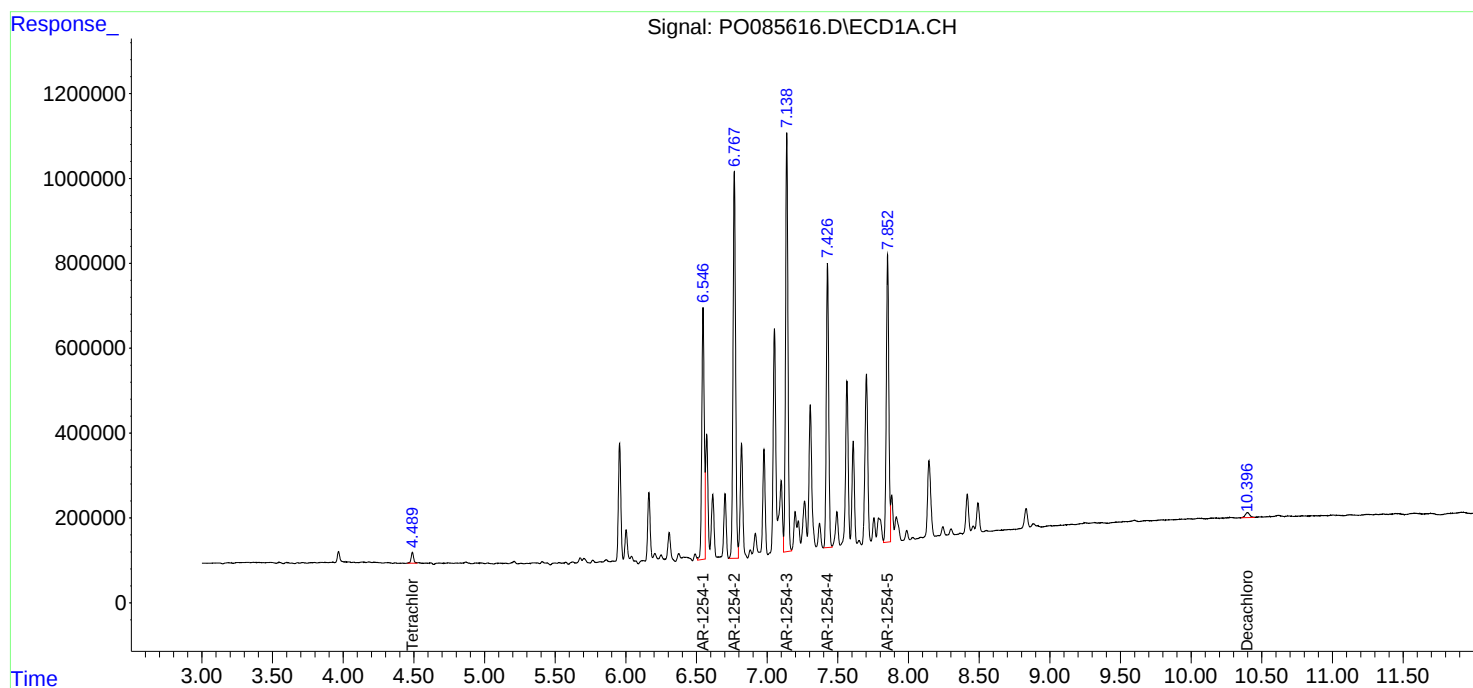

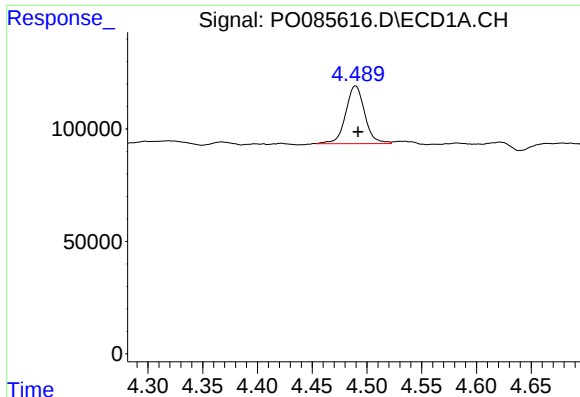


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.003 min
Response: 311913
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-32A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

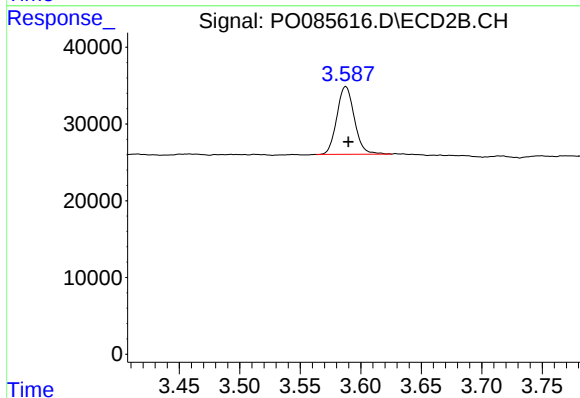


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.002 min
Response: 88845
Conc: 2.07 ng/ml

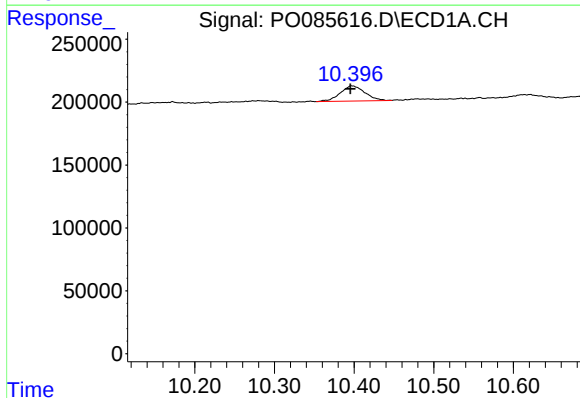


#2 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: 0.002 min
Response: 260130
Conc: 2.16 ng/ml

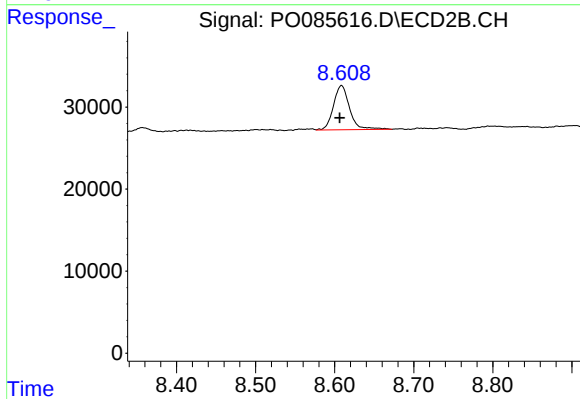

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: 0.002 min
Response: 76670
Conc: 2.00 ng/ml

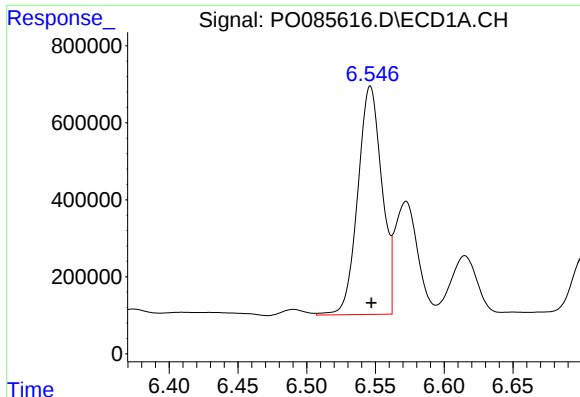


#26 AR-1254-1

R.T.: 6.546 min
Delta R.T.: 0.000 min
Response: 7218176
Conc: 1089.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-32A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

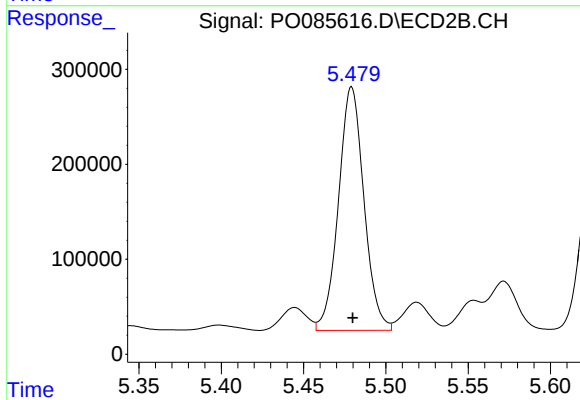


#26 AR-1254-1

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 2760653
Conc: 1050.39 ng/ml

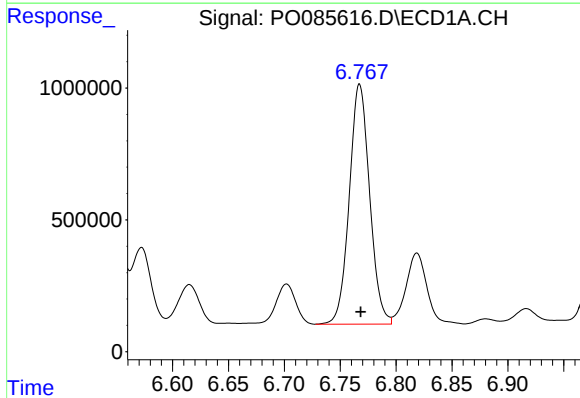


#27 AR-1254-2

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 11542062
Conc: 1153.32 ng/ml

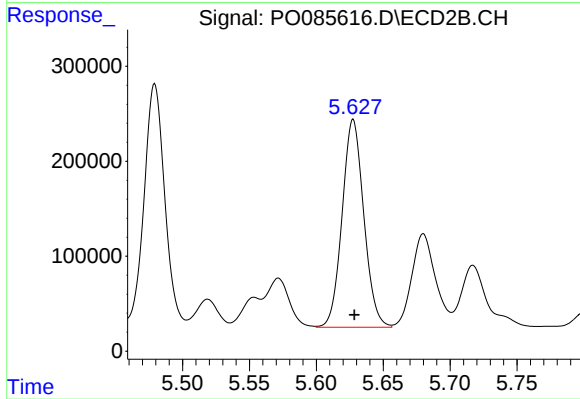

#27 AR-1254-2

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 2473161
Conc: 1059.90 ng/ml

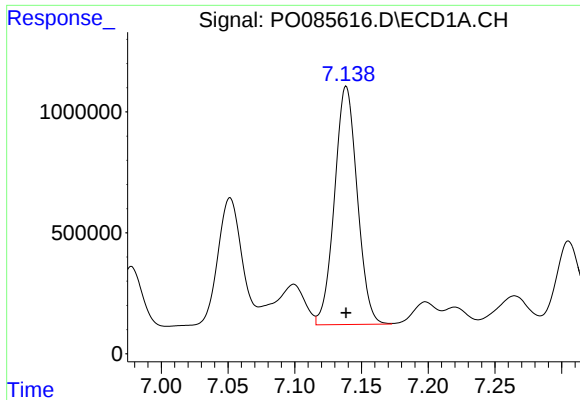


#28 AR-1254-3

R.T.: 7.139 min
Delta R.T.: 0.000 min
Response: 11684399
Conc: 1135.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-32A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

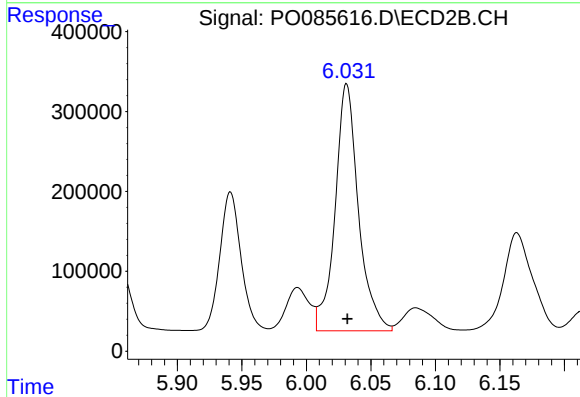


#28 AR-1254-3

R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 3898528
Conc: 1061.45 ng/ml

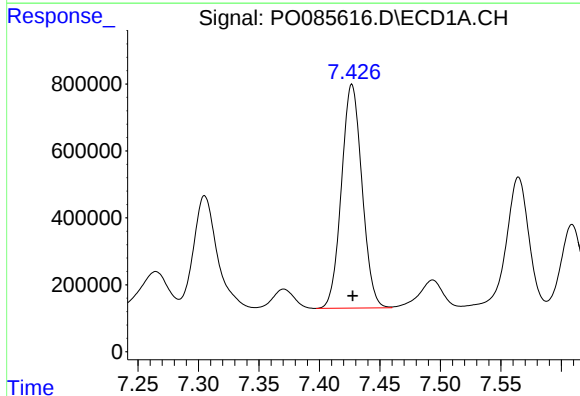


#29 AR-1254-4

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 7912653
Conc: 1127.82 ng/ml

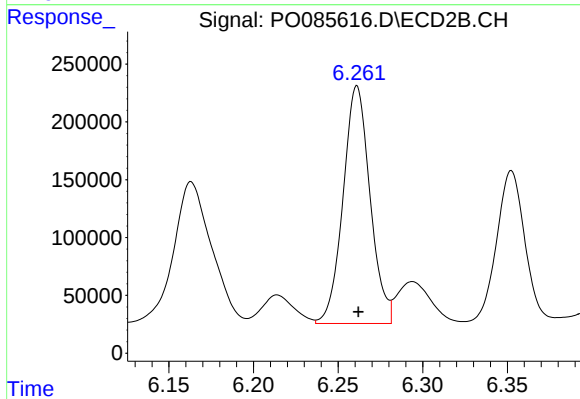

#29 AR-1254-4

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 2282585
Conc: 1030.47 ng/ml

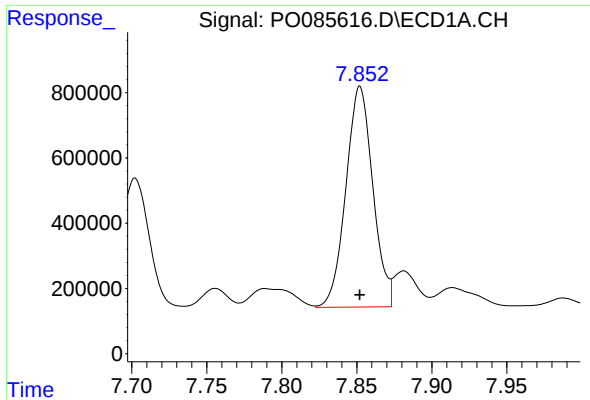


#30 AR-1254-5

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 8454090
Conc: 1104.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-32A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

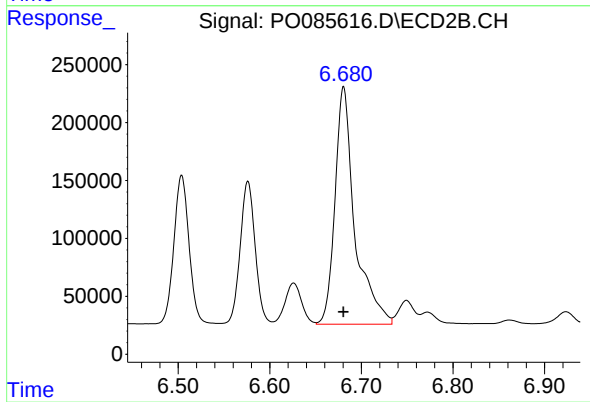

#30 AR-1254-5

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 3079516
Conc: 946.73 ng/ml